

Data File : BM021855.D
Acq On : 05 Aug 2019 22:56
Operator : HP/JU
Sample : K3863-12DL 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52F2DL

Quant Time: Aug 06 01:32:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 06 01:29:26 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	790	0.40	ng/ul	0.00
2) Naphthalene-d8	10.43	136	3361	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	1873	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	4150	0.40	ng/ul	0.00
16) Chrysene-d12	21.24	240	4218	0.40	ng/ul	0.00
20) Perylene-d12	23.46	264	5712	0.40	ng/ul	0.00

System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.97	152	4	0.00	ng/ul	-0.05
14) Fluoranthene-d10	19.08	212	385	0.03	ng/ul	0.00


Target Compounds				Qvalue		
12) Phenanthrene	17.08	178	2733	0.226	ng/ul	97
13) Anthracene	17.18	178	289	0.028	ng/ul#	47
15) Fluoranthene	19.11	202	10330	0.639	ng/ul	97
17) Pyrene	19.47	202	8966	0.517	ng/ul	98
18) Benzo(a)anthracene	21.23	228	4056	0.269	ng/ul#	91
19) Chrysene	21.28	228	4860	0.250	ng/ul#	92
21) Benzo(b)fluoranthene	22.79	252	10012	0.520	ng/ul	93
22) Benzo(k)fluoranthene	22.79	252	10012	0.459	ng/ul#	93
23) Benzo(a)pyrene	23.36	252	4208	0.215	ng/ul#	91
24) Indeno(1,2,3-cd)pyrene	25.68	276	3699	0.158	ng/ul#	91
25) Dibenzo(a,h)anthracene	25.69	278	712	0.038	ng/ul#	3
26) Benzo(g,h,i)perylene	26.36	276	3791	0.180	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM021855.D
Acq On : 05 Aug 2019 22:56
Operator : HP/JU
Sample : K3863-12DL 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52F2DL

Quant Time: Aug 06 01:32:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 06 01:29:26 2019
Response via : Initial Calibration

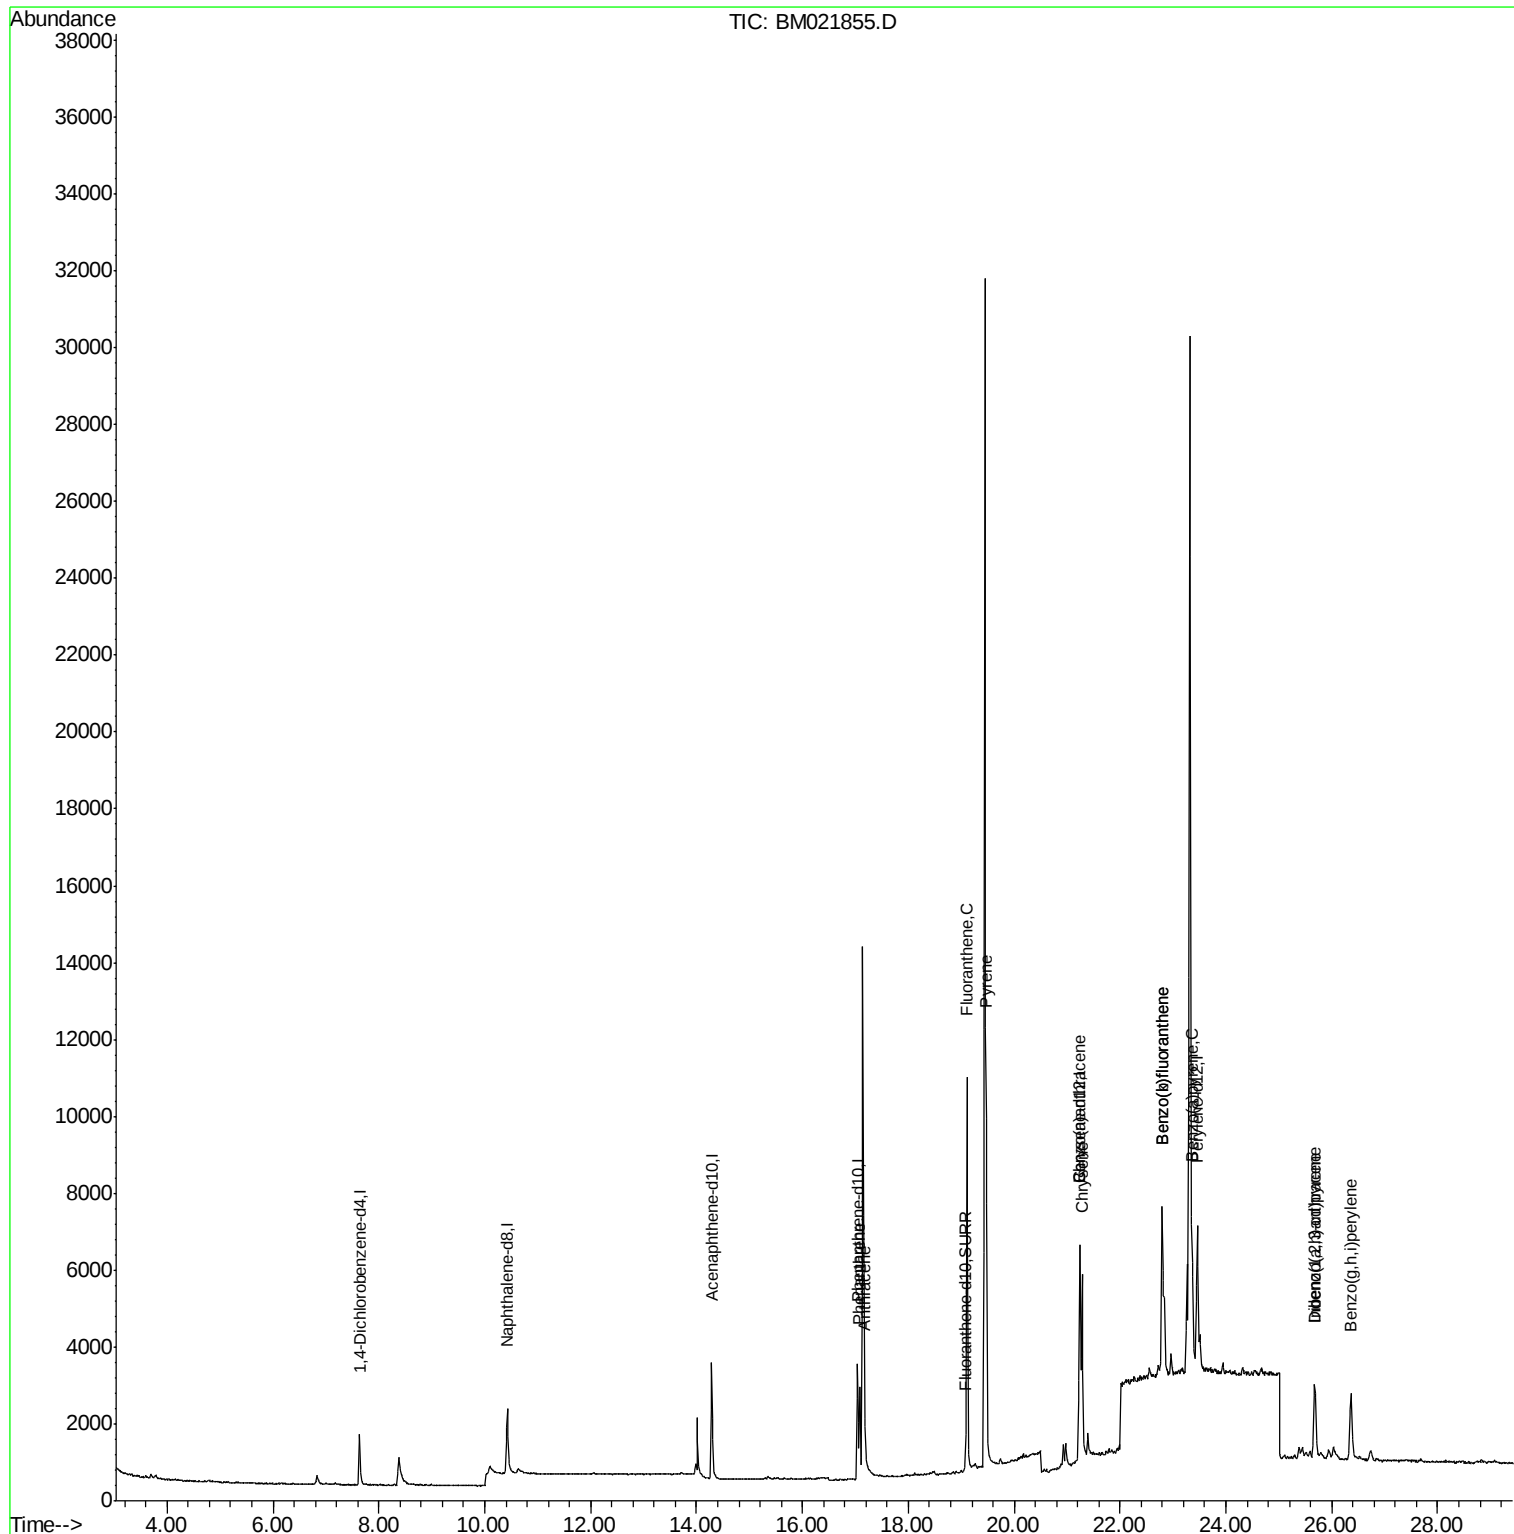

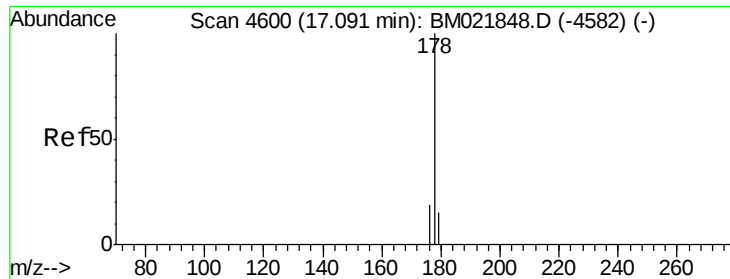

#12

Phenanthrene

Concen: 0.226 ng/ul

RT: 17.08 min Scan# 4598

Delta R.T. -0.01 min

Lab File: BM021855.D

Acq: 05 Aug 2019 22:56

Instrument :

BNA_M

ClientSampleId :

A52F2DL


Tgt Ion:178 Resp: 2733

Ion Ratio Lower Upper

178 100

179 18.9 14.2 21.2




176 22.6 16.8 25.2

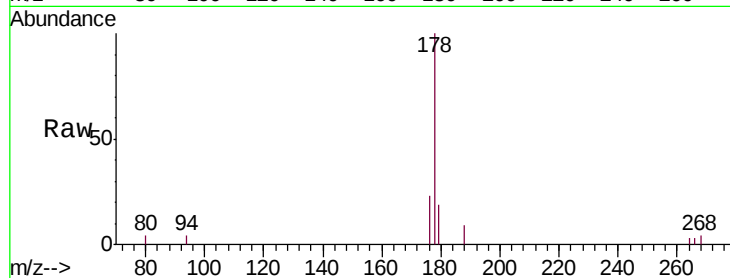

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

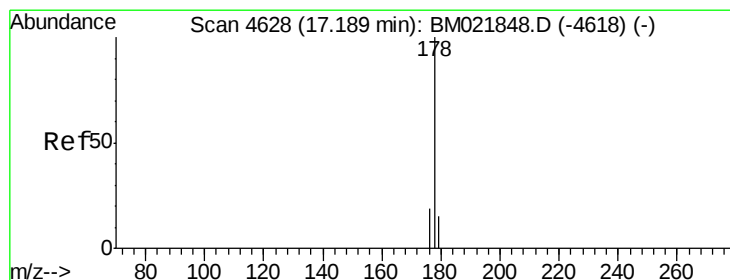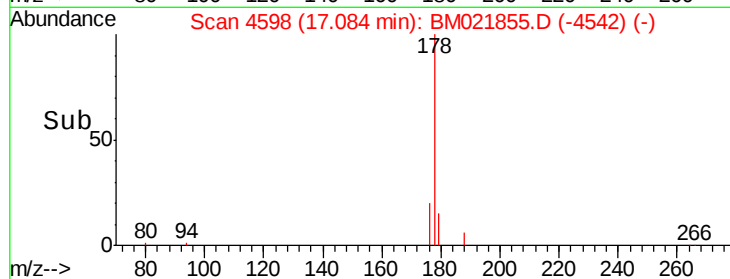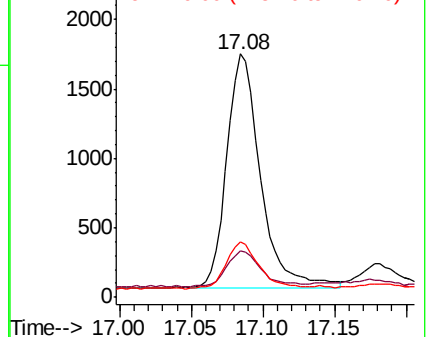

#13

Anthracene

Concen: 0.028 ng/ul

RT: 17.18 min Scan# 4625

Delta R.T. -0.01 min

Lab File: BM021855.D

Acq: 05 Aug 2019 22:56


Tgt Ion:178 Resp: 289

Ion Ratio Lower Upper

178 100

179 50.8 15.5 23.3#



176 38.3 16.6 25.0#

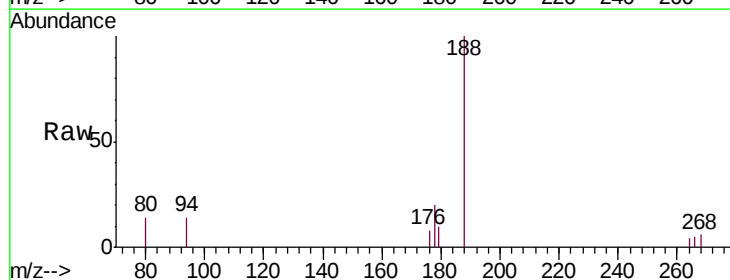


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E



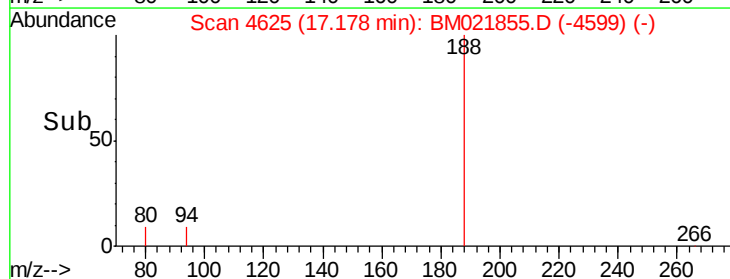
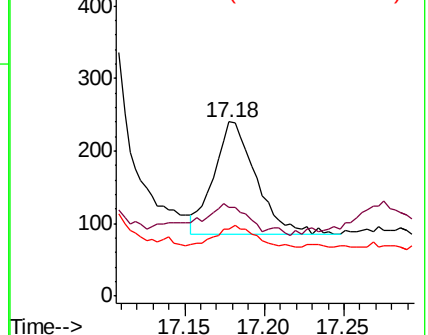


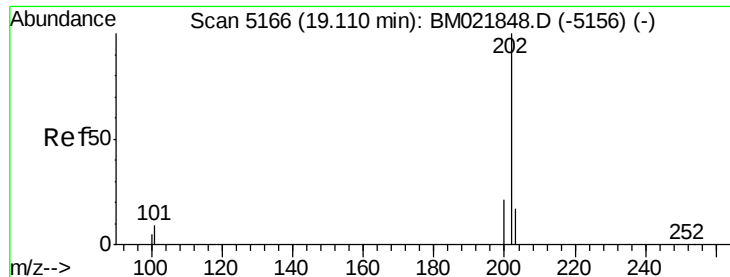

#15
Fluoranthene
 Concen: 0.639 ng/ul
 RT: 19.11 min Scan# 5166
 Delta R.T. -0.00 min
 Lab File: BM021855.D
 Acq: 05 Aug 2019 22:56




Instrument :
 BNA_M
 ClientSampleId :
 A52F2DL


Tgt Ion	Ratio	Lower	Upper
202	100		
101	9.0	0.0	30.2
100	7.1	0.0	28.1

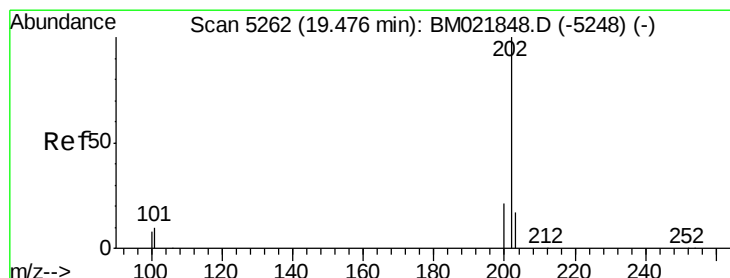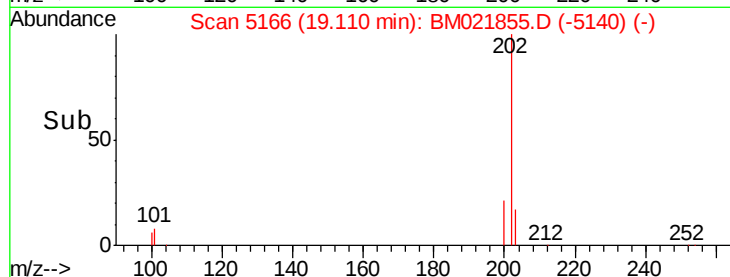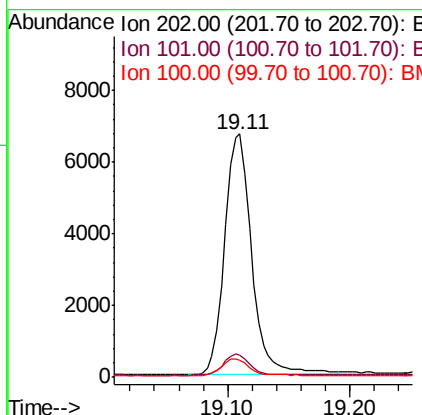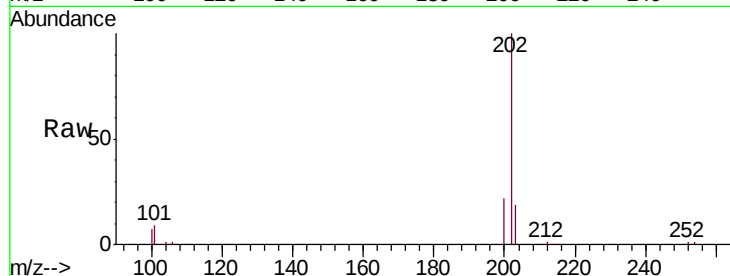

#17
Pyrene
 Concen: 0.517 ng/ul
 RT: 19.47 min Scan# 5261
 Delta R.T. -0.00 min
 Lab File: BM021855.D
 Acq: 05 Aug 2019 22:56

Tgt Ion	Ratio	Lower	Upper
202	100		
101	11.4	8.3	12.5
100	9.5	7.2	10.8

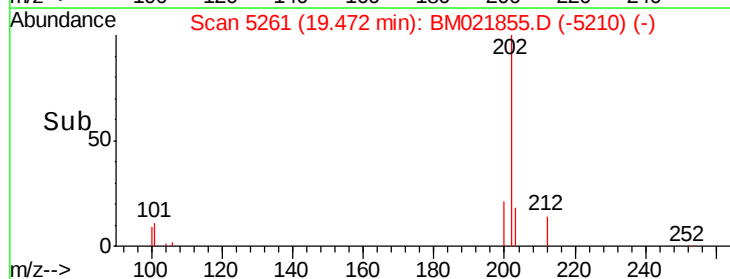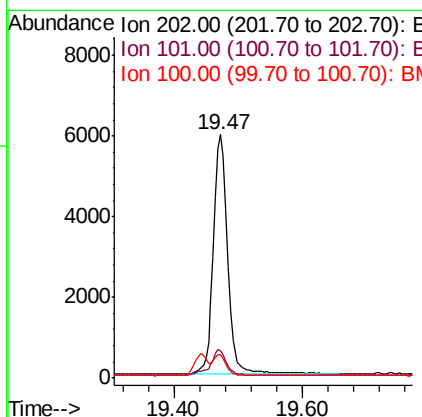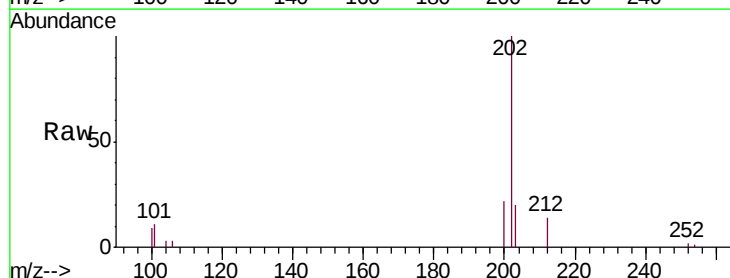

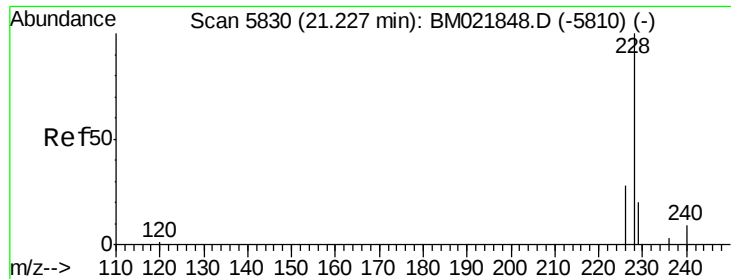

#18

Benzo(a)anthracene

Concen: 0.269 ng/ul

RT: 21.23 min Scan# 5831

Delta R.T. 0.00 min

Lab File: BM021855.D

Acq: 05 Aug 2019 22:56

Instrument :

BNA_M

ClientSampleId :

A52F2DL





Tgt Ion:228 Resp: 4056

Ion Ratio Lower Upper

228 100

229 26.4 17.2 25.8#

226 32.7 22.6 34.0

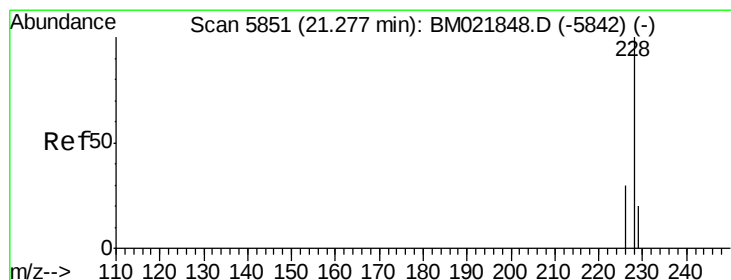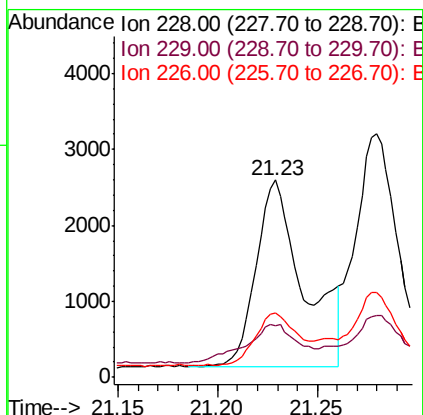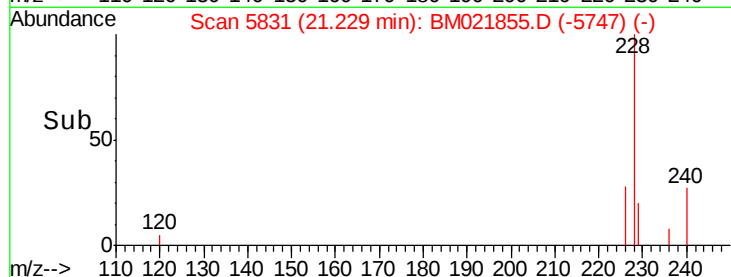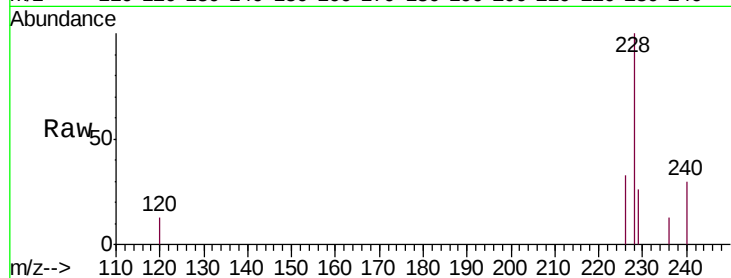

#19

Chrysene

Concen: 0.250 ng/ul

RT: 21.28 min Scan# 5852

Delta R.T. 0.00 min

Lab File: BM021855.D

Acq: 05 Aug 2019 22:56




Tgt Ion:228 Resp: 4860


Ion Ratio Lower Upper

228 100

226 34.8 24.9 37.3

229 25.2 16.6 25.0#

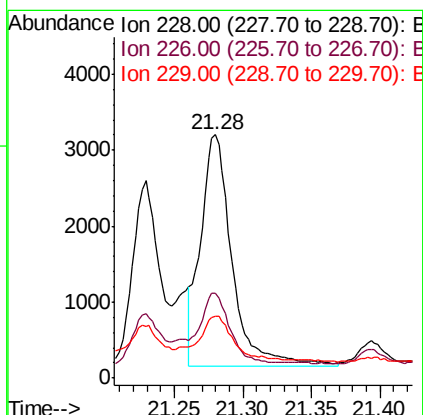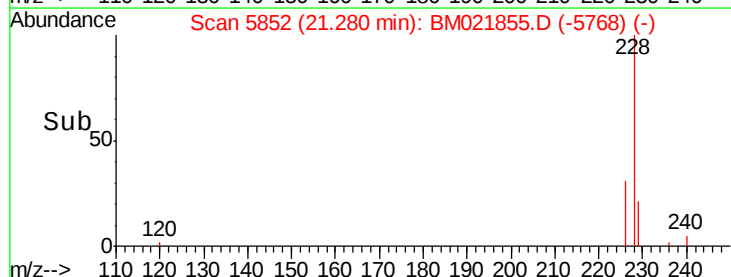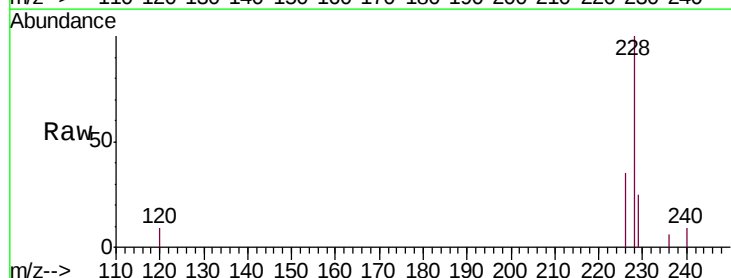

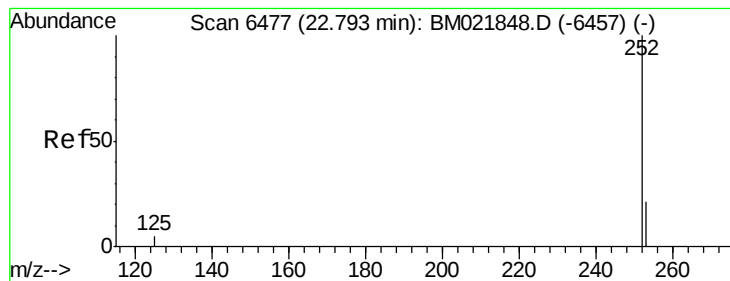

#21

Benzo(b)fluoranthene

Concen: 0.520 ng/u1

RT: 22.79 min Scan# 6477

Delta R.T. -0.00 min

Lab File: BM021855.D

Acq: 05 Aug 2019 22:56

Instrument :

BNA_M

ClientSampleId :

A52F2DL


Tgt Ion:252 Resp: 10012

Ion Ratio Lower Upper

252 100

253 36.1 0.0 67.4




125 20.5 0.0 31.0

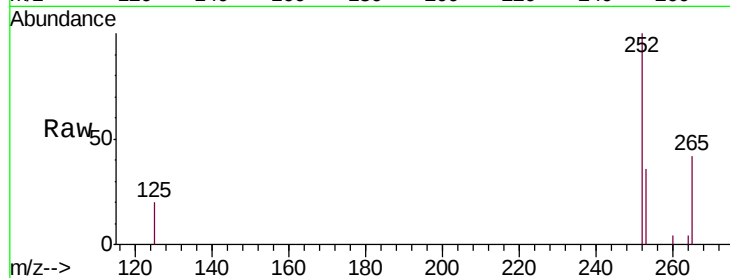

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

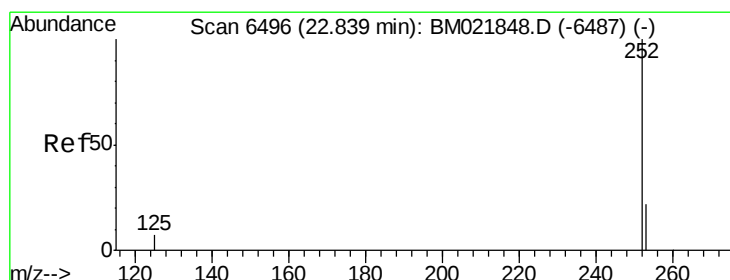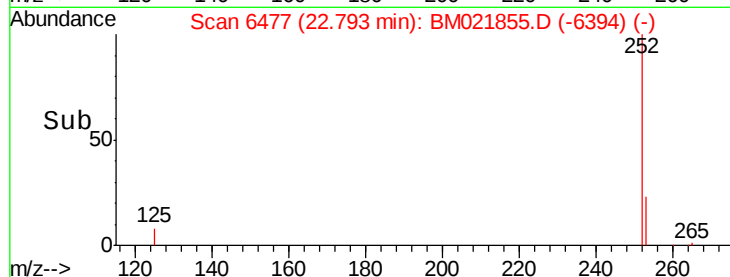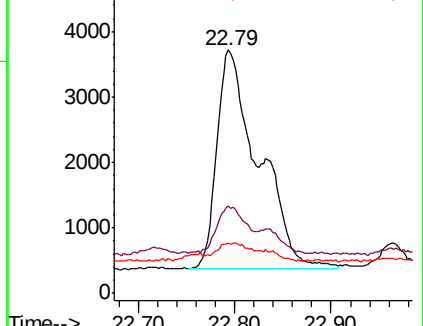

#22

Benzo(k)fluoranthene

Concen: 0.459 ng/u1

RT: 22.79 min Scan# 6477

Delta R.T. -0.05 min

Lab File: BM021855.D

Acq: 05 Aug 2019 22:56


Tgt Ion:252 Resp: 10012

Ion Ratio Lower Upper

252 100

253 36.1 27.0 40.4



125 20.5 12.2 18.2#

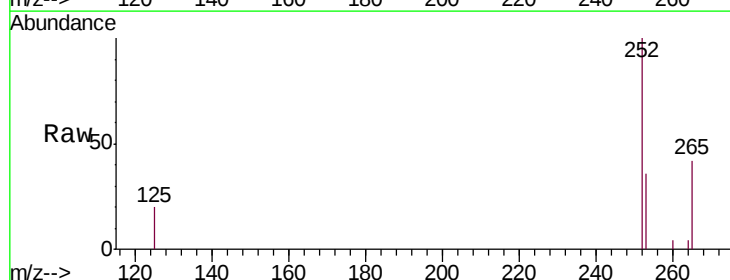


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

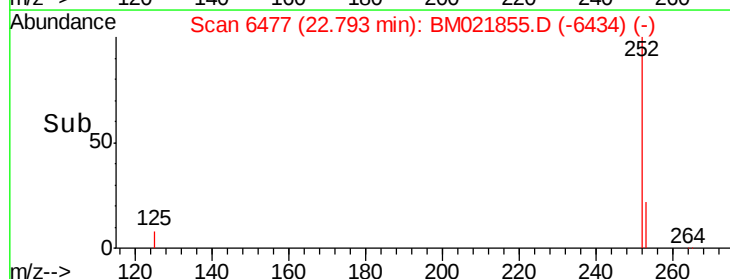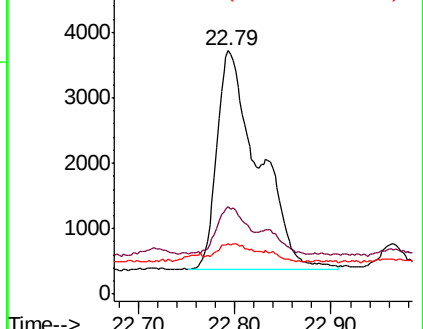

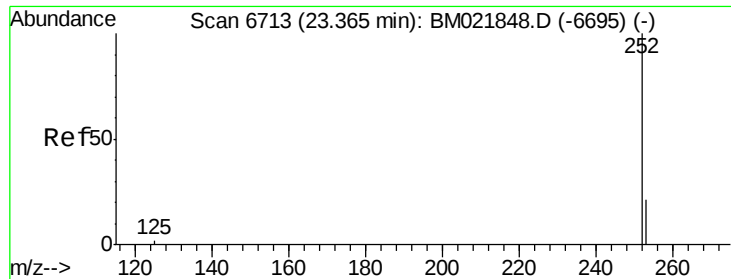

#23

Benzo(a)pyrene

Concen: 0.215 ng/u1

RT: 23.36 min Scan# 6711

Delta R.T. -0.00 min

Lab File: BM021855.D

Acq: 05 Aug 2019 22:56

Instrument :

BNA_M

ClientSampleId :

A52F2DL


Tgt Ion:252 Resp: 4208

Ion Ratio Lower Upper

252 100

253 42.6 31.7 47.5




125 25.8 14.6 21.8#

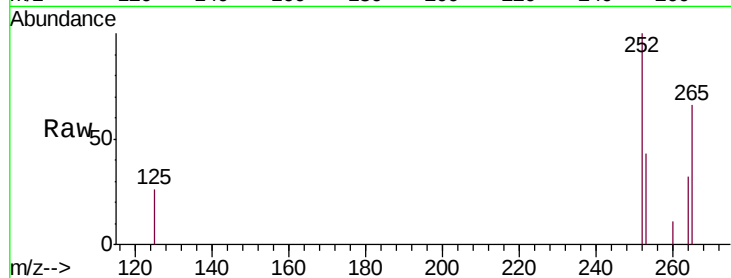

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

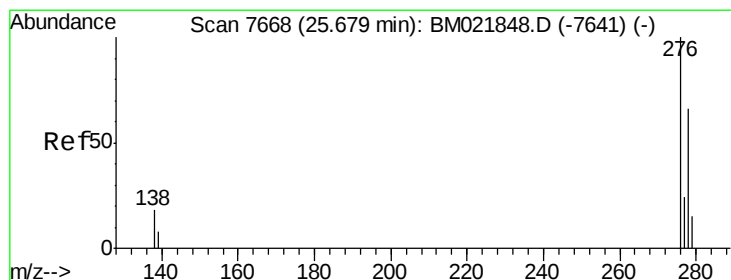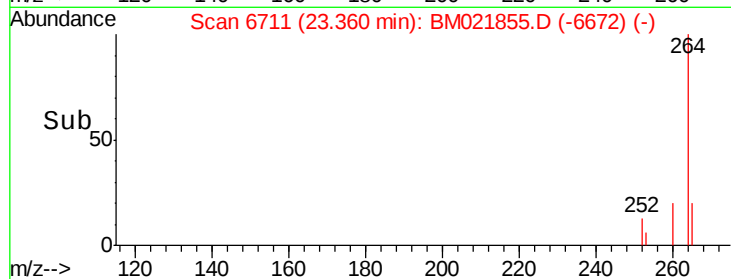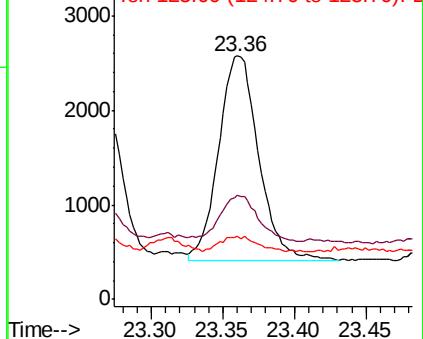

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.158 ng/u1

RT: 25.68 min Scan# 7667

Delta R.T. -0.00 min

Lab File: BM021855.D

Acq: 05 Aug 2019 22:56


Tgt Ion:276 Resp: 3699

Ion Ratio Lower Upper

276 100

138 14.9 15.1 22.7#



227 0.0 0.0 0.0

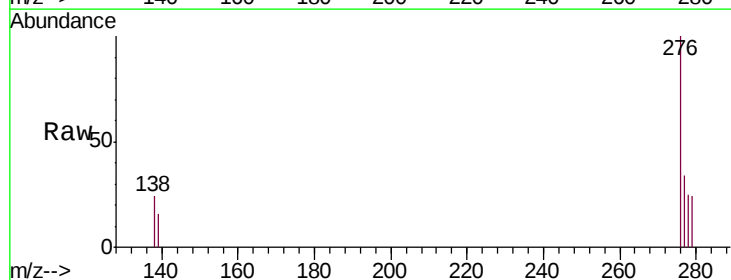


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 227.00 (226.70 to 227.70): E



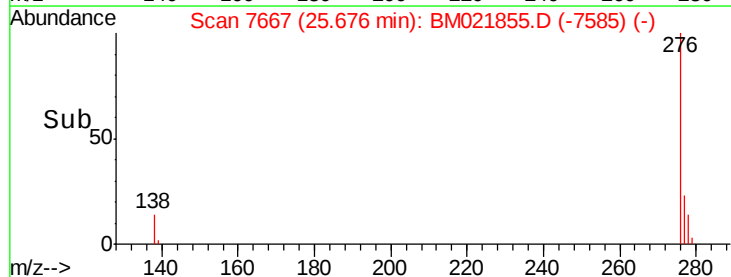
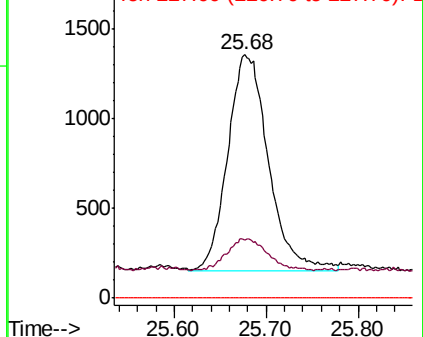


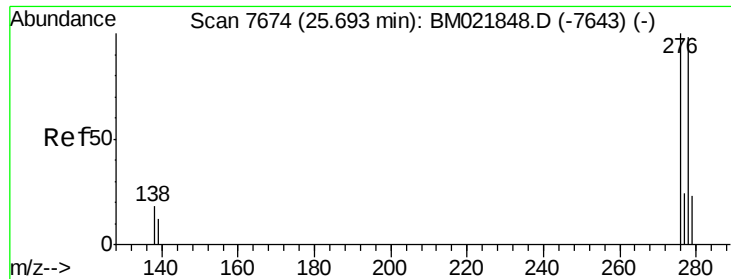

#25
Dibenzo(a,h)anthracene
Concen: 0.038 ng/u1
RT: 25.69 min Scan# 7671
Delta R.T. -0.01 min
Lab File: BM021855.D
Acq: 05 Aug 2019 22:56

Instrument :
BNA_M
ClientSampleId :
A52F2DL

Tgt Ion:278 Resp: 712
Ion Ratio Lower Upper
278 100
139 61.6 14.2 21.2#
279 91.3 28.3 42.5#

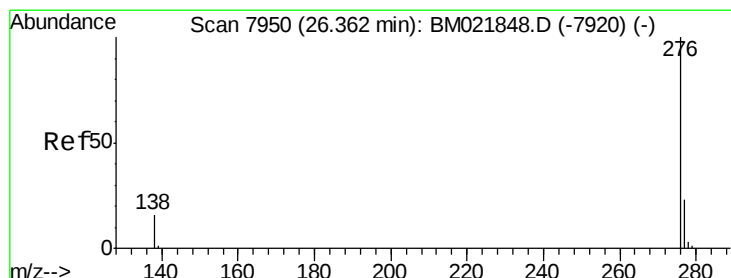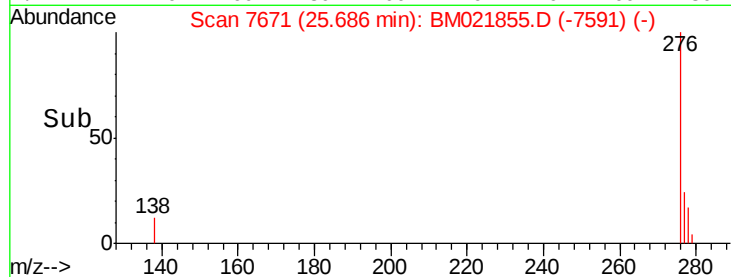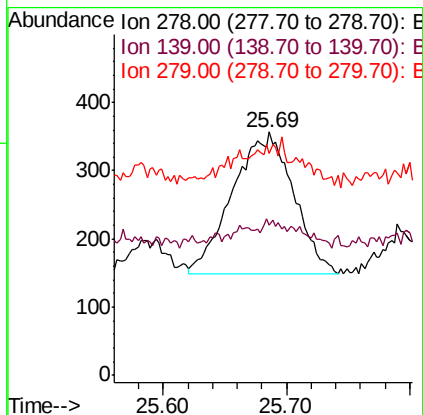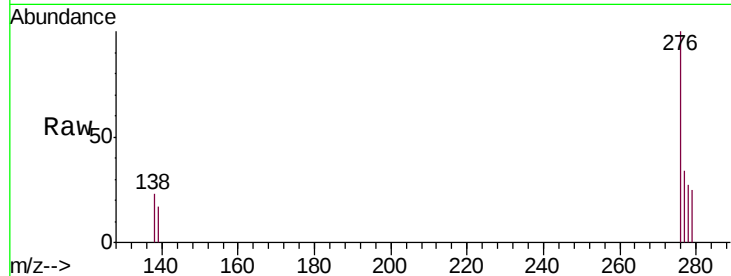

#26
Benzo(g,h,i)perylene
Concen: 0.180 ng/u1
RT: 26.36 min Scan# 7948
Delta R.T. -0.00 min
Lab File: BM021855.D
Acq: 05 Aug 2019 22:56

Tgt Ion:276 Resp: 3791
Ion Ratio Lower Upper
276 100
138 24.6 15.5 23.3#
277 33.2 21.4 32.2#

