

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\

Quantitation Report (QT Reviewed)

Data File : BM021792.D

Acq On : 04 Aug 2019 02:39

Operator : HP/JU

Sample : K3850-20

Misc :

ALS Vial : 35 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

BENS6

Manual Integrations
APPROVED

mohammad
8/5/2019 10:14:19 PM


Quant Time: Aug 04 05:08:24 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Qlast Update : Sun Aug 04 04:24:24 2019

Response via : Initial Calibration

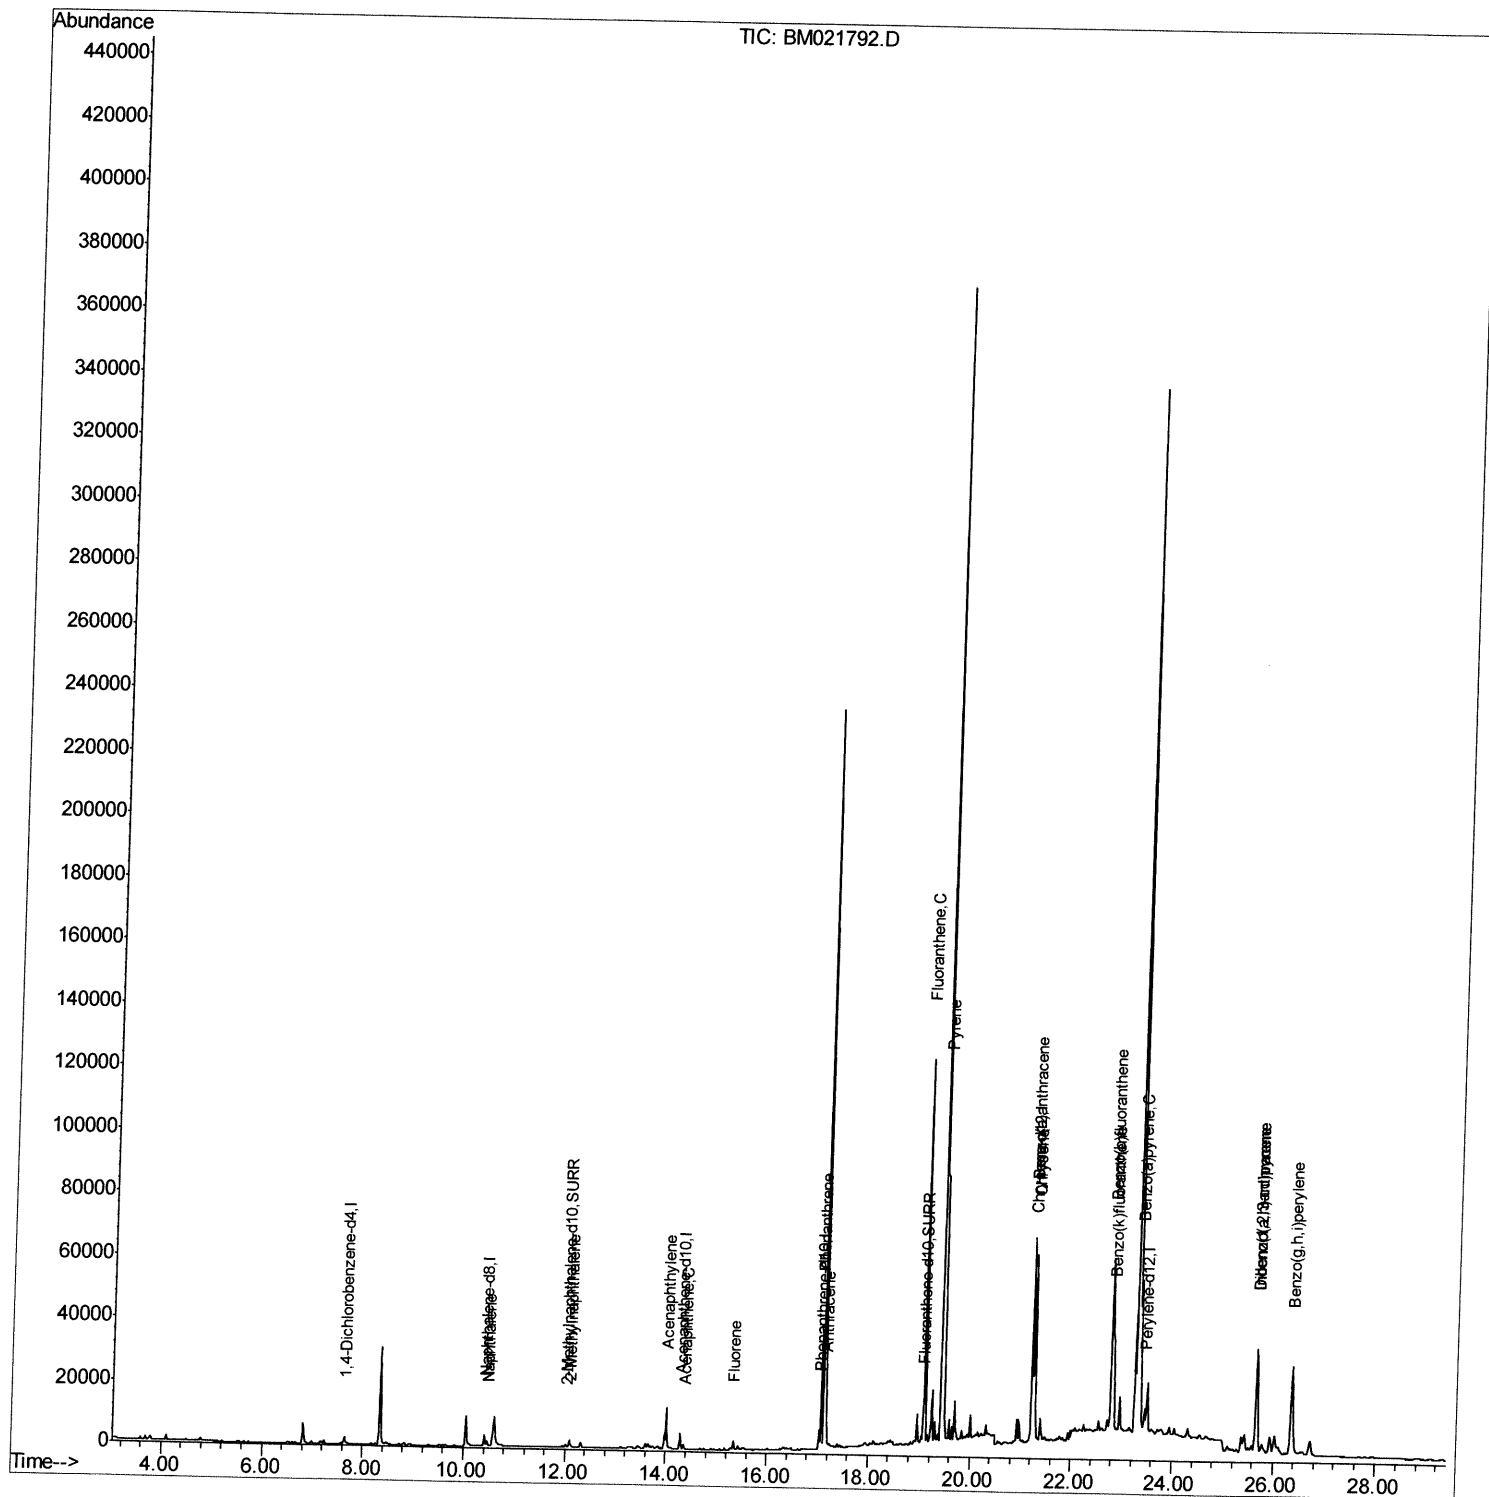

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021792.D
Acq On : 04 Aug 2019 02:39
Operator : HP/JU
Sample : K3850-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENS6

Manual Integrations
APPROVED

mohammad
8/5/2019 10:14:19 PM

Quant Time: Aug 04 04:27:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 04 04:24:24 2019
Response via : Initial Calibration

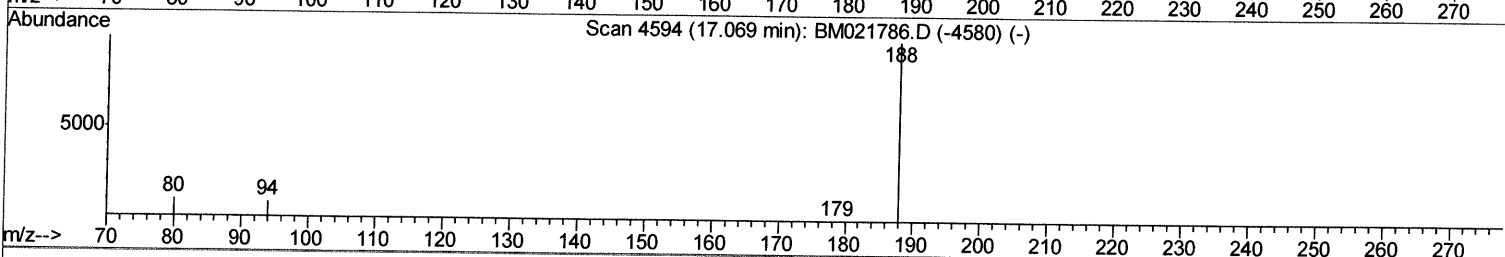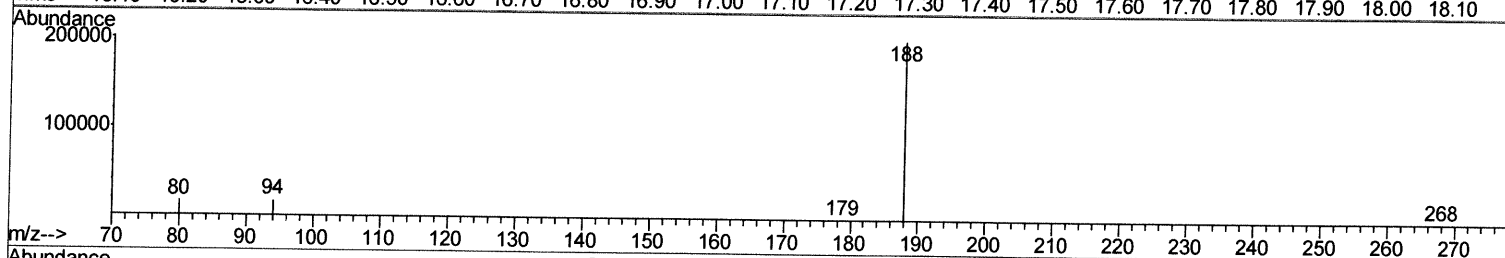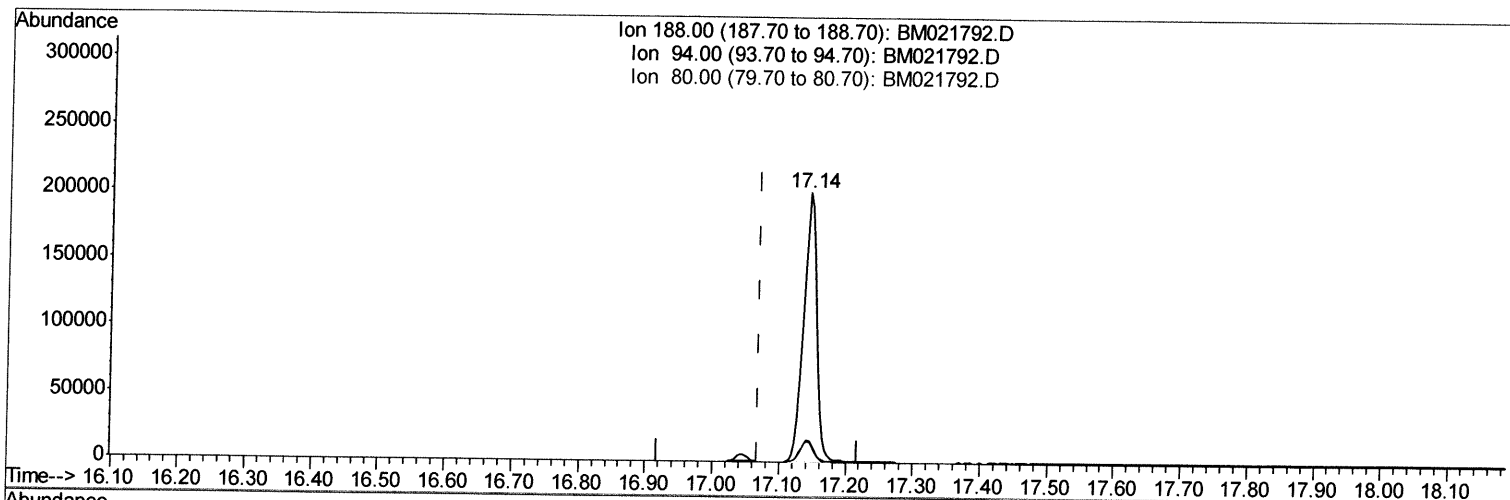

TIC: BM021792.D

(10) Phenanthrene-d10 (I)

17.143min (+0.075) 0.40ng/ul

response 281190

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	8.34
80.00	11.40	7.95#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\

Quantitation Report (Qedit)

Data File : BM021792.D

Acq On : 04 Aug 2019 02:39

Operator : HP/JU

Sample : K3850-20

Misc :

ALS Vial : 35 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

BENS6

Manual Integrations
APPROVED

mohammad
8/5/2019 10:14:19 PM


Quant Time: Aug 04 04:27:49 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun Aug 04 04:24:24 2019

Response via : Initial Calibration

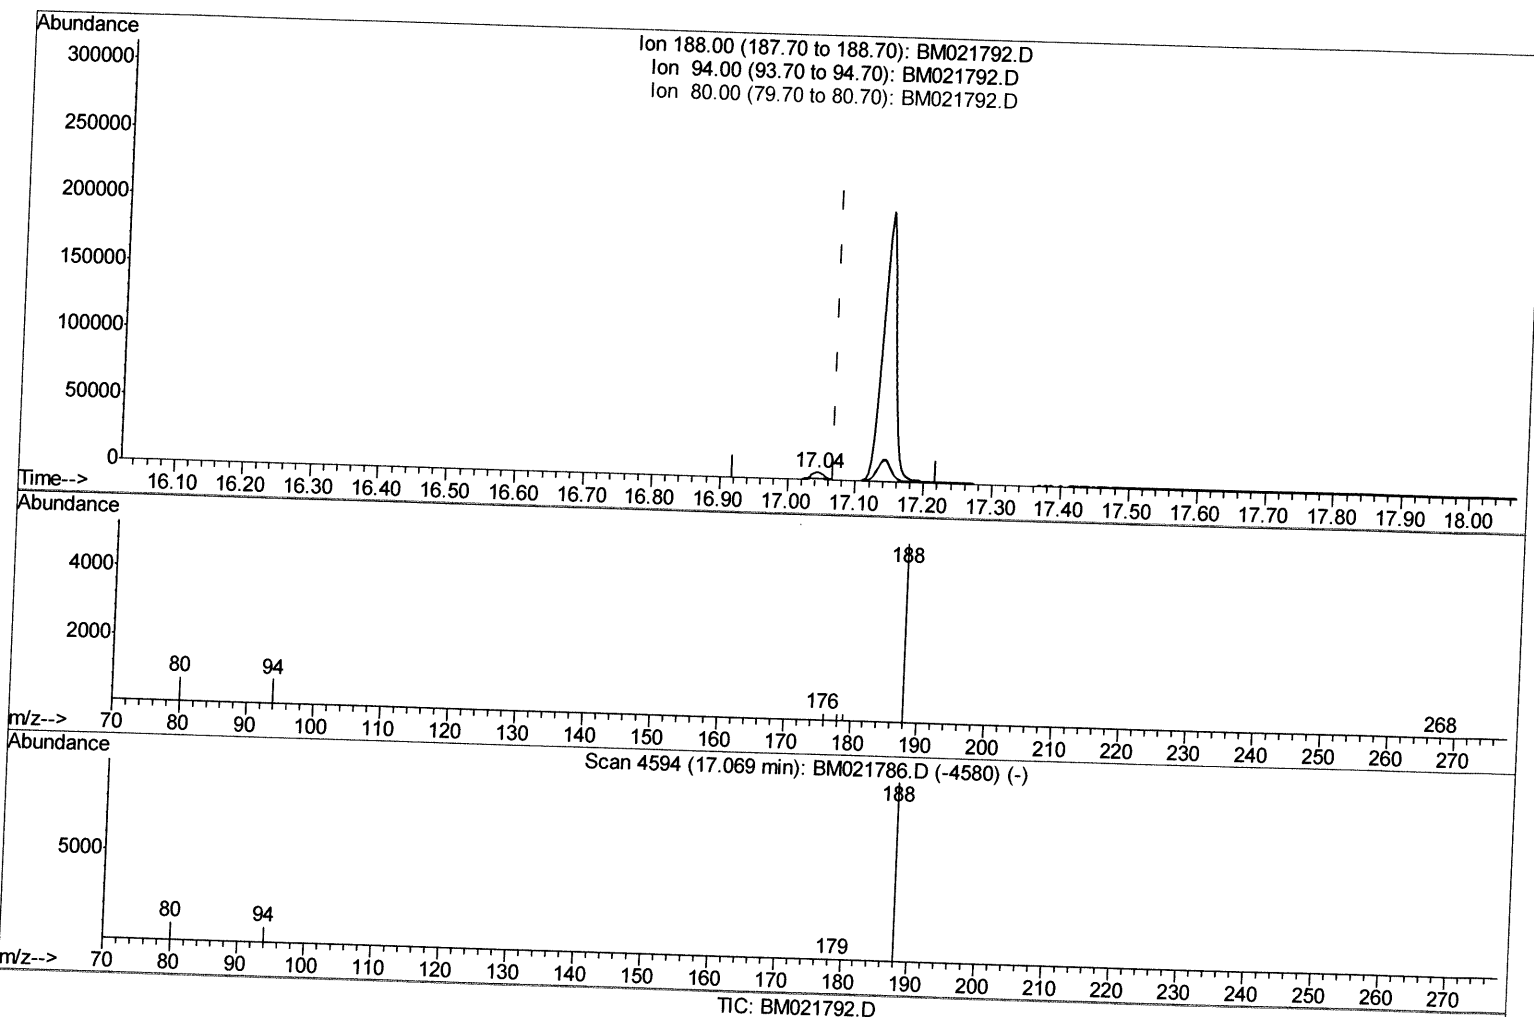

(10) Phenanthrene-d10 (I)

17.043min (-0.026) 0.40ng/ul m *JU* 08/05/19

response 7447

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	14.38#
80.00	11.40	13.97#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021792.D
Acq On : 04 Aug 2019 02:39
Operator : HP/JU
Sample : K3850-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENS6

Manual Integrations
APPROVED

mohammad
8/5/2019 10:14:19 PM

Quant Time: Aug 04 05:06:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 04 04:24:24 2019
Response via : Initial Calibration

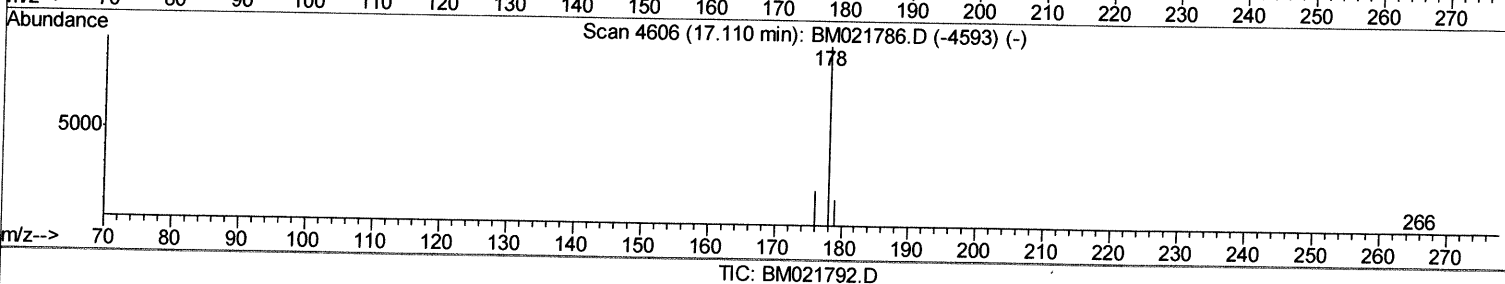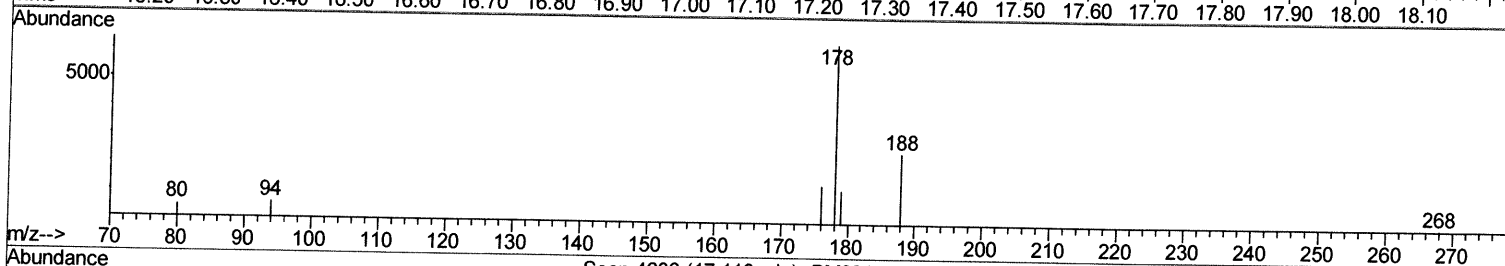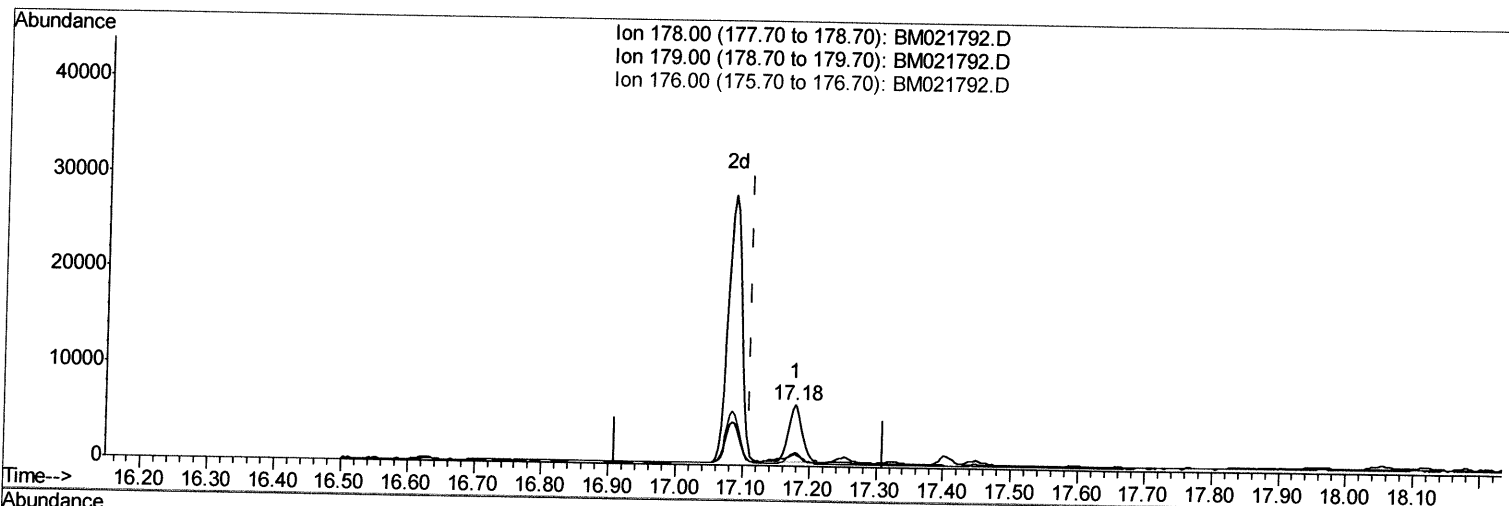

(12) Phenanthrene

17.178min (+0.068) 0.41ng/ul

response 8782

Ion	Exp%	Act%
178.00	100	100
179.00	17.70	19.53
176.00	21.00	21.97
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)


Data File : BM021792.D
Acq On : 04 Aug 2019 02:39
Operator : HP/JU
Sample : K3850-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENS6

Manual Integrations
APPROVED

mohammad
8/5/2019 10:14:19 PM

Quant Time: Aug 04 05:06:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 04 04:24:24 2019
Response via : Initial Calibration

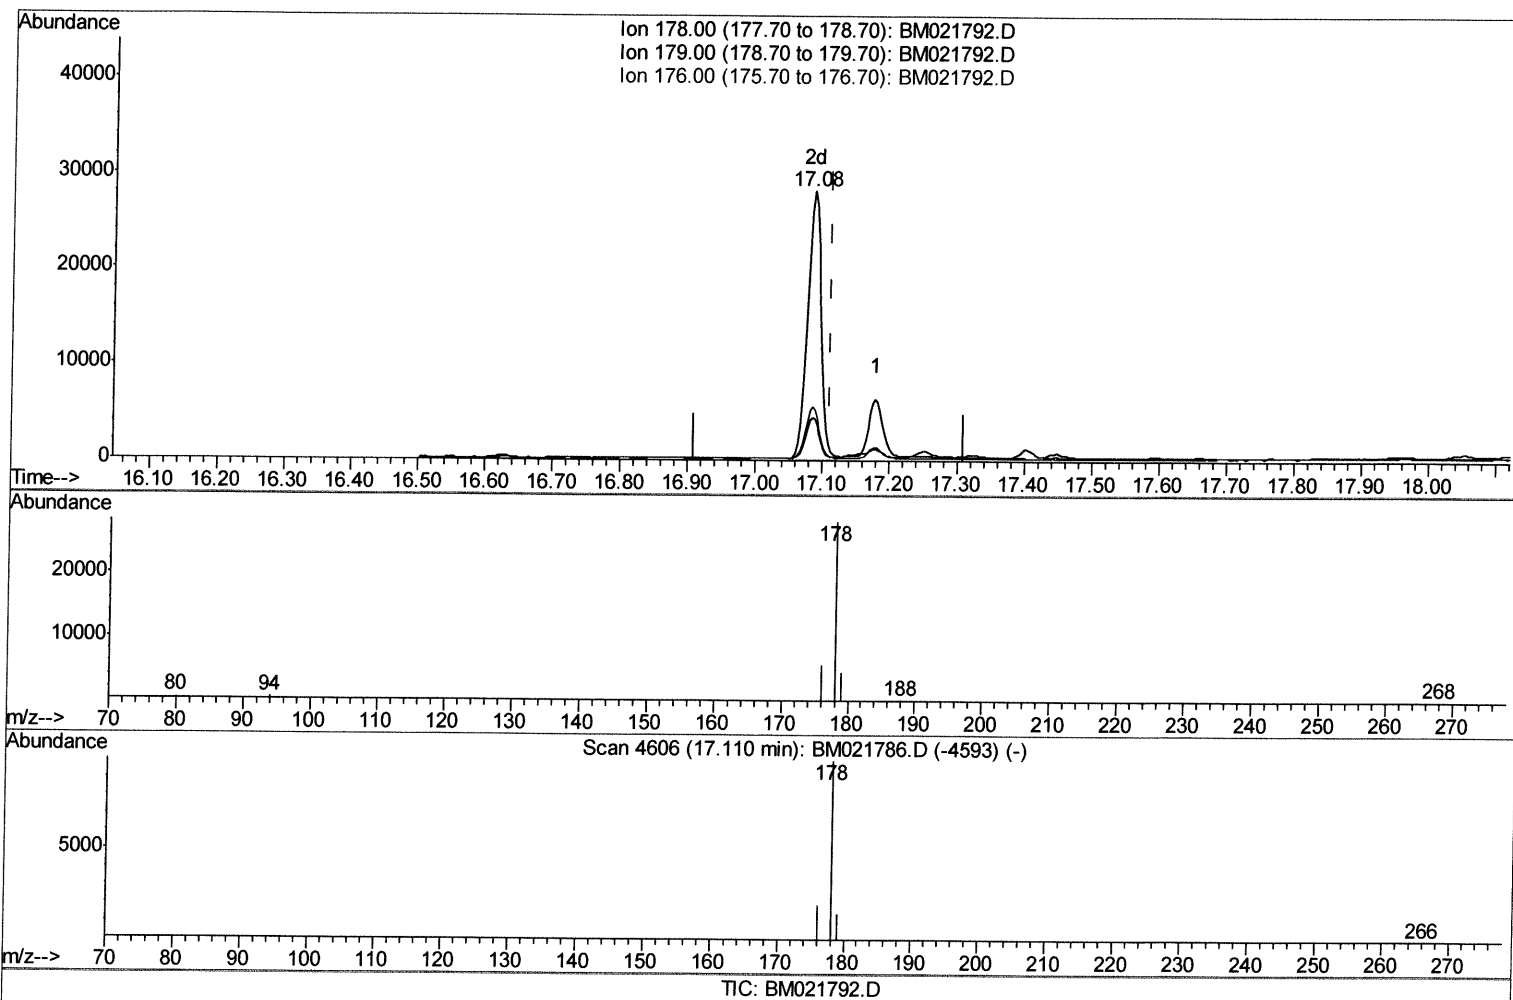

(12) Phenanthrene

17.084min (-0.026) 1.84ng/ul m *JU* 08/05/19

response 39770

Ion	Exp%	Act%
178.00	100	100
179.00	17.70	16.07
176.00	21.00	20.15
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021792.D
Acq On : 04 Aug 2019 02:39
Operator : HP/JU
Sample : K3850-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENS6

Manual Integrations
APPROVED

mohammad
8/5/2019 10:14:19 PM

Quant Time: Aug 04 05:06:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 04 04:24:24 2019
Response via : Initial Calibration

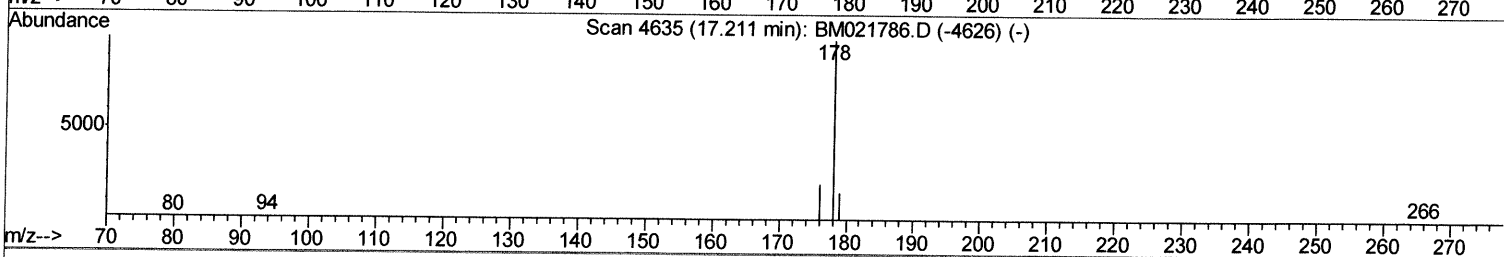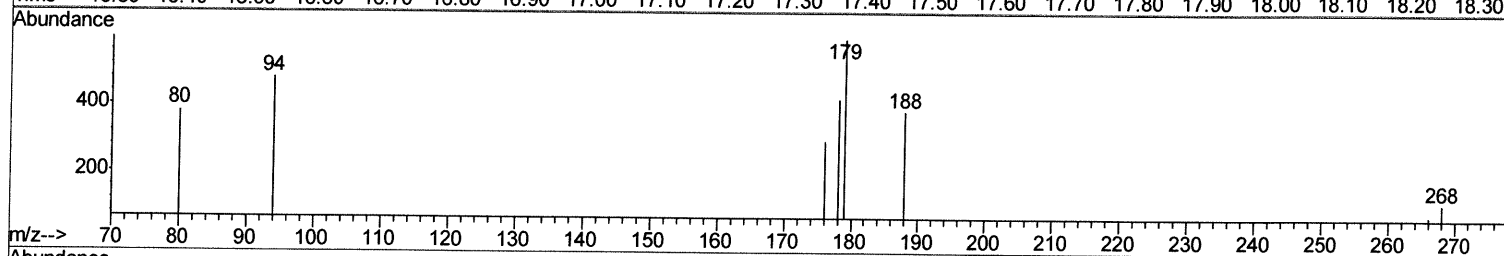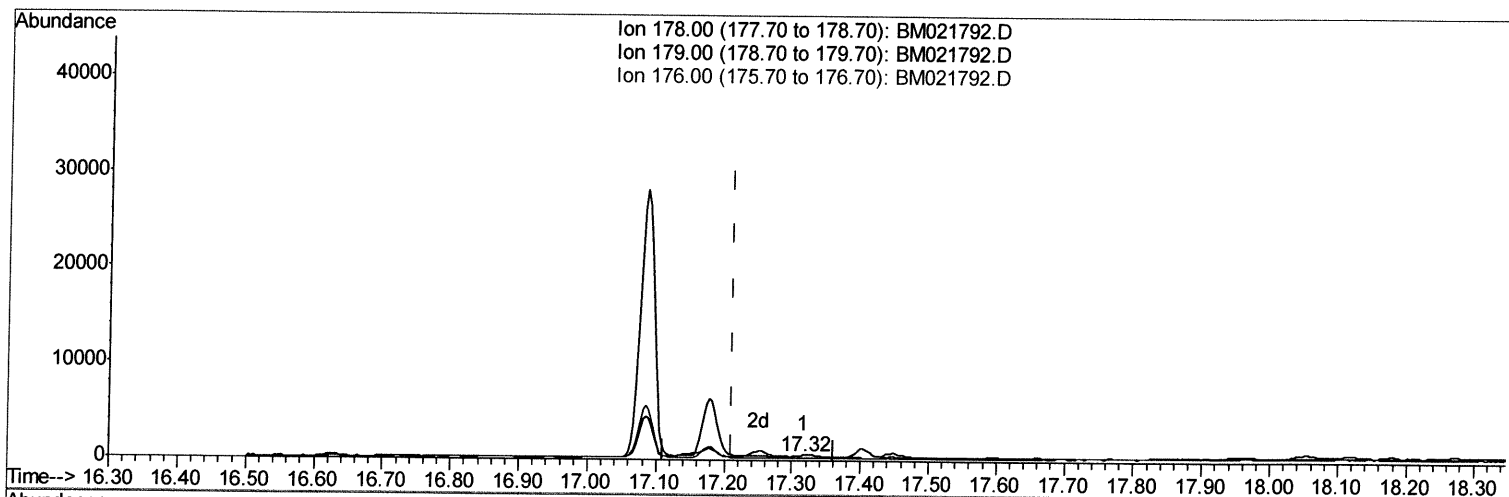

TIC: BM021792.D

(13) Anthracene

17.317min (+0.106) 0.01ng/ul

response 143

Ion	Exp%	Act%
178.00	100	100
179.00	19.40	142.14#
176.00	20.80	70.24#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021792.D
Acq On : 04 Aug 2019 02:39
Operator : HP/JU
Sample : K3850-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENS6

Manual Integrations
APPROVED

mohammad
8/5/2019 10:14:19 PM

Quant Time: Aug 04 05:06:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 04 04:24:24 2019
Response via : Initial Calibration

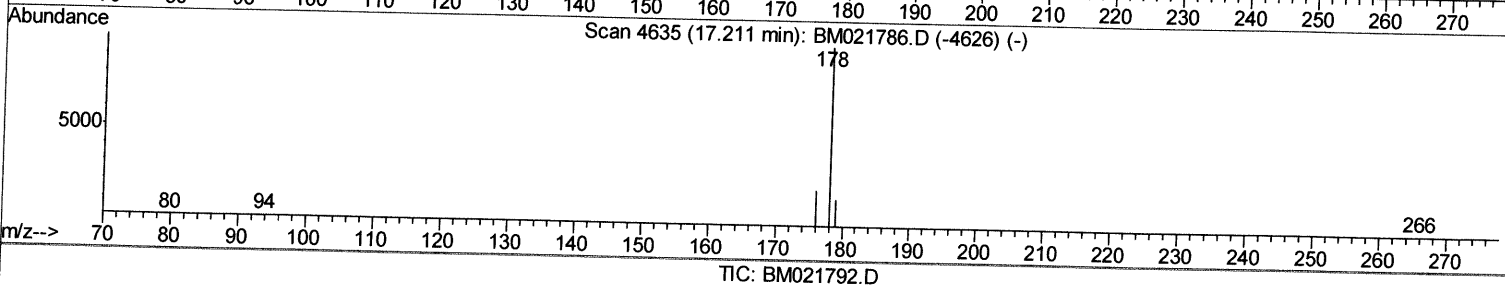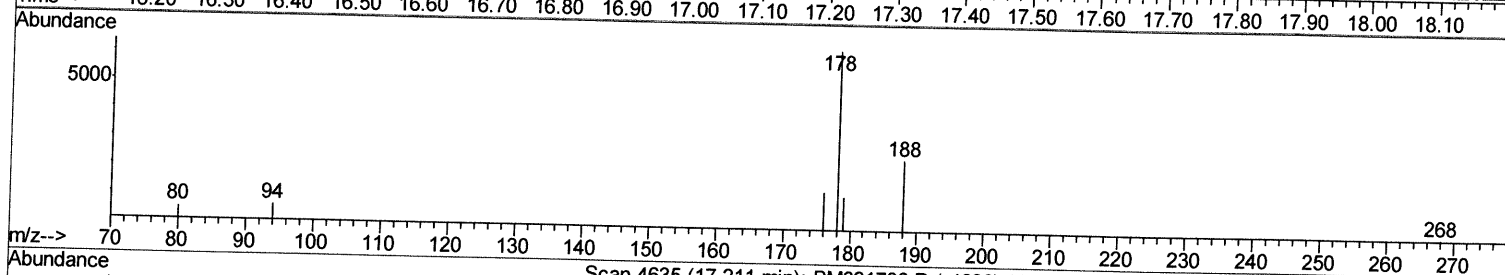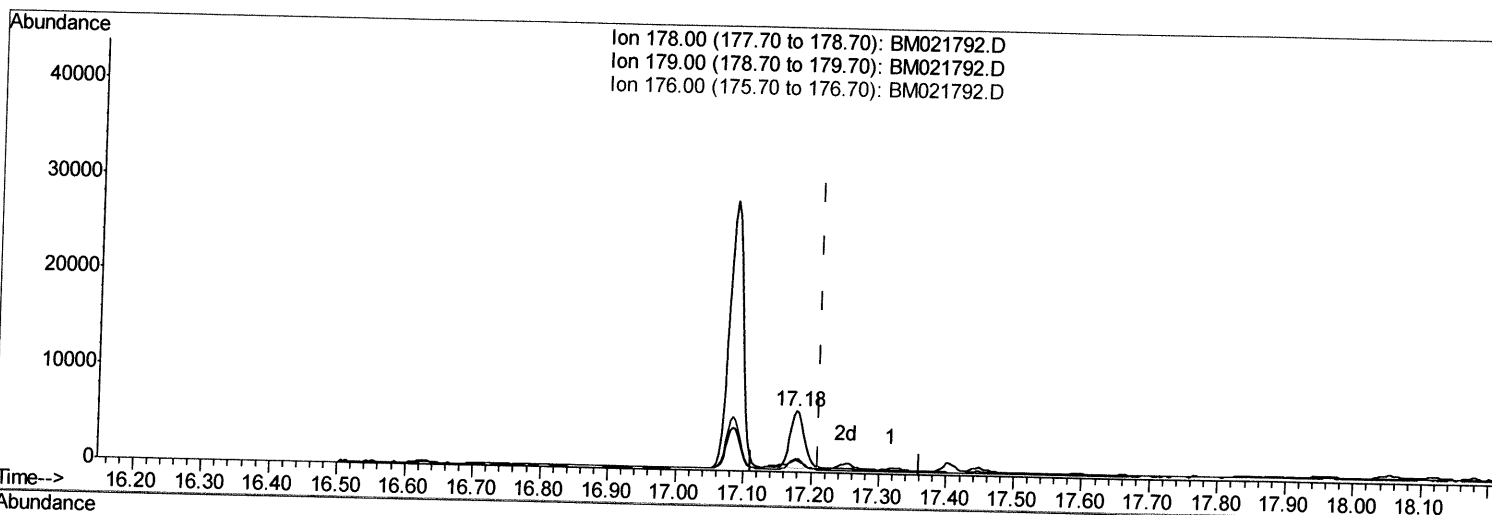

(13) Anthracene

17.178min (-0.033) 0.47ng/ul m 08/05/19

response 8722

Ion	Exp%	Act%
178.00	100	100
179.00	19.40	19.53
176.00	20.80	21.97
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021792.D
Acq On : 04 Aug 2019 02:39
Operator : HP/JU
Sample : K3850-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENS6

Manual Integrations
APPROVED

mohammad
8/5/2019 10:14:19 PM

Quant Time: Aug 04 05:06:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 04 04:24:24 2019
Response via : Initial Calibration

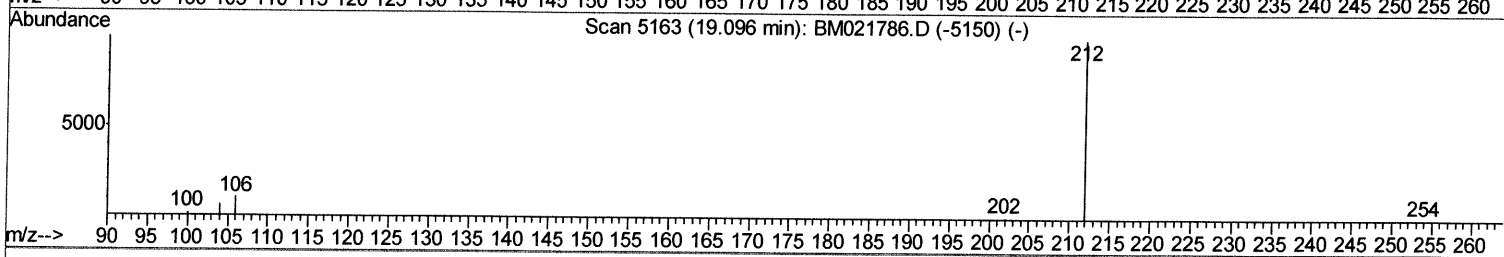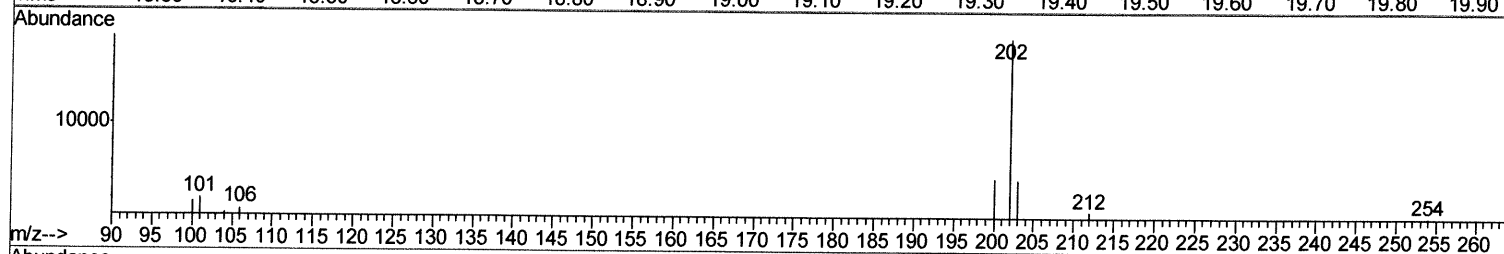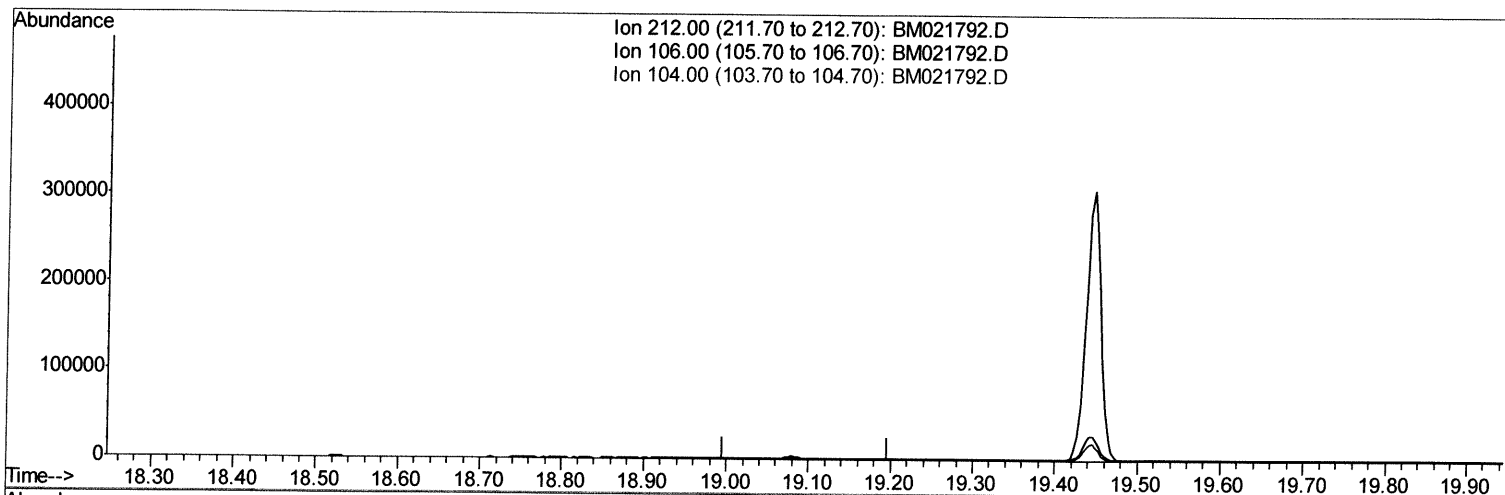

TIC: BM021792.D

(14) Fluoranthene-d10 (SURR)

19.096min (-19.096) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	9.90	0.00#
104.00	6.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021792.D
Acq On : 04 Aug 2019 02:39
Operator : HP/JU
Sample : K3850-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENS6

Manual Integrations
APPROVED

mohammad
8/5/2019 10:14:19 PM

Quant Time: Aug 04 05:06:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 04 04:24:24 2019
Response via : Initial Calibration

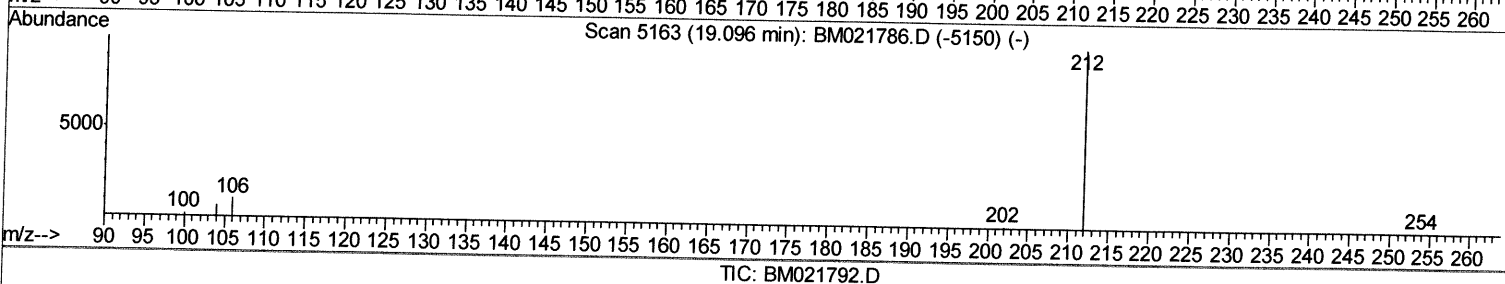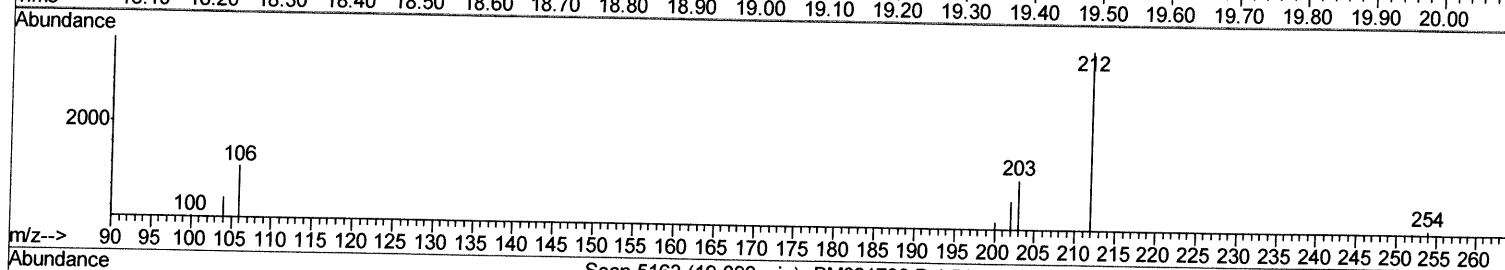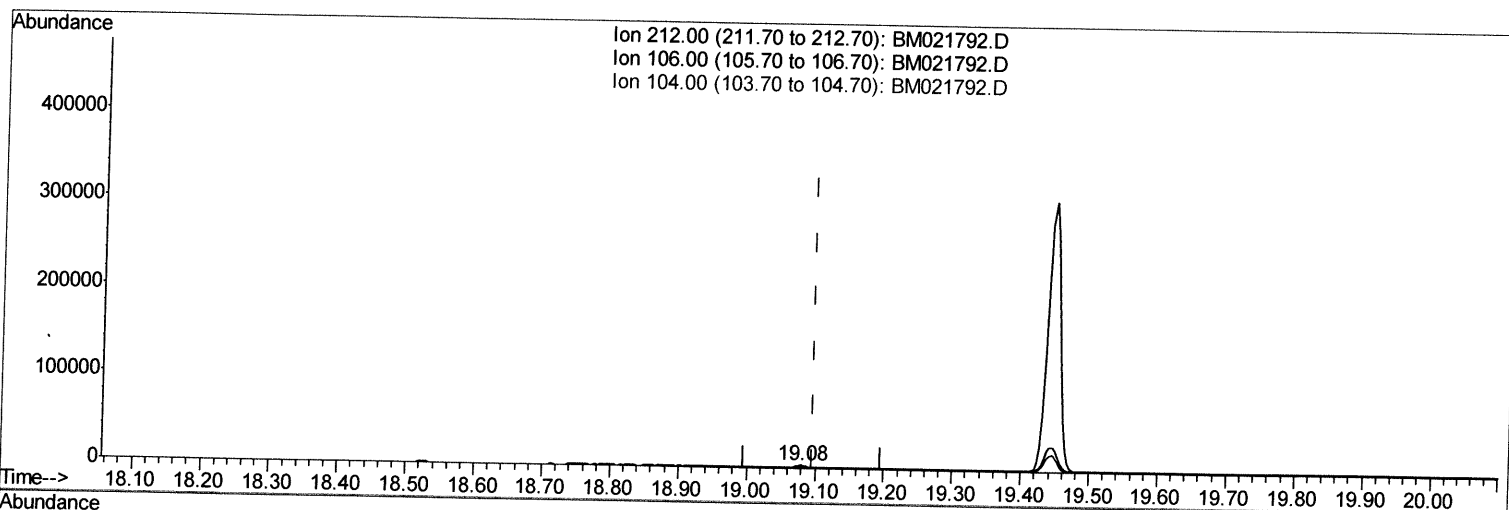

TIC: BM021792.D

(14) Fluoranthene-d10 (SURR)

19.079min (-0.017) 0.20ng/ul m

JU
08/05/19

response 4916

Ion	Exp%	Act%
212.00	100	100
106.00	9.90	0.00#
104.00	6.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021792.D
Acq On : 04 Aug 2019 02:39
Operator : HP/JU
Sample : K3850-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENS6

Manual Integrations
APPROVED

mohammad
8/5/2019 10:14:19 PM

Quant Time: Aug 04 05:06:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 04 04:24:24 2019
Response via : Initial Calibration

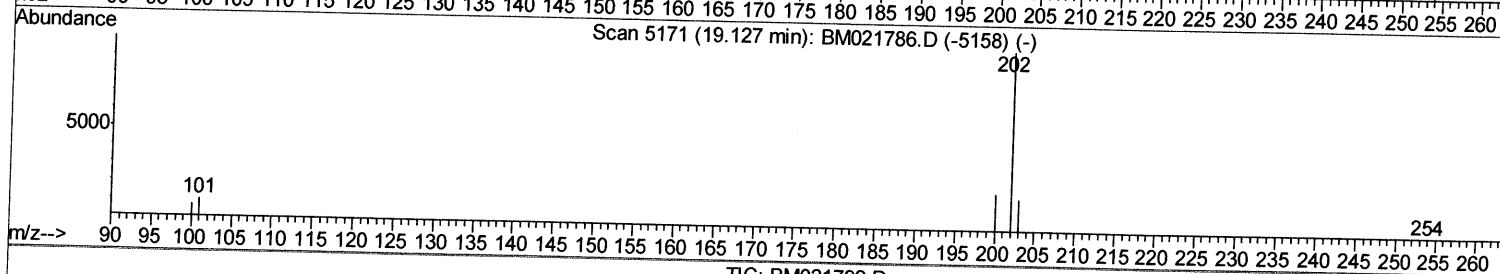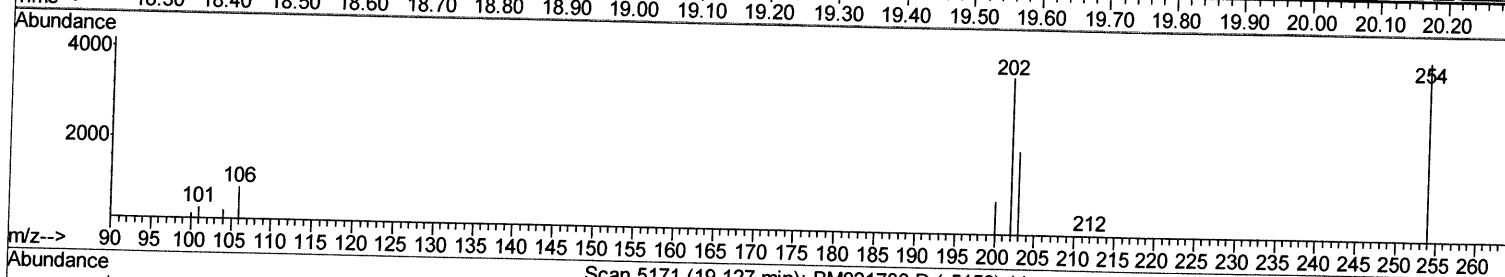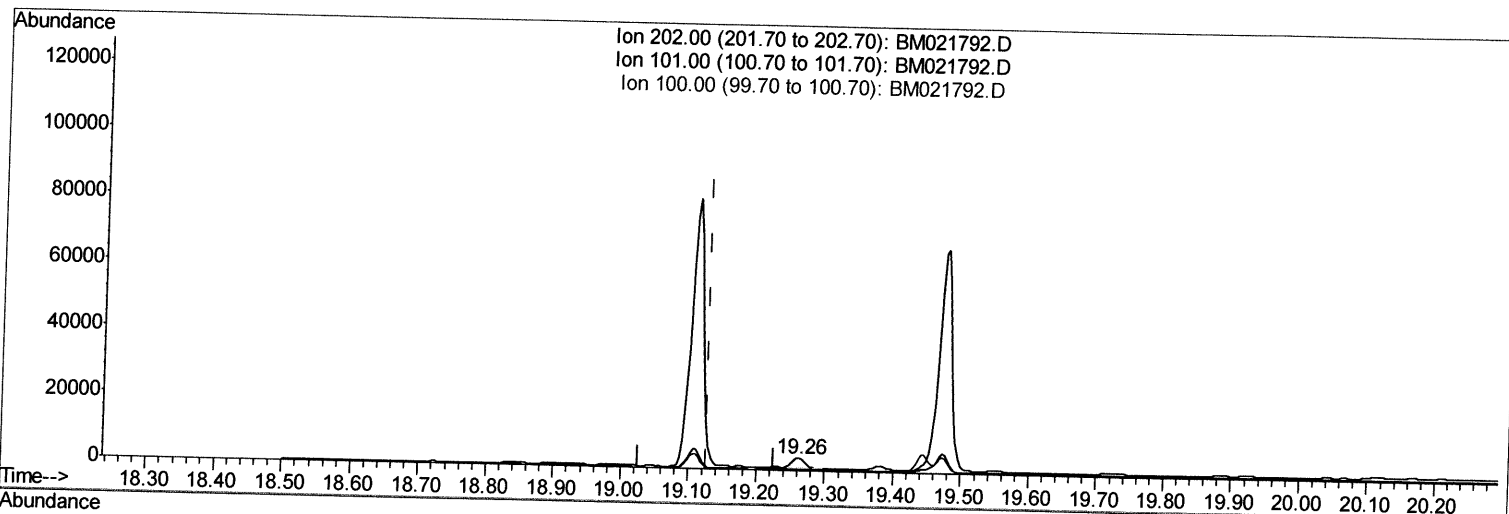

TIC: BM021792.D

(15) Fluoranthene (C)

19.262min (+0.135) 0.13ng/ul

response 3896

Ion	Exp%	Act%
202.00	100	100
101.00	10.20	12.60
100.00	8.10	9.20
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)



Data File : BM021792.D
Acq On : 04 Aug 2019 02:39
Operator : HP/JU
Sample : K3850-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENS6

Manual Integrations
APPROVED

mohammad
8/5/2019 10:14:19 PM

Quant Time: Aug 04 05:06:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 04 04:24:24 2019
Response via : Initial Calibration

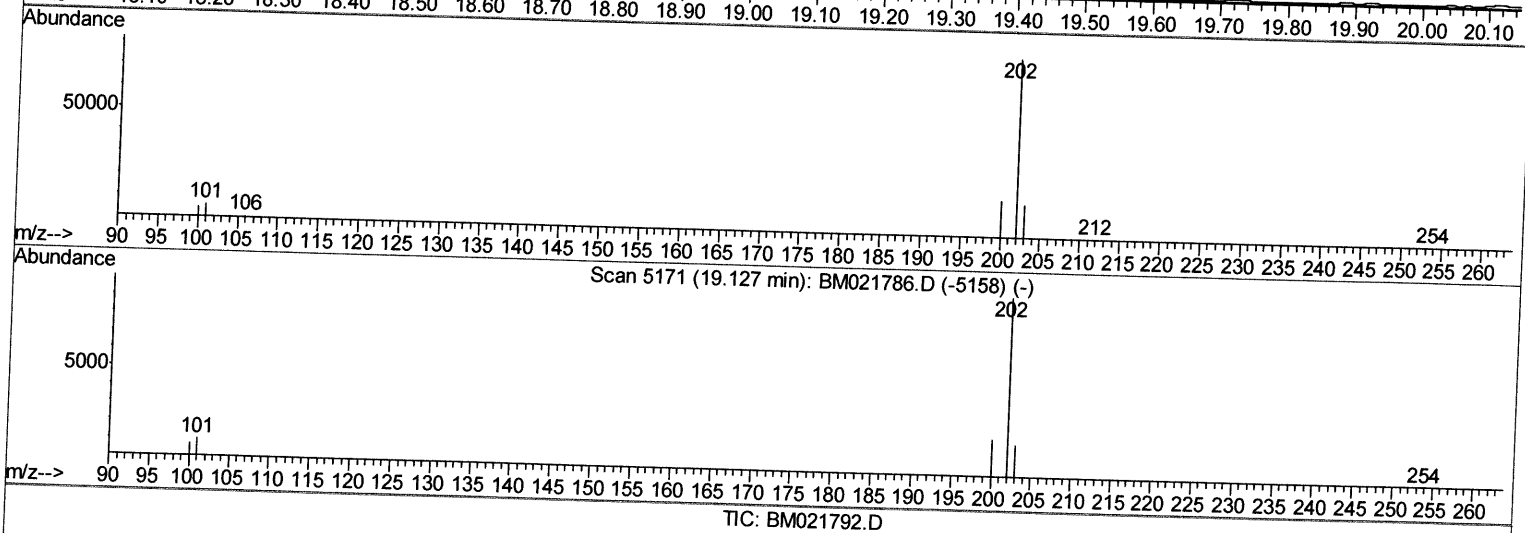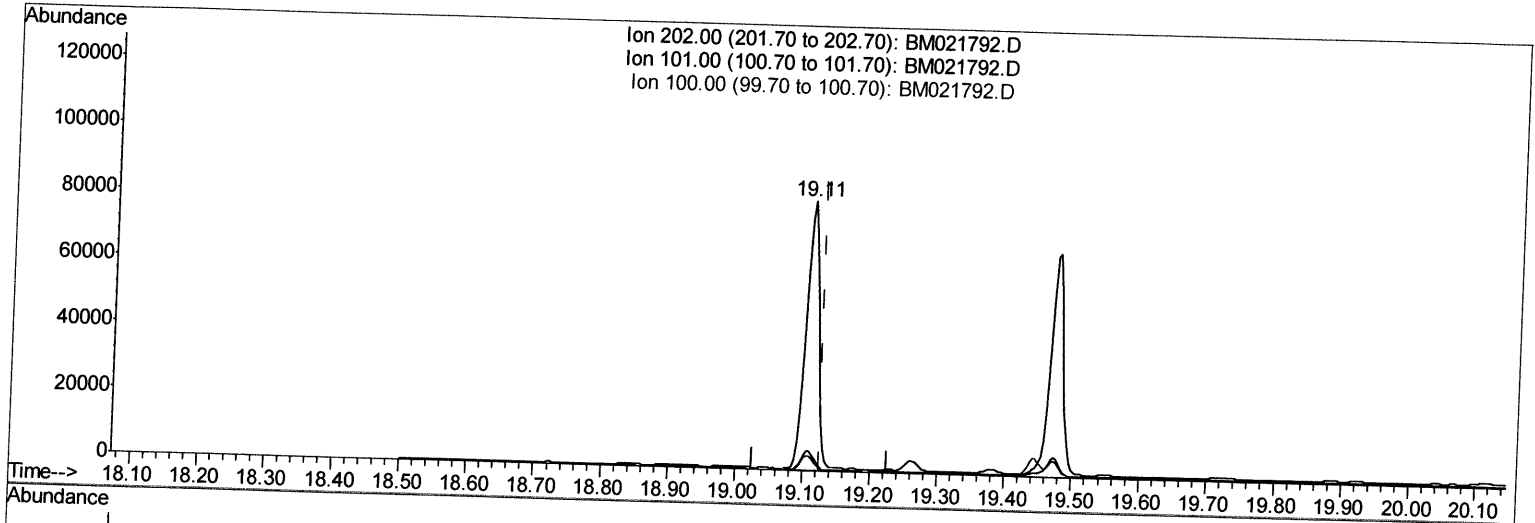

(15) Fluoranthene (C)

19.110min (-0.017) 3.62ng/ul m ^{JU} 08/05/19

response 105093

Ion	Exp%	Act%
202.00	100	100
101.00	10.20	7.23
100.00	8.10	5.51
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021792.D
Acq On : 04 Aug 2019 02:39
Operator : HP/JU
Sample : K3850-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENS6

Manual Integrations
APPROVED

mohammad
8/5/2019 10:14:19 PM

Quant Time: Aug 04 05:06:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 04 04:24:24 2019
Response via : Initial Calibration

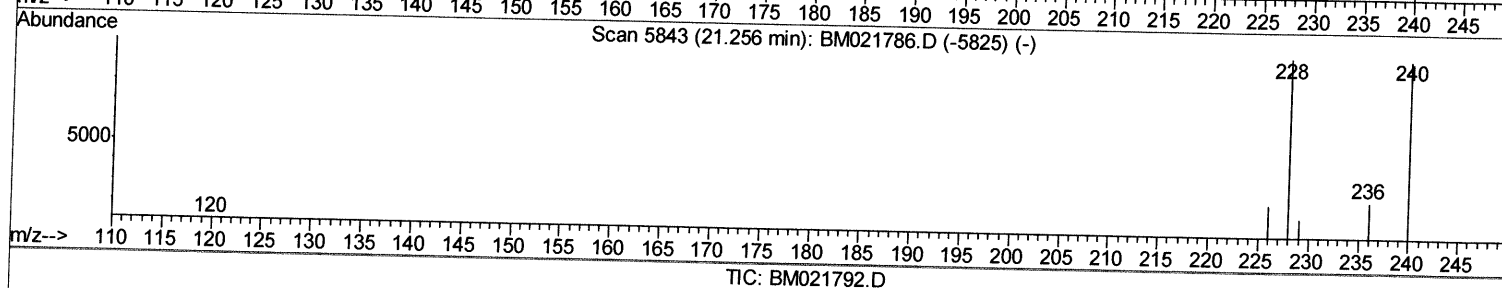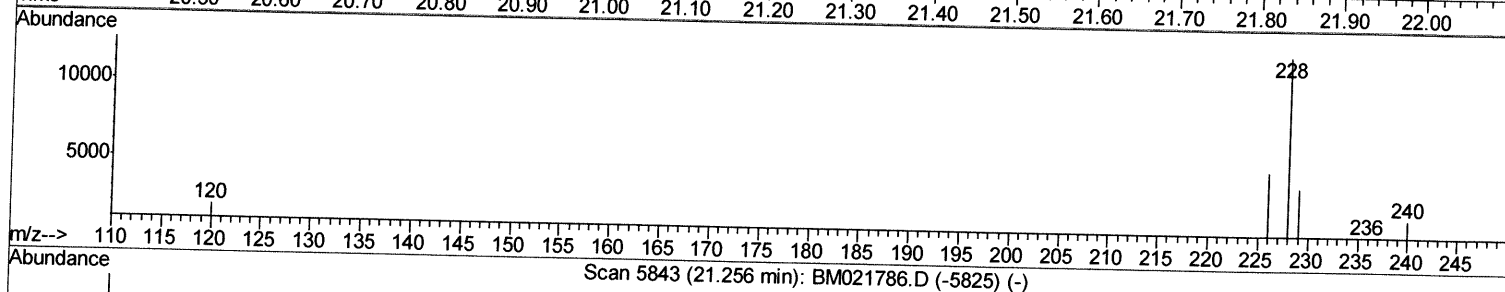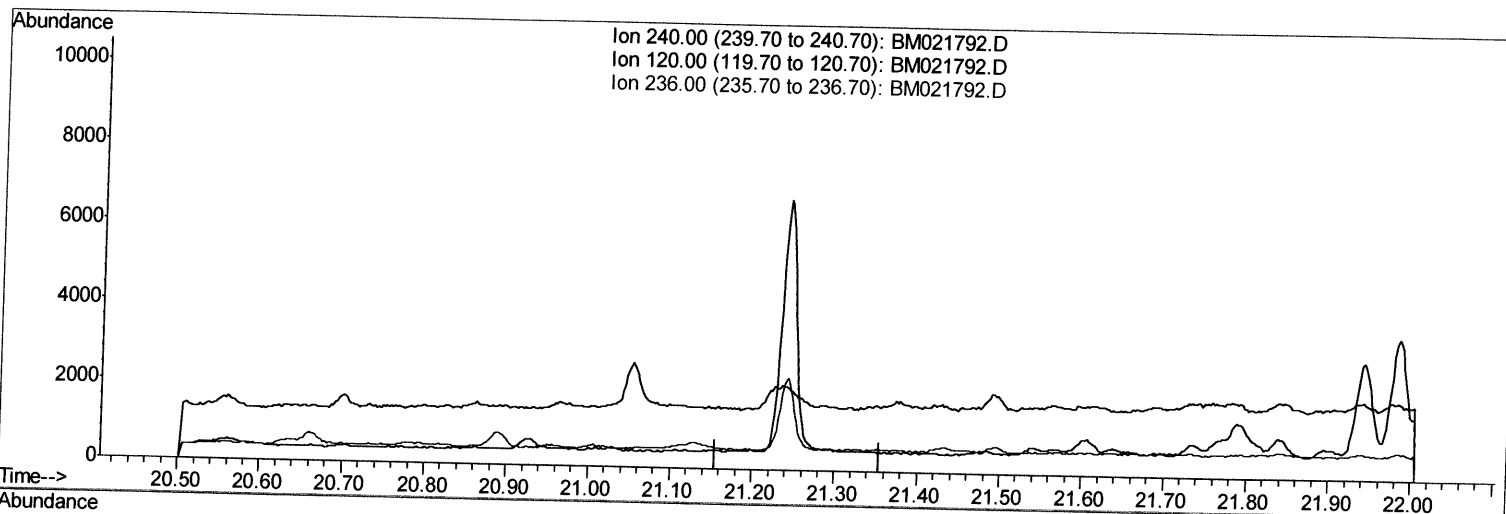

(16) Chrysene-d12 (I)

21.256min (-21.256) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.20	0.00#
236.00	32.30	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021792.D
Acq On : 04 Aug 2019 02:39
Operator : HP/JU
Sample : K3850-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENS6

Manual Integrations
APPROVED

mohammad
8/5/2019 10:14:19 PM

Quant Time: Aug 04 05:06:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 04 04:24:24 2019
Response via : Initial Calibration

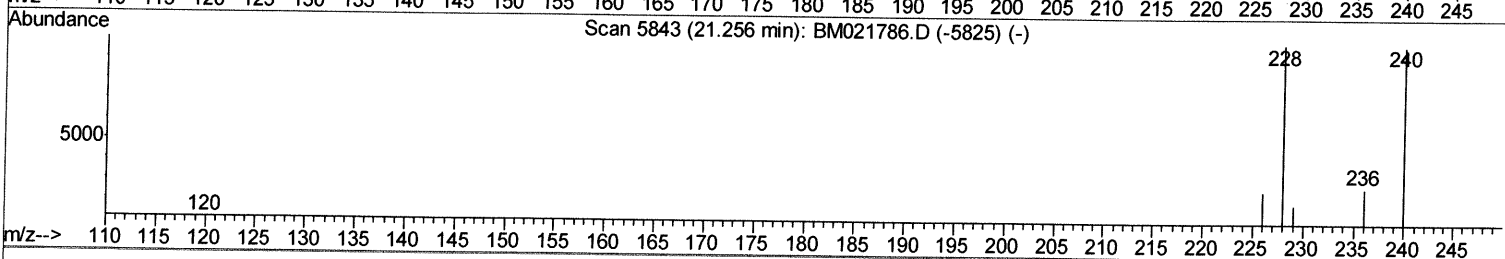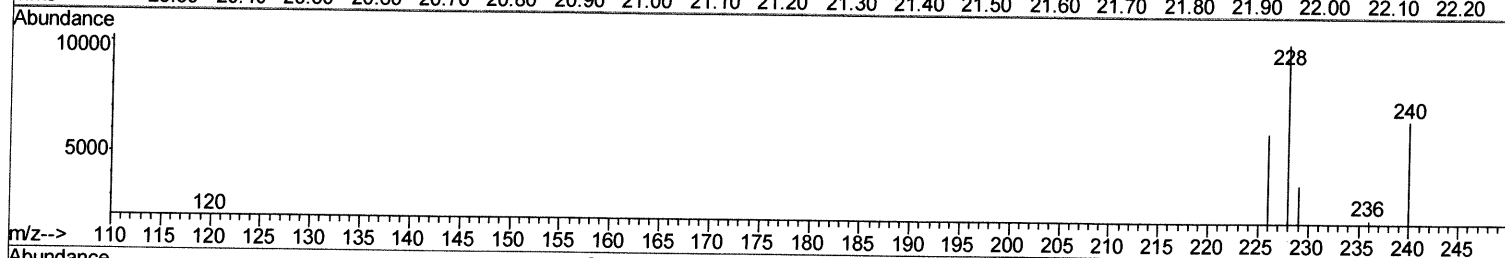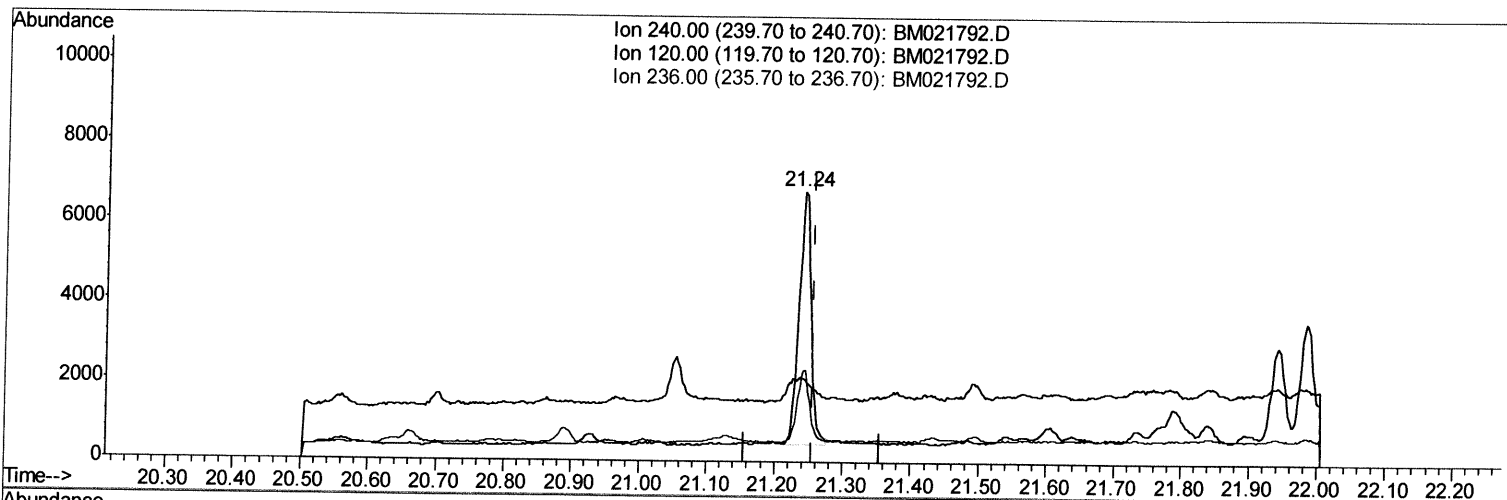

TIC: BM021792.D

(16) Chrysene-d12 (I)

21.241min (-0.015) 0.40ng/ul m ^{JU} 08/05/19

response 7822

Ion	Exp%	Act%
240.00	100	100
120.00	16.20	30.99#
236.00	32.30	33.66
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021792.D
Acq On : 04 Aug 2019 02:39
Operator : HP/JU
Sample : K3850-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENS6

Manual Integrations
APPROVED

mohammad
8/5/2019 10:14:19 PM

Quant Time: Aug 04 05:07:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 04 04:24:24 2019
Response via : Initial Calibration

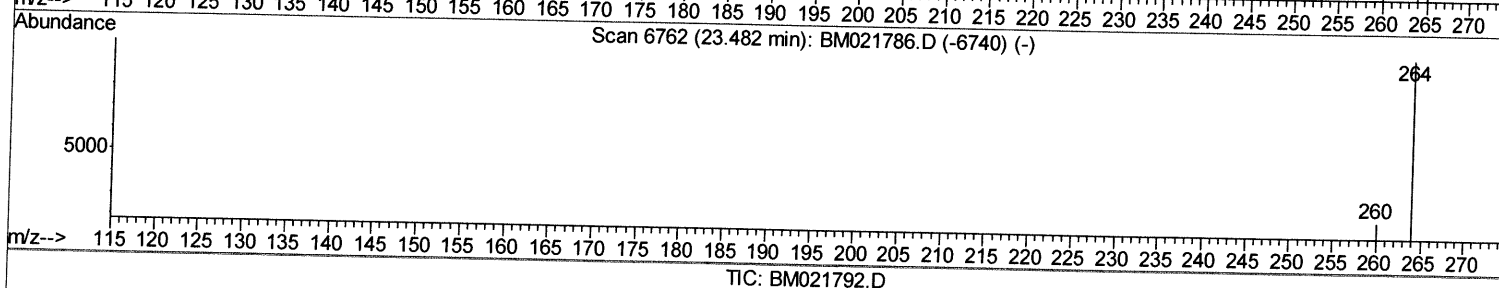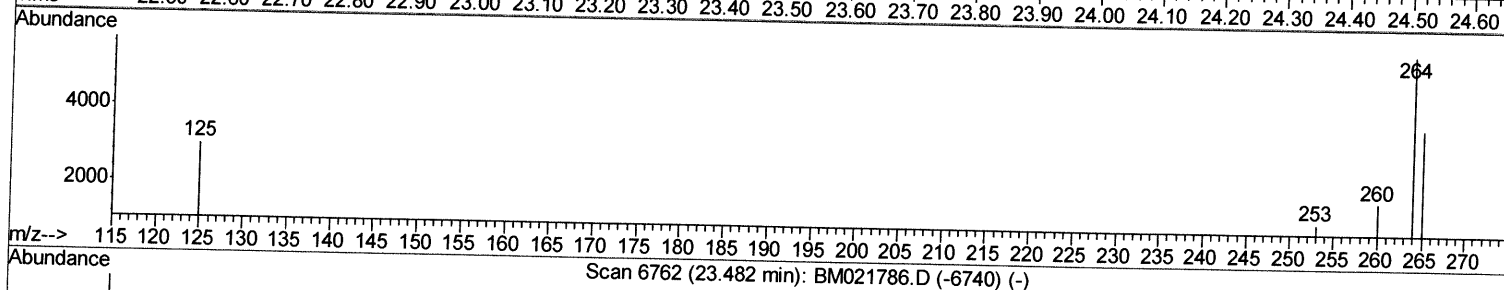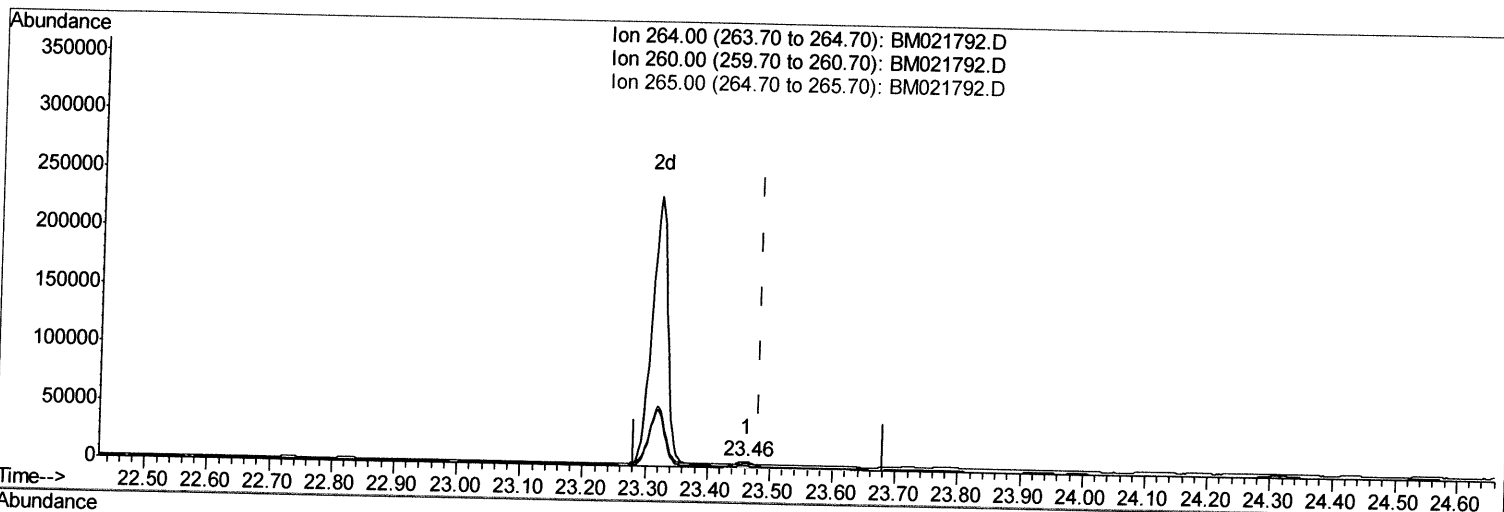

(20) Perylene-d12 (I)

23.462min (-0.020) 0.40ng/ul

response 12909

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	32.80
265.00	117.00	66.64#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021792.D
Acq On : 04 Aug 2019 02:39
Operator : HP/JU
Sample : K3850-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BENS6

Manual Integrations
APPROVED

mohammad
8/5/2019 10:14:19 PM

Quant Time: Aug 04 05:07:21 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 04 04:24:24 2019
Response via : Initial Calibration

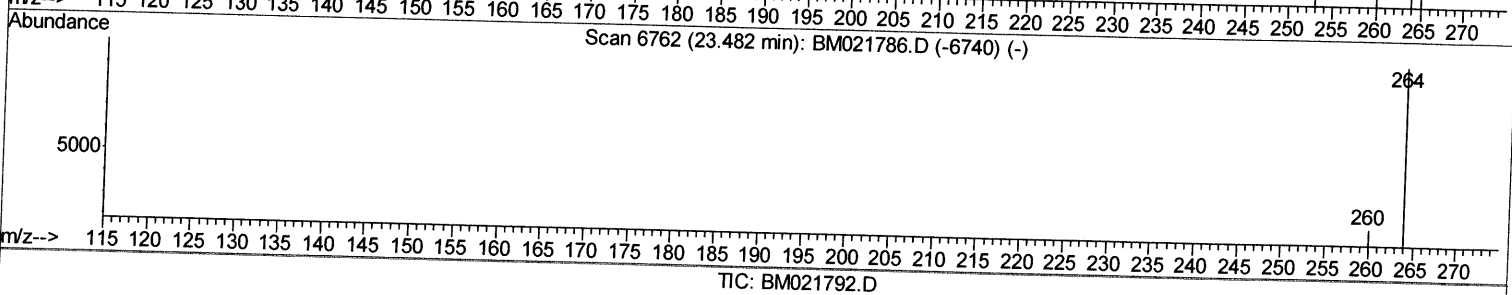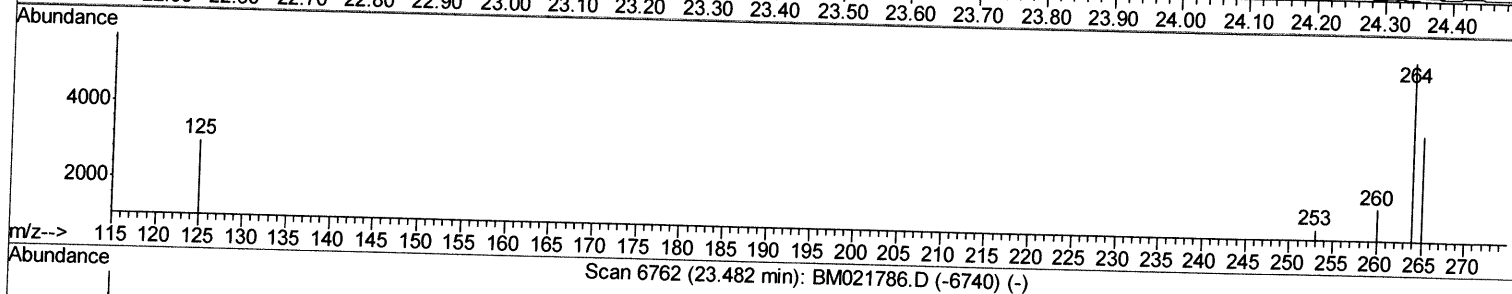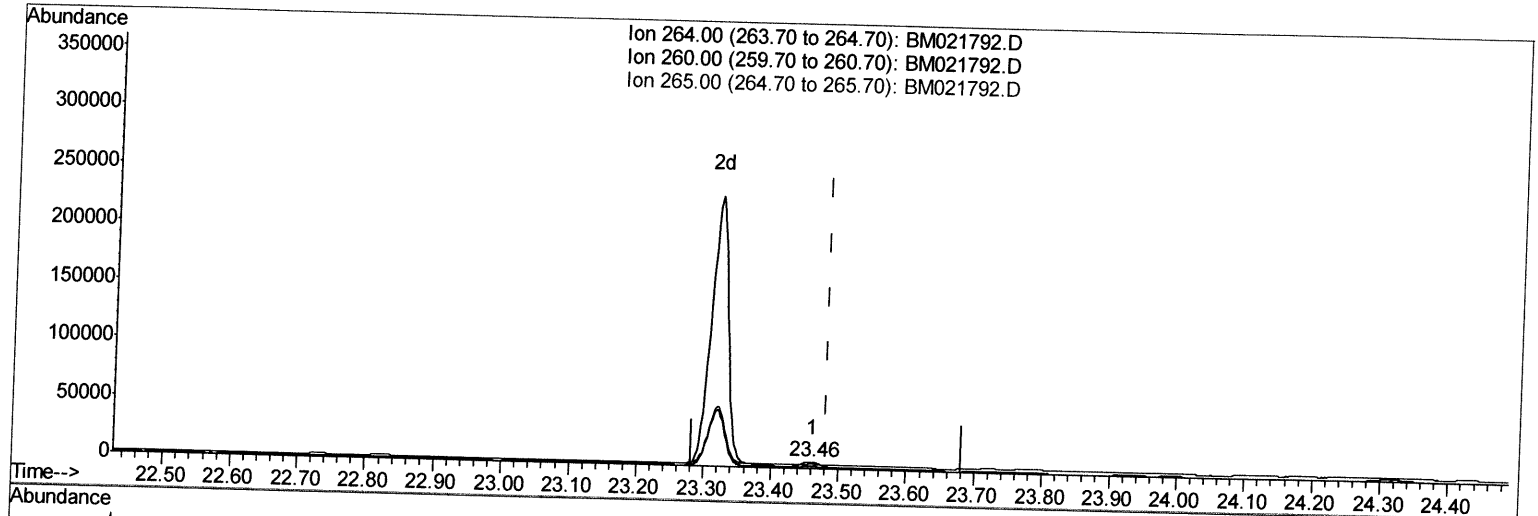

(20) Perylene-d12 (I)

23.462min (-0.020) 0.40ng/ul m 208/05/19

response 8124

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	32.80
265.00	117.00	66.64#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021792.D
Acq On : 04 Aug 2019 02:39
Operator : HP/JU
Sample : K3850-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENS6

Manual Integrations
APPROVED

mohammad
8/5/2019 10:14:19 PM

Quant Time: Aug 04 05:07:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 04 04:24:24 2019
Response via : Initial Calibration

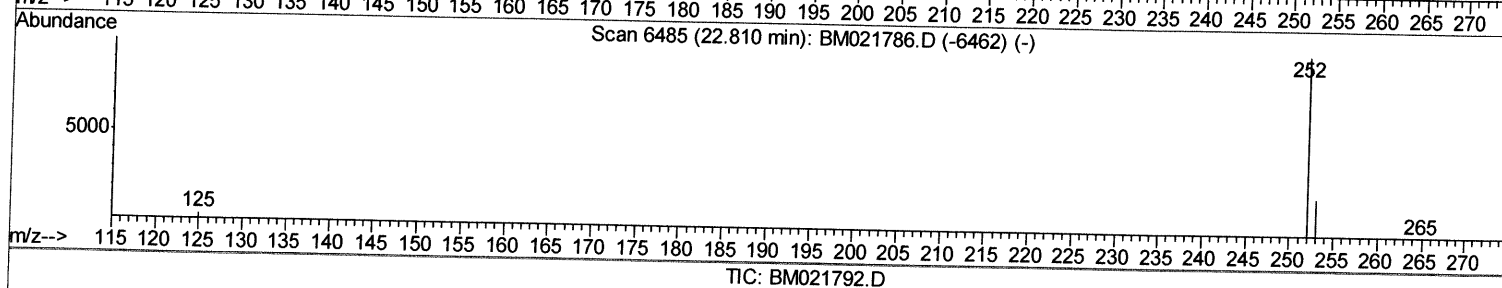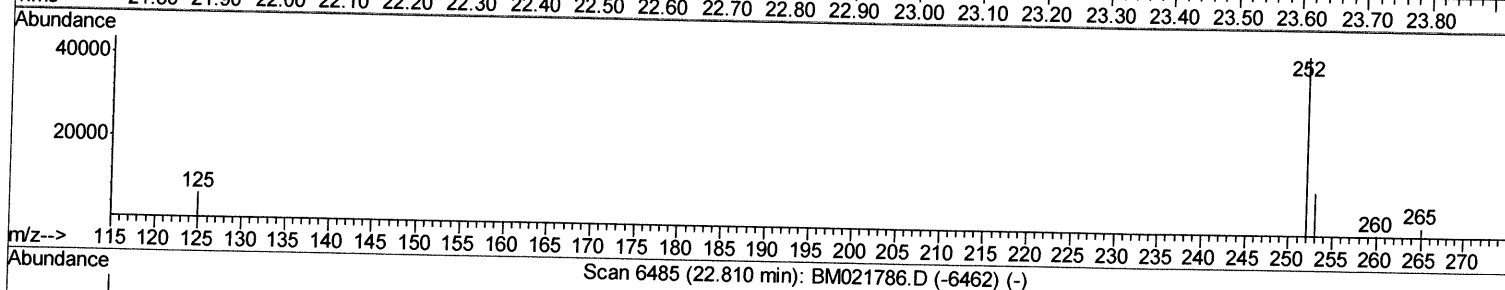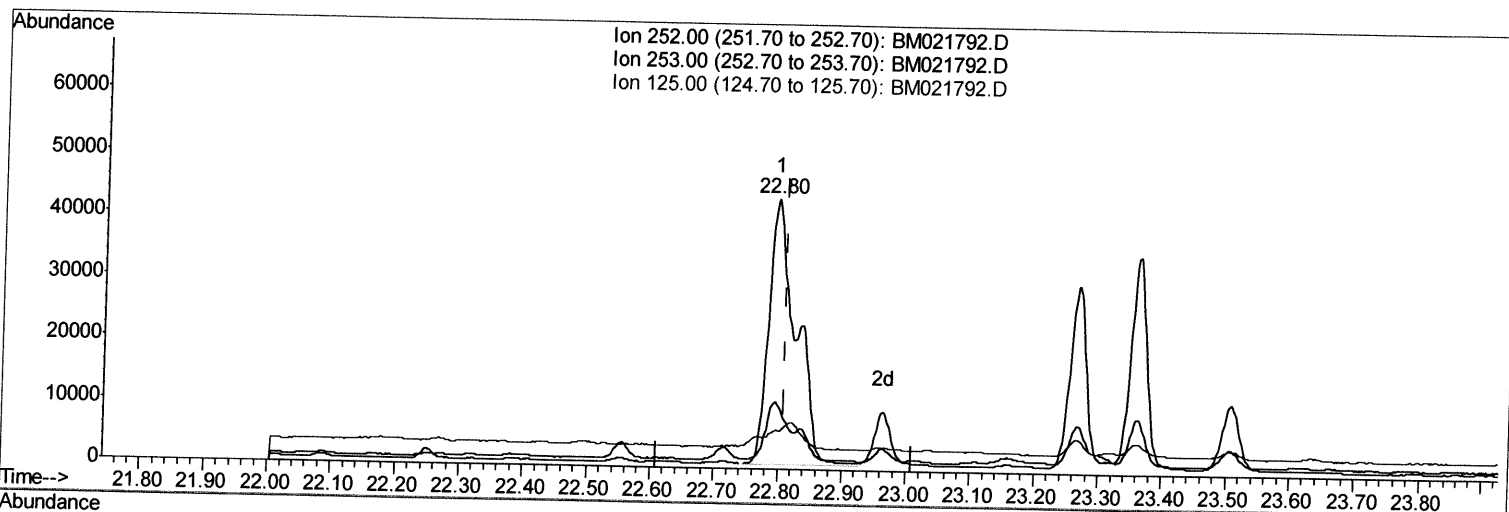

(21) Benzo(b)fluoranthene
22.795min (-0.015) 4.63ng/ul
response 126817

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	24.95
125.00	15.50	14.20
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021792.D
Acq On : 04 Aug 2019 02:39
Operator : HP/JU
Sample : K3850-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENS6

Manual Integrations
APPROVED

mohammad
8/5/2019 10:14:19 PM

Quant Time: Aug 04 05:07:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 04 04:24:24 2019
Response via : Initial Calibration

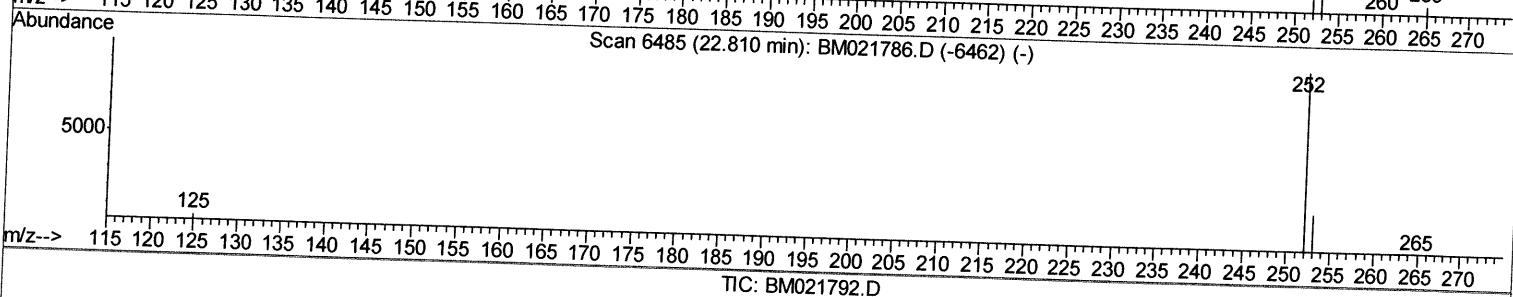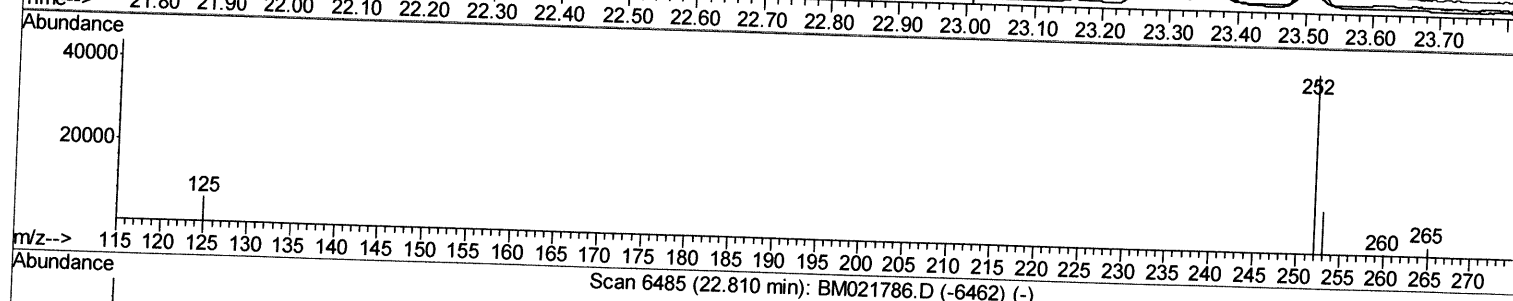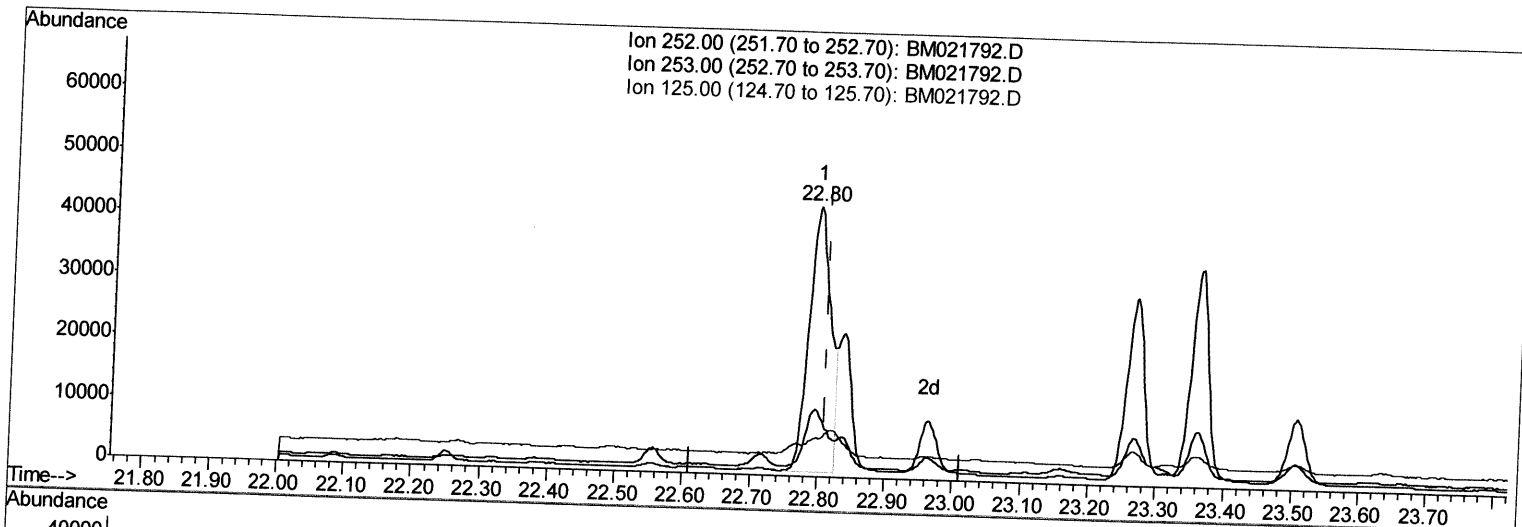

(21) Benzo(b)fluoranthene

22.795min (-0.015) 3.42ng/ul m *JU* 08/05/19

response 93725

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	24.95
125.00	15.50	14.20
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021792.D
Acq On : 04 Aug 2019 02:39
Operator : HP/JU
Sample : K3850-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENS6

Manual Integrations
APPROVED

mohammad
8/5/2019 10:14:19 PM

Quant Time: Aug 04 05:07:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 04 04:24:24 2019
Response via : Initial Calibration

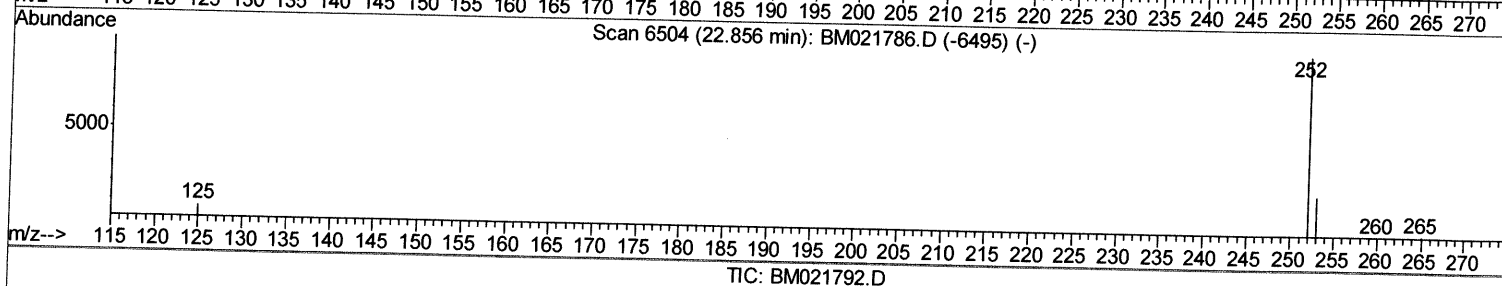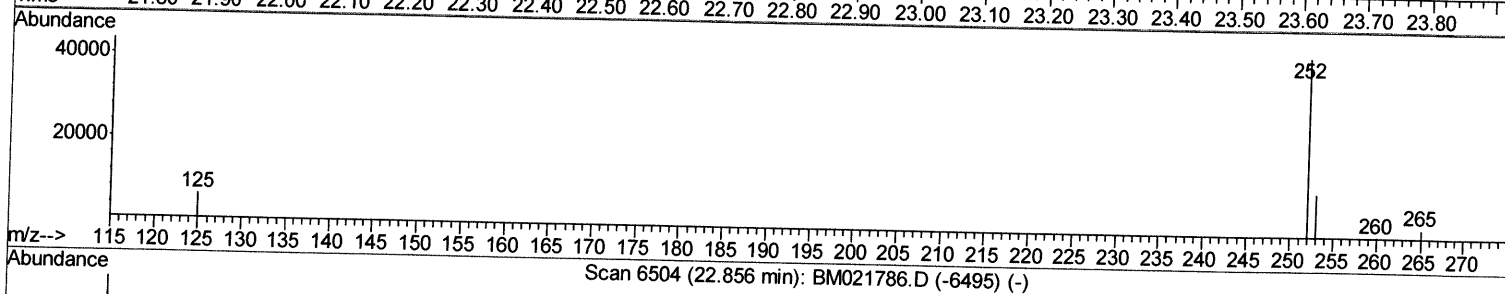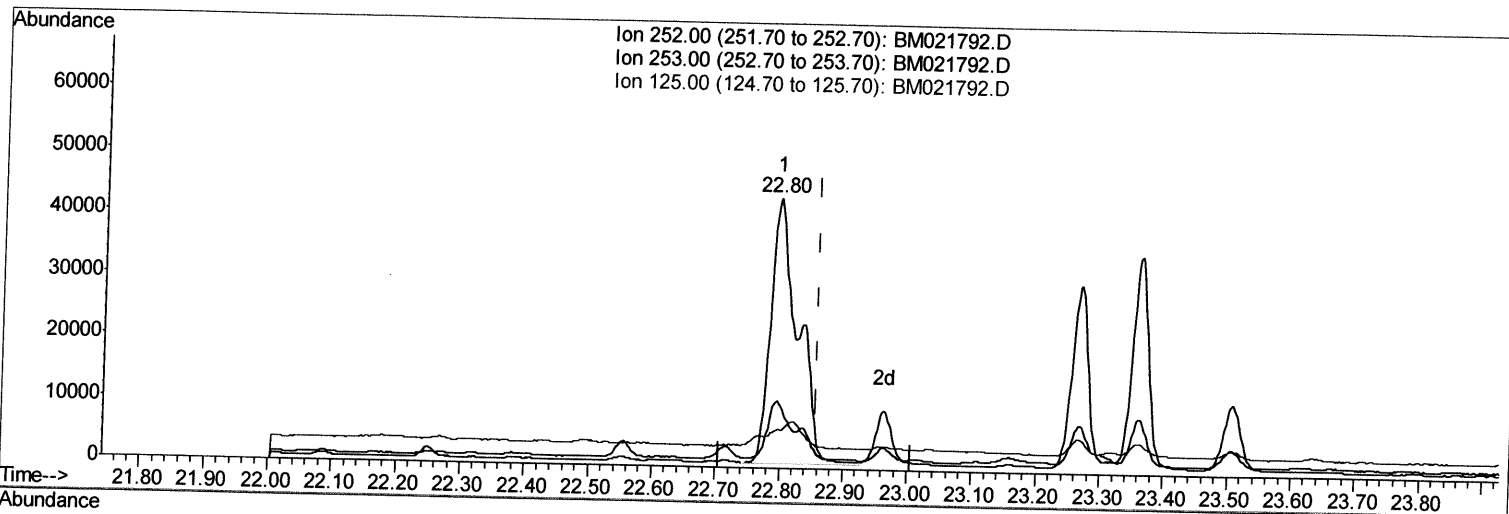

(22) Benzo(k)fluoranthene

22.795min (-0.061) 4.09ng/ul

response 126817

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	24.95#
125.00	15.20	14.20
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021792.D
Acq On : 04 Aug 2019 02:39
Operator : HP/JU
Sample : K3850-20
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENS6

Manual Integrations
APPROVED

mohammad
8/5/2019 10:14:19 PM

Quant Time: Aug 04 05:07:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 04 04:24:24 2019
Response via : Initial Calibration

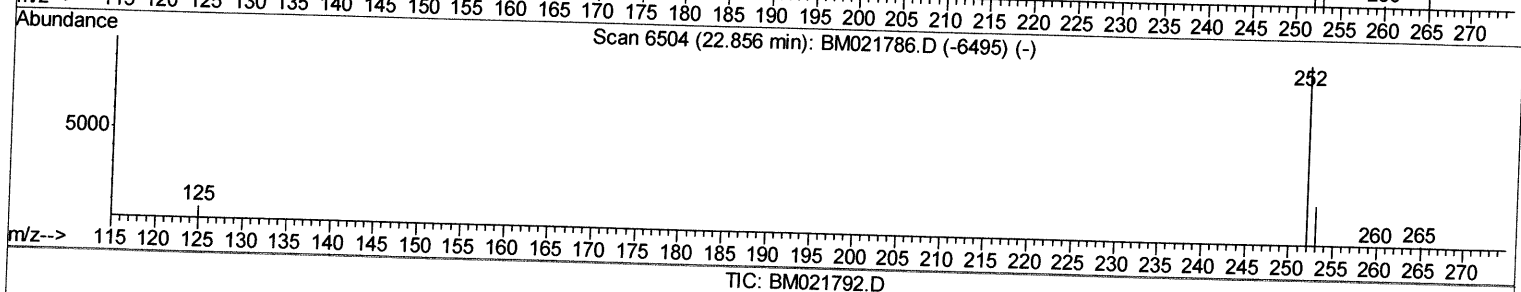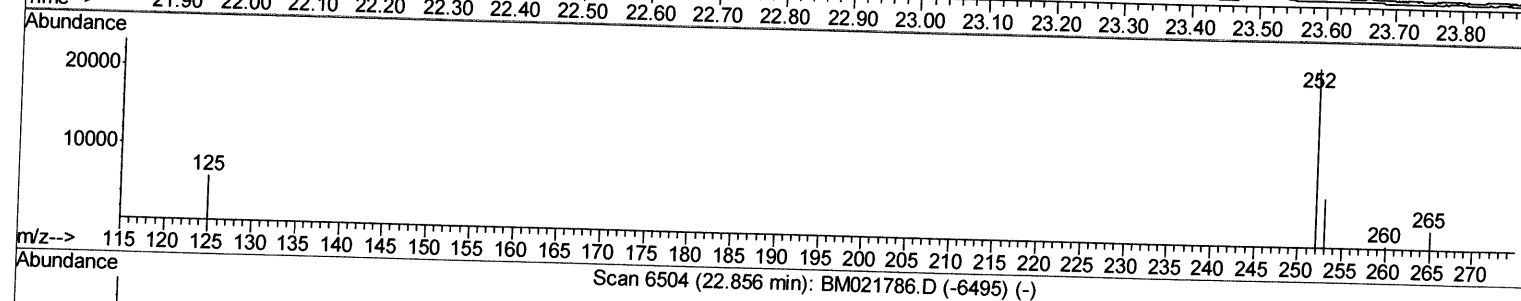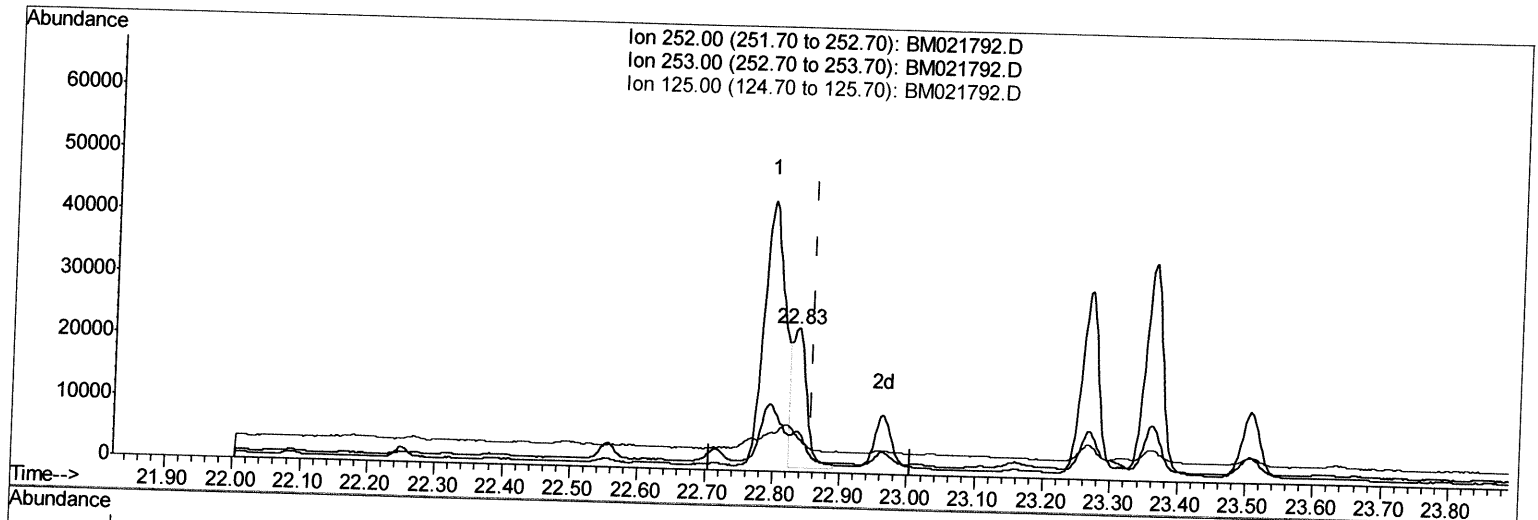

(22) Benzo(k)fluoranthene

22.834min (-0.022) 1.09ng/ul m *JU* 08/05/19

response 33919

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	28.46
125.00	15.20	25.71#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\

Quantitation Report (QT Reviewed)

Data File : BM021792.D

Acq On : 04 Aug 2019 02:39

Operator : HP/JU

Sample : K3850-20

Misc :

ALS Vial : 35 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

BENS6

Manual Integrations

APPROVED

mohammad

8/5/2019 10:14:19 PM

Quant Time: Aug 04 05:08:24 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun Aug 04 04:24:24 2019

Response via : Initial Calibration

Internal Standards

	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	1124	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	4493	0.40	ng/ul	-0.03
6) Acenaphthene-d10	14.29	164	2810	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.04	188	7447m >	0.40	ng/ul	-0.03
16) Chrysene-d12	21.24	240	7822m >	0.40	ng/ul	-0.01
20) Perylene-d12	23.46	264	8124m >	0.40	ng/ul	-0.02

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.02	152	1312	0.18	ng/ul	-0.03
14) Fluoranthene-d10	19.08	212	4916m >	0.20	ng/ul	-0.02

Target Compounds

					Qvalue
3) Naphthalene	10.47	128	1832	0.144	ng/ul 97
5) 2-Methylnaphthalene	12.09	142	1724	0.204	ng/ul 96
7) Acenaphthylene	14.01	152	7458	0.569	ng/ul 96
8) Acenaphthene	14.35	153	1078	0.101	ng/ul 95
9) Fluorene	15.34	166	1908	0.160	ng/ul# 98
12) Phenanthrene	17.08	178	39770m >	1.835	ng/ul > 97
13) Anthracene	17.18	178	8722m >	0.472	ng/ul > 97
15) Fluoranthene	19.11	202	105093m >	3.621	ng/ul > 97
17) Pyrene	19.48	202	90000	2.800	ng/ul# 94
18) Benzo(a)anthracene	21.23	228	52592	1.880	ng/ul 96
19) Chrysene	21.28	228	60405	1.679	ng/ul 96
21) Benzo(b)fluoranthene	22.80	252	93725m >	3.421	ng/ul > 97
22) Benzo(k)fluoranthene	22.83	252	33919m >	1.094	ng/ul > 97
23) Benzo(a)pyrene	23.36	252	60677	2.178	ng/ul# 82
24) Indeno(1,2,3-cd)pyrene	25.68	276	56343	1.694	ng/ul# 87
25) Dibenzo(a,h)anthracene	25.69	278	12406	0.461	ng/ul# 80
26) Benzo(g,h,i)perylene	26.36	276	62681	2.093	ng/ul# 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed