


Data File : BM021807.D
Acq On : 04 Aug 2019 11:44
Operator : HP/JU
Sample : K3850-17
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 05 05:54:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 05:26:43 2019
Response via : Initial Calibration

Instrument :
BNA_M
Client Sample Id :
BENS3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:15:22 PM

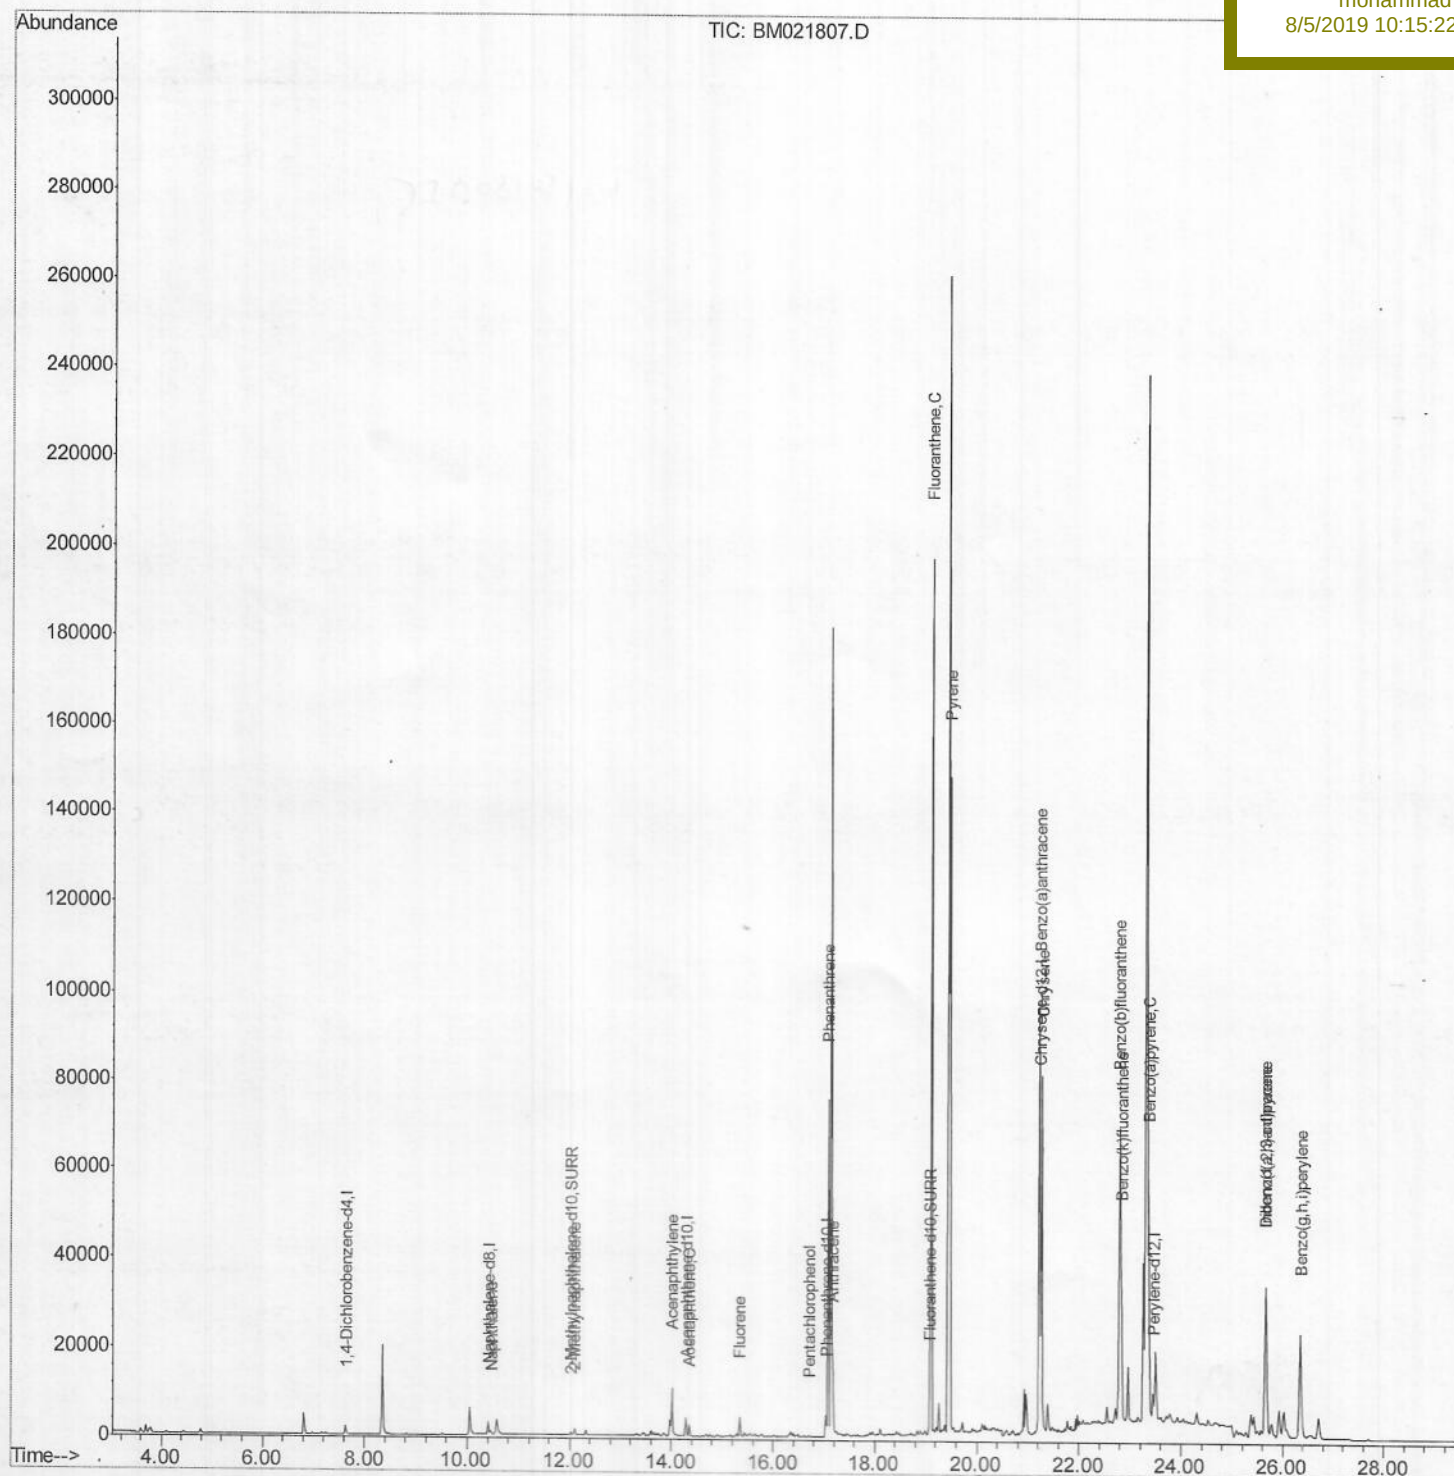

Data File : BM021807.D

Acq On : 04 Aug 2019 11:44

Operator : HP/JU

Sample : K3850-17

Misc :

ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 05 05:29:49 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Aug 05 05:26:43 2019

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




BENS3

Manual Integrations

APPROVED

mohammad

8/5/2019 10:15:22 PM

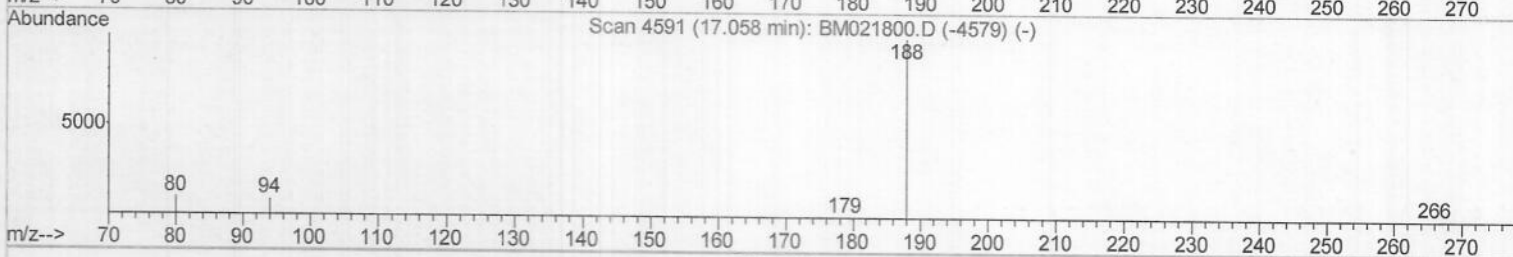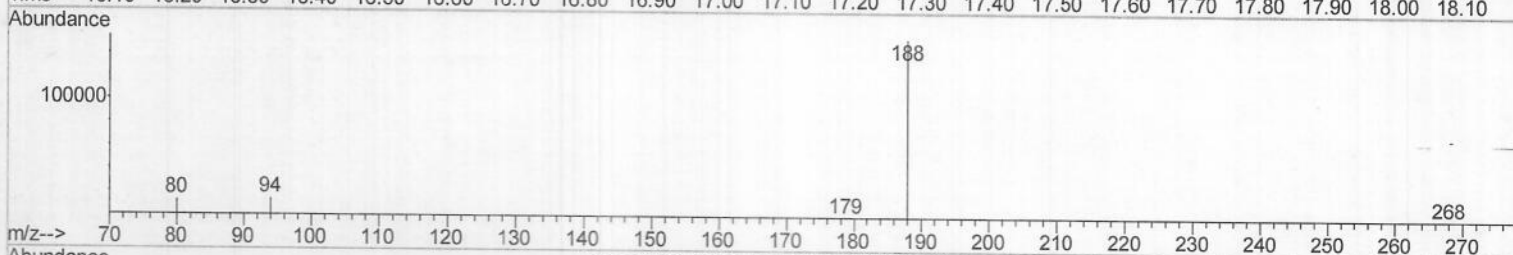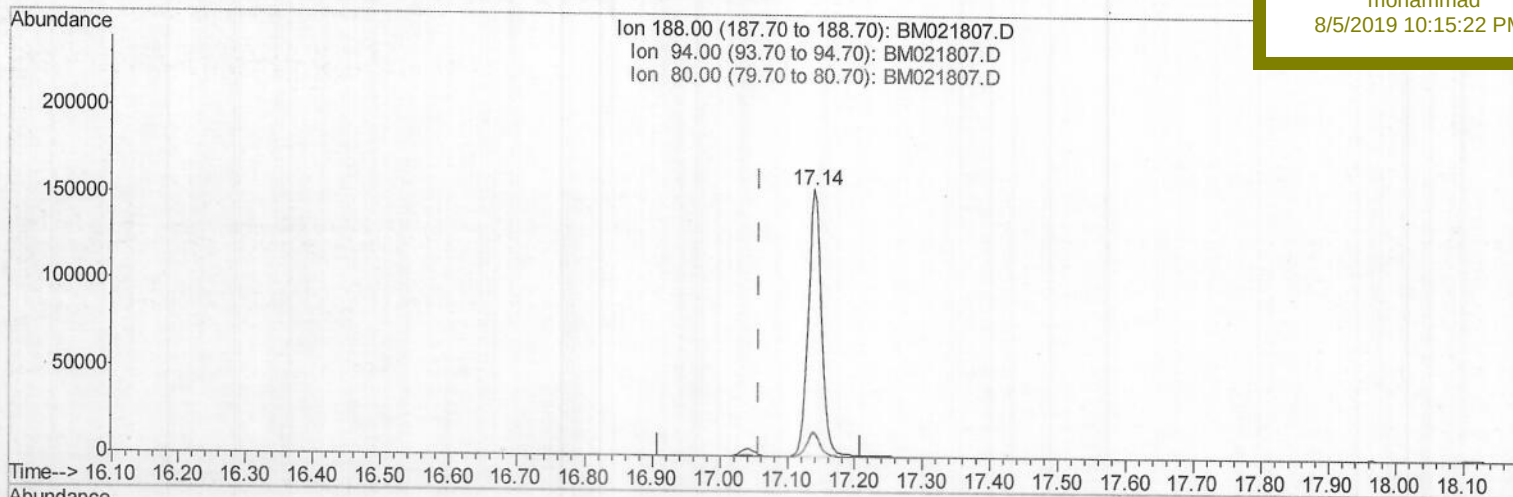

TIC: BM021807.D

(10) Phenanthrene-d10 (I)

17.140min (+0.081) 0.40ng/ul

response 212201

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	9.01
80.00	11.40	8.58#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021807.D
Acq On : 04 Aug 2019 11:44
Operator : HP/JU
Sample : K3850-17
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 05 05:29:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 05:26:43 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BENS3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:15:22 PM

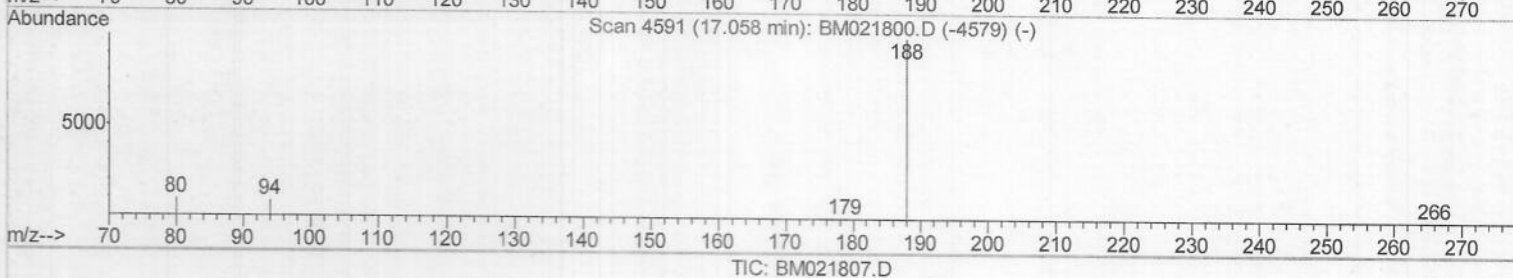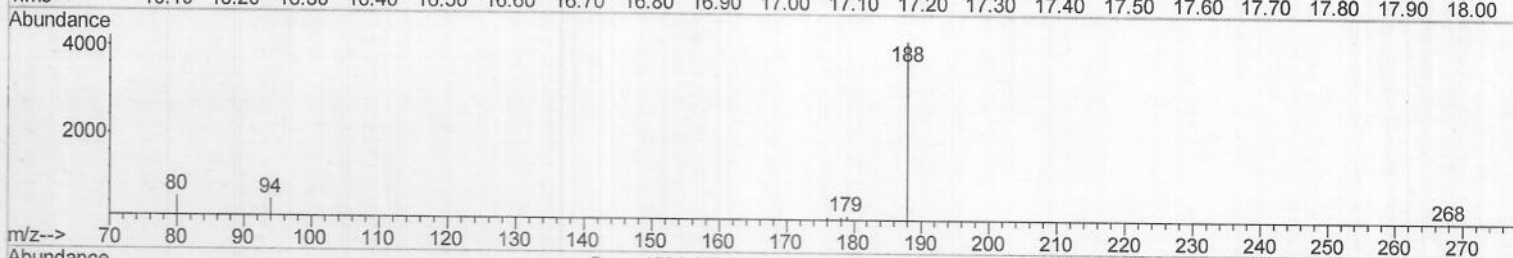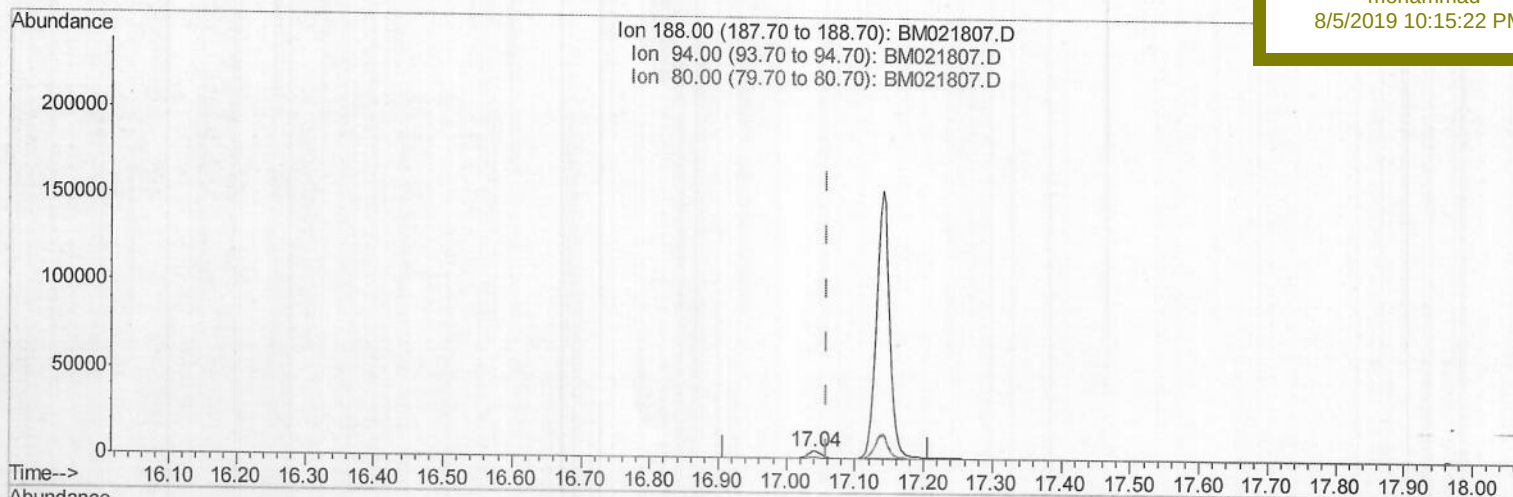

(10) Phenanthrene-d10 (I)

17.039min (-0.019) 0.40ng/ul m

response 5900

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	11.09
80.00	11.40	12.21
0.00	0.00	0.00




Data File : BM021807.D
Acq On : 04 Aug 2019 11:44
Operator : HP/JU
Sample : K3850-17
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 05 05:52:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 05:26:43 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BENS3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:15:22 PM

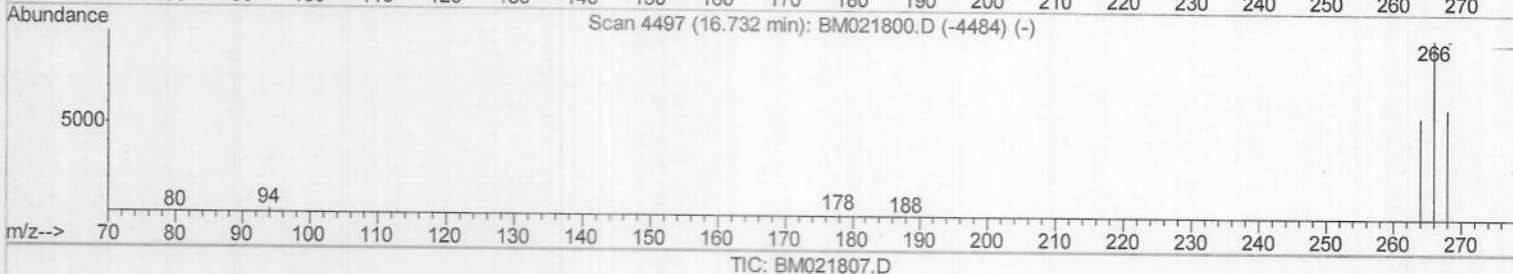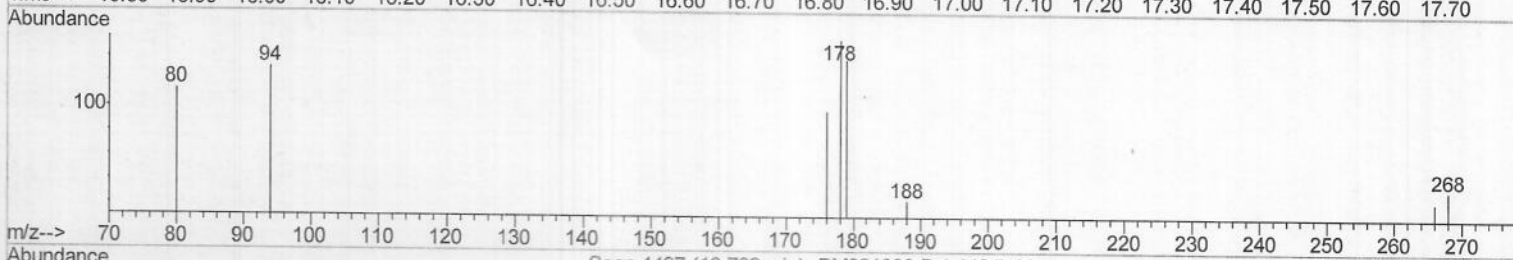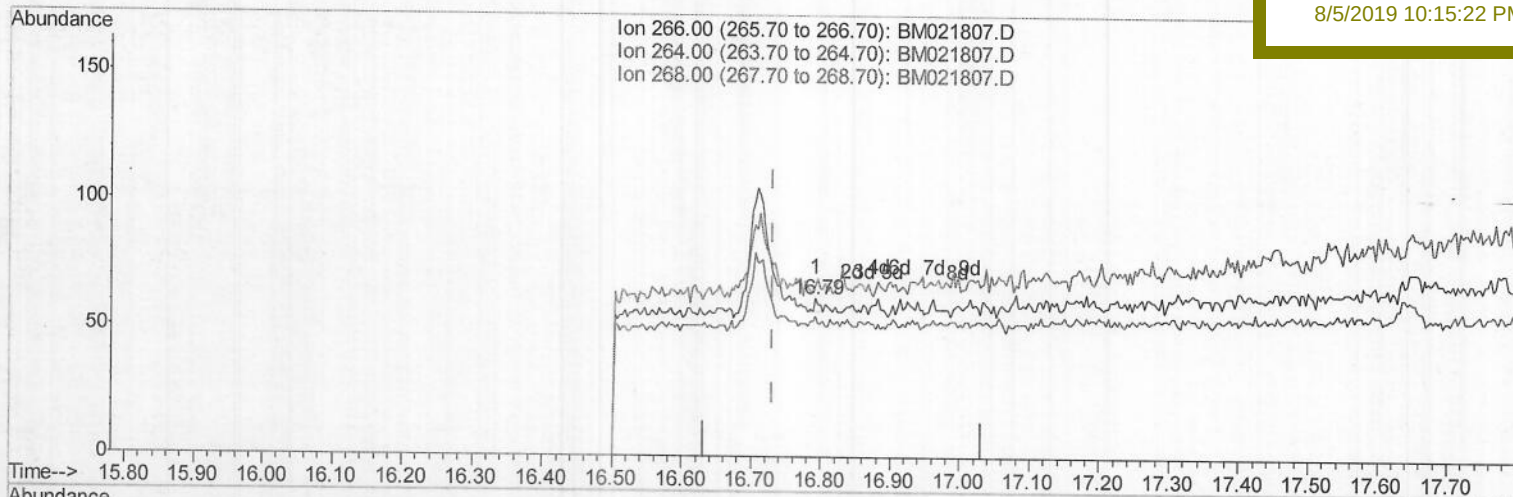

(11) Pentachlorophenol
16.793min (+0.061) 0.00ng/ul
response 3

Ion	Exp%	Act%
266.00	100	100
264.00	67.70	66.67
268.00	72.00	100.00#
0.00	0.00	0.00




Data File : BM021807.D
Acq On : 04 Aug 2019 11:44
Operator : HP/JU
Sample : K3850-17
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 05 05:52:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 05:26:43 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BENS3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:15:22 PM

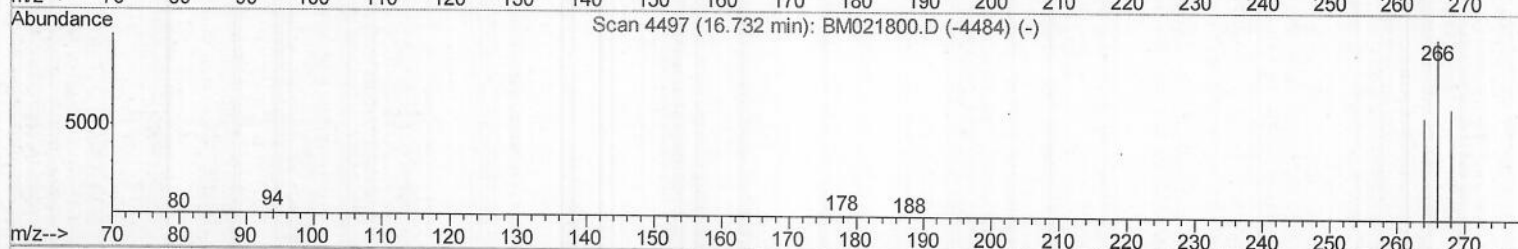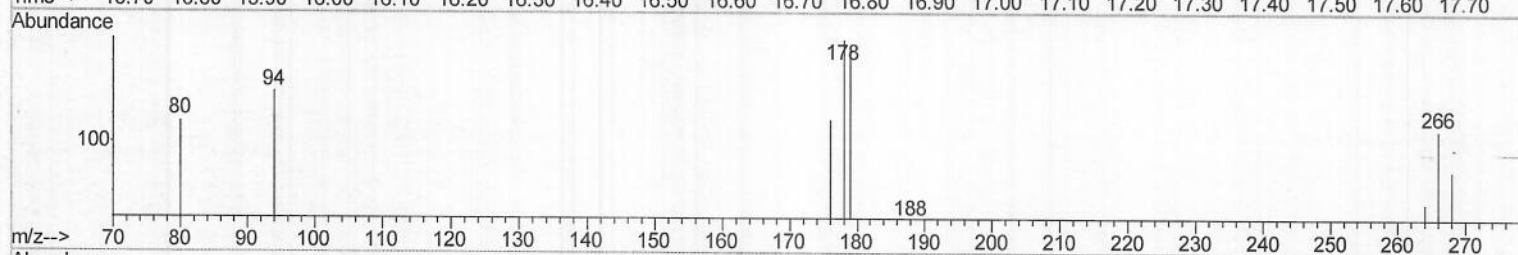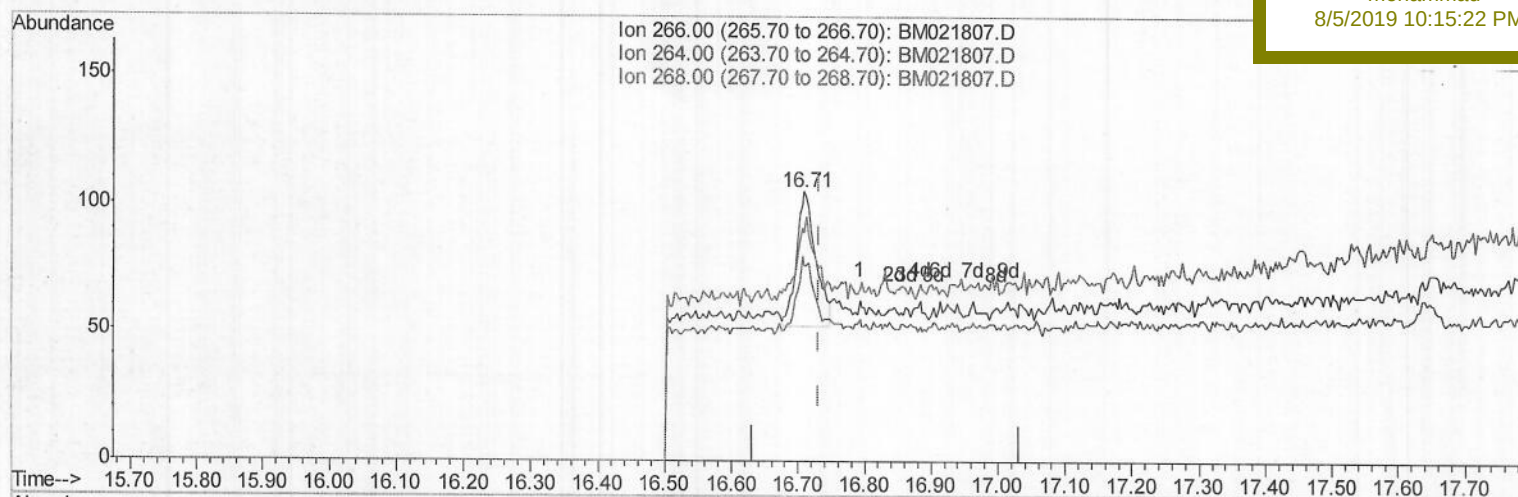

TIC: BM021807.D

(11) Pentachlorophenol

16.709min (-0.023) 0.10ng/ul m) JU 08/05/19

response 108

Ion	Exp%	Act%
266.00	100	100
264.00	67.70	1.85#
268.00	72.00	2.78#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021807.D
Acq On : 04 Aug 2019 11:44
Operator : HP/JU
Sample : K3850-17
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 05 05:52:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 05:26:43 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BENS3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:15:22 PM

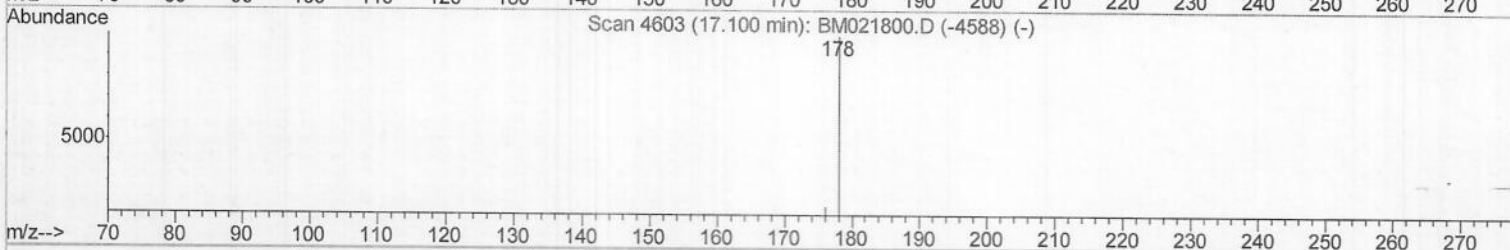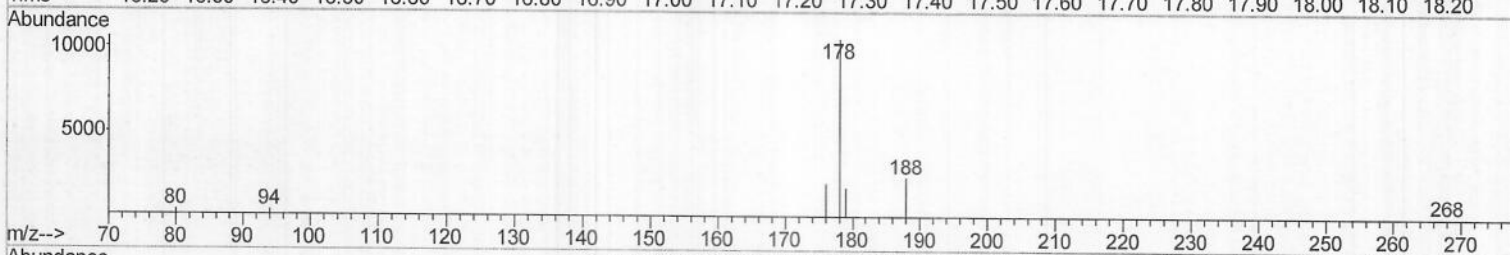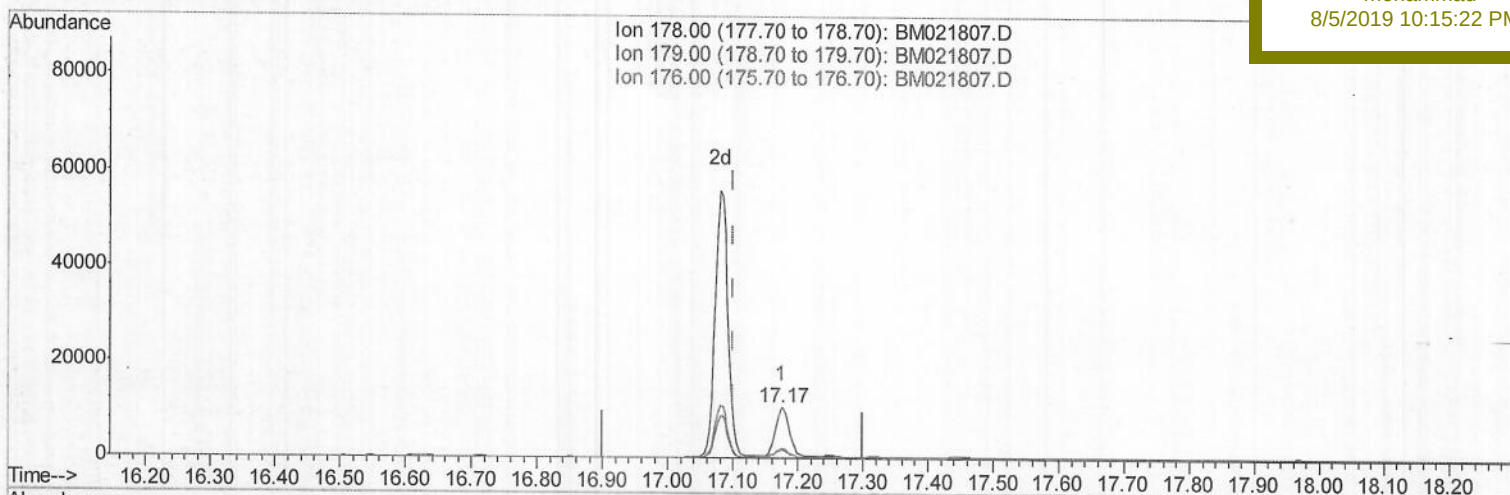

TIC: BM021807.D

(12) Phenanthrene

17.174min (+0.075) 0.97ng/ul

response 16706

Ion	Exp%	Act%
178.00	100	100
179.00	17.70	17.09
176.00	21.00	19.91
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021807.D
Acq On : 04 Aug 2019 11:44
Operator : HP/JU
Sample : K3850-17
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 05 05:52:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 05:26:43 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BENS3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:15:22 PM

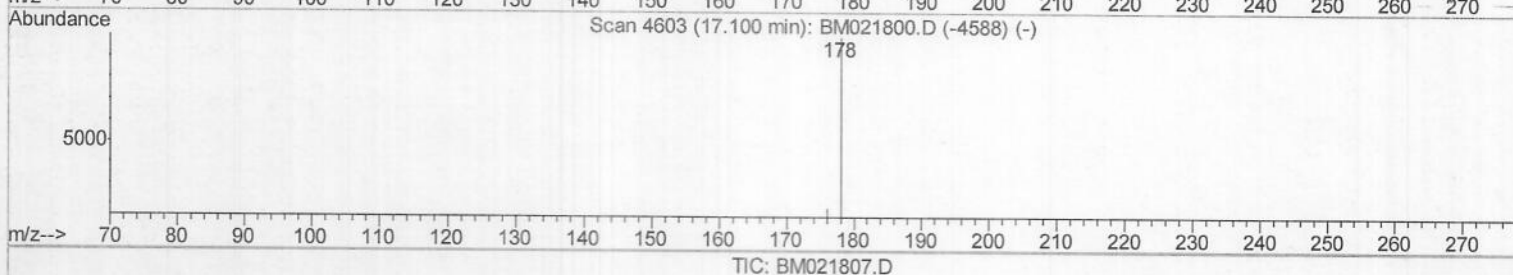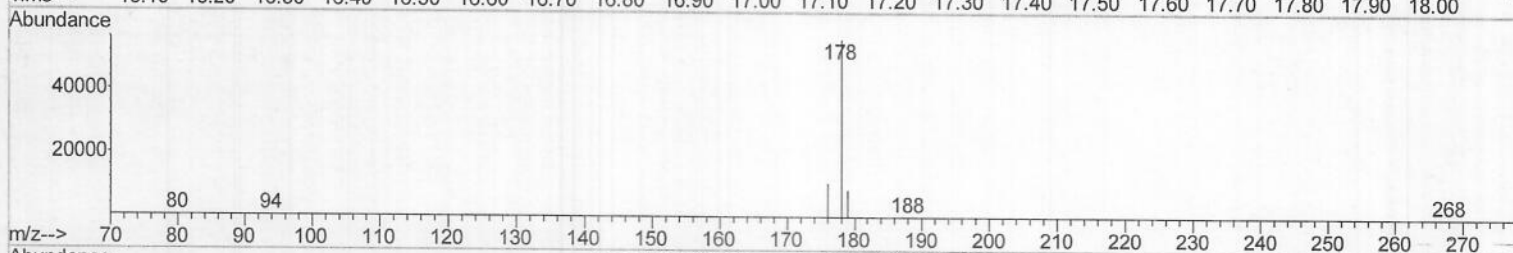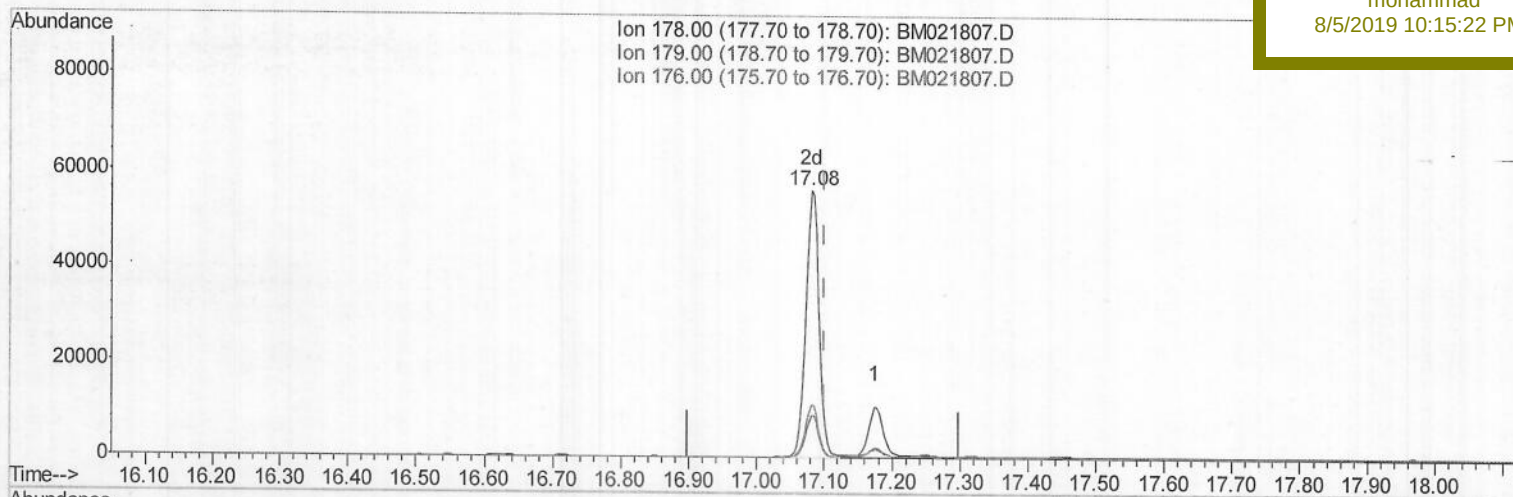

(12) Phenanthrene

17.081min (-0.019) 4.45ng/ul m) 50 08/05/19

response 76321

Ion	Exp%	Act%
178.00	100	100
179.00	17.70	15.38
176.00	21.00	19.54
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021807.D
Acq On : 04 Aug 2019 11:44
Operator : HP/JU
Sample : K3850-17
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 05 05:52:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 05:26:43 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BENS3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:15:22 PM

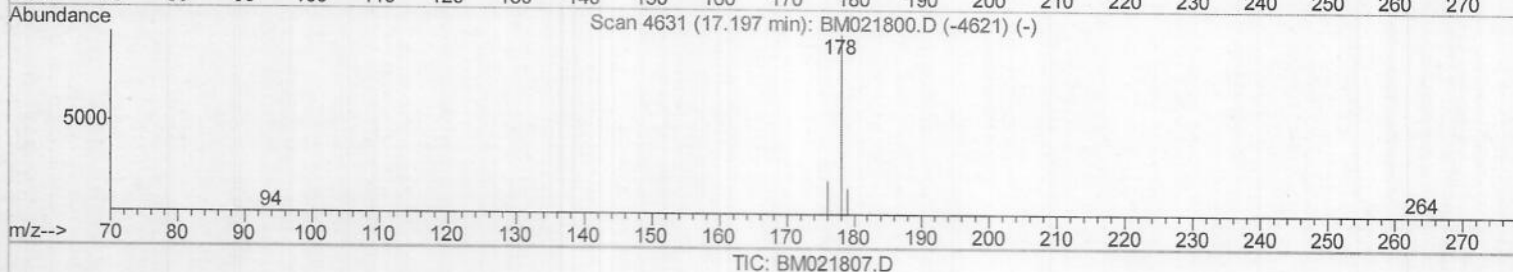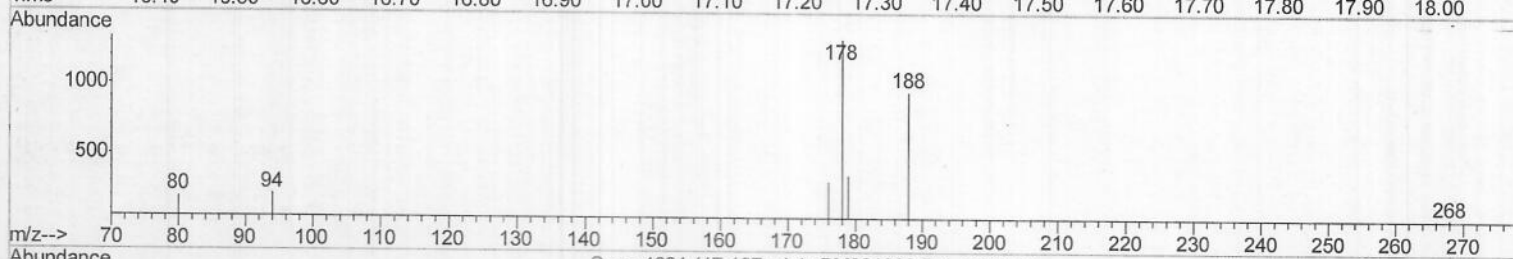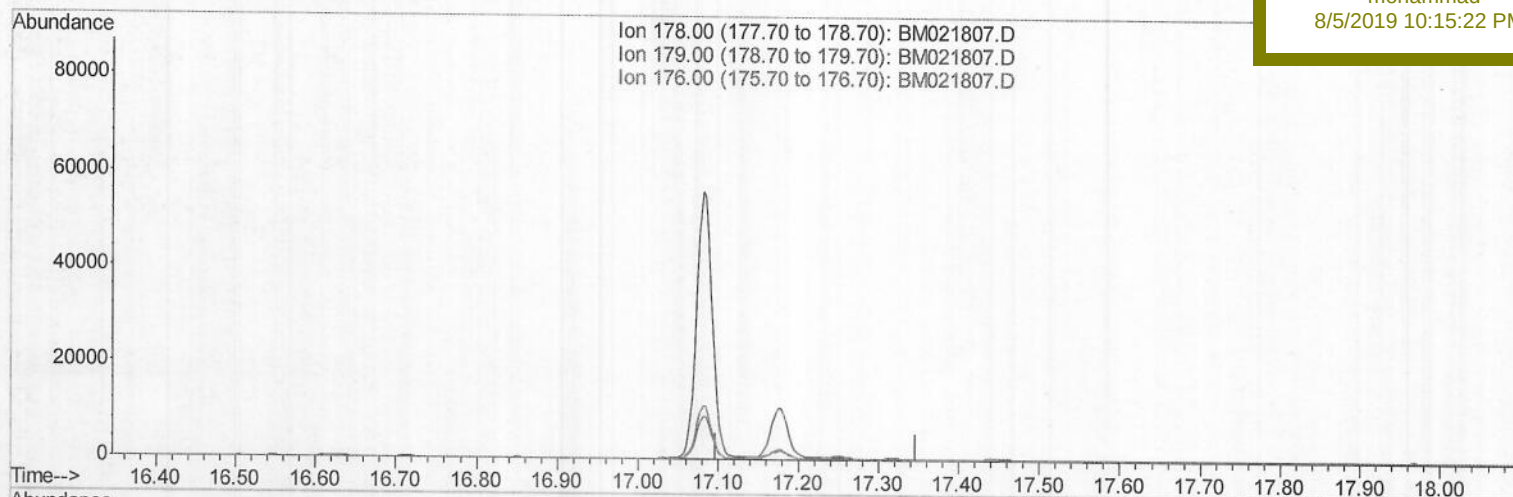

(13) Anthracene

17.197min (-17.197) 0.00ng/ul

response 0

Ion	Exp%	Act%
178.00	100	0.00
179.00	19.40	0.00#
176.00	20.80	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021807.D
Acq On : 04 Aug 2019 11:44
Operator : HP/JU
Sample : K3850-17
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 05 05:52:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 05:26:43 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BENS3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:15:22 PM

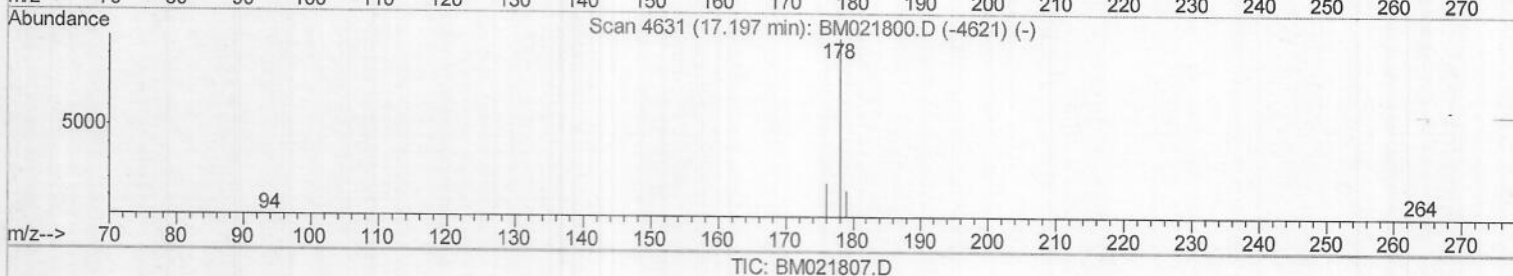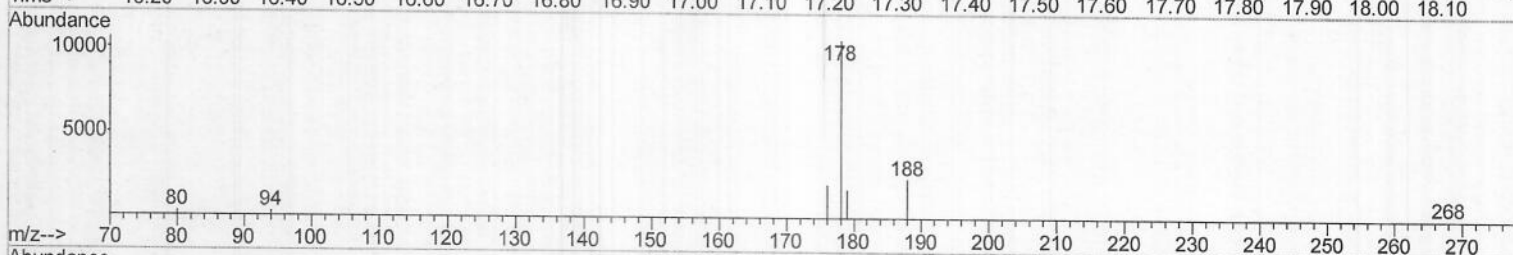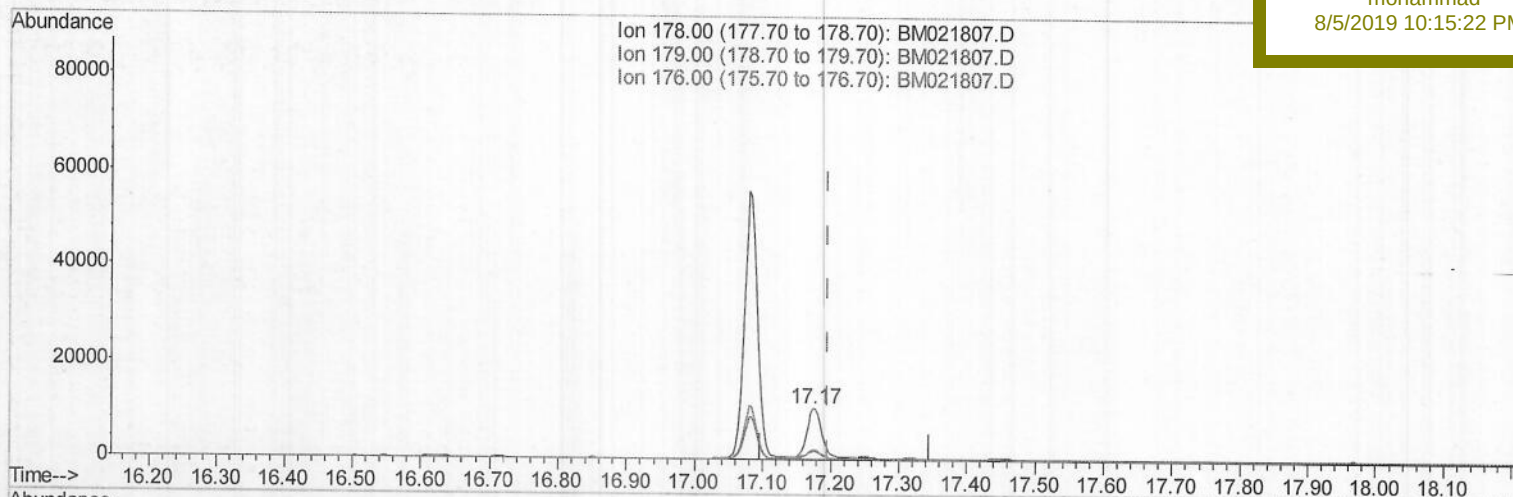

(13) Anthracene

17.174min (-0.023) 1.05ng/ul m) JU 08/05/19

response 15409

Ion	Exp%	Act%
178.00	100	100
179.00	19.40	17.09
176.00	20.80	19.91
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021807.D
Acq On : 04 Aug 2019 11:44
Operator : HP/JU
Sample : K3850-17
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 05 05:52:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 05:26:43 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BENS3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:15:22 PM

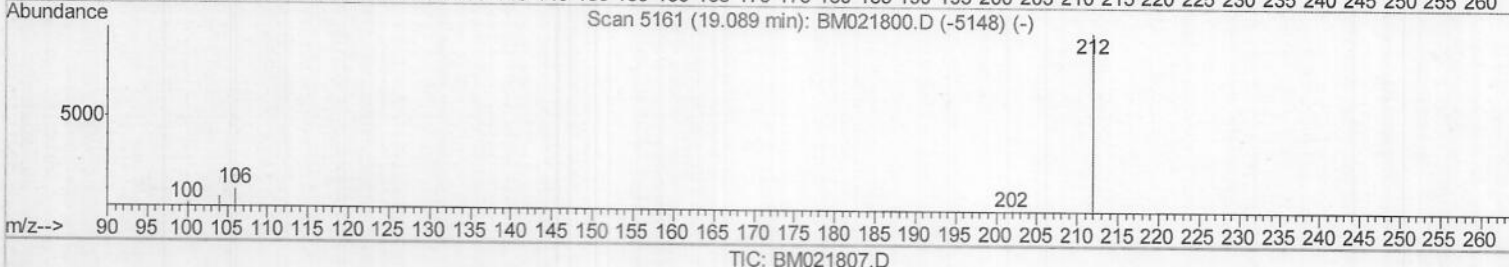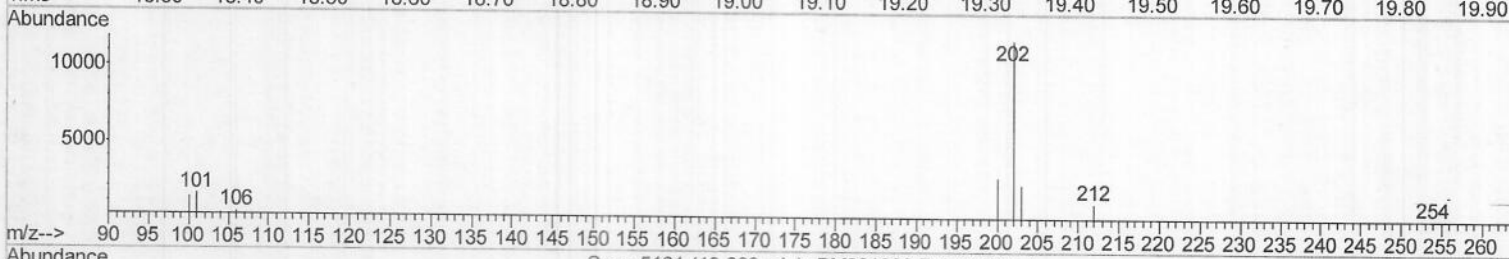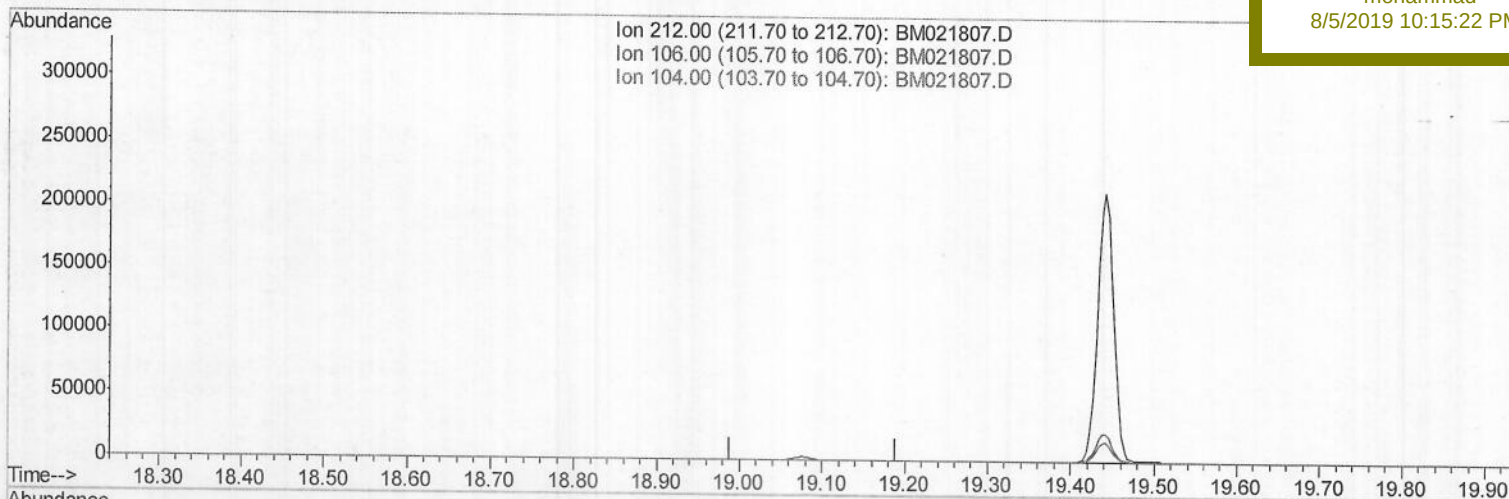

(14) Fluoranthene-d10 (SURR)

19.089min (-19.089) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	9.90	0.00#
104.00	6.00	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021807.D
Acq On : 04 Aug 2019 11:44
Operator : HP/JU
Sample : K3850-17
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 05 05:52:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 05:26:43 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BENS3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:15:22 PM

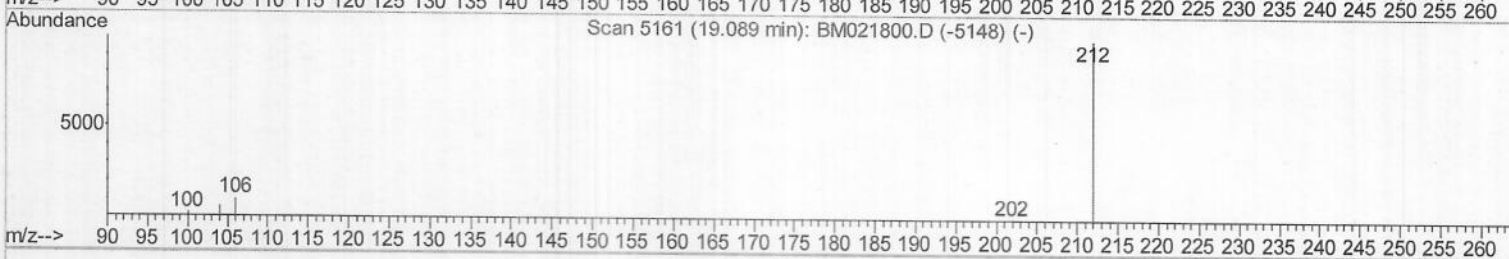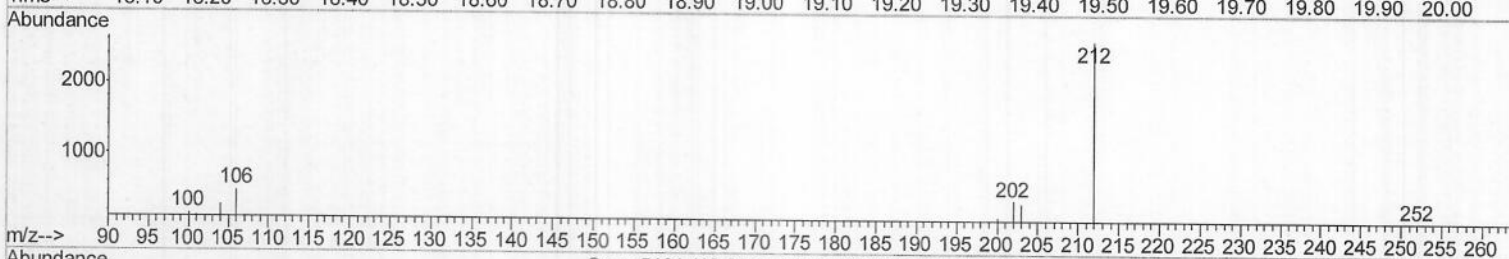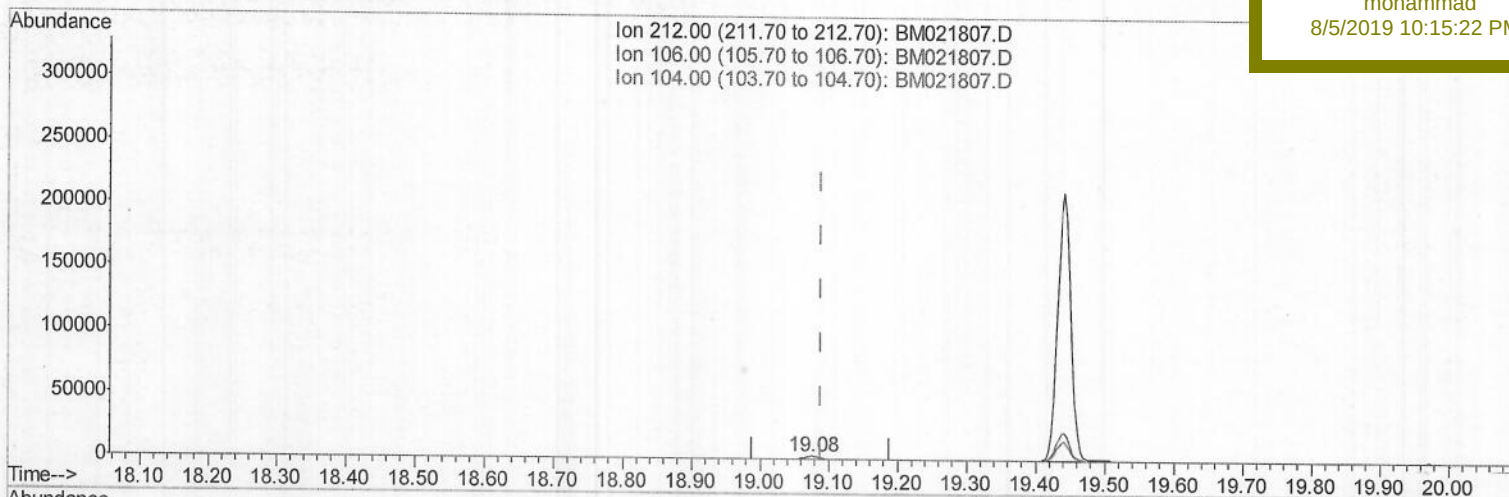

TIC: BM021807.D

(14) Fluoranthene-d10 (SURR)

19.076min (-0.013) 0.17ng/ul m) JU 08/05/19

response 3335

Ion	Exp%	Act%
212.00	100	100
106.00	9.90	0.00#
104.00	6.00	0.00#
0.00	0.00	0.00

Data File : BM021807.D

Acq On : 04 Aug 2019 11:44

Operator : HP/JU

Sample : K3850-17

Misc :

ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 05 05:52:02 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Aug 05 05:26:43 2019

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




BENS3

Manual Integrations

APPROVED

mohammad

8/5/2019 10:15:22 PM

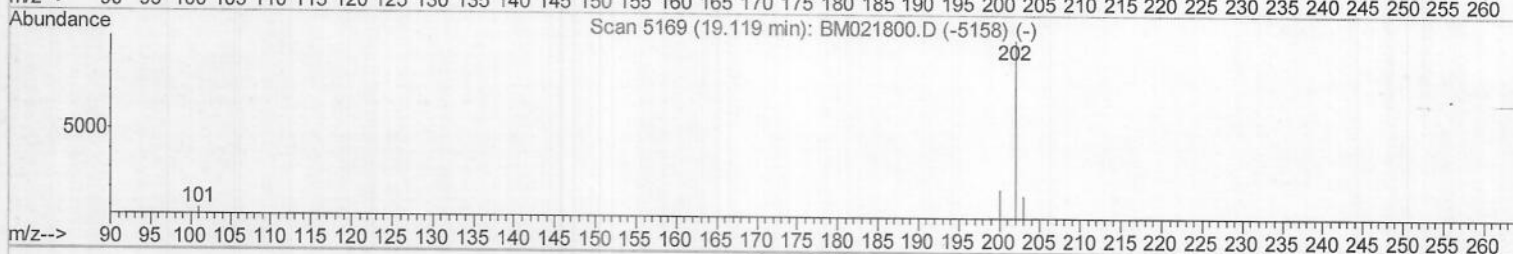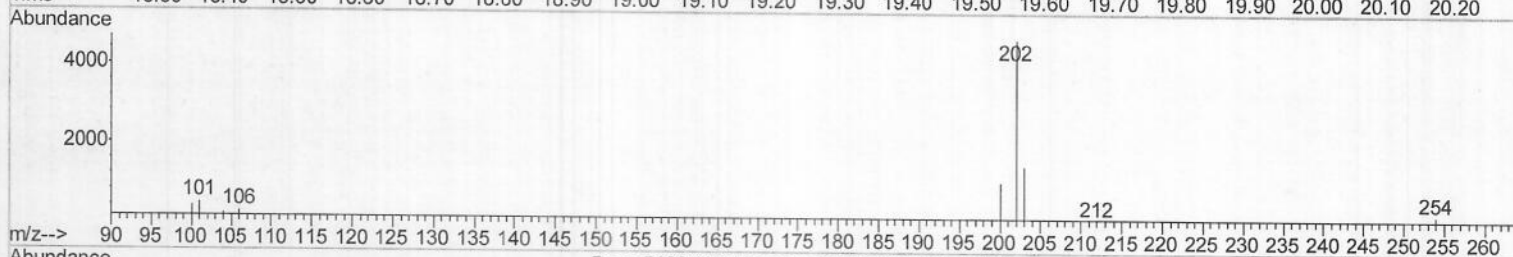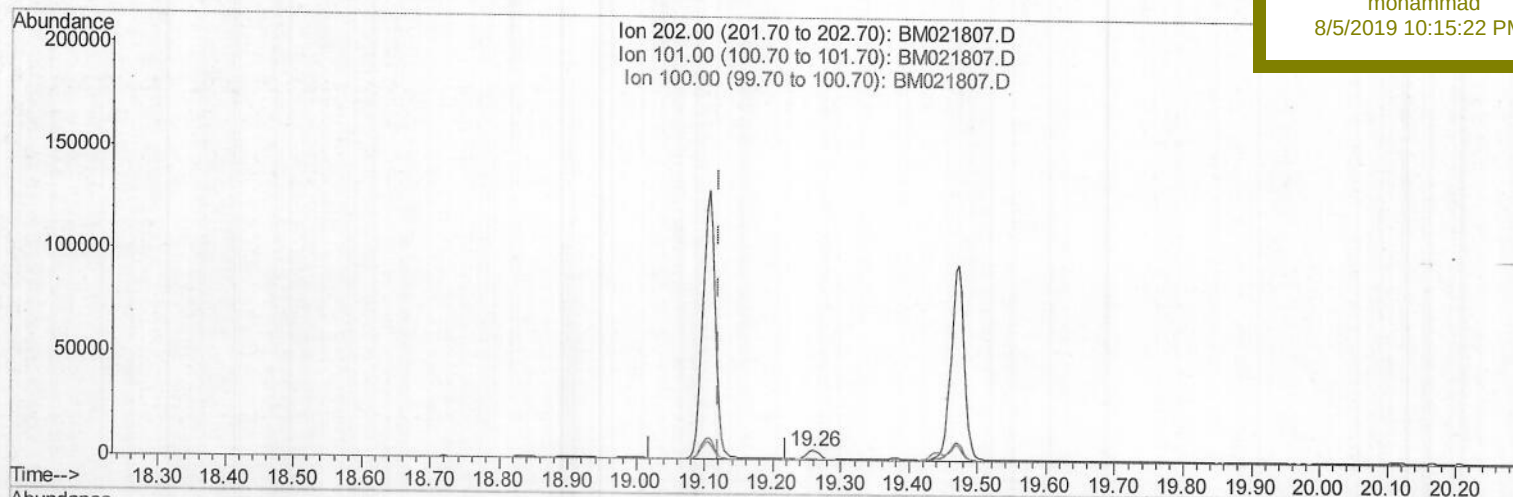

(15) Fluoranthene (C)

19.259min (+0.139) 0.23ng/ul

response 5404

Ion	Exp%	Act%
202.00	100	100
101.00	10.20	9.72
100.00	8.10	7.57
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021807.D
Acq On : 04 Aug 2019 11:44
Operator : HP/JU
Sample : K3850-17
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 05 05:52:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 05:26:43 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BENS3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:15:22 PM

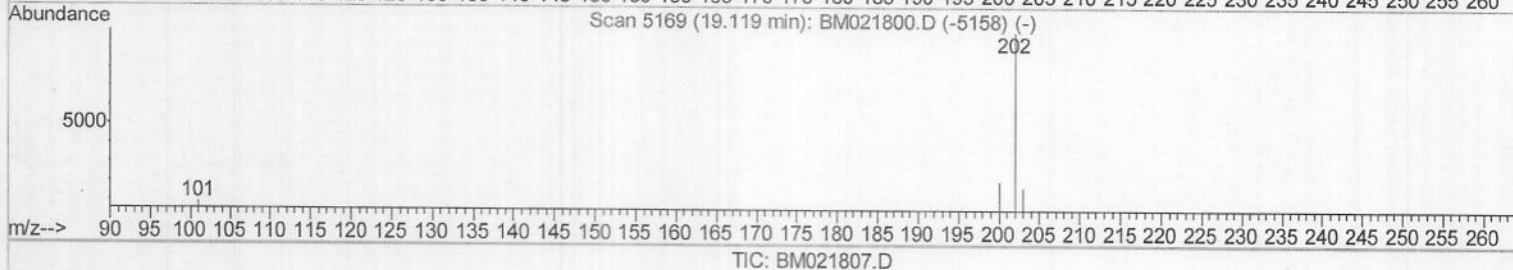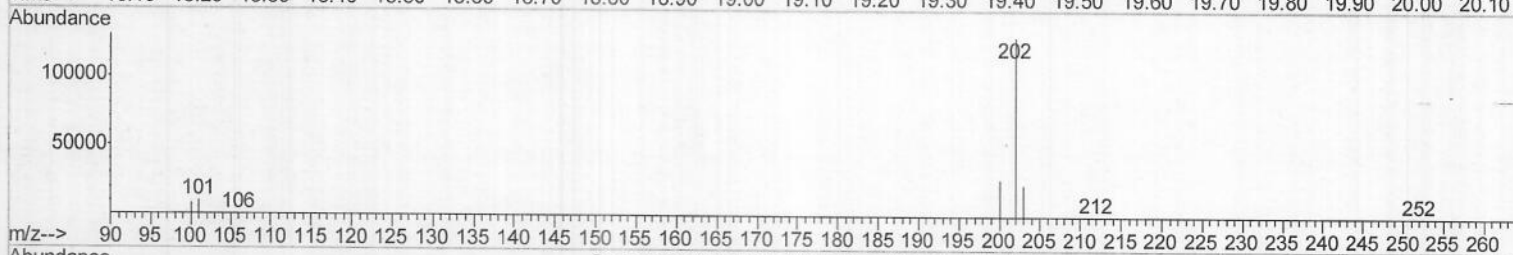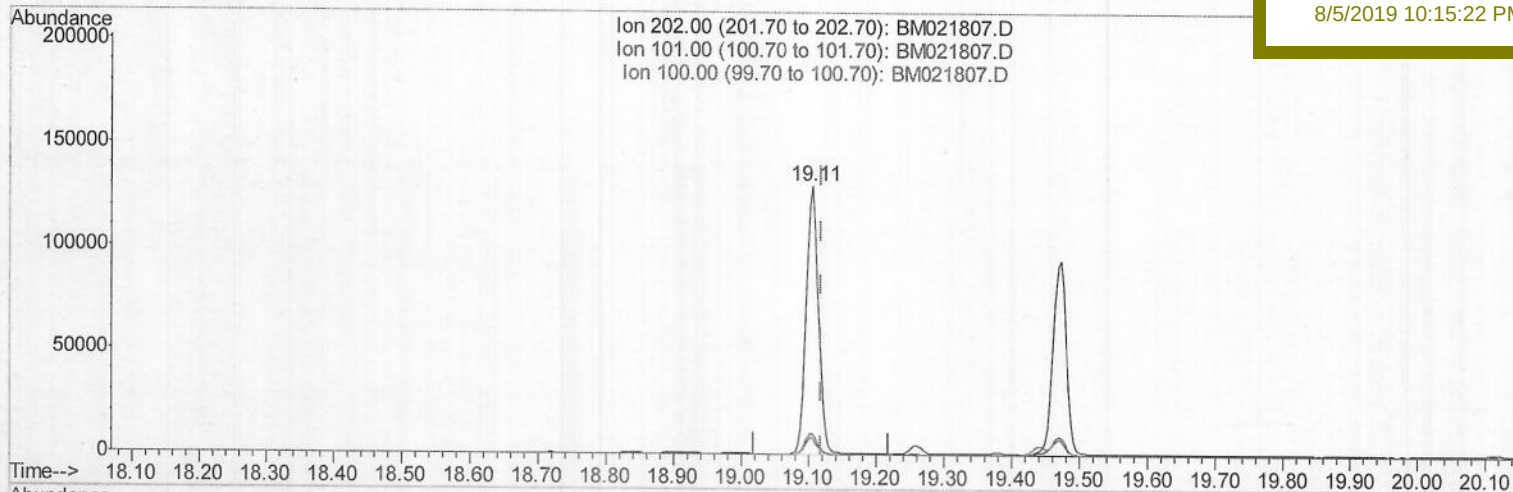

(15) Fluoranthene (C)

19.106min (-0.013) 7.21ng/ul m

response 165854

Ion	Exp%	Act%
202.00	100	100
101.00	10.20	7.79
100.00	8.10	5.92
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021807.D
Acq On : 04 Aug 2019 11:44
Operator : HP/JU
Sample : K3850-17
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 05 05:52:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 05:26:43 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BENS3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:15:22 PM

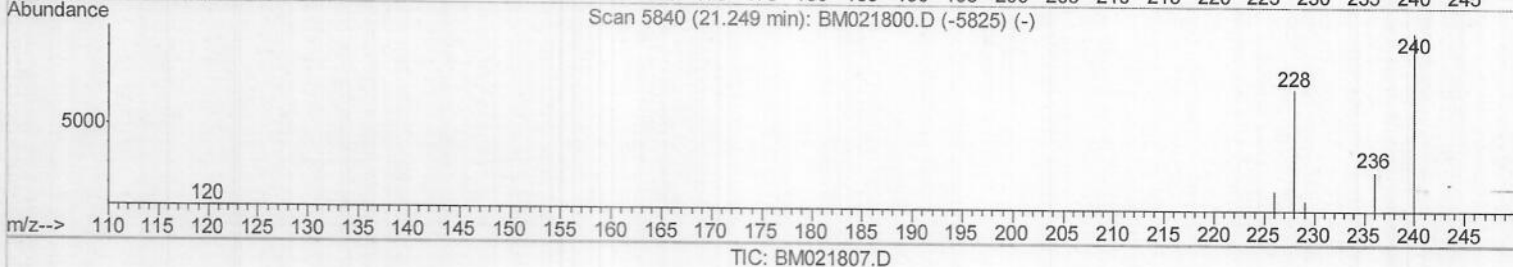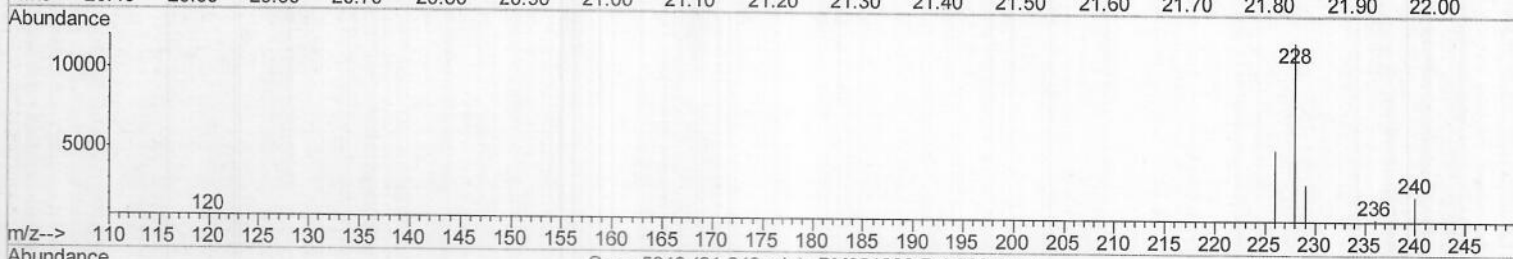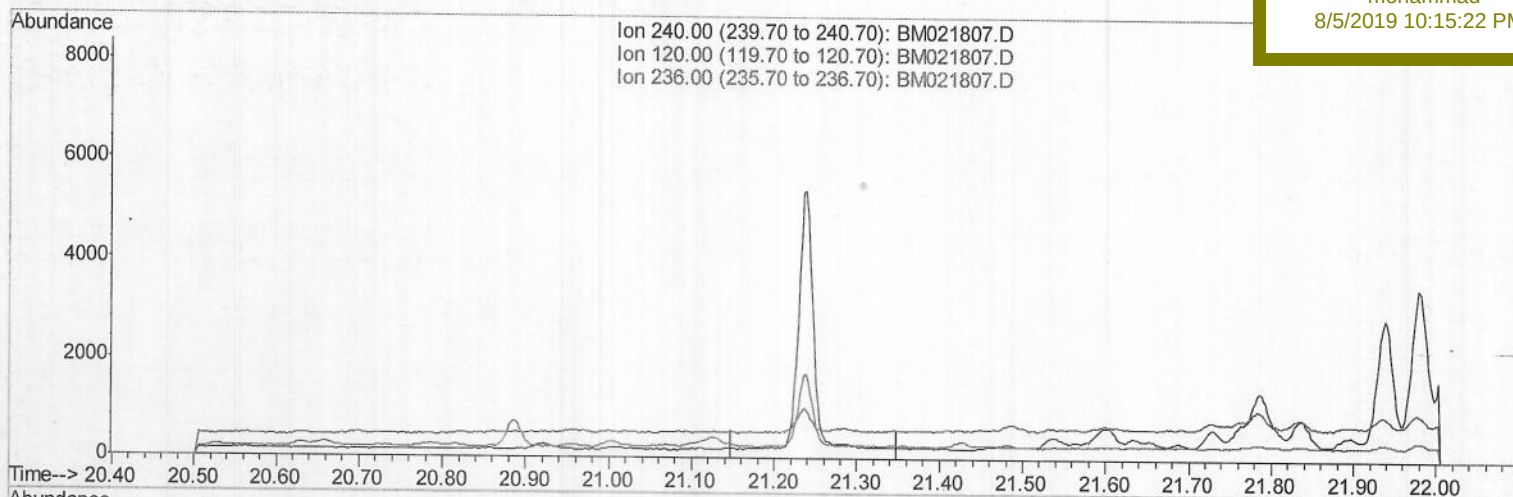

(16) Chrysene-d12 (I)

21.249min (-21.249) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.20	0.00#
236.00	32.30	0.00#
0.00	0.00	0.00




Data File : BM021807.D
Acq On : 04 Aug 2019 11:44
Operator : HP/JU
Sample : K3850-17
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 05 05:52:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 05:26:43 2019
Response via : Initial Calibration

Instrument :
BNA_M
Client Sample ID :
BENS3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:15:22 PM

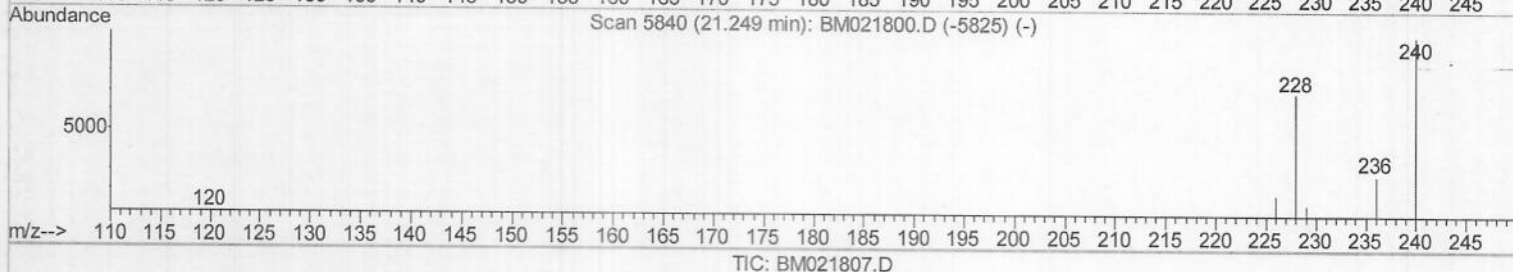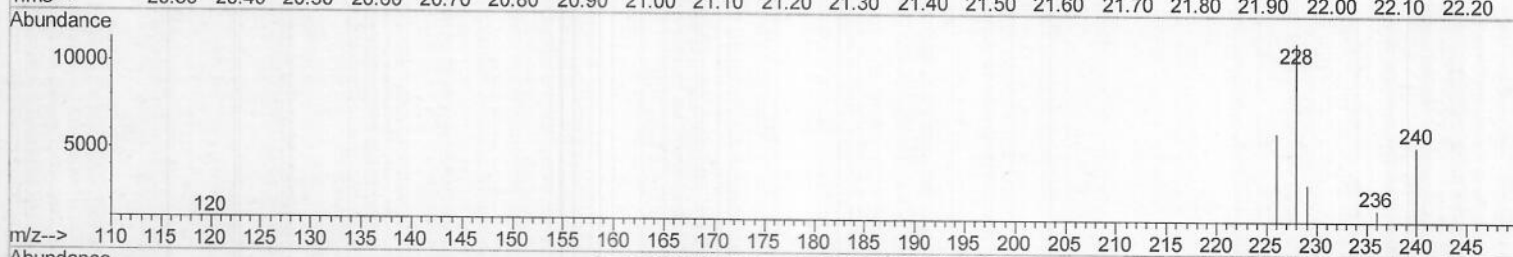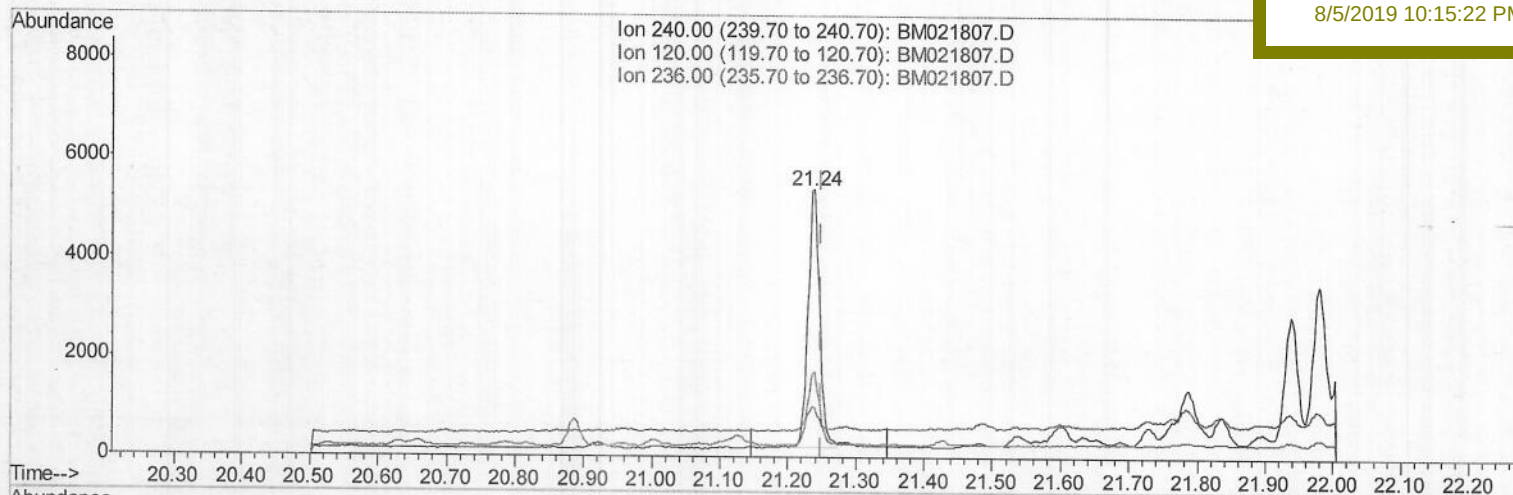

TIC: BM021807.D

(16) Chrysene-d12 (I)

21.239min (-0.010) 0.40ng/ul m) 3008/05/19

response 6194

Ion	Exp%	Act%
240.00	100	100
120.00	16.20	18.17
236.00	32.30	31.68
0.00	0.00	0.00




Data File : BM021807.D
Acq On : 04 Aug 2019 11:44
Operator : HP/JU
Sample : K3850-17
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 05 05:53:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 05:26:43 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BENS3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:15:22 PM

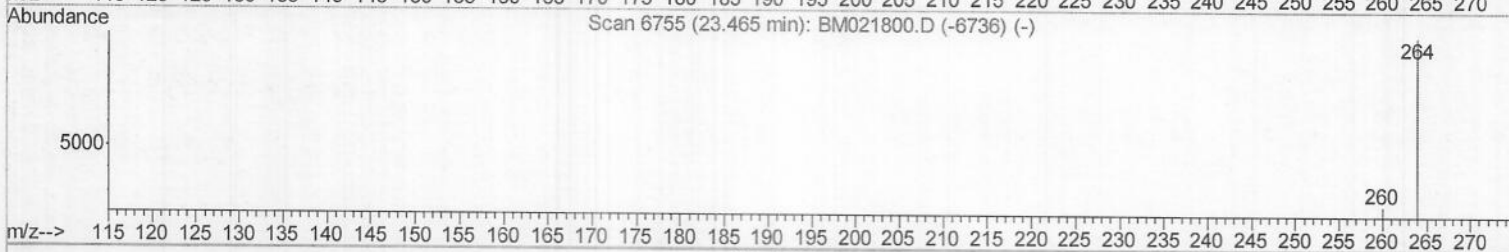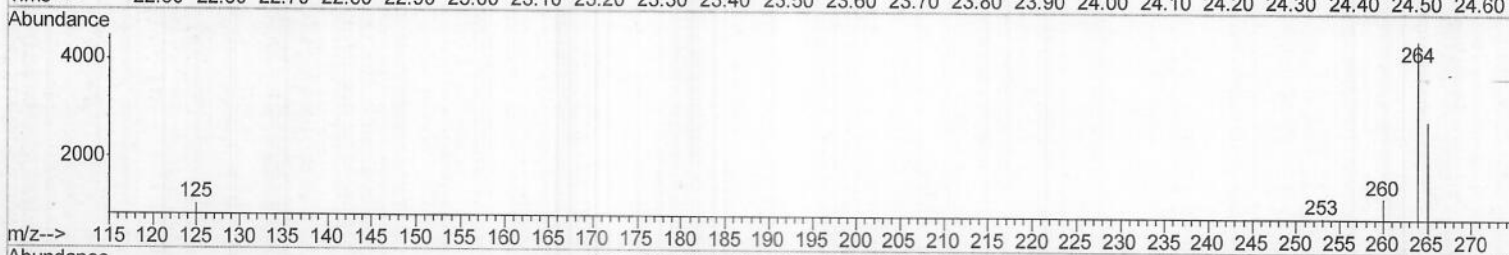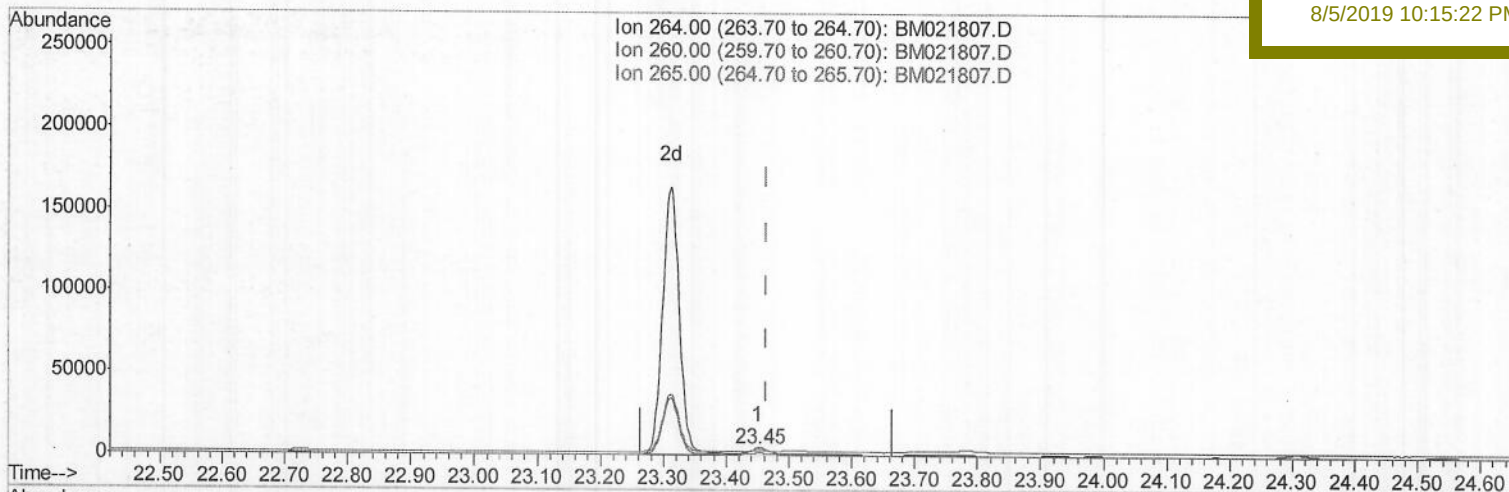

TIC: BM021807.D

(20) Perylene-d12 (I)
23.450min (-0.015) 0.40ng/ul
response 10551

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	27.96
265.00	117.00	63.71#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Qedit)




Data File : BM021807.D
Acq On : 04 Aug 2019 11:44
Operator : HP/JU
Sample : K3850-17
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 05 05:53:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 05:26:43 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BENS3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:15:22 PM

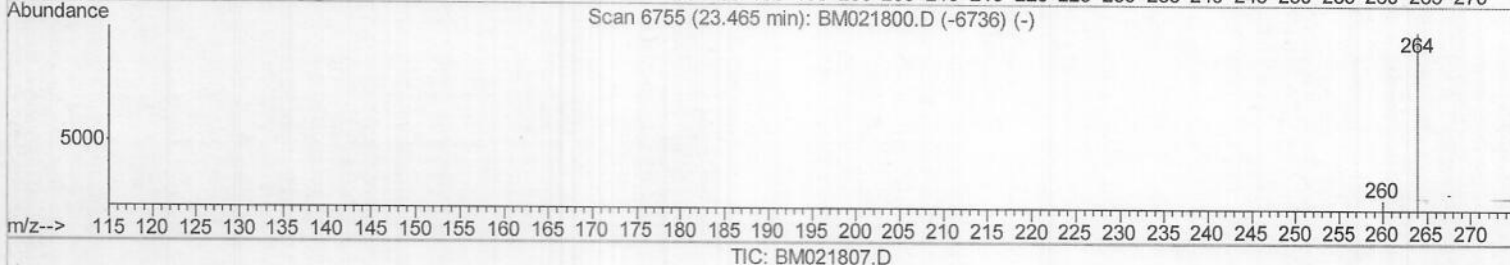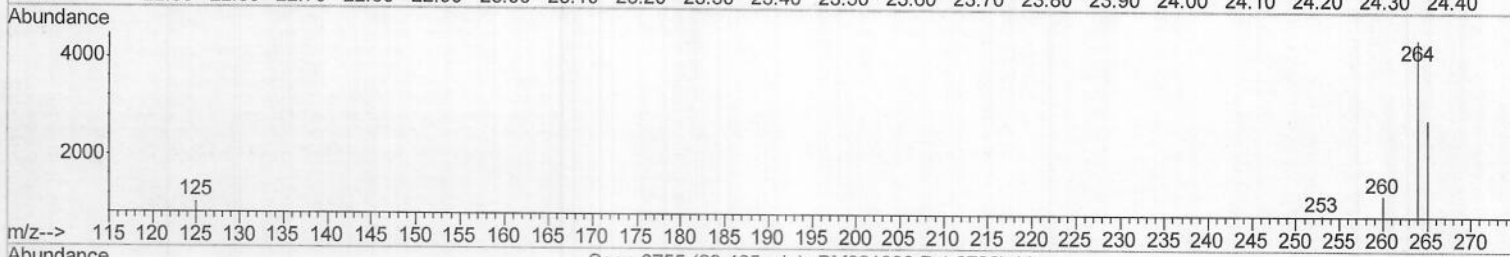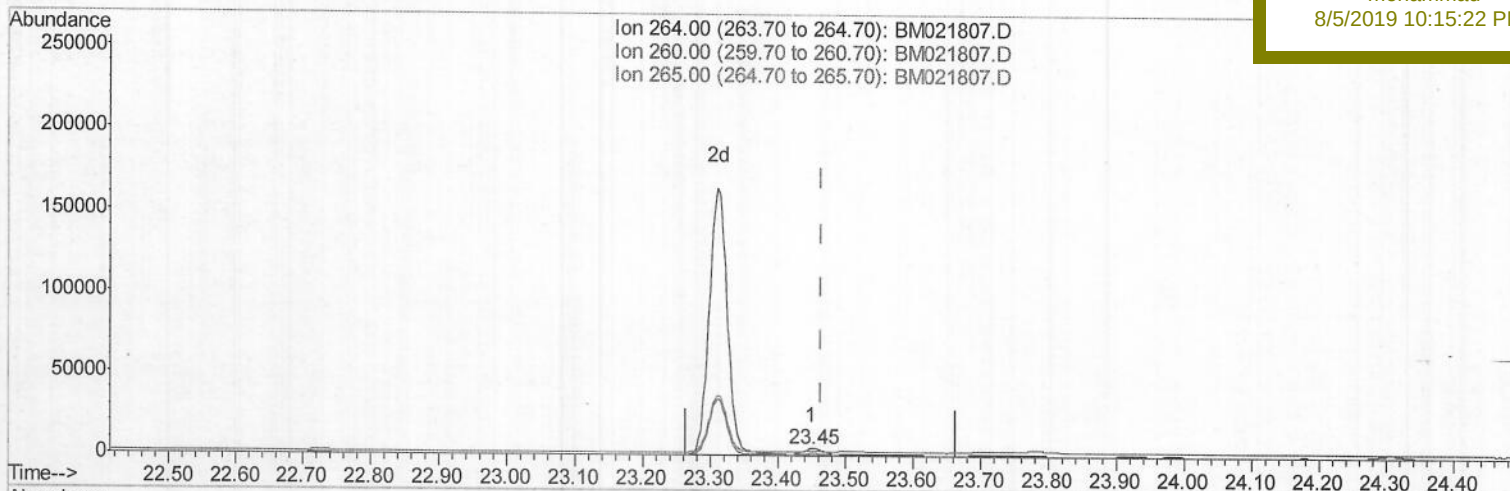

(20) Perylene-d12 (I)

23.450min (-0.015) 0.40ng/ul m) JU 08/05/19

response 7044

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	27.96
265.00	117.00	63.71#
0.00	0.00	0.00




Data File : BM021807.D
Acq On : 04 Aug 2019 11:44
Operator : HP/JU
Sample : K3850-17
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 05 05:54:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 05:26:43 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BENS3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:15:22 PM

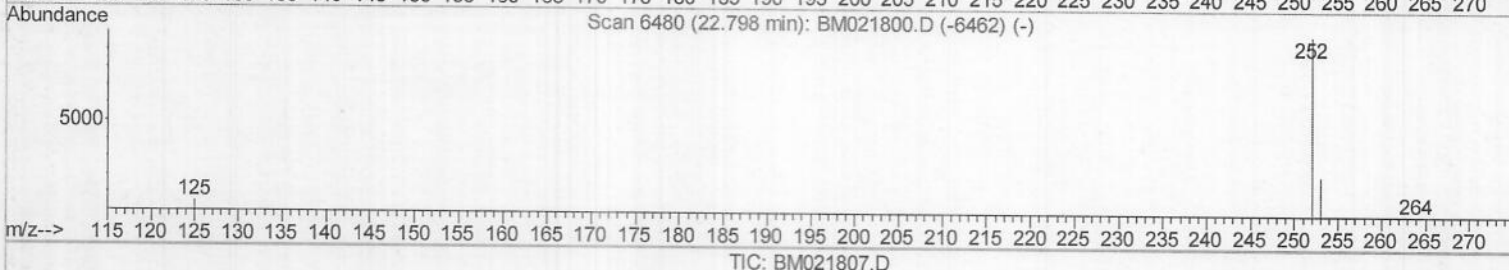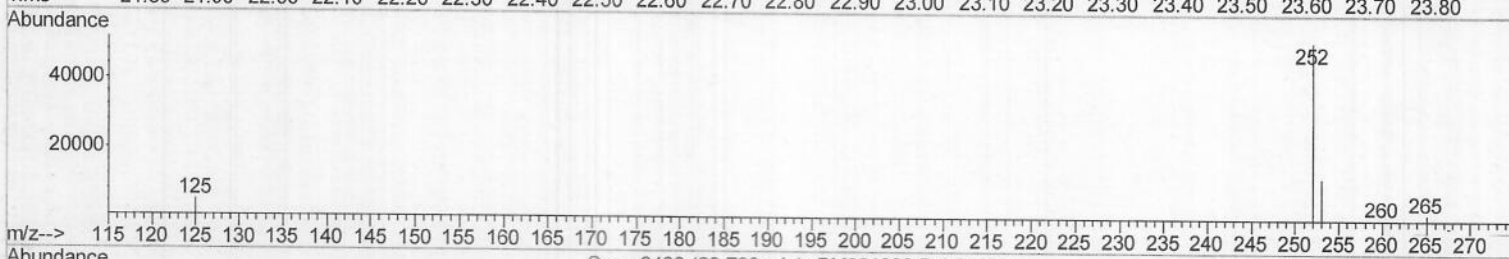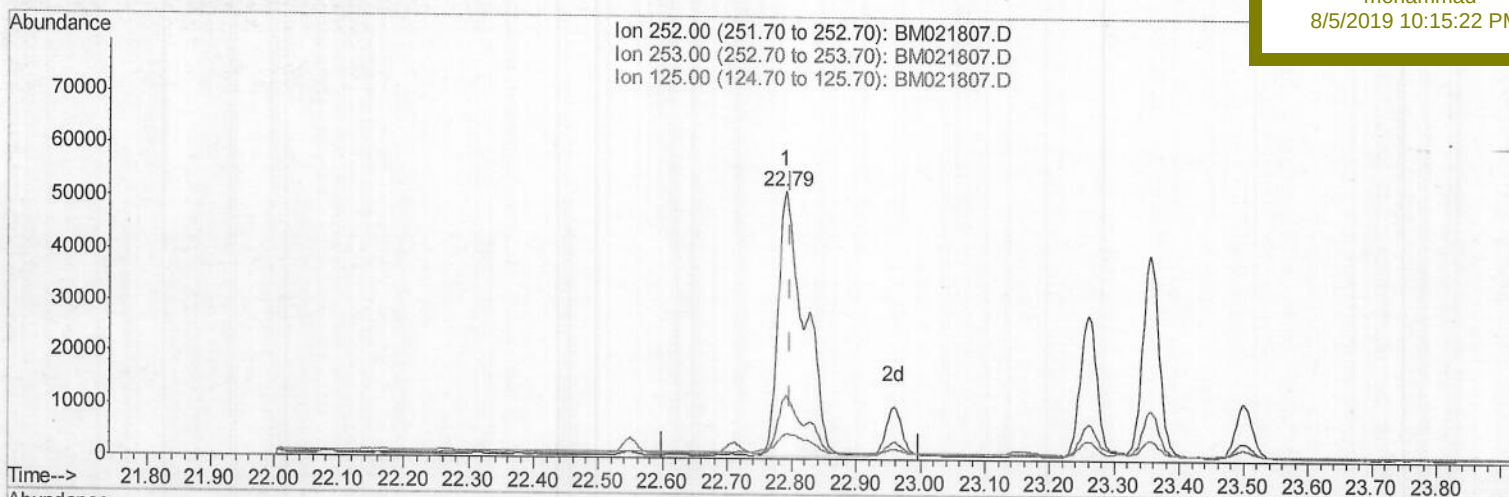

(21) Benzo(b)fluoranthene
22.791min (-0.008) 6.19ng/ui
response 147147

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	23.62
125.00	15.50	9.07
0.00	0.00	0.00




Data File : BM021807.D
Acq On : 04 Aug 2019 11:44
Operator : HP/JU
Sample : K3850-17
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 05 05:54:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 05:26:43 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BENS3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:15:22 PM

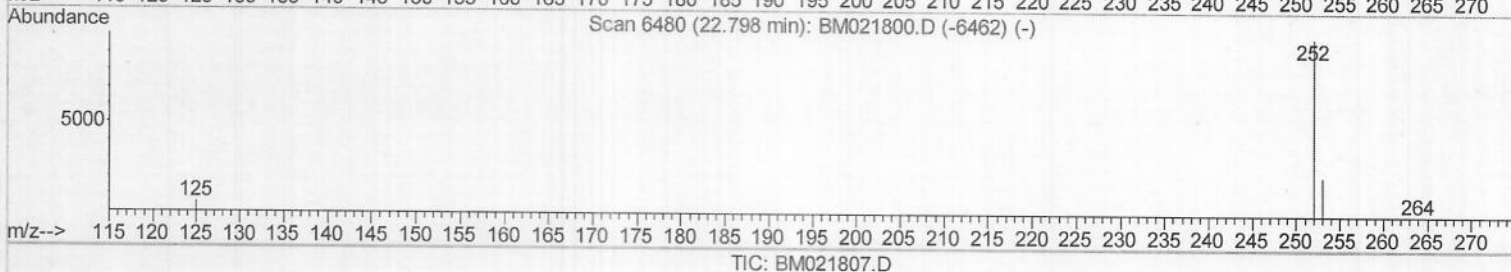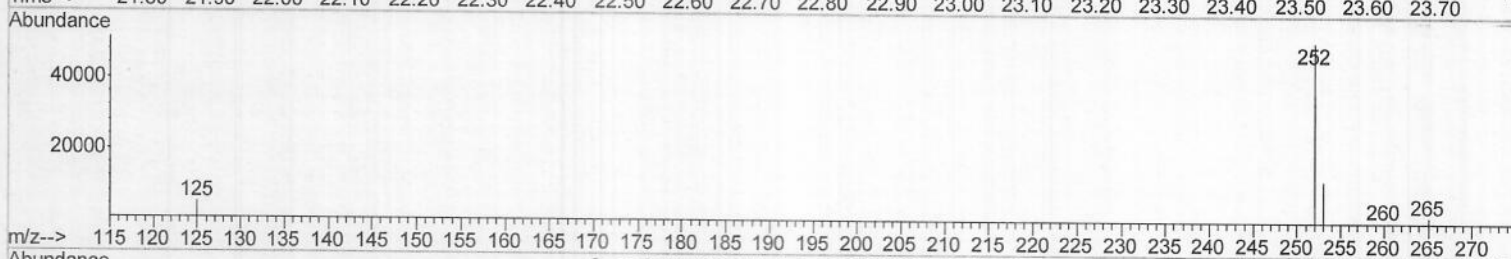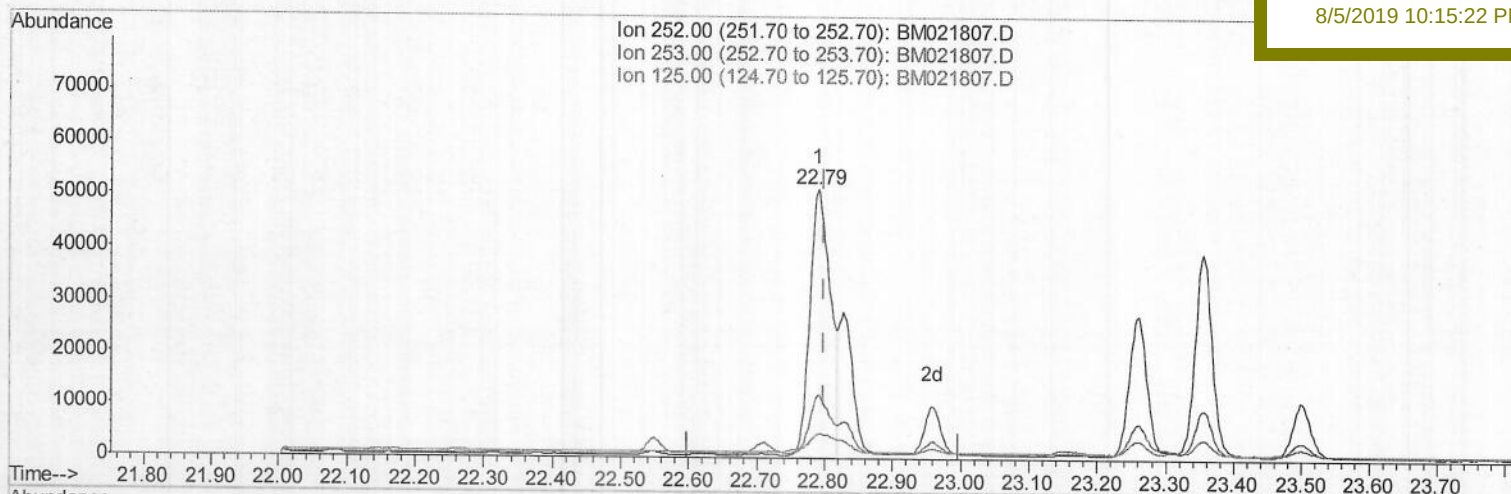

(21) Benzo(b)fluoranthene

22.791min (-0.008) 4.47ng/ul m

JU
08/05/19

response 106094

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	23.62
125.00	15.50	9.07
0.00	0.00	0.00




Data File : BM021807.D
Acq On : 04 Aug 2019 11:44
Operator : HP/JU
Sample : K3850-17
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 05 05:54:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 05:26:43 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BENS3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:15:22 PM

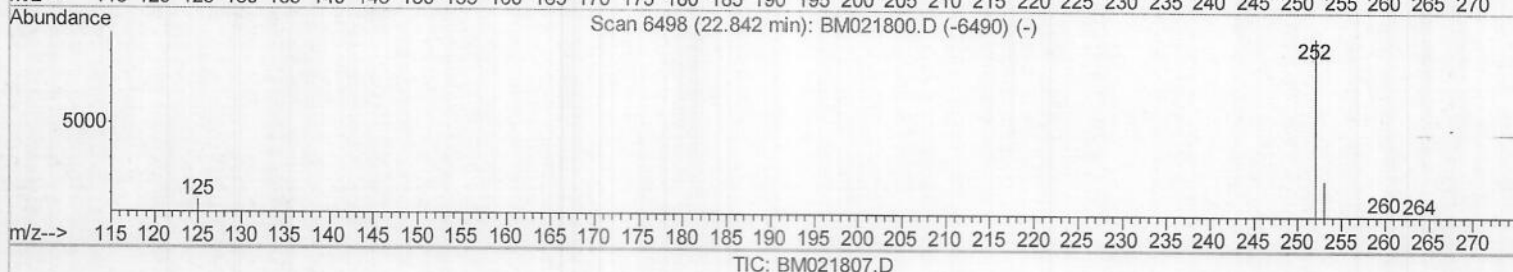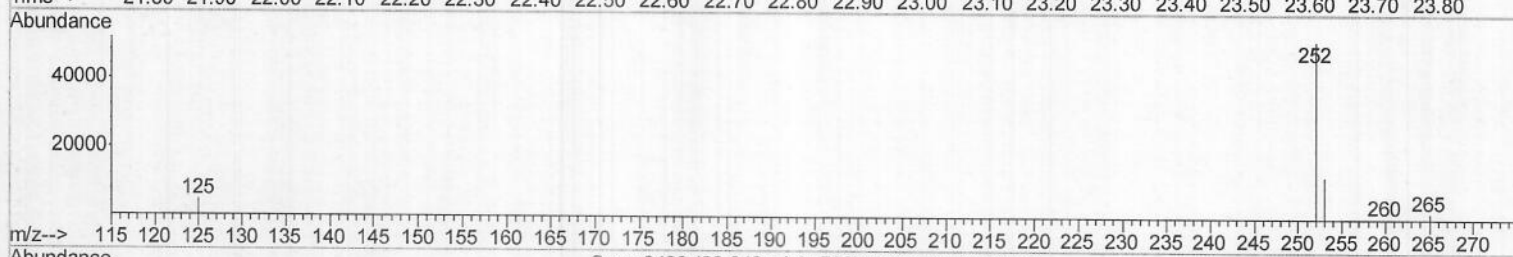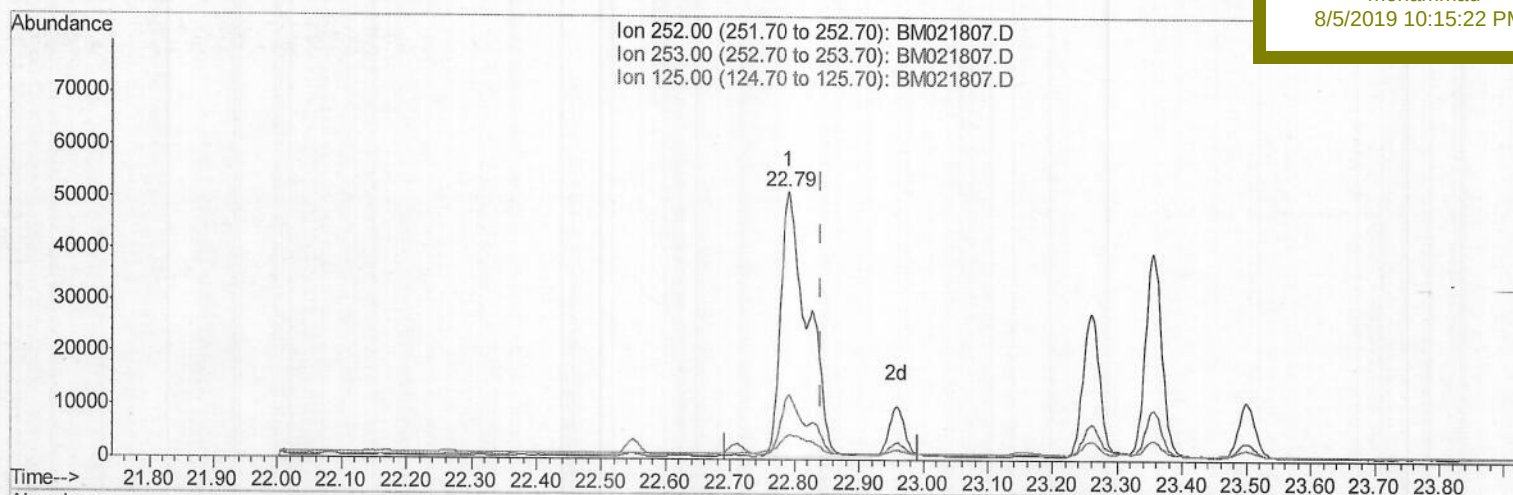

(22) Benzo(k)fluoranthene
22.791min (-0.051) 5.47ng/ul
response 147147

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	23.62#
125.00	15.20	9.07#
0.00	0.00	0.00




Data File : BM021807.D
Acq On : 04 Aug 2019 11:44
Operator : HP/JU
Sample : K3850-17
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 05 05:54:01 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 05:26:43 2019
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
BENS3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:15:22 PM

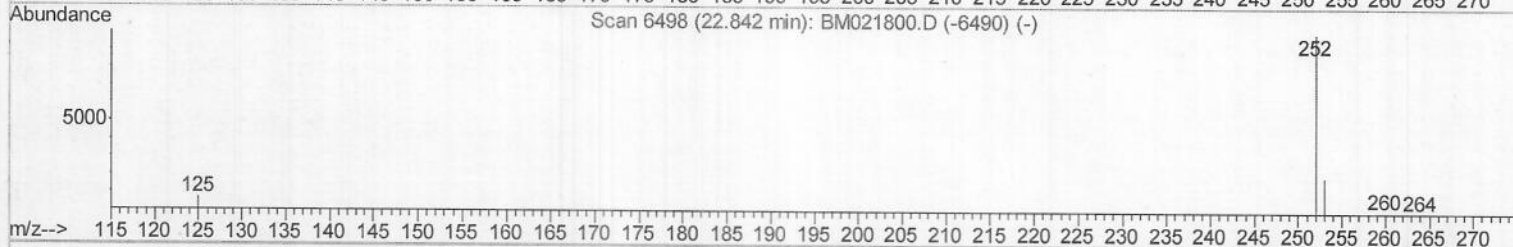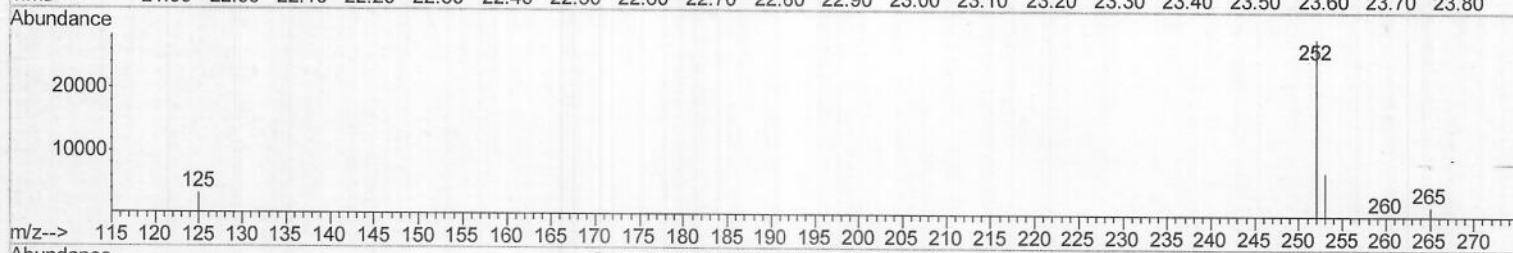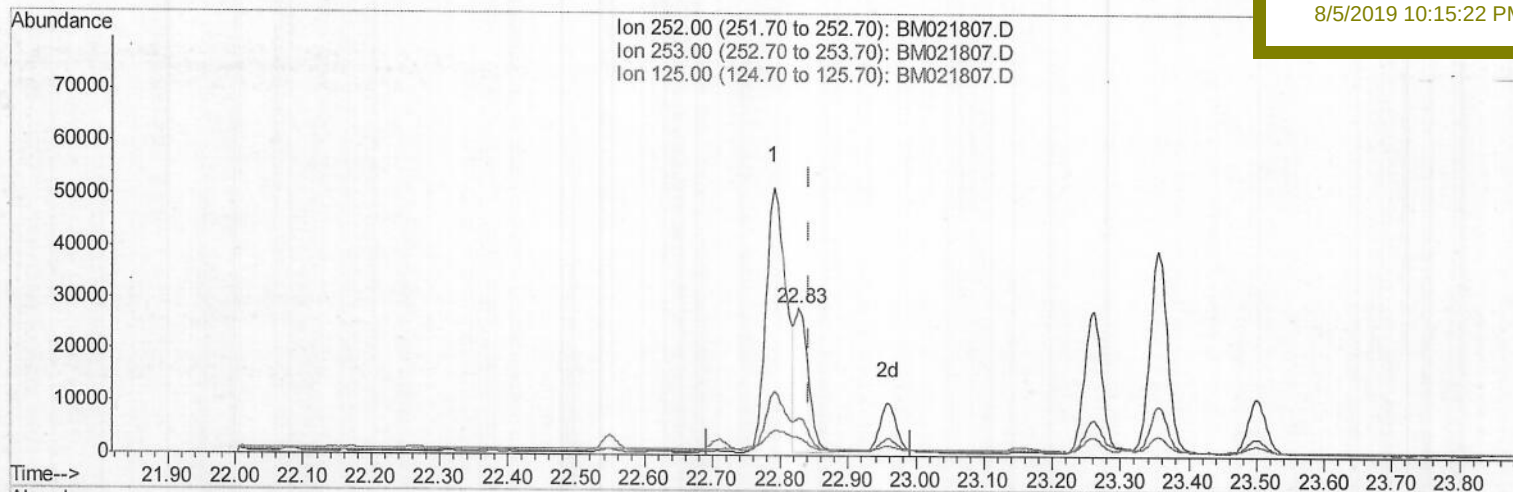

TIC: BM021807.D

(22) Benzo(k)fluoranthene

22.827min (-0.015) 1.53ng/ul m) JU 08/05/19

response 41211

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	24.93#
125.00	15.20	11.75#
0.00	0.00	0.00

Data File : BM021807.D

Acq On : 04 Aug 2019 11:44

Operator : HP/JU

Sample : K3850-17

Misc :

ALS Vial : 50 Sample Multiplier: 1

Quant Time: Aug 05 05:54:46 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Aug 05 05:26:43 2019

Response via : Initial Calibration

Instrument :

BNA_M

Client Sampled :

BENS3

Manual Integrations

APPROVED

mohammad

8/5/2019 10:15:22 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
--------------------	------	------	----------	------	-------	-----------

1) 1,4-Dichlorobenzene-d4	7.64	152	1014	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.42	136	3916	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.29	164	2328	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	5900m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.24	240	6194m	0.40	ng/ul	-0.01
20) Perylene-d12	23.45	264	7044m	0.40	ng/ul	-0.02

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.02	152	1038	0.16	ng/ul	-0.02
14) Fluoranthene-d10	19.08	212	3335m	0.17	ng/ul	-0.01

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.47	128	1417	0.128	ng/ul	95
5) 2-Methylnaphthalene	12.10	142	1275	0.173	ng/ul	95
7) Acenaphthylene	14.01	152	8321	0.766	ng/ul	95
8) Acenaphthene	14.35	153	1573	0.177	ng/ul	95
9) Fluorene	15.34	166	2907	0.295	ng/ul	98
11) Pentachlorophenol	16.71	266	108m	0.099	ng/ul	
12) Phenanthrene	17.08	178	76321m	4.446	ng/ul	
13) Anthracene	17.17	178	15409m	1.052	ng/ul	
15) Fluoranthene	19.11	202	165854m	7.212	ng/ul	
17) Pyrene	19.47	202	127971	5.028	ng/ul	96
18) Benzo(a)anthracene	21.22	228	78602	3.548	ng/ul	99
19) Chrysene	21.27	228	78817	2.766	ng/ul	99
21) Benzo(b)fluoranthene	22.79	252	106094m	4.466	ng/ul	
22) Benzo(k)fluoranthene	22.83	252	41211m	1.533	ng/ul	
23) Benzo(a)pyrene	23.36	252	69128	2.862	ng/ul#	76
24) Indeno(1,2,3-cd)pyrene	25.67	276	53100	1.841	ng/ul#	90
25) Dibenzo(a,h)anthracene	25.67	278	14319	0.614	ng/ul	95
26) Benzo(g,h,i)perylene	26.35	276	49980	1.925	ng/ul#	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed