


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080319\
Data File : BM021831.D
Acq On : 05 Aug 2019 03:32
Operator : HP/JU
Sample : K3863-13
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52F3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:16:48 PM

Quant Time: Aug 05 09:03:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 08:19:16 2019
Response via : Initial Calibration

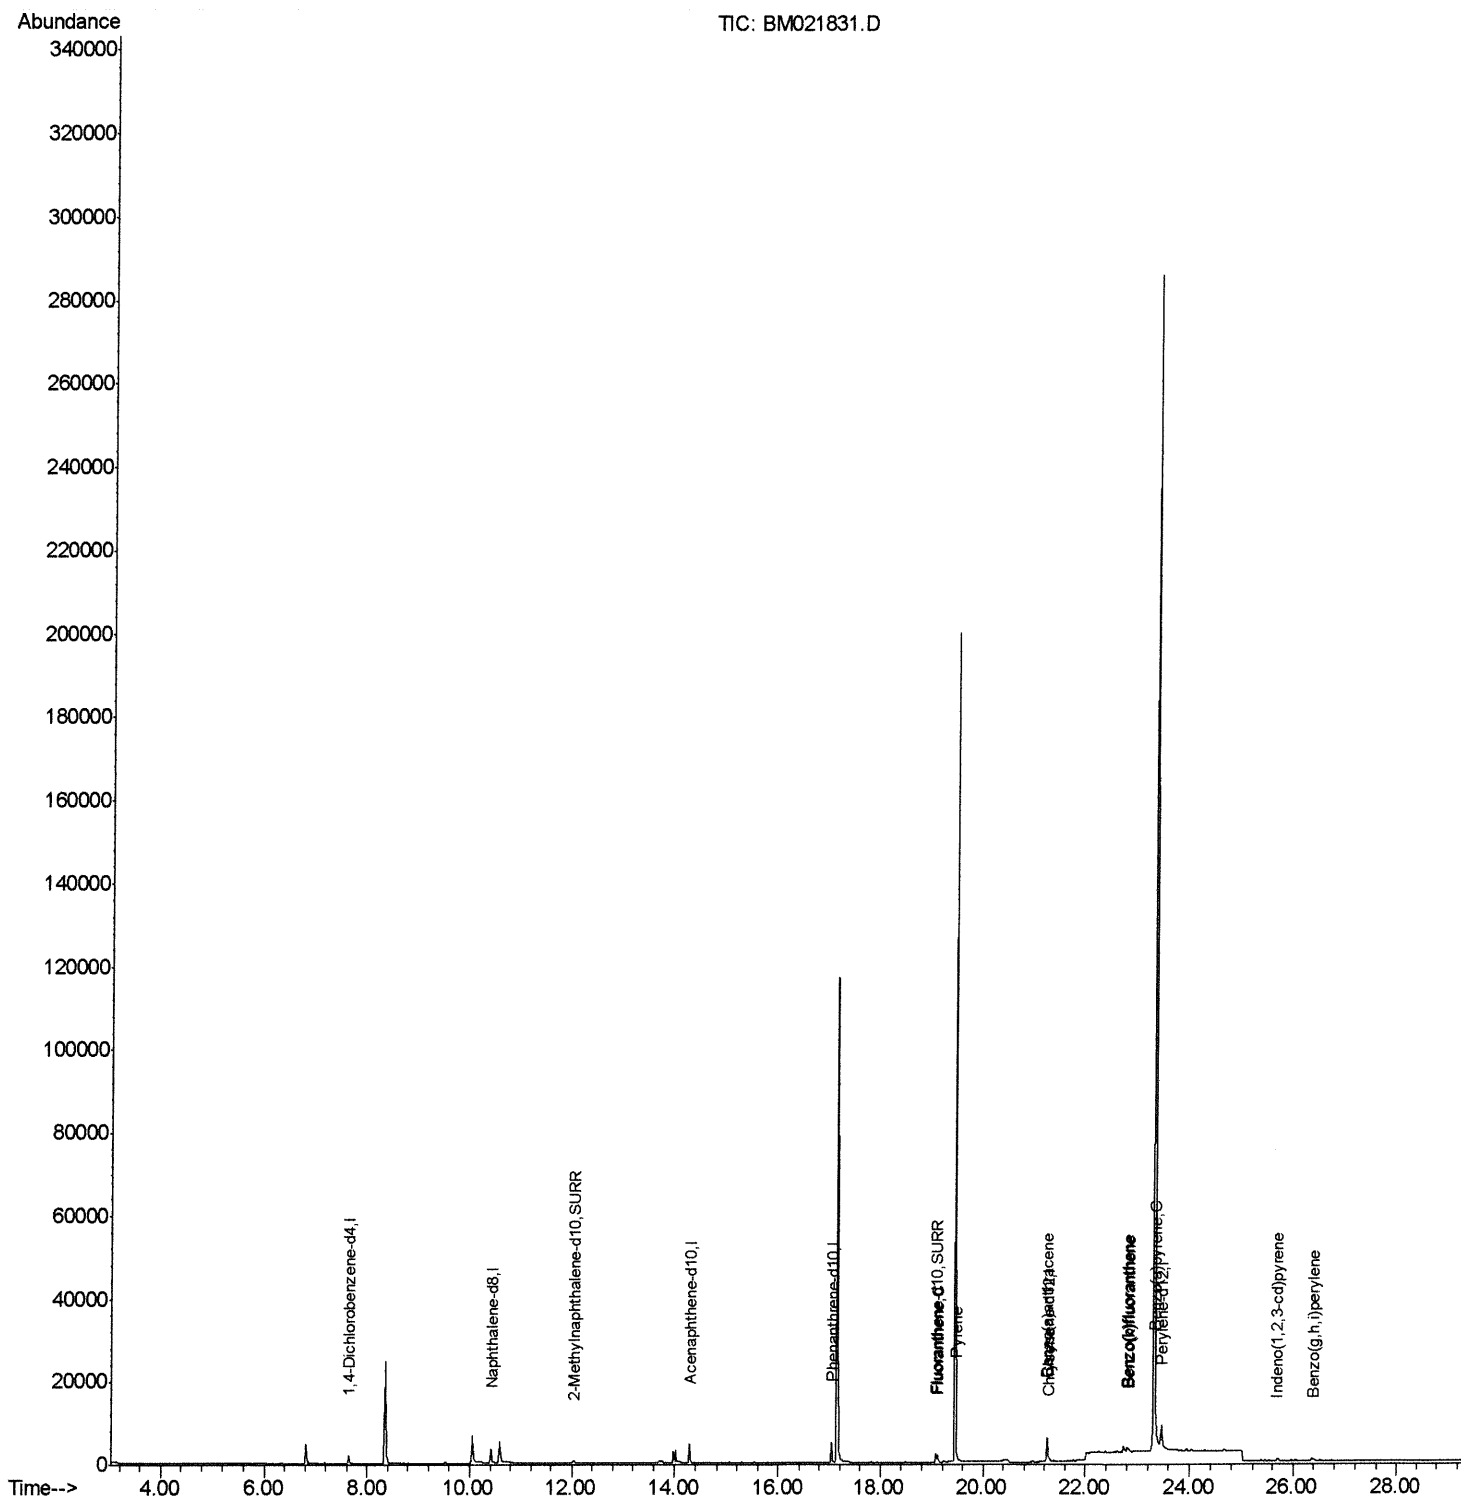




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080319\
Data File : BM021830.D
Acq On : 05 Aug 2019 02:56
Operator : HP/JU
Sample : K3863-03RE
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52F3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:16:48 PM

Quant Time: Aug 05 08:24:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 08:19:16 2019
Response via : Initial Calibration

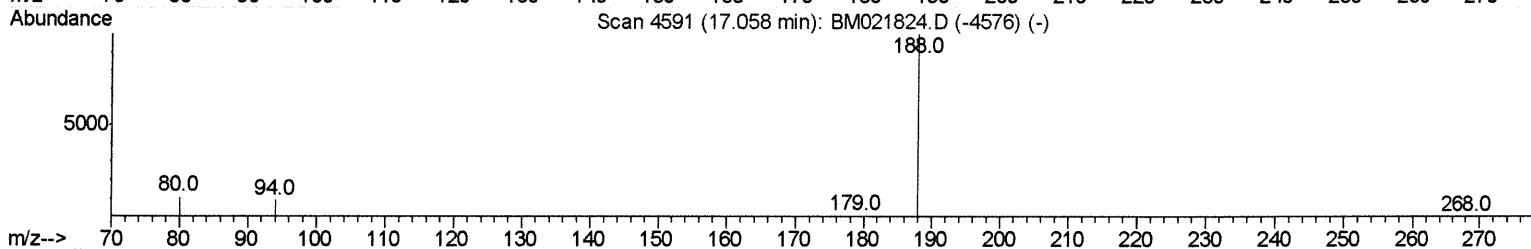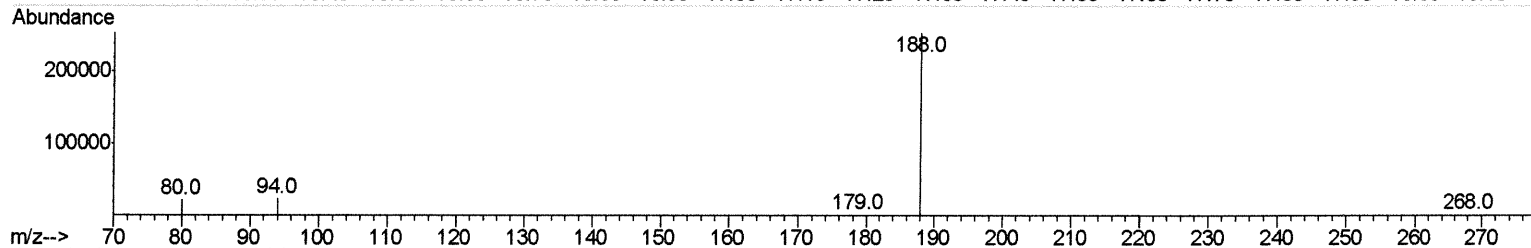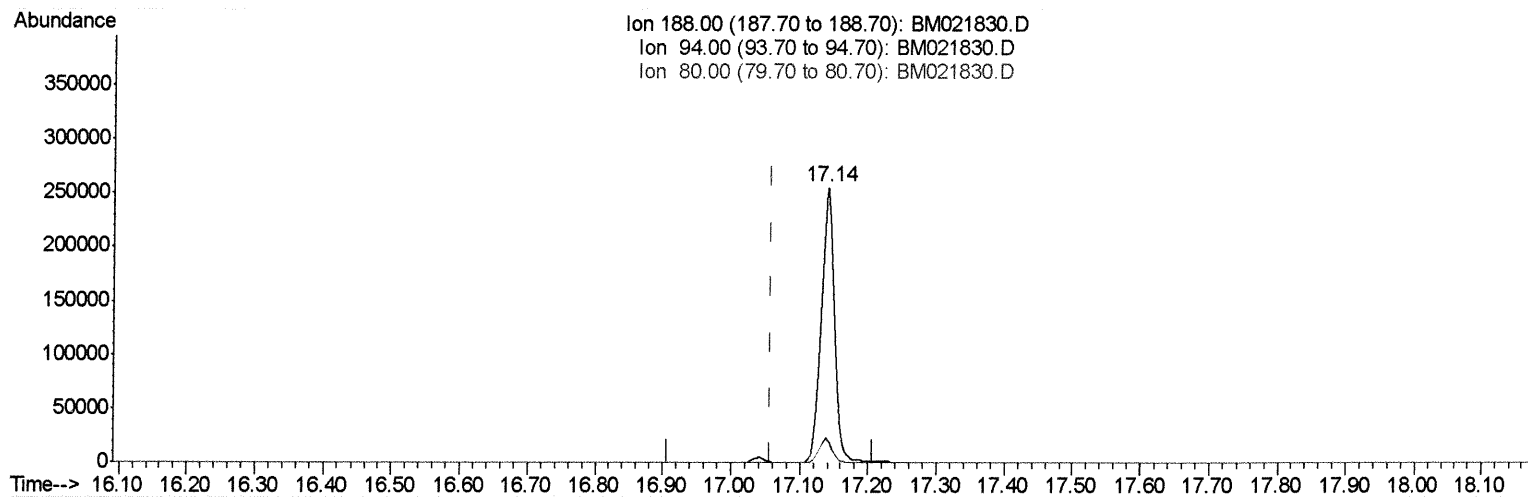

TIC: BM021830.D

(10) Phenanthrene-d10 (I)

17.140min (+0.082) 0.40ng/ul

response 344727

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	8.66
80.00	11.40	8.22#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080319\
 Data File : BM021830.D
 Acq On : 05 Aug 2019 02:56
 Operator : HP/JU
 Sample : K3863-03RE
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52F3

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:16:48 PM

Quant Time: Aug 05 08:24:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 08:19:16 2019
 Response via : Initial Calibration

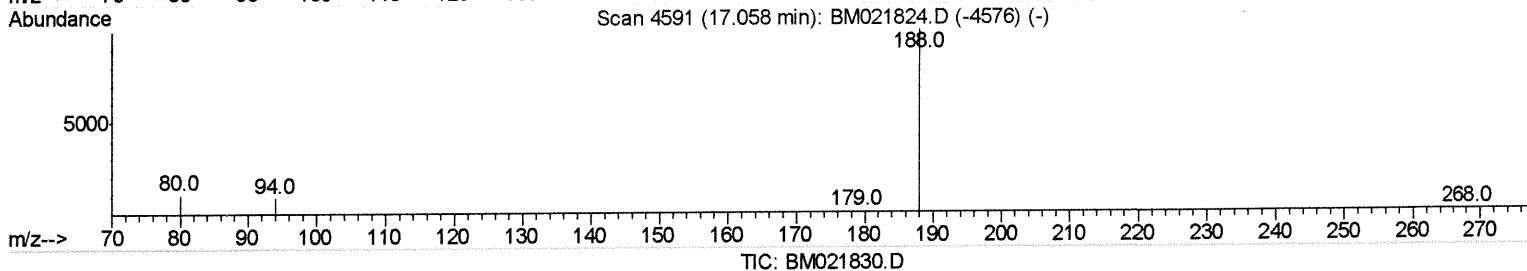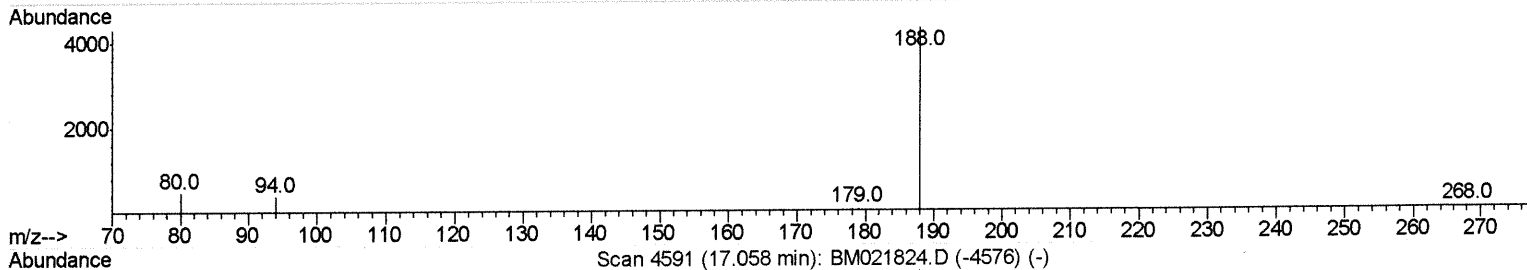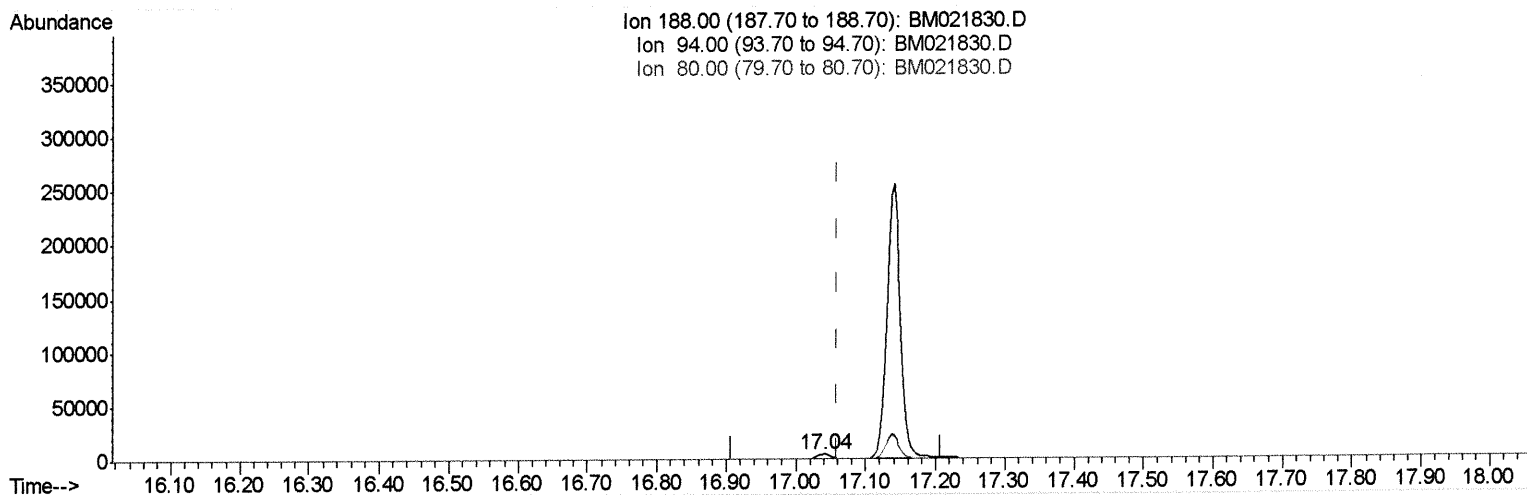

(10) Phenanthrene-d10 (I)

17.039min (-0.019) 0.40ng/ul m *JU 08/05/19*

response 6161

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	9.01
80.00	11.40	11.14
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080319\
 Data File : BM021830.D
 Acq On : 05 Aug 2019 02:56
 Operator : HP/JU
 Sample : K3863-03RE
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52F3

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:16:48 PM

Quant Time: Aug 05 08:56:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 08:19:16 2019
 Response via : Initial Calibration

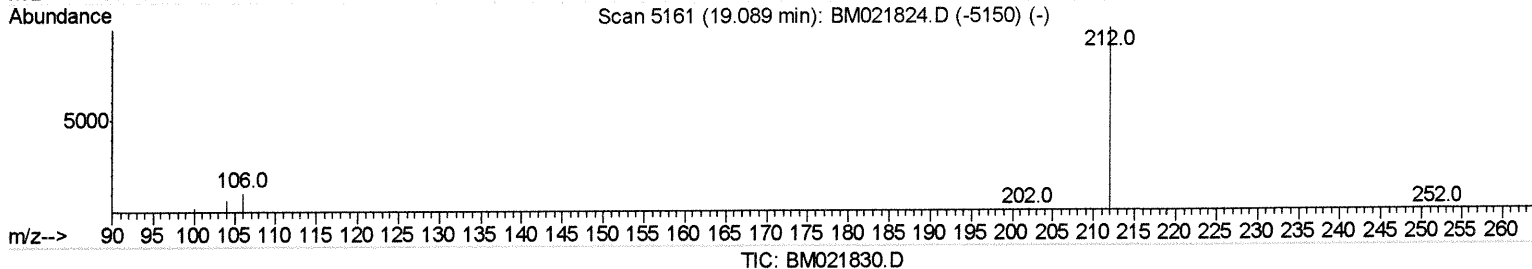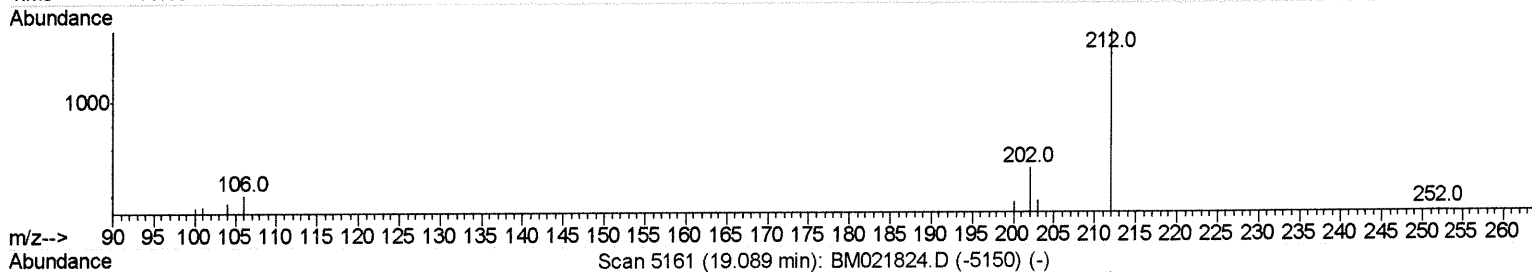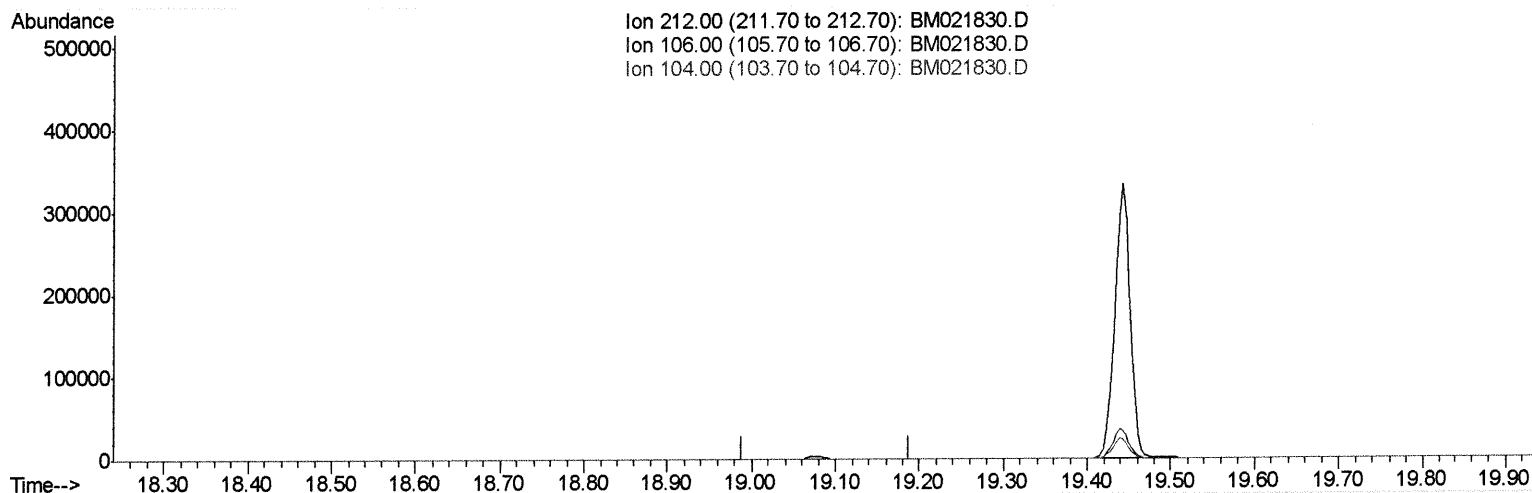

(14) Fluoranthene-d10 (SURR)

19.089min (-19.089) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	9.90	0.00#
104.00	6.00	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080319\
Data File : BM021830.D
Acq On : 05 Aug 2019 02:56
Operator : HP/JU
Sample : K3863-03RE
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52F3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:16:48 PM

Quant Time: Aug 05 08:56:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 08:19:16 2019
Response via : Initial Calibration

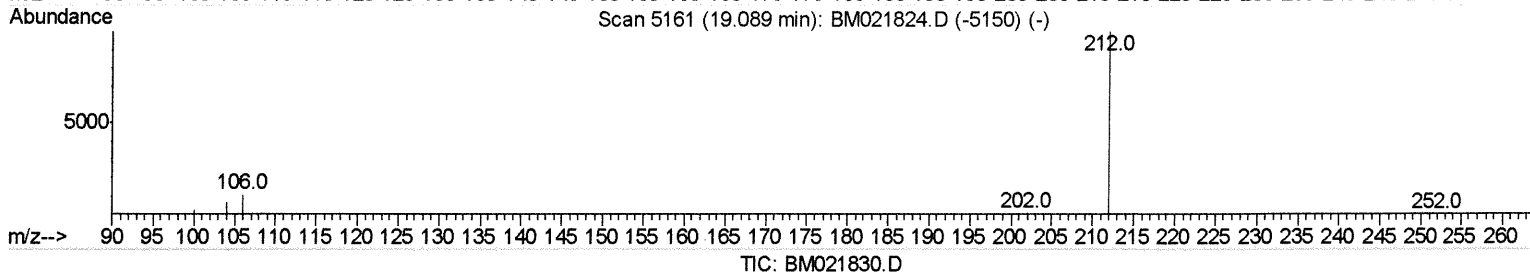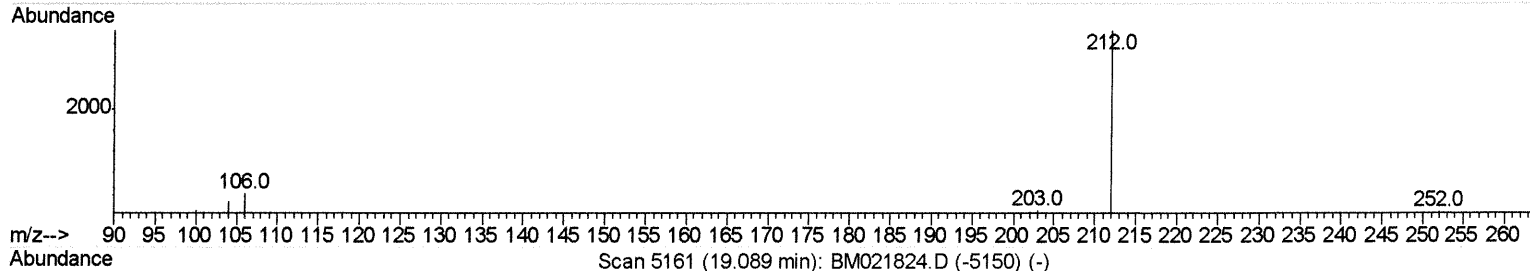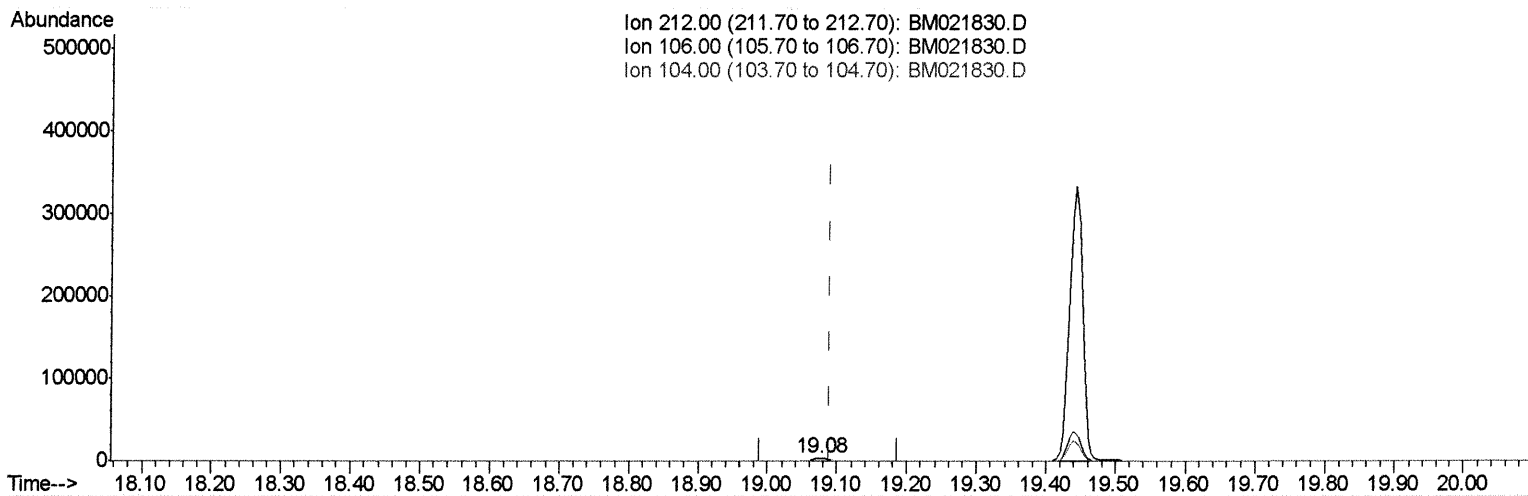

(14) Fluoranthene-d10 (SURR)

19.076min (-0.013) 0.23ng/ul m

JU
08/05/19

response 4727

Ion	Exp%	Act%
212.00	100	100
106.00	9.90	0.00#
104.00	6.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080319\
 Data File : BM021830.D
 Acq On : 05 Aug 2019 02:56
 Operator : HP/JU
 Sample : K3863-03RE
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52F3

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:16:48 PM

Quant Time: Aug 05 08:56:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 08:19:16 2019
 Response via : Initial Calibration

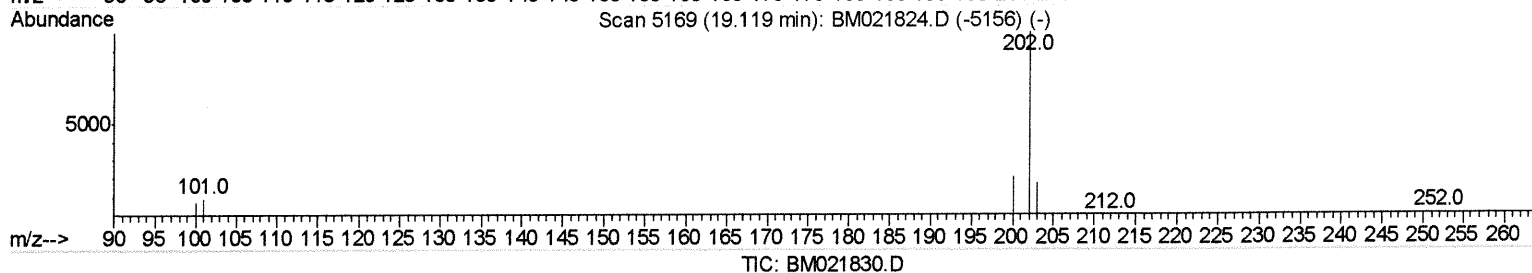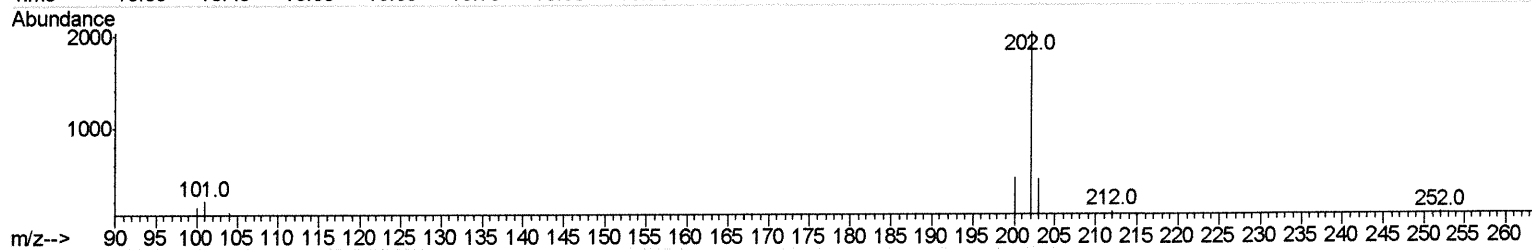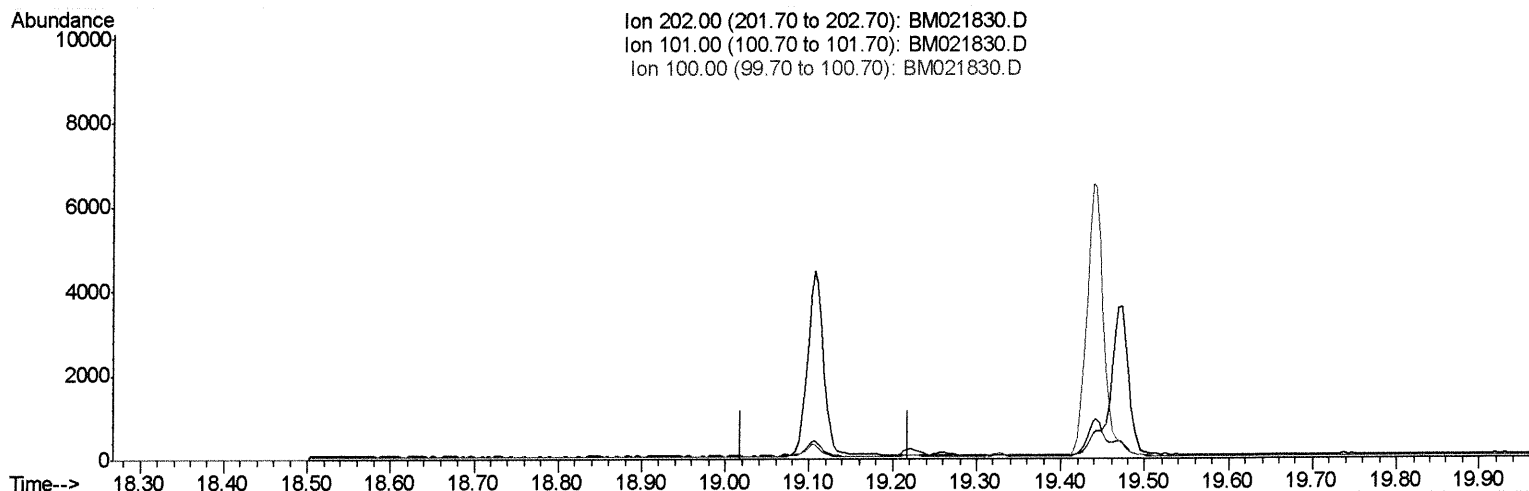

(15) Fluoranthene (C)

19.119min (-19.119) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	10.20	0.00
100.00	8.10	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080319\
 Data File : BM021830.D
 Acq On : 05 Aug 2019 02:56
 Operator : HP/JU
 Sample : K3863-03RE
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52F3

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:16:48 PM

Quant Time: Aug 05 08:56:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 08:19:16 2019
 Response via : Initial Calibration

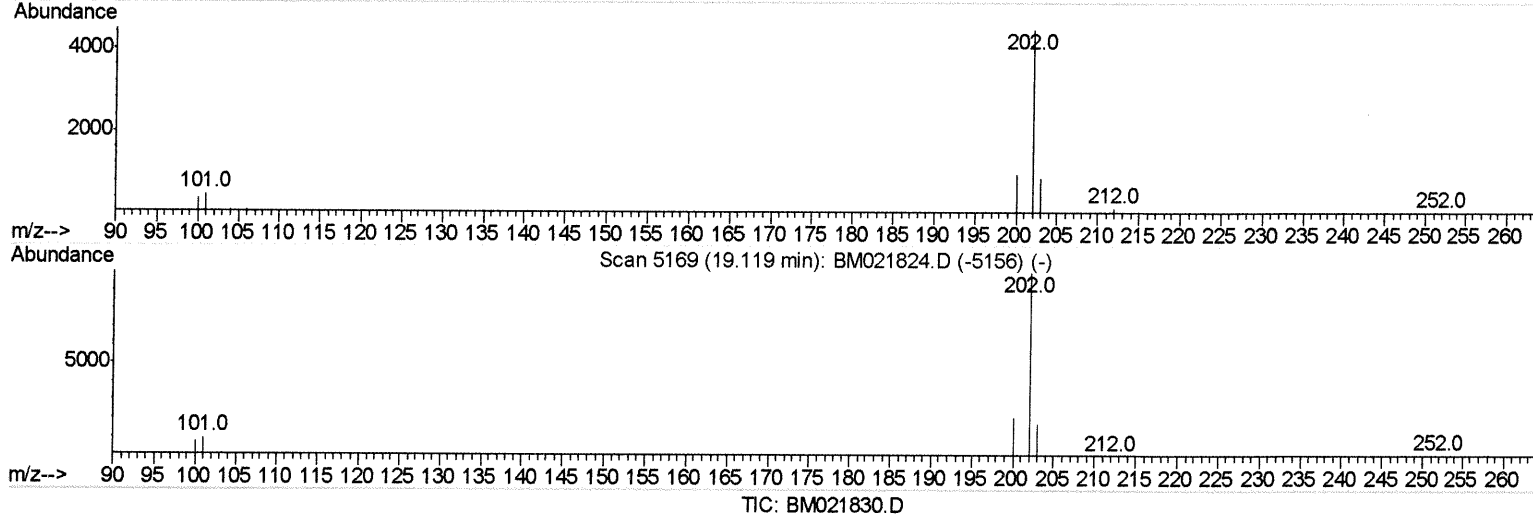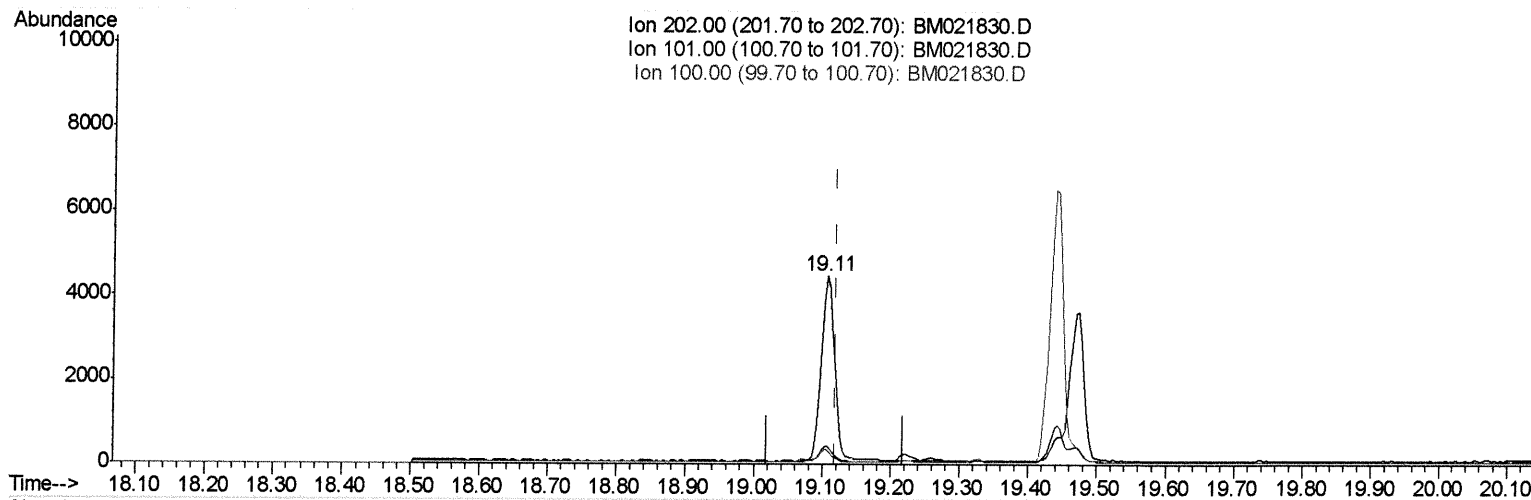

(15) Fluoranthene (C)

19.106min (-0.013) 0.25ng/ul m *JU 08/05/19*

response 5978

Ion	Exp%	Act%
202.00	100	100
101.00	10.20	10.29
100.00	8.10	7.98
0.00	0.00	0.00



Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080319\
Data File : BM021830.D
Acq On : 05 Aug 2019 02:56
Operator : HP/JU
Sample : K3863-03RE
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52F3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:16:48 PM

Quant Time: Aug 05 08:56:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 08:19:16 2019
Response via : Initial Calibration

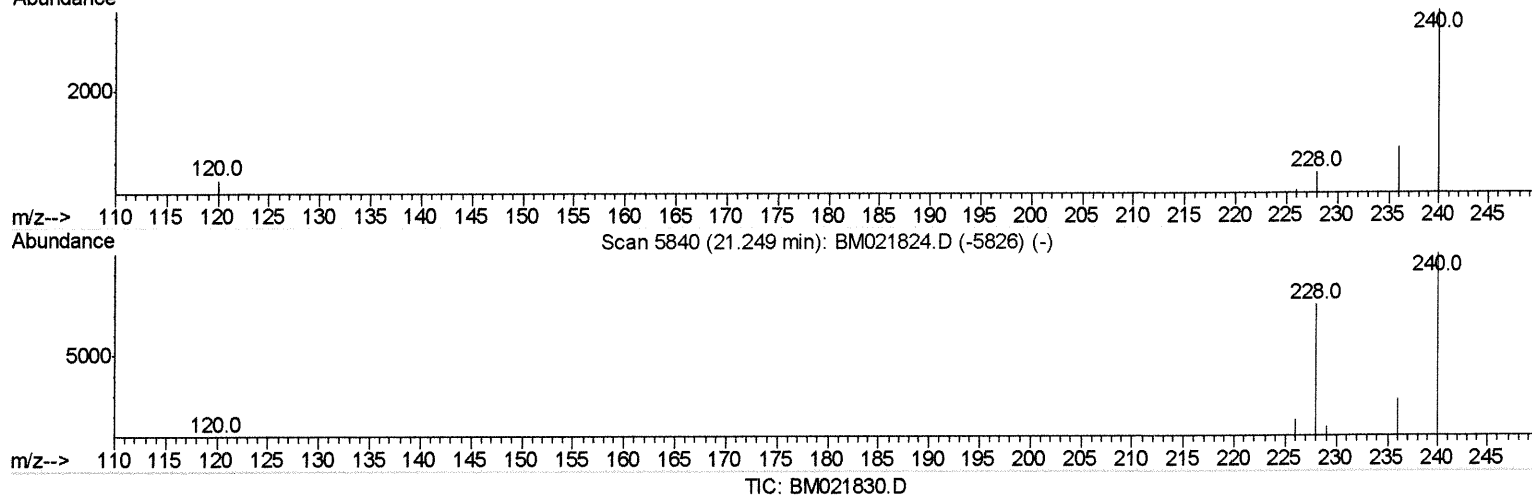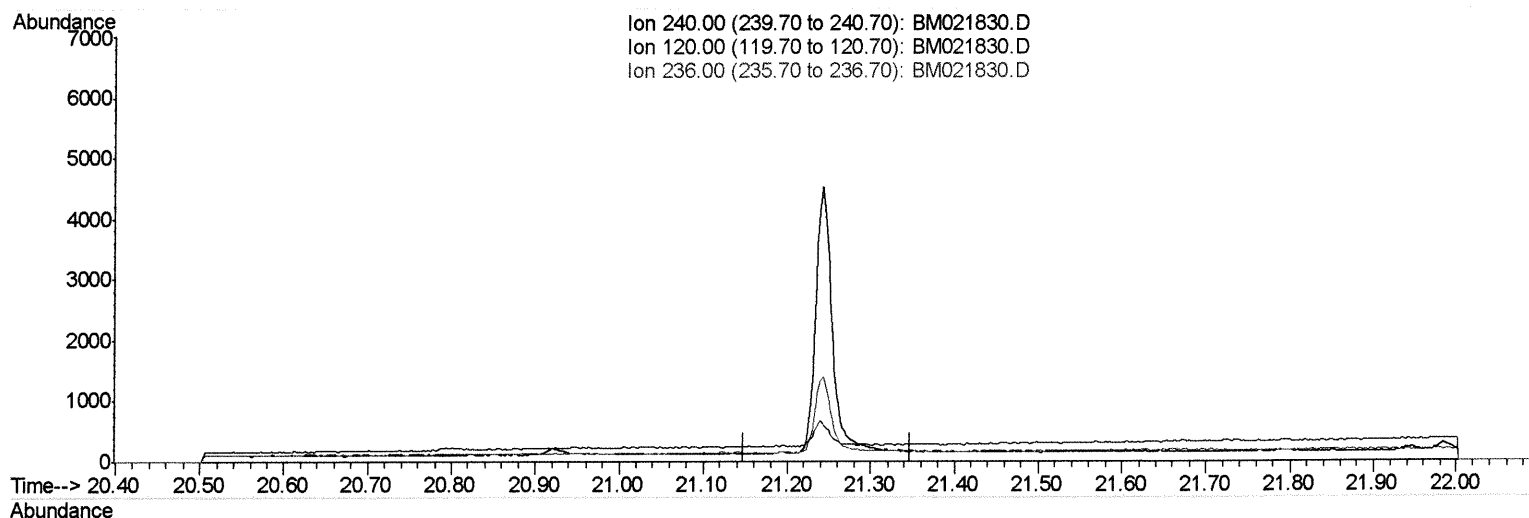

(16) Chrysene-d12 (I)

21.249min (-21.249) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.20	0.00#
236.00	32.30	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080319\
 Data File : BM021830.D
 Acq On : 05 Aug 2019 02:56
 Operator : HP/JU
 Sample : K3863-03RE
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52F3

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:16:48 PM

Quant Time: Aug 05 08:56:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 08:19:16 2019
 Response via : Initial Calibration

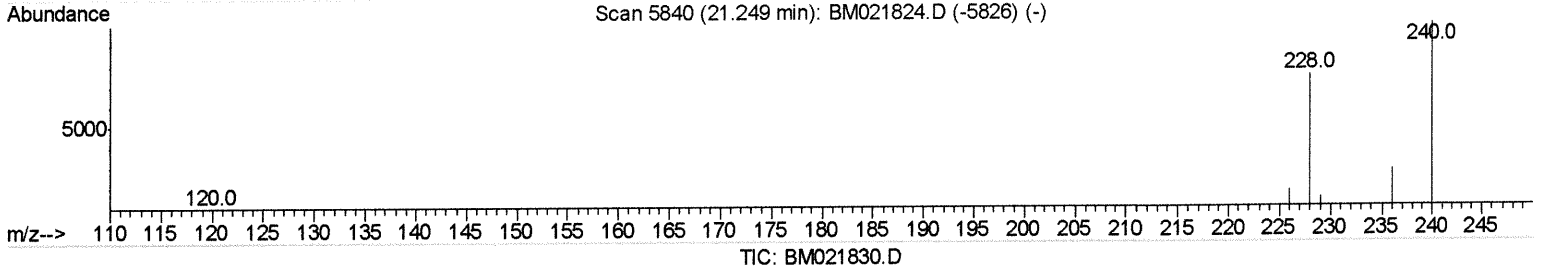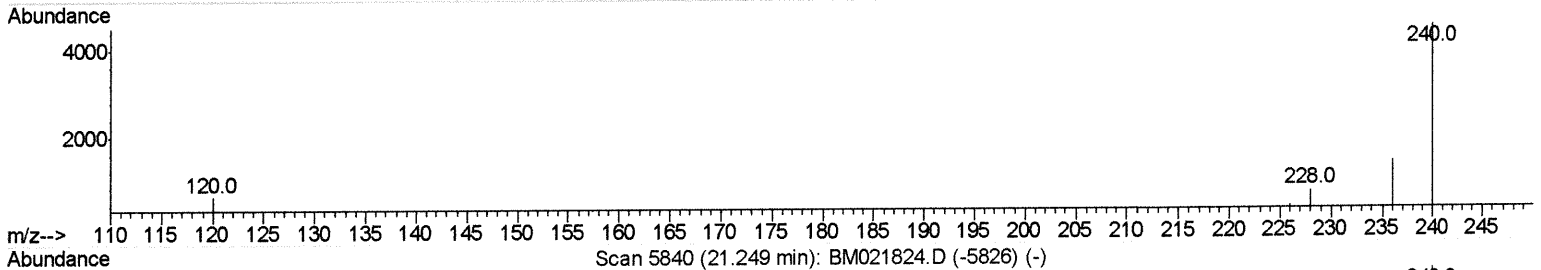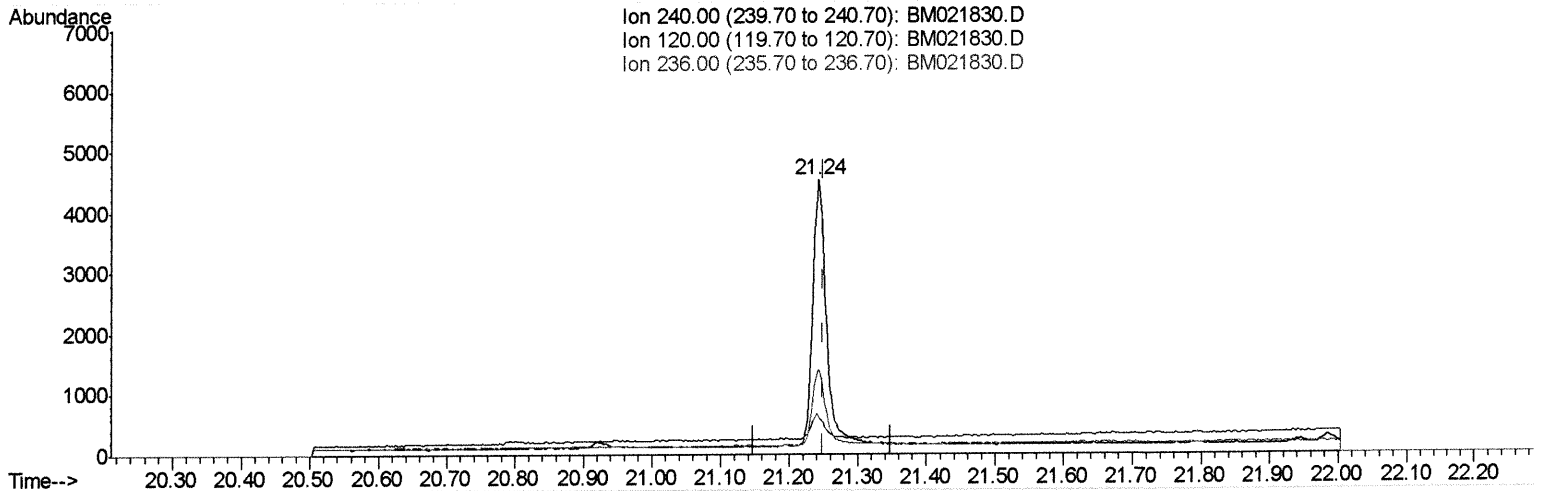

(16) Chrysene-d12 (I)

21.241min (-0.007) 0.40ng/ul m *JU 08/05/19*

response 5953

Ion	Exp%	Act%
240.00	100	100
120.00	16.20	14.06
236.00	32.30	30.93
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080319\
Data File : BM021830.D
Acq On : 05 Aug 2019 02:56
Operator : HP/JU
Sample : K3863-03RE
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52F3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:16:48 PM

Quant Time: Aug 05 08:57:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 08:19:16 2019
Response via : Initial Calibration

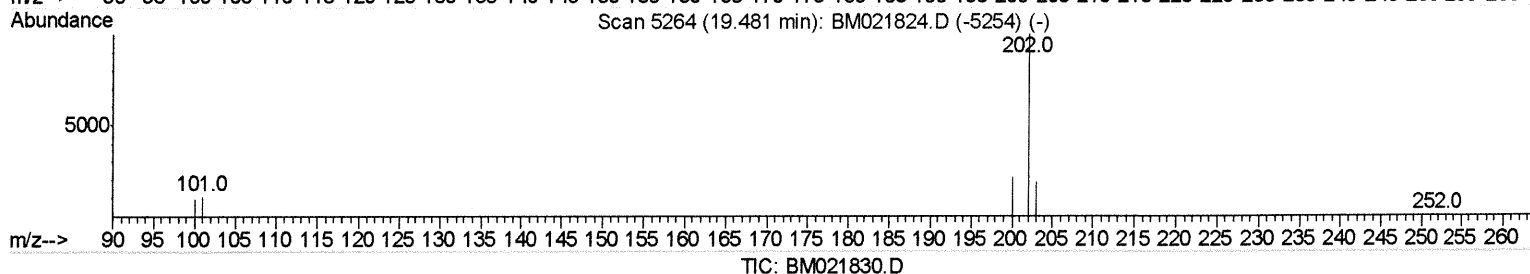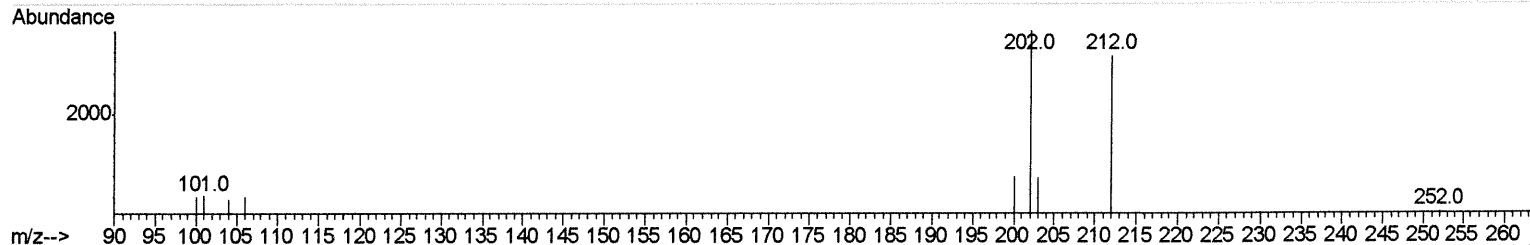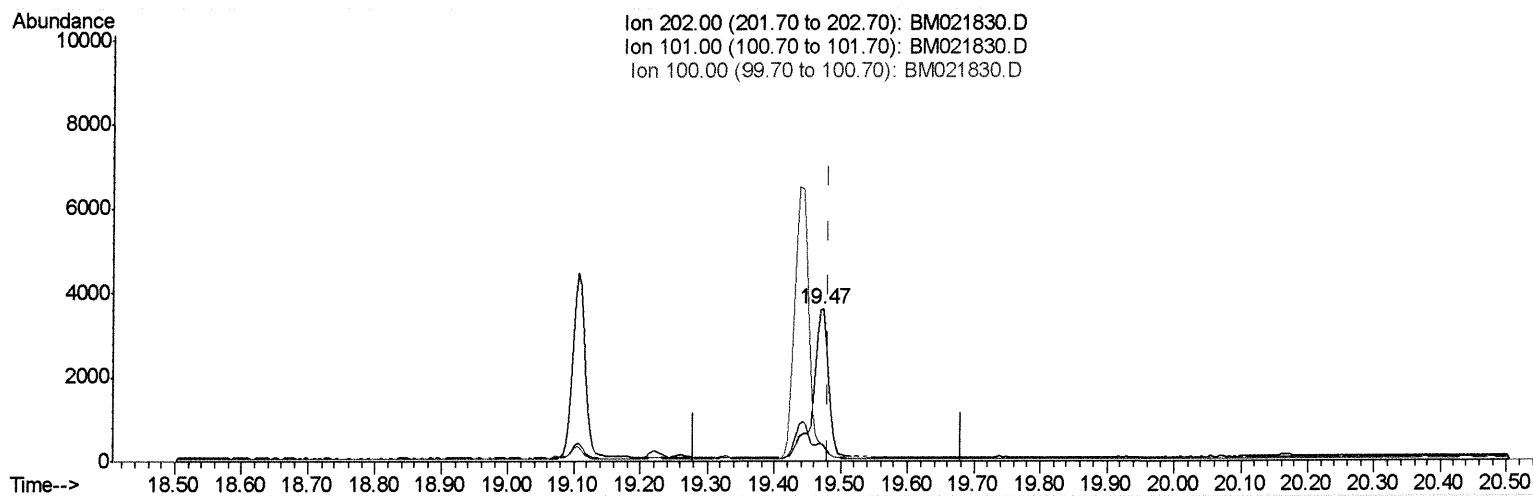

(17) Pyrene

19.472min (-0.009) 0.23ng/ul

response 5653

Ion	Exp%	Act%
202.00	100	100
101.00	10.40	11.30
100.00	9.00	10.91#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080319\
Data File : BM021830.D
Acq On : 05 Aug 2019 02:56
Operator : HP/JU
Sample : K3863-03RE
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52F3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:16:48 PM

Quant Time: Aug 05 08:57:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 08:19:16 2019
Response via : Initial Calibration

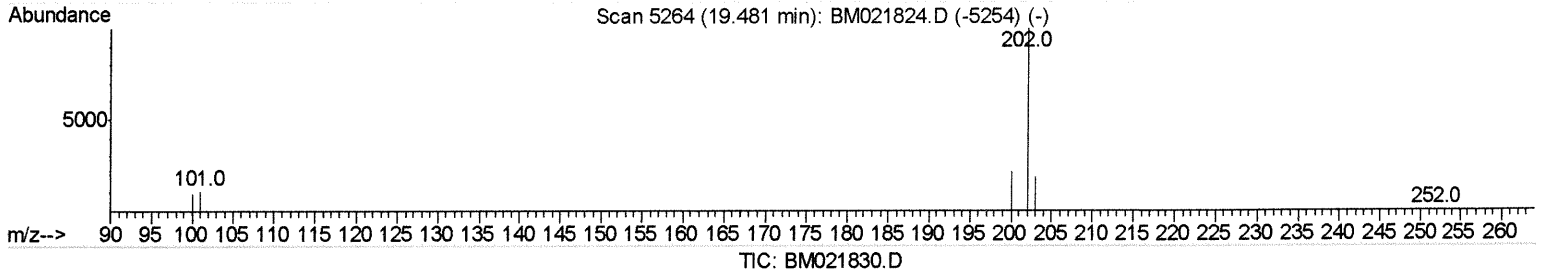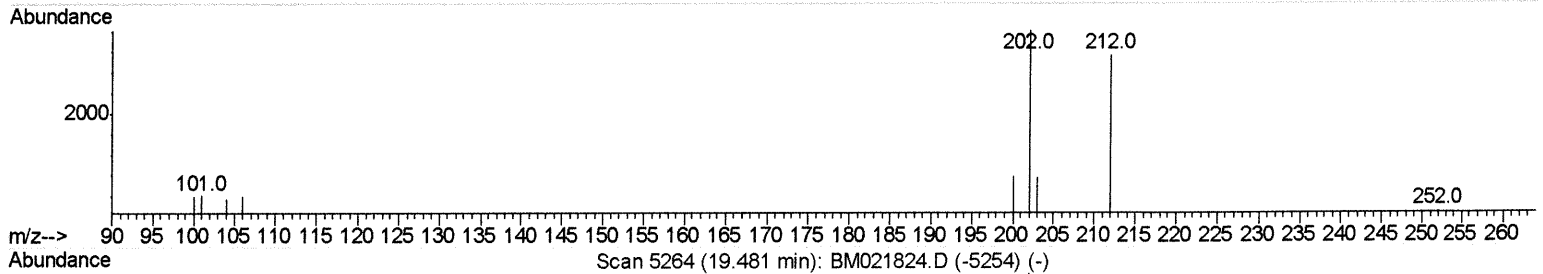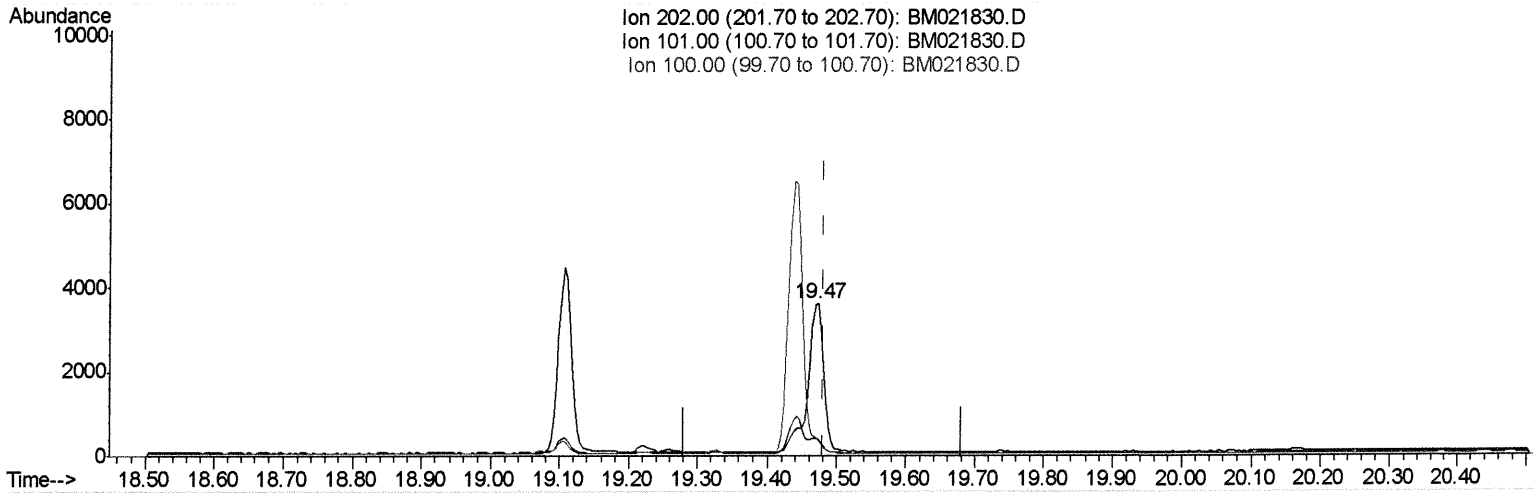

(17) Pyrene

19.472min (-0.009) 0.20ng/ul m *JU 8/5/19*

response 4890

Ion	Exp%	Act%
202.00	100	100
101.00	10.40	11.30
100.00	9.00	10.91#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080319\
Data File : BM021830.D
Acq On : 05 Aug 2019 02:56
Operator : HP/JU
Sample : K3863-03RE
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52F3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:16:48 PM

Quant Time: Aug 05 08:57:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 08:19:16 2019
Response via : Initial Calibration

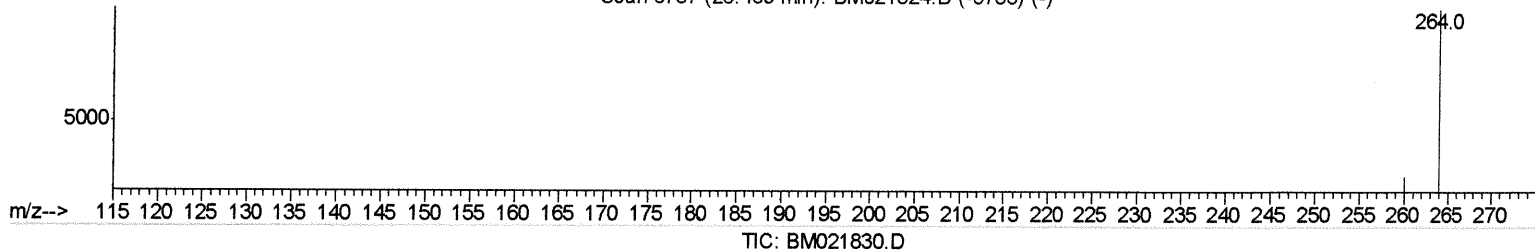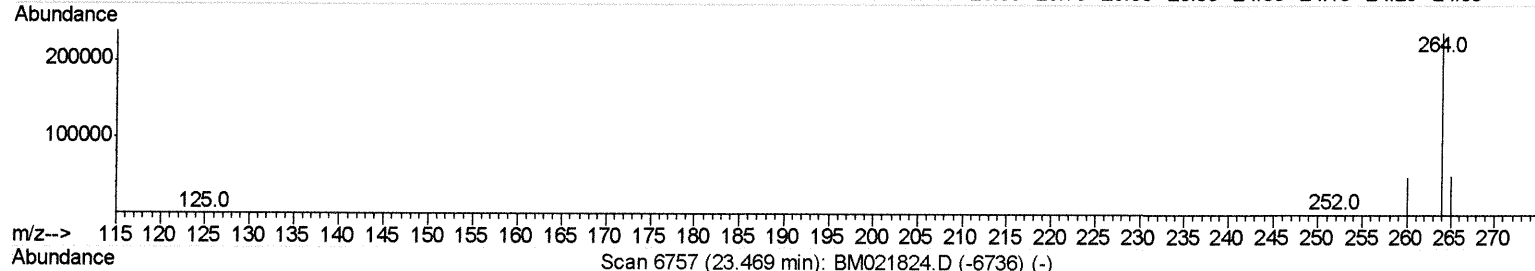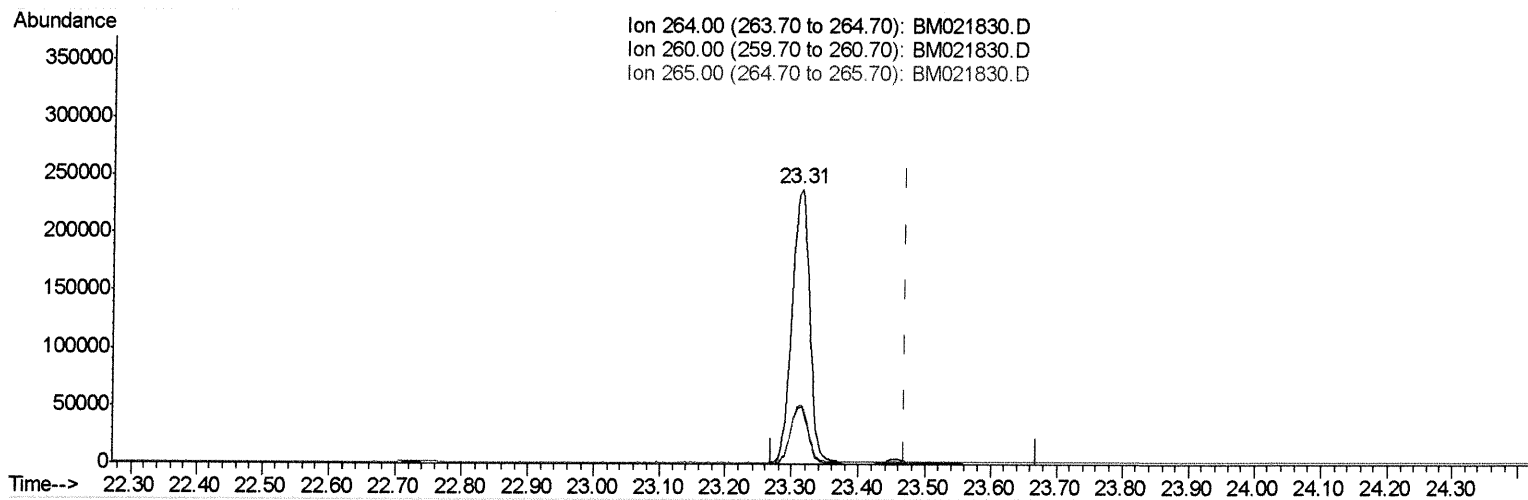

(20) Perylene-d12 (I)

23.312min (-0.158) 0.40ng/ul

response 435627

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	21.03#
265.00	117.00	21.82#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080319\
 Data File : BM021830.D
 Acq On : 05 Aug 2019 02:56
 Operator : HP/JU
 Sample : K3863-03RE
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52F3

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:16:48 PM

Quant Time: Aug 05 08:57:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 08:19:16 2019
 Response via : Initial Calibration

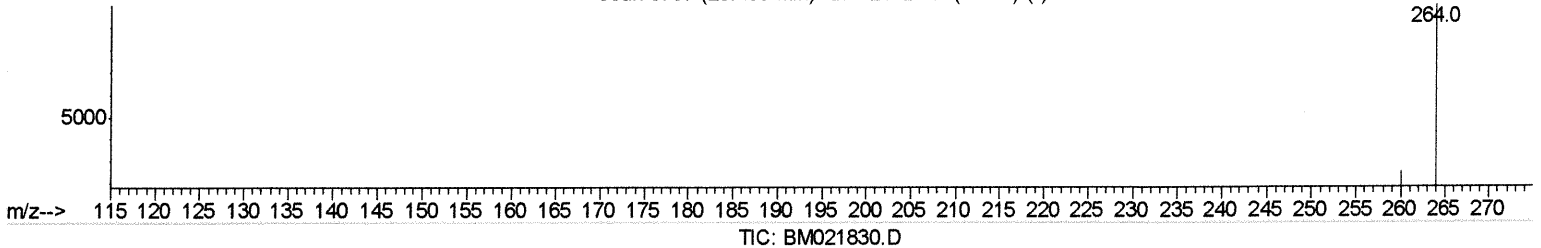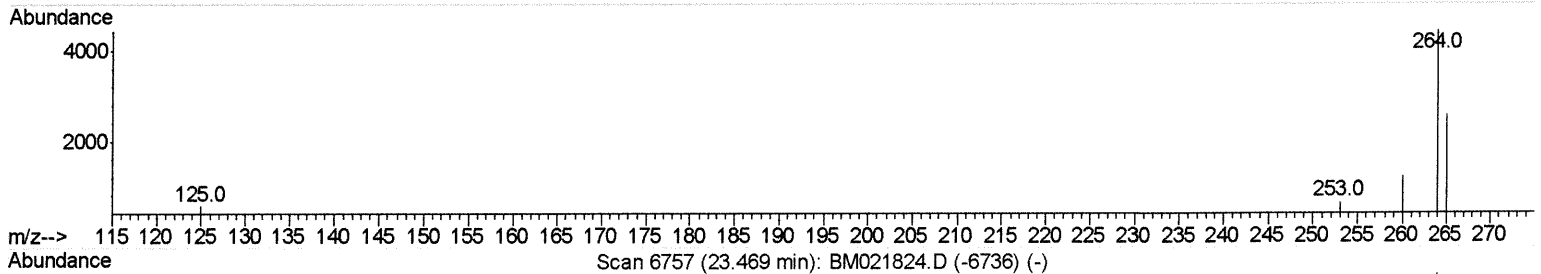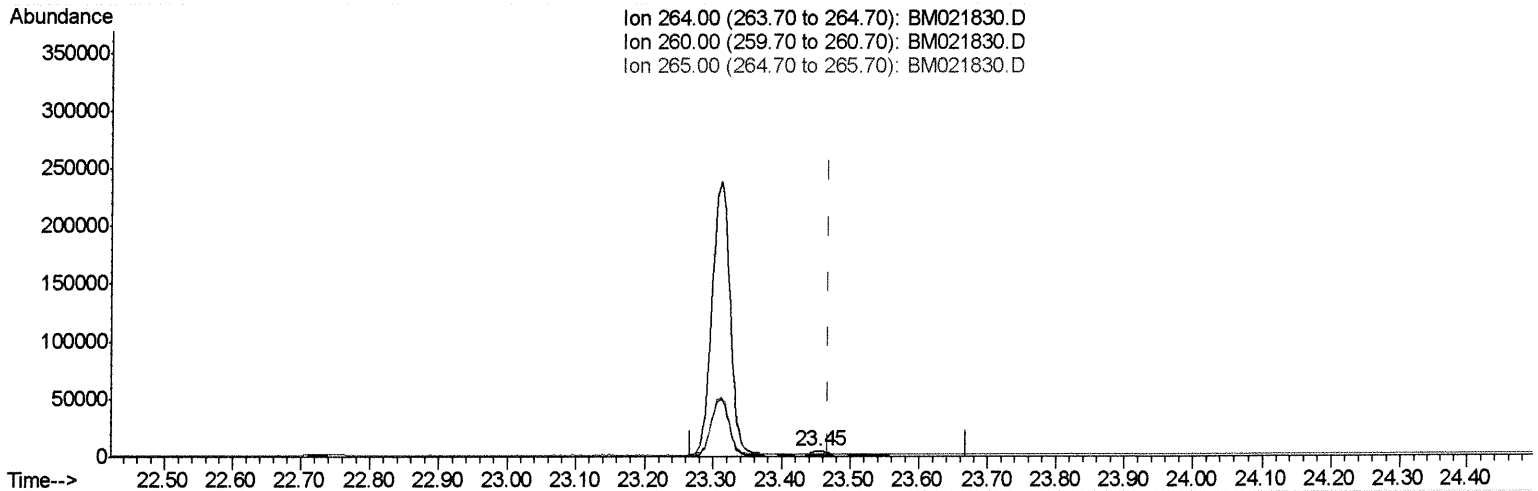

(20) Perylene-d12 (I)

23.455min (-0.015) 0.40ng/ul m *JU 08/05/19*

response 6378

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	27.27
265.00	117.00	57.79#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080319\
Data File : BM021830.D
Acq On : 05 Aug 2019 02:56
Operator : HP/JU
Sample : K3863-03RE
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52F3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:16:48 PM

Quant Time: Aug 05 08:58:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 08:19:16 2019
Response via : Initial Calibration

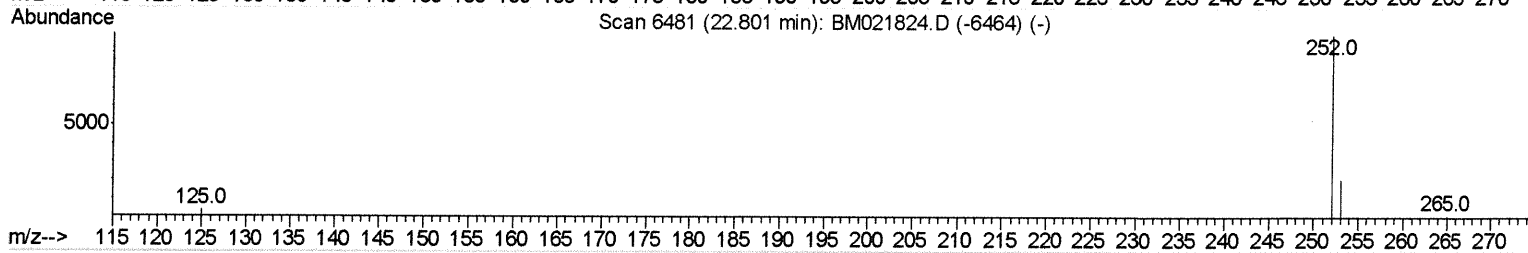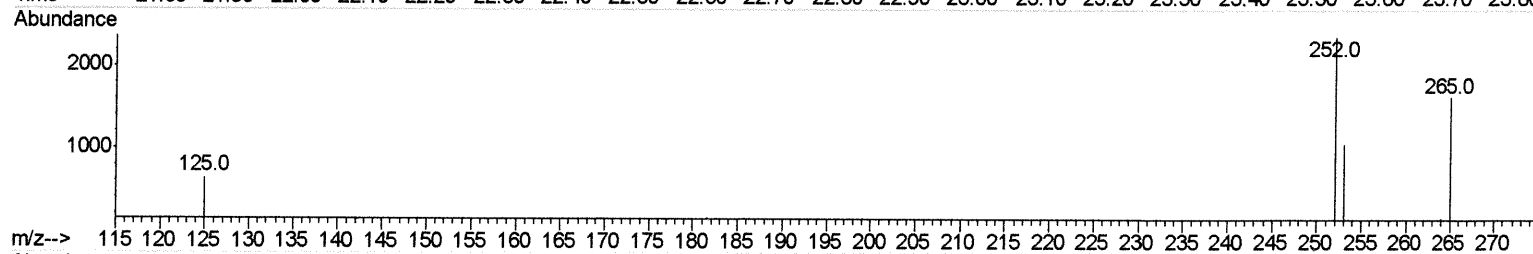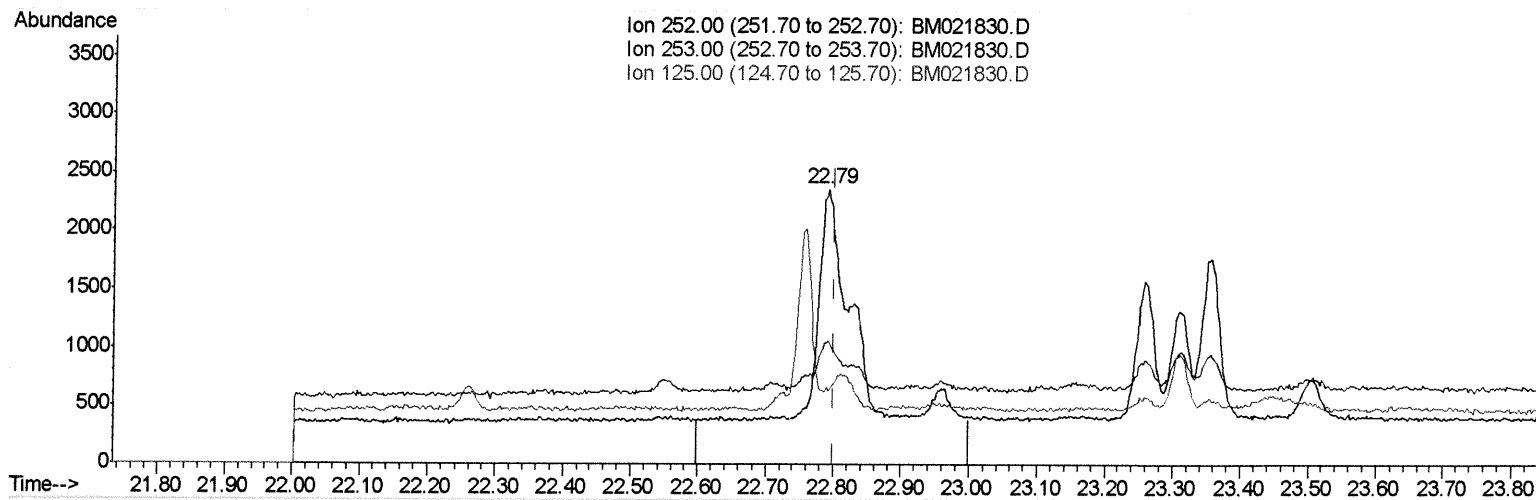

TIC: BM021830.D

(21) Benzo(b)fluoranthene

22.791min (-0.010) 0.24ng/ul

response 5225

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	44.93
125.00	15.50	27.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080319\
 Data File : BM021830.D
 Acq On : 05 Aug 2019 02:56
 Operator : HP/JU
 Sample : K3863-03RE
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52F3

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:16:48 PM

Quant Time: Aug 05 08:58:13 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 08:19:16 2019
 Response via : Initial Calibration

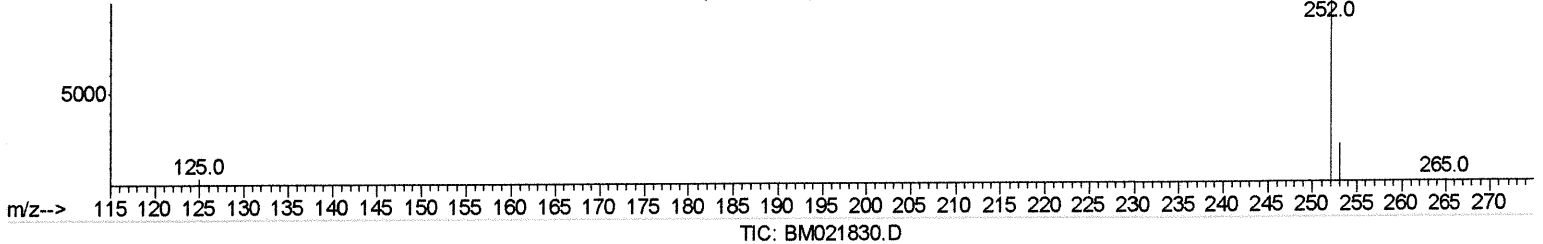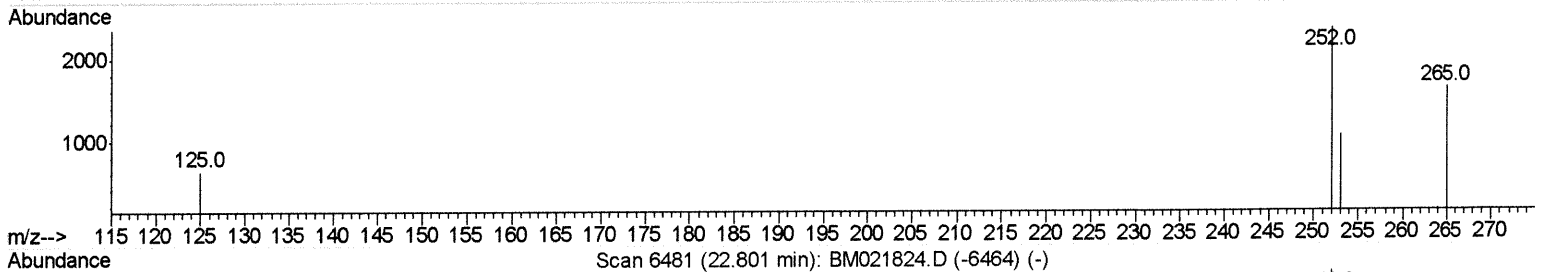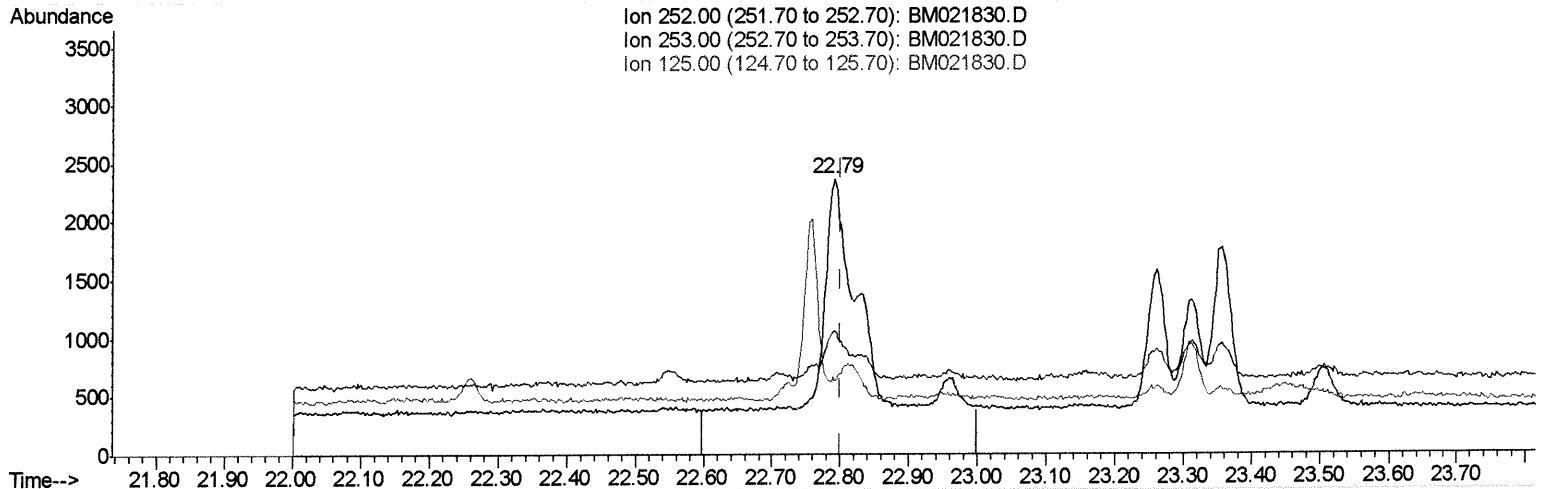

(21) Benzo(b)fluoranthene

22.791min (-0.010) 0.19ng/ul m *Ju* *08/05/19*

response 4139

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	44.93
125.00	15.50	27.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080319\
 Data File : BM021831.D
 Acq On : 05 Aug 2019 03:32
 Operator : HP/JU
 Sample : K3863-13
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52F3

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:16:48 PM

Quant Time: Aug 05 09:01:54 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 08:19:16 2019
 Response via : Initial Calibration

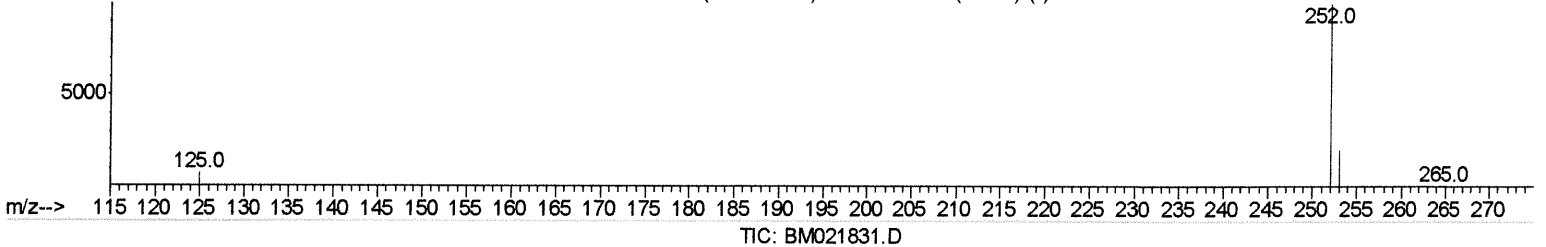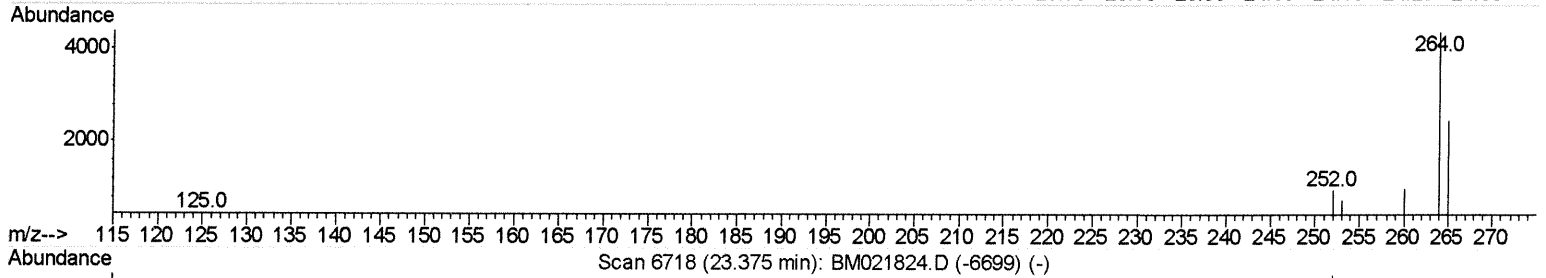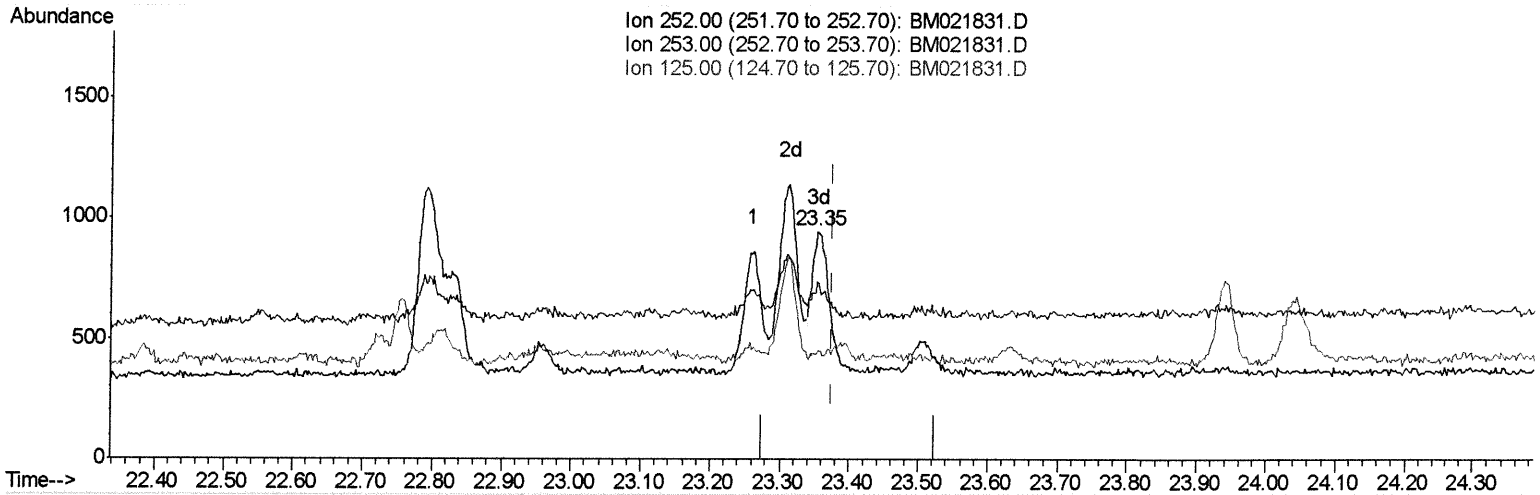

(23) Benzo(a)pyrene (C)

23.353min (-0.022) 0.04ng/ul m *Ju* 08/05/19

response 1035

Ion	Exp%	Act%
252.00	100	100
253.00	39.60	78.01#
125.00	18.20	46.72#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080319\
 Data File : BM021831.D
 Acq On : 05 Aug 2019 03:32
 Operator : HP/JU
 Sample : K3863-13
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52F3

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:16:48 PM

Quant Time: Aug 05 09:01:54 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 08:19:16 2019
 Response via : Initial Calibration

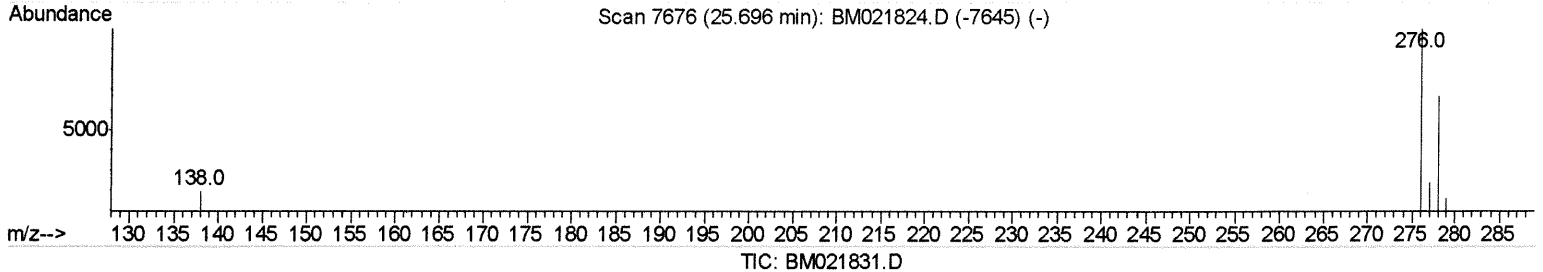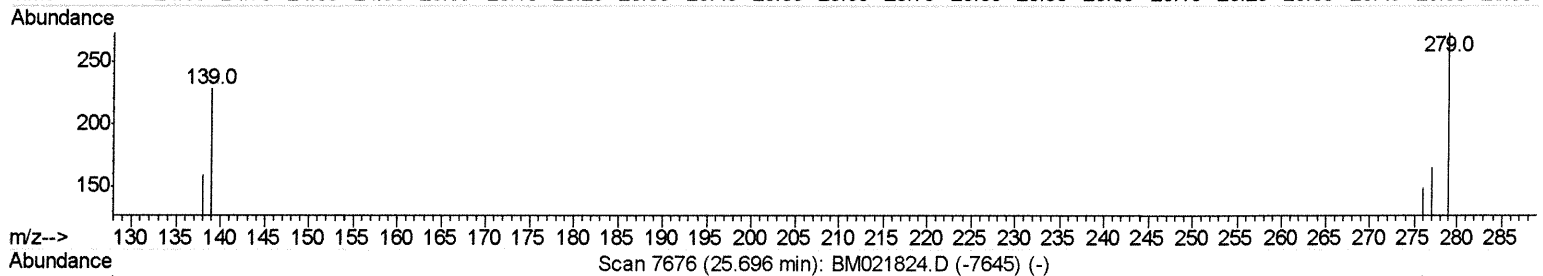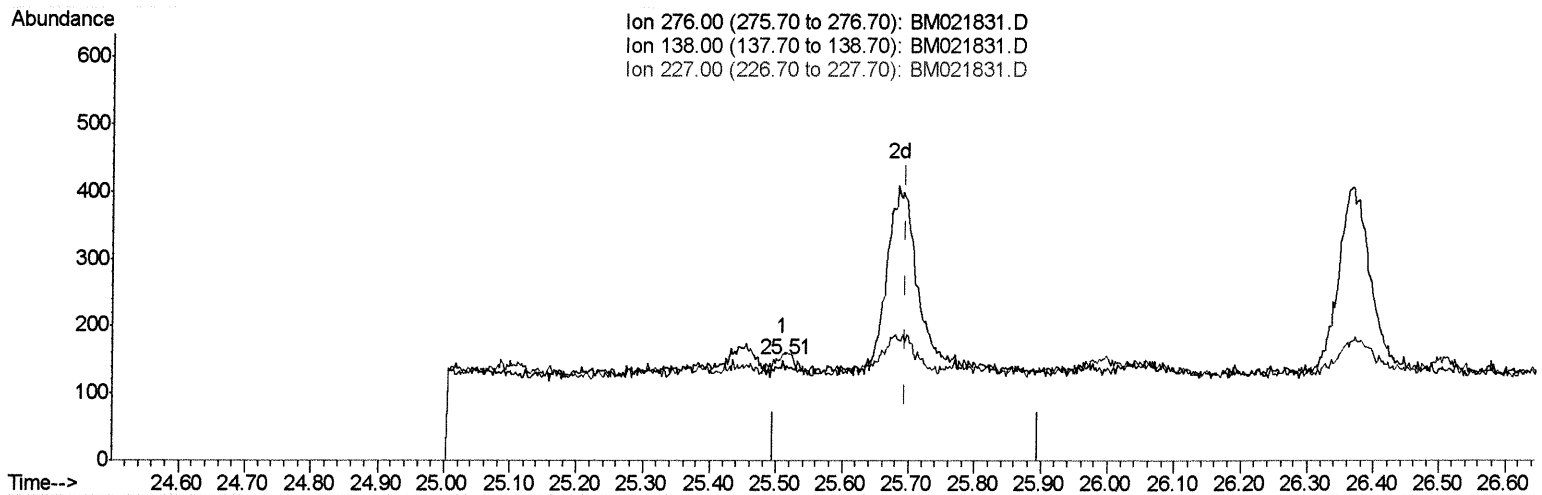

(24) Indeno(1,2,3-cd)pyrene

25.509min (-0.187) 0.00ng/ul

response 29

Ion	Exp%	Act%
276.00	100	100
138.00	18.90	231.03#
227.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080319\
 Data File : BM021831.D
 Acq On : 05 Aug 2019 03:32
 Operator : HP/JU
 Sample : K3863-13
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 A52F3

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:16:48 PM

Quant Time: Aug 05 09:01:54 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 08:19:16 2019
 Response via : Initial Calibration

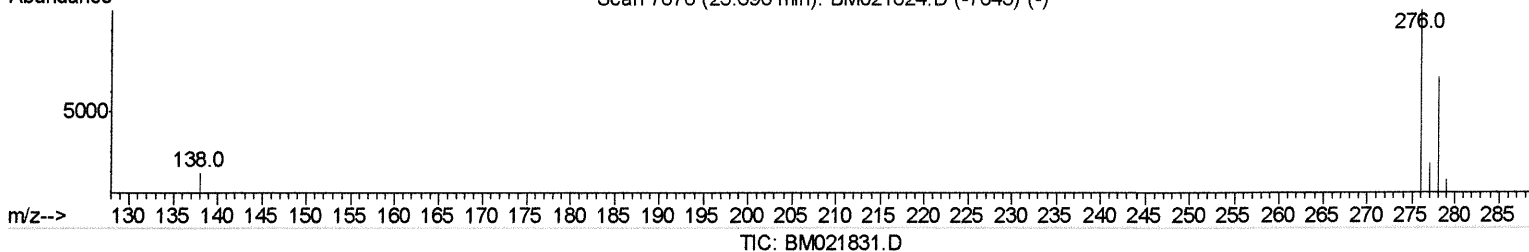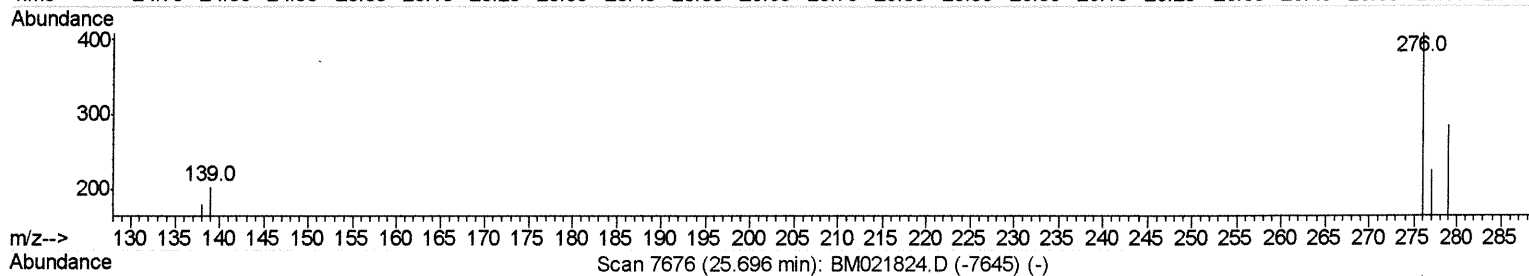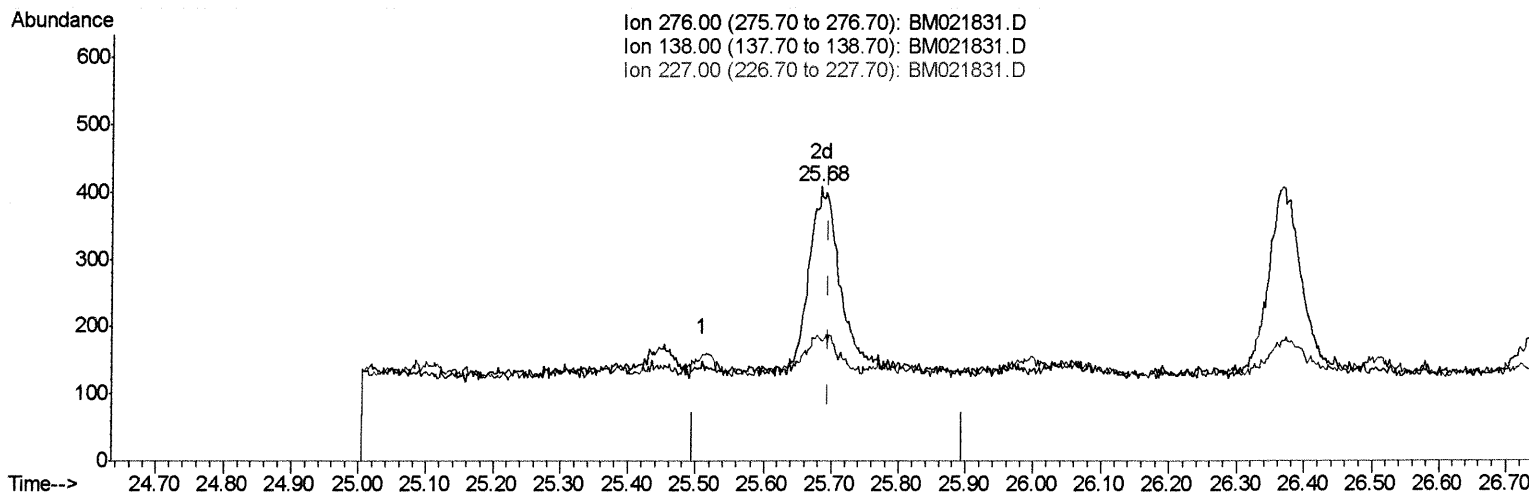

(24) Indeno(1,2,3-cd)pyrene

25.684min (-0.012) 0.03ng/ul m *50 08/05/19*

response 936

Ion	Exp%	Act%
276.00	100	100
138.00	18.90	7.16#
227.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080319\
 Data File : BM021831.D
 Acq On : 05 Aug 2019 03:32
 Operator : HP/JU
 Sample : K3863-13
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52F3

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:16:48 PM

Quant Time: Aug 05 09:01:54 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 08:19:16 2019
 Response via : Initial Calibration

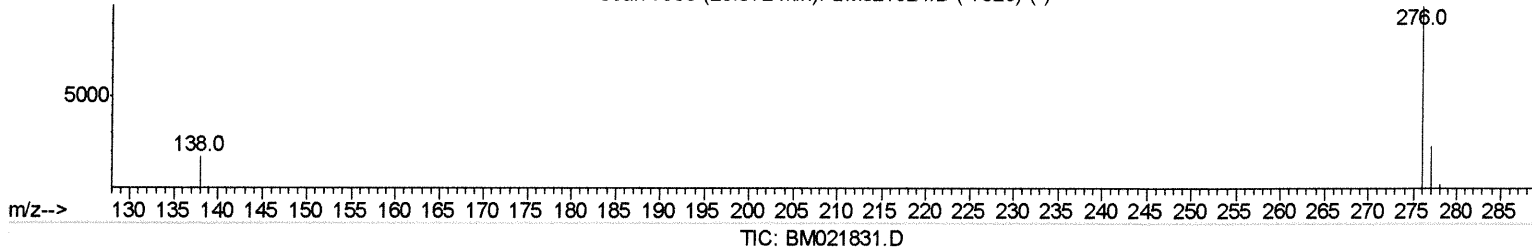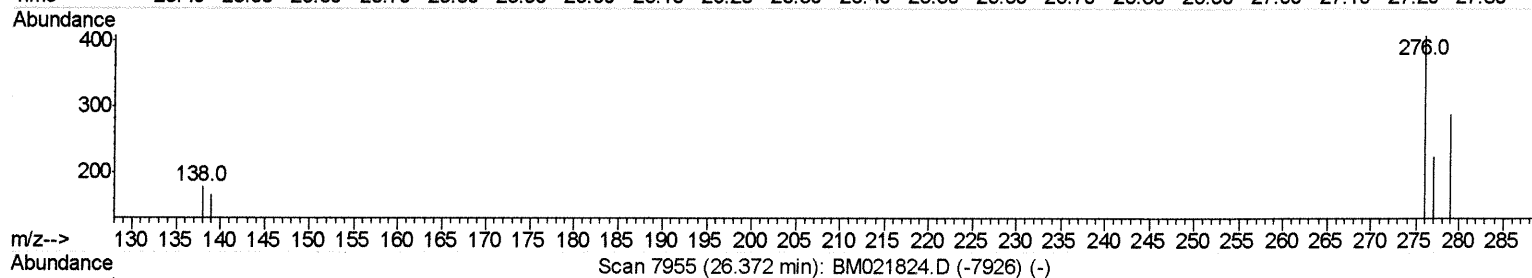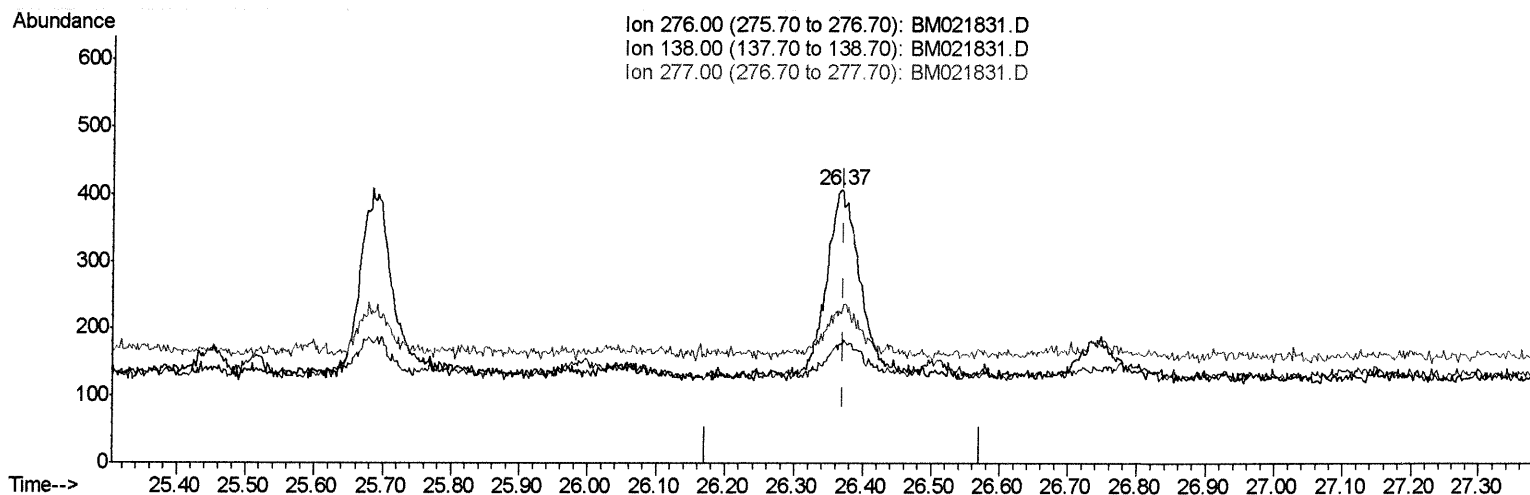

(26) Benzo(g,h,i)perylene

26.367min (-0.005) 0.03ng/ul

response 670

Ion	Exp%	Act%
276.00	100	100
138.00	19.40	43.73#
277.00	26.80	55.04#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080319\
Data File : BM021831.D
Acq On : 05 Aug 2019 03:32
Operator : HP/JU
Sample : K3863-13
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52F3

Manual Integrations
APPROVED

mohammad
8/5/2019 10:16:48 PM

Quant Time: Aug 05 09:01:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 08:19:16 2019
Response via : Initial Calibration

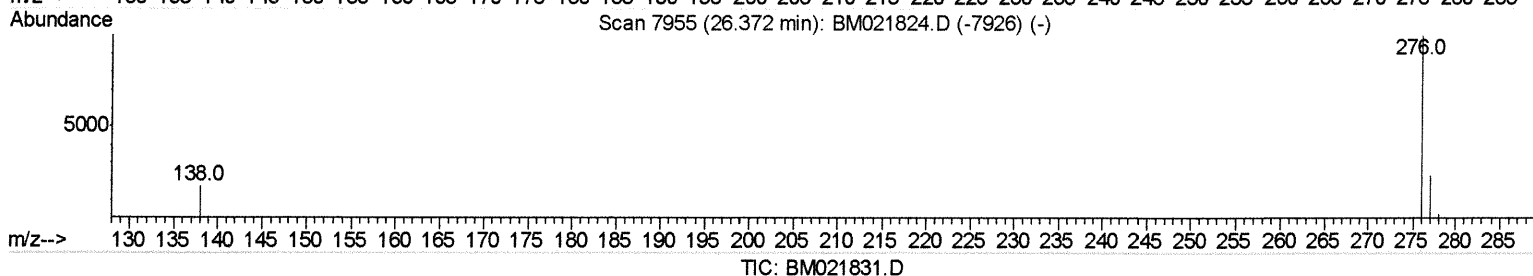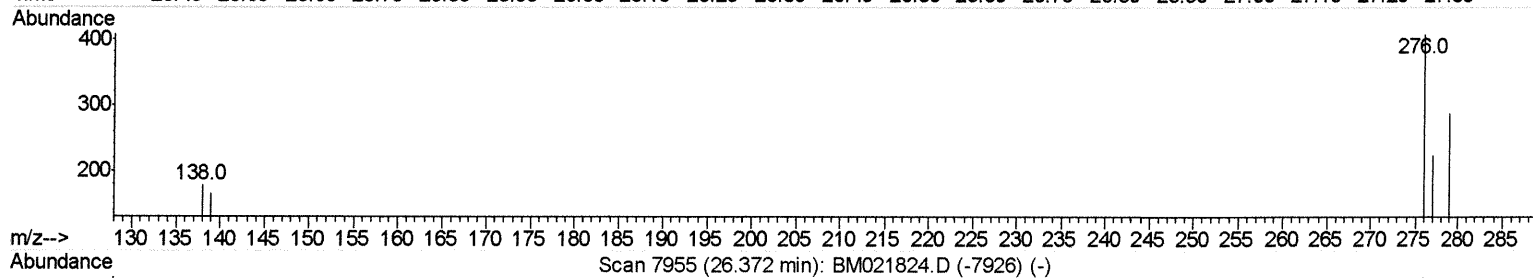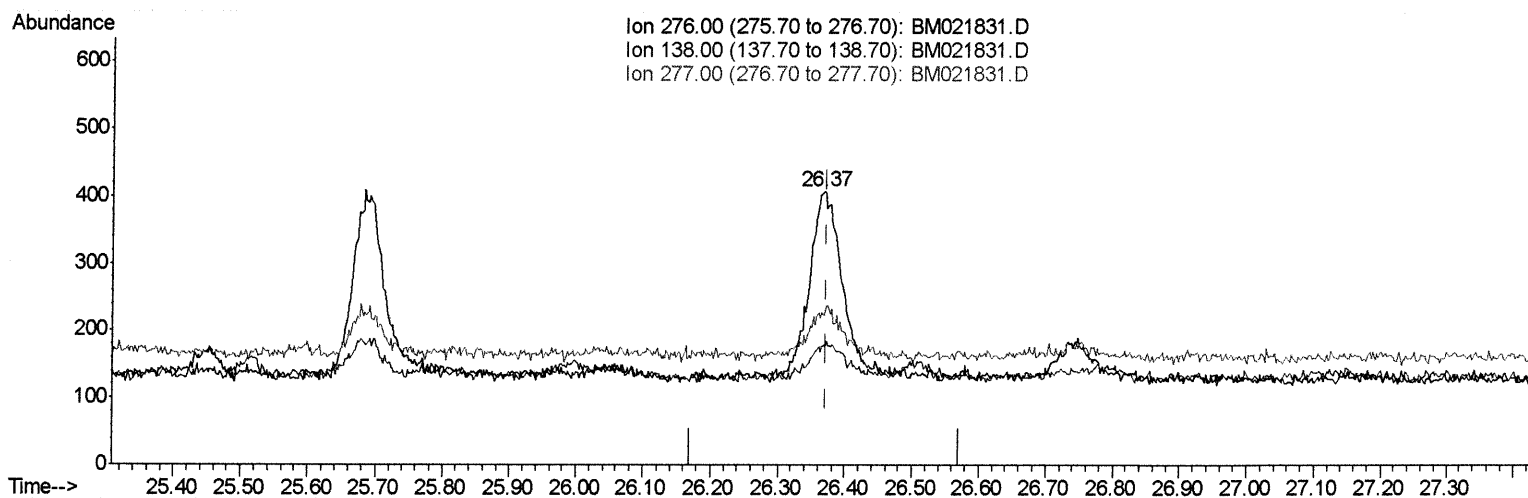

(26) Benzo(g,h,i)perylene

26.367min (-0.005) 0.04ng/ul m

JU 8/5/19

response 906

Ion	Exp%	Act%
276.00	100	100
138.00	19.40	43.73#
277.00	26.80	55.04#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080319\
 Data File : BM021831.D
 Acq On : 05 Aug 2019 03:32
 Operator : HP/JU
 Sample : K3863-13
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52F3

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:16:48 PM

Quant Time: Aug 05 09:03:28 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 08:19:16 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	1069	0.40	ng/ul	0.00
2) Naphthalene-d8	10.41	136	4435	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.29	164	2527	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	6023	0.40	ng/ul	-0.02
16) Chrysene-d12	21.24	240	5909	0.40	ng/ul	0.00
20) Perylene-d12	23.46	264	6877m	0.40	ng/ul	0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	727	0.10	ng/ul	0.00
14) Fluoranthene-d10	19.08	212	2327	0.11	ng/ul	-0.01
Target Compounds				Ovalue		
15) Fluoranthene	19.11	202	1445	0.062	ng/ul	80
17) Pyrene	19.47	202	1248m	0.051	ng/ul	56
18) Benzo(a)anthracene	21.23	228	750	0.035	ng/ul#	74
19) Chrysene	21.28	228	1030	0.038	ng/ul#	
21) Benzo(b)fluoranthene	22.79	252	1624m	0.070	ng/ul	
22) Benzo(k)fluoranthene	22.83	252	799m	0.030	ng/ul	
23) Benzo(a)pyrene	23.35	252	1035m	0.044	ng/ul	
24) Indeno(1,2,3-cd)pyrene	25.68	276	936m	0.033	ng/ul	
26) Benzo(g,h,i)perylene	26.37	276	906m	0.036	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed