


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Data File : BM021846.D
Acq On : 05 Aug 2019 17:27
Operator : HP/JU
Sample : K3850-19DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleID :
BENS5DL

Manual Integrations
APPROVED

mohammad
8/5/2019 10:17:31 PM

Quant Time: Aug 05 18:08:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 17:14:32 2019
Response via : Initial Calibration

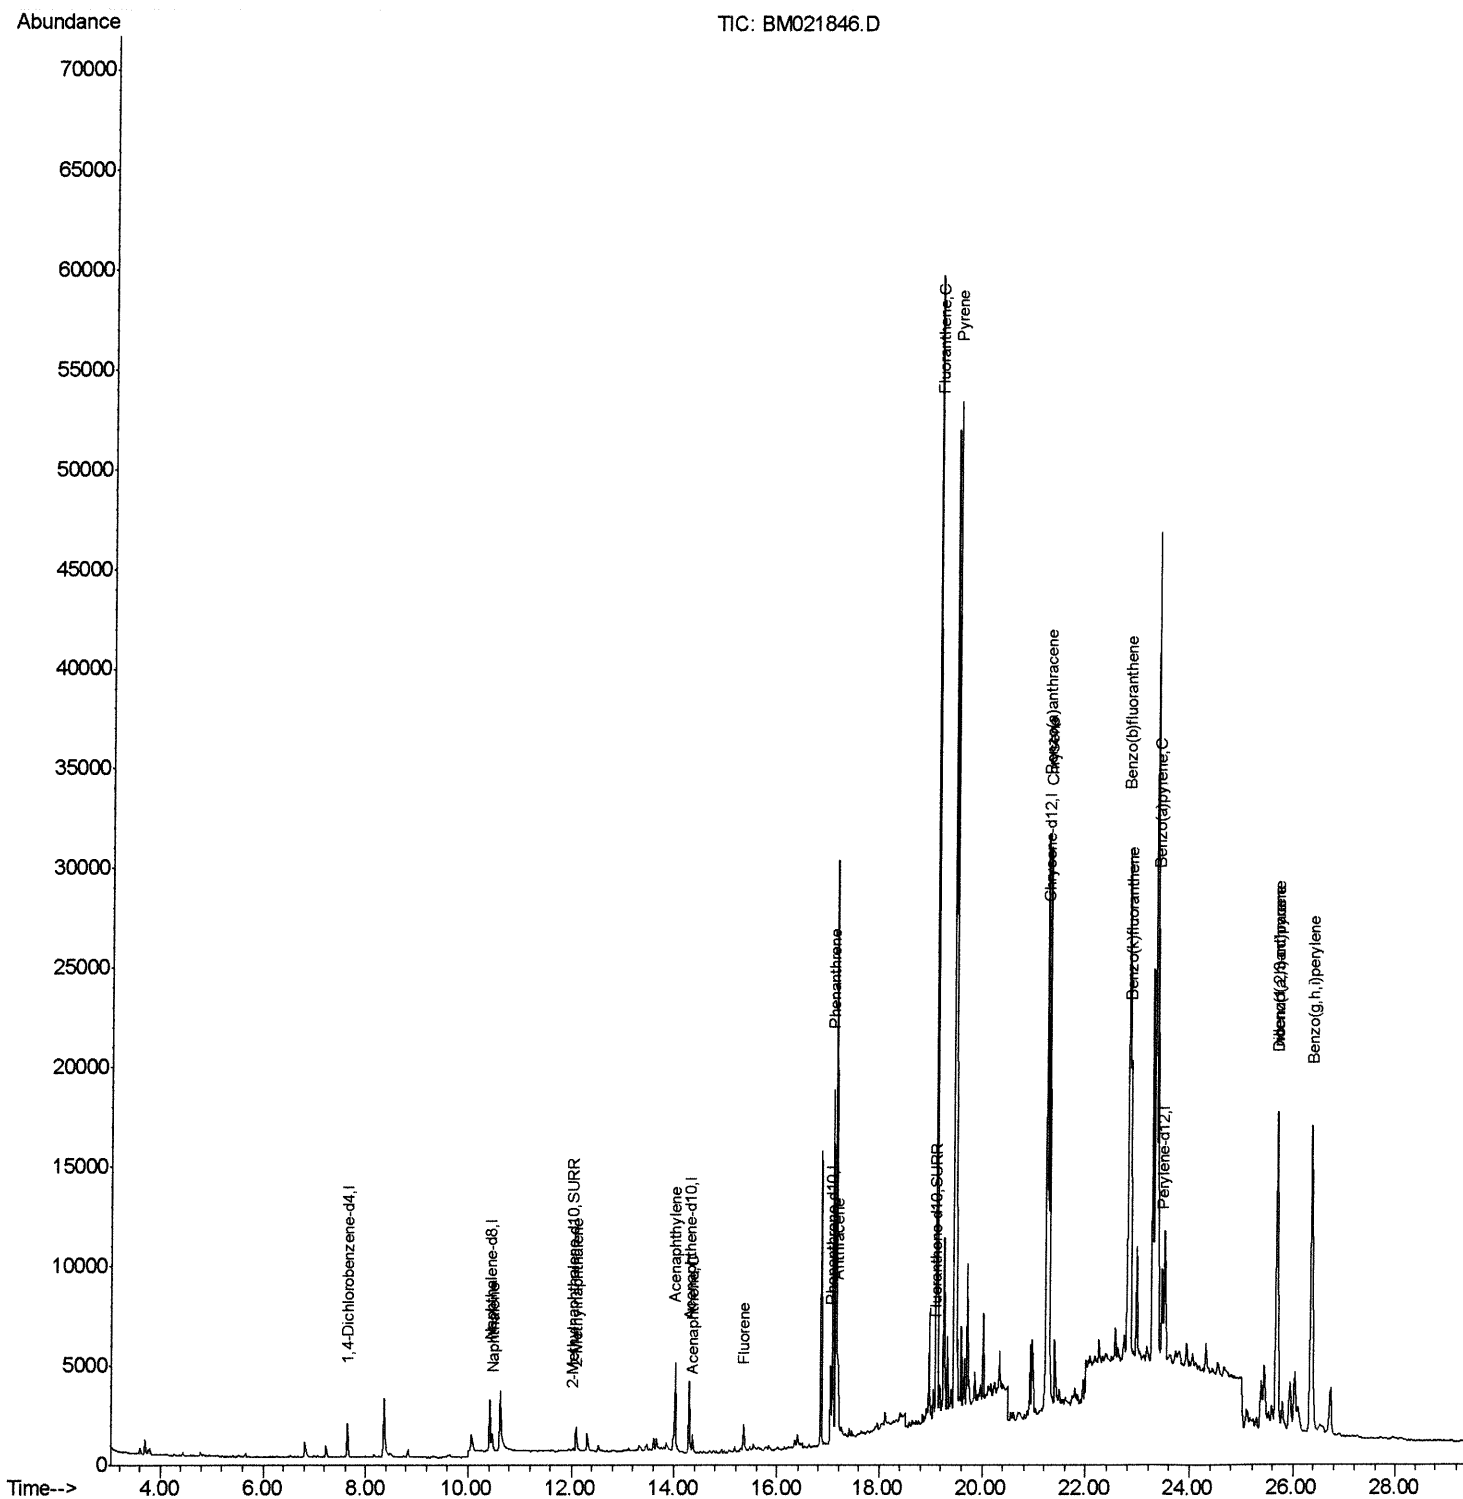

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
 Data File : BM021846.D
 Acq On : 05 Aug 2019 17:27
 Operator : HP/JU
 Sample : K3850-19DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENS5DL

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:17:31 PM

Quant Time: Aug 05 18:03:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 17:14:32 2019
 Response via : Initial Calibration

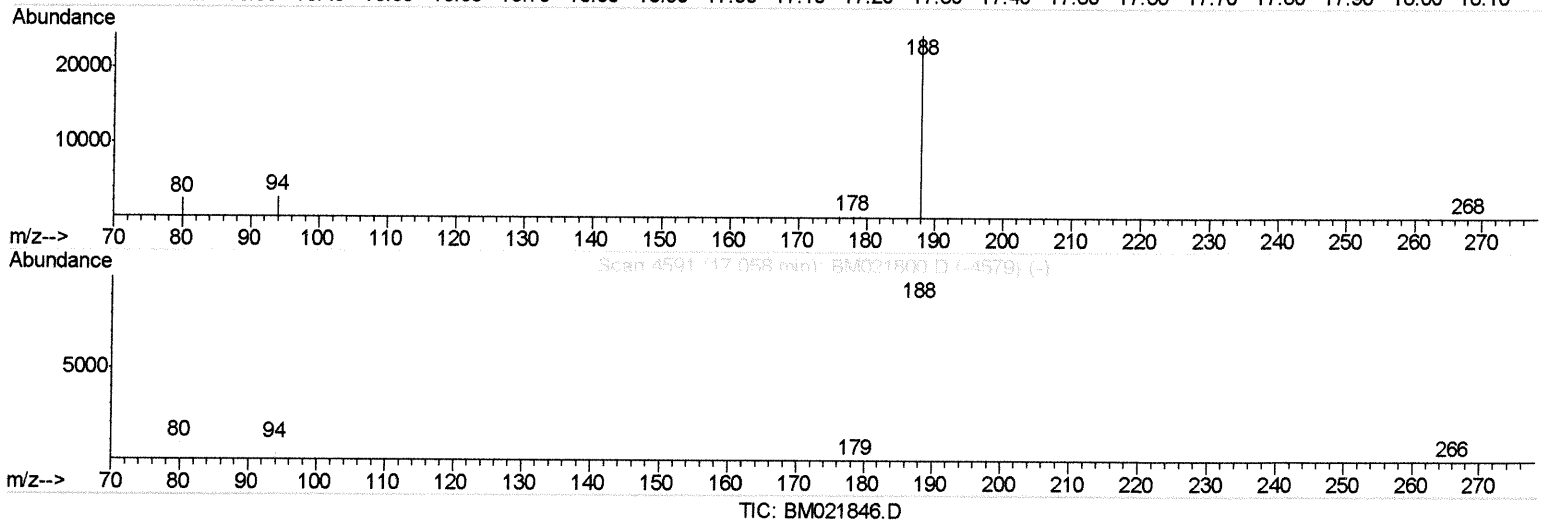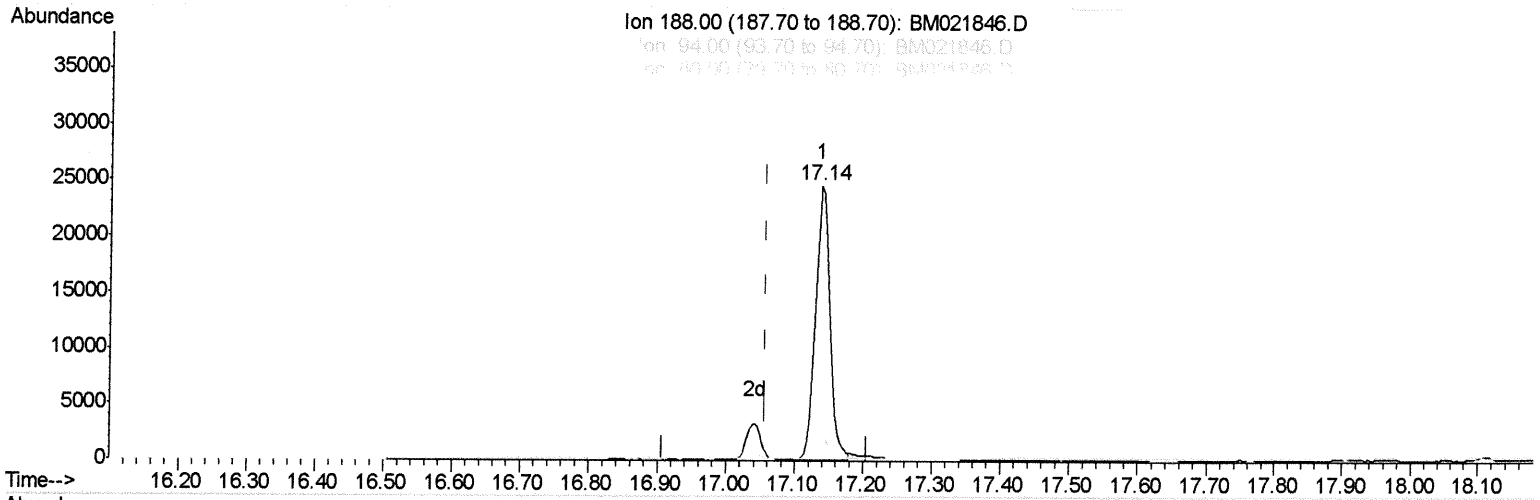

(10) Phenanthrene-d10 (I)
 17.138min (+0.080) 0.40ng/ul
 response 36509

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	10.46
80.00	11.40	9.67
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
 Data File : BM021846.D
 Acq On : 05 Aug 2019 17:27
 Operator : HP/JU
 Sample : K3850-19DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENS5DL

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:17:31 PM

Quant Time: Aug 05 18:03:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 17:14:32 2019
 Response via : Initial Calibration

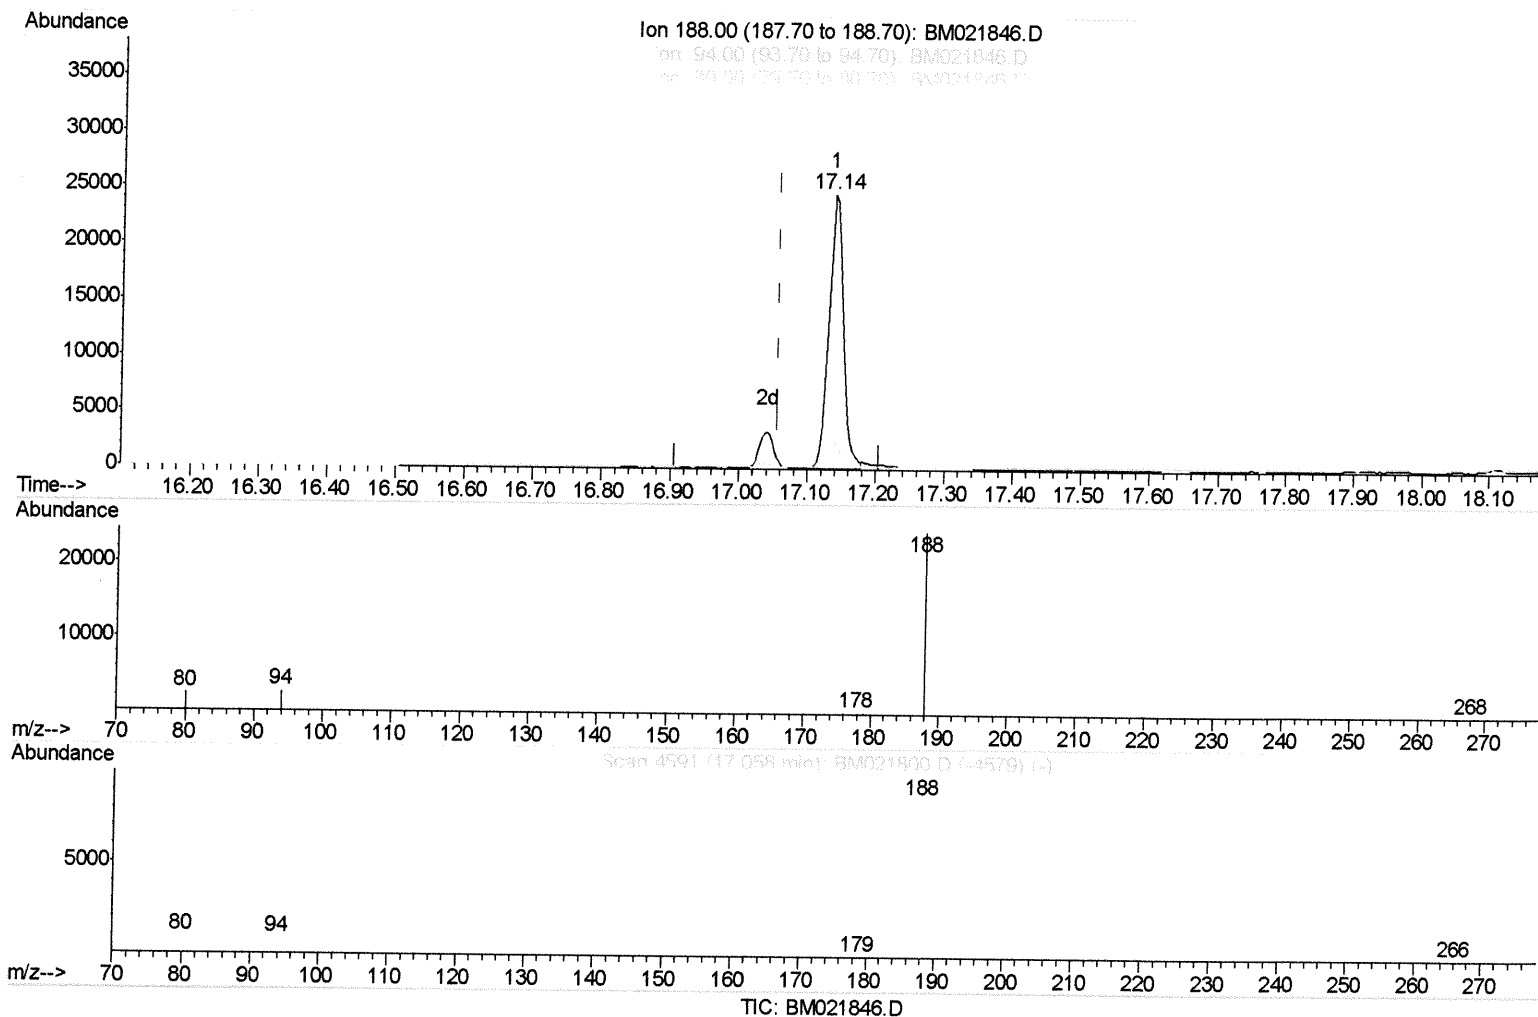

(10) Phenanthrene-d10 (I)

17.138min (+0.080) 0.40ng/ul

response 36509

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	10.46
80.00	11.40	9.67
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
 Data File : BM021846.D
 Acq On : 05 Aug 2019 17:27
 Operator : HP/JU
 Sample : K3850-19DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENS5DL

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:17:31 PM

Quant Time: Aug 05 18:03:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 17:14:32 2019
 Response via : Initial Calibration

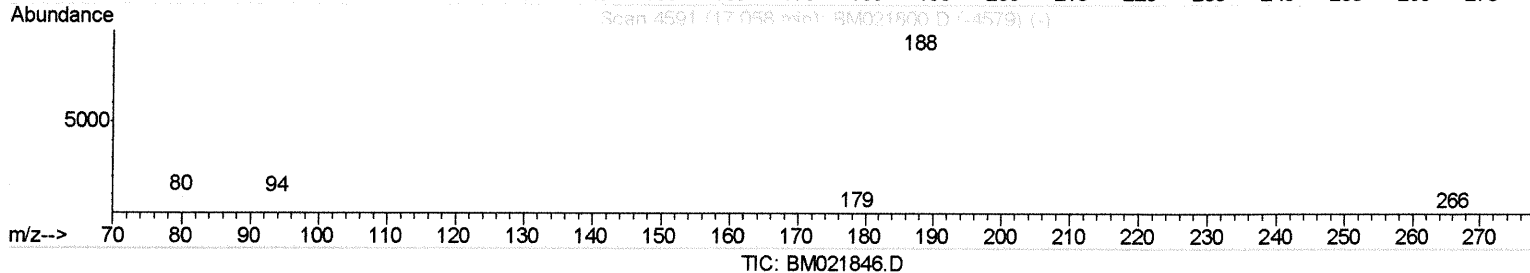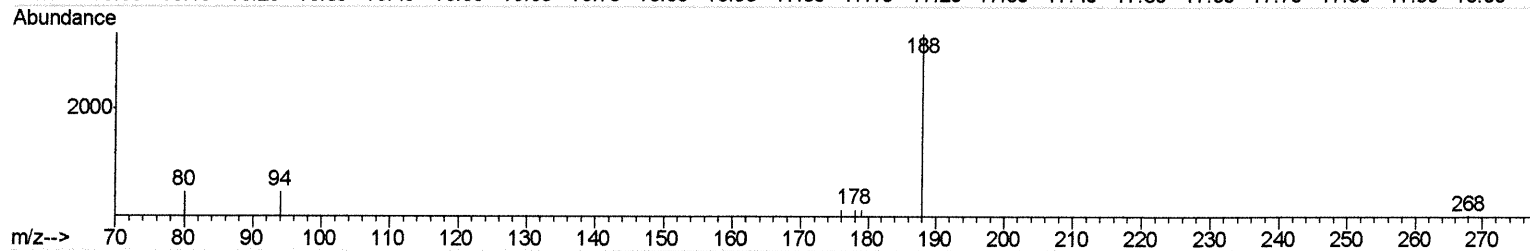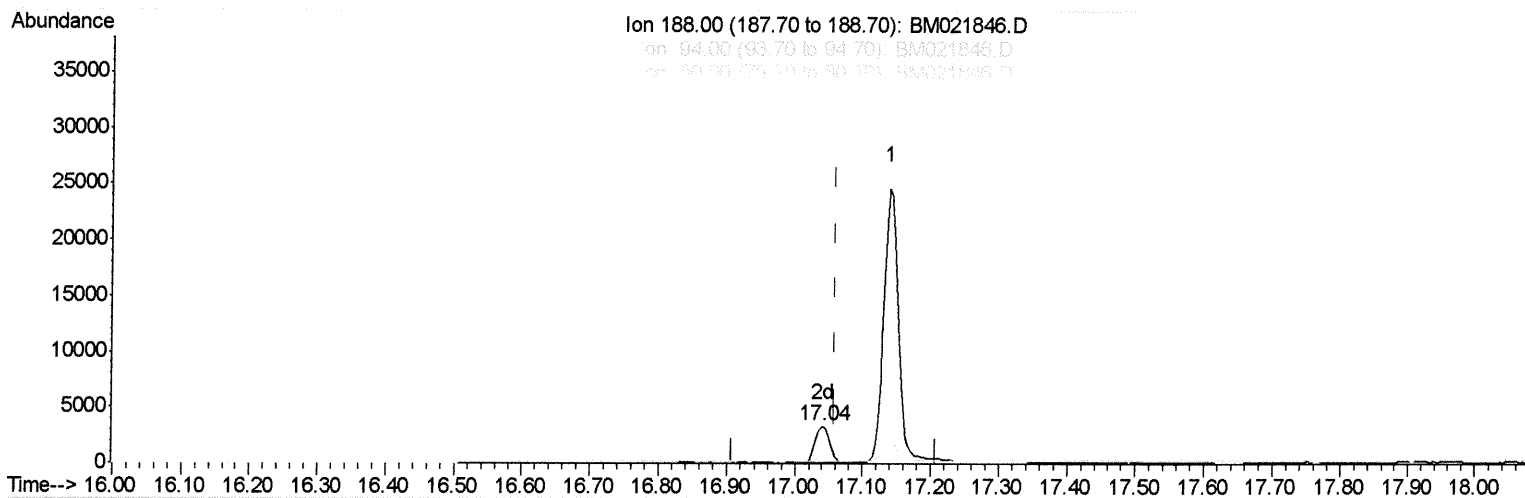

(10) Phenanthrene-d10 (I)

17.041min (-0.017) 0.40ng/ul m *Ju* *17.041*

response 4878

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	14.39#
80.00	11.40	14.45#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
 Data File : BM021846.D
 Acq On : 05 Aug 2019 17:27
 Operator : HP/JU
 Sample : K3850-19DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENS5DL

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:17:31 PM

Quant Time: Aug 05 18:04:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 17:14:32 2019
 Response via : Initial Calibration

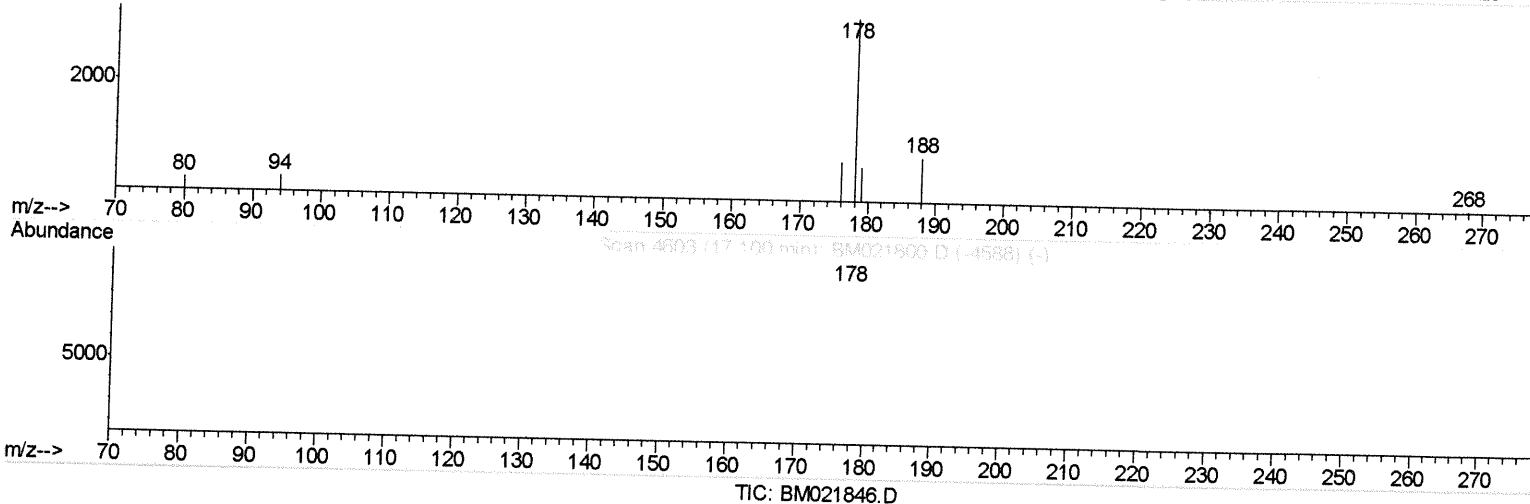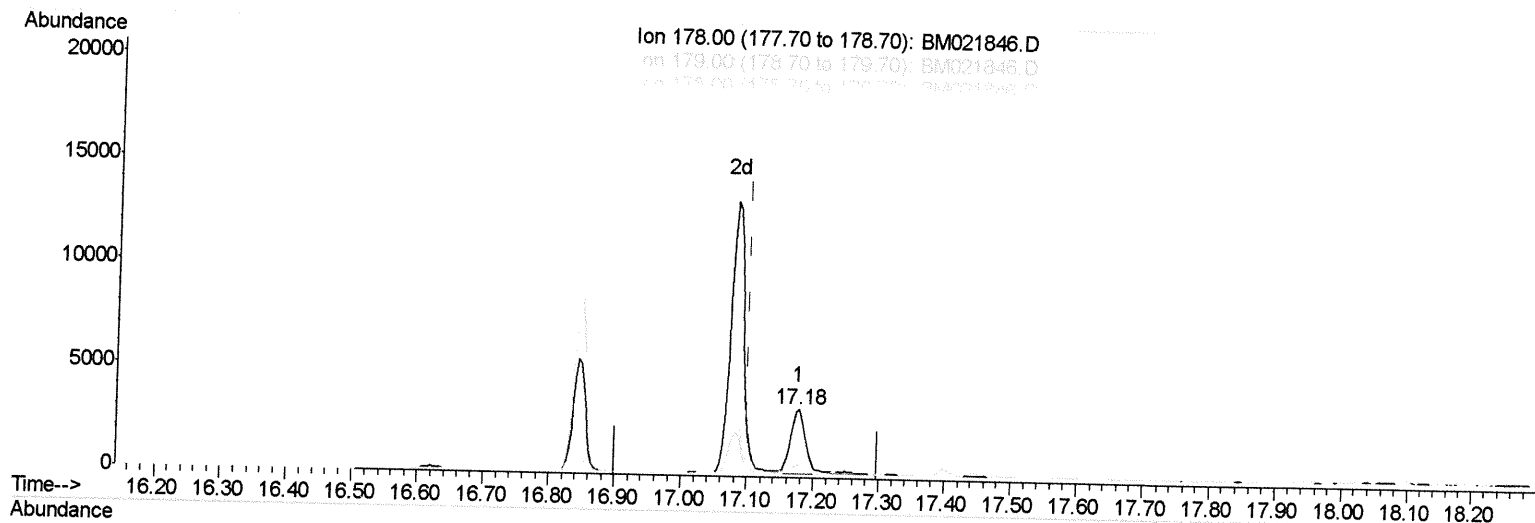

(12) Phenanthrene

17.176min (+0.076) 0.37ng/ul

response 5291

Ion	Exp%	Act%
178.00	100	100
179.00	17.70	19.93
176.00	21.00	22.79
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
 Data File : BM021846.D
 Acq On : 05 Aug 2019 17:27
 Operator : HP/JU
 Sample : K3850-19DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENS5DL

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:17:31 PM

Quant Time: Aug 05 18:04:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 17:14:32 2019
 Response via : Initial Calibration

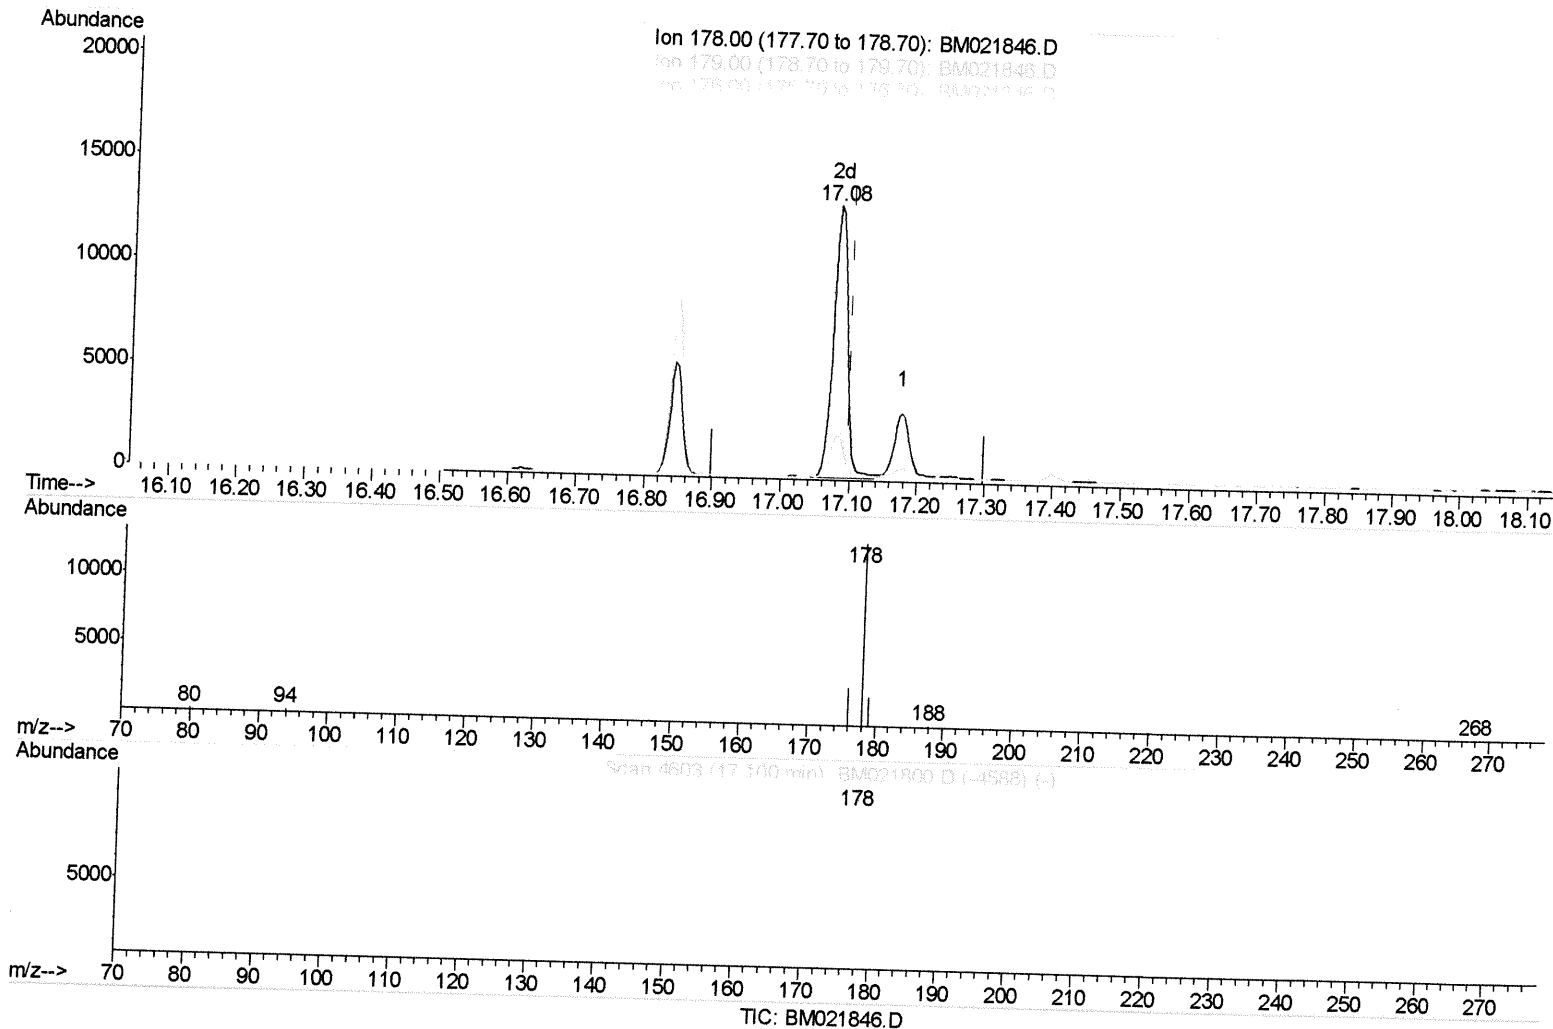

(12) Phenanthrene

17.079min (-0.021) 1.34ng/ul m

Ju
 08/05/19

response 18954

Ion	Exp%	Act%
178.00	100	100
179.00	17.70	16.21
176.00	21.00	20.69
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Data File : BM021846.D
Acq On : 05 Aug 2019 17:27
Operator : HP/JU
Sample : K3850-19DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENS5DL

Manual Integrations
APPROVED

mohammad
8/5/2019 10:17:31 PM

Quant Time: Aug 05 18:04:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 17:14:32 2019
Response via : Initial Calibration

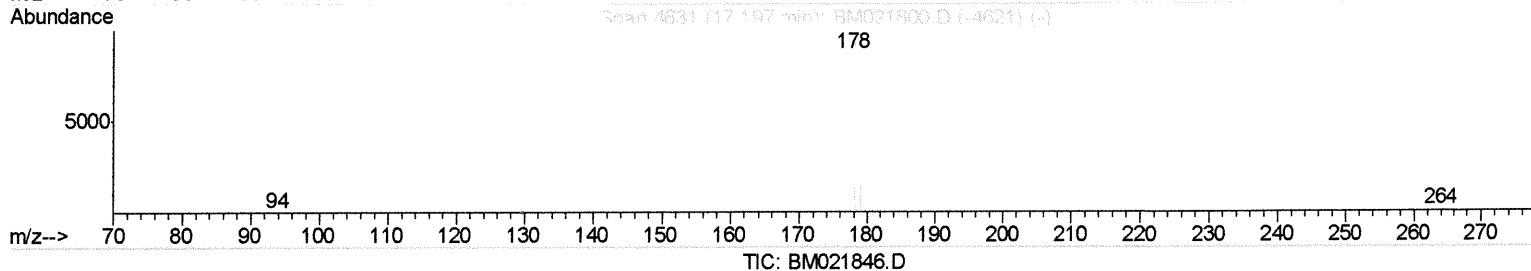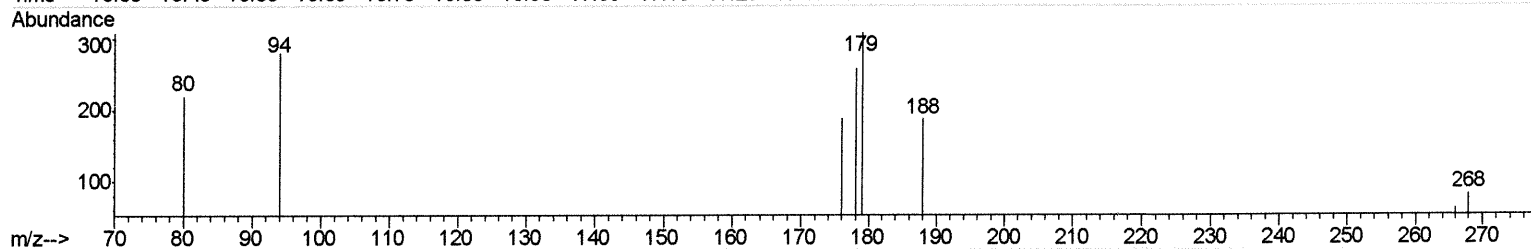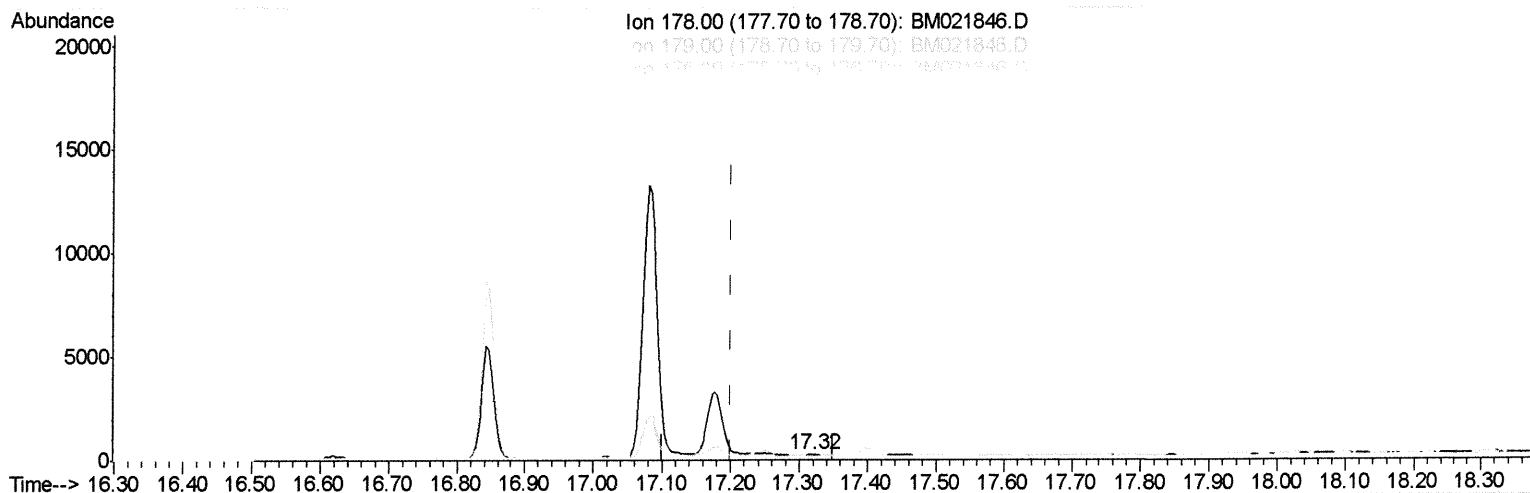

(13) Anthracene

17.319min (+0.118) 0.01ng/ul

response 88

Ion	Exp%	Act%
178.00	100	100
179.00	19.40	119.38#
176.00	20.80	72.48#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
 Data File : BM021846.D
 Acq On : 05 Aug 2019 17:27
 Operator : HP/JU
 Sample : K3850-19DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENS5DL

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:17:31 PM

Quant Time: Aug 05 18:04:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 17:14:32 2019
 Response via : Initial Calibration

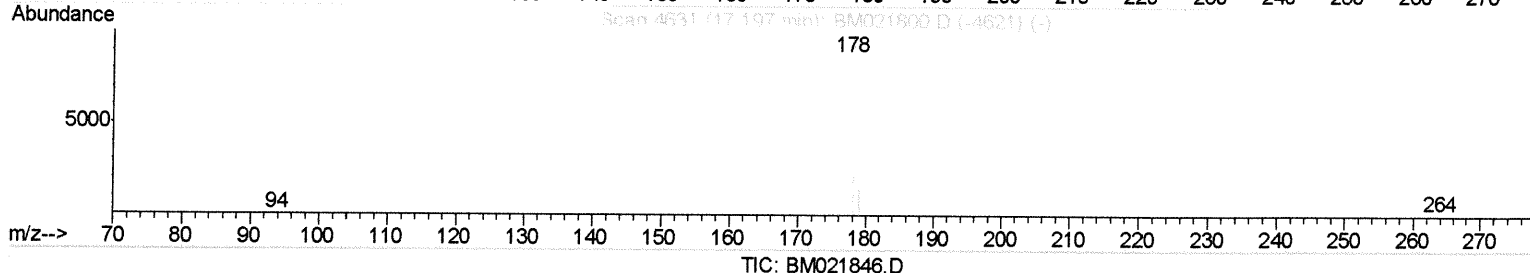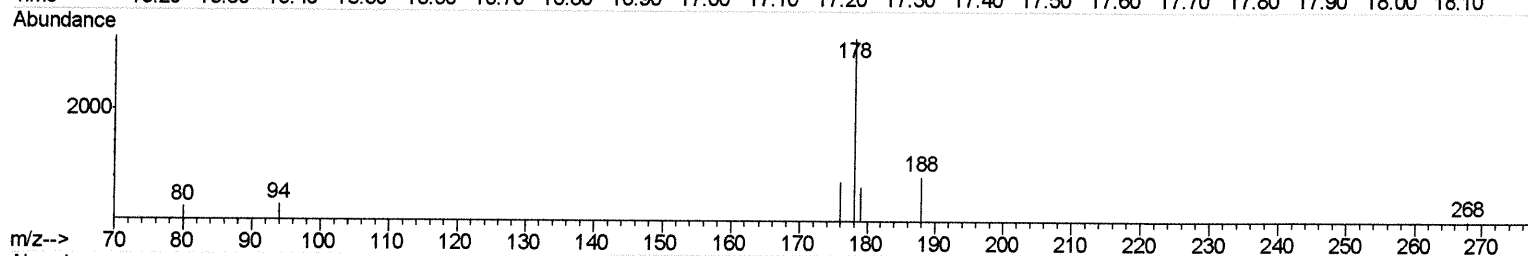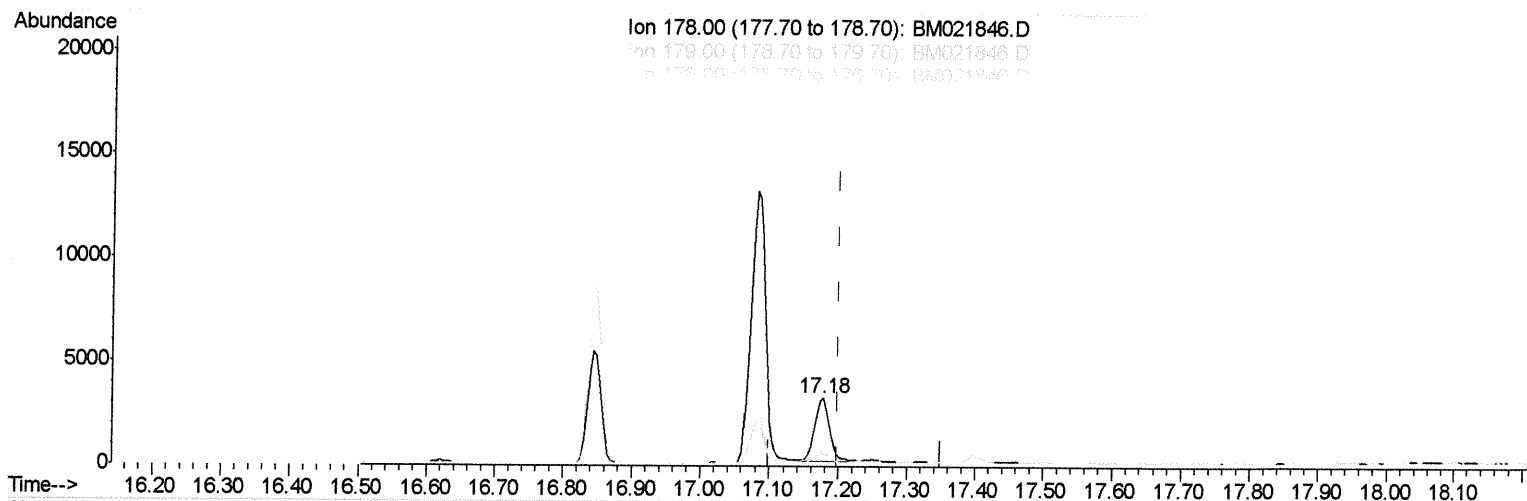

TIC: BM021846.D

(13) Anthracene

17.176min (-0.024) 0.40ng/ul m *50 38/05/19*

response 4833

Ion	Exp%	Act%
178.00	100	100
179.00	19.40	19.93
176.00	20.80	22.79
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
 Data File : BM021846.D
 Acq On : 05 Aug 2019 17:27
 Operator : HP/JU
 Sample : K3850-19DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 BENS5DL

Manual Integrations
APPROVED

mohammad
 8/5/2019 10:17:31 PM

Quant Time: Aug 05 18:04:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 17:14:32 2019
 Response via : Initial Calibration

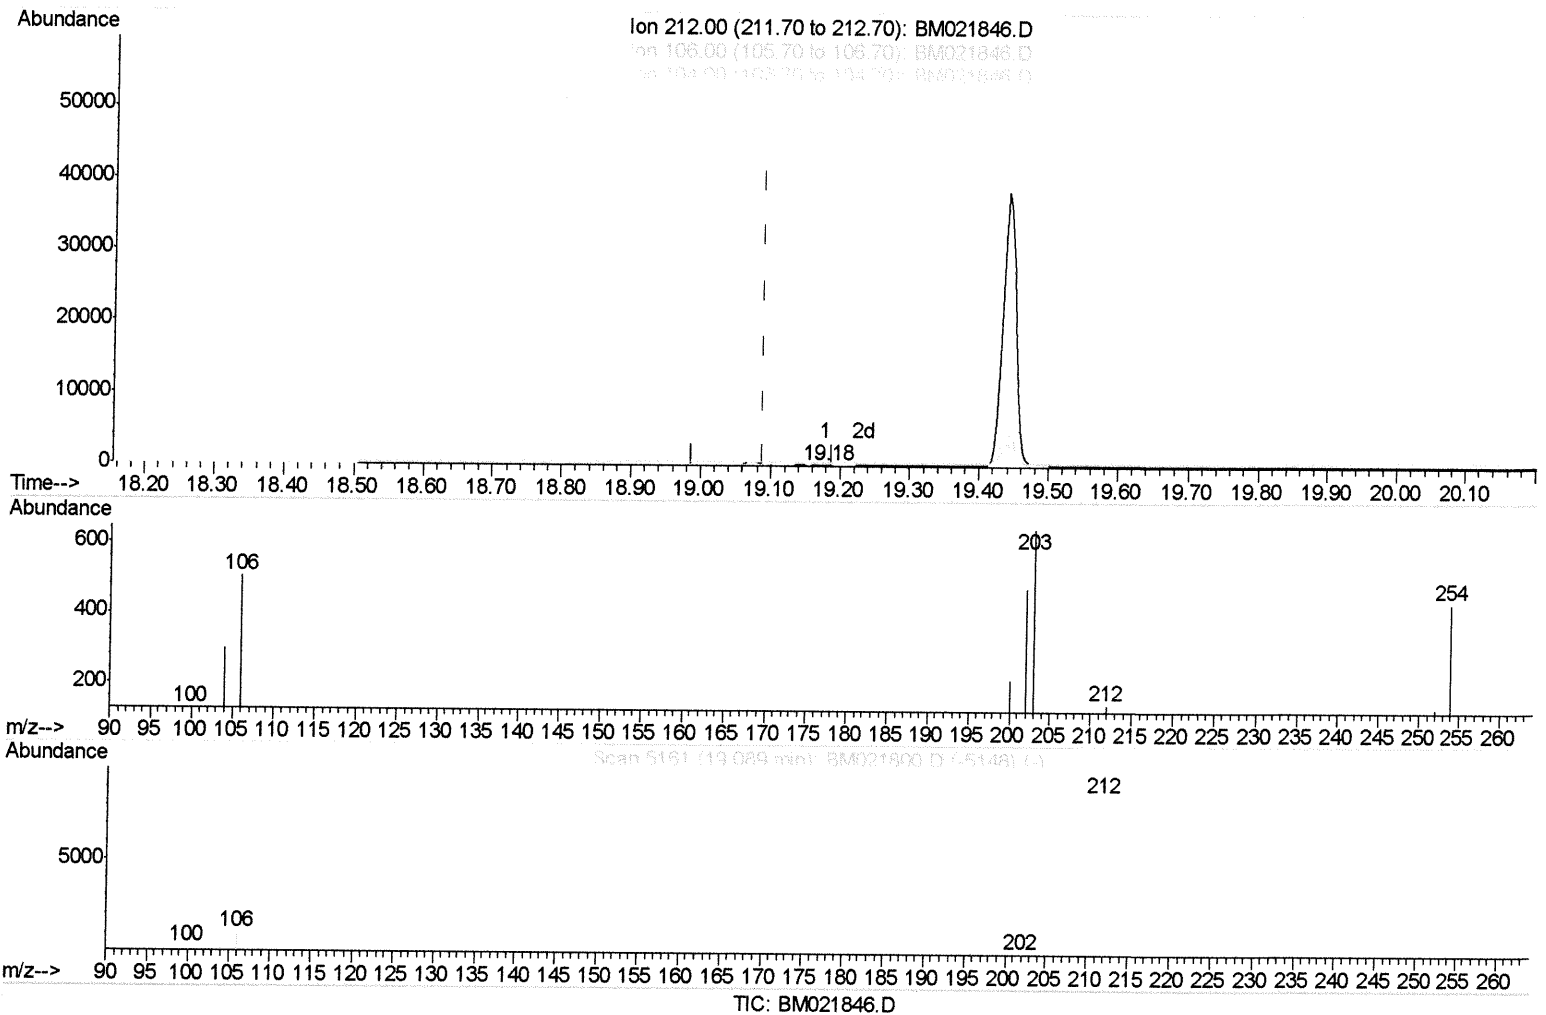

(14) Fluoranthene-d10 (SURR)

19.180min (+0.092) 0.00ng/ul

response 31

Ion	Exp%	Act%
212.00	100	100
106.00	9.90	125.81#
104.00	6.00	409.68#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
 Data File : BM021846.D
 Acq On : 05 Aug 2019 17:27
 Operator : HP/JU
 Sample : K3850-19DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENS5DL

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:17:31 PM

Quant Time: Aug 05 18:04:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 17:14:32 2019
 Response via : Initial Calibration

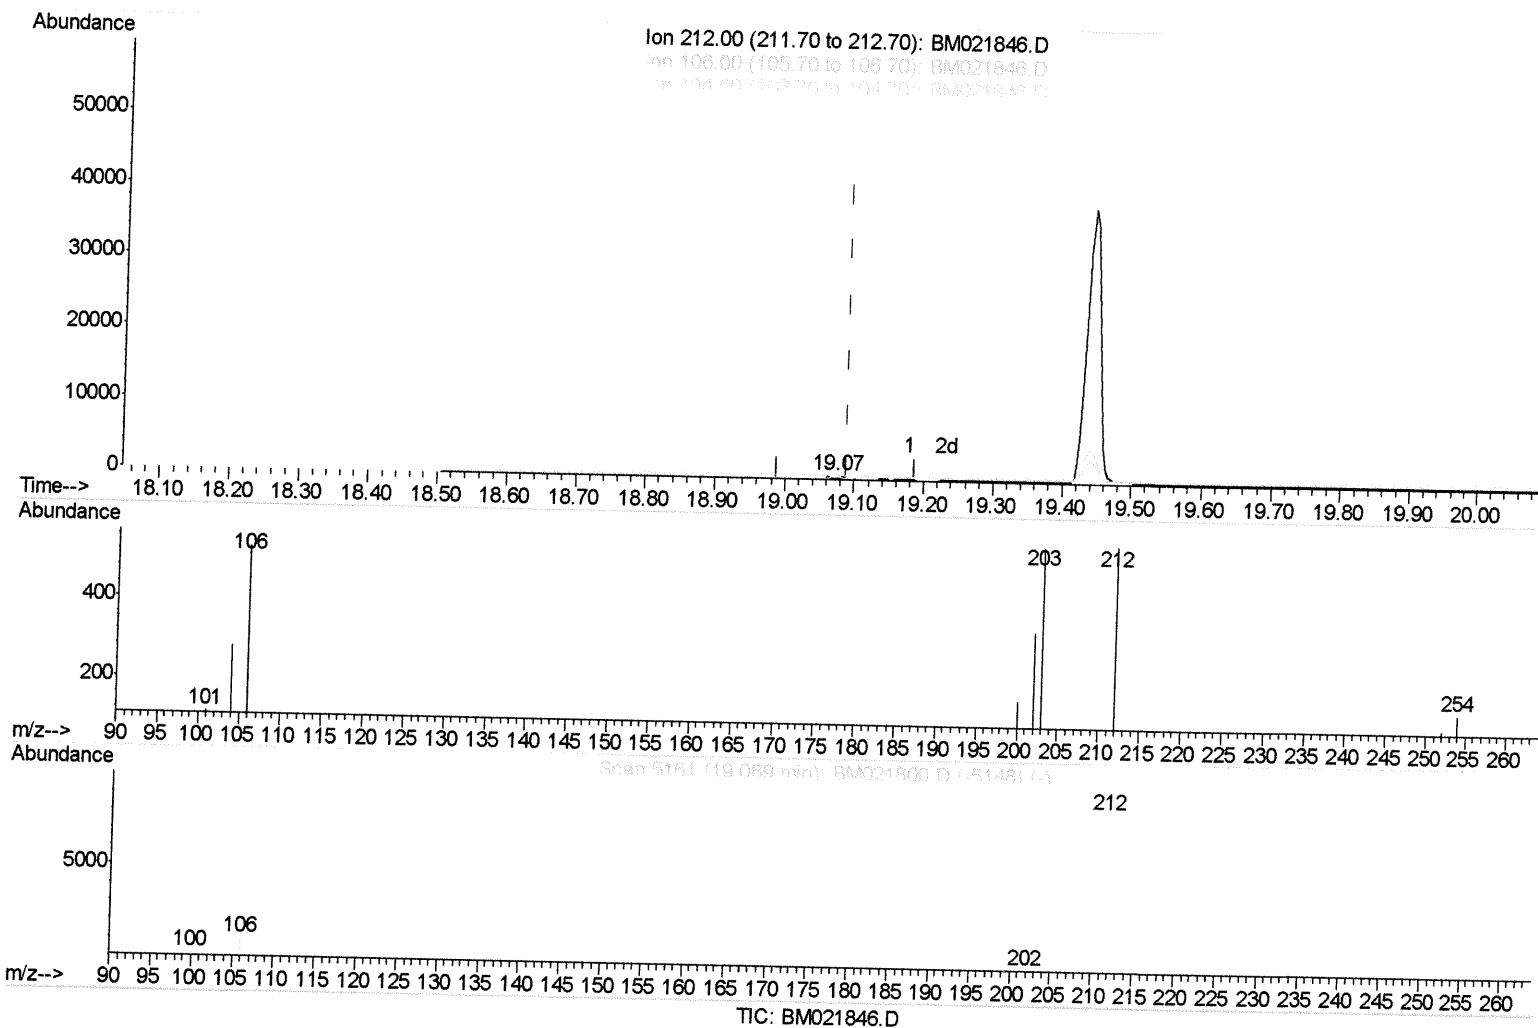

(14) Fluoranthene-d10 (SURR)

19.073min (-0.015) 0.04ng/ul m

50805119

response 576

Ion	Exp%	Act%
212.00	100	100
106.00	9.90	6.77#
104.00	6.00	22.05#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
 Data File : BM021846.D
 Acq On : 05 Aug 2019 17:27
 Operator : HP/JU
 Sample : K3850-19DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENS5DL

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:17:31 PM

Quant Time: Aug 05 18:04:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 17:14:32 2019
 Response via : Initial Calibration

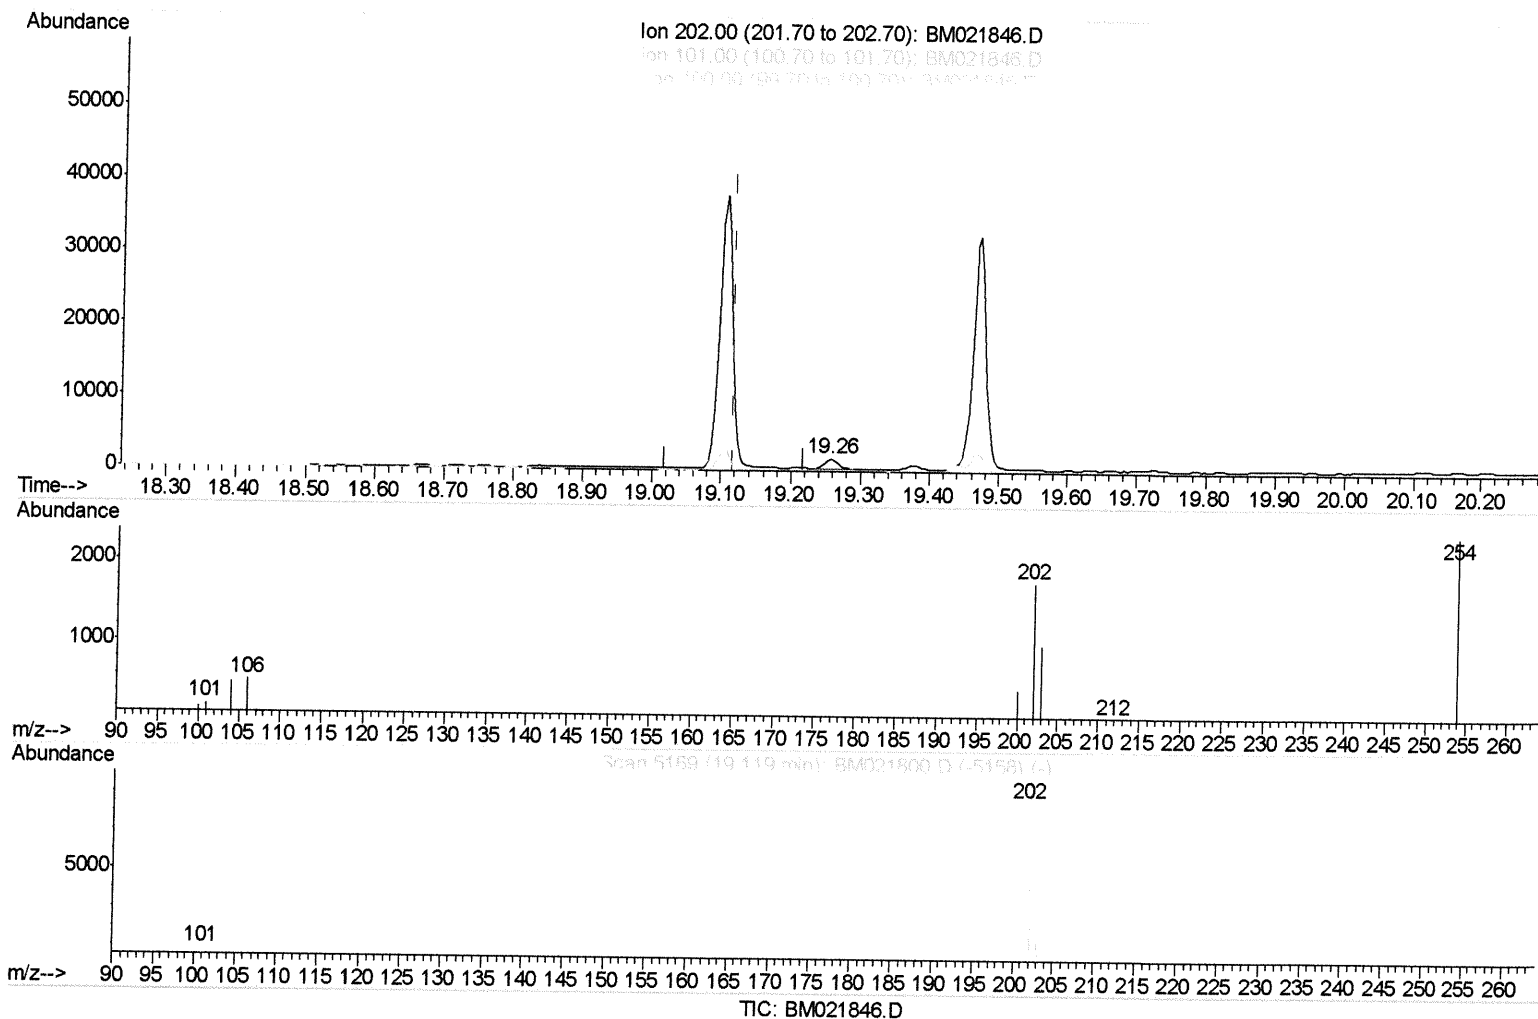

(15) Fluoranthene (C)

19.257min (+0.137) 0.09ng/ul

response 1739

Ion	Exp%	Act%
202.00	100	100
101.00	10.20	13.05
100.00	8.10	11.02
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
 Data File : BM021846.D
 Acq On : 05 Aug 2019 17:27
 Operator : HP/JU
 Sample : K3850-19DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENS5DL

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:17:31 PM

Quant Time: Aug 05 18:04:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 17:14:32 2019
 Response via : Initial Calibration

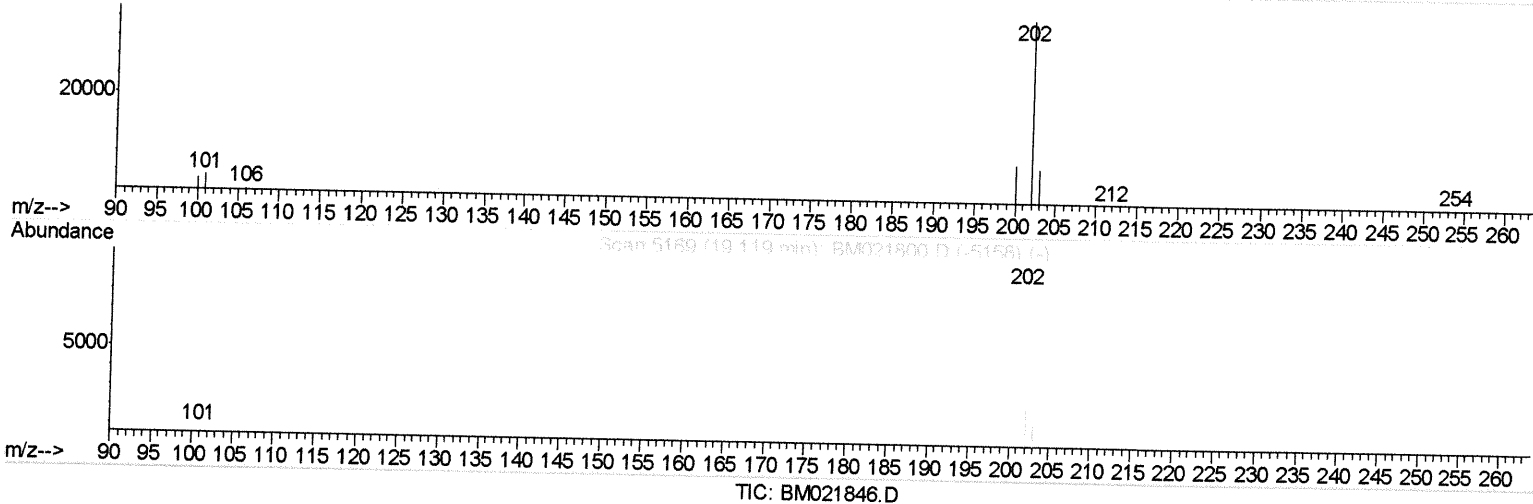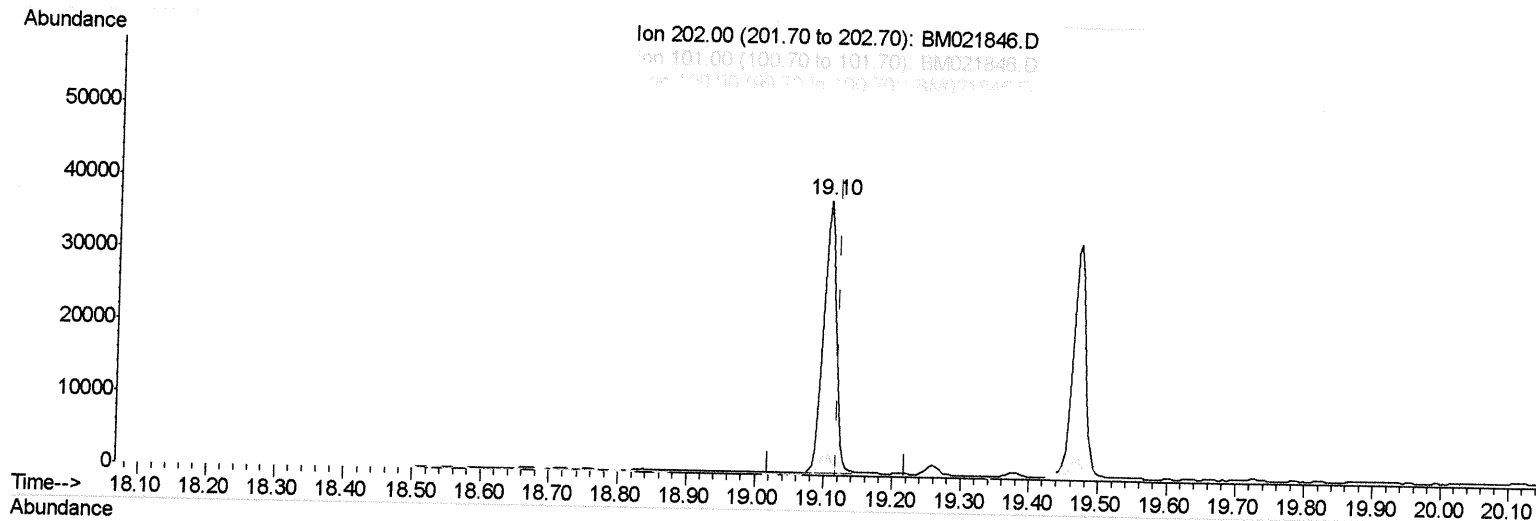

(15) Fluoranthene (C)

19.104min (-0.015) 2.54ng/ul m

508/05/19

response 48345

Ion	Exp%	Act%
202.00	100	100
101.00	10.20	8.42
100.00	8.10	6.53
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Data File : BM021846.D
Acq On : 05 Aug 2019 17:27
Operator : HP/JU
Sample : K3850-19DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENS5DL

Manual Integrations
APPROVED

mohammad
8/5/2019 10:17:31 PM

Quant Time: Aug 05 18:04:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 17:14:32 2019
Response via : Initial Calibration

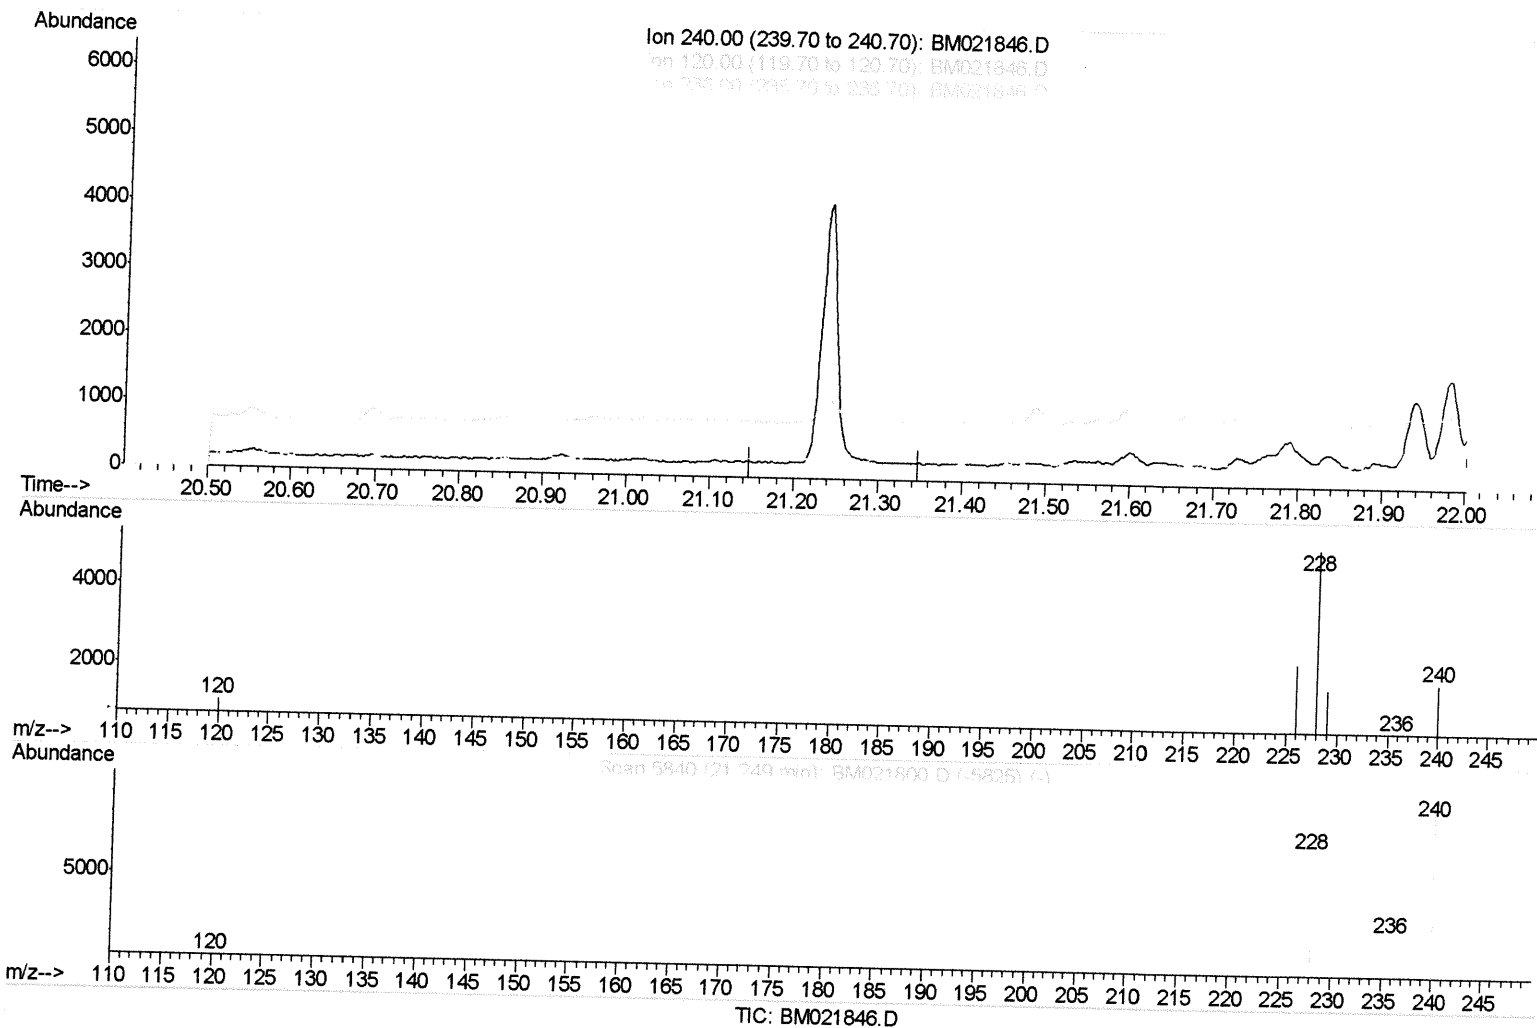

(16) Chrysene-d12 (I)

21.249min (-21.249) 0.00ng/ui

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.20	0.00#
236.00	32.30	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Data File : BM021846.D
Acq On : 05 Aug 2019 17:27
Operator : HP/JU
Sample : K3850-19DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENS5DL

Manual Integrations
APPROVED

mohammad
8/5/2019 10:17:31 PM

Quant Time: Aug 05 18:04:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 17:14:32 2019
Response via : Initial Calibration

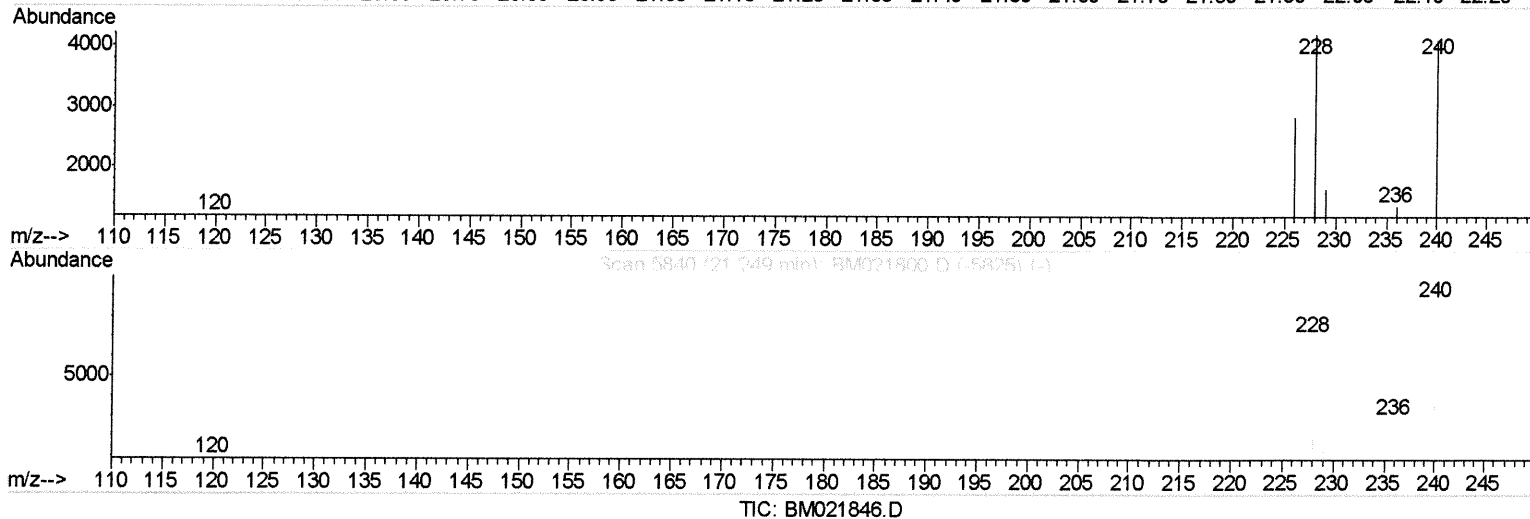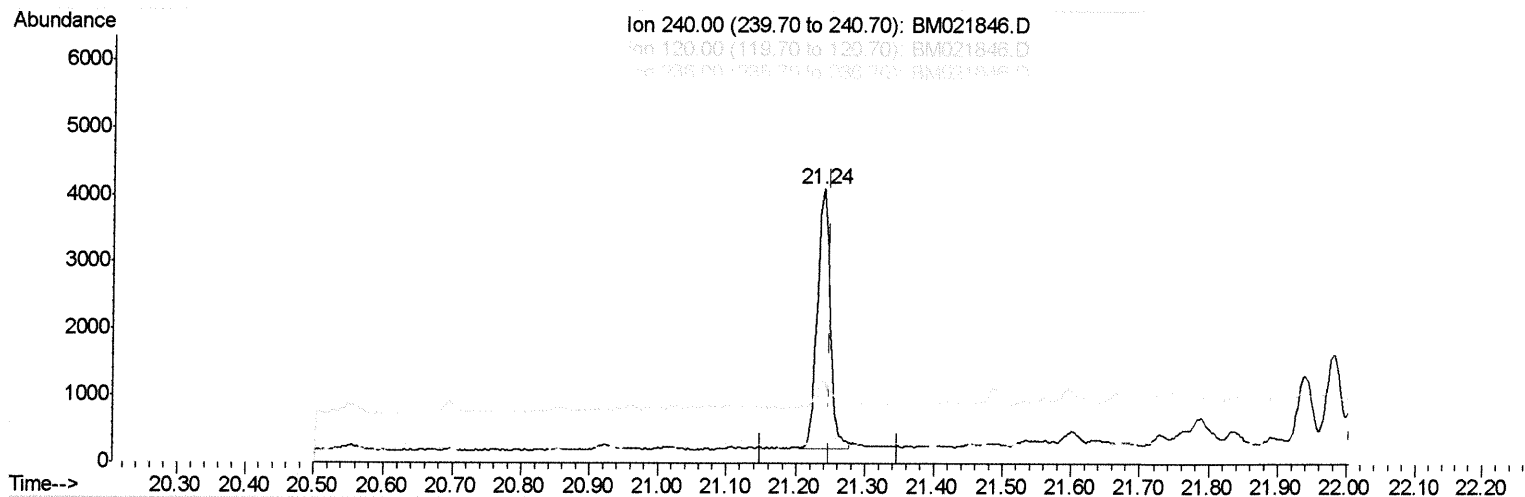

(16) Chrysene-d12 (I)

21.239min (-0.010) 0.40ng/ul m

50 08/05/19

response 5066

Ion	Exp%	Act%
240.00	100	100
120.00	16.20	29.37#
236.00	32.30	33.29
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
 Data File : BM021846.D
 Acq On : 05 Aug 2019 17:27
 Operator : HP/JU
 Sample : K3850-19DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENS5DL

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:17:31 PM

Quant Time: Aug 05 18:04:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 17:14:32 2019
 Response via : Initial Calibration

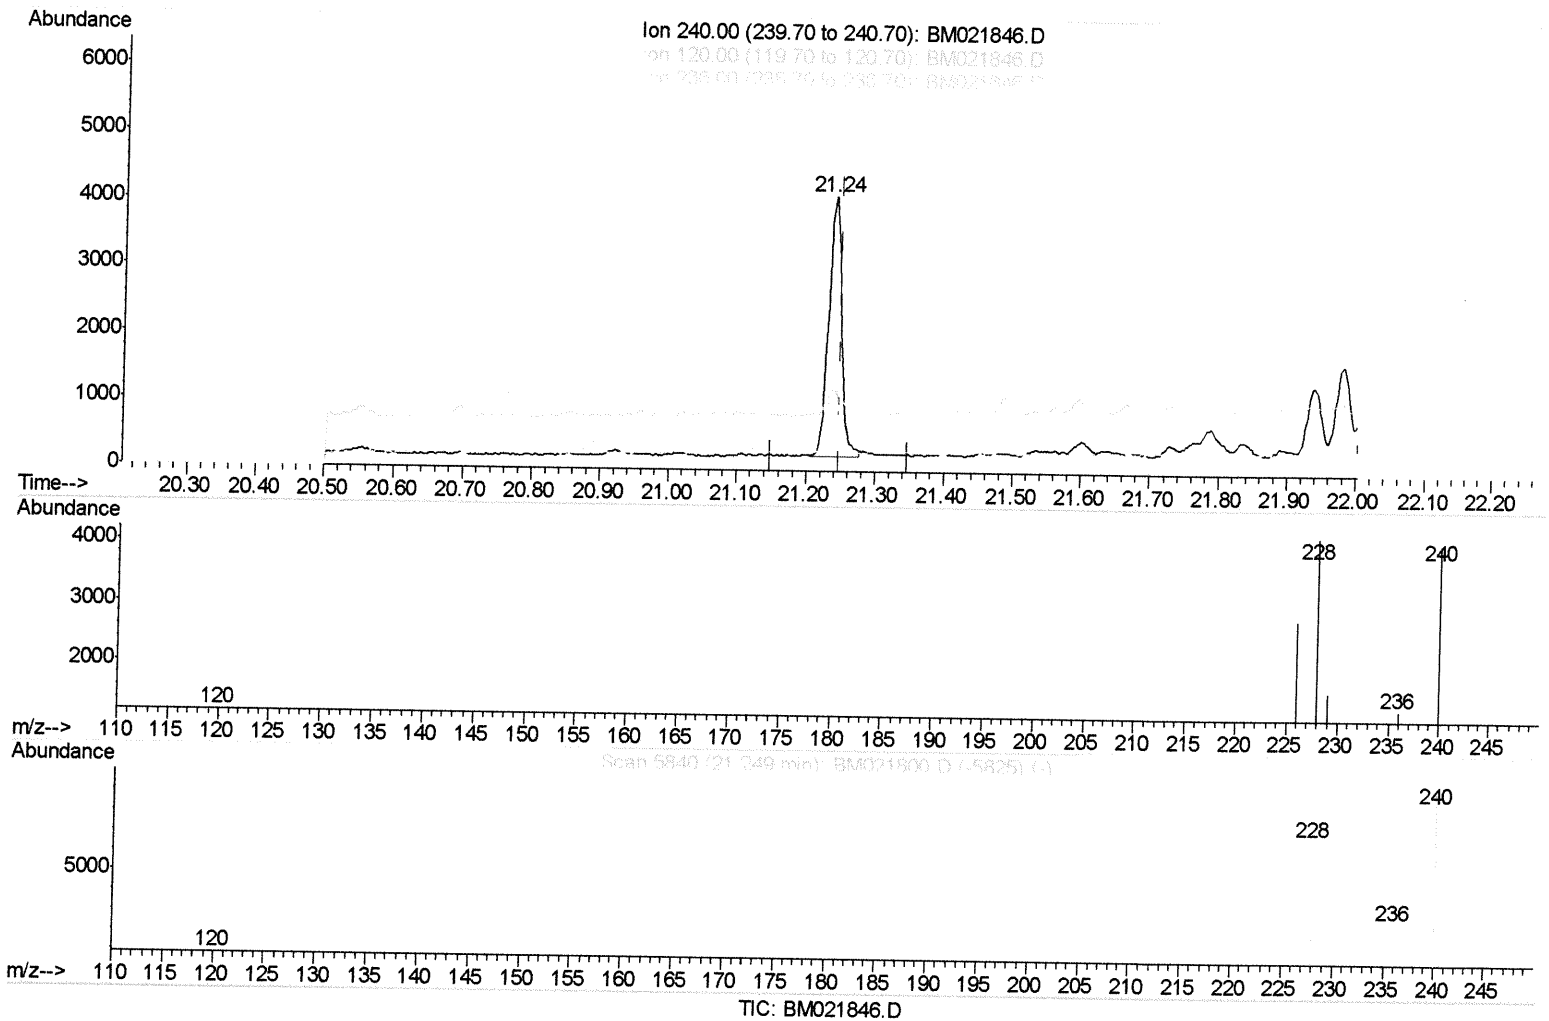

(16) Chrysene-d12 (I)

21.239min (-0.010) 0.40ng/ul m *Ju 8/5/19*

response 5066

Ion	Exp%	Act%
240.00	100	100
120.00	16.20	29.37#
236.00	32.30	33.29
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
 Data File : BM021846.D
 Acq On : 05 Aug 2019 17:27
 Operator : HP/JU
 Sample : K3850-19DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENS5DL

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:17:31 PM

Quant Time: Aug 05 18:06:41 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 17:14:32 2019
 Response via : Initial Calibration

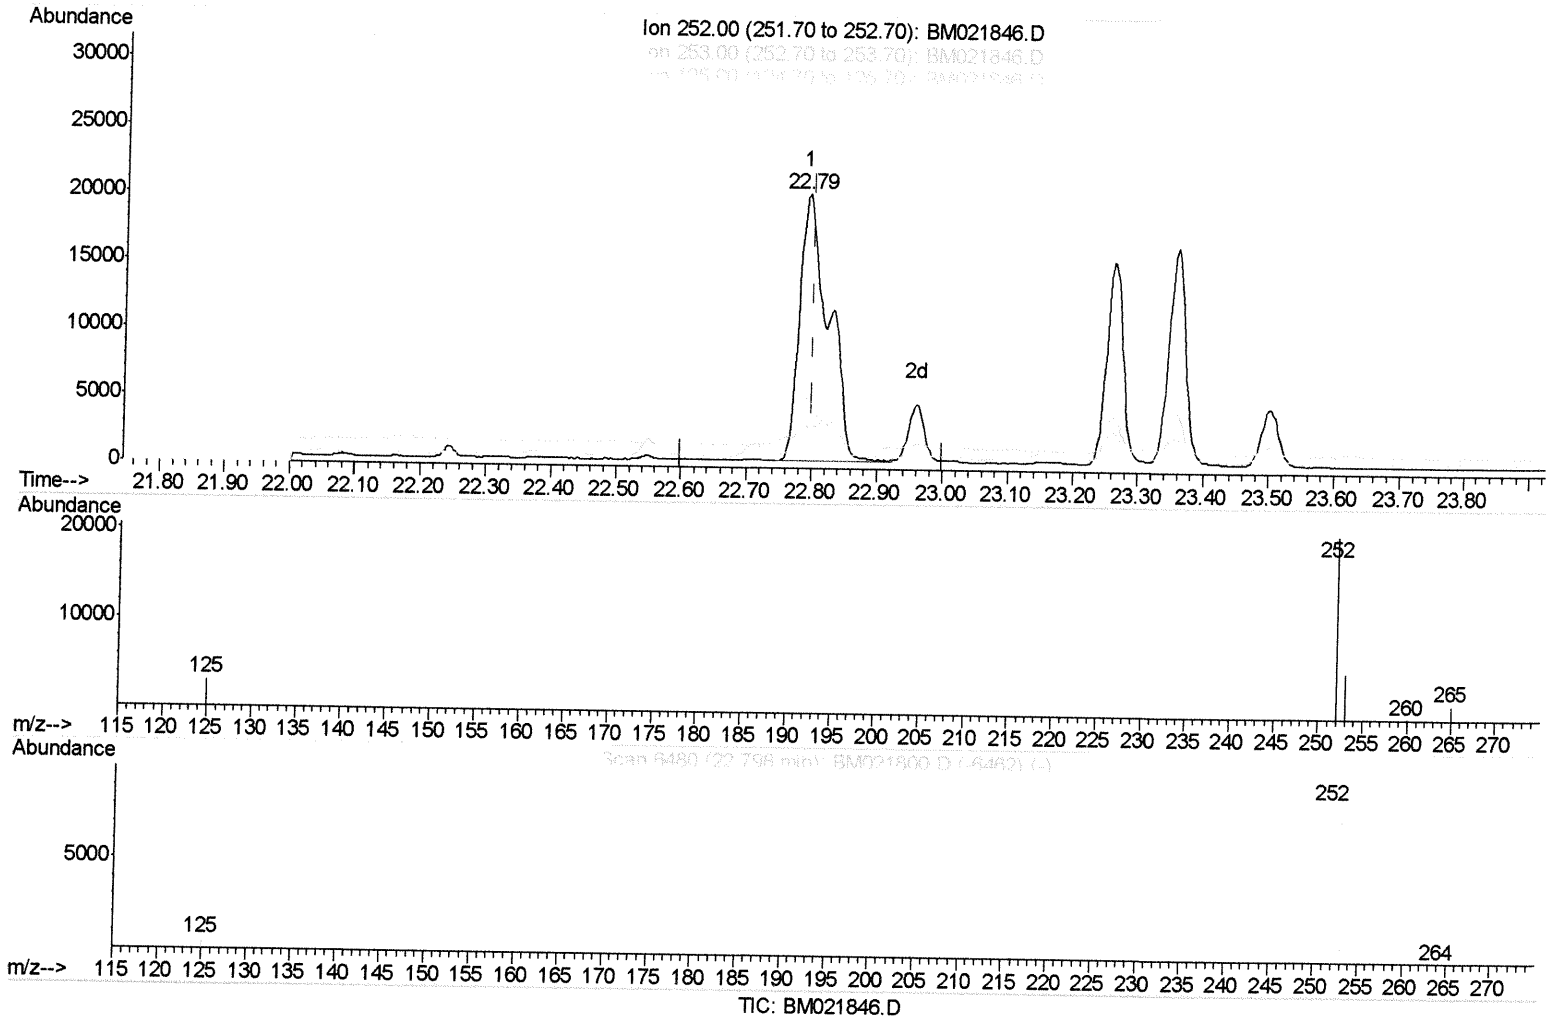

(21) Benzo(b)fluoranthene

22.791min (-0.010) 2.59ng/ui

response 61145

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	25.48
125.00	15.50	15.47
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
 Data File : BM021846.D
 Acq On : 05 Aug 2019 17:27
 Operator : HP/JU
 Sample : K3850-19DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleID :
 BENS5DL

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:17:31 PM

Quant Time: Aug 05 18:06:41 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 17:14:32 2019
 Response via : Initial Calibration

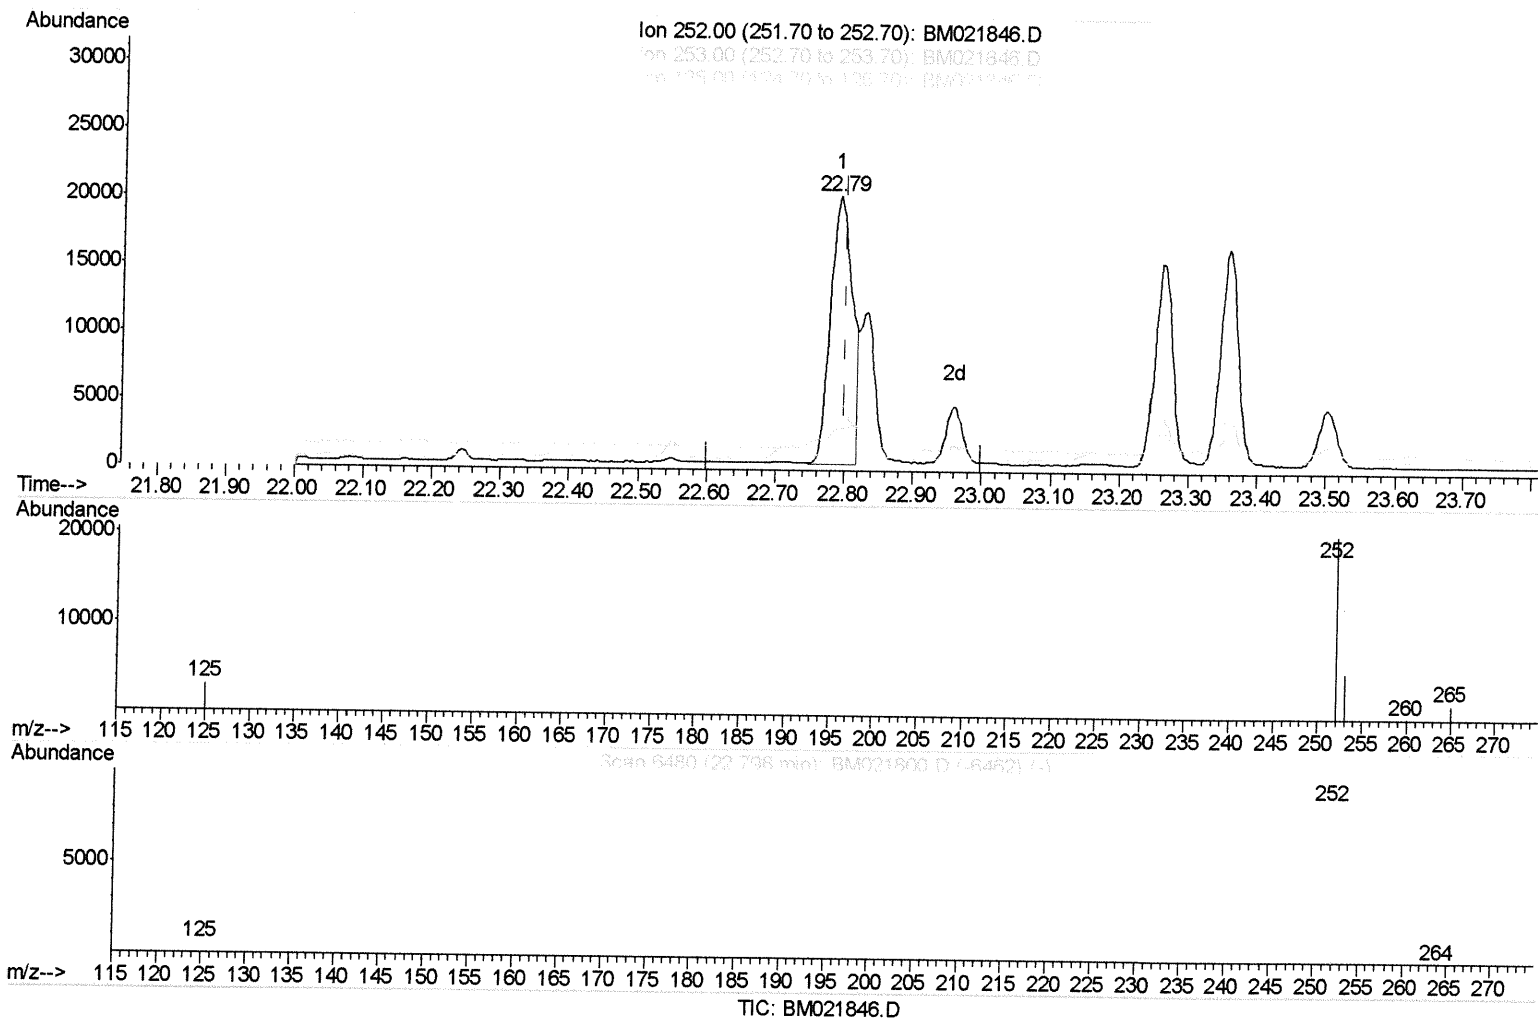

(21) Benzo(b)fluoranthene

22.791min (-0.010) 1.84ng/ul m *Ju 08/05/19*

response 43410

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	25.48
125.00	15.50	15.47
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
 Data File : BM021846.D
 Acq On : 05 Aug 2019 17:27
 Operator : HP/JU
 Sample : K3850-19DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENS5DL

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:17:31 PM

Quant Time: Aug 05 18:06:41 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 17:14:32 2019
 Response via : Initial Calibration

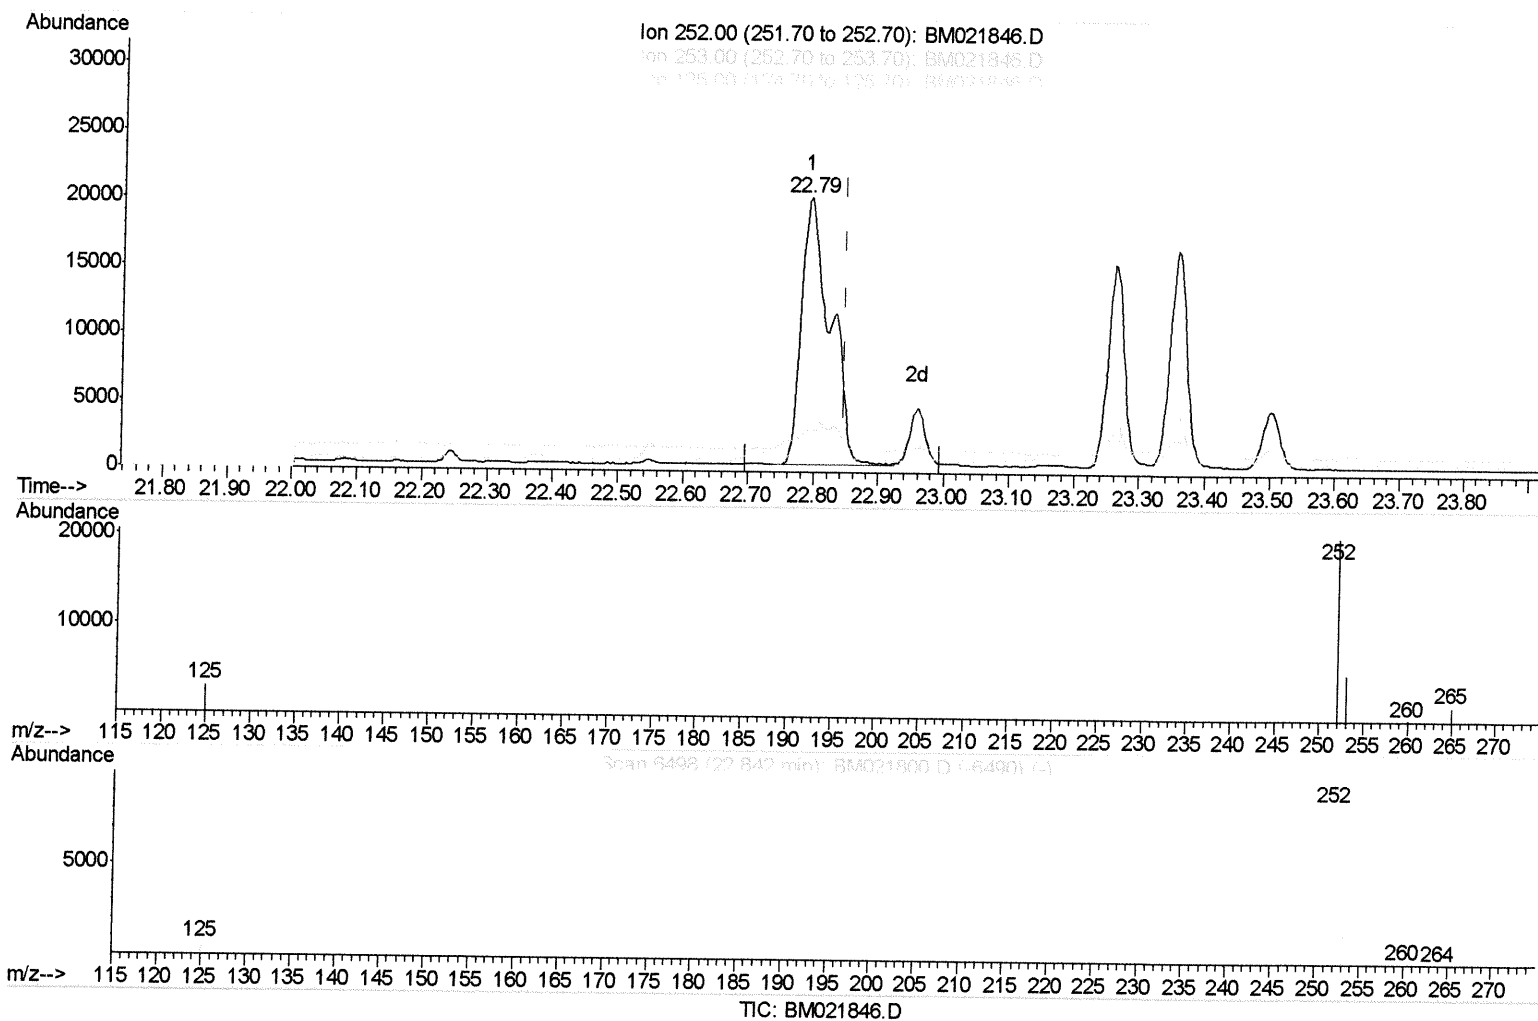

(22) Benzo(k)fluoranthene

22.791min (-0.056) 2.29ng/ui

response 61124

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	25.48#
125.00	15.20	15.47
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
 Data File : BM021846.D
 Acq On : 05 Aug 2019 17:27
 Operator : HP/JU
 Sample : K3850-19DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENS5DL

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:17:31 PM

Quant Time: Aug 05 18:06:41 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 17:14:32 2019
 Response via : Initial Calibration

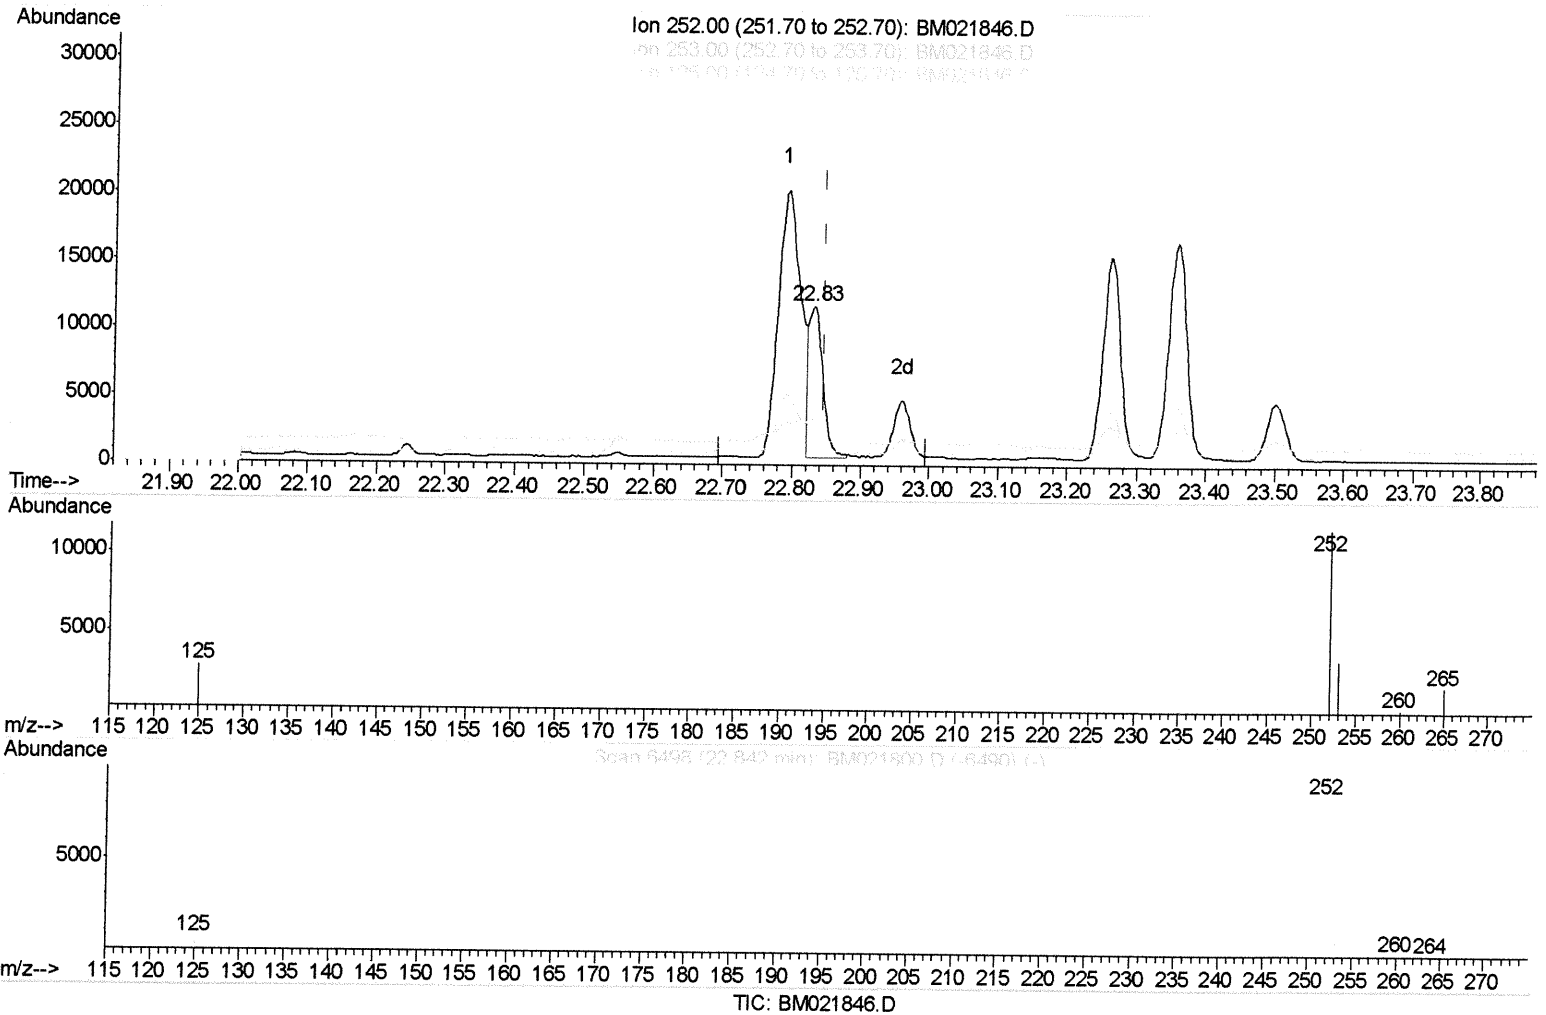

(22) Benzo(k)fluoranthene

22.830min (-0.017) 0.61ng/ul m

JU
 08/05/19

response 16186

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	29.65
125.00	15.20	23.87#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
 Data File : BM021846.D
 Acq On : 05 Aug 2019 17:27
 Operator : HP/JU
 Sample : K3850-19DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleID :
 BENS5DL

Manual Integrations
 APPROVED

mohammad
 8/5/2019 10:17:31 PM

Quant Time: Aug 05 18:08:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 05 17:14:32 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	938	0.40	ng/ul	0.00
2) Naphthalene-d8	10.41	136	3764	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.28	164	2115	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.04	188	4878m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.24	240	5066m	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	7007	0.40	ng/ul	-0.01

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.02	152	201	0.03	ng/ul	-0.02
14) Fluoranthene-d10	19.07	212	576m	0.04	ng/ul	-0.02

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.46	128	1295	0.122	ng/ul	94
5) 2-Methylnaphthalene	12.09	142	996	0.141	ng/ul	95
7) Acenaphthylene	14.01	152	3953	0.401	ng/ul	99
8) Acenaphthene	14.35	153	591	0.073	ng/ul	95
9) Fluorene	15.34	166	982	0.110	ng/ul#	97
12) Phenanthrene	17.08	178	18954m	1.335	ng/ul	
13) Anthracene	17.18	178	4833m	0.399	ng/ul	
15) Fluoranthene	19.10	202	48345m	2.543	ng/ul	
17) Pyrene	19.47	202	42996	2.065	ng/ul	98
18) Benzo(a)anthracene	21.22	228	24404	1.347	ng/ul	95
19) Chrysene	21.28	228	28278	1.213	ng/ul	95
21) Benzo(b)fluoranthene	22.79	252	43410m	1.837	ng/ul	
22) Benzo(k)fluoranthene	22.83	252	16186m	0.605	ng/ul	
23) Benzo(a)pyrene	23.36	252	28916	1.203	ng/ul#	85
24) Indeno(1,2,3-cd)pyrene	25.67	276	28047	0.978	ng/ul#	92
25) Dibenzo(a,h)anthracene	25.68	278	6231	0.269	ng/ul#	78
26) Benzo(g,h,i)perylene	26.35	276	32855	1.272	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed