
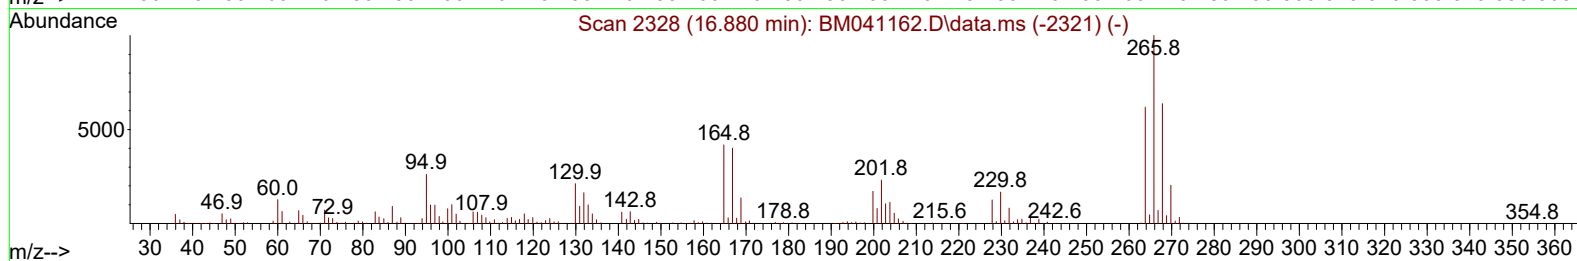
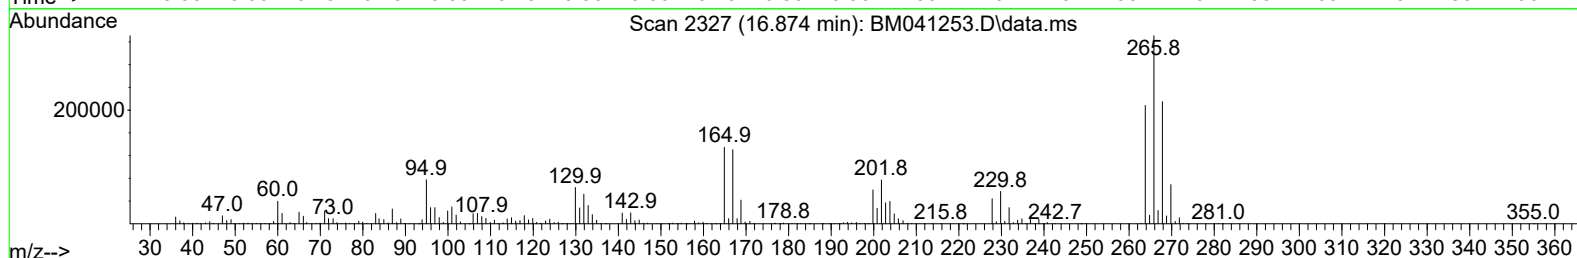


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080323\
Data File : BM041253.D
Acq On : 03 Aug 2023 08:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 11:02:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 19:20:51 2023
Response via : Initial Calibration

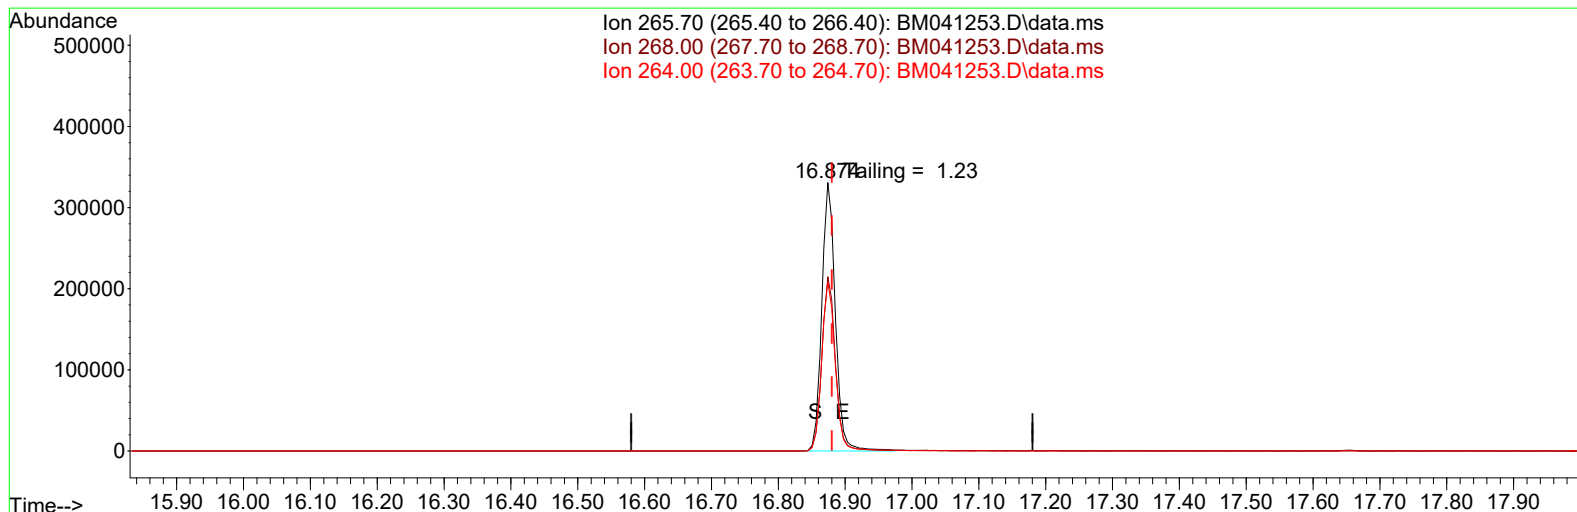

TIC: BM041253.D\data.ms

(70) Pentachlorophenol (C)




16.874min (-0.006) 0.00 ng

response 468496

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.92
264.00	61.80	62.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080323\
Data File : BM041253.D
Acq On : 03 Aug 2023 08:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 11:02:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 19:20:51 2023
Response via : Initial Calibration

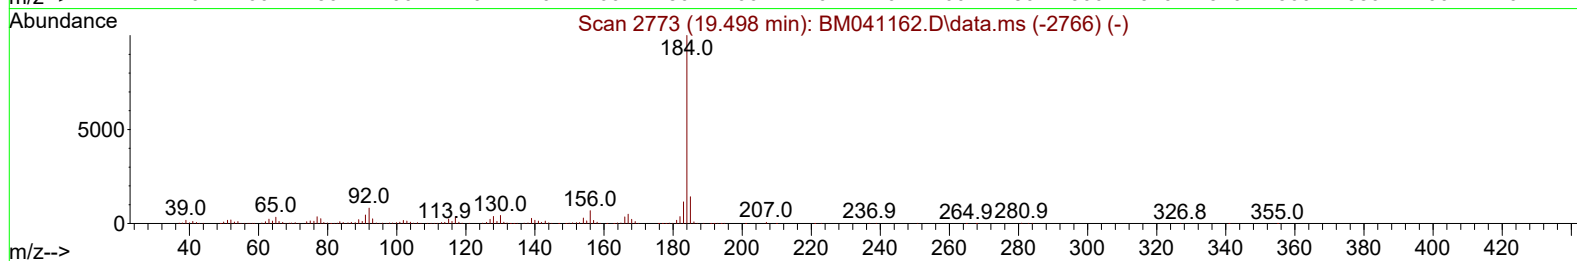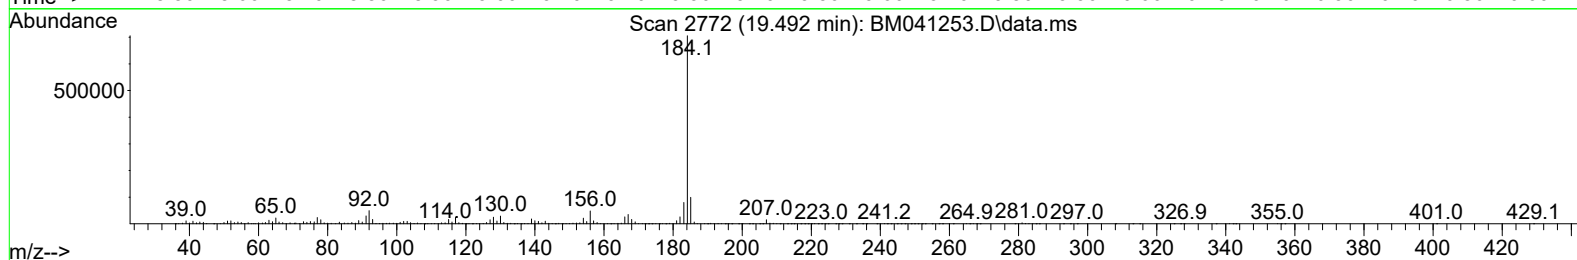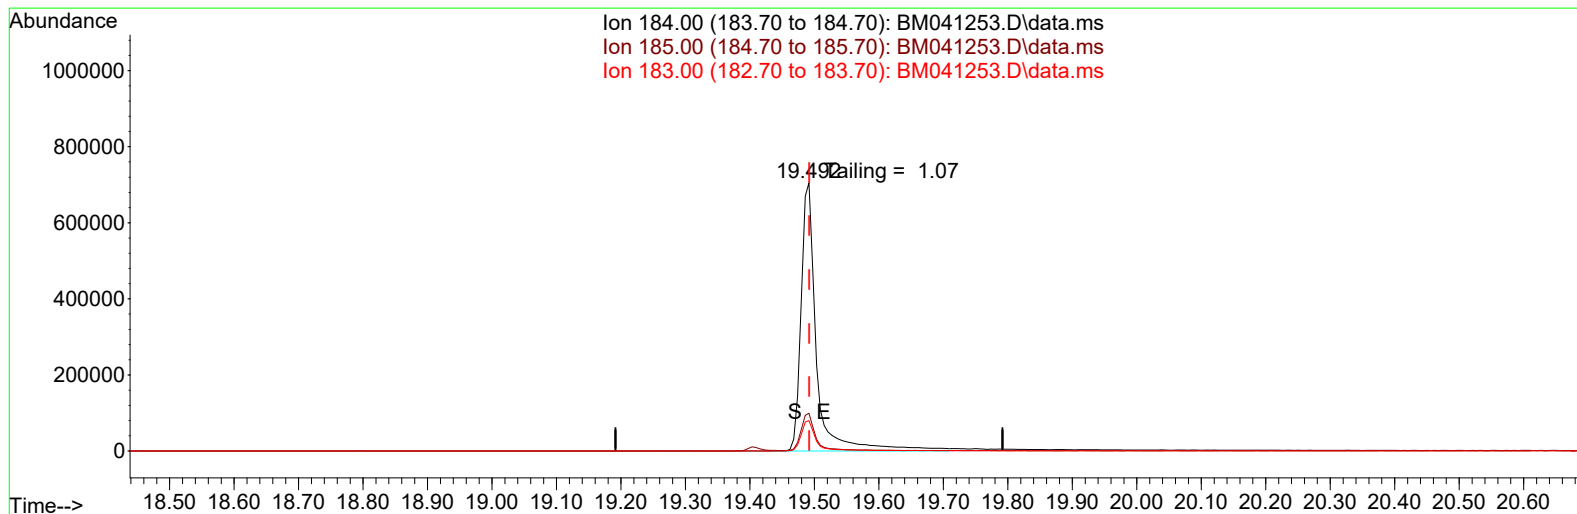

TIC: BM041253.D\data.ms

(77) Benzidine**19.492min (-0.000) 69186.33 ng****response 1168380**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.07
183.00	11.50	11.32
0.00	0.00	0.00