
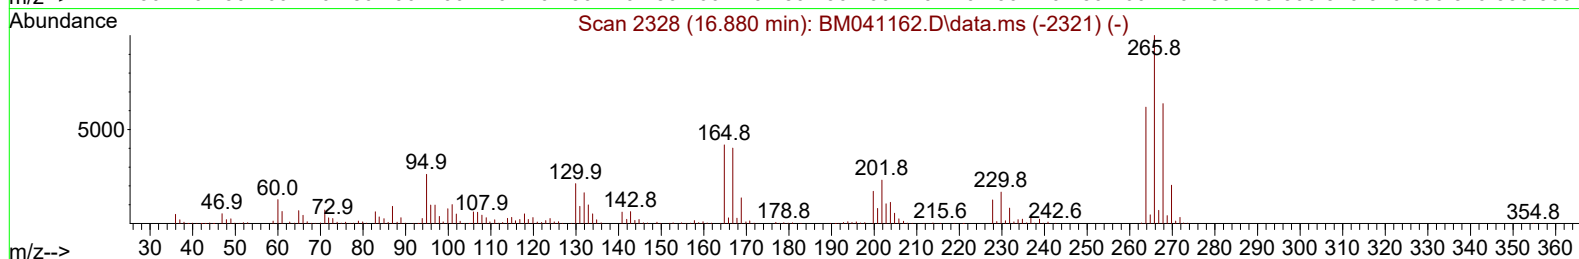
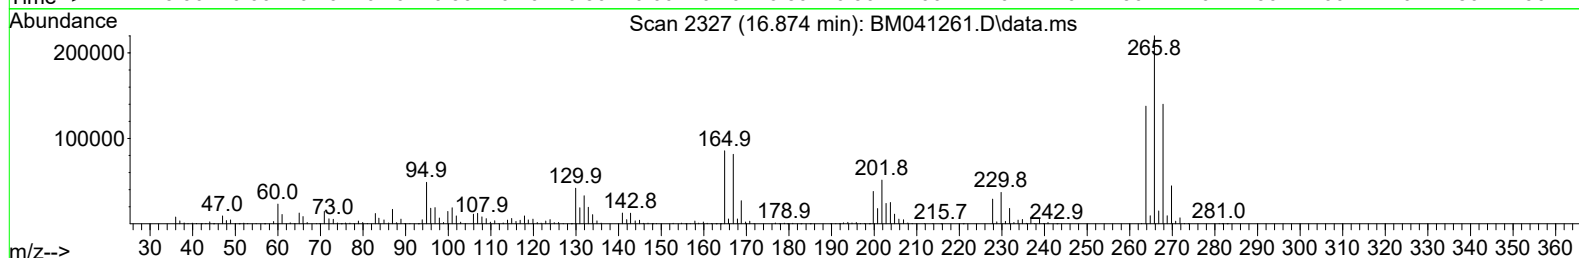


Quant Time: Aug 03 14:56:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 19:20:51 2023
Response via : Initial Calibration

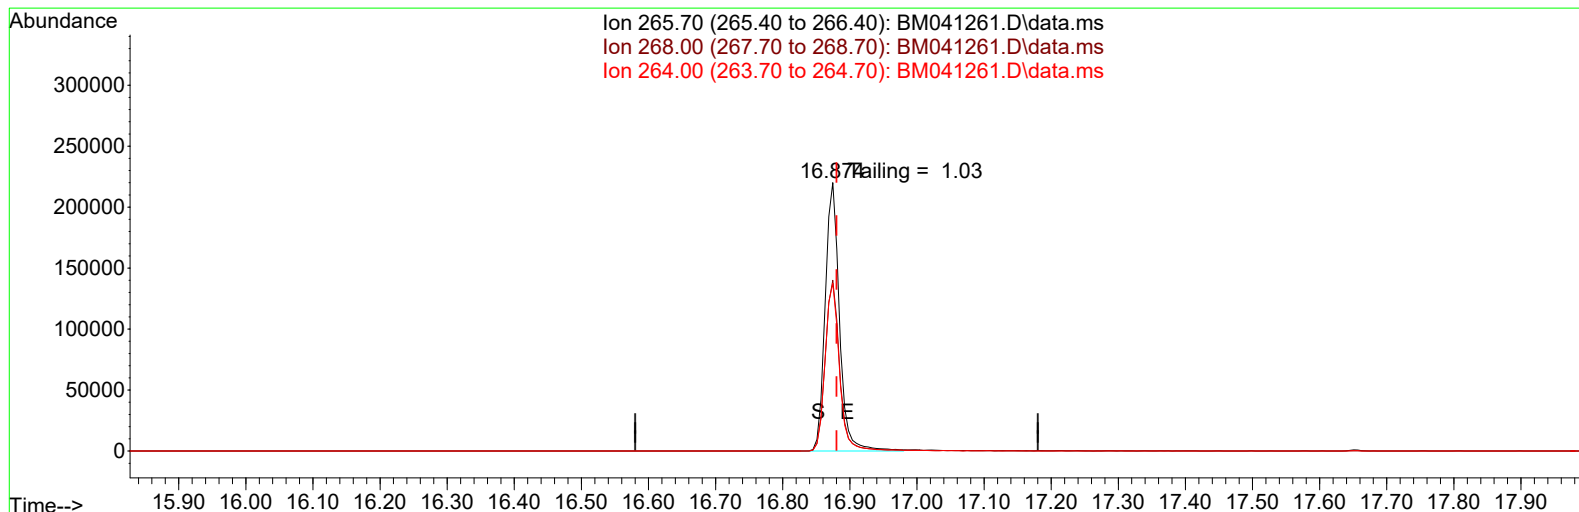

TIC: BM041261.D\data.ms

(70) Pentachlorophenol (C)




16.874min (-0.006) 0.00 ng

response **325977**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.59
264.00	61.80	62.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080323\
Data File : BM041261.D
Acq On : 03 Aug 2023 14:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 14:56:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 19:20:51 2023
Response via : Initial Calibration

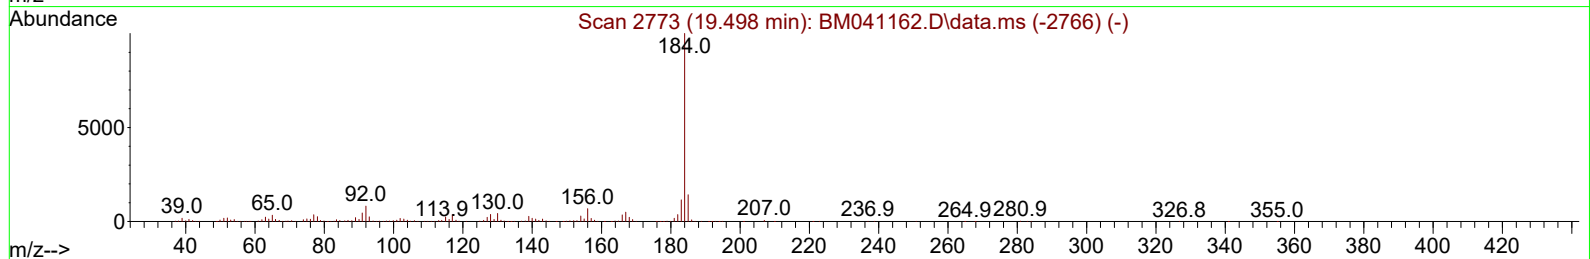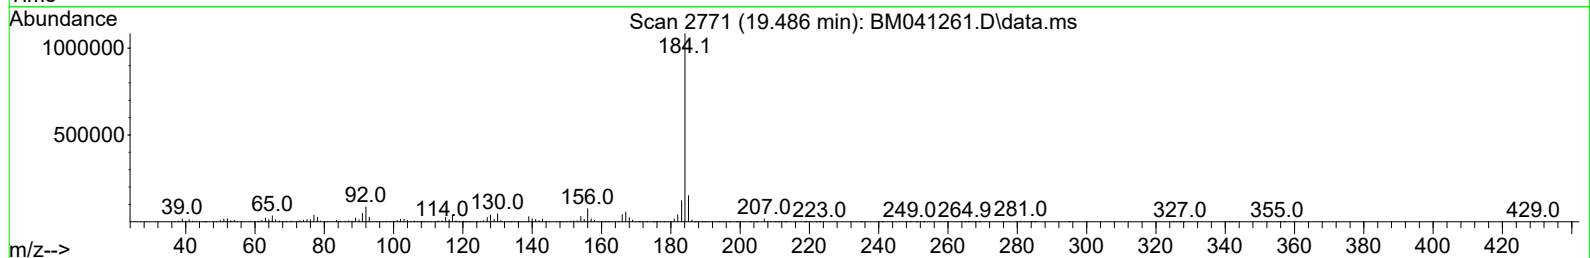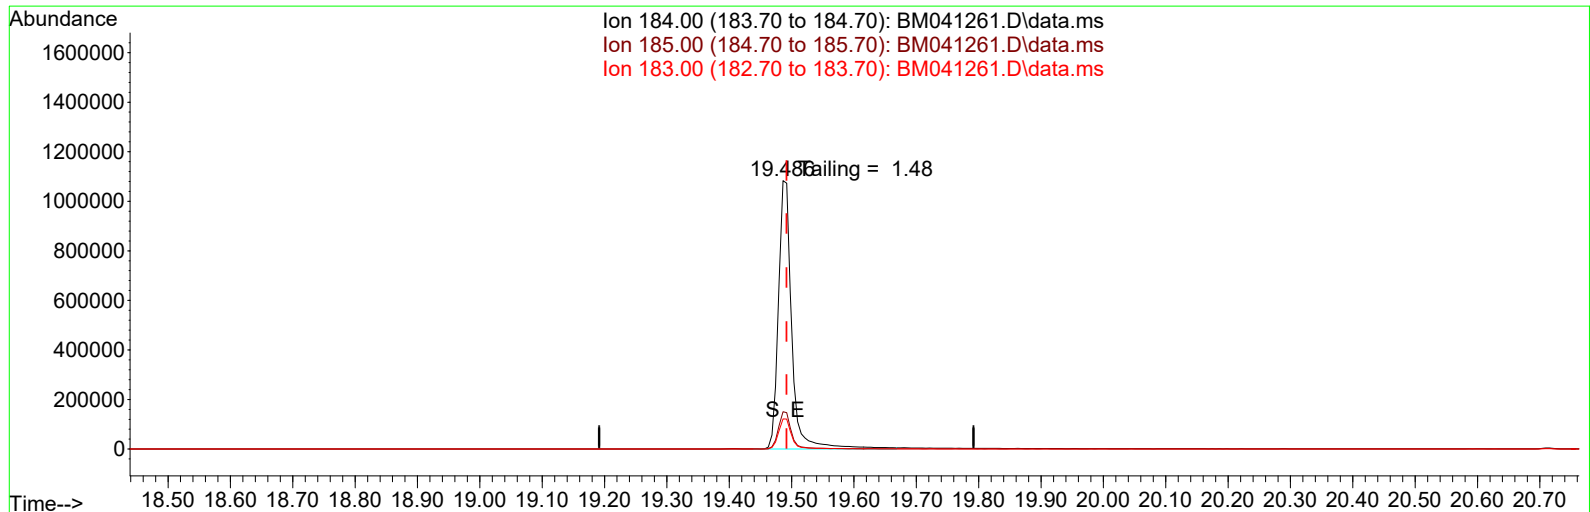

TIC: BM041261.D\data.ms

(77) Benzidine**19.486min (-0.006) 99987.84 ng****response 1639477**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.93
183.00	11.50	11.25
0.00	0.00	0.00