

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080323\
 Data File : BM041279.D
 Acq On : 04 Aug 2023 01:45
 Operator : MA/JU
 Sample : 03862-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BUILDING-B-3-(5-10)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/04/2023
 Supervised By :mohammad ahmed 08/04/2023

Quant Time: Aug 04 02:26:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 02 19:20:51 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.792	152	152859	20.000	ng	0.00
21) Naphthalene-d8	10.604	136	675661	20.000	ng	0.00
39) Acenaphthene-d10	14.463	164	443163	20.000	ng	0.00
64) Phenanthrene-d10	17.227	188	861812	20.000	ng	0.00
76) Chrysene-d12	21.433	240	566866	20.000	ng	0.00
86) Perylene-d12	23.809	264	618097	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.369	112	1043487	102.027	ng	0.00
7) Phenol-d6	6.981	99	1407248	106.149	ng	0.00
23) Nitrobenzene-d5	8.975	82	932186	64.161	ng	0.00
42) 2,4,6-Tribromophenol	15.968	330	671500	107.126	ng	0.00
45) 2-Fluorobiphenyl	13.080	172	2292821	65.357	ng	0.00
79) Terphenyl-d14	19.862	244	2827576	90.187	ng	0.00
Target Compounds						Qvalue
31) Naphthalene	10.657	128	3298054	89.950	ng	99
37) 2-Methylnaphthalene	12.275	142	2743478	110.987	ng	98
38) 1-Methylnaphthalene	12.504	142	3726191	161.059	ng	99
46) 1,1'-Biphenyl	13.292	154	607658	16.914	ng	99
49) Acenaphthylene	14.186	152	1567317	36.198	ng	# 92
52) Acenaphthene	14.527	154	1099520	42.153	ng	100
55) Dibenzofuran	14.863	168	284146	6.677	ng	# 50
58) Fluorene	15.521	166	1970030	58.679	ng	99
71) Phenanthrene	17.280	178	7542590	157.522	ng	99
72) Anthracene	17.362	178	1834452	38.737	ng	99
73) Carbazole	17.645	167	103550	2.416	ng	# 79
75) Fluoranthene	19.303	202	2922588	54.328	ng	98
78) Pyrene	19.668	202	4792199	120.888	ng	99
81) Benzo(a)anthracene	21.415	228	1340959	34.895	ng	# 88
83) Chrysene	21.468	228	1369102	36.833	ng	# 94
87) Indeno(1,2,3-cd)pyrene	26.262	276	494302	10.877	ng	# 93
88) Benzo(b)fluoranthene	23.091	252	919324m	25.037	ng	
89) Benzo(k)fluoranthene	23.127	252	251009m	6.683	ng	
90) Benzo(a)pyrene	23.703	252	1030531	29.209	ng	95
91) Dibenzo(a,h)anthracene	26.262	278	162375	4.284	ng	# 72
92) Benzo(g,h,i)perylene	27.026	276	613809	16.550	ng	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080323\
Data File : BM041279.D
Acq On : 04 Aug 2023 01:45
Operator : MA/JU
Sample : 03862-02
Misc :
ALS Vial : 24 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BUILDING-B-3-(5-10)

Quant Time: Aug 04 02:26:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 19:20:51 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/04/2023
Supervised By :mohammad ahmed 08/04/2023

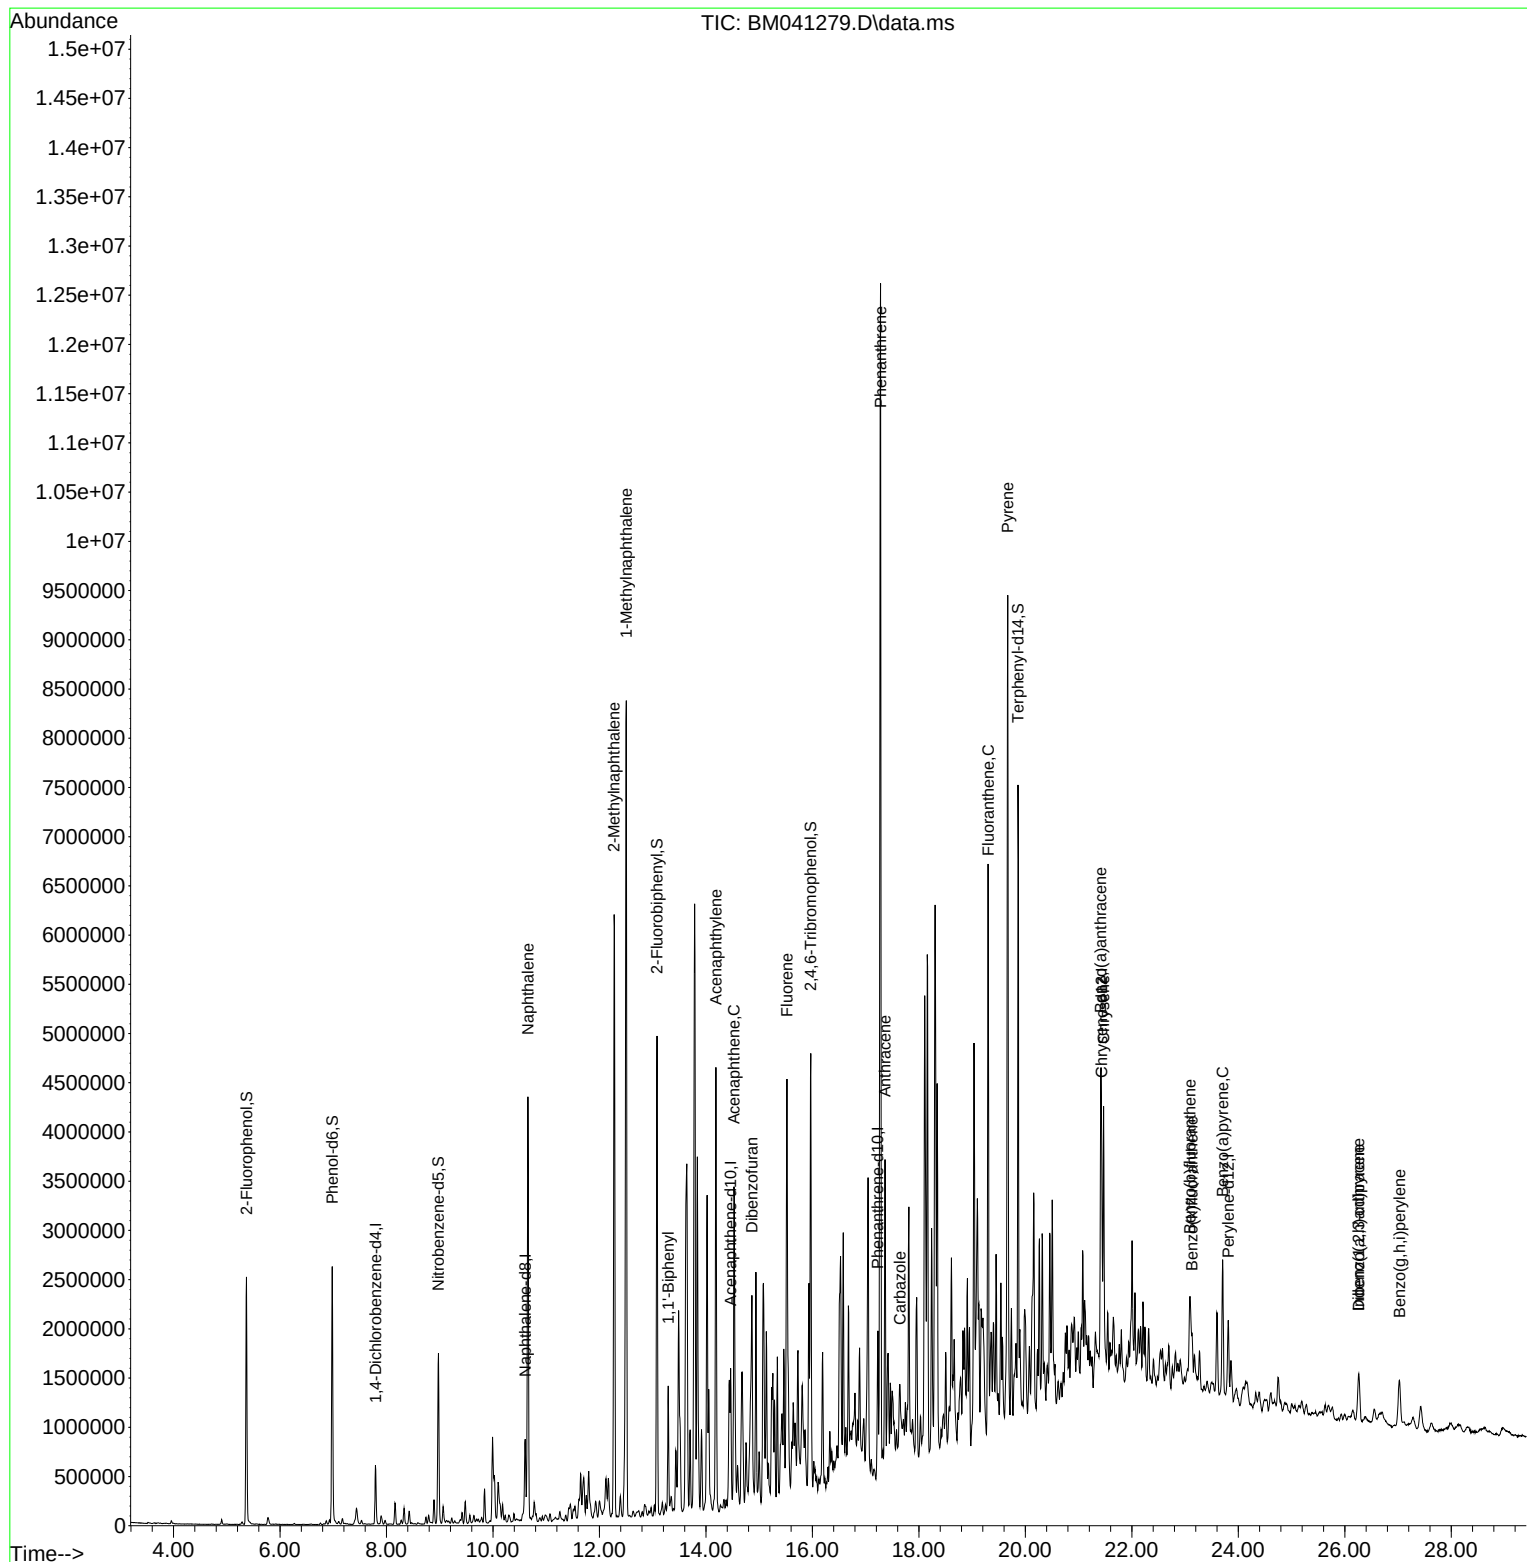



#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.792 min Scan# 71
Delta R.T. -0.001 min
Lab File: BM041279.D
Acq: 04 Aug 2023 01:45




Instrument :
BNA_M
ClientSampleId :
BUILDING-B-3-(5-10)



Tgt Ion:152 Resp: 152859
Ion Ratio Lower Upper
152 100
150 156.9 125.5 188.3
115 60.0 48.0 72.0




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/04/2023
Supervised By :mohammad ahmed 08/04/2023

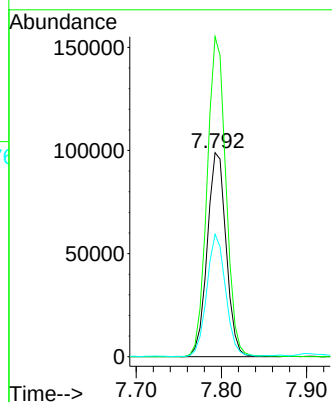

#5
2-Fluorophenol
Concen: 102.027 ng
RT: 5.369 min Scan# 371
Delta R.T. -0.000 min
Lab File: BM041279.D
Acq: 04 Aug 2023 01:45


Tgt Ion:112 Resp: 1043487
Ion Ratio Lower Upper
112 100
64 57.3 48.5 72.7
63 31.3 26.5 39.7

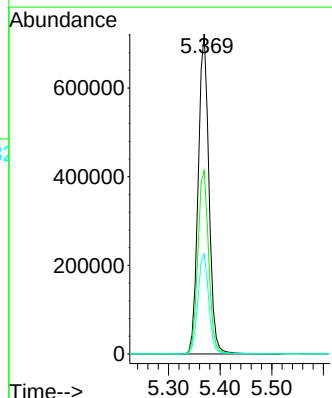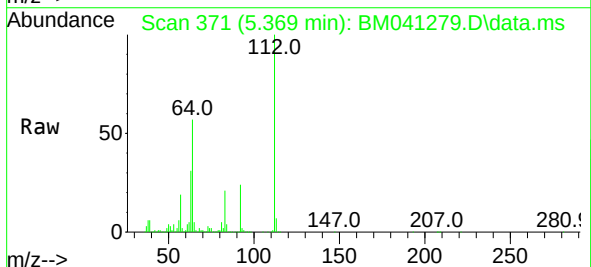



#7
Phenol-d6
Concen: 106.149 ng
RT: 6.981 min Scan# 645
Delta R.T. -0.000 min
Lab File: BM041279.D
Acq: 04 Aug 2023 01:45




Instrument :
BNA_M
ClientSampleId :
BUILDING-B-3-(5-10)




Tgt Ion: 99 Resp: 1407248
Ion Ratio Lower Upper
99 100
42 17.9 15.4 23.0
71 36.7 28.2 42.4

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 08/04/2023
Supervised By :mohammad ahmed 08/04/2023

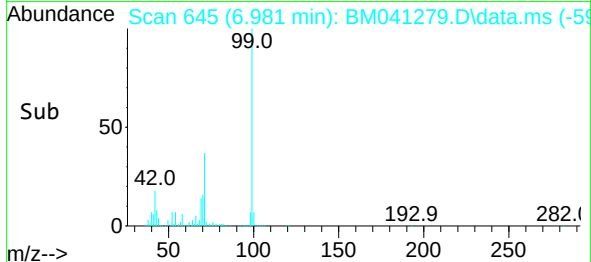


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.604 min Scan# 1261
Delta R.T. -0.000 min
Lab File: BM041279.D
Acq: 04 Aug 2023 01:45

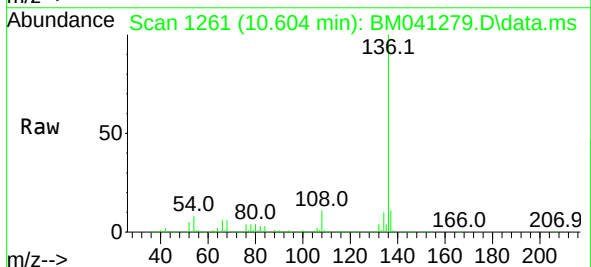


Tgt Ion:136 Resp: 675661
Ion Ratio Lower Upper
136 100
137 11.2 8.8 13.2
54 7.5 6.9 10.3
68 6.4 5.4 8.2

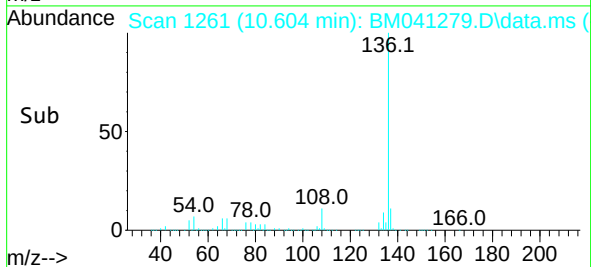

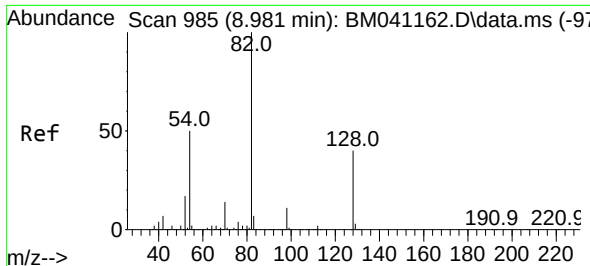

#23
Nitrobenzene-d5
Concen: 64.161 ng
RT: 8.975 min Scan# 91
Delta R.T. -0.000 min
Lab File: BM041279.D
Acq: 04 Aug 2023 01:45




Instrument :
BNA_M
ClientSampleId :
BUILDING-B-3-(5-10)

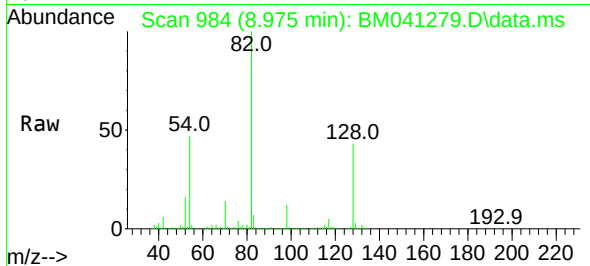


Tgt Ion: 82 Resp: 932180
Ion Ratio Lower Upper
82 100
128 42.6 31.8 47.6
54 46.6 40.1 60.1

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 08/04/2023
Supervised By :mohammad ahmed 08/04/2023

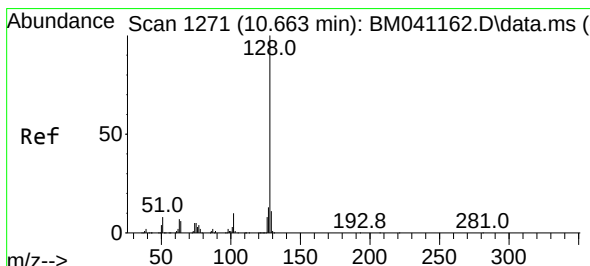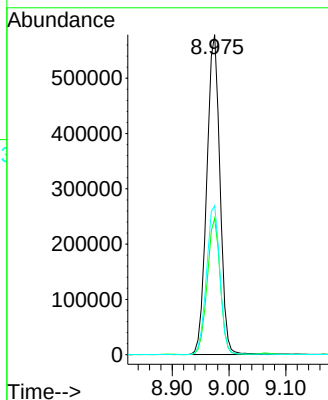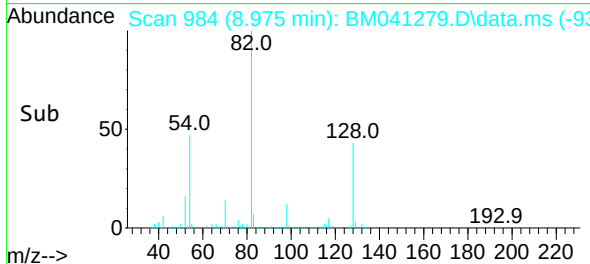


#31
Naphthalene
Concen: 89.950 ng
RT: 10.657 min Scan# 1270
Delta R.T. 0.006 min
Lab File: BM041279.D
Acq: 04 Aug 2023 01:45

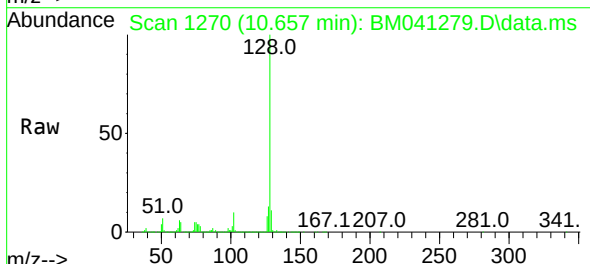


Tgt Ion:128 Resp: 3298054
Ion Ratio Lower Upper
128 100
129 11.0 9.0 13.4
127 13.3 10.5 15.7

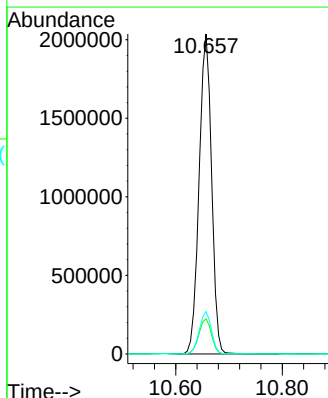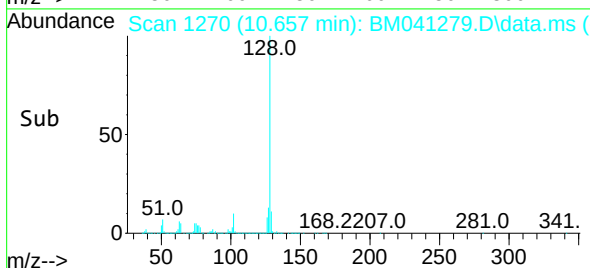

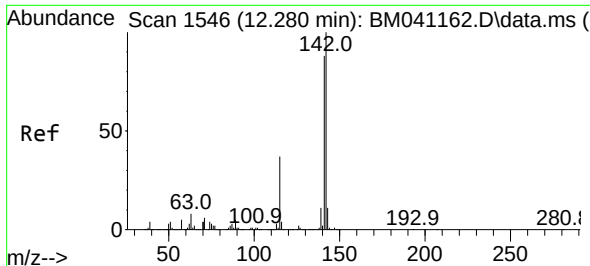

#37
2-Methylnaphthalene
Concen: 110.987 ng
RT: 12.275 min Scan# 1545
Delta R.T. -0.000 min
Lab File: BM041279.D
Acq: 04 Aug 2023 01:45




Instrument :
BNA_M
ClientSampleId :
BUILDING-B-3-(5-10)

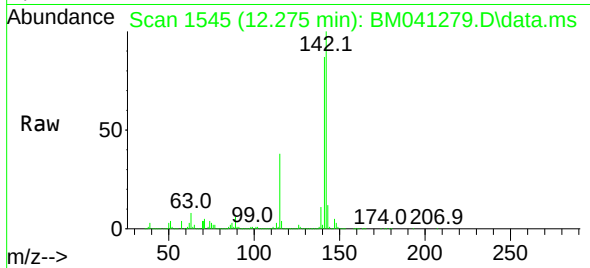

Tgt Ion:142 Resp: 2743478
Ion Ratio Lower Upper
142 100
141 87.1 70.7 106.1
115 37.7 29.3 43.9




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/04/2023
Supervised By :mohammad ahmed 08/04/2023

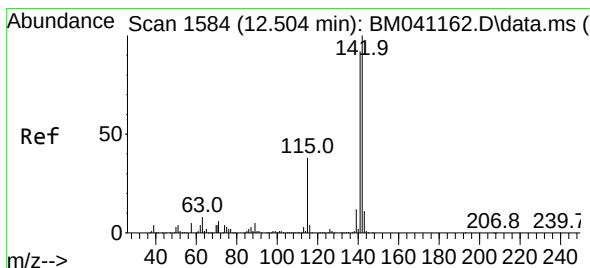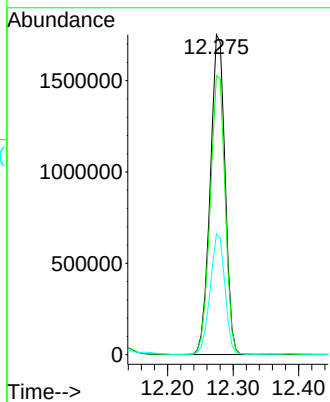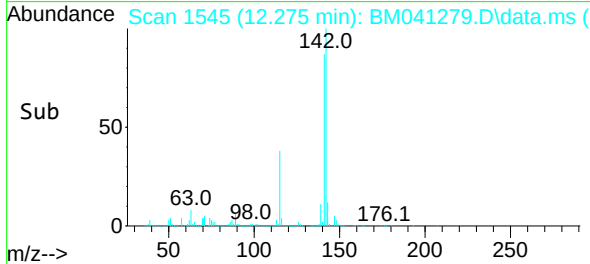

#38
1-Methylnaphthalene
Concen: 161.059 ng
RT: 12.504 min Scan# 1584
Delta R.T. 0.012 min
Lab File: BM041279.D
Acq: 04 Aug 2023 01:45


Tgt Ion:142 Resp: 3726191
Ion Ratio Lower Upper
142 100
141 90.9 73.4 110.2
116 4.1 3.2 4.8

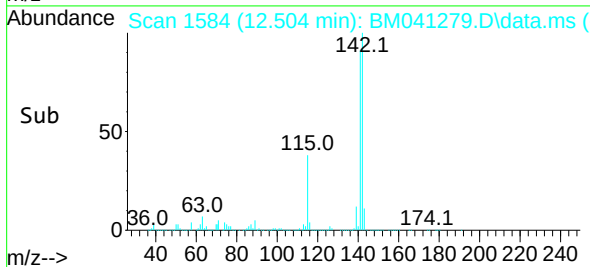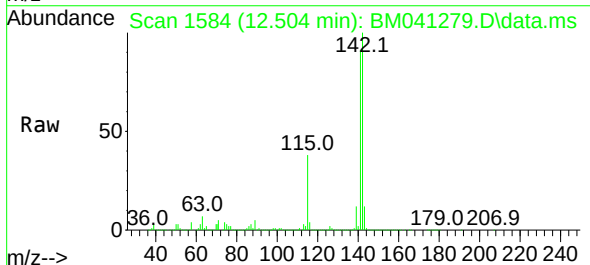

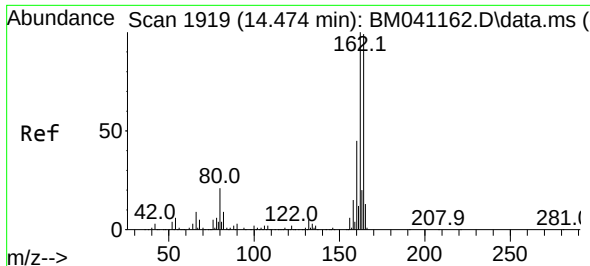

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.463 min Scan# 1917
Delta R.T. -0.000 min
Lab File: BM041279.D
Acq: 04 Aug 2023 01:45




Instrument :
BNA_M
ClientSampleId :
BUILDING-B-3-(5-10)

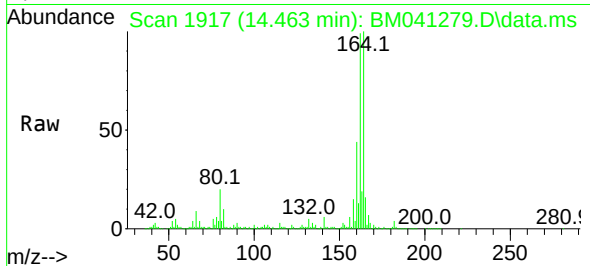


Tgt Ion:164 Resp: 44316
Ion Ratio Lower Upper
164 100
162 98.8 80.4 120.6
160 44.2 36.2 54.2

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 08/04/2023
Supervised By :mohammad ahmed 08/04/2023

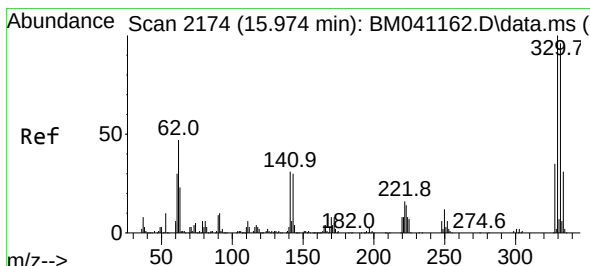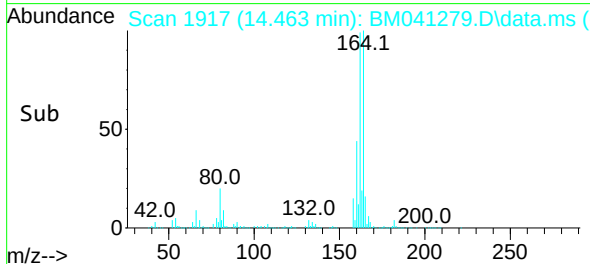


#42
2,4,6-Tribromophenol
Concen: 107.126 ng
RT: 15.968 min Scan# 2173
Delta R.T. -0.000 min
Lab File: BM041279.D
Acq: 04 Aug 2023 01:45

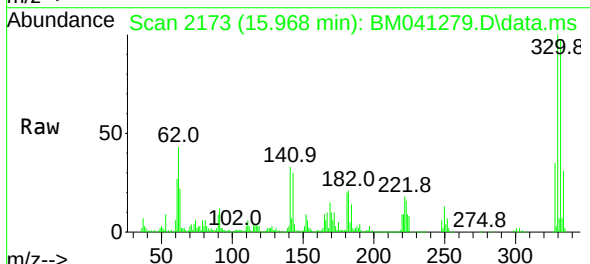


Tgt Ion:330 Resp: 671500
Ion Ratio Lower Upper
330 100
332 96.6 77.7 116.5
141 32.8 28.3 42.5

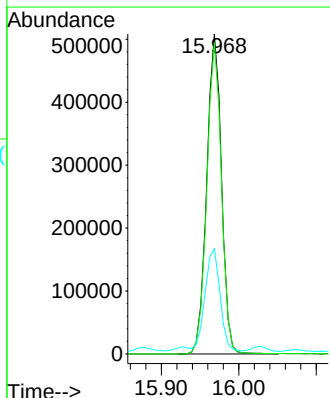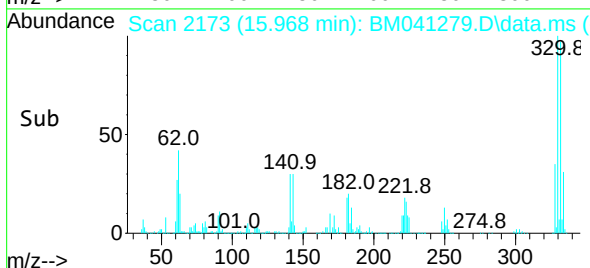



#45
2-Fluorobiphenyl
Concen: 65.357 ng
RT: 13.080 min Scan# 1718
Delta R.T. -0.000 min
Lab File: BM041279.D
Acq: 04 Aug 2023 01:45




Instrument :
BNA_M
ClientSampleId :
BUILDING-B-3-(5-10)

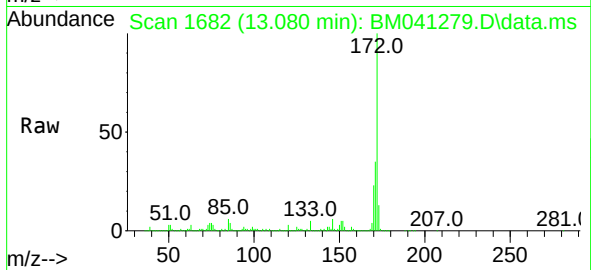


Tgt Ion:172 Resp: 229282
Ion Ratio Lower Upper
172 100
171 34.6 28.1 42.1
170 23.5 18.9 28.3

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 08/04/2023
Supervised By :mohammad ahmed 08/04/2023

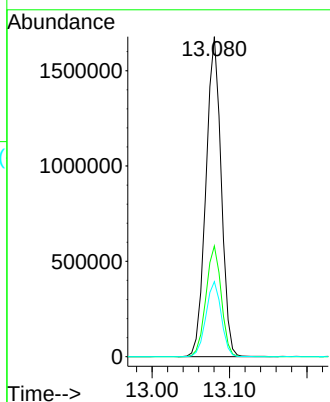


#46
1,1'-Biphenyl
Concen: 16.914 ng
RT: 13.292 min Scan# 1718
Delta R.T. -0.000 min
Lab File: BM041279.D
Acq: 04 Aug 2023 01:45

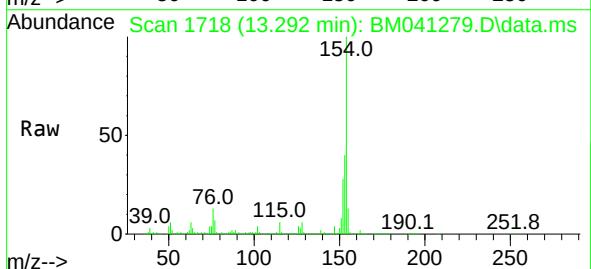


Tgt Ion:154 Resp: 607658
Ion Ratio Lower Upper
154 100
153 40.0 20.5 60.5
76 13.3 0.0 34.1



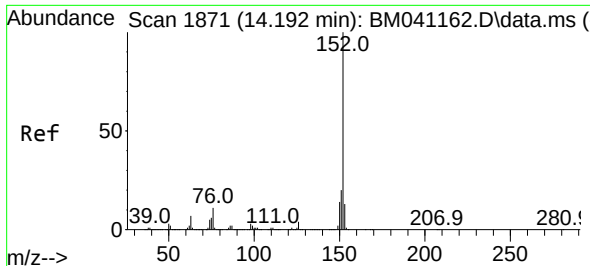

#49
Acenaphthylene
Concen: 36.198 ng
RT: 14.186 min Scan# 1871
Delta R.T. -0.000 min
Lab File: BM041279.D
Acq: 04 Aug 2023 01:45




Instrument :
BNA_M
ClientSampleId :
BUILDING-B-3-(5-10)

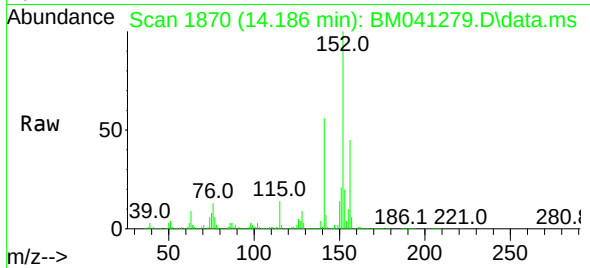


Tgt Ion:152 Resp: 1567317
Ion Ratio Lower Upper
152 100
151 20.7 16.1 24.1
153 20.1 10.5 15.7

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 08/04/2023
Supervised By :mohammad ahmed 08/04/2023

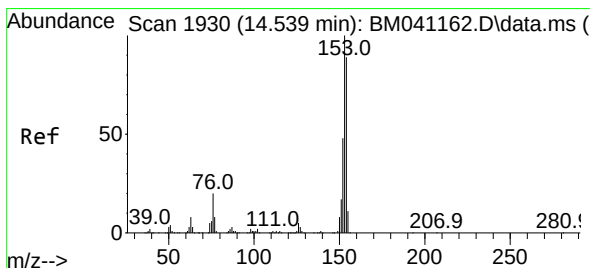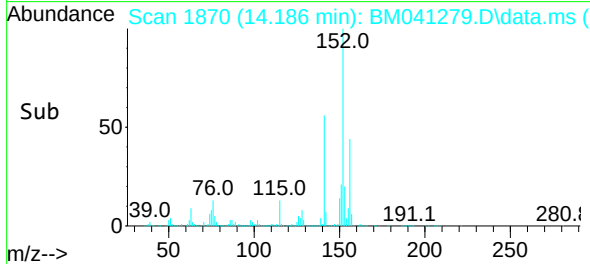


#52
Acenaphthene
Concen: 42.153 ng
RT: 14.527 min Scan# 1928
Delta R.T. -0.000 min
Lab File: BM041279.D
Acq: 04 Aug 2023 01:45

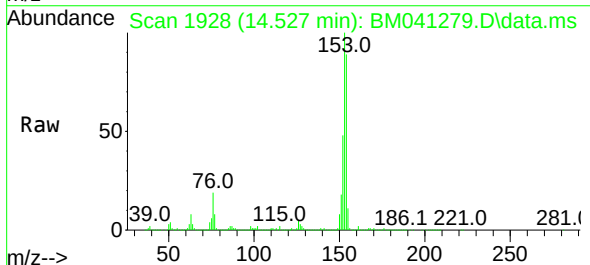


Tgt Ion:154 Resp: 1099520
Ion Ratio Lower Upper
154 100
153 112.7 90.2 135.4
152 54.0 43.4 65.0

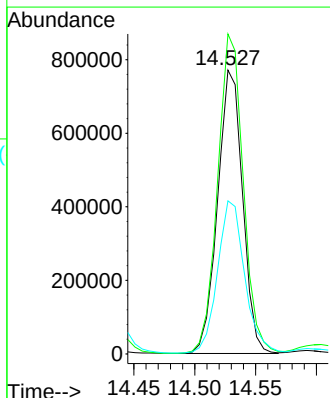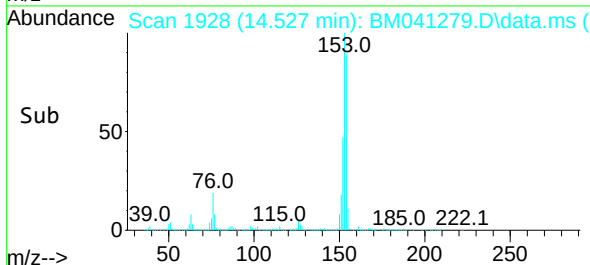

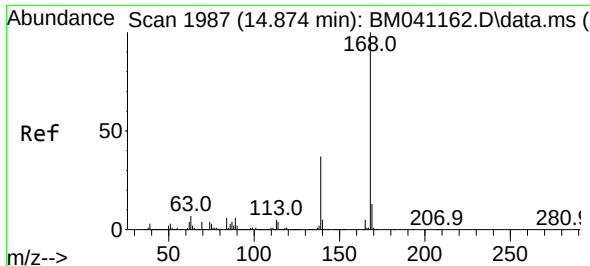

#55
Dibenzenofuran
Concen: 6.677 ng
RT: 14.863 min Scan# 1985
Delta R.T. -0.000 min
Lab File: BM041279.D
Acq: 04 Aug 2023 01:45




Instrument :
BNA_M
ClientSampleId :
BUILDING-B-3-(5-10)

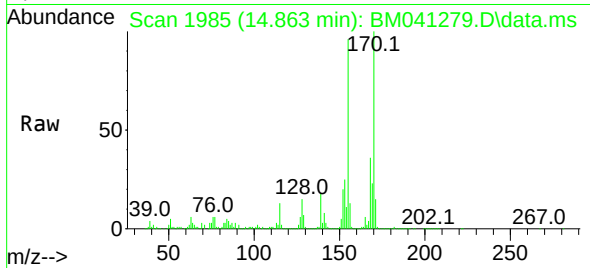

Tgt Ion:168 Resp: 284140
Ion Ratio Lower Upper
168 100
139 50.7 29.8 44.6
169 63.9 10.5 15.7




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/04/2023
Supervised By :mohammad ahmed 08/04/2023

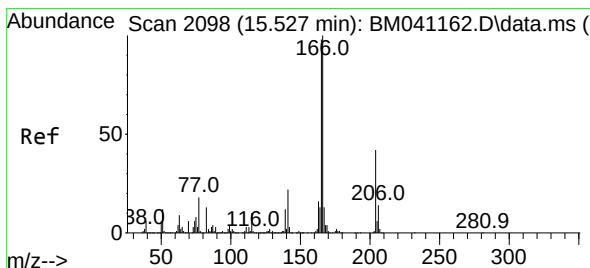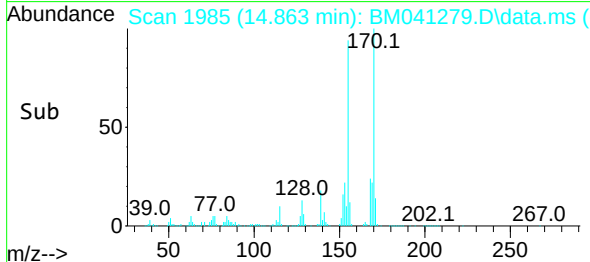

#58
Fluorene
Concen: 58.679 ng
RT: 15.521 min Scan# 2097
Delta R.T. 0.006 min
Lab File: BM041279.D
Acq: 04 Aug 2023 01:45

Tgt Ion:166 Resp: 1970030
Ion Ratio Lower Upper
166 100
165 98.4 78.2 117.4
167 14.5 10.6 16.0

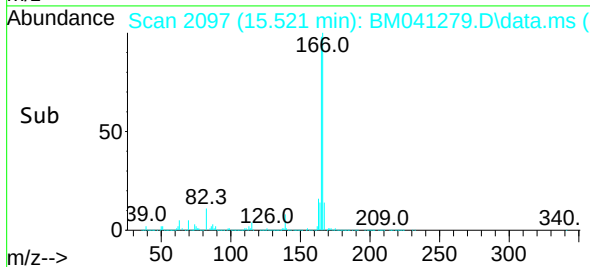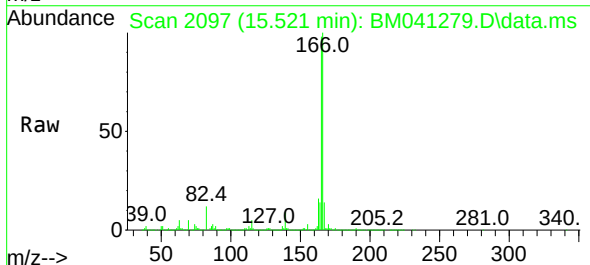



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.227 min Scan# 21

Delta R.T. 0.006 min

Lab File: BM041279.D

Acq: 04 Aug 2023 01:45

Instrument :

BNA_M

ClientSampleId :

BUILDING-B-3-(5-10)

Tgt Ion:188 Resp: 86181

Ion Ratio Lower Upper

188 100

94 8.7 8.2 12.2





80 9.5 8.6 13.0

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 08/04/2023

Supervised By :mohammad ahmed 08/04/2023



#71

Phenanthrene

Concen: 157.522 ng

RT: 17.280 min Scan# 2396

Delta R.T. 0.012 min

Lab File: BM041279.D

Acq: 04 Aug 2023 01:45




Tgt Ion:178 Resp: 7542590


Ion Ratio Lower Upper

178 100

176 19.8 15.6 23.4

179 15.8 12.1 18.1

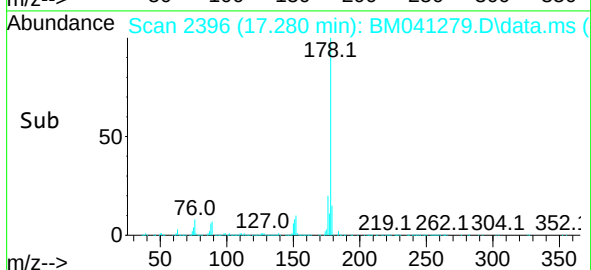



#72

Anthracene

Concen: 38.737 ng

RT: 17.362 min Scan# 2410

Delta R.T. 0.006 min

Lab File: BM041279.D

Acq: 04 Aug 2023 01:45

Instrument :

BNA_M

ClientSampleId :

BUILDING-B-3-(5-10)

Tgt Ion:178 Resp: 183445

Ion Ratio Lower Upper

178 100

176 19.2 15.2 22.8





179 15.8 12.4 18.6

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 08/04/2023

Supervised By :mohammad ahmed 08/04/2023

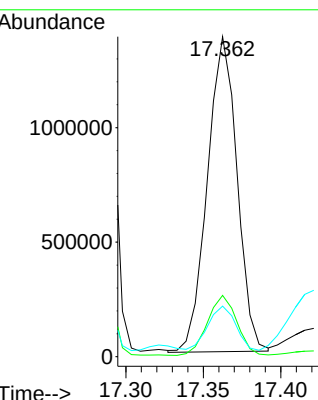

#73

Carbazole

Concen: 2.416 ng

RT: 17.645 min Scan# 2458

Delta R.T. 0.006 min

Lab File: BM041279.D

Acq: 04 Aug 2023 01:45




Tgt Ion:167 Resp: 103550


Ion Ratio Lower Upper

167 100

166 31.2 17.3 25.9#


139 22.1 10.3 15.5#

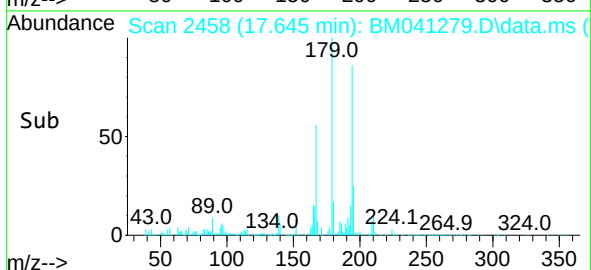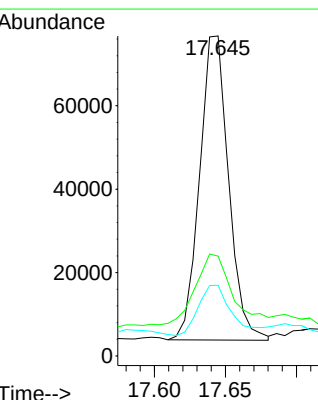



#75
Fluoranthene
Concen: 54.328 ng
RT: 19.303 min Scan# 21
Delta R.T. 0.012 min
Lab File: BM041279.D
Acq: 04 Aug 2023 01:45




Instrument :
BNA_M
ClientSampleId :
BUILDING-B-3-(5-10)



Tgt Ion:202 Resp: 292258
Ion Ratio Lower Upper
202 100
101 9.1 0.0 30.8
203 17.9 0.0 37.6




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/04/2023
Supervised By :mohammad ahmed 08/04/2023

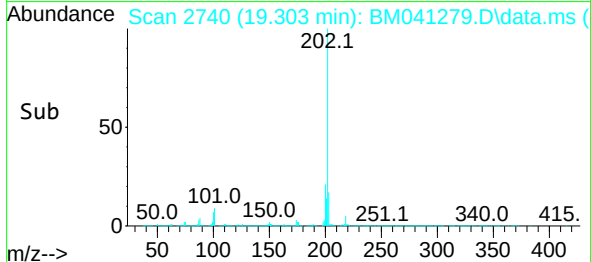

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.433 min Scan# 3102
Delta R.T. -0.000 min
Lab File: BM041279.D
Acq: 04 Aug 2023 01:45

Tgt Ion:240 Resp: 566866
Ion Ratio Lower Upper
240 100
120 9.1 8.3 12.5
236 27.0 20.6 30.8

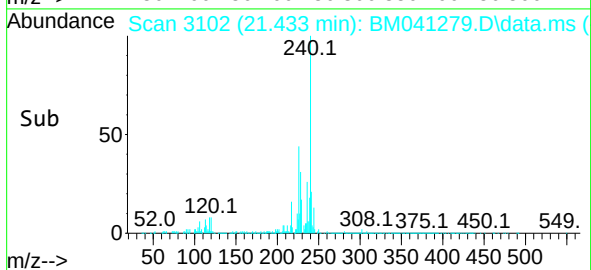



#78

Pyrene

Concen: 120.888 ng

RT: 19.668 min Scan# 2801

Delta R.T. 0.012 min

Lab File: BM041279.D

Acq: 04 Aug 2023 01:45

Instrument :

BNA_M

ClientSampleId :

BUILDING-B-3-(5-10)

Tgt Ion:202 Resp: 4792199

Ion Ratio Lower Upper

202 100

200 21.1 16.9 25.3





203 18.7 14.1 21.1

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 08/04/2023

Supervised By :mohammad ahmed 08/04/2023

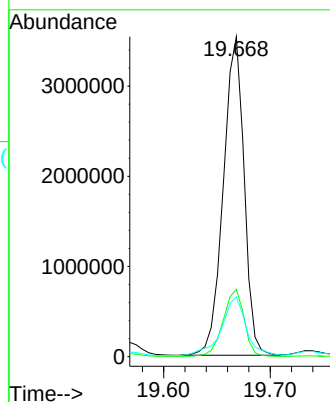

#79

Terphenyl-d14

Concen: 90.187 ng

RT: 19.862 min Scan# 2835

Delta R.T. -0.000 min

Lab File: BM041279.D

Acq: 04 Aug 2023 01:45




Tgt Ion:244 Resp: 2827576


Ion Ratio Lower Upper

244 100

212 7.1 5.4 8.2

122 9.0 7.8 11.6

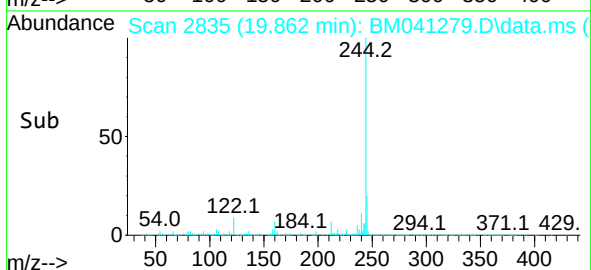



#81

Benzo(a)anthracene

Concen: 34.895 ng

RT: 21.415 min Scan# 3099

Delta R.T. -0.000 min

Lab File: BM041279.D

Acq: 04 Aug 2023 01:45

Instrument :

BNA_M

ClientSampleId :

BUILDING-B-3-(5-10)

Tgt Ion:228 Resp: 134095

Ion Ratio Lower Upper

228 100

226 32.9 22.4 33.6





229 27.1 15.8 23.8

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 08/04/2023

Supervised By :mohammad ahmed 08/04/2023

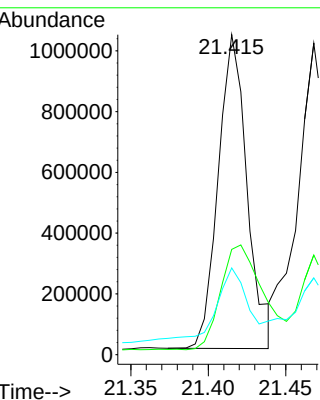

#83

Chrysene

Concen: 36.833 ng

RT: 21.468 min Scan# 3108

Delta R.T. -0.000 min

Lab File: BM041279.D

Acq: 04 Aug 2023 01:45




Tgt Ion:228 Resp: 1369102


Ion Ratio Lower Upper

228 100

226 32.0 24.5 36.7

229 24.6 15.8 23.8

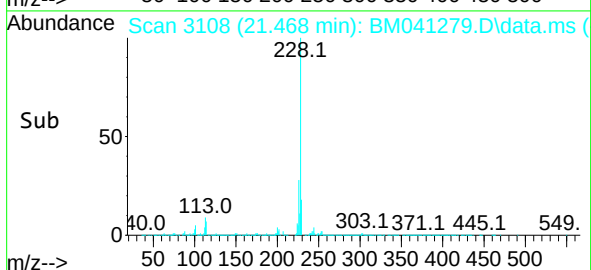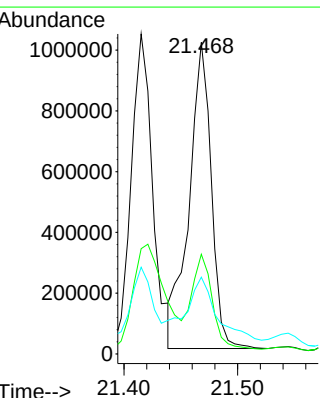



#86

Perylene-d12

Concen: 20.000 ng

RT: 23.809 min Scan# 3

Delta R.T. 0.006 min

Lab File: BM041279.D

Acq: 04 Aug 2023 01:45

Instrument :

BNA_M

ClientSampleId :

BUILDING-B-3-(5-10)





Tgt Ion:	264	Resp:	61809
Ion Ratio	Lower	Upper	
264	100		
260	23.3	18.5	27.7
265	25.1	17.4	26.0

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 08/04/2023

Supervised By :mohammad ahmed 08/04/2023



#87

Indeno(1,2,3-cd)pyrene

Concen: 10.877 ng




RT: 26.262 min Scan# 3923


Delta R.T. -0.000 min

Lab File: BM041279.D

Acq: 04 Aug 2023 01:45


Tgt Ion:	276	Resp:	494302
Ion Ratio	Lower	Upper	
276	100		
138	18.5	20.0	30.0#
277	25.8	20.1	30.1

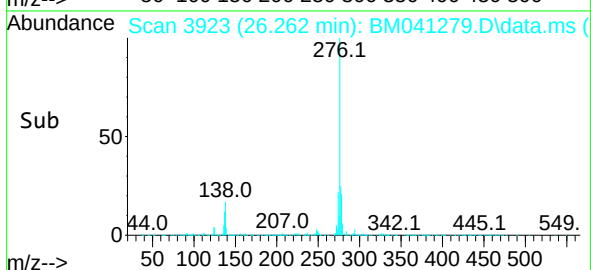



#88
Benzo(b)fluoranthene
Concen: 25.037 ng m
RT: 23.091 min Scan# 31
Delta R.T. 0.006 min
Lab File: BM041279.D
Acq: 04 Aug 2023 01:45




Instrument :
BNA_M
ClientSampleId :
BUILDING-B-3-(5-10)



Tgt Ion:252 Resp: 919324
Ion Ratio Lower Upper
252 100
253 24.1 17.7 26.5
125 10.1 8.2 12.4




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 08/04/2023
Supervised By :mohammad ahmed 08/04/2023



#89
Benzo(k)fluoranthene
Concen: 6.683 ng m
RT: 23.127 min Scan# 3390
Delta R.T. -0.006 min
Lab File: BM041279.D
Acq: 04 Aug 2023 01:45


Tgt Ion:252 Resp: 251009
Ion Ratio Lower Upper
252 100
253 27.9 17.4 26.0#
125 11.4 7.6 11.4

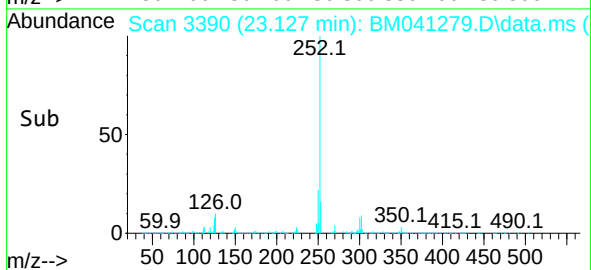



#90
Benzo(a)pyrene
Concen: 29.209 ng
RT: 23.703 min Scan# 3488
Delta R.T. 0.006 min
Lab File: BM041279.D
Acq: 04 Aug 2023 01:45




Instrument :
BNA_M
ClientSampleId :
BUILDING-B-3-(5-10)

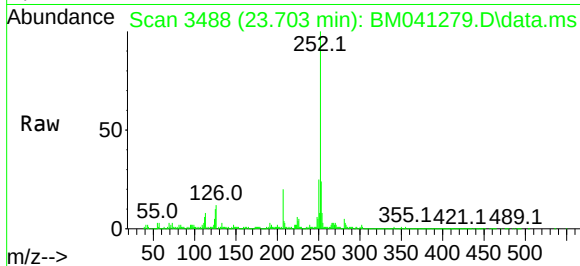


Tgt Ion:252 Resp: 103053
Ion Ratio Lower Upper
252 100
253 23.9 17.3 25.9
125 9.5 9.0 13.4

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 08/04/2023
Supervised By :mohammad ahmed 08/04/2023

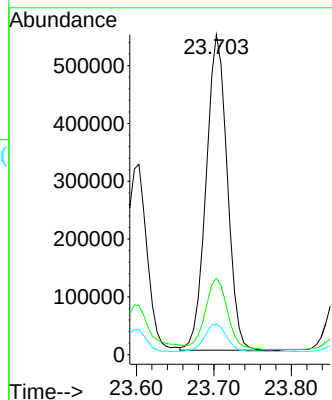


#91
Dibenzo(a,h)anthracene
Concen: 4.284 ng
RT: 26.262 min Scan# 3923
Delta R.T. -0.012 min
Lab File: BM041279.D
Acq: 04 Aug 2023 01:45

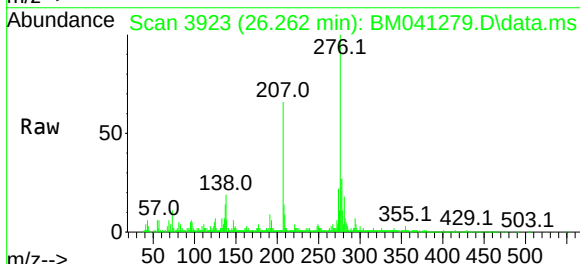


Tgt Ion:278 Resp: 162375
Ion Ratio Lower Upper
278 100
139 22.5 12.7 19.1#
279 41.4 19.1 28.7#

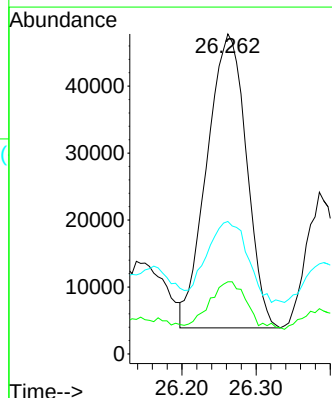



#92
Benzo(g,h,i)perylene
Concen: 16.550 ng
RT: 27.026 min Scan# 4053
Delta R.T. 0.012 min
Lab File: BM041279.D
Acq: 04 Aug 2023 01:45

Instrument :
BNA_M
ClientSampleId :
BUILDING-B-3-(5-10)

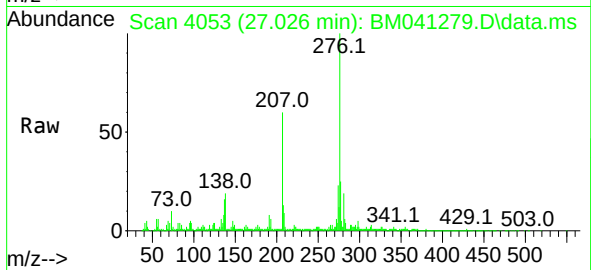

Tgt Ion:276 Resp: 613809
Ion Ratio Lower Upper
276 100
277 25.4 19.1 28.7
138 18.5 17.1 25.7

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/04/2023
Supervised By :mohammad ahmed 08/04/2023

