
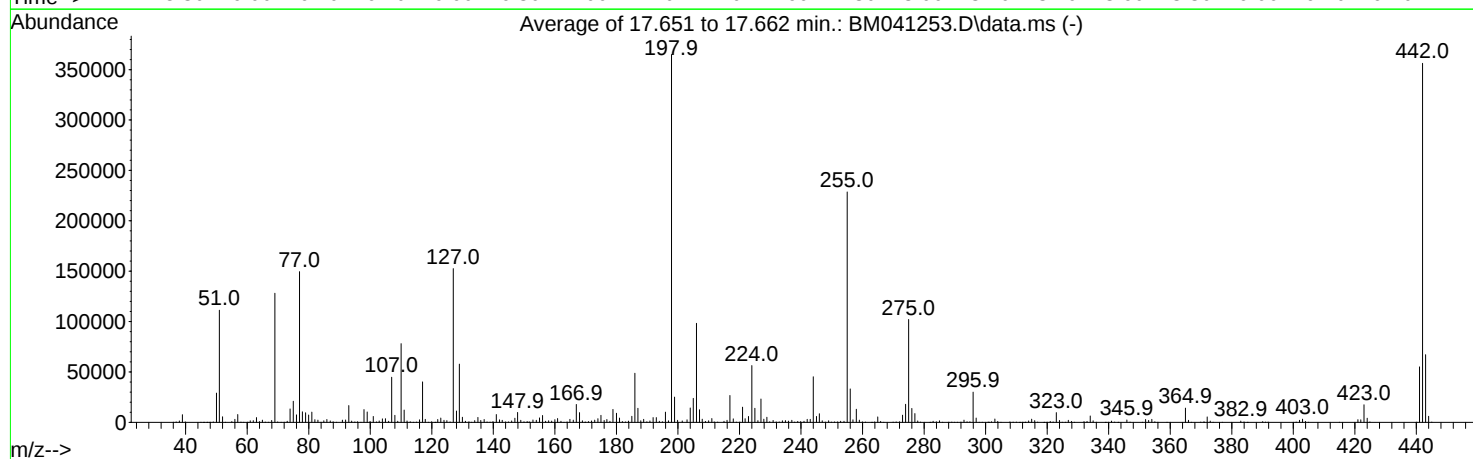


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080323\
Data File : BM041253.D
Acq On : 03 Aug 2023 08:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 02 19:20:51 2023

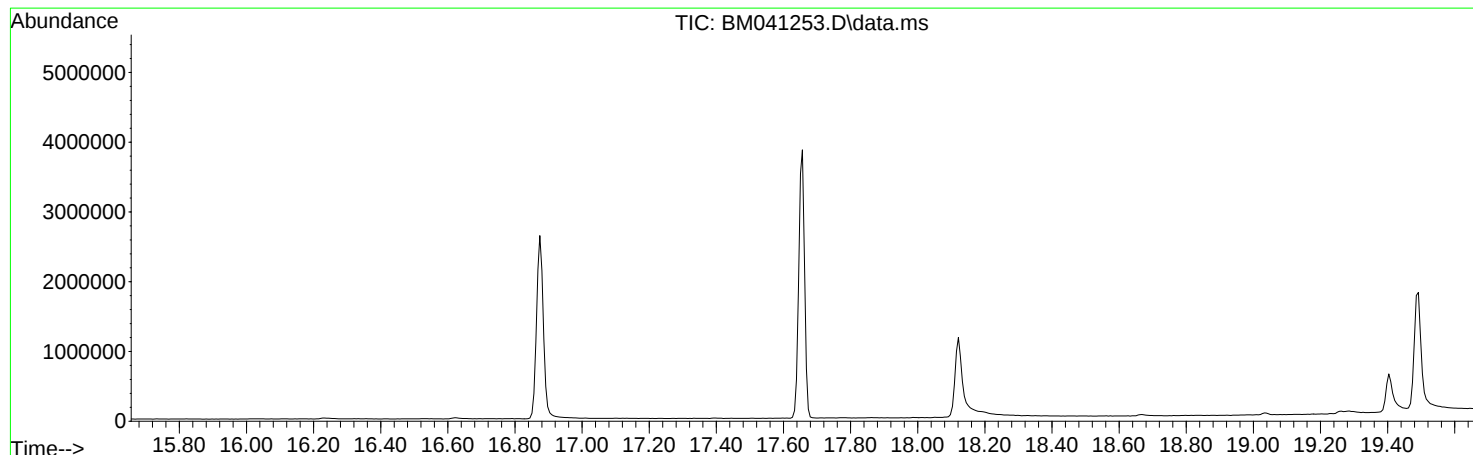




AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	111294	PASS
68	69	0.00	2	1.5	1982	PASS
69	198	0.00	100	35.1	128064	PASS
70	69	0.00	2	0.4	543	PASS
127	198	10	80	41.8	152621	PASS
197	198	0.00	2	0.4	1584	PASS
198	198	100	100	100.0	365013	PASS
199	198	5	9	6.9	25165	PASS
275	198	10	60	28.0	102149	PASS
365	198	1	100	3.9	14172	PASS
441	198	0.01	100	15.1	55149	PASS
442	442	50	100	100.0	356288	PASS
443	442	15	24	18.8	67133	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080323\
Data File : BM041253.D
Acq On : 03 Aug 2023 08:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 03 11:02:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 19:20:51 2023
Response via : Initial Calibration

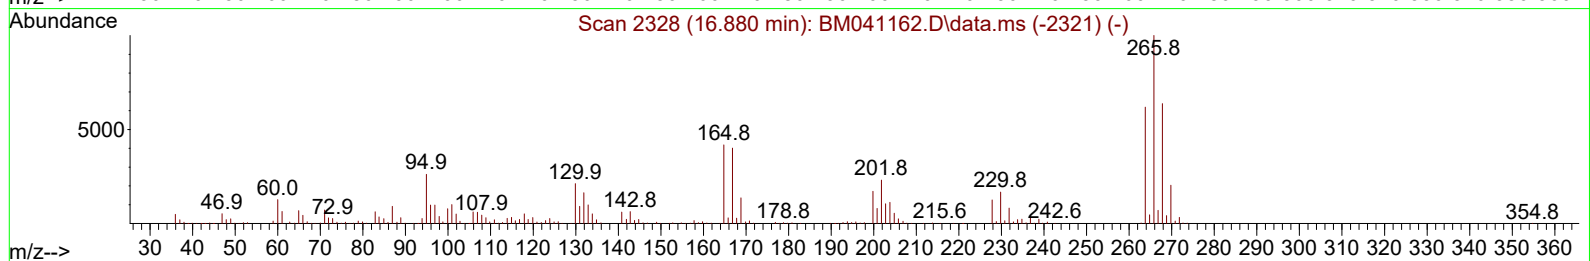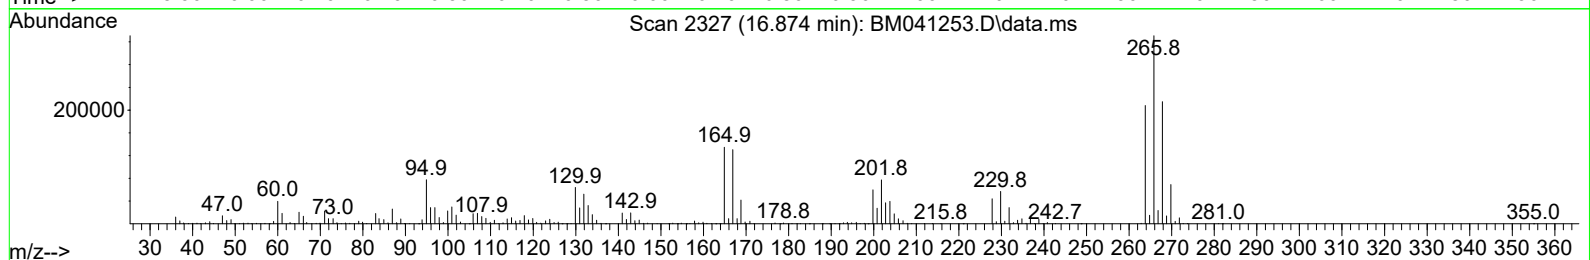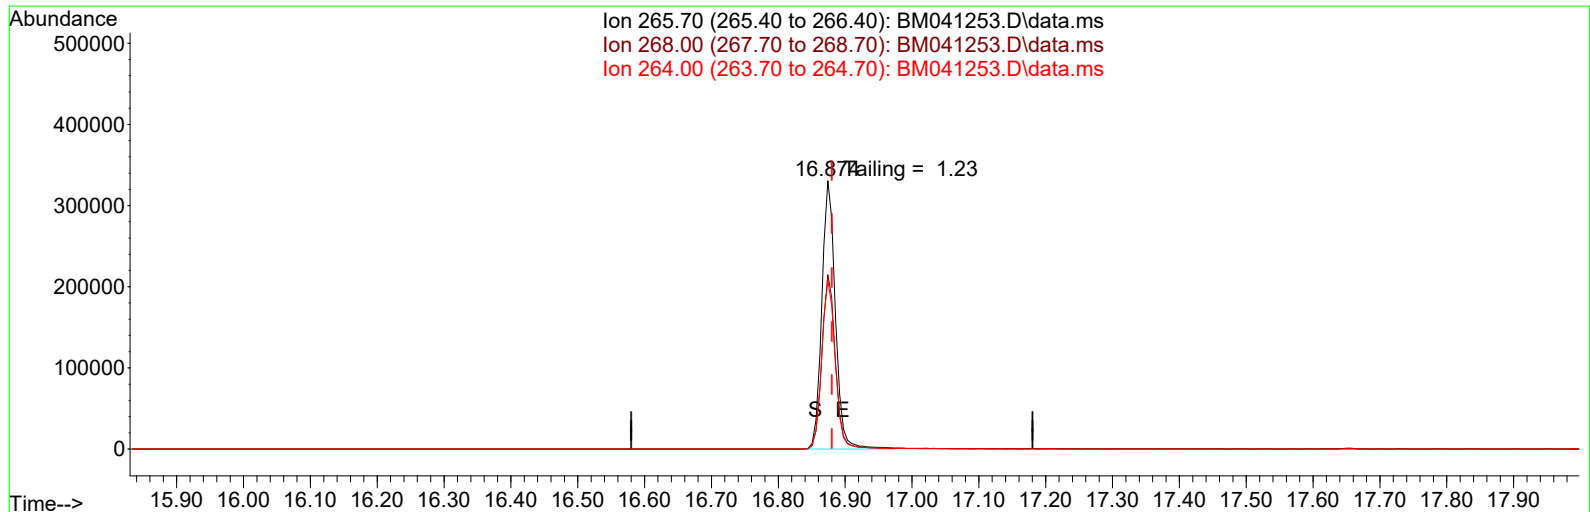

TIC: BM041253.D\data.ms

(70) Pentachlorophenol (C)

16.874min (-0.006) 0.00 ng




response 468496

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.92
264.00	61.80	62.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080323\
Data File : BM041253.D
Acq On : 03 Aug 2023 08:20
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 03 11:02:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 19:20:51 2023
Response via : Initial Calibration

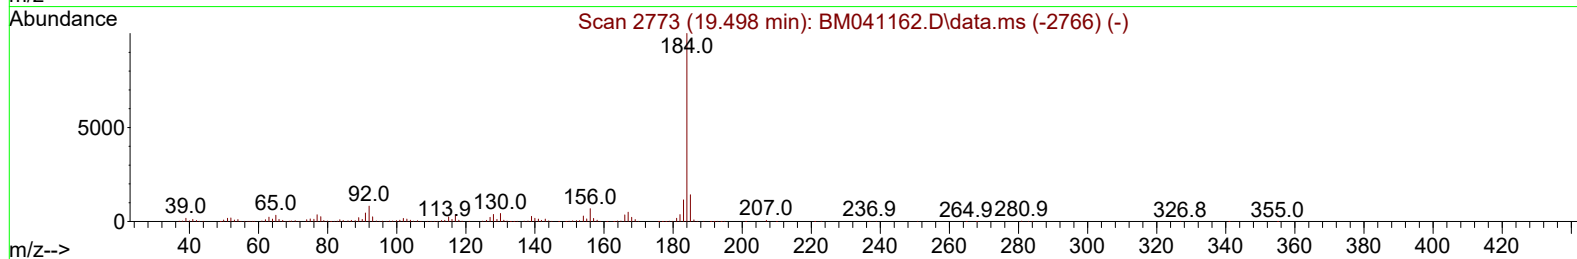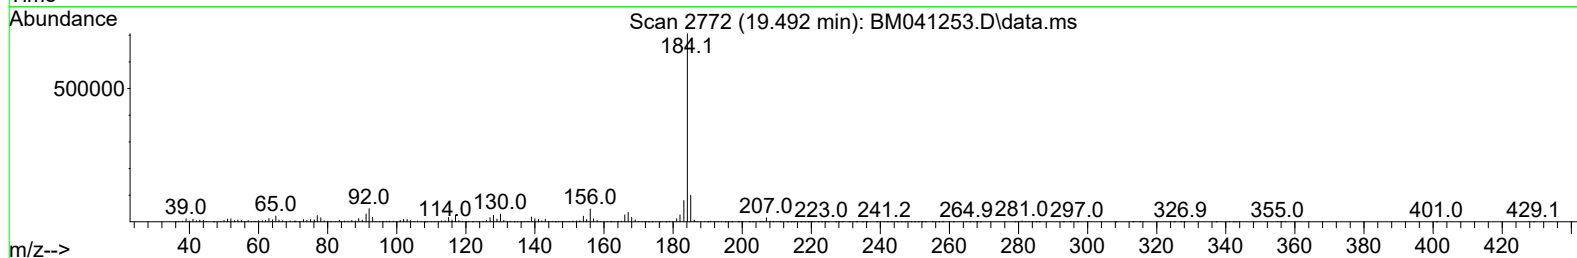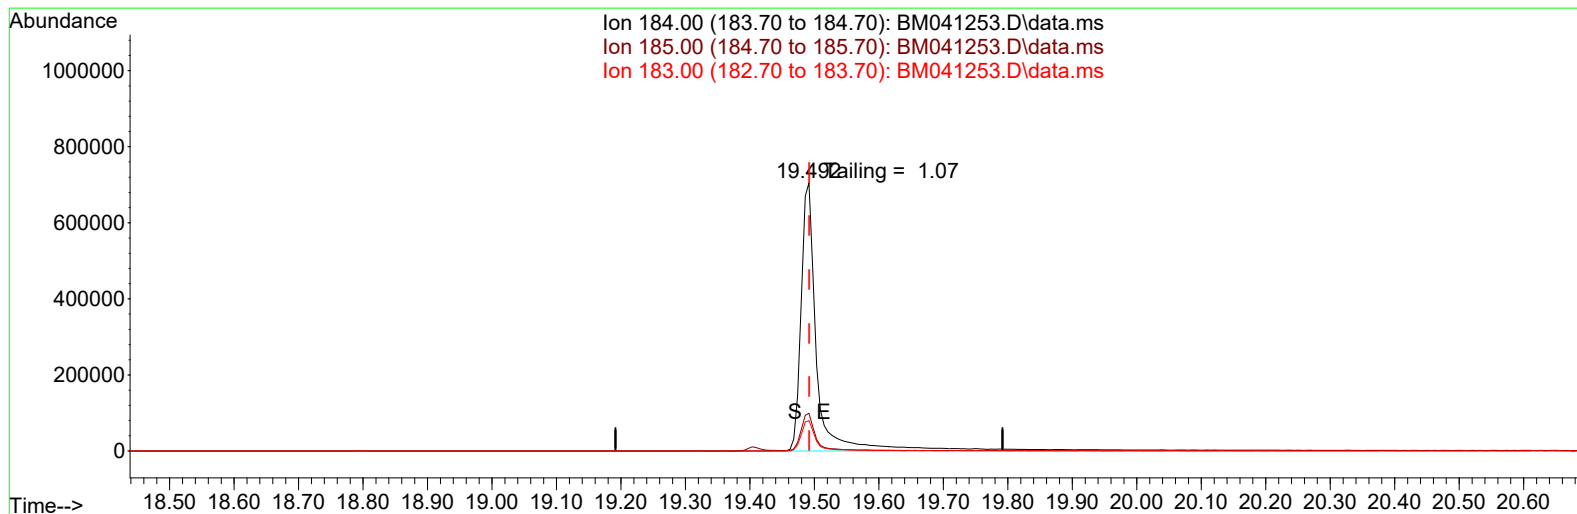

TIC: BM041253.D\data.ms

(77) Benzidine

19.492min (-0.000) 69186.33 ng

response 1168380

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.07
183.00	11.50	11.32
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/3/2023	BNA_M	<u>BM041253.D</u>
Compound Name	Response	Retention Time
DDT	1175542	20.715
DDD	29052	20.274
DDE	1545	19.756
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30597	1206139	2.54

Instrument :
BNA_M
ClientSampleId :
DFTPP