


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080323\
Data File : BM041261.D
Acq On : 03 Aug 2023 14:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 02 19:20:51 2023

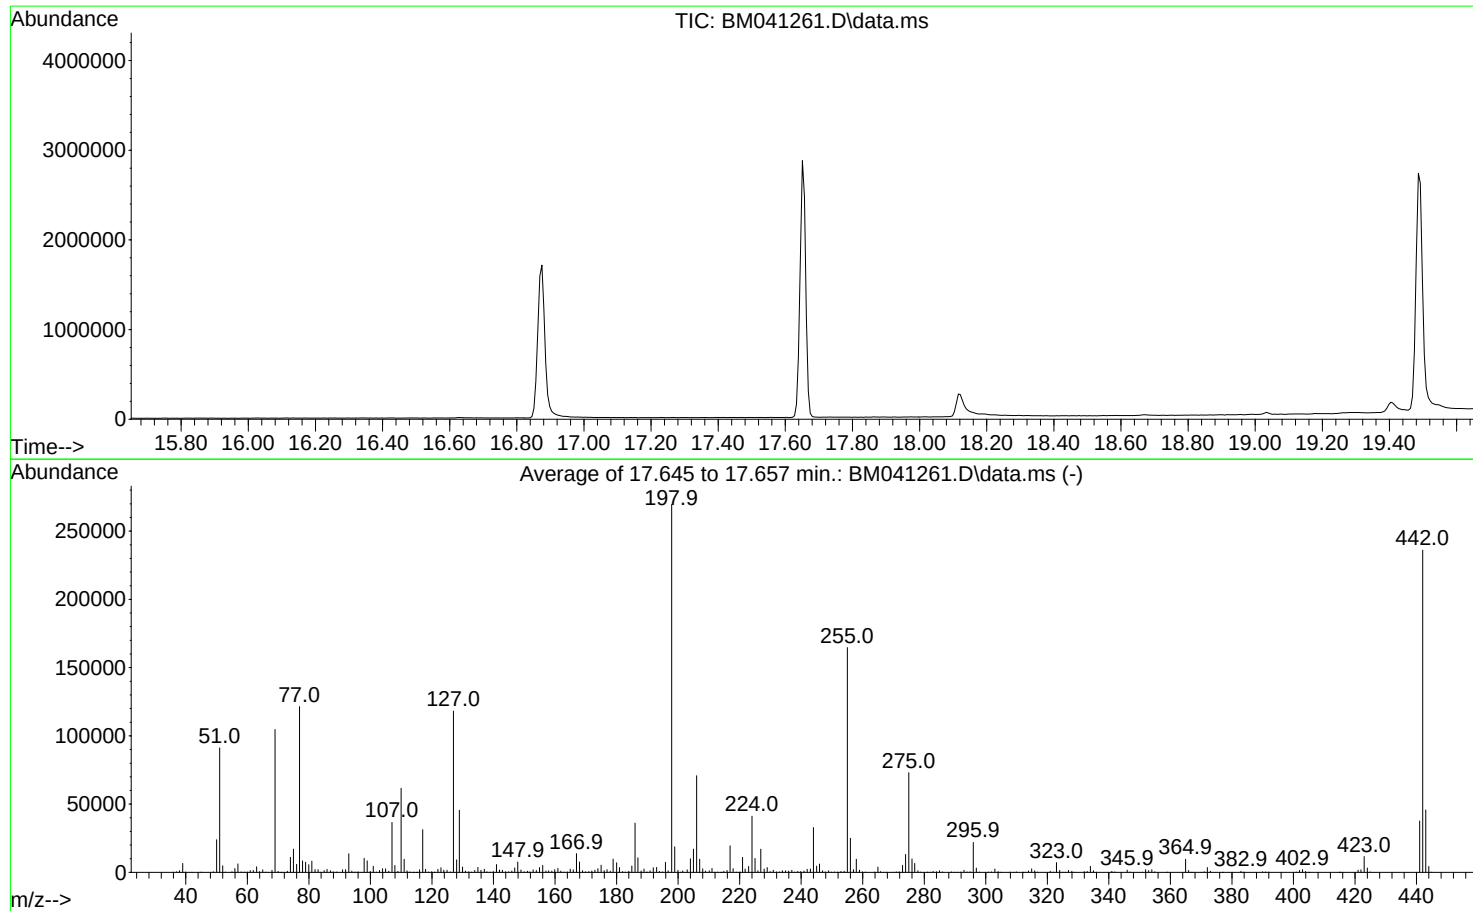




AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	91242	PASS
68	69	0.00	2	1.5	1592	PASS
69	198	0.00	100	38.9	104730	PASS
70	69	0.00	2	0.7	681	PASS
127	198	10	80	43.8	118163	PASS
197	198	0.00	2	0.4	1197	PASS
198	198	100	100	100.0	269504	PASS
199	198	5	9	7.0	18827	PASS
275	198	10	60	27.1	73008	PASS
365	198	1	100	3.6	9616	PASS
441	198	0.01	100	14.0	37664	PASS
442	442	50	100	100.0	236032	PASS
443	442	15	24	19.4	45709	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080323\
 Data File : BM041261.D
 Acq On : 03 Aug 2023 14:25
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 03 14:56:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 02 19:20:51 2023
 Response via : Initial Calibration

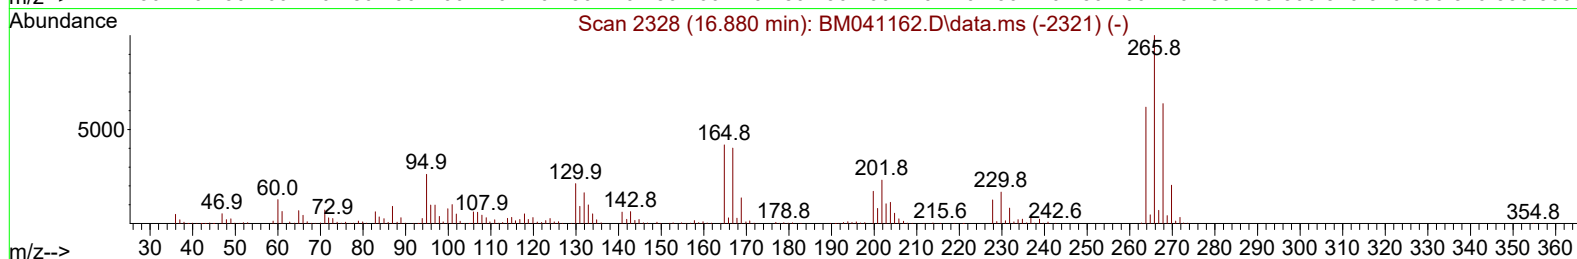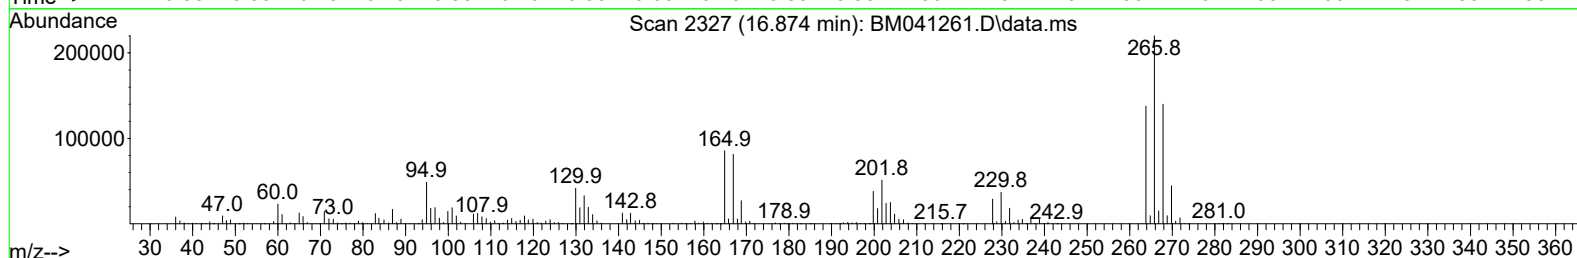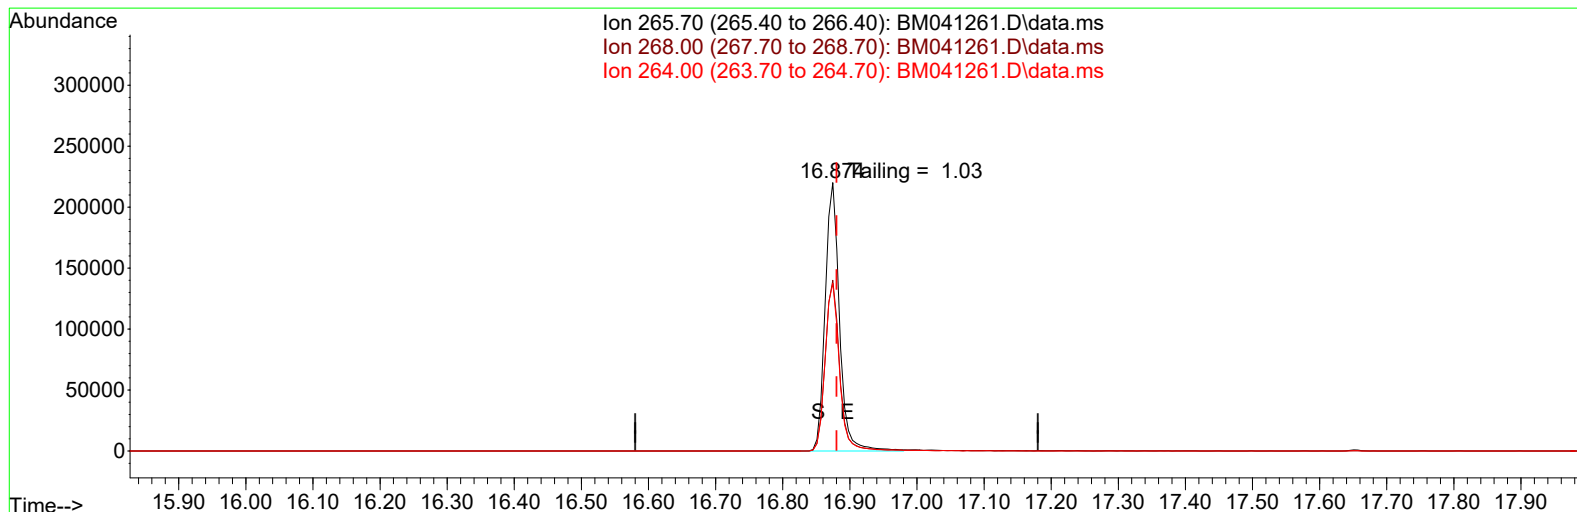

TIC: BM041261.D\data.ms

(70) Pentachlorophenol (C)

16.874min (-0.006) 0.00 ng




response 325977

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.59
264.00	61.80	62.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080323\
Data File : BM041261.D
Acq On : 03 Aug 2023 14:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 03 14:56:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 19:20:51 2023
Response via : Initial Calibration

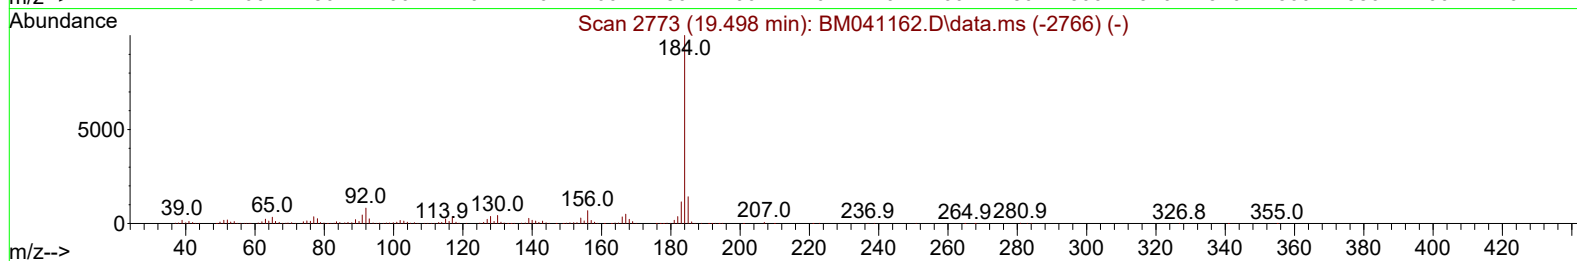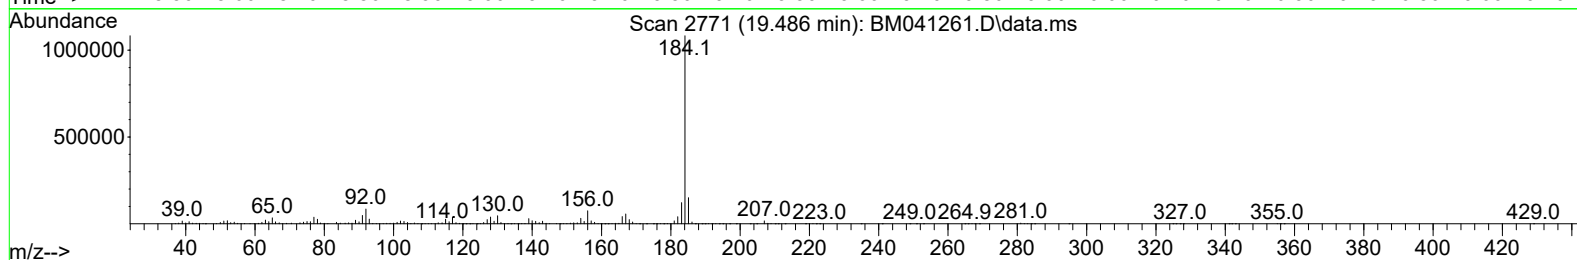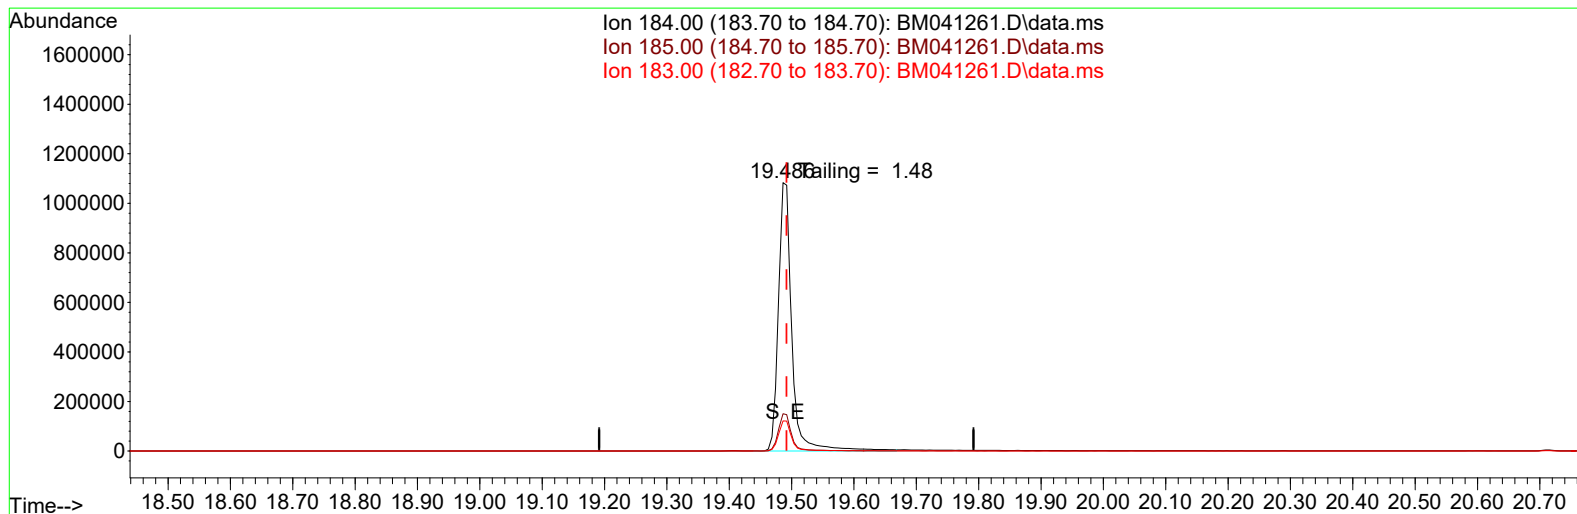

TIC: BM041261.D\data.ms

(77) Benzidine

19.486min (-0.006) 99987.84 ng

response 1639477

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.93
183.00	11.50	11.25
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/3/2023	BNA_M	<u>BM041261.D</u>
Compound Name	Response	Retention Time
DDT	950513	20.715
DDD	21261	20.274
DDE	1290	19.757
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22551	973064	2.32

Instrument :
BNA_M
ClientSampleId :
DFTPP