
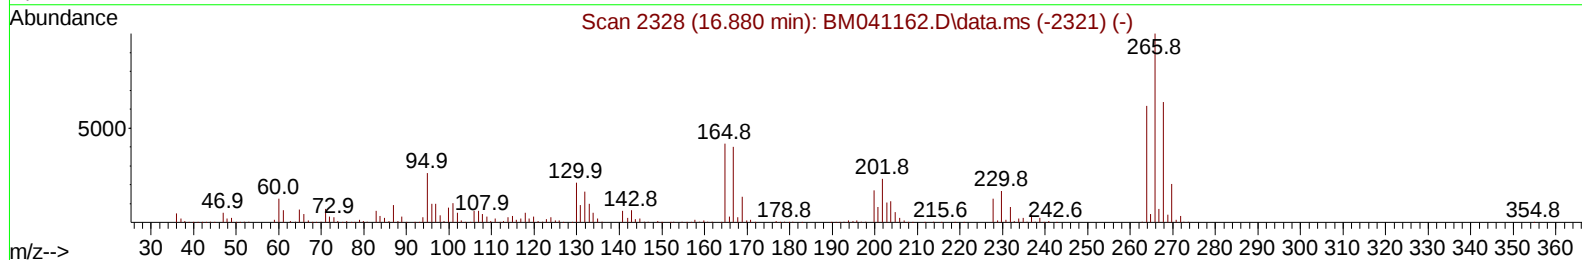
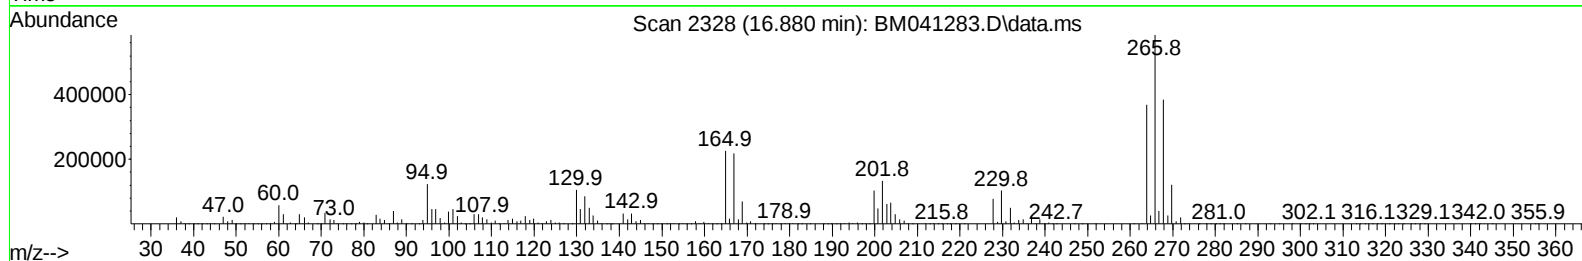


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080423\
Data File : BM041283.D
Acq On : 04 Aug 2023 08:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 04 17:24:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 19:20:51 2023
Response via : Initial Calibration

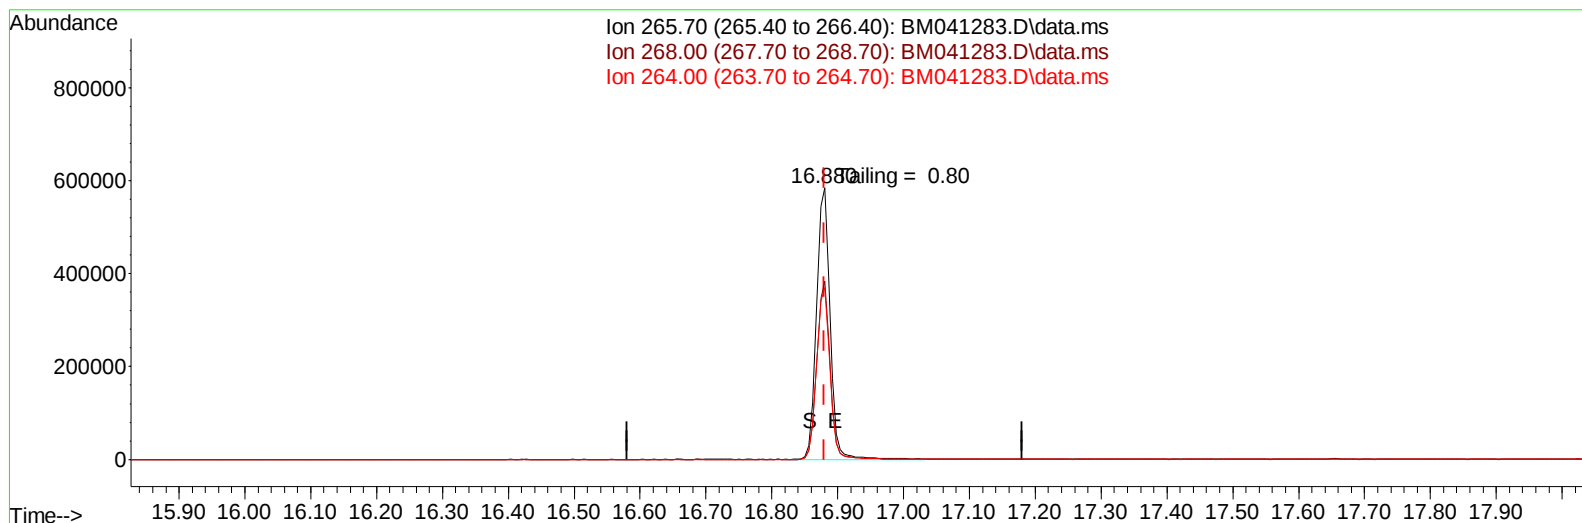

TIC: BM041283.D\data.ms

(70) Pentachlorophenol (C)




16.880min (-0.000) 362559.08 ng

response 823360

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	65.69
264.00	61.80	63.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080423\
Data File : BM041283.D
Acq On : 04 Aug 2023 08:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 04 17:24:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP.BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 19:20:51 2023
Response via : Initial Calibration

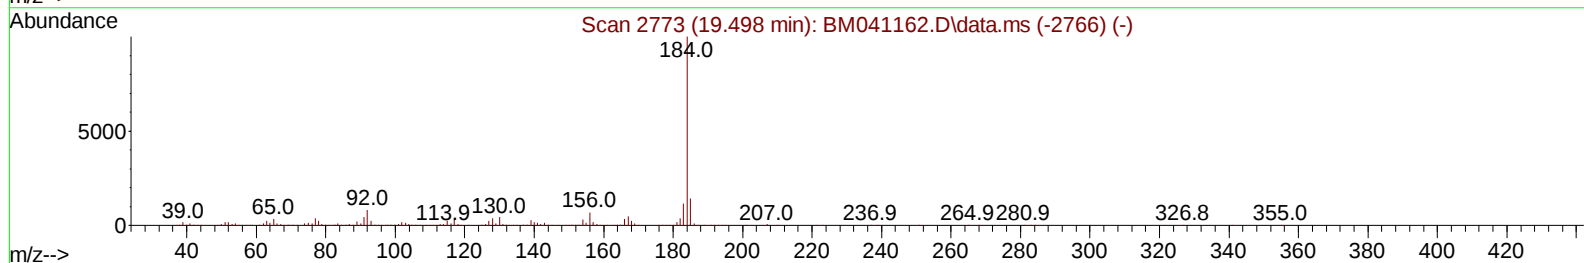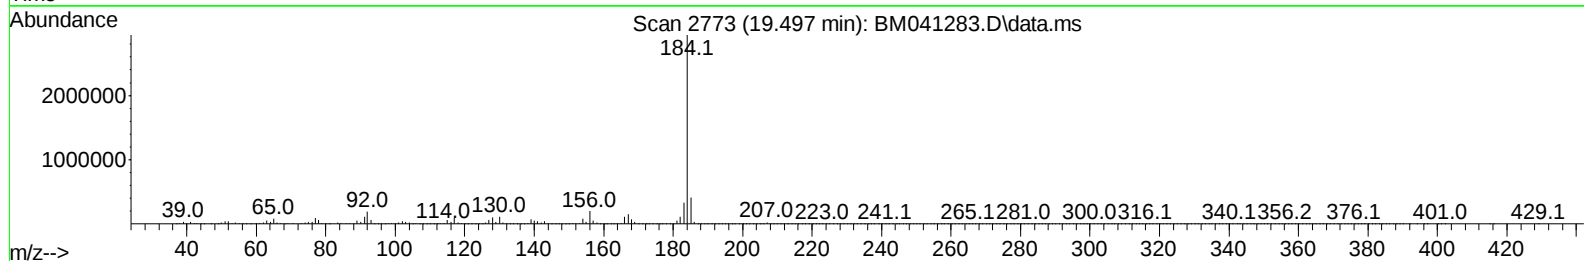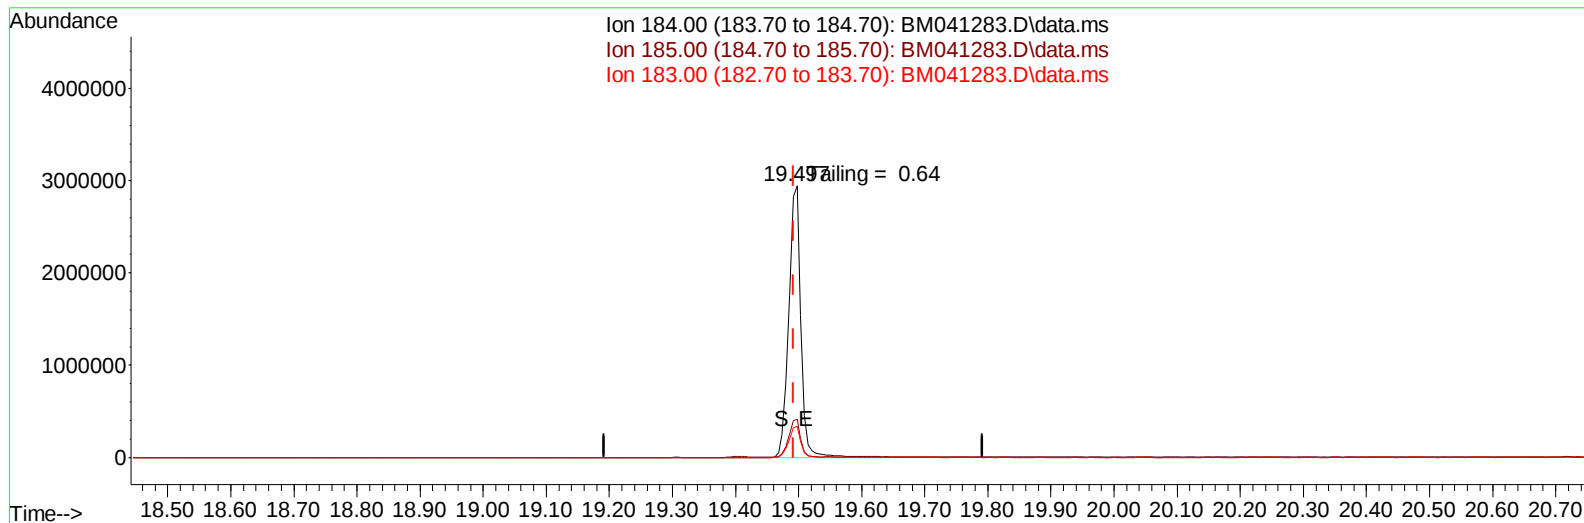

TIC: BM041283.D\data.ms

(77) Benzidine**19.497min (+ 0.006) 255853.83 ng****response 3971990**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.98
183.00	11.50	11.36
0.00	0.00	0.00