


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080423\
Data File : BM041283.D
Acq On : 04 Aug 2023 08:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 02 19:20:51 2023

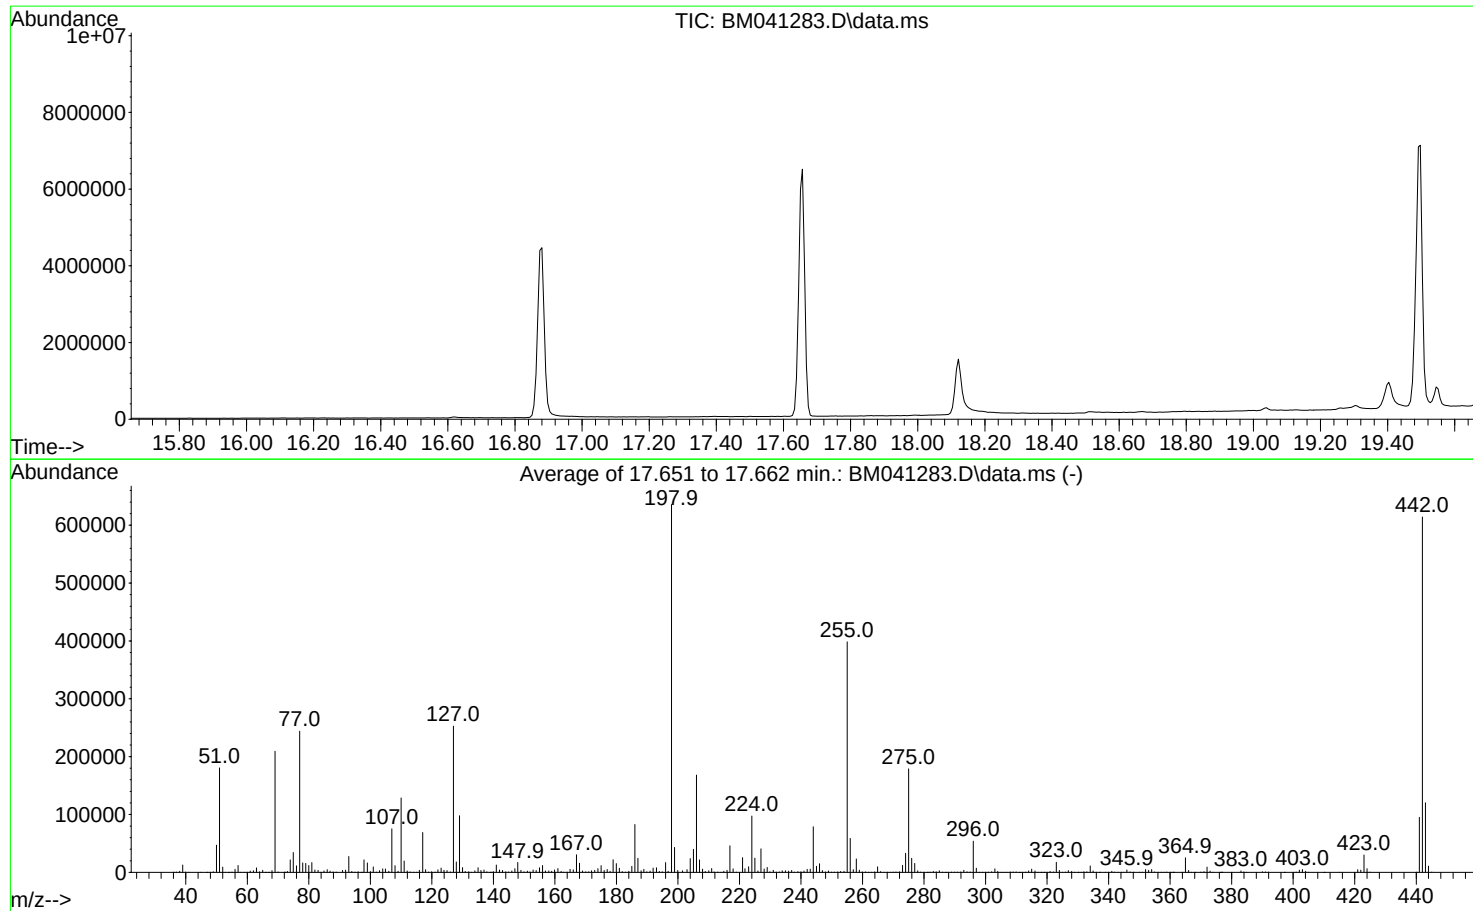




AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.4	180675	PASS
68	69	0.00	2	1.5	3047	PASS
69	198	0.00	100	32.9	209288	PASS
70	69	0.00	2	0.4	902	PASS
127	198	10	80	39.8	252800	PASS
197	198	0.00	2	0.3	2042	PASS
198	198	100	100	100.0	635776	PASS
199	198	5	9	6.8	43085	PASS
275	198	10	60	28.1	178901	PASS
365	198	1	100	4.0	25235	PASS
441	198	0.01	100	15.0	95285	PASS
442	442	50	100	100.0	614080	PASS
443	442	15	24	19.6	120397	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080423\
Data File : BM041283.D
Acq On : 04 Aug 2023 08:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 04 17:24:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 19:20:51 2023
Response via : Initial Calibration

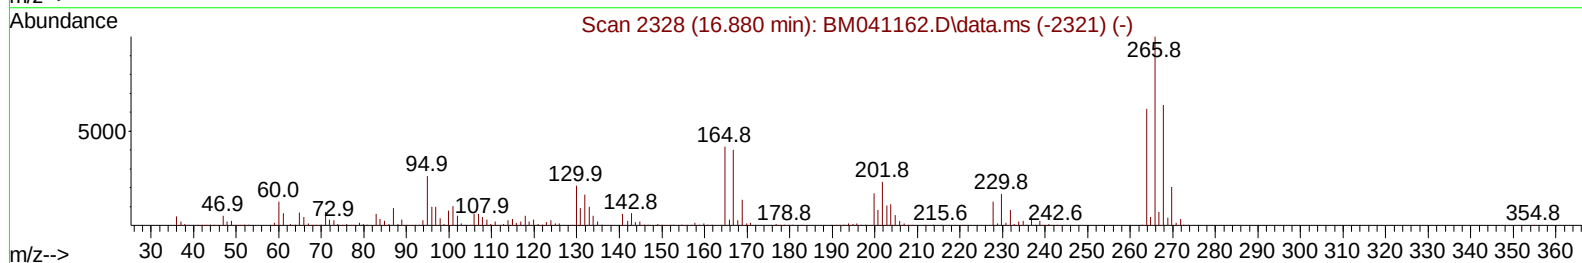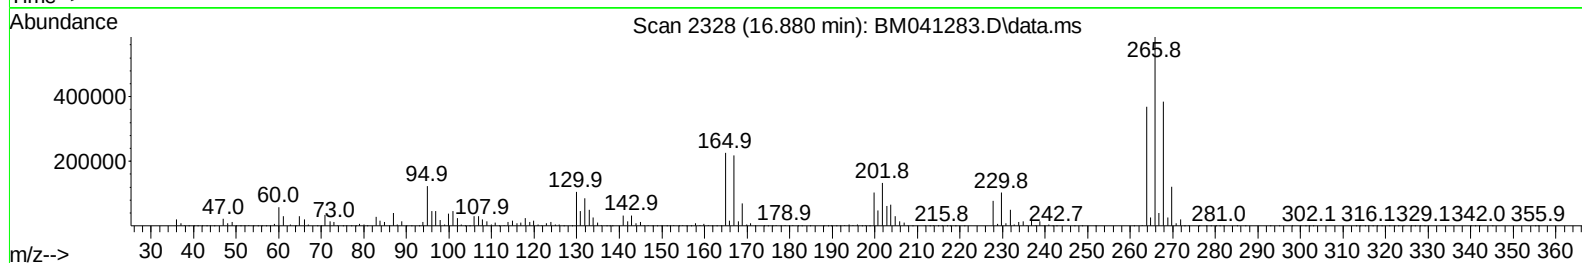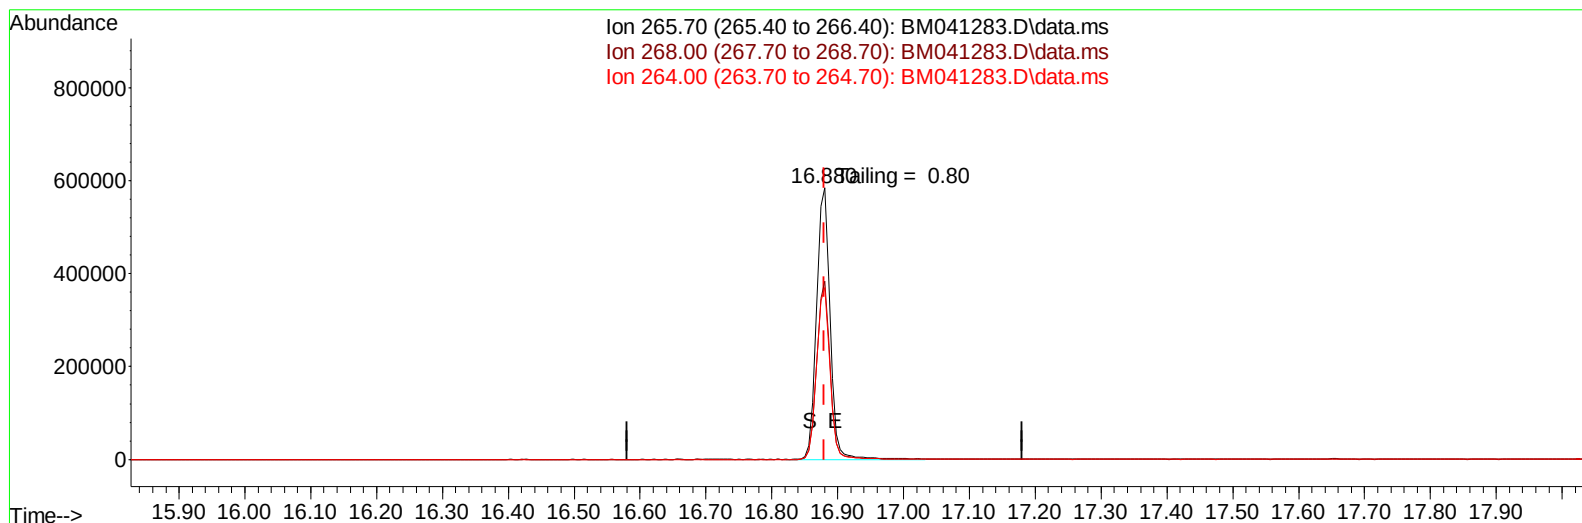

TIC: BM041283.D\data.ms

(70) Pentachlorophenol (C)

16.880min (-0.000) 362559.08 ng




response 823360

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	65.69
264.00	61.80	63.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080423\
Data File : BM041283.D
Acq On : 04 Aug 2023 08:05
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 04 17:24:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP.BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 19:20:51 2023
Response via : Initial Calibration

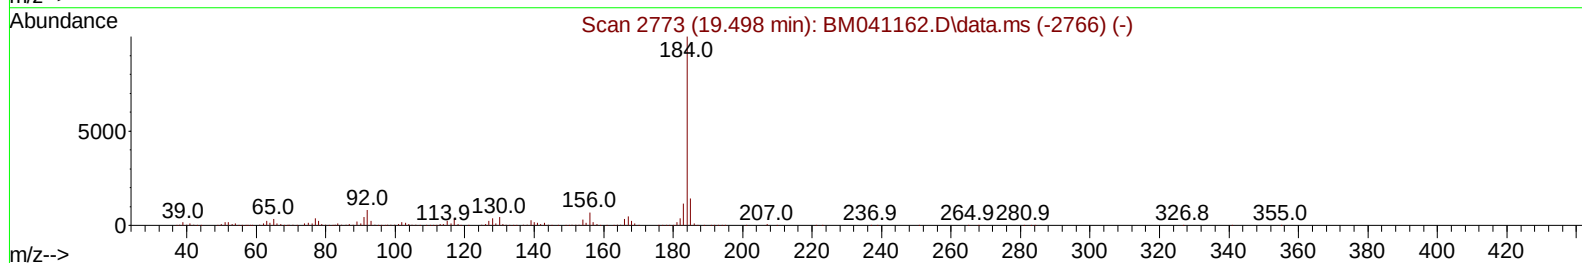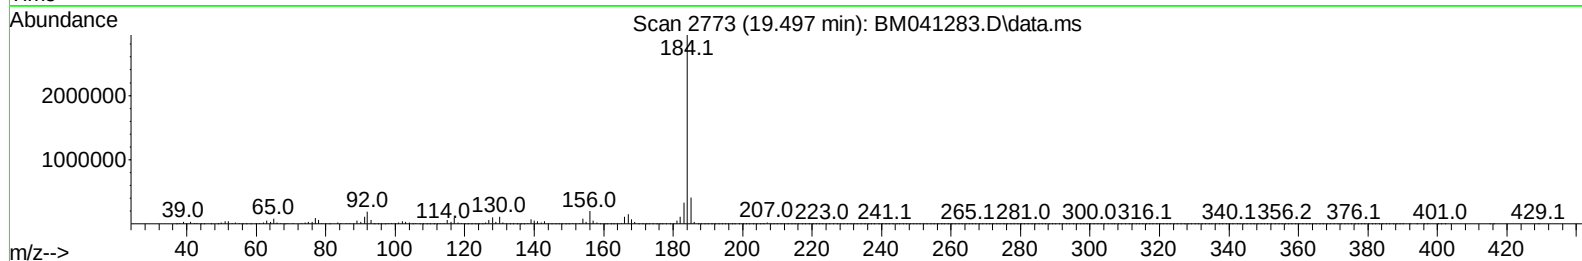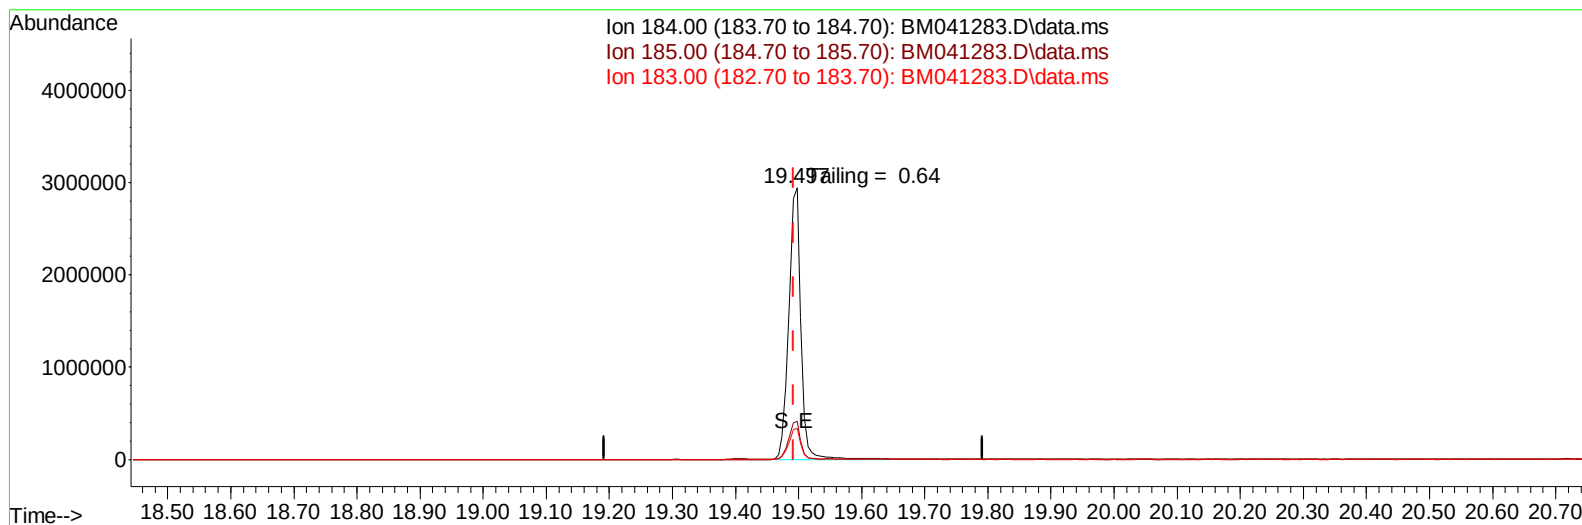

TIC: BM041283.D\data.ms

(77) Benzidine

19.497min (+ 0.006) 255853.83 ng

response 3971990

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.98
183.00	11.50	11.36
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/4/2023	BNA_M	<u>BM041283.D</u>
Compound Name	Response	Retention Time
DDT	2247667	20.715
DDD	58435	20.28
DDE	3358	19.762
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
61793	2309460	2.68

Instrument :
BNA_M
ClientSampleId :
DFTPP