


Data Path : Z:\HPCHEM1\BNA_M\Data\BM080515\
Data File : BM002234.D
Acq On : 05 Aug 2015 13:40
Operator : TP/UM
Sample : DFTPP90
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP90

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM080415.M
Title : SVOA CALIBRATION
Last Update : Thu Aug 06 01:44:45 2015

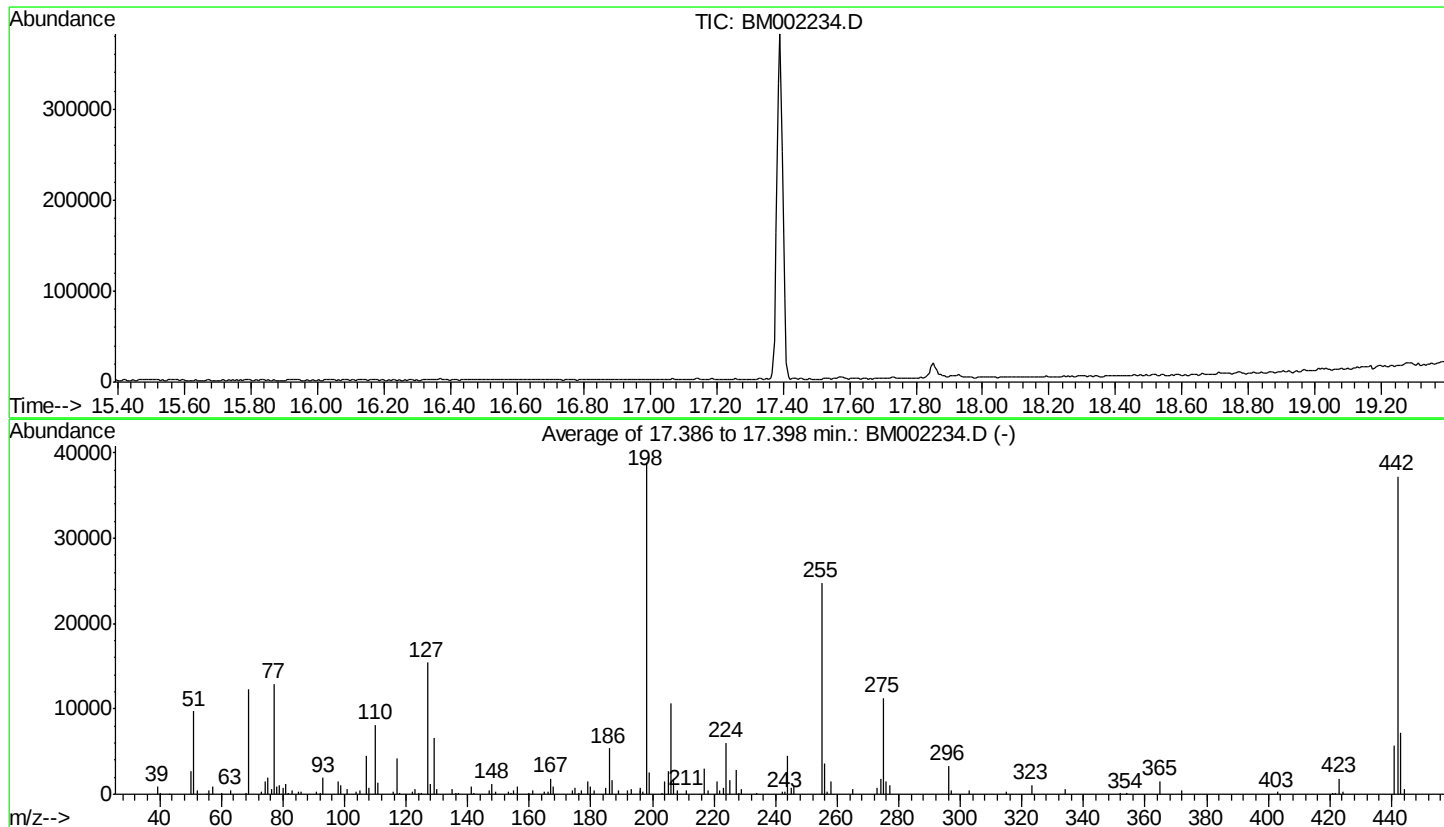

AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.9	9687	PASS
68	69	0.00	2	1.0	128	PASS
69	198	0.00	100	31.7	12319	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.6	15376	PASS
197	198	0.00	2	0.9	335	PASS
198	198	100	100	100.0	38845	PASS
199	198	5	9	6.5	2522	PASS
275	198	10	60	29.0	11284	PASS
365	198	1	100	4.0	1535	PASS
441	443	0.01	100	78.5	5639	PASS
442	198	50	100	95.8	37229	PASS
443	442	15	24	19.3	7181	PASS

m/z	Abundance
41.00	417.0
43.10	965.0
44.00	485.0
45.00	683.0
55.10	357.0
60.00	380.0

Instrument :
BNA_M
ClientSampleId :
DFTPP90

m/z	Abundance
39.10	901.0
41.00	458.0
43.00	975.0
44.00	397.0
45.00	597.0
50.00	3065.0
51.10	12303.0
52.10	615.0
55.00	370.0
56.00	461.0
57.00	1033.0
60.00	528.0
63.00	531.0
69.00	14629.0
73.00	403.0
74.00	1579.0
75.00	2313.0
76.10	883.0
77.10	15016.0
78.10	1006.0
79.00	1267.0
80.00	1015.0
81.00	1511.0
81.90	344.0
83.10	453.0
85.00	414.0
85.90	438.0
90.90	331.0
91.90	320.0
93.00	2043.0
98.00	1645.0
98.90	1114.0
100.90	627.0
103.90	485.0
105.10	522.0
107.00	5273.0
108.00	774.0
110.00	9396.0
111.00	1518.0
115.90	339.0
117.00	4997.0
121.90	329.0
123.00	713.0
124.00	343.0
125.00	356.0
127.00	17200.0
128.00	1473.0
129.00	7344.0
130.00	583.0
135.00	661.0
136.00	321.0
141.00	1135.0
141.90	380.0
147.00	621.0
148.00	1249.0
149.10	379.0
153.00	311.0
154.90	472.0
156.00	910.0
159.90	326.0
160.90	588.0
165.00	418.0
166.00	367.0
167.00	2202.0
168.00	1027.0
173.90	318.0
175.00	944.0
175.90	346.0
176.90	479.0
179.00	1515.0
180.00	904.0
181.00	490.0
185.00	906.0
186.00	5386.0
187.00	1699.0
189.00	455.0
191.90	437.0
193.00	712.0
195.90	1149.0
197.10	348.0
198.00	39328.0
198.90	2778.0
204.00	1552.0
205.00	2598.0
206.00	10883.0
207.00	1774.0
208.00	494.0
211.10	360.0
217.00	2940.0
218.00	487.0
221.00	1496.0

Instrument :
BNA_M
ClientSampleId :
DFTPP90

221.80	496.0
223.00	719.0
224.00	5869.0
225.00	1666.0
227.00	2986.0
228.90	634.0
242.00	311.0
243.10	376.0
244.00	4581.0
245.00	665.0
246.00	818.0
255.00	23928.0
256.00	3595.0
256.90	383.0
257.90	1264.0
264.90	490.0
273.00	515.0
274.00	1841.0
275.00	10498.0
276.00	1458.0
277.00	1025.0
296.00	3172.0
297.10	419.0
302.90	460.0
314.90	358.0
323.10	901.0
334.00	475.0
353.90	312.0
364.90	1330.0
372.00	470.0
423.10	1352.0
441.10	5062.0
442.10	30080.0
443.00	5734.0
444.10	460.0

Instrument :
BNA_M
ClientSampleId :
DFTPP90

m/z	Abundance
39.10	996.0
40.00	311.0
41.00	410.0
43.00	1087.0
44.00	555.0
45.00	684.0
50.10	3137.0
51.10	10672.0
52.00	498.0
55.00	374.0
56.00	481.0
57.00	883.0
60.00	487.0
63.00	598.0
68.10	386.0
69.00	14108.0
73.10	318.0
74.10	1747.0
75.00	2278.0
76.10	739.0
77.10	15032.0
78.00	987.0
79.00	1302.0
80.00	842.0
81.00	1363.0
83.00	391.0
85.00	356.0
85.90	421.0
91.00	366.0
91.90	360.0
93.00	2379.0
98.00	1724.0
98.90	1157.0
101.00	742.0
103.90	488.0
104.90	543.0
107.00	5004.0
107.90	873.0
110.00	9485.0
111.00	1428.0
116.00	361.0
117.00	5032.0
118.00	365.0
122.00	536.0
122.90	788.0
127.00	18072.0
128.00	1322.0
129.00	7896.0
130.00	744.0
135.00	670.0
136.90	427.0
141.00	887.0
146.90	449.0
148.00	1551.0
148.90	333.0
153.00	303.0
153.90	322.0
155.00	570.0
156.00	997.0
160.00	327.0
160.90	562.0
165.00	504.0
165.90	463.0
167.10	1914.0
167.90	1062.0
173.90	490.0
175.00	903.0
177.00	490.0
179.00	1672.0
180.00	1139.0
180.90	509.0
185.00	901.0
186.00	6623.0
187.00	1847.0
188.90	479.0
191.90	576.0
192.90	571.0
196.10	1493.0
197.00	338.0
197.90	46832.0
198.90	2904.0
203.00	312.0
204.00	1713.0
205.10	3295.0
206.00	13079.0
207.00	2189.0
207.90	546.0
211.00	480.0
216.90	3791.0
218.00	461.0
220.90	2012.0

Instrument :
BNA_M
ClientSampleId :
DFTPP90

221.80	494.0
223.00	807.0
224.00	7437.0
225.00	1893.0
227.00	3402.0
228.10	395.0
229.00	681.0
233.90	329.0
242.00	490.0
243.00	454.0
244.00	5529.0
245.00	893.0
246.00	1147.0
255.00	29544.0
256.00	4245.0
256.90	342.0
258.00	1801.0
265.00	697.0
272.90	967.0
274.00	2134.0
275.00	13325.0
276.00	1999.0
276.90	1227.0
296.00	3956.0
296.90	498.0
303.00	580.0
315.00	395.0
323.10	1364.0
334.10	808.0
354.10	451.0
365.00	1793.0
372.00	616.0
403.00	371.0
421.00	319.0
421.80	371.0
423.10	2156.0
424.00	441.0
441.00	6598.0
442.10	43976.0
443.10	8580.0
444.10	861.0

Instrument :
BNA_M
ClientSampleId :
DFTPP90

m/z	Abundance
39.00	623.0
43.00	1002.0
43.90	425.0
45.00	610.0
50.10	1952.0
51.00	6087.0
52.00	439.0
55.00	373.0
56.00	362.0
57.00	675.0
60.00	473.0
63.00	340.0
69.00	8221.0
74.00	1070.0
75.00	1364.0
76.00	390.0
77.10	8754.0
78.00	576.0
78.90	751.0
79.90	449.0
81.00	954.0
83.00	301.0
93.00	1329.0
98.00	1015.0
98.90	752.0
100.90	383.0
105.00	443.0
107.00	3150.0
107.90	578.0
110.00	5550.0
111.00	914.0
117.00	2555.0
122.90	482.0
127.00	10856.0
128.00	708.0
129.00	4549.0
130.00	364.0
134.90	595.0
141.00	770.0
146.90	377.0
148.00	997.0
148.90	320.0
153.00	344.0
155.00	427.0
156.00	587.0
161.00	414.0
167.00	1379.0
168.00	584.0
174.00	367.0
174.90	539.0
176.90	465.0
178.90	1339.0
179.90	728.0
181.00	334.0
185.10	522.0
186.00	3995.0
187.00	1296.0
189.00	347.0
191.90	472.0
193.00	462.0
196.00	969.0
197.10	320.0
197.90	30376.0
198.90	1885.0
204.00	1283.0
205.00	2122.0
206.00	7901.0
207.00	1392.0
207.90	300.0
211.00	366.0
217.00	2276.0
217.90	392.0
221.00	1227.0
221.80	312.0
223.00	557.0
224.00	4720.0
225.00	1333.0
227.00	2343.0
229.00	485.0
244.00	3605.0
245.00	503.0
245.90	878.0
255.00	20760.0
256.00	2824.0
256.90	313.0
258.00	1248.0
264.90	609.0
273.00	734.0
274.00	1521.0
275.00	10030.0
276.00	1100.0

Instrument :
BNA_M
ClientSampleId :
DFTPP90

277.00	962.0
296.00	2938.0
297.00	393.0
303.00	325.0
323.00	932.0
333.90	499.0
352.00	311.0
365.00	1484.0
372.10	488.0
403.00	373.0
423.00	1913.0
424.10	346.0
441.00	5258.0
442.10	37632.0
443.00	7230.0
444.00	524.0

Instrument :
BNA_M
ClientSampleId :
DFTPP90