
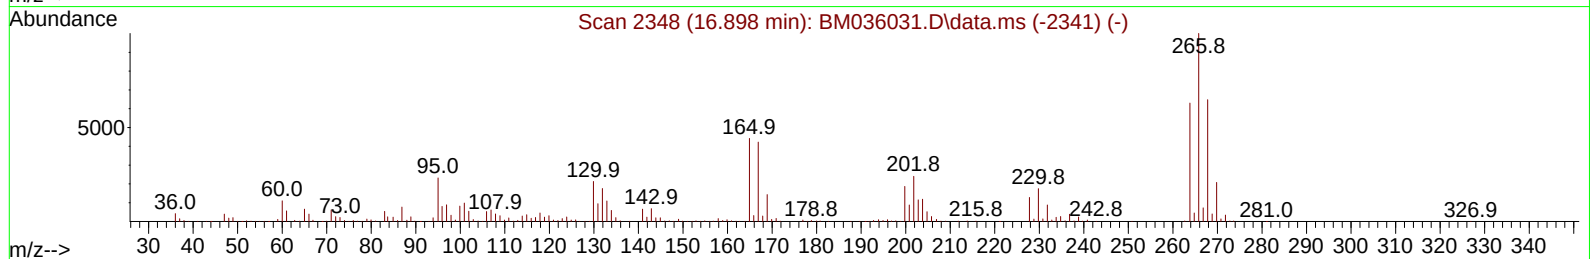
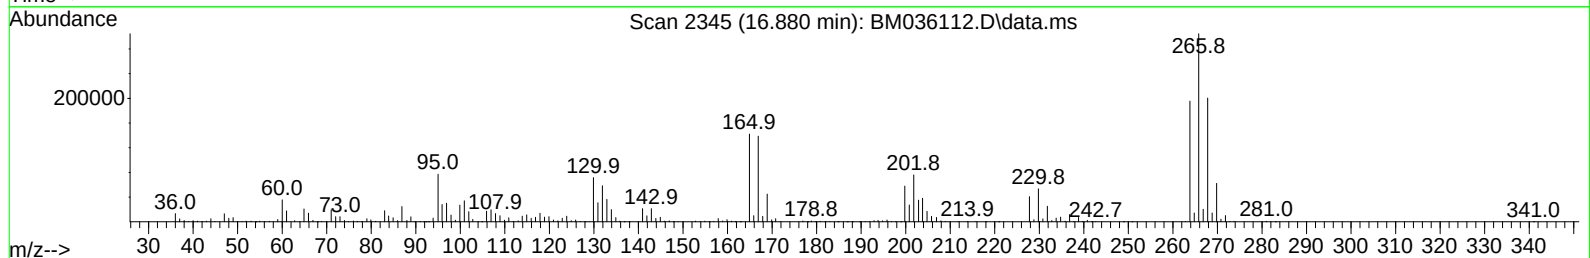


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080522\
 Data File : BM036112.D
 Acq On : 05 Aug 2022 10:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 06:56:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 05 03:36:25 2022
 Response via : Initial Calibration

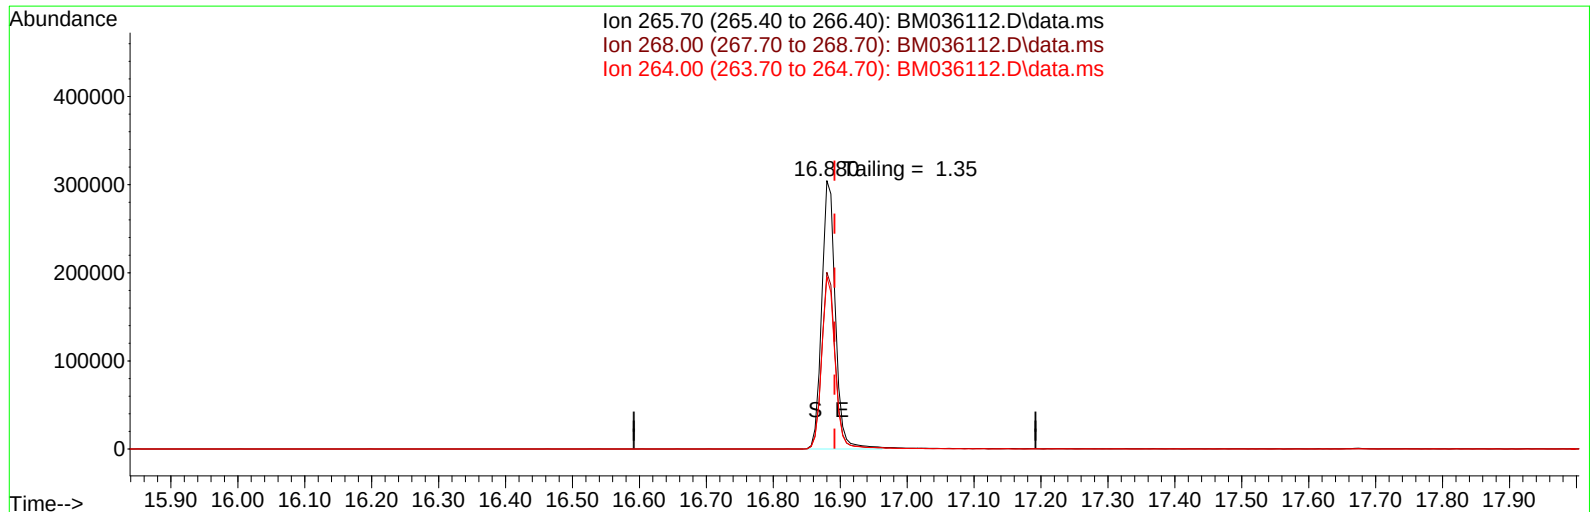

TIC: BM036112.D\data.ms

(70) Pentachlorophenol (C)




16.880min (-0.012) 276308.14 ng

response 434592

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	65.81
264.00	63.30	64.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080522\
Data File : BM036112.D
Acq On : 05 Aug 2022 10:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 06:56:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 05 03:36:25 2022
Response via : Initial Calibration

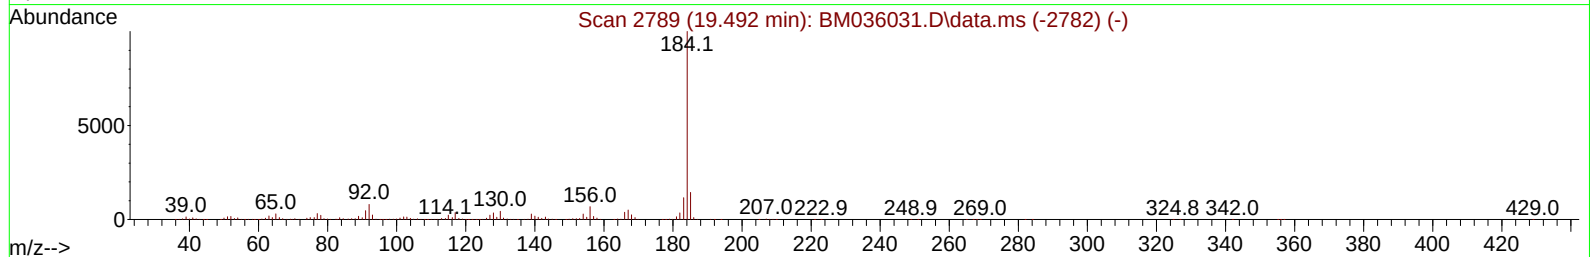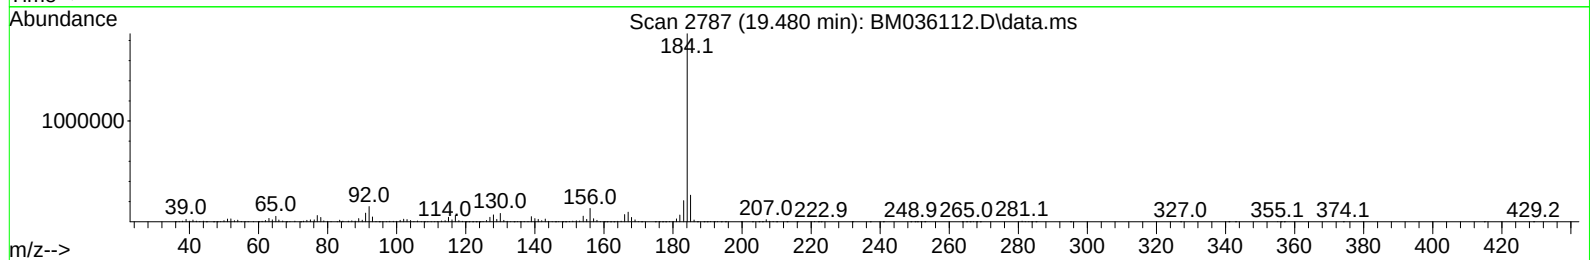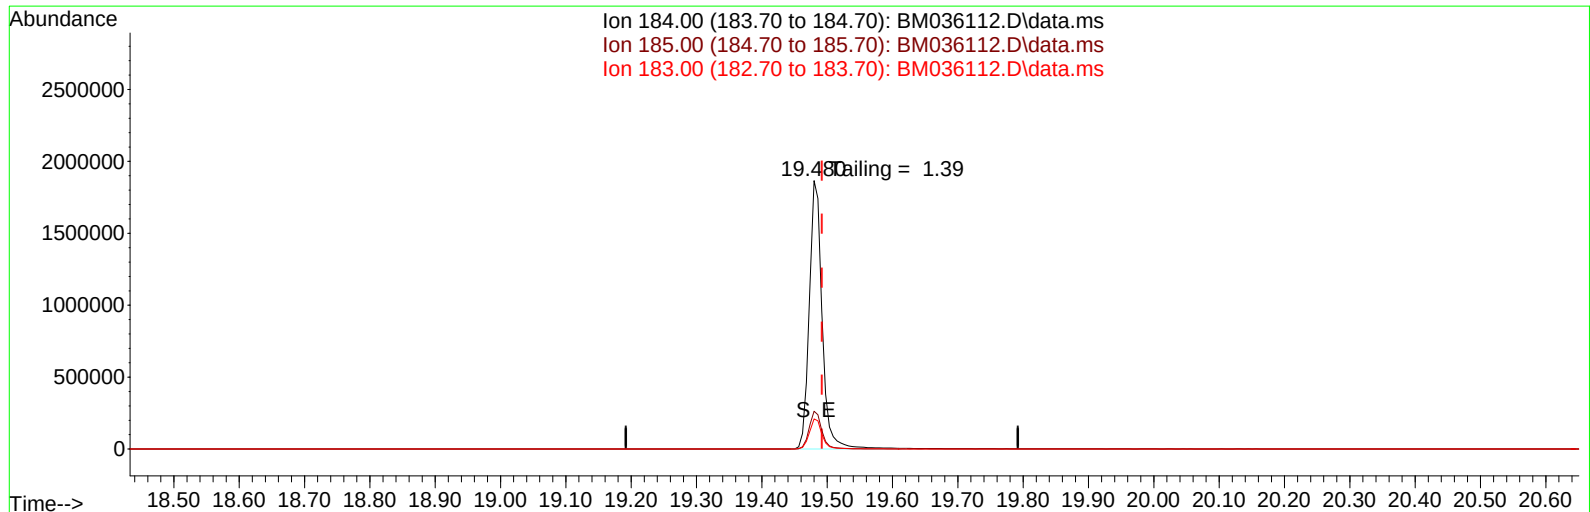

TIC: BM036112.D\data.ms

(77) Benzidine**19.480min (-0.012) 74792.08 ng****response 2566359**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.10
183.00	11.90	11.23
0.00	0.00	0.00