

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080522\
 Data File : BM036114.D
 Acq On : 05 Aug 2022 11:20
 Operator : CG/JU
 Sample : PB146605BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB146605BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM036114.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.416	390	396	411	rBV	5704673	8076801	72.16%	12.401%
2	7.028	662	670	690	rVB	5306048	8212908	73.37%	12.610%
3	7.851	803	810	820	rVB	1087741	1616860	14.44%	2.482%
4	9.022	1001	1009	1020	rBV	3202274	5152702	46.03%	7.911%
5	10.657	1279	1287	1300	rBV	1368954	2315788	20.69%	3.556%
6	13.122	1699	1706	1718	rBV	7736548	11193563	100.00%	17.186%
7	14.492	1931	1939	1949	rBV	1999898	2824197	25.23%	4.336%
8	15.980	2185	2192	2205	rBV	5508477	7487539	66.89%	11.496%
9	17.233	2399	2405	2413	rBV	2070913	2873481	25.67%	4.412%
10	19.856	2846	2851	2860	rBV	8850017	10910984	97.48%	16.752%
11	21.415	3111	3116	3120	rBV	1757258	2309197	20.63%	3.545%
12	23.768	3511	3516	3527	rVB2	1132445	2157437	19.27%	3.312%




Sum of corrected areas: 65131457

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080522\
Data File : BM036114.D
Acq On : 05 Aug 2022 11:20
Operator : CG/JU
Sample : PB146605BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146605BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

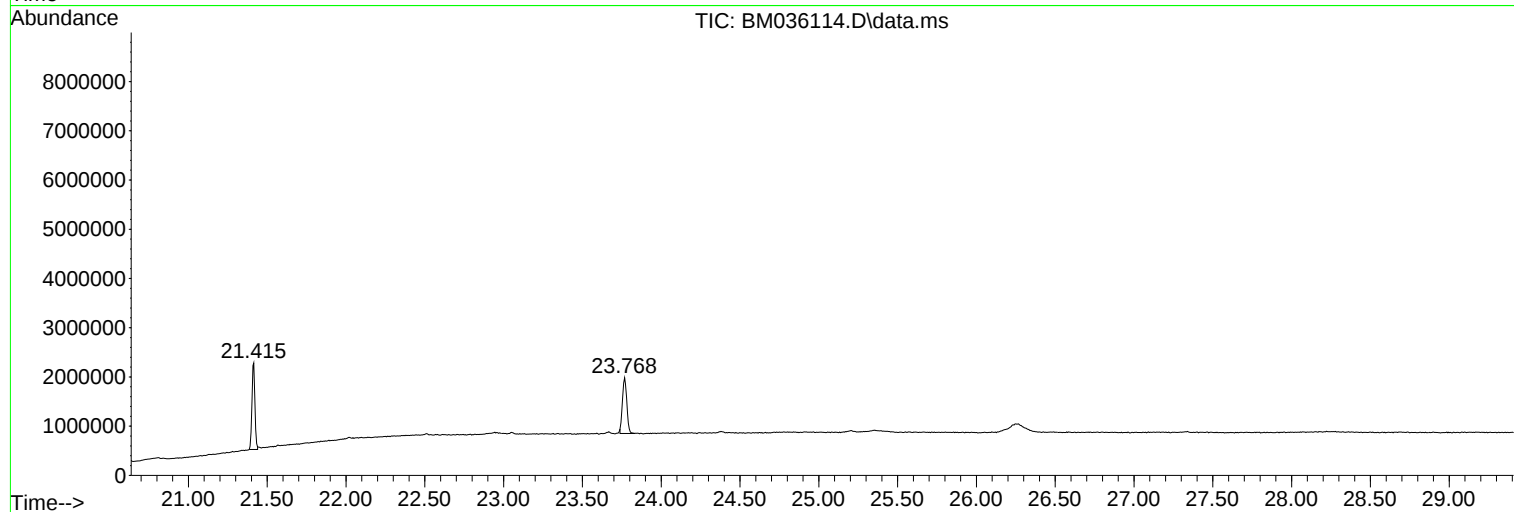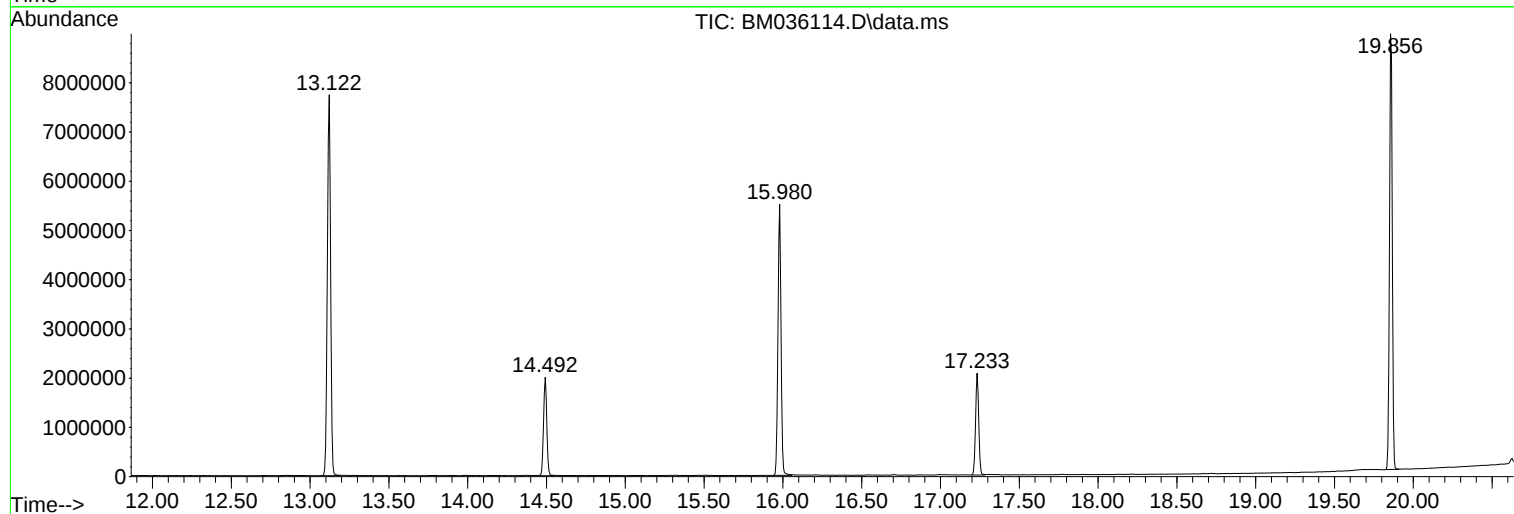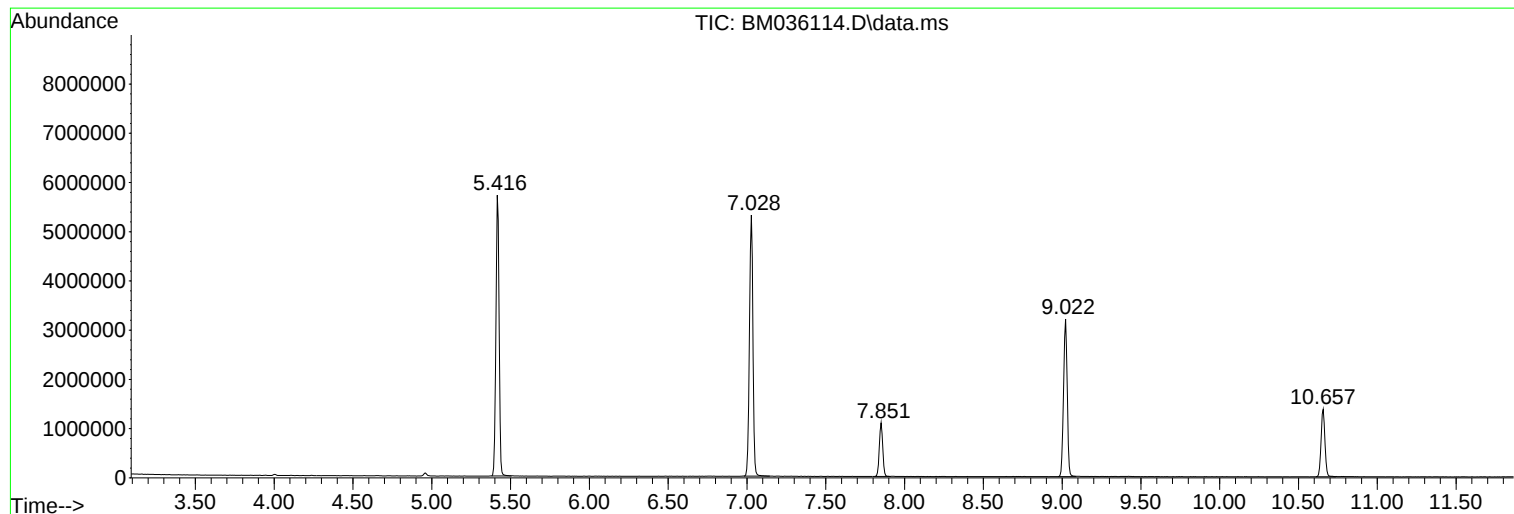

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080522\
Data File : BM036114.D
Acq On : 05 Aug 2022 11:20
Operator : CG/JU
Sample : PB146605BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146605BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080522\
Data File : BM036114.D
Acq On : 05 Aug 2022 11:20
Operator : CG/JU
Sample : PB146605BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146605BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------