

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080522\
 Data File : BM036136.D
 Acq On : 06 Aug 2022 01:30
 Operator : CG/JU
 Sample : N4044-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 VNJ-230

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM036136.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.957	311	318	322	rBV	112640	164644	1.80%	0.267%
2	5.446	395	401	412	rBV	4282364	6000238	65.51%	9.714%
3	7.069	670	677	687	rBV	4061040	6180093	67.48%	10.005%
4	7.857	801	811	818	rBV	1073995	1698068	18.54%	2.749%
5	9.028	1002	1010	1027	rBV	2523916	4086689	44.62%	6.616%
6	10.663	1278	1288	1298	rBV	1375271	2331607	25.46%	3.775%
7	13.122	1699	1706	1720	rBV	5325166	7944937	86.75%	12.862%
8	14.498	1933	1940	1947	rBV	1940051	2774843	30.30%	4.492%
9	15.986	2187	2193	2200	rBV	4182152	5979646	65.29%	9.680%
10	17.239	2400	2406	2410	rBV	2190340	3031679	33.10%	4.908%
11	17.280	2410	2413	2419	rVB	228829	295930	3.23%	0.479%
12	17.368	2424	2428	2434	rVB2	82837	126461	1.38%	0.205%
13	17.909	2516	2520	2524	rBV	75288	91885	1.00%	0.149%
14	18.139	2552	2559	2568	rBV2	362923	634116	6.92%	1.027%
15	18.309	2583	2588	2592	rBV2	72093	139700	1.53%	0.226%
16	18.998	2701	2705	2709	rBV	361808	481392	5.26%	0.779%
17	19.292	2751	2755	2763	rBV	599210	819350	8.95%	1.326%
18	19.656	2813	2817	2826	rVB	532615	747356	8.16%	1.210%
19	19.862	2847	2852	2857	rBV	7514157	9158856	100.00%	14.827%
20	21.127	3064	3067	3075	rVB3	1047509	1286884	14.05%	2.083%
21	21.415	3111	3116	3120	rBV	2679592	3615010	39.47%	5.852%
22	23.056	3391	3395	3400	rBV2	657834	971551	10.61%	1.573%
23	23.774	3512	3517	3524	rVB2	1686630	3209233	35.04%	5.195%




Sum of corrected areas: 61770168

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080522\
Data File : BM036136.D
Acq On : 06 Aug 2022 01:30
Operator : CG/JU
Sample : N4044-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VNJ-230

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

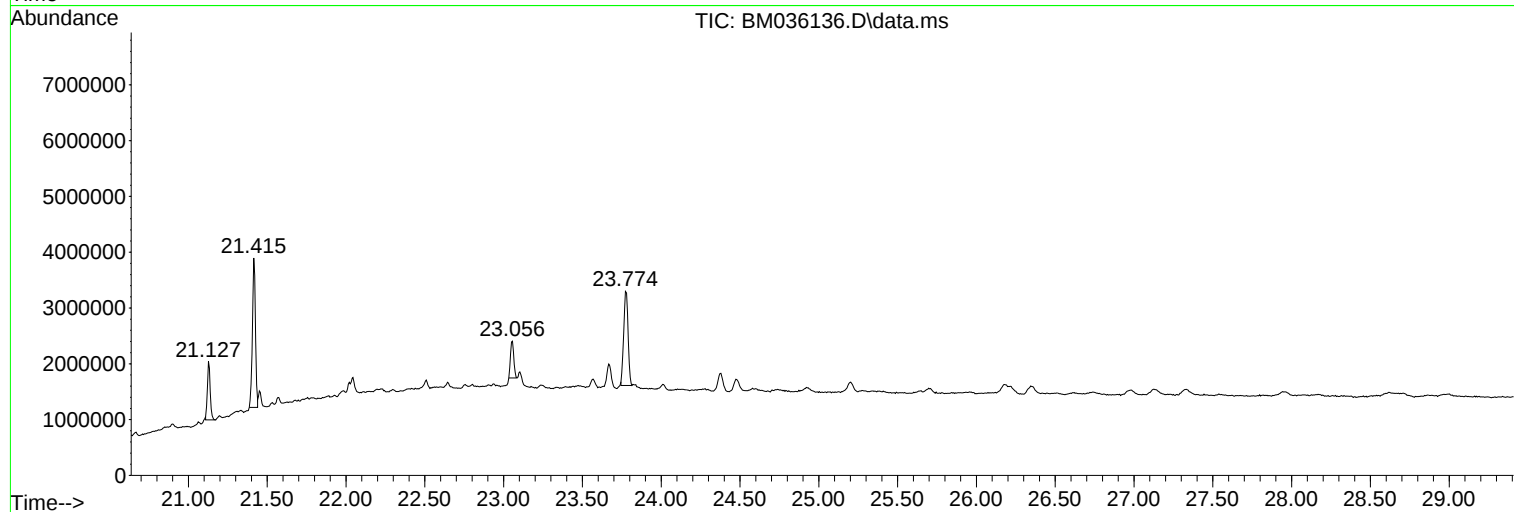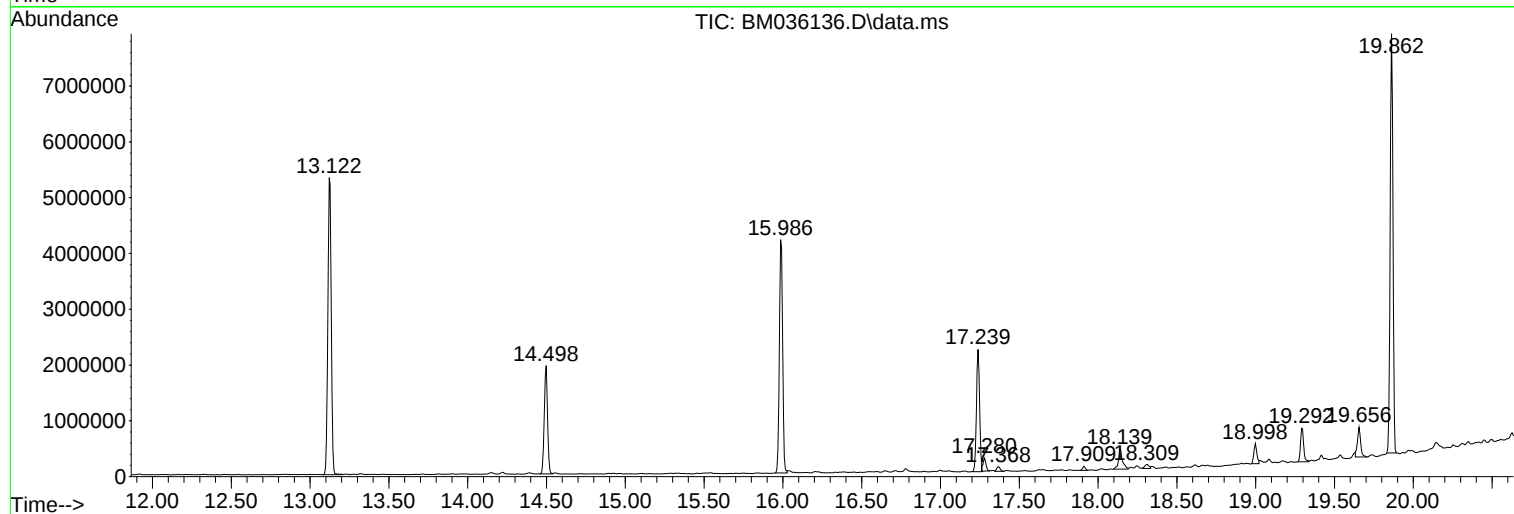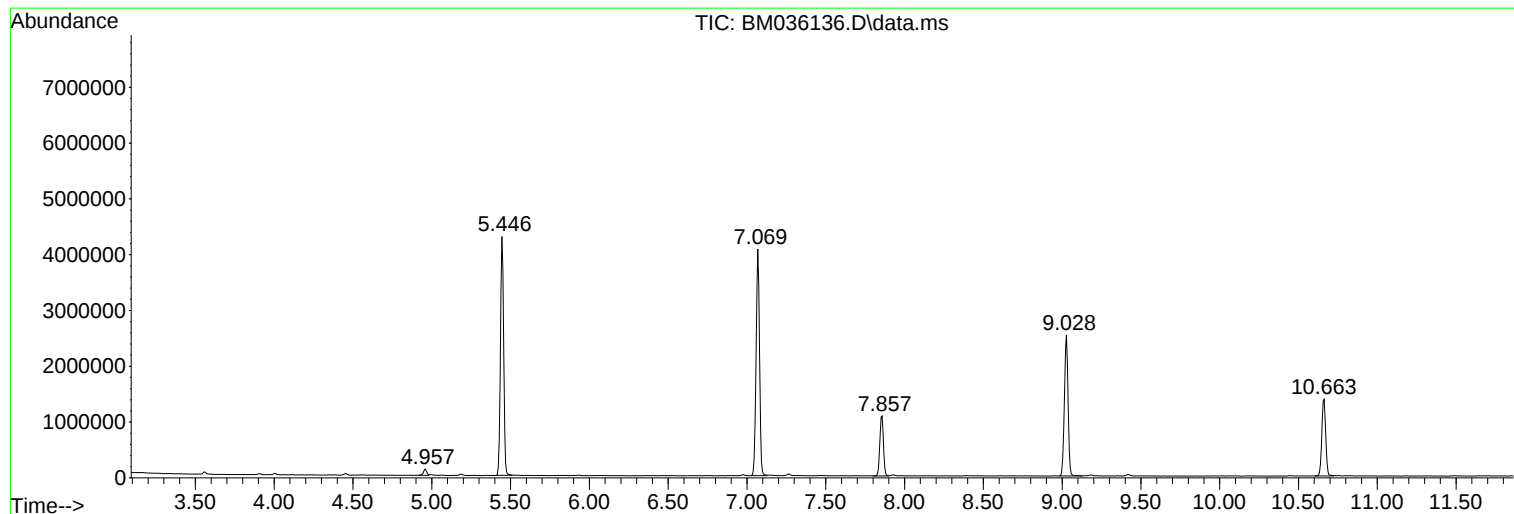

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080522\
Data File : BM036136.D
Acq On : 06 Aug 2022 01:30
Operator : CG/JU
Sample : N4044-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VNJ-230

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080522\
Data File : BM036136.D
Acq On : 06 Aug 2022 01:30
Operator : CG/JU
Sample : N4044-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VNJ-230

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------