
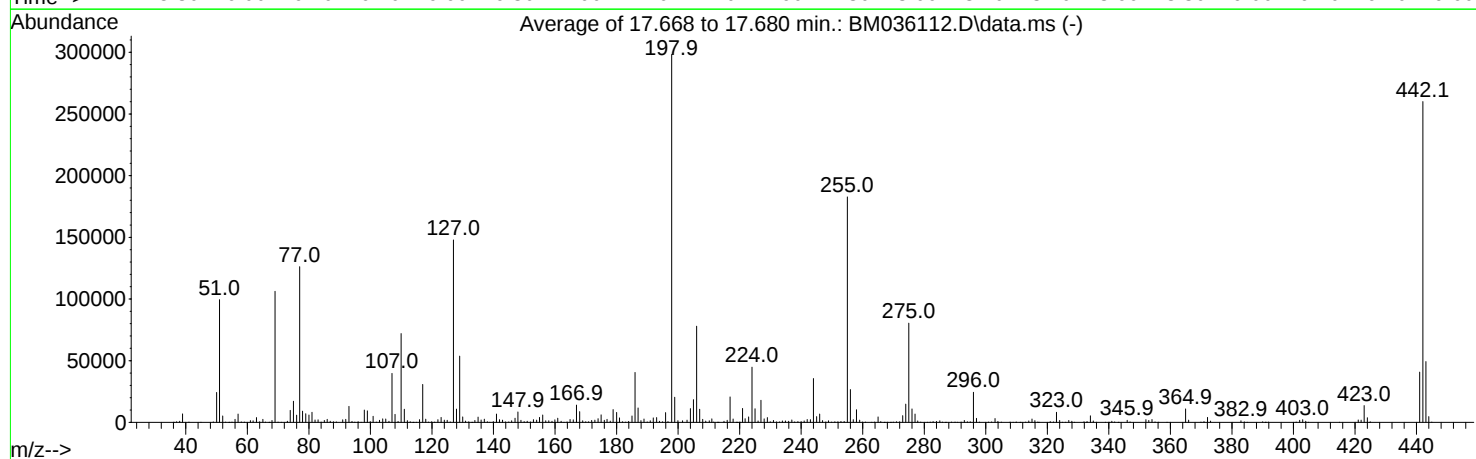


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080522\
 Data File : BM036112.D
 Acq On : 05 Aug 2022 10:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 08 23:36:56 2022

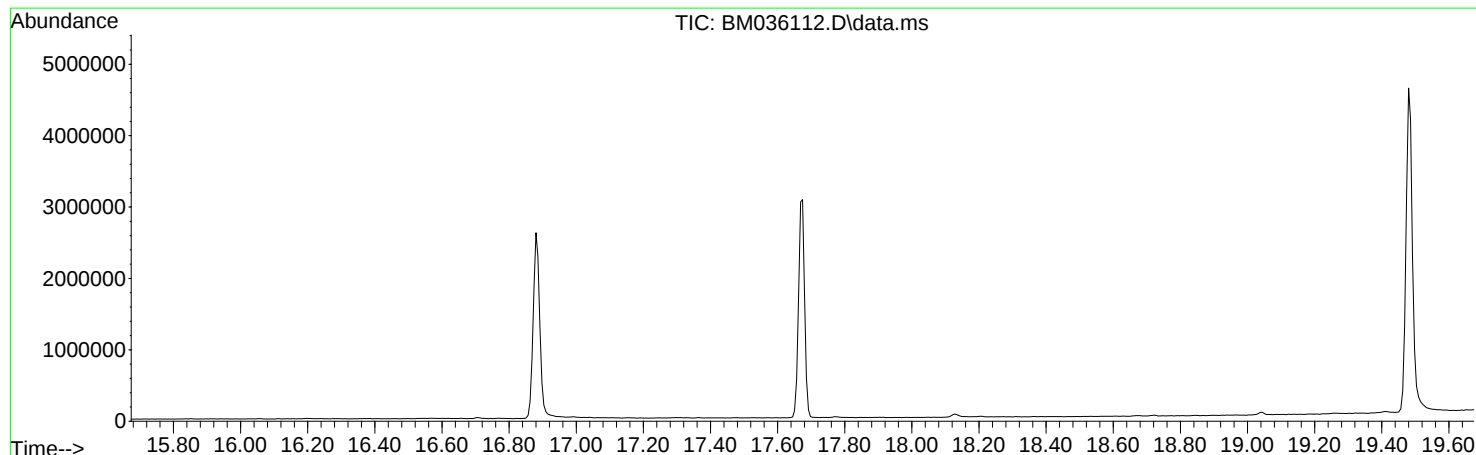




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	99519	PASS
68	69	0.00	2	1.5	1613	PASS
69	198	0.00	100	35.6	106289	PASS
70	69	0.00	2	0.2	262	PASS
127	198	10	80	49.6	147936	PASS
197	198	0.00	2	0.2	713	PASS
198	198	100	100	100.0	298219	PASS
199	198	5	9	6.8	20362	PASS
275	198	10	60	27.0	80403	PASS
365	198	1	100	3.7	10961	PASS
441	198	0.01	100	13.7	40736	PASS
442	442	50	100	100.0	260032	PASS
443	442	15	24	18.9	49264	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080522\
 Data File : BM036112.D
 Acq On : 05 Aug 2022 10:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 06 06:56:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 05 03:36:25 2022
 Response via : Initial Calibration

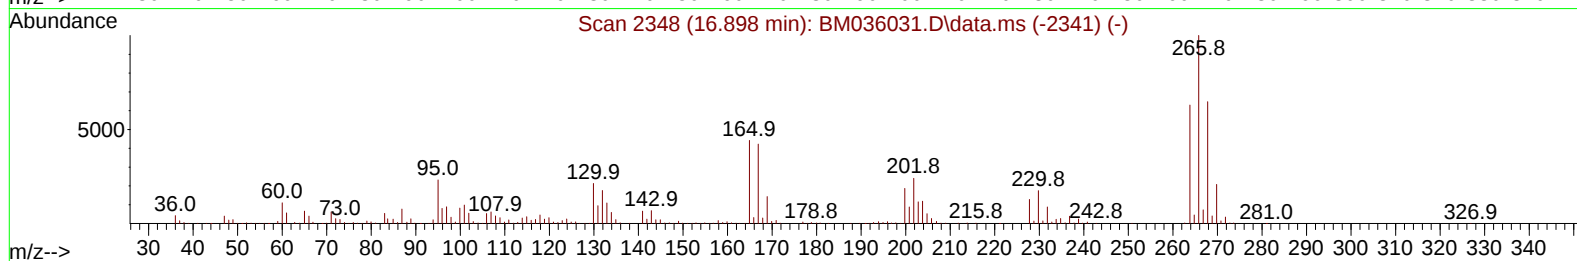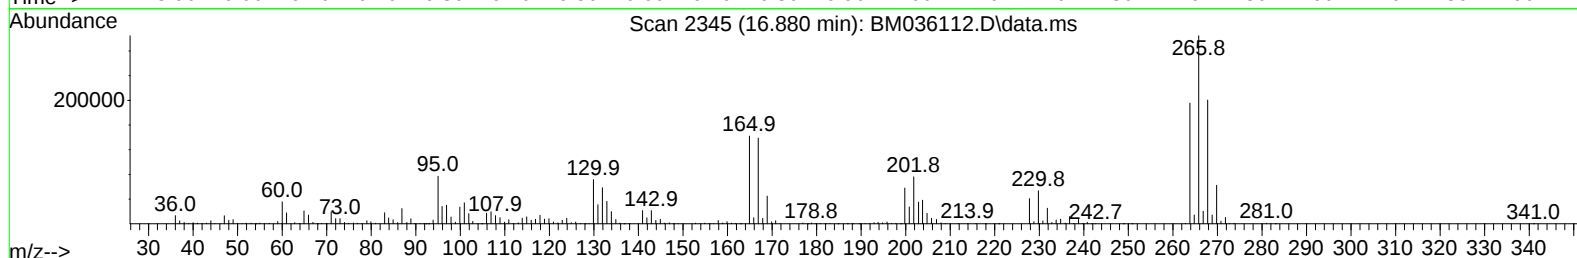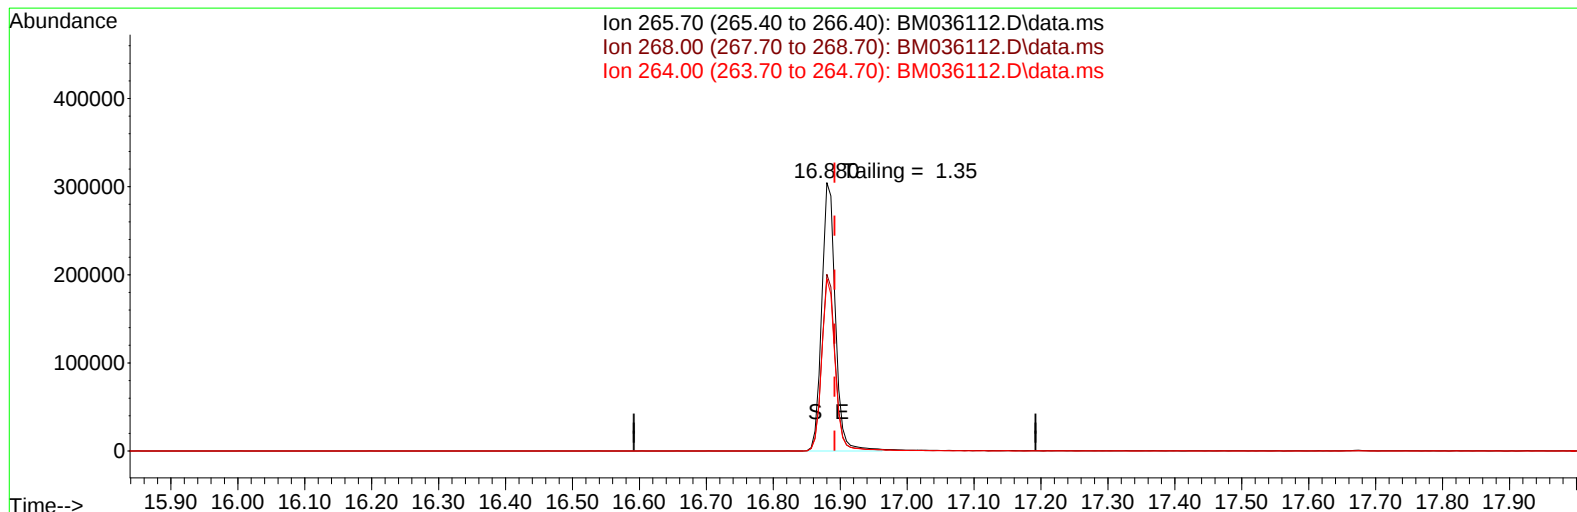

TIC: BM036112.D\data.ms

(70) Pentachlorophenol (C)

16.880min (-0.012) 276308.14 ng




response 434592

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	65.81
264.00	63.30	64.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080522\
Data File : BM036112.D
Acq On : 05 Aug 2022 10:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 06 06:56:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 05 03:36:25 2022
Response via : Initial Calibration

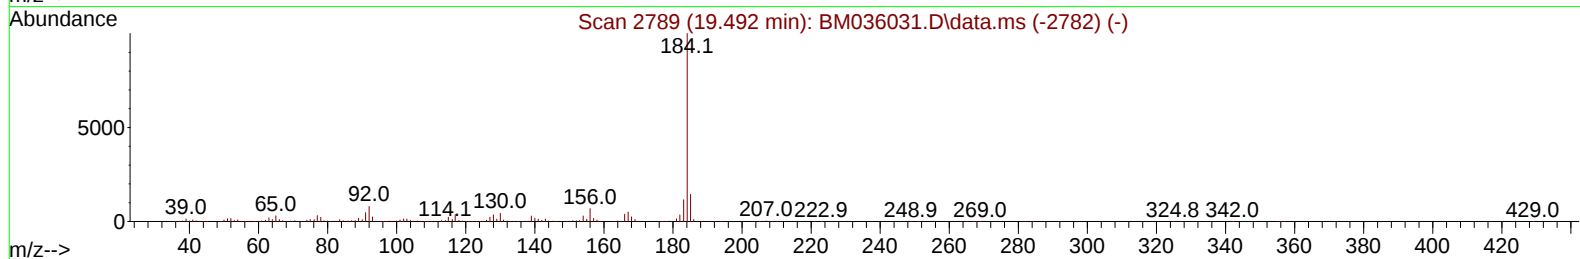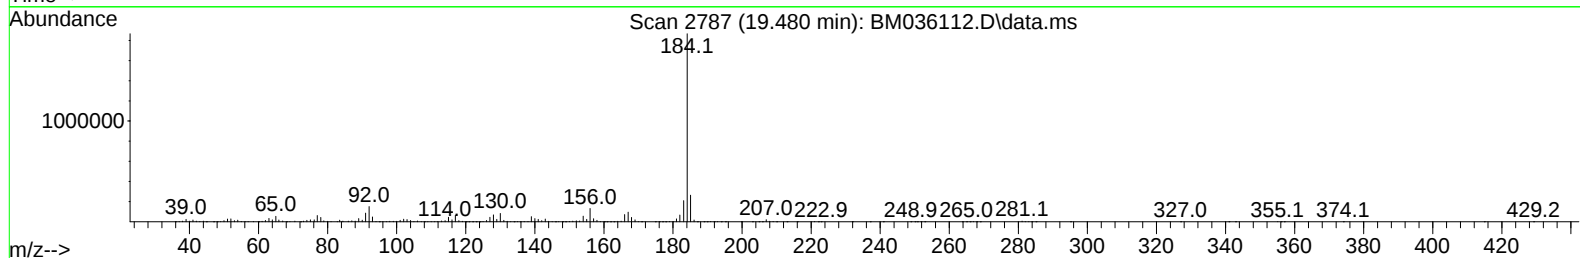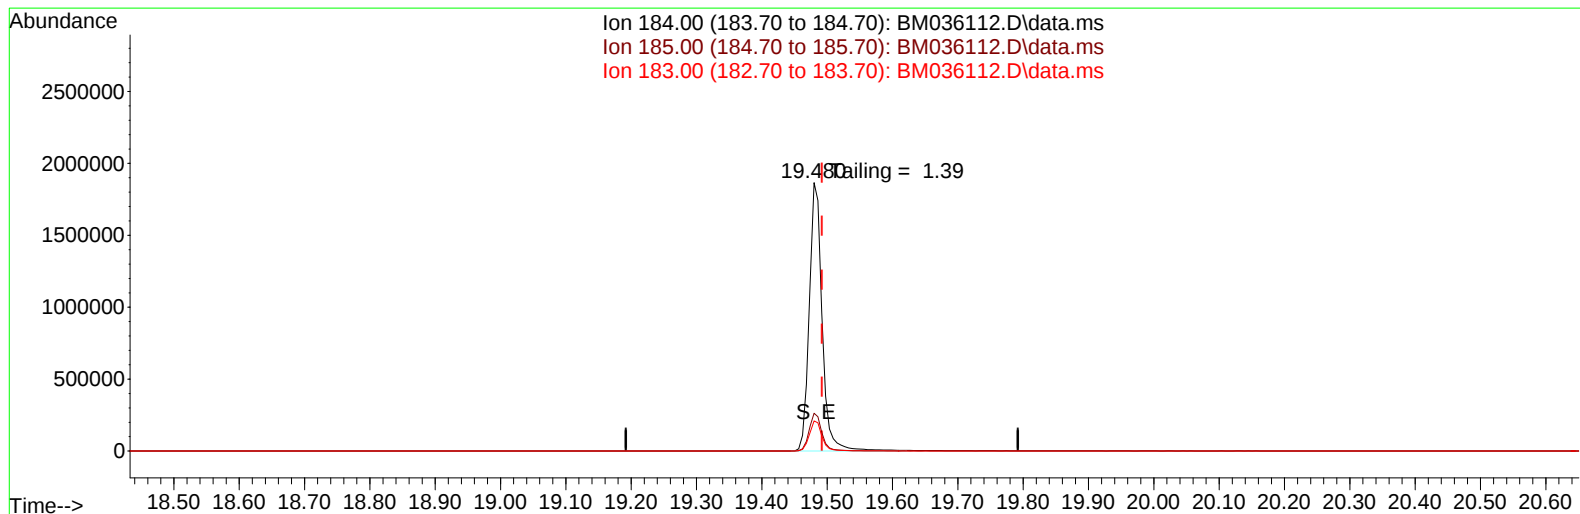

TIC: BM036112.D\data.ms

(77) Benzidine

19.480min (-0.012) 74792.08 ng

response 2566359

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.10
183.00	11.90	11.23
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/5/2022	BNA_M	<u>BM036112.D</u>
Compound Name	Response	Retention Time
DDT	1134590	20.709
DDD	12117	20.321
DDE	726	19.762
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12843	1147433	1.12

Instrument :
BNA_M
ClientSampleId :
DFTPP