
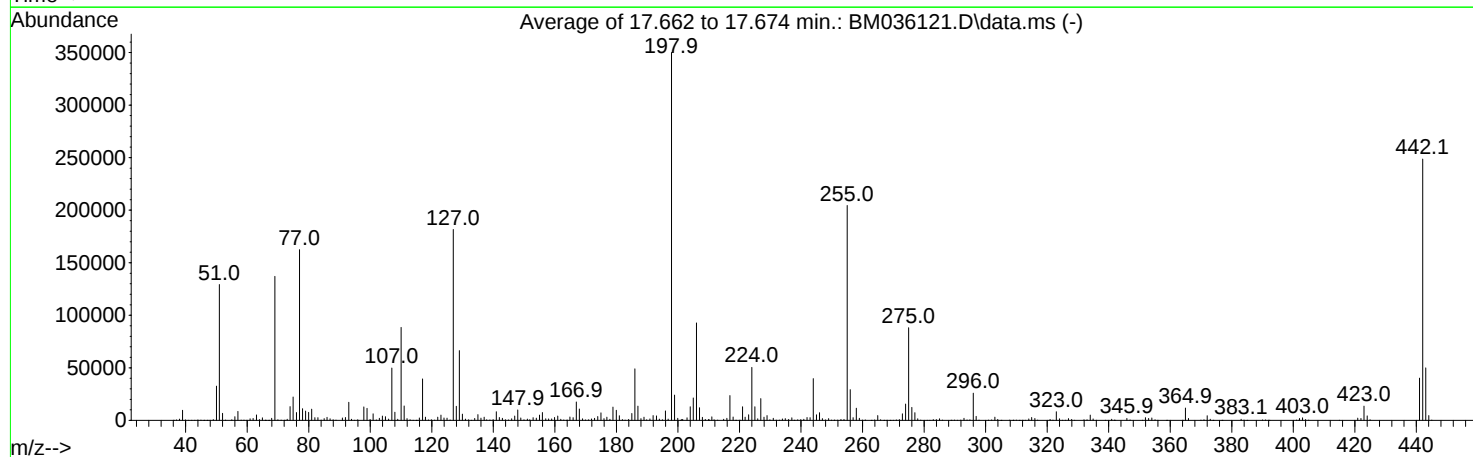


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080522\
 Data File : BM036121.D
 Acq On : 05 Aug 2022 16:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 08 23:36:56 2022

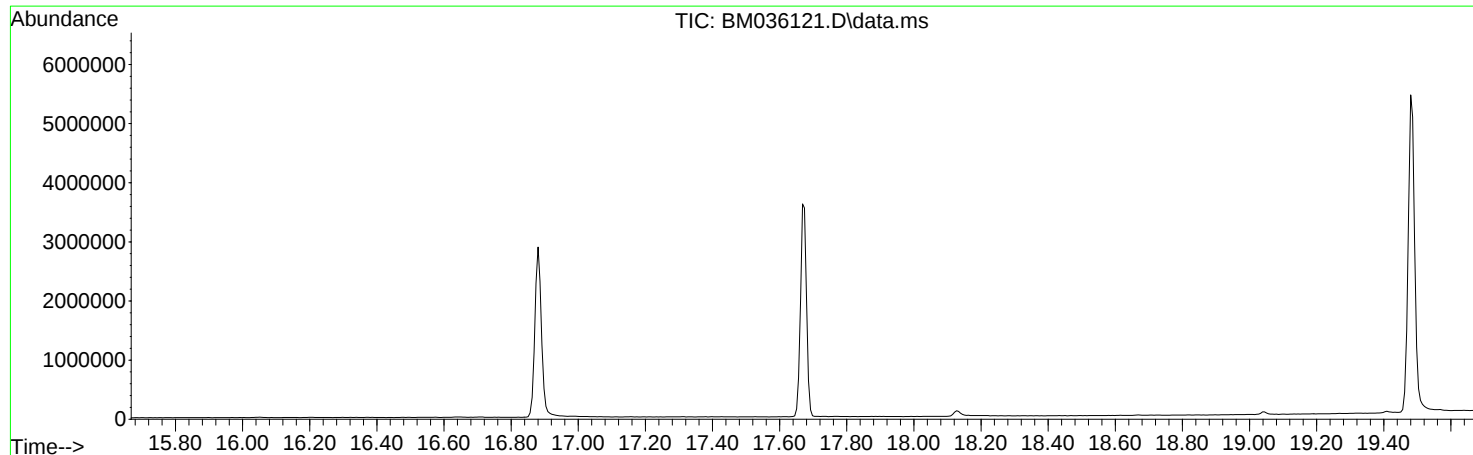




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	129297	PASS
68	69	0.00	2	1.4	1932	PASS
69	198	0.00	100	39.2	137100	PASS
70	69	0.00	2	0.4	615	PASS
127	198	10	80	51.9	181616	PASS
197	198	0.00	2	0.4	1276	PASS
198	198	100	100	100.0	350059	PASS
199	198	5	9	6.9	24040	PASS
275	198	10	60	25.2	88237	PASS
365	198	1	100	3.4	11797	PASS
441	198	0.01	100	11.5	40149	PASS
442	442	50	100	100.0	248664	PASS
443	442	15	24	20.1	49880	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080522\
 Data File : BM036121.D
 Acq On : 05 Aug 2022 16:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 06 06:58:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 05 03:36:25 2022
 Response via : Initial Calibration

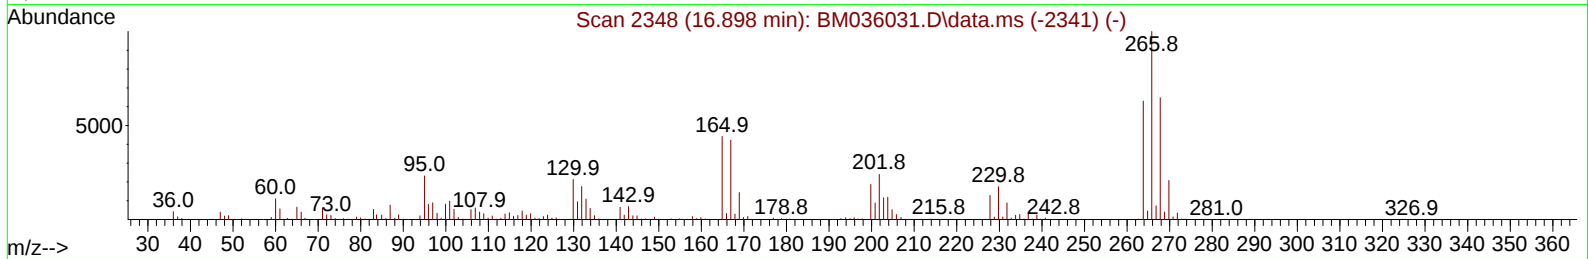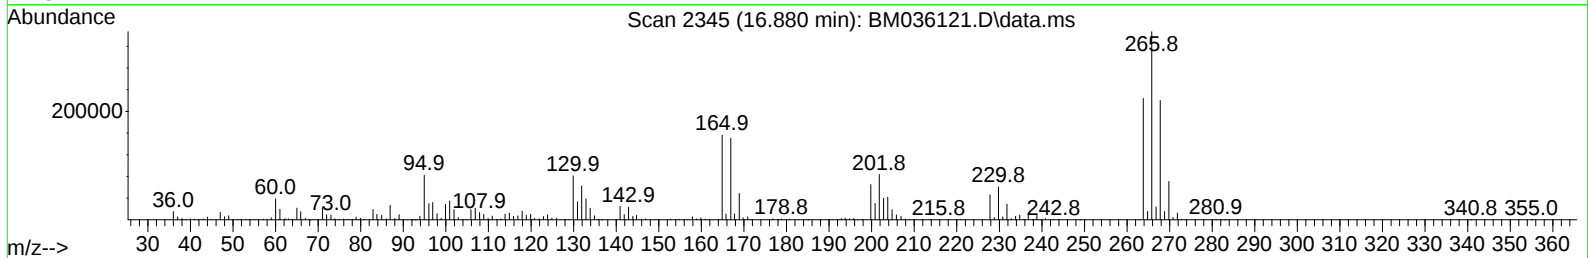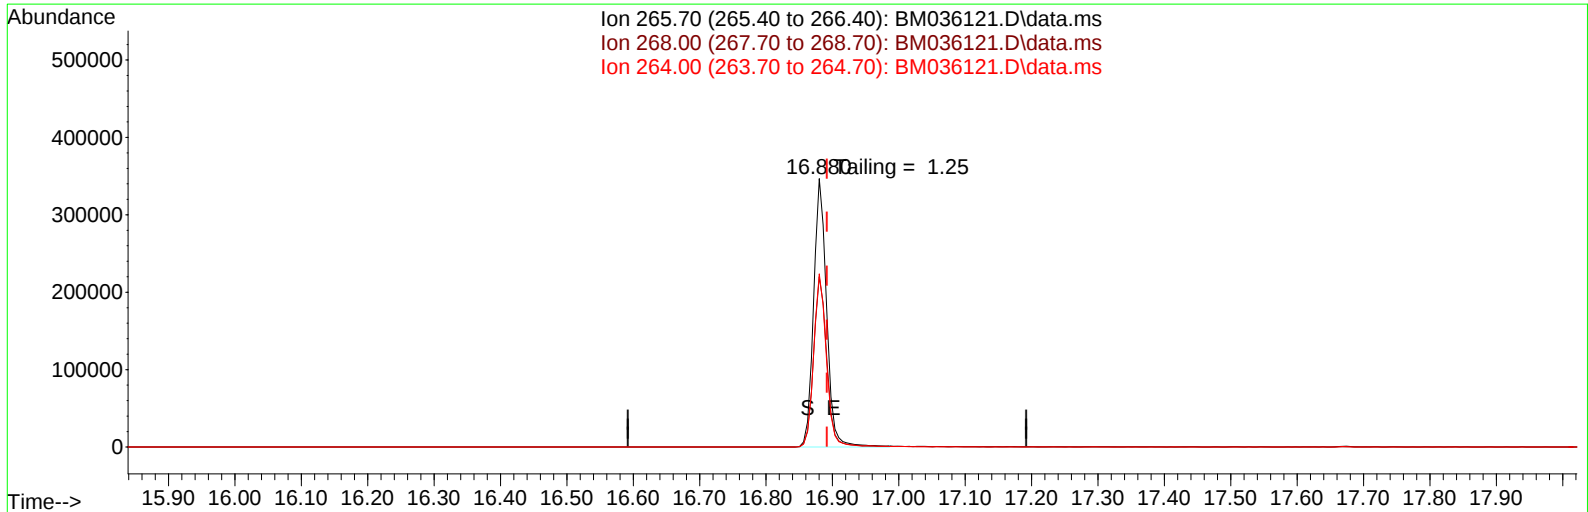

TIC: BM036121.D\data.ms

(70) Pentachlorophenol (C)

16.880min (-0.012) 187246.97 ng




response 475750

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.42
264.00	63.30	64.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080522\
Data File : BM036121.D
Acq On : 05 Aug 2022 16:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 06 06:58:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM080122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 05 03:36:25 2022
Response via : Initial Calibration

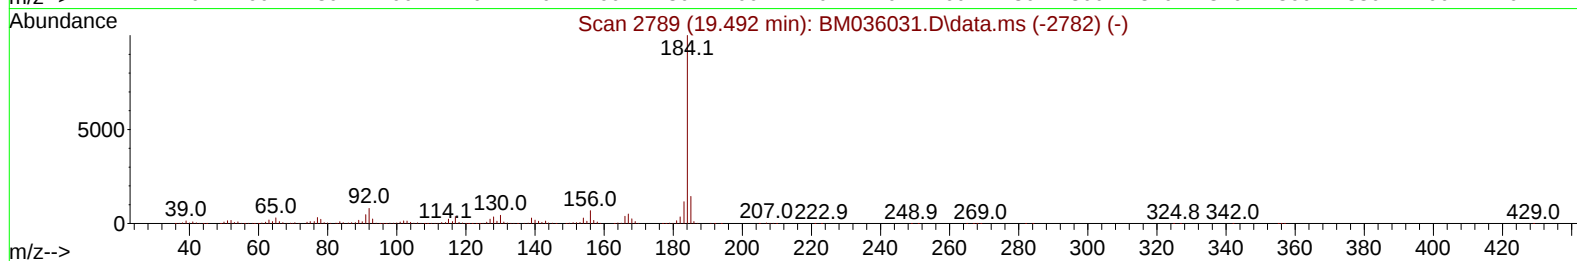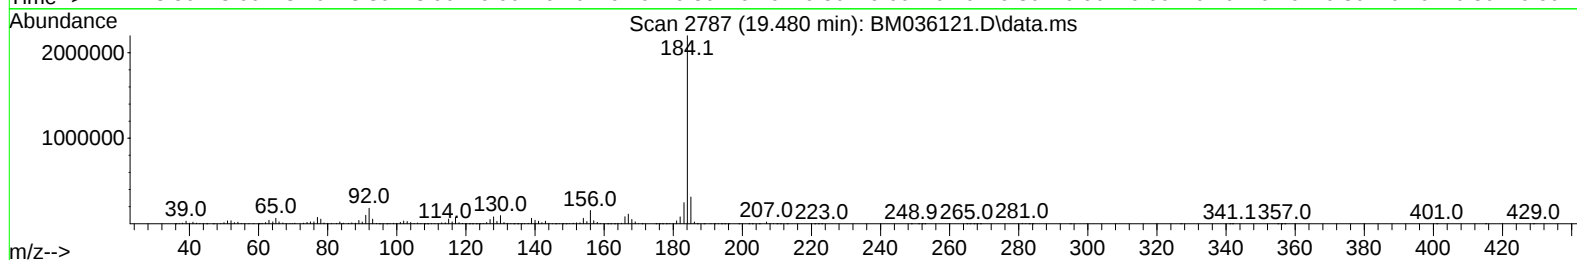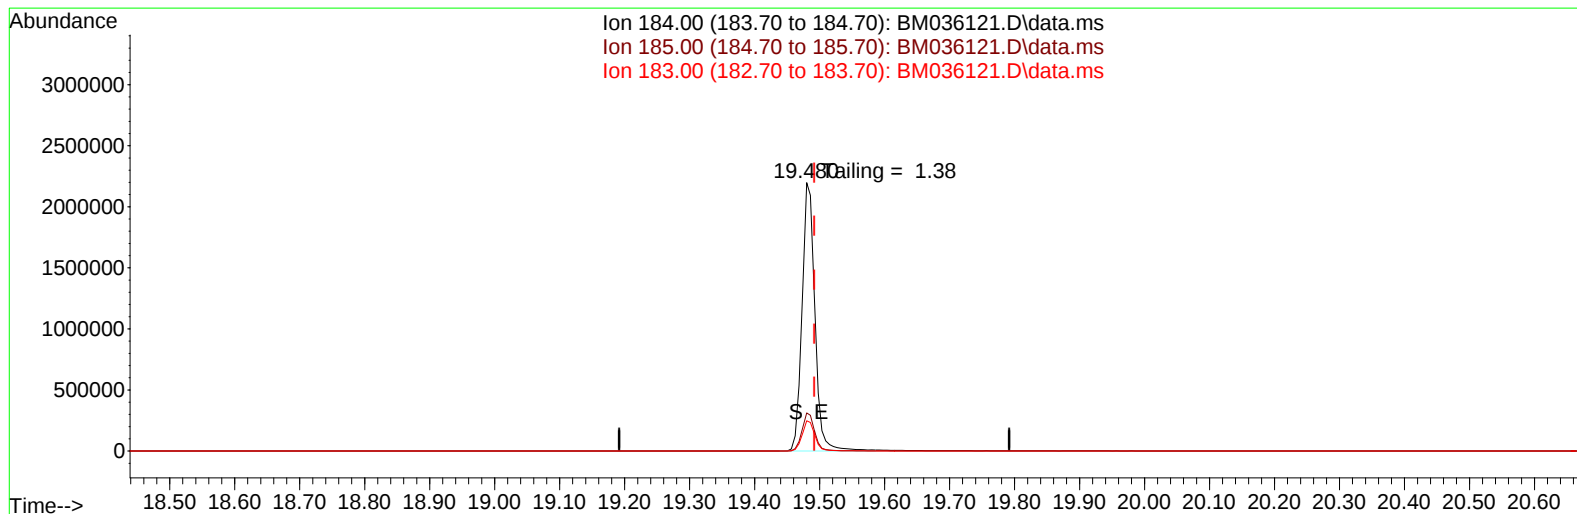

TIC: BM036121.D\data.ms

(77) Benzidine

19.480min (-0.012) 146710.37 ng

response 3045108

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.19
183.00	11.90	11.28
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/5/2022	BNA_M	<u>BM036121.D</u>
Compound Name	Response	Retention Time
DDT	1365044	20.709
DDD	12712	20.274
DDE	1098	19.762
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13810	1378854	1.00

Instrument :
BNA_M
ClientSampleId :
DFTPP