




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080524\
 Data File : BM047023.D
 Acq On : 06 Aug 2024 12:56
 Operator : RC/JU
 Sample : P3329-06DL 5X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F7E08DL

Manual IntegrationsAPPROVED

Quant Time: Aug 06 13:32:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 06 04:53:02 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/06/2024
 Supervised By :mohammad ahmed 08/07/2024

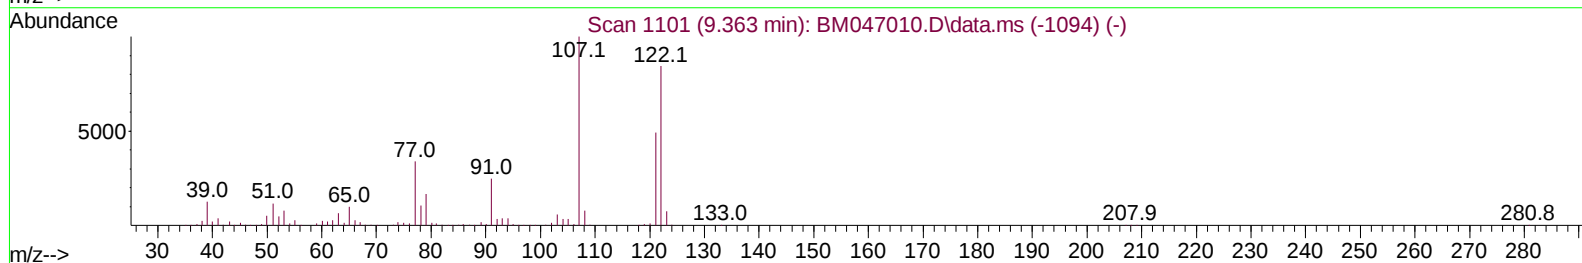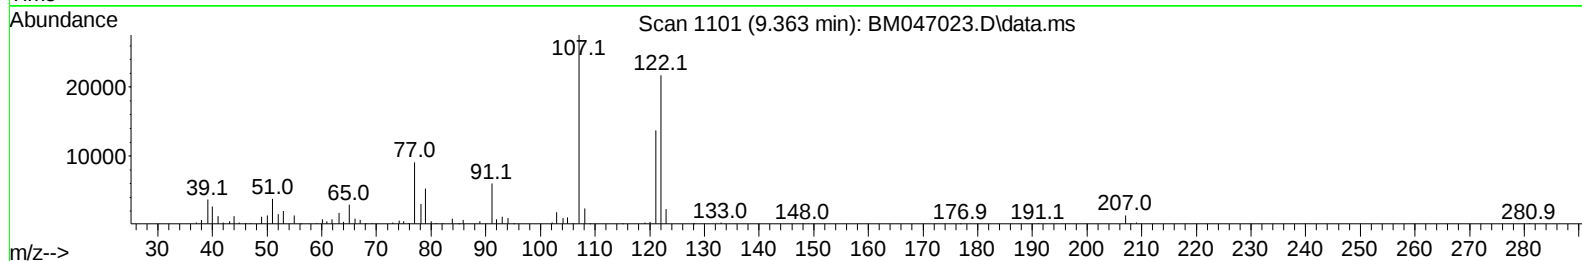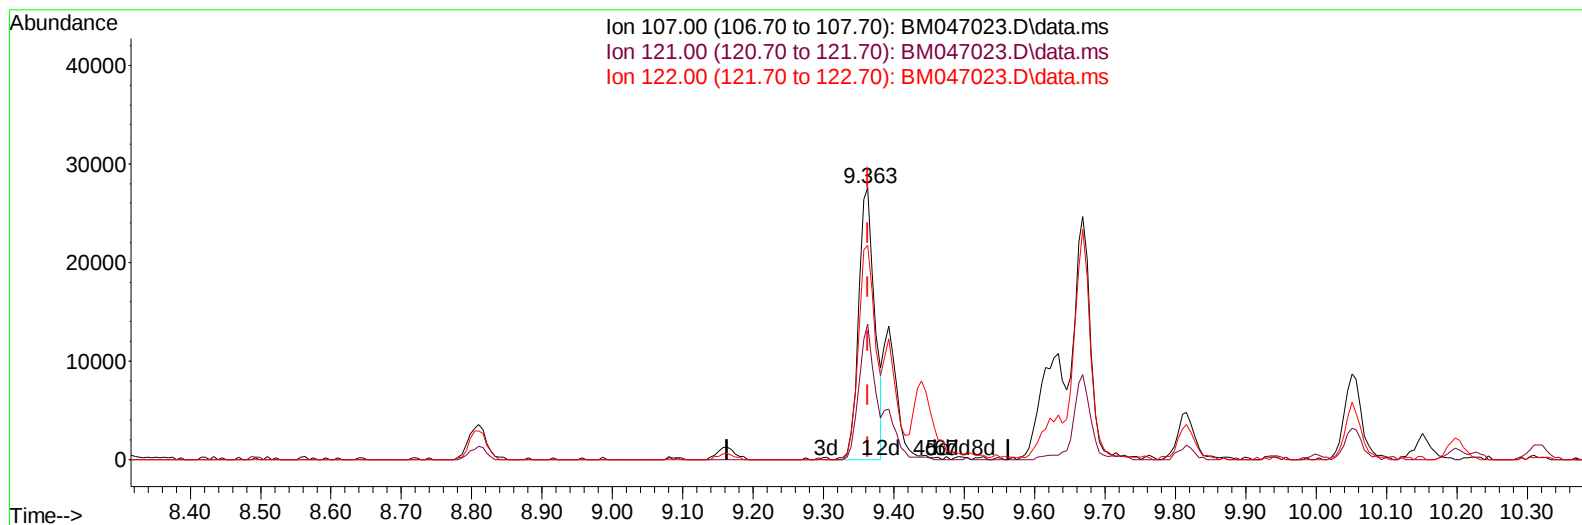

TIC: BM047023.D\data.ms

(26) 2,4-Dimethylphenol

9.363min (-0.000) 3.26 ng/u1

response 43400

Ion	Exp%	Act%
107.00	100.00	100.00
121.00	46.60	49.82
122.00	82.20	78.82
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080524\
 Data File : BM047023.D
 Acq On : 06 Aug 2024 12:56
 Operator : RC/JU
 Sample : P3329-06DL 5X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F7E08DL

Manual IntegrationsAPPROVED

Quant Time: Aug 06 13:32:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 06 04:53:02 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/06/2024
 Supervised By :mohammad ahmed 08/07/2024

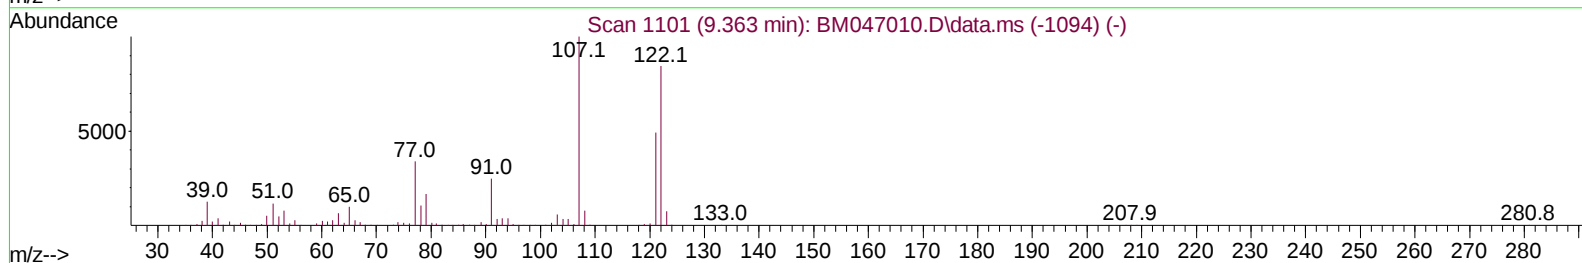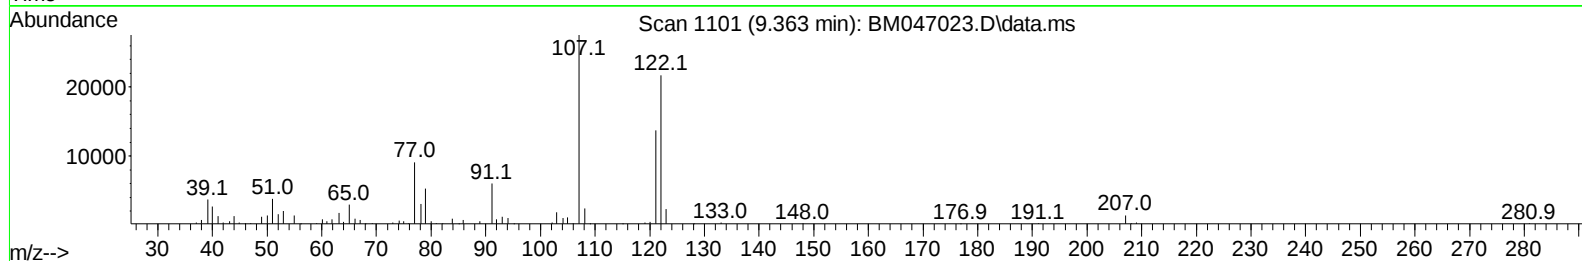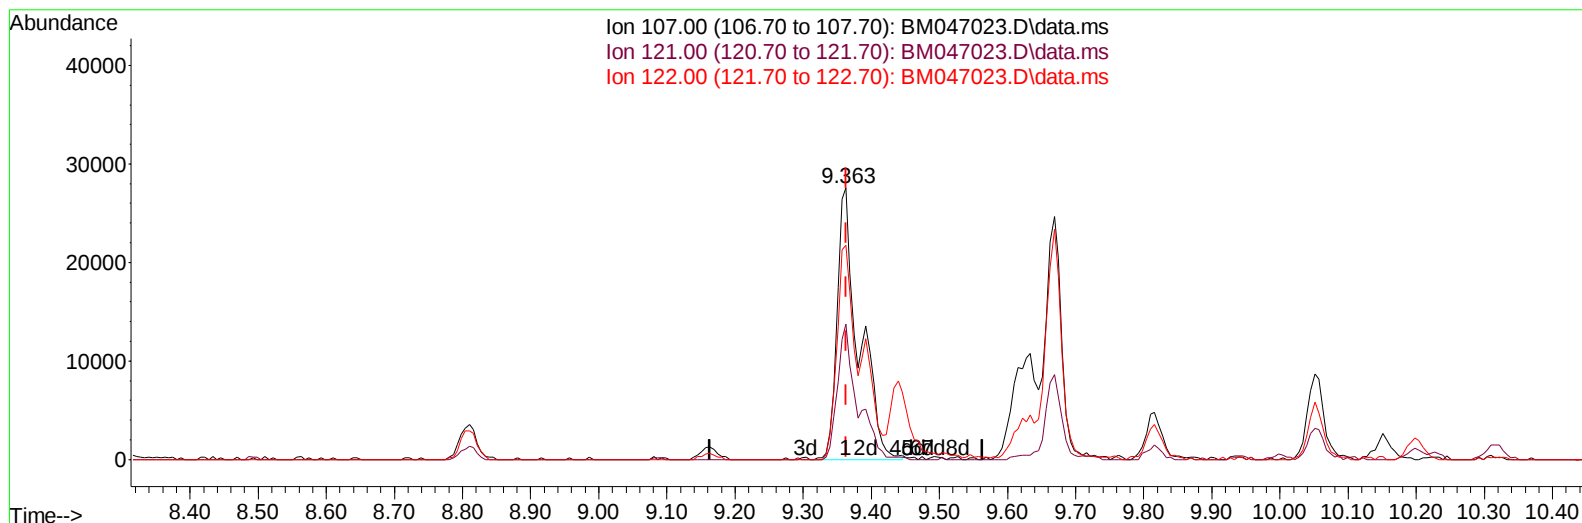

TIC: BM047023.D\data.ms

(26) 2,4-Dimethylphenol

9.363min (-0.000) 4.63 ng/ul m

response 61576

Ion	Exp%	Act%
107.00	100.00	100.00
121.00	46.60	49.82
122.00	82.20	78.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080524\
 Data File : BM047023.D
 Acq On : 06 Aug 2024 12:56
 Operator : RC/JU
 Sample : P3329-06DL 5X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F7E08DL

Manual IntegrationsAPPROVED

Quant Time: Aug 07 01:28:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 06 04:53:02 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/06/2024
 Supervised By :mohammad ahmed 08/07/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.392	152		183585	20.000	ng/ul	0.00
20) Naphthalene-d8	10.151	136		703654	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.051	164		453337	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.809	188		968176	20.000	ng/ul	0.00
79) Chrysene-d12	21.050	240		909971	20.000	ng/ul	0.00
88) Perylene-d12	23.756	264		1045603	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	0.000	96		0d	0.000	ng/uL	
4) Pyridine-d5	3.422	84		32173	2.545	ng/ul	0.01
7) Phenol-d5	6.598	99		45887	3.290	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.751	67		31508	3.434	ng/ul	0.00
11) 2-Chlorophenol-d4	6.934	132		35146	2.975	ng/ul	0.00
15) 4-Methylphenol-d8	8.110	113		37242	3.371	ng/ul	0.00
21) Nitrobenzene-d5	8.539	128		17493	3.098	ng/ul	0.00
24) 2-Nitrophenol-d4	9.251	143		17278	2.802	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.786	165		35936	3.035	ng/ul	0.00
31) 4-Chloroaniline-d4	10.304	131		48952	3.146	ng/ul	0.00
46) Dimethylphthalate-d6	13.474	166		121268	3.499	ng/ul	0.00
49) Acenaphthylene-d8	13.739	160		134020	3.464	ng/ul	0.00
54) 4-Nitrophenol-d4	14.298	143		14496	2.163	ng/ul	0.00
60) Fluorene-d10	15.057	176		104369	3.520	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.192	200		8136	1.330	ng/ul	0.00
73) Anthracene-d10	16.909	188		165802	3.612	ng/ul	0.00
81) Pyrene-d10	19.221	212		191858	3.683	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.568	264		193005	3.505	ng/ul	0.00
Target Compounds							
						Qvalue	
8) Phenol	6.622	94		107152	7.629	ng/ul	93
13) 2-Methylphenol	7.851	108		40449	3.781	ng/ul	95
18) 4-Methylphenol	8.175	108		128502	11.116	ng/ul	98
26) 2,4-Dimethylphenol	9.363	107		61576m	4.631	ng/ul	
30) Naphthalene	10.198	128		1386917	37.227	ng/ul	99
36) 2-Methylnaphthalene	11.827	142		238000	9.149	ng/ul	97
37) 1-Methylnaphthalene	12.051	142		103933	3.947	ng/ul	100
43) 1,1'-Biphenyl	12.868	154		55488	1.636	ng/ul	98
52) Acenaphthene	14.115	153		160410	5.445	ng/ul	98
56) Dibenzofuran	14.457	168		197325	4.773	ng/ul	95
61) Fluorene	15.110	166		196042	5.749	ng/ul	99
72) Phenanthrene	16.851	178		842115	15.516	ng/ul	99
74) Anthracene	16.945	178		571815	10.448	ng/ul	99
77) Carbazole	17.221	167		228509	4.504	ng/ul	99
80) Fluoranthene	18.886	202		479716	7.706	ng/ul	99
82) Pyrene	19.250	202		326312	4.919	ng/ul#	95
85) Benzo(a)anthracene	21.033	228		101314	1.524	ng/ul	100
87) Chrysene	21.086	228		111357	1.757	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

