

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080524\
 Data File : BM046989.D
 Acq On : 05 Aug 2024 12:18
 Operator : RC/JU
 Sample : P3171-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCVX2

Quant Time: Aug 05 12:55:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 03 02:51:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.398	152	165876	20.000	ng/u1	0.00
20) Naphthalene-d8	10.157	136	622928	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.057	164	393035	20.000	ng/u1	0.00
64) Phenanthrene-d10	16.815	188	821822	20.000	ng/u1	0.00
79) Chrysene-d12	21.050	240	738759	20.000	ng/u1	0.00
88) Perylene-d12	23.762	264	832013	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.022	96	17379	4.151	ng/uL	0.00
4) Pyridine-d5	3.410	84	285280	24.979	ng/u1	0.00
7) Phenol-d5	6.598	99	373534	29.644	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.751	67	234536	28.288	ng/u1	0.00
11) 2-Chlorophenol-d4	6.940	132	294653	27.605	ng/u1	0.00
15) 4-Methylphenol-d8	8.116	113	313009	31.357	ng/u1	0.00
21) Nitrobenzene-d5	8.540	128	144645	28.937	ng/u1	0.00
24) 2-Nitrophenol-d4	9.257	143	167223	30.634	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	9.792	165	313322	29.896	ng/u1	0.00
31) 4-Chloroaniline-d4	10.304	131	433680	31.485	ng/u1	0.00
46) Dimethylphthalate-d6	13.480	166	1105133	36.774	ng/u1	0.00
49) Acenaphthylene-d8	13.739	160	1155106	34.435	ng/u1	0.00
54) 4-Nitrophenol-d4	14.292	143	162751	28.010	ng/u1	0.00
60) Fluorene-d10	15.057	176	895534	34.836	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.198	200	136596	26.308	ng/u1	0.00
73) Anthracene-d10	16.915	188	1471530	37.771	ng/u1	0.00
81) Pyrene-d10	19.227	212	1649358	39.001	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.580	264	1723659	39.343	ng/u1	0.00
Target Compounds						
					Qvalue	
58) 2,3,4,6-Tetrachlorophenol	14.698	232	73179	9.450	ng/u1	99
71) Pentachlorophenol	16.474	266	896639	126.439	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080524\
Data File : BM046989.D
Acq On : 05 Aug 2024 12:18
Operator : RC/JU
Sample : P3171-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCVX2


Quant Time: Aug 05 12:55:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 03 02:51:11 2024
Response via : Initial Calibration

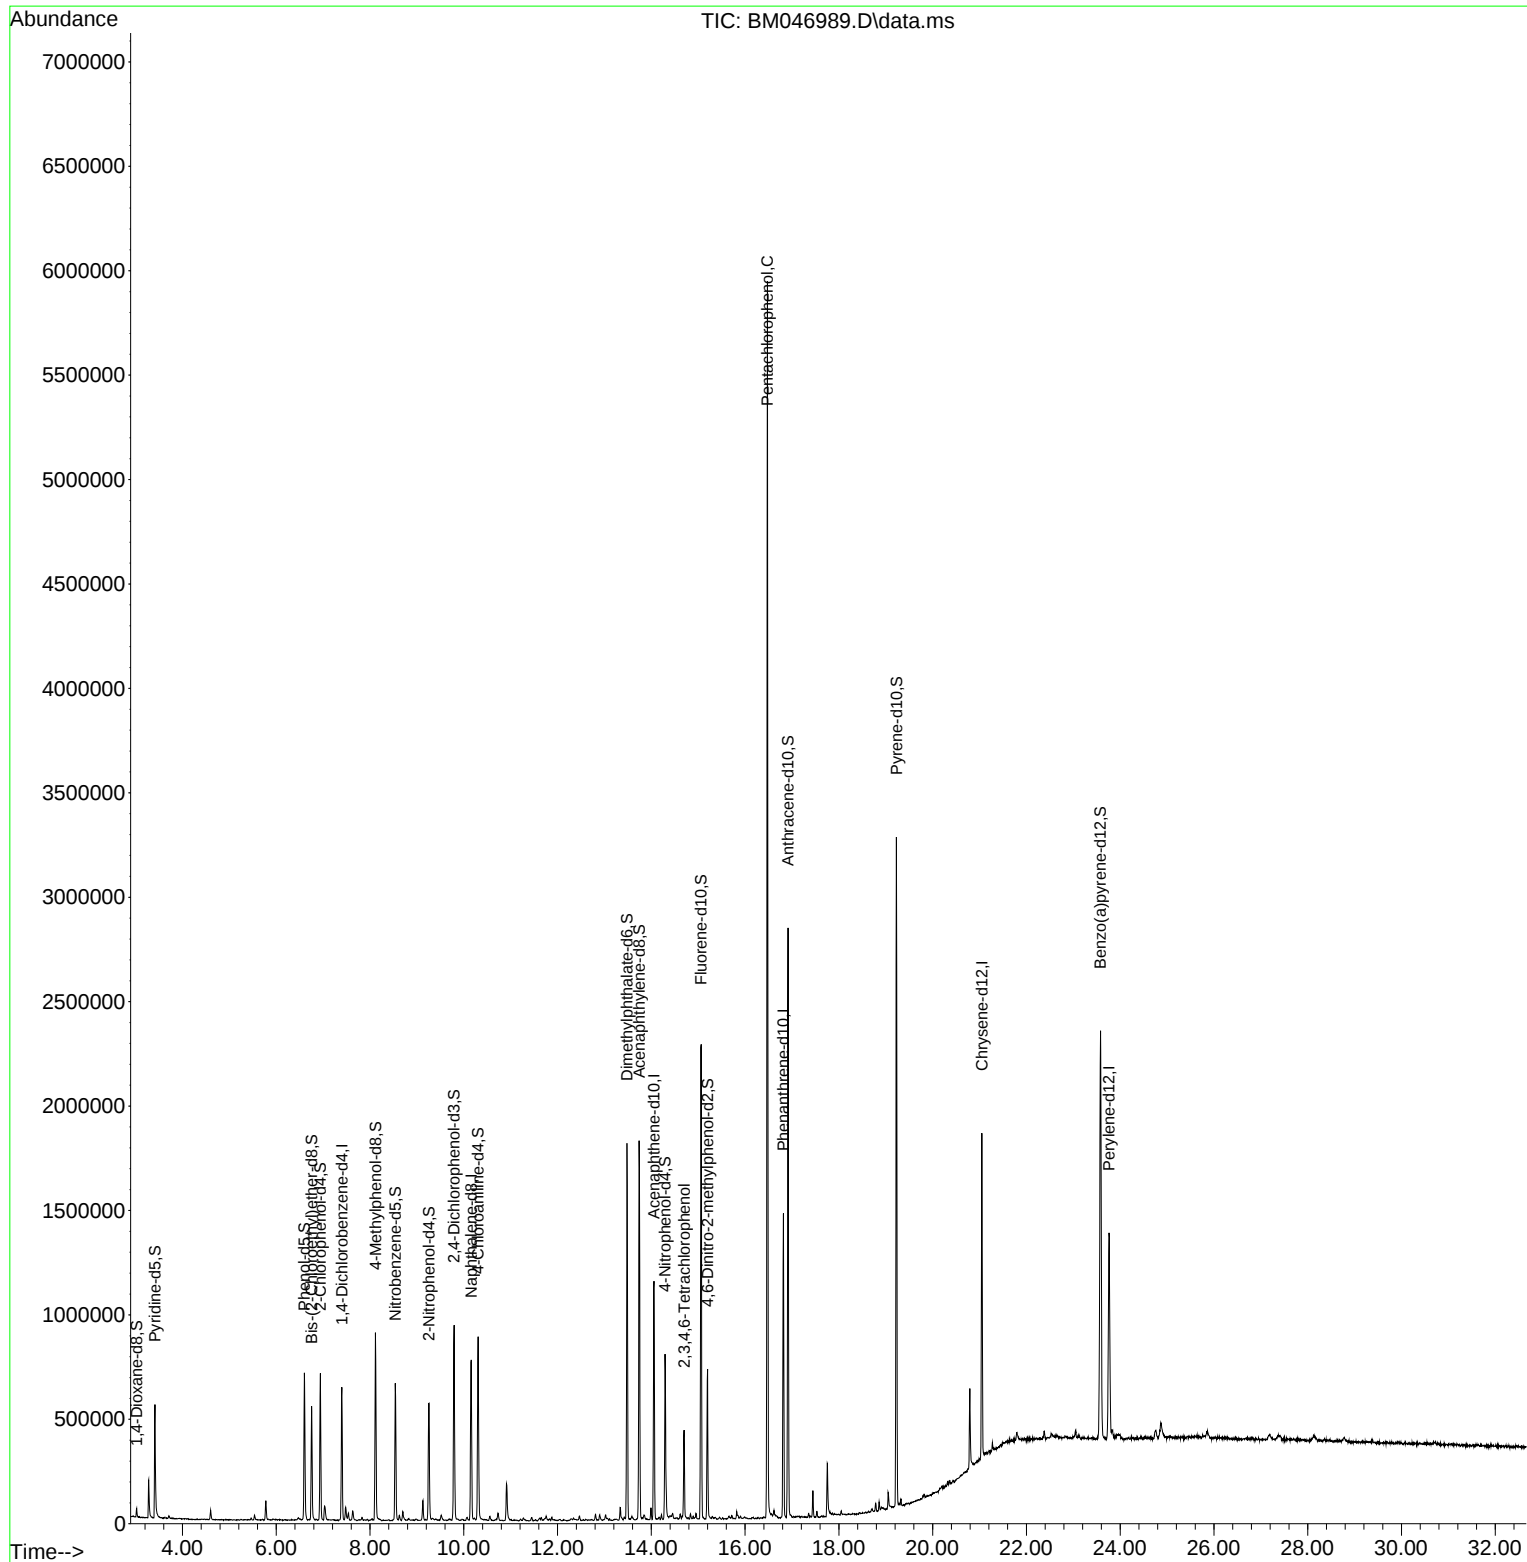



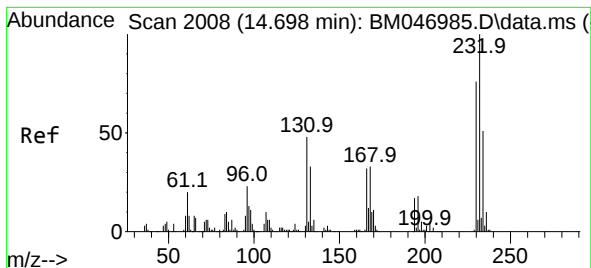


#58
2,3,4,6-Tetrachlorophenol
Concen: 9.450 ng/ul
RT: 14.698 min Scan# 2008
Delta R.T. -0.006 min
Lab File: BM046989.D
Acq: 05 Aug 2024 12:18


Instrument :
BNA_M
ClientSampleId :
DCVX2

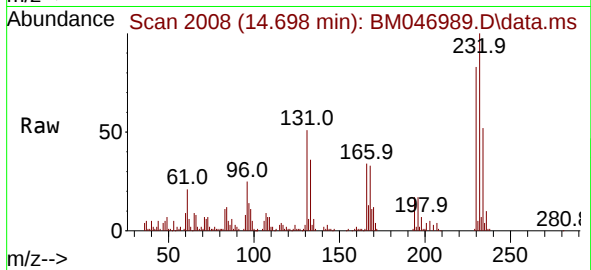

Tgt Ion:232 Resp: 73179
Ion Ratio Lower Upper
232 100
131 51.0 40.8 61.2
130 2.7 2.6 3.8
166 33.8 28.7 43.1

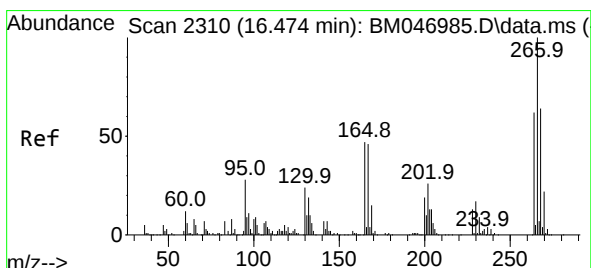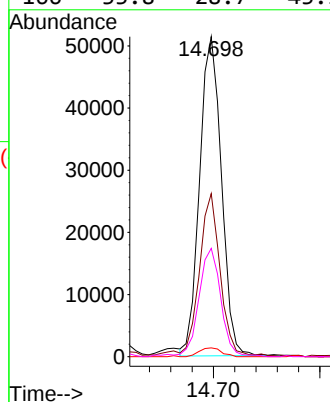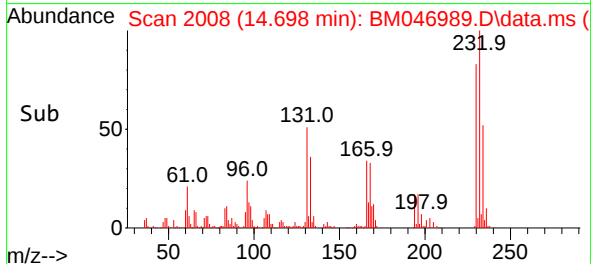

#71
Pentachlorophenol
Concen: 126.439 ng/ul
RT: 16.474 min Scan# 2310
Delta R.T. -0.006 min
Lab File: BM046989.D
Acq: 05 Aug 2024 12:18

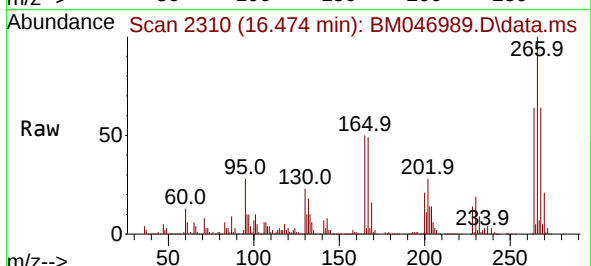

Tgt Ion:266 Resp: 896639
Ion Ratio Lower Upper
266 100
264 63.7 50.7 76.1
268 64.4 53.0 79.6

