

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080524\
 Data File : BM047002.D
 Acq On : 05 Aug 2024 21:59
 Operator : RC/JU
 Sample : P3329-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F7E24

Quant Time: Aug 06 01:58:15 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 03 02:51:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.398	152	190252	20.000	ng/u1	0.00
20) Naphthalene-d8	10.157	136	698641	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.051	164	435905	20.000	ng/u1	-0.01
64) Phenanthrene-d10	16.815	188	908587	20.000	ng/u1	0.00
79) Chrysene-d12	21.045	240	829065	20.000	ng/u1	-0.01
88) Perylene-d12	23.762	264	969913	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.022	96	12515	2.606	ng/uL	0.00
4) Pyridine-d5	3.410	84	205291	15.672	ng/u1	0.00
7) Phenol-d5	6.598	99	265509	18.371	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.751	67	179510	18.877	ng/u1	0.00
11) 2-Chlorophenol-d4	6.940	132	226182	18.475	ng/u1	0.00
15) 4-Methylphenol-d8	8.116	113	207365	18.112	ng/u1	0.00
21) Nitrobenzene-d5	8.539	128	104863	18.705	ng/u1	0.00
24) 2-Nitrophenol-d4	9.257	143	113471	18.534	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	9.792	165	207421	17.646	ng/u1	0.00
31) 4-Chloroaniline-d4	10.304	131	282787	18.305	ng/u1	0.00
46) Dimethylphthalate-d6	13.480	166	639228	19.179	ng/u1	0.00
49) Acenaphthylene-d8	13.739	160	714321	19.200	ng/u1	0.00
54) 4-Nitrophenol-d4	14.292	143	101958	15.821	ng/u1	0.00
60) Fluorene-d10	15.057	176	530916	18.621	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.192	200	81438	14.187	ng/u1	-0.01
73) Anthracene-d10	16.909	188	830249	19.276	ng/u1	0.00
81) Pyrene-d10	19.227	212	917493	19.332	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.574	264	959929	18.795	ng/u1	-0.01
Target Compounds						
					Qvalue	
30) Naphthalene	10.204	128	229103	6.194	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080524\
Data File : BM047002.D
Acq On : 05 Aug 2024 21:59
Operator : RC/JU
Sample : P3329-16
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7E24

Quant Time: Aug 06 01:58:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 03 02:51:11 2024
Response via : Initial Calibration

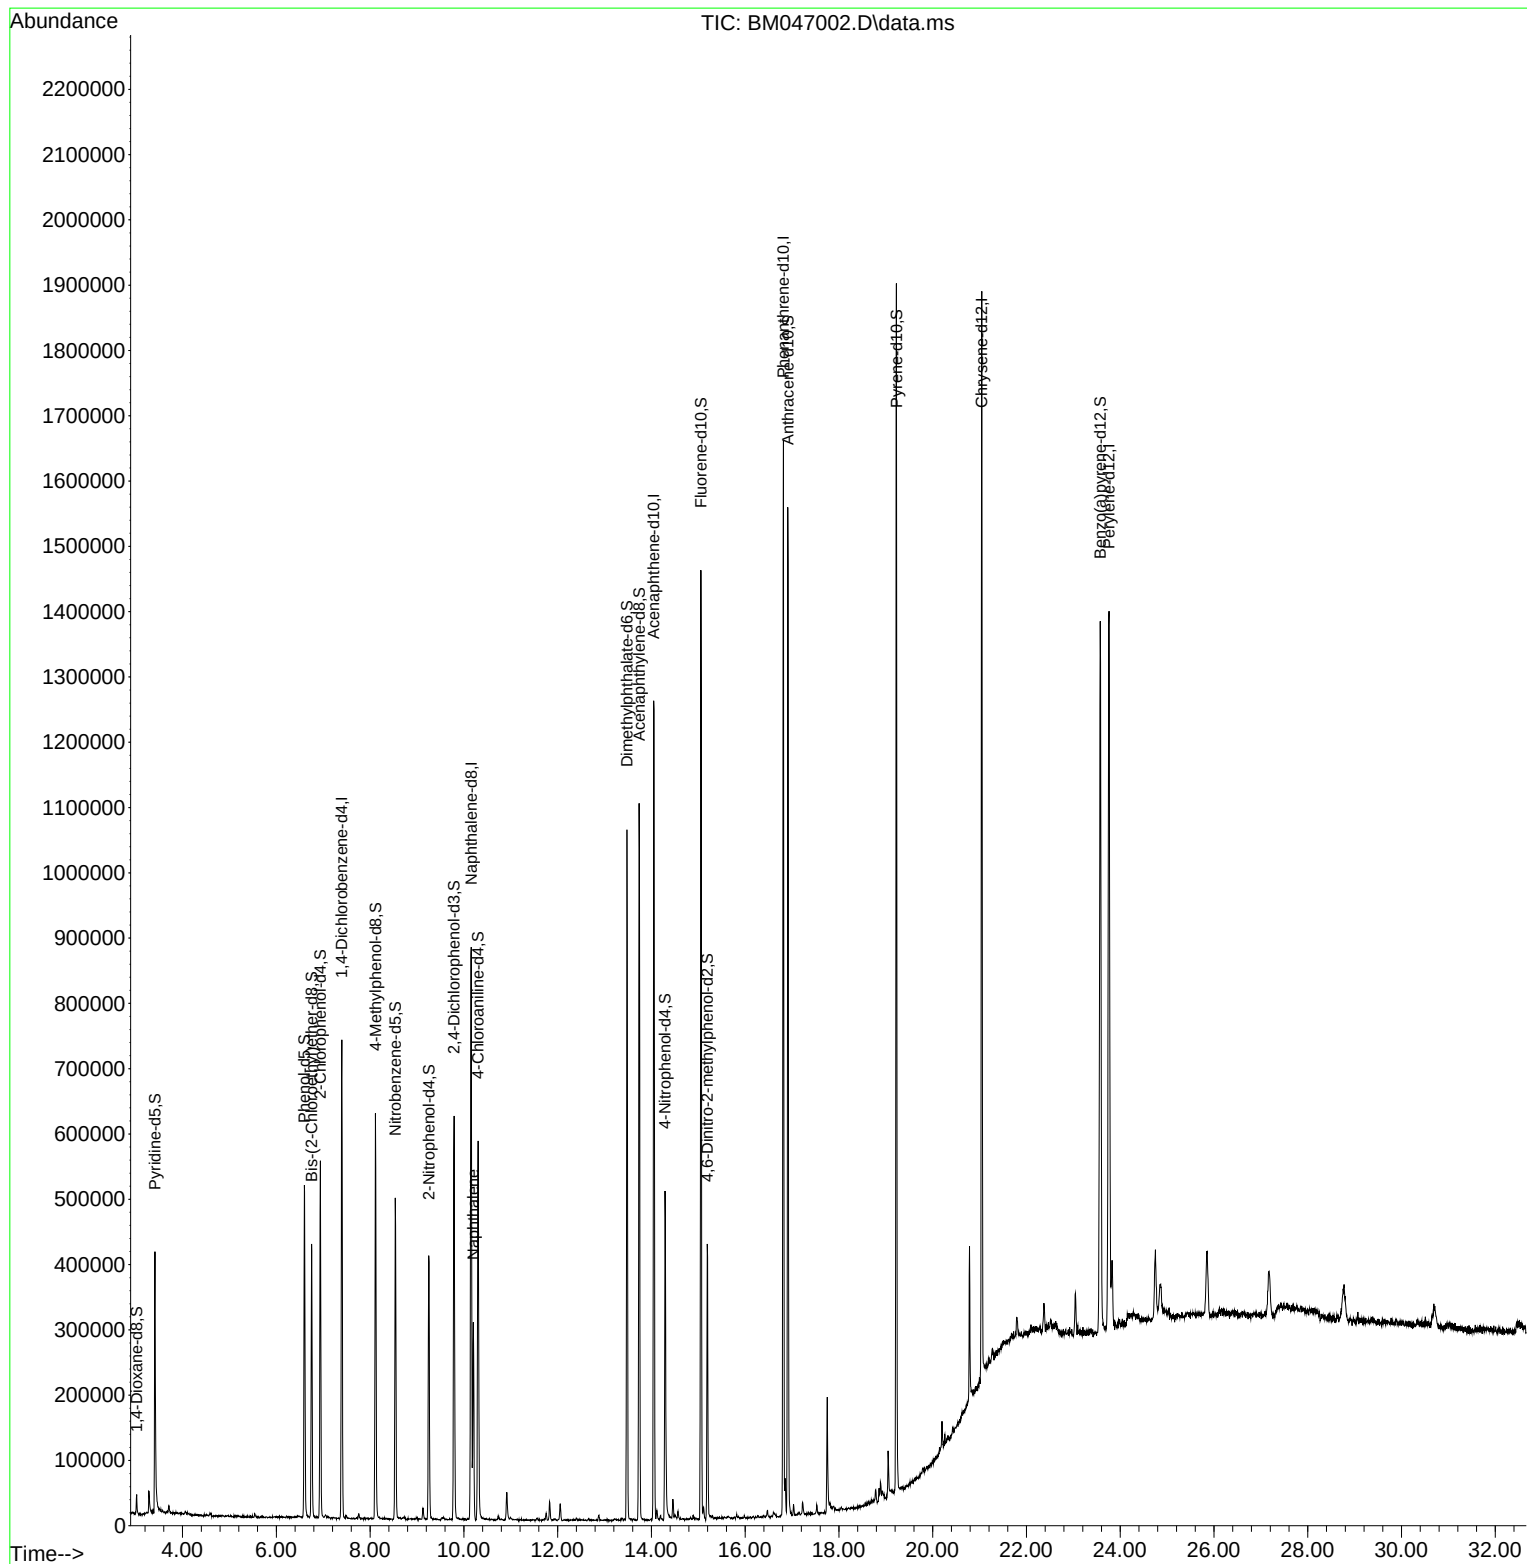

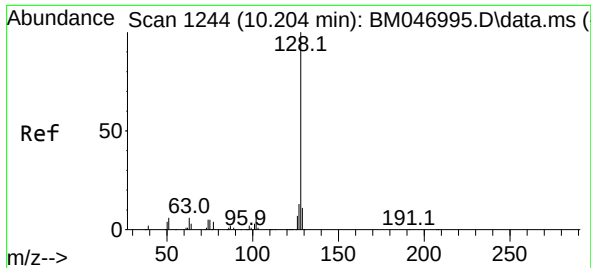

#30
Naphthalene
Concen: 6.194 ng/ul
RT: 10.204 min Scan# 11
Delta R.T. -0.006 min
Lab File: BM047002.D
Acq: 05 Aug 2024 21:59

Instrument :
BNA_M
ClientSampleId :
F7E24

Tgt Ion:128 Resp: 229103
Ion Ratio Lower Upper
128 100
129 11.3 8.6 13.0
127 13.6 10.4 15.6

