

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080524\
 Data File : BM047021.D
 Acq On : 06 Aug 2024 11:35
 Operator : RC/JU
 Sample : P3171-09
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCVX1

Quant Time: Aug 06 12:18:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 06 04:53:02 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.393	152	221718	20.000	ng/ul	0.00
20) Naphthalene-d8	10.151	136	842739	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.051	164	540643	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.810	188	1115259	20.000	ng/ul	0.00
79) Chrysene-d12	21.045	240	997478	20.000	ng/ul	0.00
88) Perylene-d12	23.756	264	1108404	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.016	96	20548	3.672	ng/uL	0.00
4) Pyridine-d5	3.411	84	259275	16.985	ng/ul	0.00
7) Phenol-d5	6.599	99	425267	25.249	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.752	67	271636	24.511	ng/ul	0.00
11) 2-Chlorophenol-d4	6.934	132	345256	24.199	ng/ul	0.00
15) 4-Methylphenol-d8	8.110	113	344040	25.785	ng/ul	0.00
21) Nitrobenzene-d5	8.540	128	169066	25.001	ng/ul	0.00
24) 2-Nitrophenol-d4	9.251	143	193719	26.232	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.787	165	350815	24.742	ng/ul	0.00
31) 4-Chloroaniline-d4	10.298	131	450447	24.173	ng/ul	0.00
46) Dimethylphthalate-d6	13.475	166	1087517	26.308	ng/ul	0.00
49) Acenaphthylene-d8	13.739	160	1215441	26.341	ng/ul	0.00
54) 4-Nitrophenol-d4	14.292	143	185574	23.218	ng/ul	0.00
60) Fluorene-d10	15.057	176	907398	25.660	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.192	200	141458	20.076	ng/ul	0.00
73) Anthracene-d10	16.910	188	1396679	26.417	ng/ul	0.00
81) Pyrene-d10	19.221	212	1581327	27.694	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.574	264	1604423	27.489	ng/ul	0.00
Target Compounds						
58) 2,3,4,6-Tetrachlorophenol	14.692	232	25024	2.349	ng/ul#	94
71) Pentachlorophenol	16.469	266	319991	33.251	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080524\
Data File : BM047021.D
Acq On : 06 Aug 2024 11:35
Operator : RC/JU
Sample : P3171-09
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCVX1

Quant Time: Aug 06 12:18:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 06 04:53:02 2024
Response via : Initial Calibration




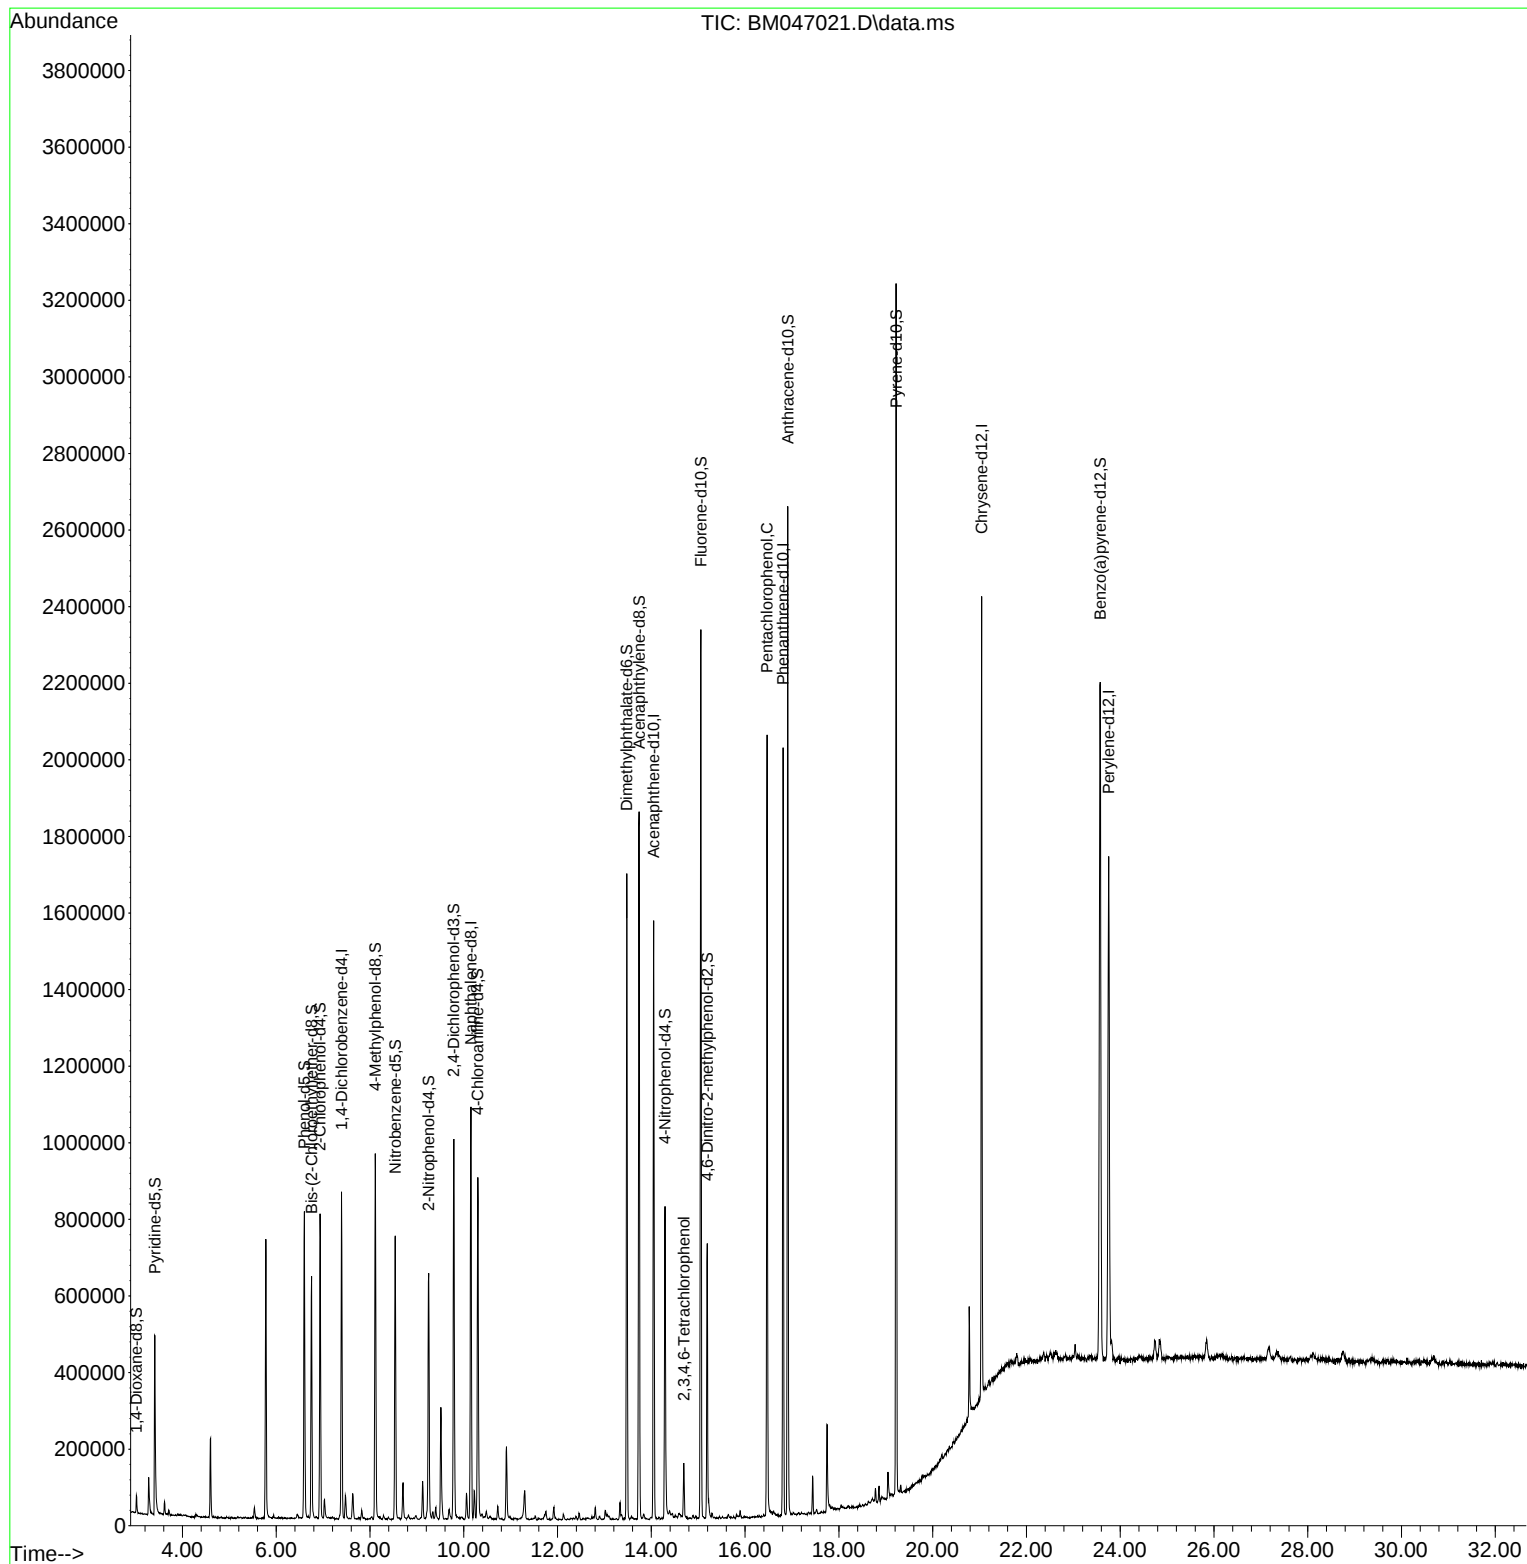


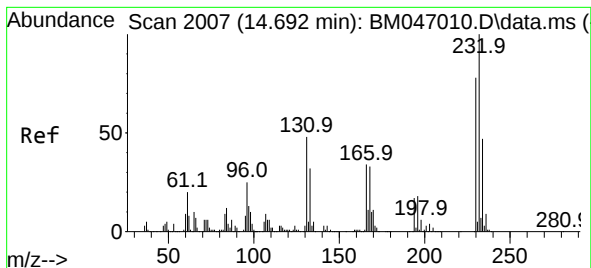

#58
2,3,4,6-Tetrachlorophenol
Concen: 2.349 ng/ul
RT: 14.692 min Scan# 2007
Delta R.T. 0.000 min
Lab File: BM047021.D
Acq: 06 Aug 2024 11:35

Instrument :
BNA_M
ClientSampleId :
DCVX1

Tgt Ion:	232	Resp:	25024
Ion Ratio	Lower	Upper	
232	100		
131	45.9	40.8	61.2
130	3.9	2.6	3.8#
166	32.8	28.7	43.1

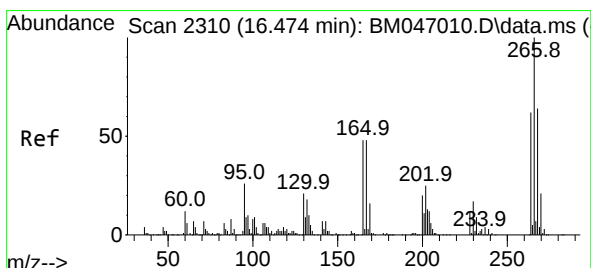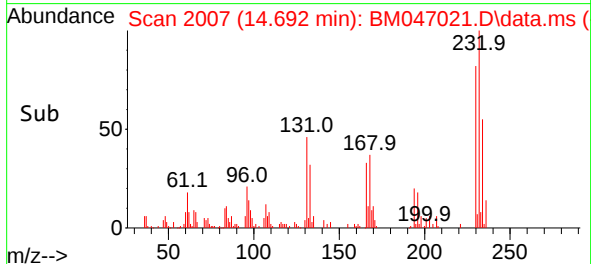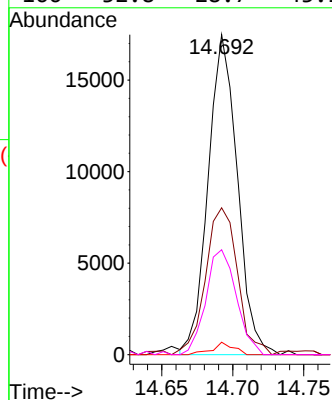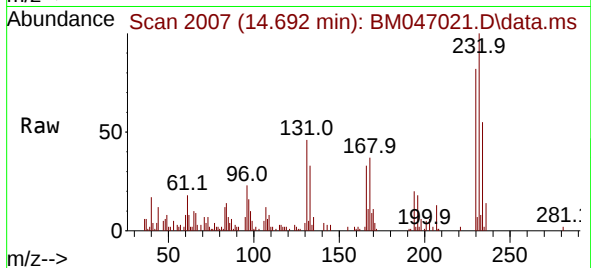

#71
Pentachlorophenol
Concen: 33.251 ng/ul
RT: 16.469 min Scan# 2309
Delta R.T. -0.006 min
Lab File: BM047021.D
Acq: 06 Aug 2024 11:35

Tgt Ion:	266	Resp:	319991
Ion Ratio	Lower	Upper	
266	100		
264	64.0	50.7	76.1
268	63.0	53.0	79.6

