

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080524\
 Data File : BM046986.D
 Acq On : 05 Aug 2024 09:47
 Operator : RC/JU
 Sample : PB162449BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK449

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM046986.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.016	18	22	28	rBV	53858	67228	2.06%	0.174%
2	3.293	67	69	71	rBV3	3776	3548	0.11%	0.009%
3	3.405	85	88	108	rBV	669982	927369	28.35%	2.405%
4	3.705	136	139	143	rVB	14657	16163	0.49%	0.042%
5	5.122	378	380	382	rBV3	3123	3548	0.11%	0.009%
6	6.540	615	621	622	rBV6	2666	3670	0.11%	0.010%
7	6.598	625	631	640	rVV	757157	1120451	34.25%	2.906%
8	6.751	651	657	668	rBV	595951	909926	27.81%	2.360%
9	6.940	682	689	696	rBV	730284	1121143	34.27%	2.908%
10	7.069	709	711	714	rBV4	2373	3338	0.10%	0.009%
11	7.240	738	740	742	rBV3	2913	3343	0.10%	0.009%
12	7.398	759	767	775	rBV	617168	963665	29.46%	2.499%
13	7.781	829	832	836	rVB5	1976	3369	0.10%	0.009%
14	8.116	882	889	903	rBV	834379	1335964	40.84%	3.465%
15	8.539	954	961	972	rBV	701429	1125226	34.40%	2.918%
16	9.004	1038	1040	1047	rVB7	2651	5583	0.17%	0.014%
17	9.251	1074	1082	1094	rBV	586567	925909	28.30%	2.401%
18	9.786	1165	1173	1188	rBV	840479	1397716	42.73%	3.625%
19	10.151	1228	1235	1242	rBV	789871	1268526	38.78%	3.290%
20	10.304	1253	1261	1275	rBV	799148	1393501	42.60%	3.614%
21	10.869	1353	1357	1361	rVB6	2165	3820	0.12%	0.010%
22	11.757	1503	1508	1519	rVB5	11348	27941	0.85%	0.072%
23	12.722	1667	1672	1675	rVV6	1885	3491	0.11%	0.009%
24	13.280	1764	1767	1769	rBV4	2350	3594	0.11%	0.009%
25	13.322	1771	1774	1779	rVB5	2398	4576	0.14%	0.012%
26	13.374	1779	1783	1785	rBV5	2161	3841	0.12%	0.010%
27	13.480	1794	1801	1813	rBV	1443477	1961815	59.97%	5.088%
28	13.739	1838	1845	1854	rBV	1584893	2266971	69.30%	5.879%
29	14.051	1892	1898	1907	rBV	1123046	1608234	49.16%	4.171%
30	14.292	1933	1939	1951	rBV	673148	1015476	31.04%	2.634%
31	14.469	1967	1969	1972	rBV3	3103	3314	0.10%	0.009%
32	14.839	2030	2032	2035	rBV4	3092	4187	0.13%	0.011%
33	15.057	2062	2069	2081	rBV	1964278	2749212	84.04%	7.130%
34	15.192	2086	2092	2102	rBV	689314	916377	28.01%	2.377%
35	15.298	2107	2110	2114	rVB2	9551	12700	0.39%	0.033%
36	15.845	2199	2203	2207	rBV6	5743	8353	0.26%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080524\
 Data File : BM046986.D
 Acq On : 05 Aug 2024 09:47
 Operator : RC/JU
 Sample : PB162449BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK449

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

37	16.415	2296	2300	2302	rBV5	1915	3302	0.10%	0.009%
38	16.498	2311	2314	2317	rVV5	4261	5624	0.17%	0.015%
39	16.815	2361	2368	2378	rBV	1317470	1868445	57.11%	4.846%
40	16.910	2378	2384	2395	rVV2	2163480	2949470	90.16%	7.650%
41	16.998	2397	2399	2404	rVB5	4164	5997	0.18%	0.016%
42	17.115	2416	2419	2421	rBV3	2554	3544	0.11%	0.009%
43	17.504	2483	2485	2489	rBV5	4343	6240	0.19%	0.016%
44	17.557	2492	2494	2497	rBV3	4564	6576	0.20%	0.017%
45	17.886	2548	2550	2552	rBV3	3513	3687	0.11%	0.010%
46	18.786	2699	2703	2708	rVB2	26419	38778	1.19%	0.101%
47	18.856	2712	2715	2720	rVB	24201	28493	0.87%	0.074%
48	19.227	2772	2778	2787	rBV	2389589	3266753	99.86%	8.472%
49	21.050	3083	3088	3097	rBV	1377921	1878943	57.44%	4.873%
50	23.574	3510	3517	3527	rVB2	1479600	3271382	100.00%	8.484%
51	23.762	3541	3549	3557	rBV	875871	2027097	61.96%	5.257%




Sum of corrected areas: 38557419

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080524\
Data File : BM046986.D
Acq On : 05 Aug 2024 09:47
Operator : RC/JU
Sample : PB162449BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK449

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

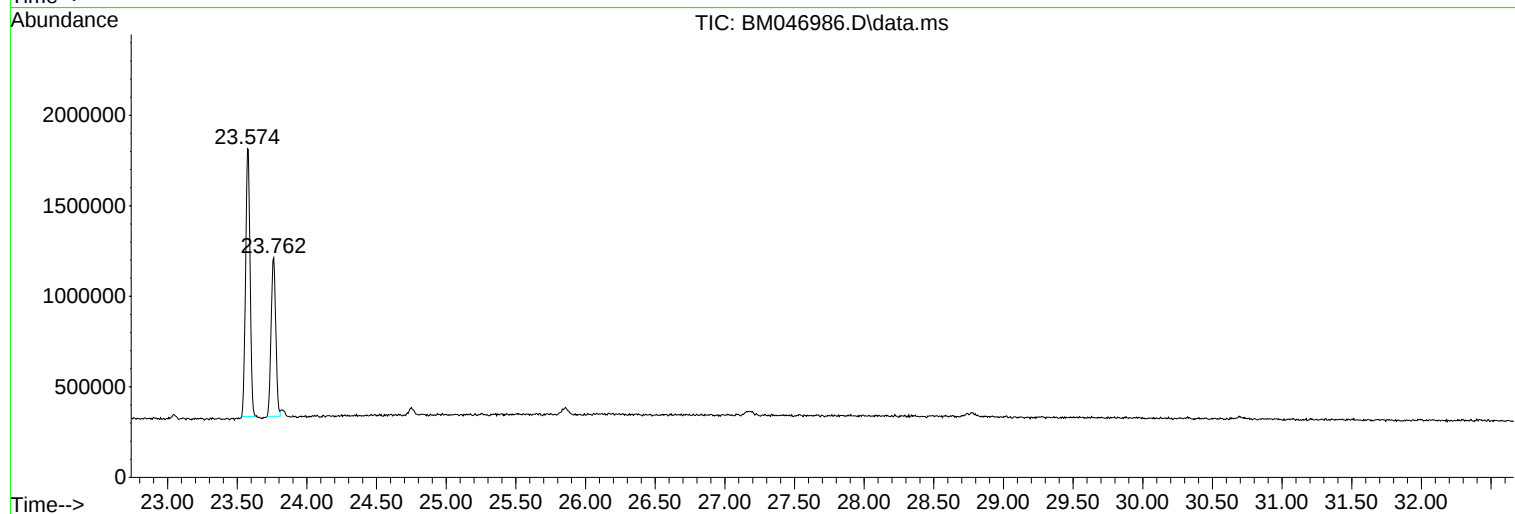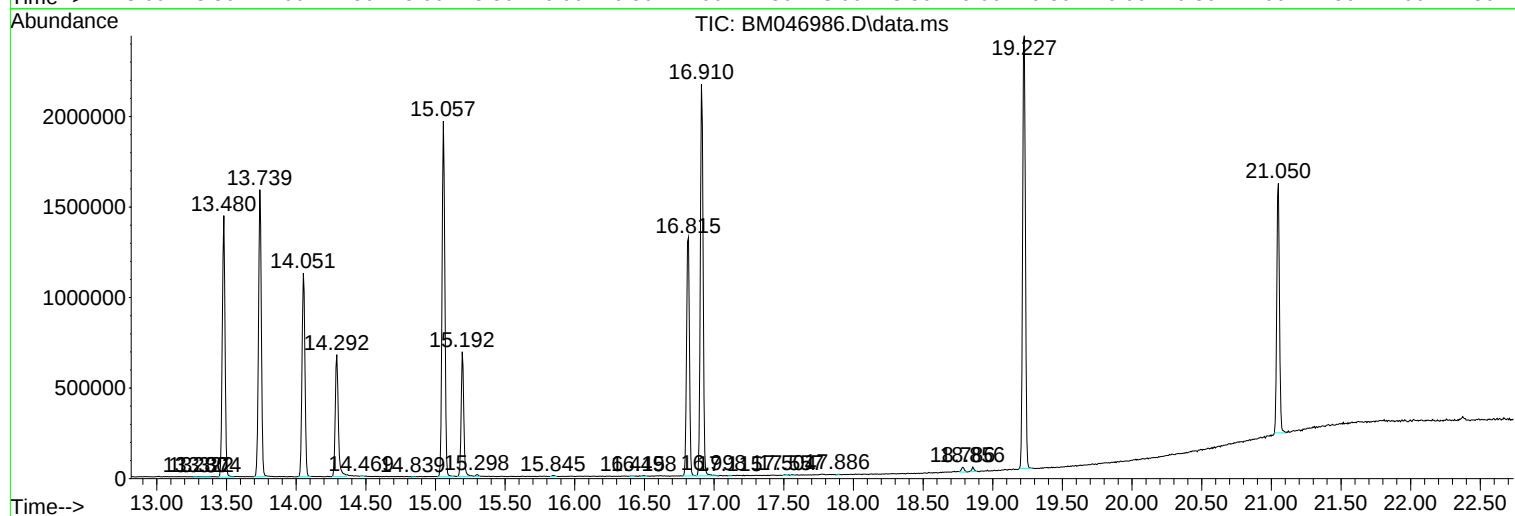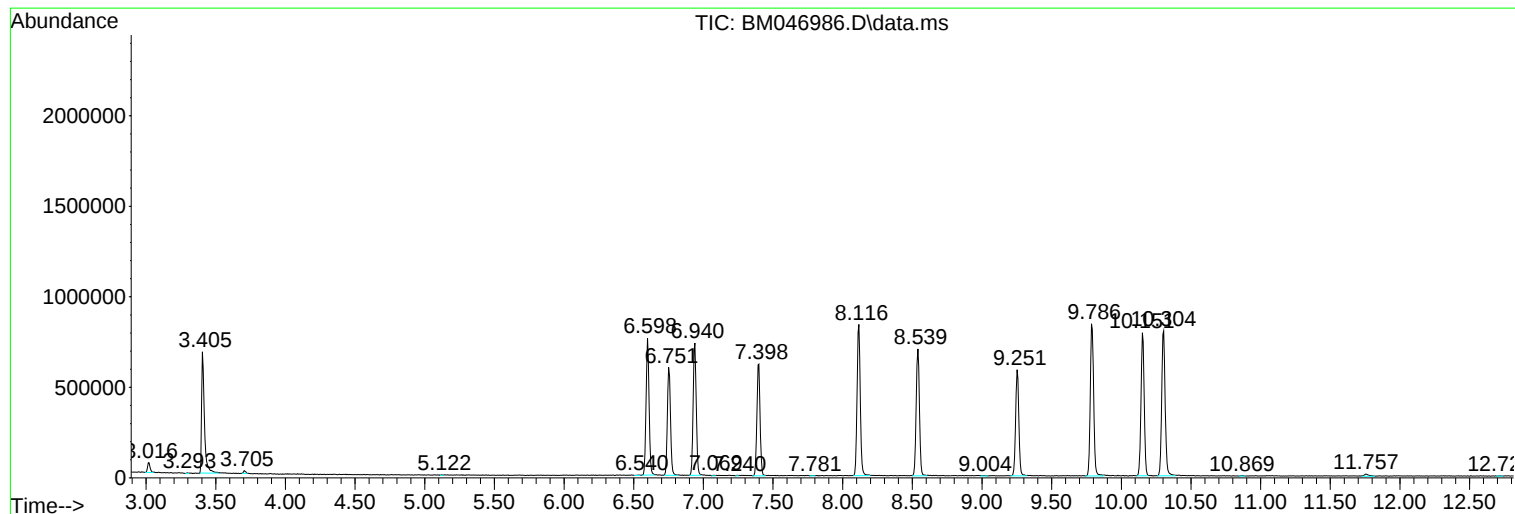

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080524\
Data File : BM046986.D
Acq On : 05 Aug 2024 09:47
Operator : RC/JU
Sample : PB162449BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK449

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080524\
Data File : BM046986.D
Acq On : 05 Aug 2024 09:47
Operator : RC/JU
Sample : PB162449BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK449

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------