

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080524\
 Data File : BM047012.D
 Acq On : 06 Aug 2024 05:30
 Operator : RC/JU
 Sample : PB162381BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK381

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM047012.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.022	19	23	30	rVB	57873	70122	1.69%	0.145%
2	3.404	85	88	108	rBV	726193	1061646	25.61%	2.189%
3	3.710	135	140	147	rVB	22837	32943	0.79%	0.068%
4	3.910	170	174	175	rBV4	4376	6331	0.15%	0.013%
5	6.598	624	631	641	rBV	854833	1302552	31.42%	2.685%
6	6.751	651	657	668	rBV	697507	1034583	24.95%	2.133%
7	6.940	681	689	703	rBV	841209	1326757	32.00%	2.735%
8	7.392	758	766	778	rBV	881069	1367441	32.98%	2.819%
9	8.010	868	871	877	rVB7	3053	4590	0.11%	0.009%
10	8.116	882	889	901	rBV	969832	1536802	37.07%	3.168%
11	8.539	953	961	972	rBV	804354	1278744	30.84%	2.636%
12	9.251	1076	1082	1093	rBV	674201	1068033	25.76%	2.202%
13	9.328	1093	1095	1098	rVV4	4073	5045	0.12%	0.010%
14	9.786	1165	1173	1189	rBV	976612	1599416	38.58%	3.297%
15	10.151	1228	1235	1245	rVB	1093279	1782418	42.99%	3.674%
16	10.298	1254	1260	1275	rBV	908681	1597844	38.54%	3.294%
17	11.751	1502	1507	1517	rVB2	14301	27646	0.67%	0.057%
18	13.016	1717	1722	1726	rBV6	3307	5866	0.14%	0.012%
19	13.480	1794	1801	1812	rBV	1693550	2278176	54.95%	4.696%
20	13.739	1838	1845	1860	rBV2	1798486	2601728	62.76%	5.363%
21	14.051	1891	1898	1905	rBV	1639239	2308587	55.68%	4.759%
22	14.292	1932	1939	1960	rBV	830938	1300020	31.36%	2.680%
23	15.057	2063	2069	2082	rBV	2260219	3177580	76.65%	6.550%
24	15.192	2086	2092	2104	rBV	718902	976102	23.54%	2.012%
25	15.298	2107	2110	2113	rVB4	10956	12399	0.30%	0.026%
26	15.633	2163	2167	2170	rVB5	2983	4358	0.11%	0.009%
27	15.751	2184	2187	2191	rBV5	3148	4360	0.11%	0.009%
28	15.845	2202	2203	2208	rVB4	5420	4958	0.12%	0.010%
29	16.480	2306	2311	2317	rBV8	3984	7217	0.17%	0.015%
30	16.598	2326	2331	2335	rBV3	4176	6733	0.16%	0.014%
31	16.809	2361	2367	2374	rBV	1976782	2752136	66.38%	5.673%
32	16.909	2377	2384	2399	rVB2	2574776	3535632	85.28%	7.288%
33	17.404	2463	2468	2470	rBV6	3290	5004	0.12%	0.010%
34	17.756	2524	2528	2534	rVB9	8403	12679	0.31%	0.026%
35	18.086	2583	2584	2591	rVB7	3349	4538	0.11%	0.009%
36	18.145	2591	2594	2596	rBV4	3792	4194	0.10%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080524\
Data File : BM047012.D
Acq On : 06 Aug 2024 05:30
Operator : RC/JU
Sample : PB162381BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK381

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Title : SVOA CALIBRATION

37	18.339	2626	2627	2630	rBV3	4616	4305	0.10%	0.009%
38	18.656	2677	2681	2683	rBV5	6841	11719	0.28%	0.024%
39	18.786	2699	2703	2707	rVB2	34499	48154	1.16%	0.099%
40	18.856	2711	2715	2719	rBV2	29036	41816	1.01%	0.086%
41	19.221	2771	2777	2787	rBV	2942950	3999847	96.48%	8.245%
42	21.044	3082	3087	3096	rBV	2234417	2932948	70.74%	6.046%
43	23.574	3509	3517	3530	rVB2	1907519	4145826	100.00%	8.546%
44	23.756	3540	3548	3556	rBV	1450585	3220140	77.67%	6.638%




Sum of corrected areas: 48509935

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080524\
Data File : BM047012.D
Acq On : 06 Aug 2024 05:30
Operator : RC/JU
Sample : PB162381BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK381

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

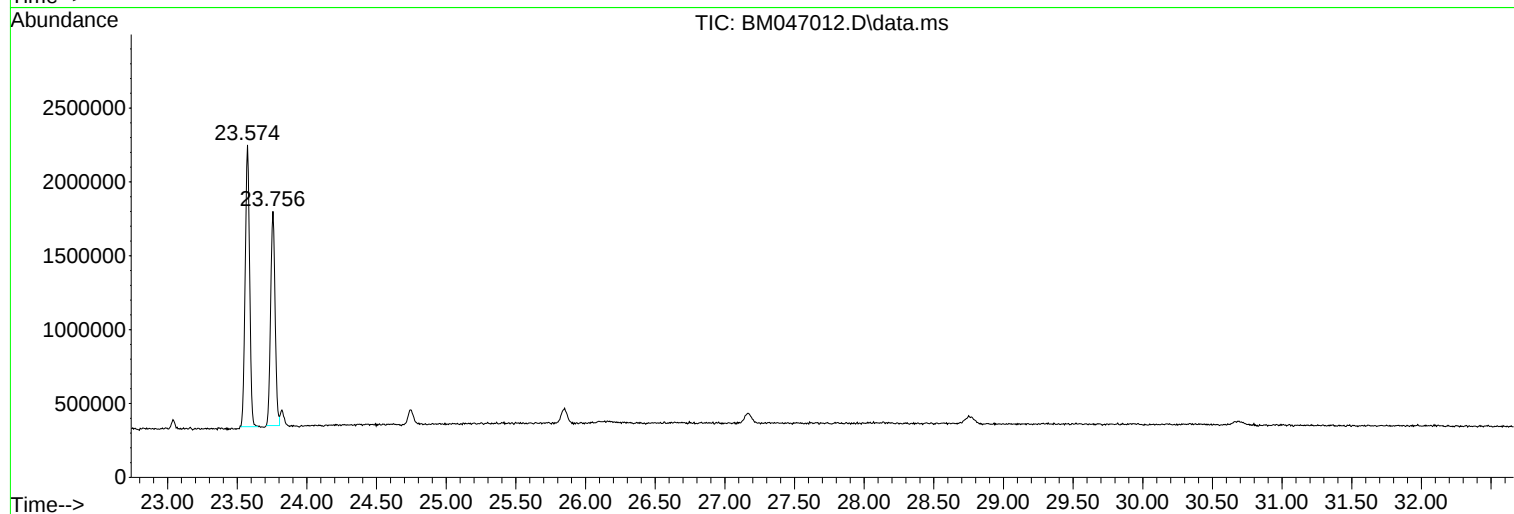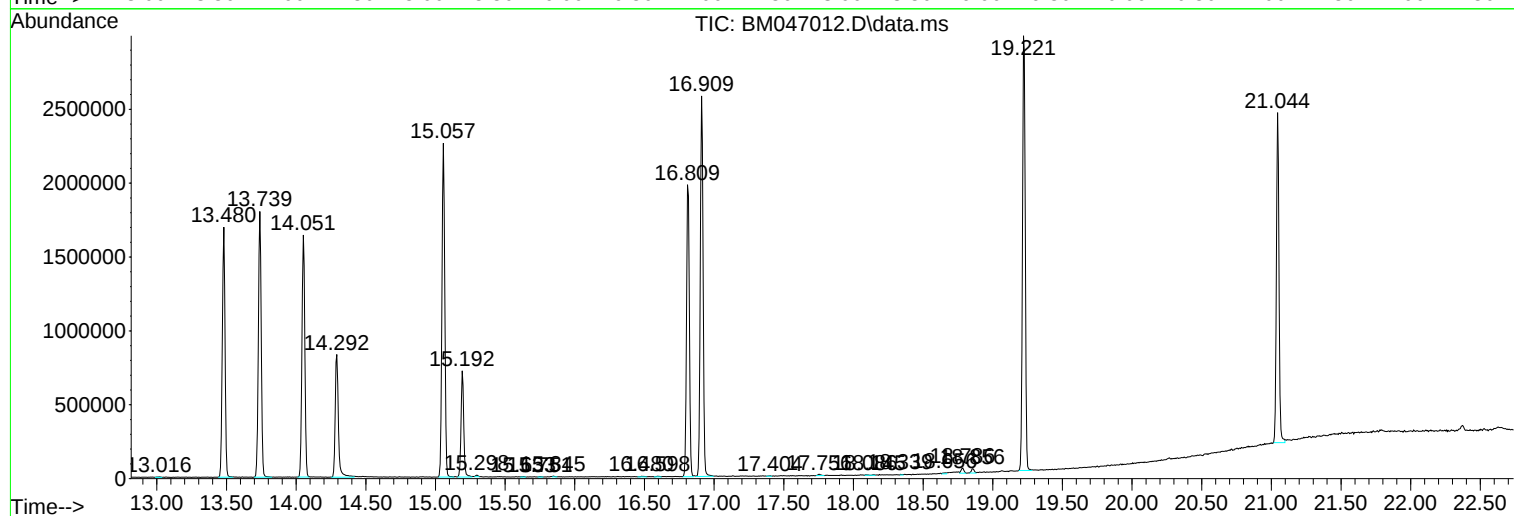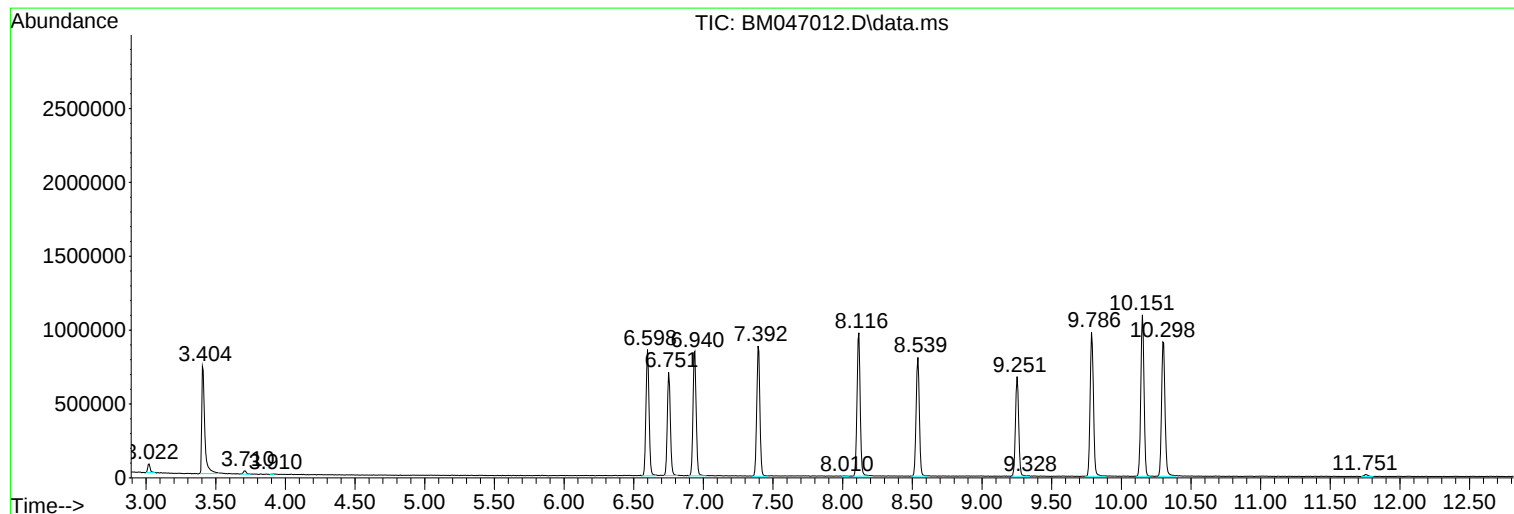

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080524\
Data File : BM047012.D
Acq On : 06 Aug 2024 05:30
Operator : RC/JU
Sample : PB162381BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK381

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080524\
Data File : BM047012.D
Acq On : 06 Aug 2024 05:30
Operator : RC/JU
Sample : PB162381BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK381

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM080224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc