

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080618\
 Data File : BM016207.D
 Acq On : 07 Aug 2018 00:49
 Operator : SJ/JU
 Sample : J4330-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 07 05:14:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM072318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 23 16:08:38 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	38592	20.00	ng	-0.07
21) Naphthalene-d8	10.99	136	145393	20.00	ng	-0.07
38) Acenaphthene-d10	14.80	164	75218	20.00	ng	-0.06
63) Phenanthrene-d10	17.53	188	159290	20.00	ng	-0.05
75) Chrysene-d12	21.66	240	168970	20.00	ng	-0.04
86) Perylene-d12	24.01	264	180521	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.69	112	98023	42.19	ng	-0.05
7) Phenol-d6	7.33	99	73256	24.14	ng	-0.05
23) Nitrobenzene-d5	9.36	82	315101	100.80	ng	-0.06
41) 2,4,6-Tribromophenol	16.29	330	84689	88.77	ng	-0.05
44) 2-Fluorobiphenyl	13.42	172	573415	92.76	ng	-0.06
78) Terphenyl-d14	20.11	244	840018	104.07	ng	-0.05
Target Compounds						
15) Benzyl Alcohol	8.49	79	5042	2.087	ng	Qvalue # 36
49) Dimethylphthalate	14.26	163	15775	2.396	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080618\
Data File : BM016207.D
Acq On : 07 Aug 2018 00:49
Operator : SJ/JU
Sample : J4330-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Aug 07 05:14:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 23 16:08:38 2018
Response via : Initial Calibration

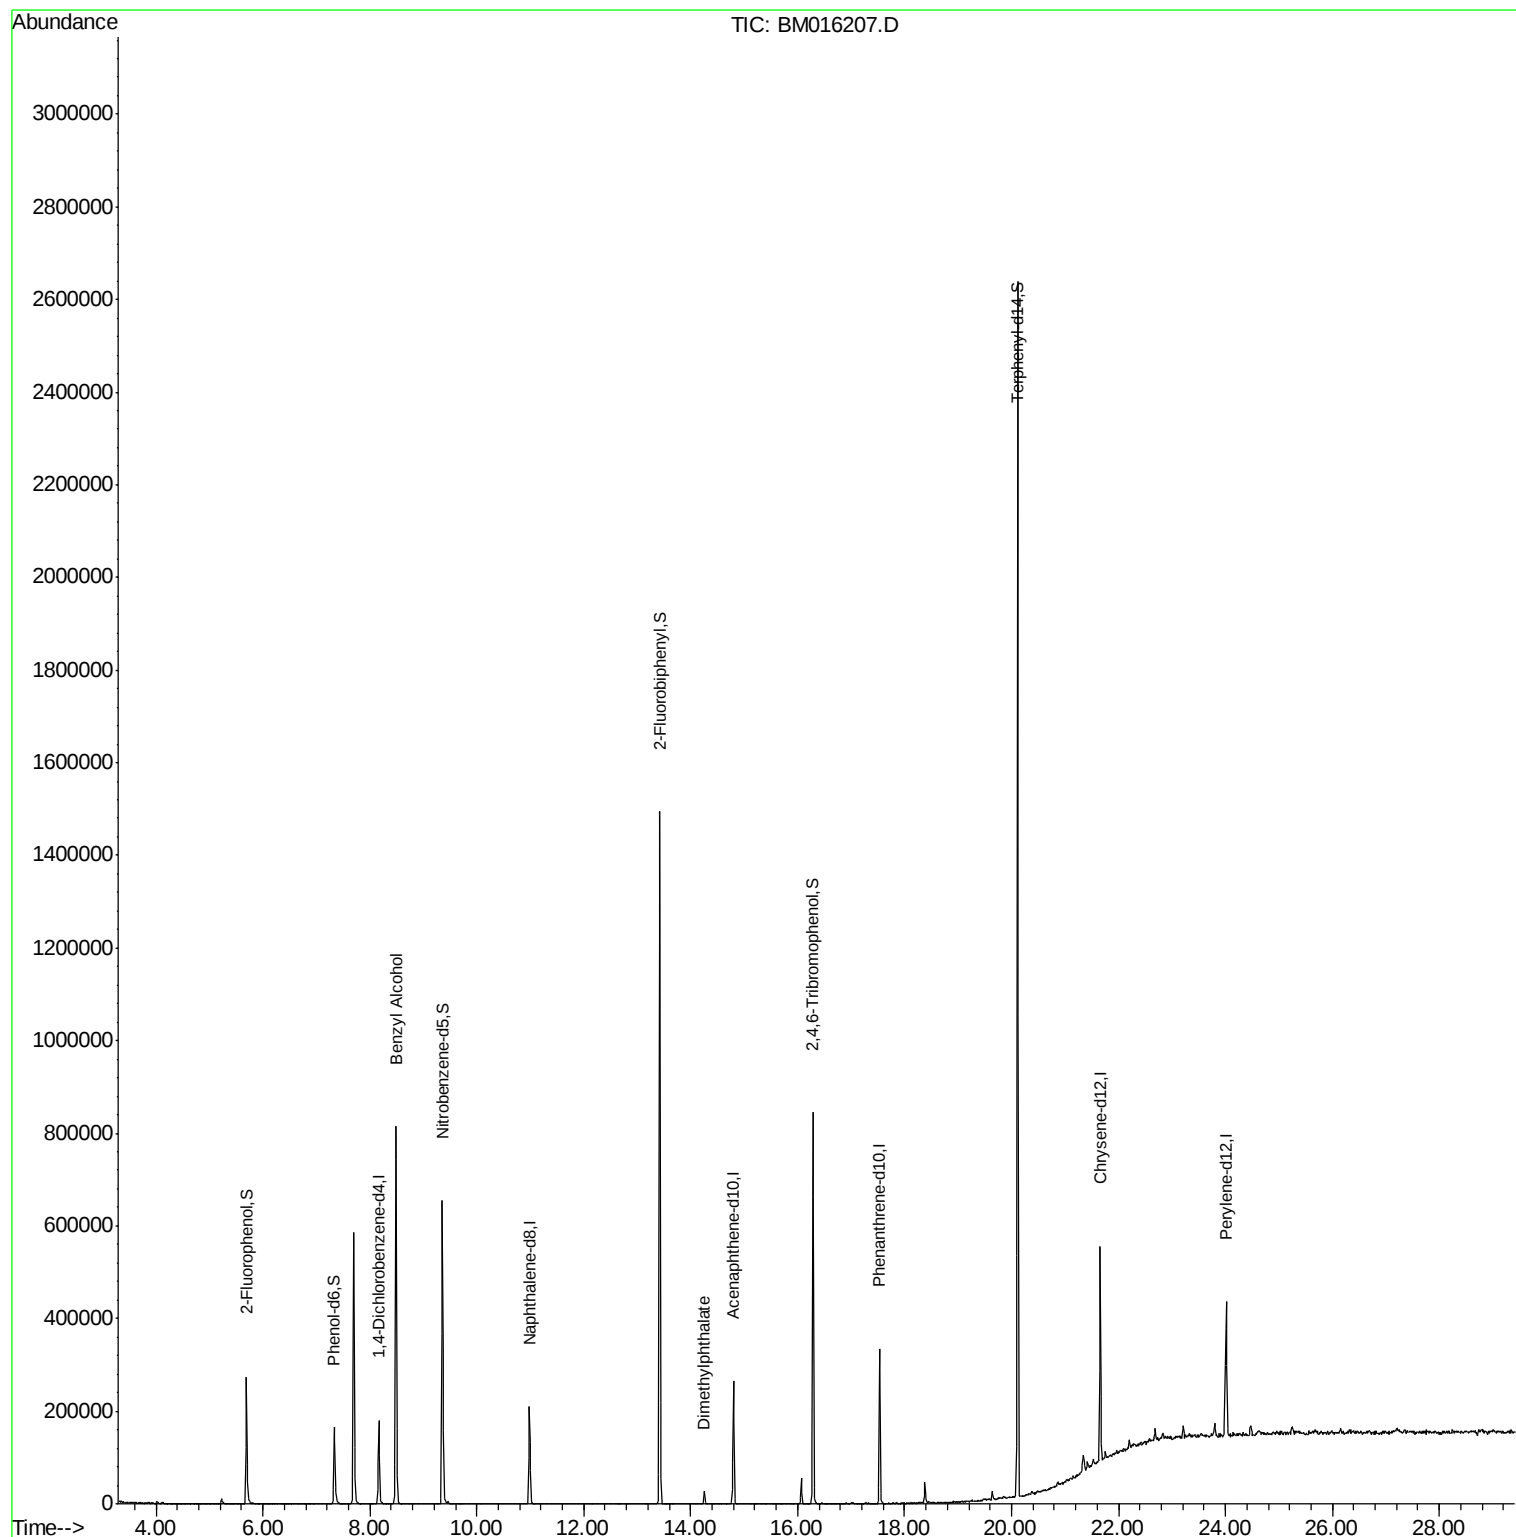

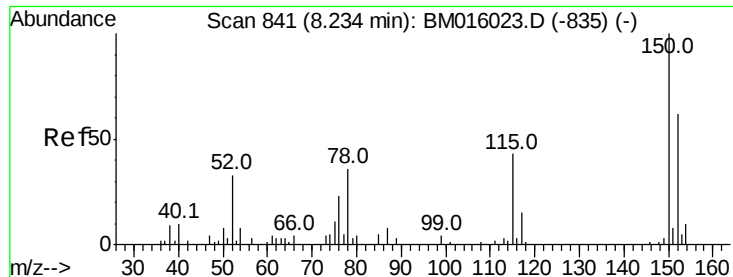


#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.17 min Scan# 830
 Delta R.T. -0.07 min
 Lab File: BM016207.D
 Acq: 07 Aug 2018 00:49

Instrument :
 BNA_M
 ClientSampled :

Tot Ion	Ratio	Lower	Upper
152	100		
150	151.4	119.5	179.3
115	63.5	43.0	64.4

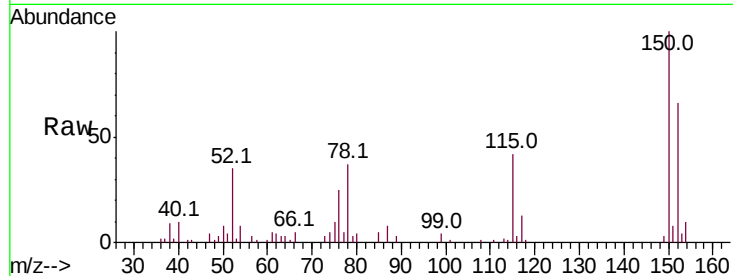


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

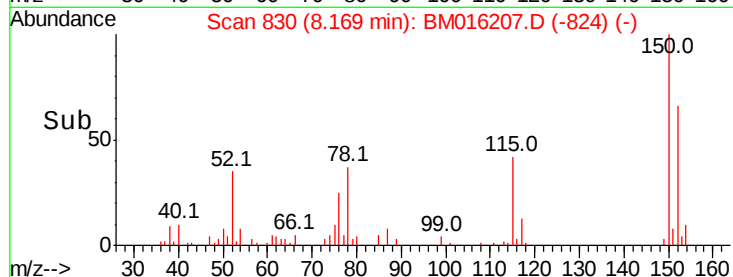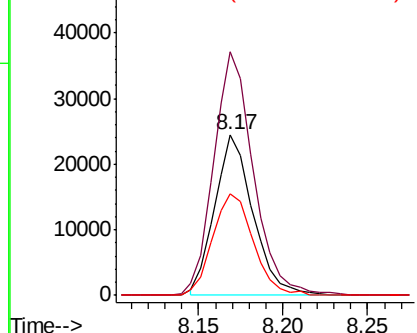



#5

2-Fluorophenol
 Concen: Below ng
 RT: 5.69 min Scan# 409
 Delta R.T. -0.05 min
 Lab File: BM016207.D
 Acq: 07 Aug 2018 00:49

Tgt Ion	Ratio	Lower	Upper
112	100		
64	63.6	38.6	57.8#
63	44.9	19.3	28.9#

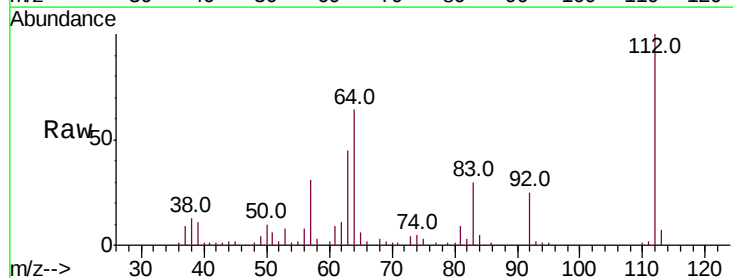

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BM0
 Ion 63.00 (62.70 to 63.70): BM0

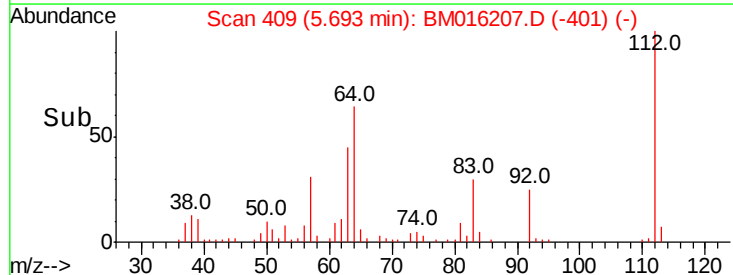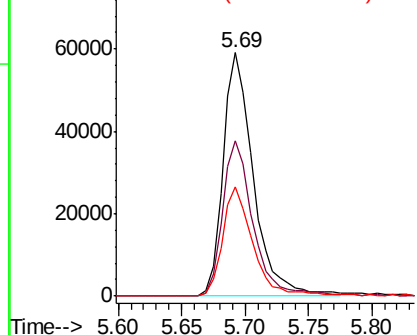



#7

Phenol-d6

Concen: N.D. ng

RT: 7.33 min Scan# 688

Delta R.T. -0.05 min

Lab File: BM016207.D

Acq: 07 Aug 2018 00:49

Instrument :

BNA_M

ClientSampled :


Tot Ion: 99 Resp: 73256

Ion Ratio Lower Upper

99 100

42 35.1 11.0 16.4#




71 53.8 23.4 35.2#

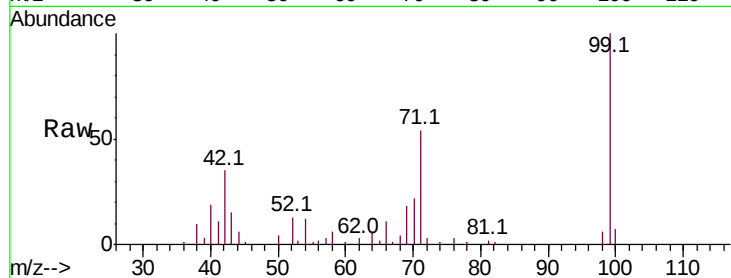

Abundance Ion 99.00 (98.70 to 99.70): BM016207.D (-680) (-)

Ion 42.00 (41.70 to 42.70): BM016207.D (-680) (-)

Ion 71.00 (70.70 to 71.70): BM016207.D (-680) (-)

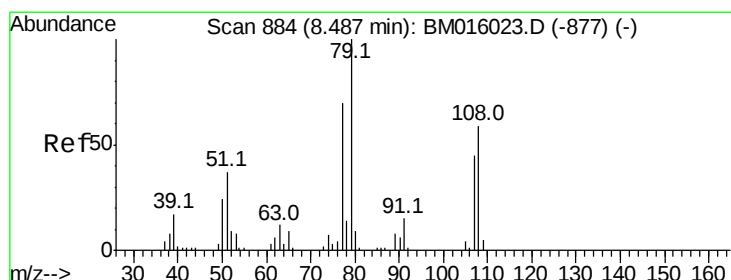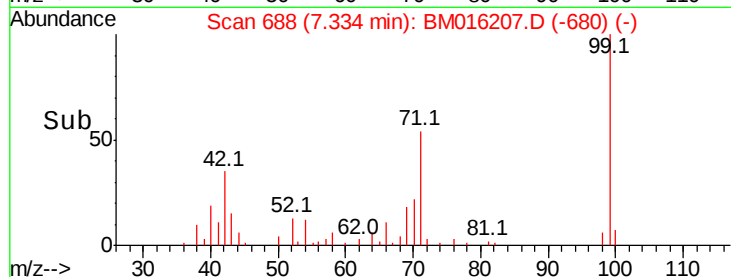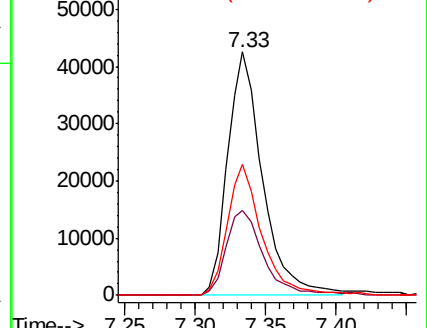

#15

Benzyl Alcohol

Concen: 2.087 ng

RT: 8.49 min Scan# 885

Delta R.T. 0.01 min

Lab File: BM016207.D

Acq: 07 Aug 2018 00:49


Tgt Ion: 79 Resp: 5042

Ion Ratio Lower Upper

79 100

108 77.1 65.0 97.4



77 175.9 53.0 79.6#

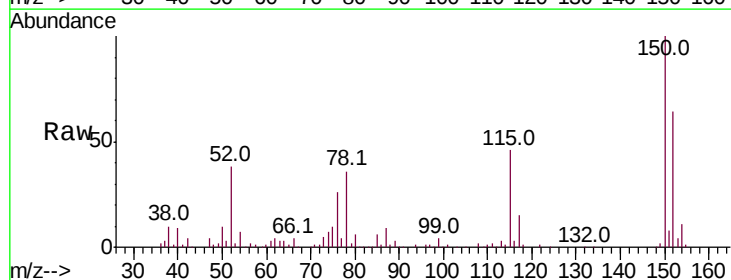

Abundance Ion 79.00 (78.70 to 79.70): BM016207.D (-867) (-)

Ion 108.00 (107.70 to 108.70): BM016207.D (-867) (-)

Ion 77.00 (76.70 to 77.70): BM016207.D (-867) (-)



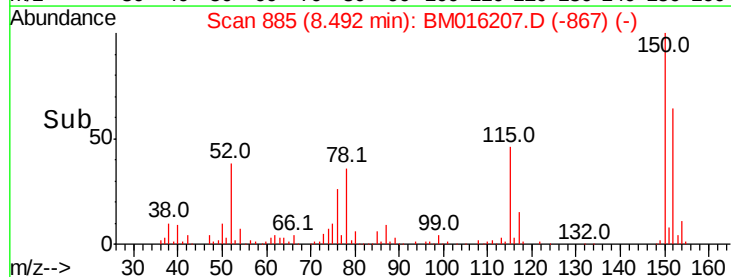
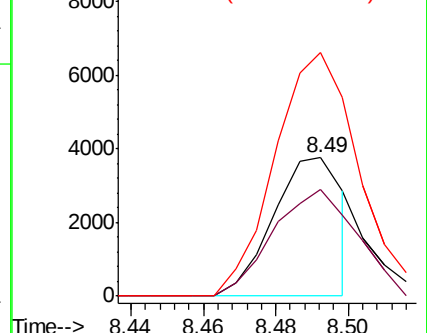




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.99 min Scan# 1309
Delta R.T. -0.07 min
Lab File: BM016207.D
Acq: 07 Aug 2018 00:49




Instrument :
BNA_M
ClientSampleId :


Tot Ion:	136	Resp:	145393
Ion	Ratio	Lower	Upper
136	100		
137	11.2	8.7	13.1
54	9.3	4.6	6.8#
68	4.3	3.7	5.5

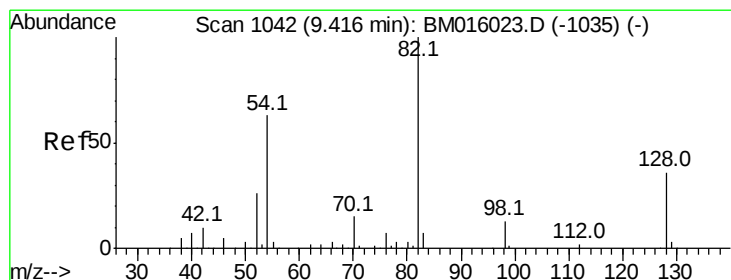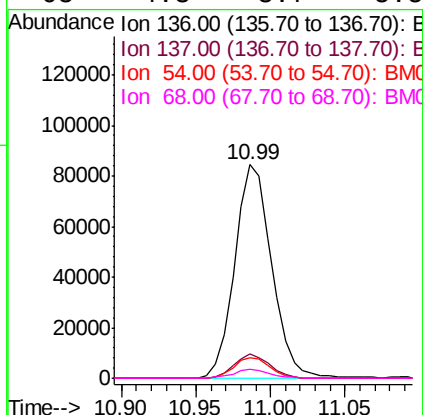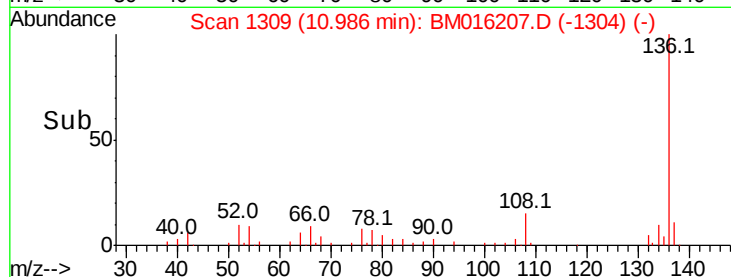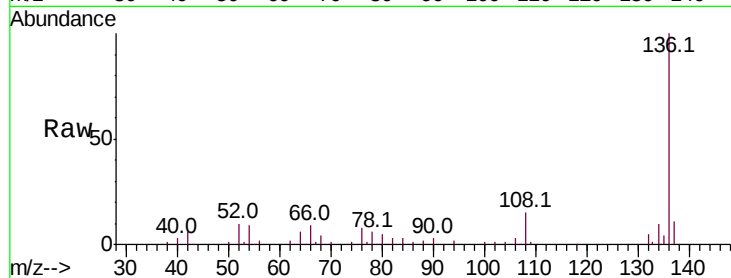

#23
Nitrobenzene-d5
Concen: N.D. ng
RT: 9.36 min Scan# 1032
Delta R.T. -0.06 min
Lab File: BM016207.D
Acq: 07 Aug 2018 00:49

Tgt Ion:	82	Resp:	315101
Ion	Ratio	Lower	Upper
82	100		
128	36.7	32.8	49.2
54	63.1	40.6	60.8#

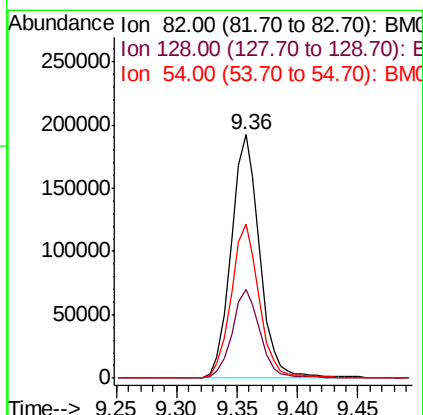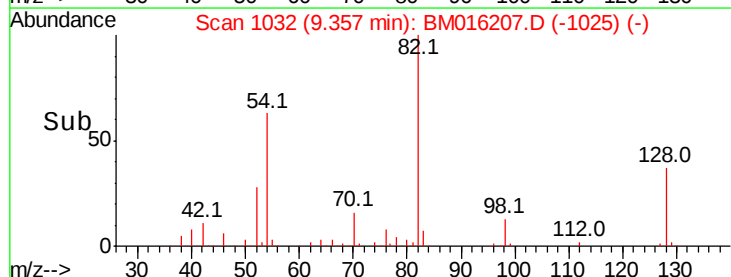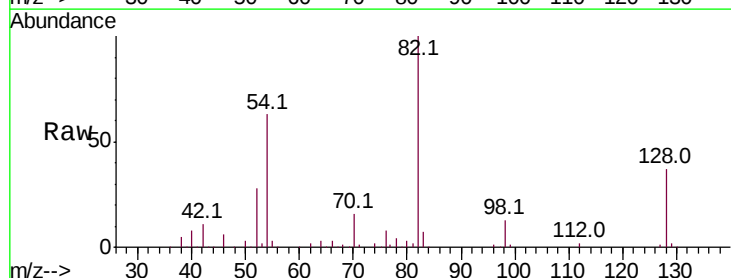

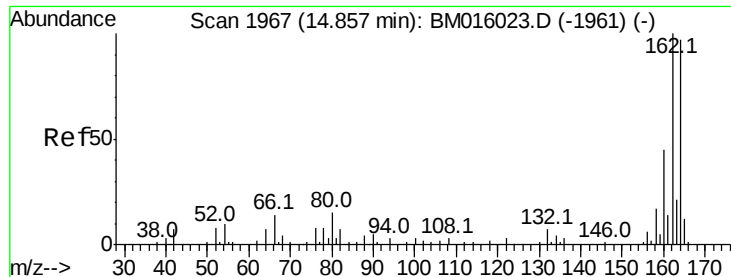

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.80 min Scan# 1957

Delta R.T. -0.06 min

Lab File: BM016207.D

Acq: 07 Aug 2018 00:49

Instrument :

BNA_M

ClientSampleId :


Tot Ion:164 Resp: 75218

Ion Ratio Lower Upper

164 100

162 107.6 82.4 123.6




160 49.1 35.8 53.6

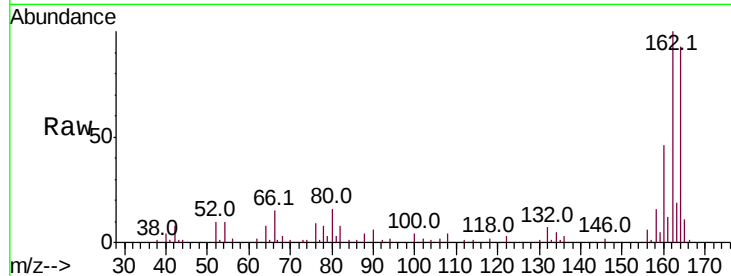

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

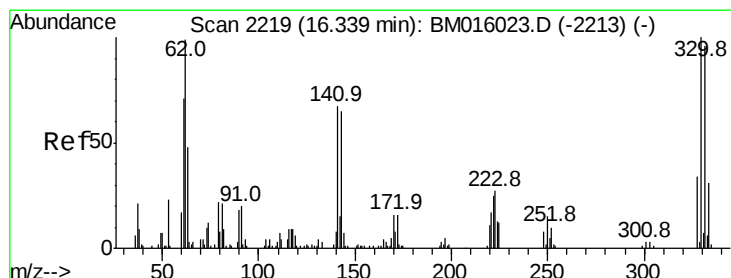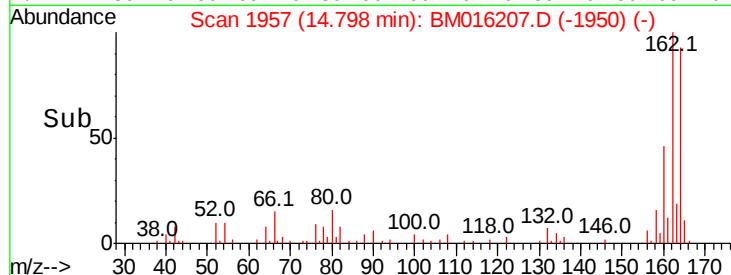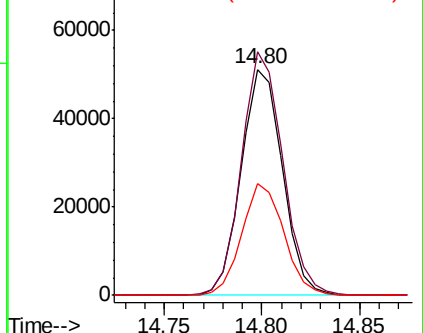

#41

2,4,6-Tribromophenol

Concen: N.D. ng

RT: 16.29 min Scan# 2210

Delta R.T. -0.05 min

Lab File: BM016207.D

Acq: 07 Aug 2018 00:49


Tgt Ion:330 Resp: 84689

Ion Ratio Lower Upper

330 100

332 96.8 0.0 0.0#



141 76.5 0.0 0.0#

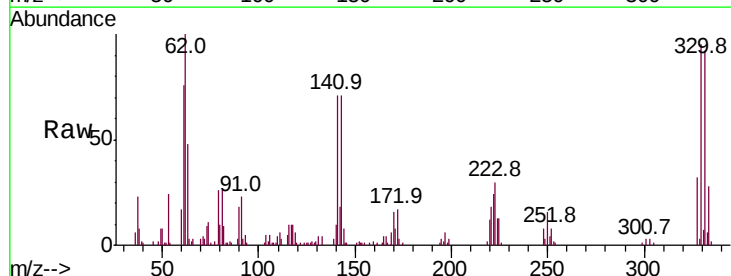


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



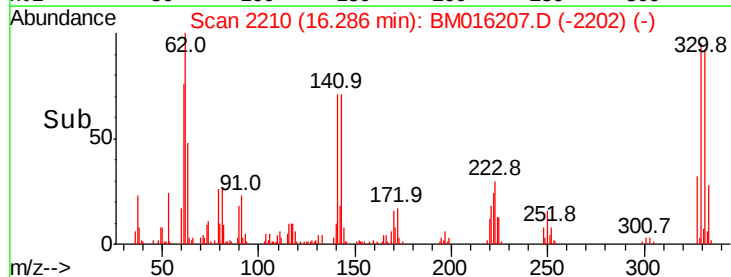
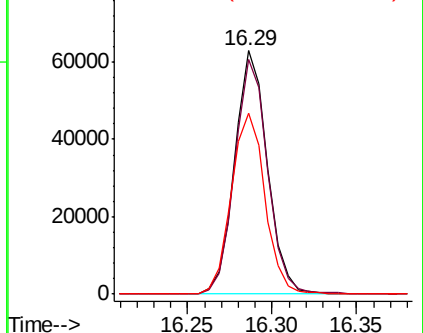


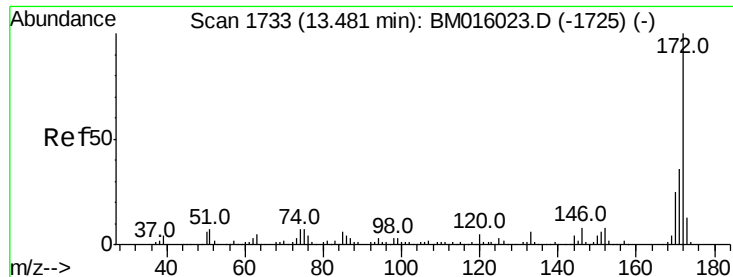

#44
 2-Fluorobiphenyl
 Concen: N.D. na
 RT: 13.42 min Scan# 1723
 Delta R.T. -0.06 min
 Lab File: BM016207.D
 Acq: 07 Aug 2018 00:49




Instrument :
 BNA_M
 ClientSampled :


Tot Ion:172 Resp: 573415
 Ion Ratio Lower Upper
 172 100
 171 36.4 28.5 42.7
 170 24.1 18.8 28.2

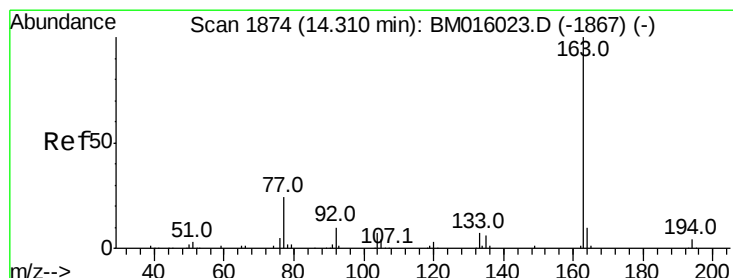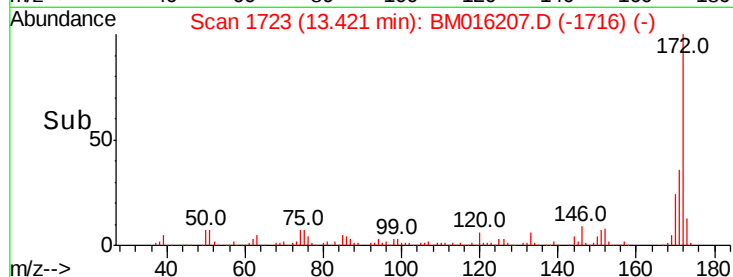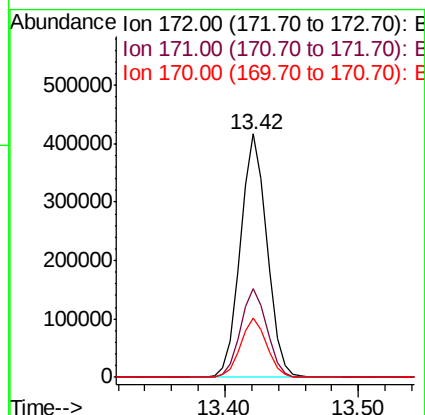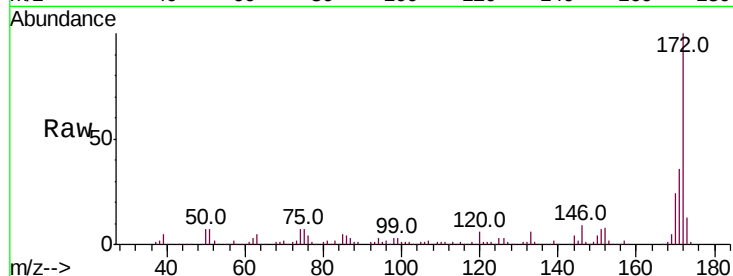

#49
 Dimethylphthalate
 Concen: 2.396 ng
 RT: 14.26 min Scan# 1865
 Delta R.T. -0.05 min
 Lab File: BM016207.D
 Acq: 07 Aug 2018 00:49

Tgt Ion:163 Resp: 15775
 Ion Ratio Lower Upper
 163 100
 194 3.8 2.7 4.1
 164 11.6 8.2 12.2

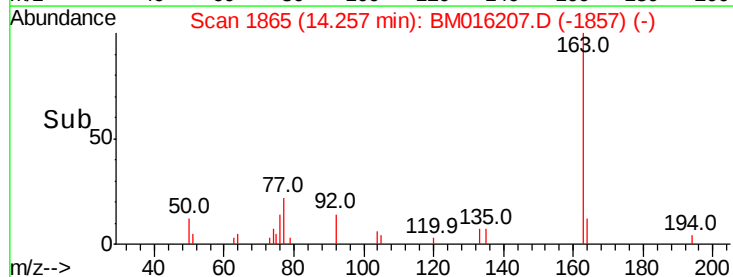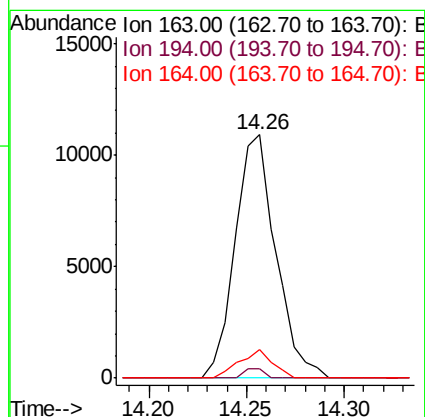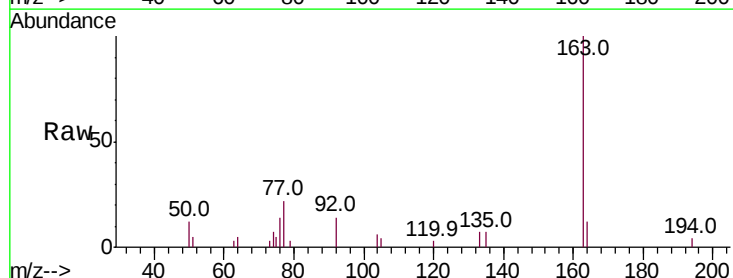


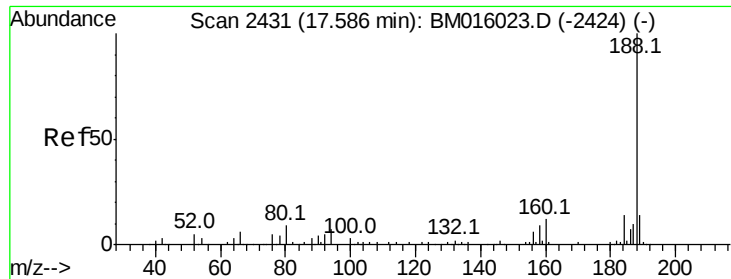




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.53 min Scan# 2422
Delta R.T. -0.05 min
Lab File: BM016207.D
Acq: 07 Aug 2018 00:49

Instrument :
BNA_M
ClientSampleId :

Tot Ion:188 Resp: 159290
Ion Ratio Lower Upper
188 100
94 7.0 8.7 13.1#
80 8.9 9.3 13.9#

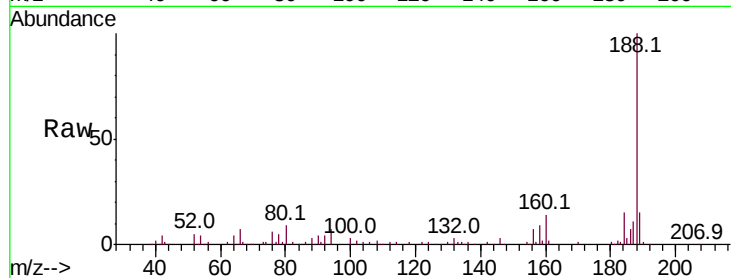


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM
Ion 80.00 (79.70 to 80.70): BM

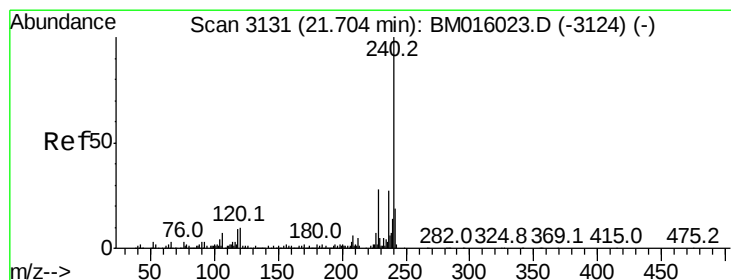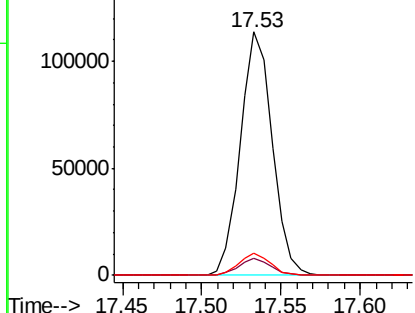
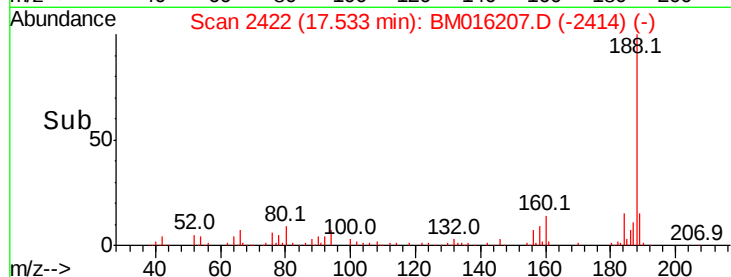



#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.66 min Scan# 3124
Delta R.T. -0.04 min
Lab File: BM016207.D
Acq: 07 Aug 2018 00:49

Tgt Ion:240 Resp: 168970
Ion Ratio Lower Upper
240 100
120 8.5 8.2 12.2
236 27.8 20.0 30.0

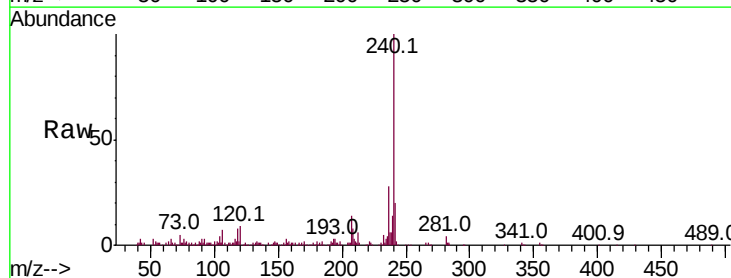

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



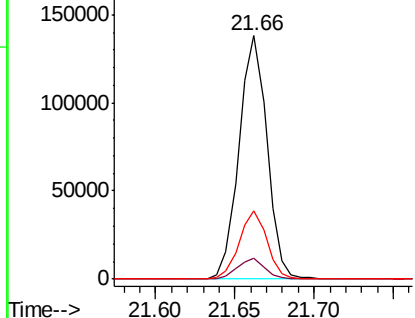
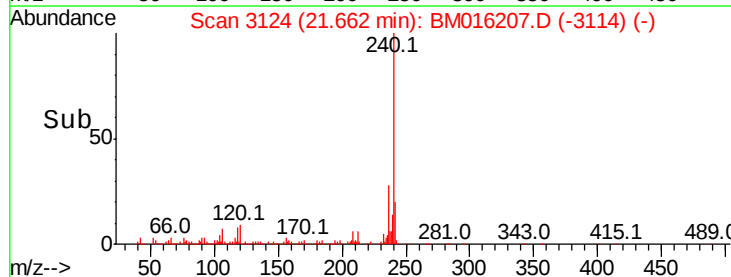


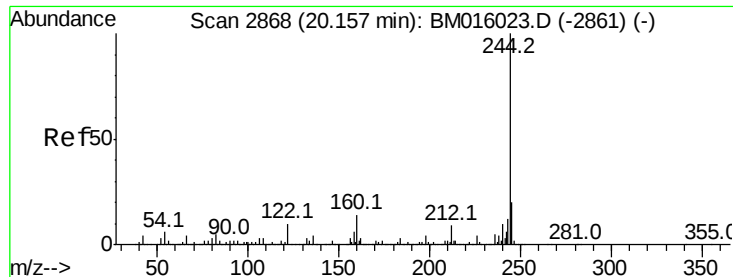

#78
 Terphenyl-d14
 Concen: Below na
 RT: 20.11 min Scan# 2860
 Delta R.T. -0.05 min
 Lab File: BM016207.D
 Acq: 07 Aug 2018 00:49

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
244	100		
212	10.2	4.9	7.3#
122	10.2	6.2	9.4#

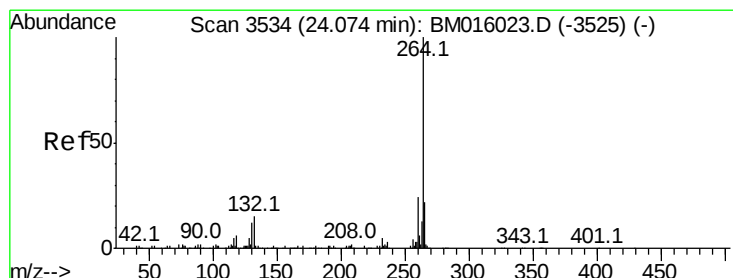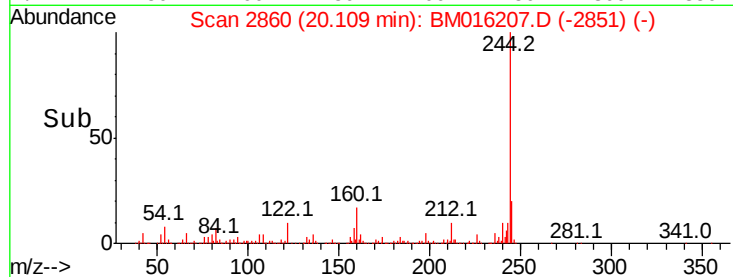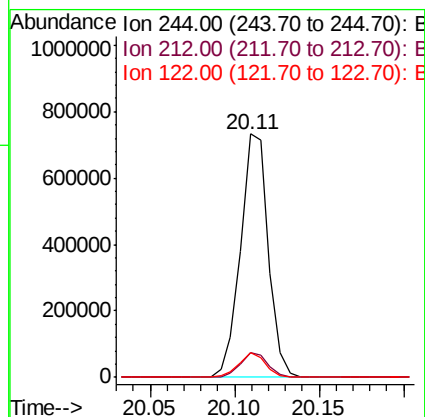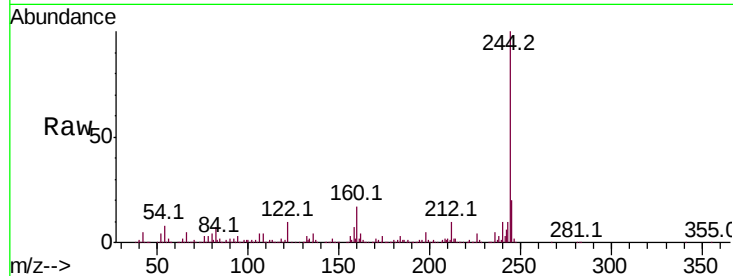

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.01 min Scan# 3524
 Delta R.T. -0.06 min
 Lab File: BM016207.D
 Acq: 07 Aug 2018 00:49

Tgt Ion	Ratio	Lower	Upper
264	100		
260	25.7	18.6	27.8
265	22.9	17.3	25.9

