
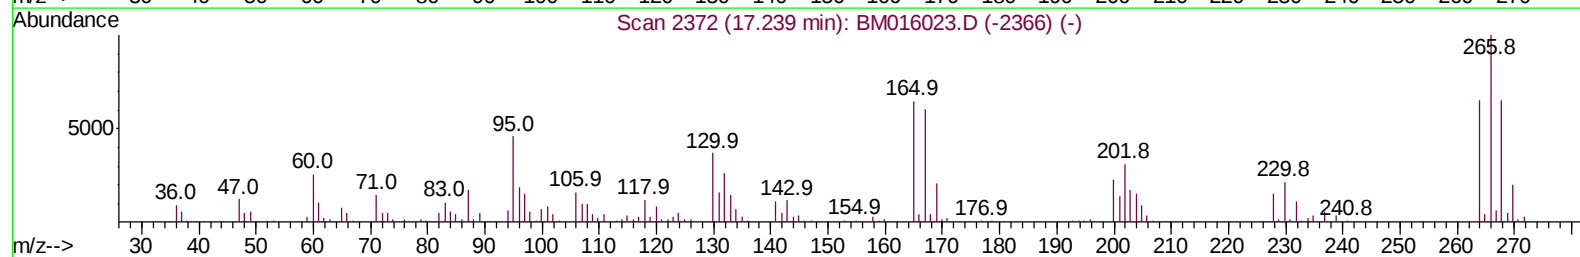
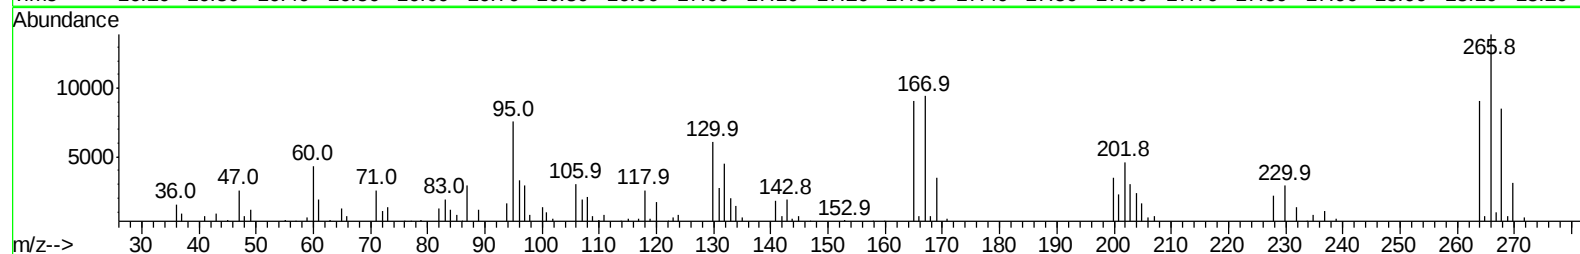


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080618\
Data File : BM016192.D
Acq On : 06 Aug 2018 13:01
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 09:52:15 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 23 16:08:38 2018
Response via : Initial Calibration

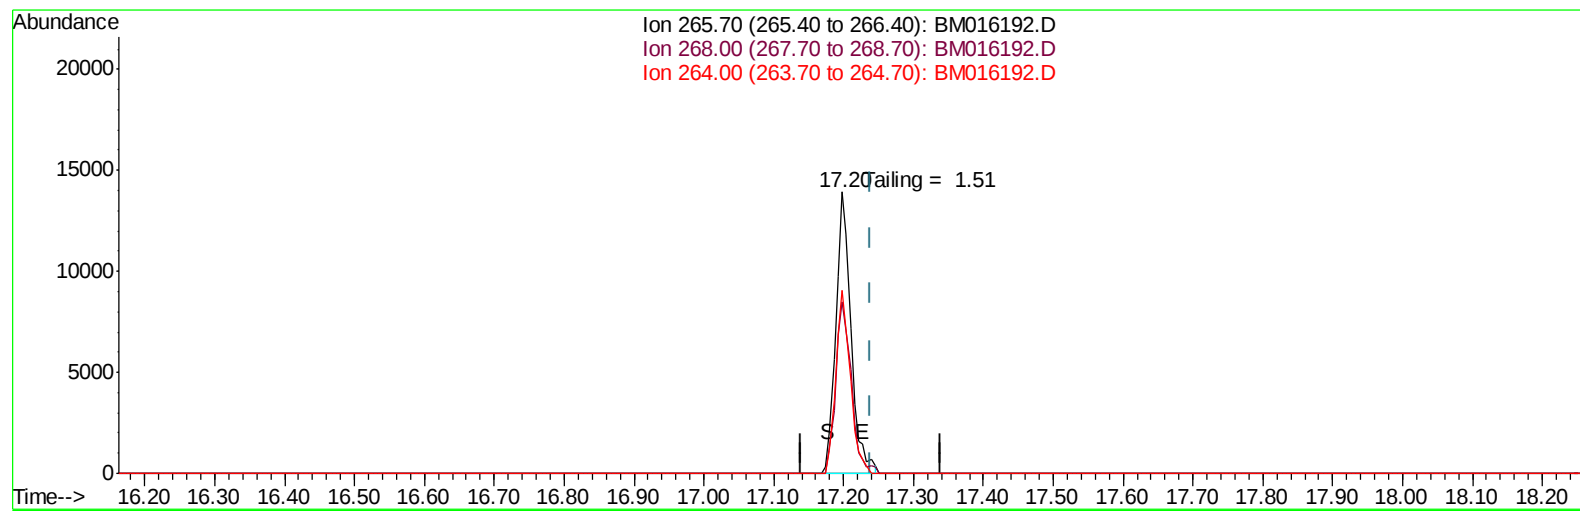

TIC: BM016192.D

(69) Pentachlorophenol (C)




17.198min (-0.041) 0.00ng

response 20799

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	60.86
264.00	61.20	64.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080618\
 Data File : BM016192.D
 Acq On : 06 Aug 2018 13:01
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 09:52:15 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM072318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 23 16:08:38 2018
 Response via : Initial Calibration

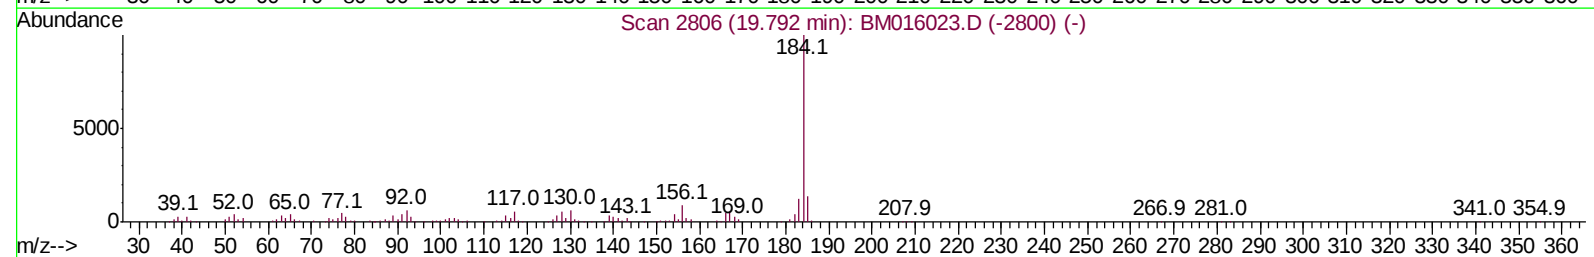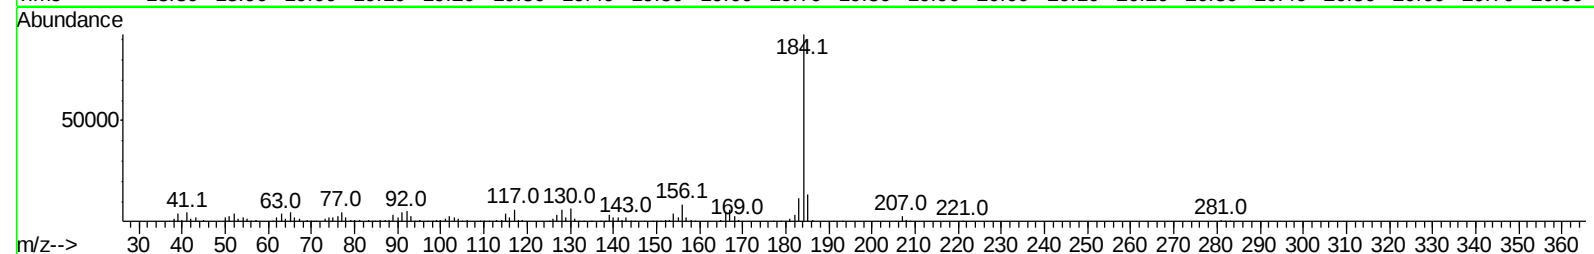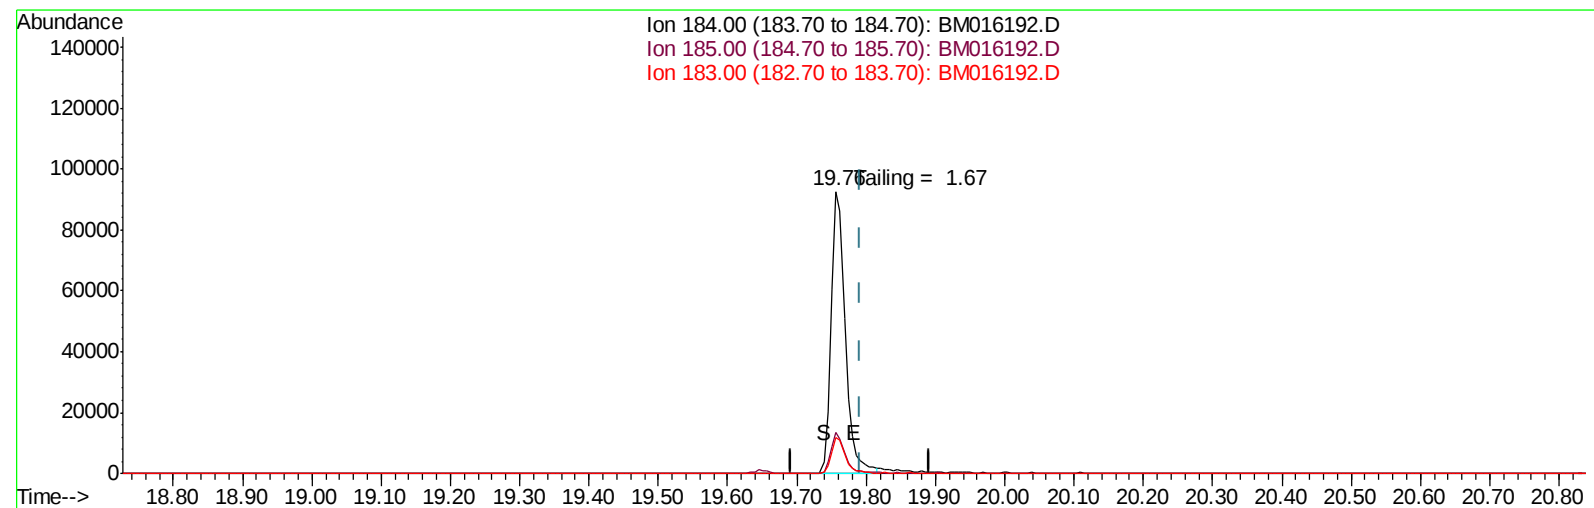

TIC: BM016192.D

(76) Benzidine

19.757min (-0.036) 9581.73ng

response 132271

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.47
183.00	11.10	12.82
0.00	0.00	0.00