

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080618\
 Data File : BM016215.D
 Acq On : 07 Aug 2018 06:14
 Operator : SJ/JU
 Sample : J4332-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 080118-DBRI-E-D-B

Quant Time: Aug 07 08:03:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM072318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 23 16:08:38 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	30972	20.00	ng	-0.07
21) Naphthalene-d8	10.99	136	117666	20.00	ng	-0.07
38) Acenaphthene-d10	14.80	164	60695	20.00	ng	-0.06
63) Phenanthrene-d10	17.53	188	130349	20.00	ng	-0.05
75) Chrysene-d12	21.66	240	143023	20.00	ng	-0.05
86) Perylene-d12	24.01	264	150548	20.00	ng	-0.07
System Monitoring Compounds						
5) 2-Fluorophenol	5.69	112	71656	38.43	ng	-0.05
7) Phenol-d6	7.33	99	53413	21.94	ng	-0.05
23) Nitrobenzene-d5	9.35	82	261746	103.46	ng	-0.07
41) 2,4,6-Tribromophenol	16.29	330	68924	89.53	ng	-0.05
44) 2-Fluorobiphenyl	13.42	172	499933	100.22	ng	-0.06
78) Terphenyl-d14	20.11	244	716575	104.88	ng	-0.05


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080618\
Data File : BM016215.D
Acq On : 07 Aug 2018 06:14
Operator : SJ/JU
Sample : J4332-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
080118-DBRI-E-D-B

Quant Time: Aug 07 08:03:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 23 16:08:38 2018
Response via : Initial Calibration

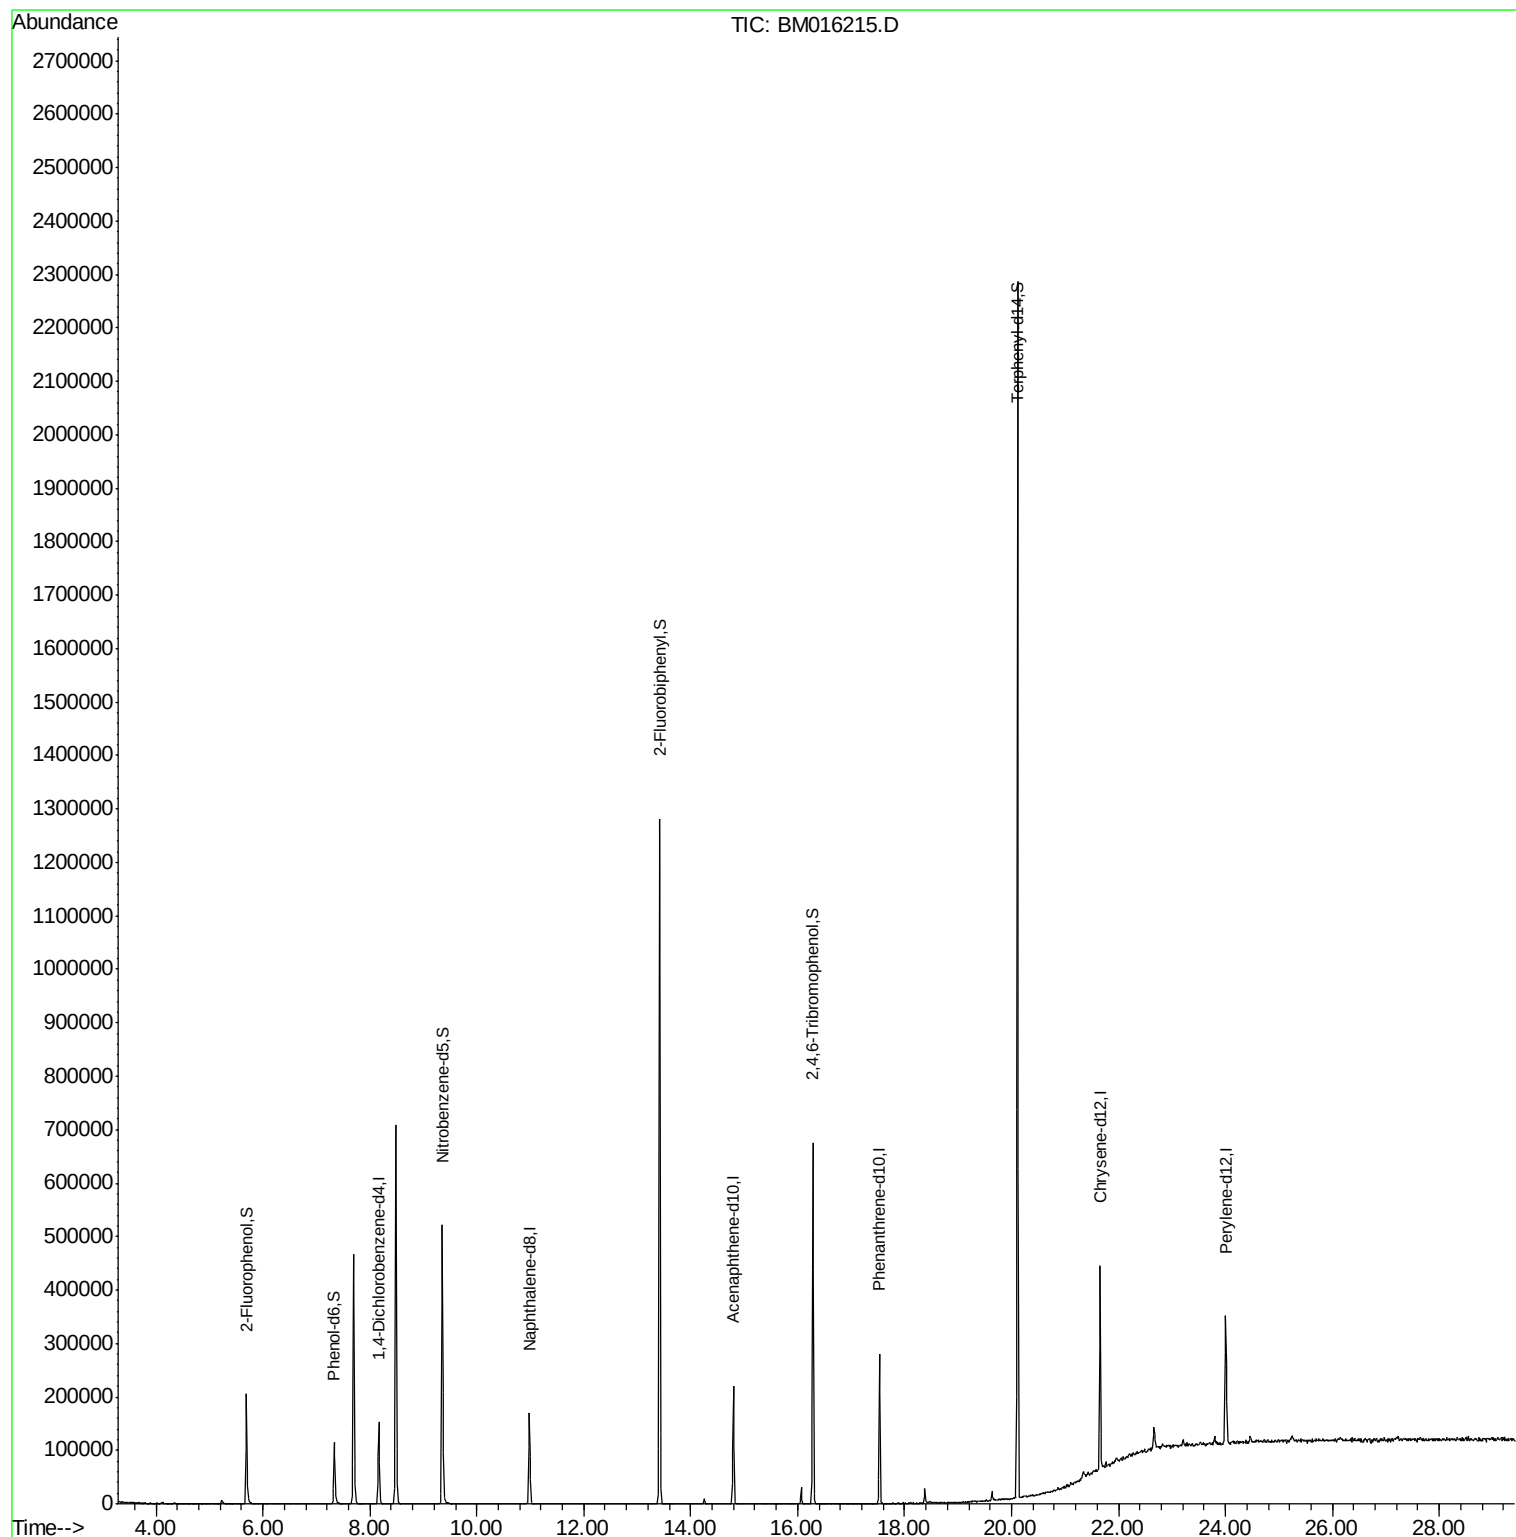

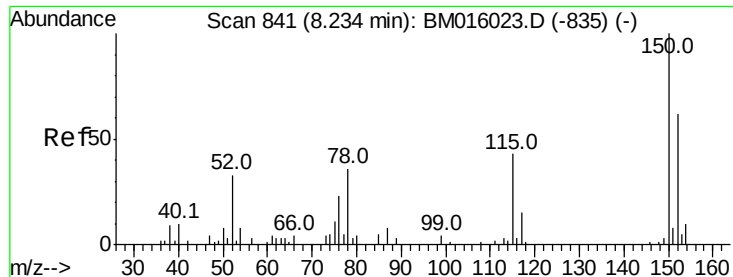


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.17 min Scan# 830
 Delta R.T. -0.07 min
 Lab File: BM016215.D
 Acq: 07 Aug 2018 06:14

Instrument :
 BNA_M
 ClientSampleId :
 080118-DBRI-E-D-B

Tot Ion:152 Resp: 30972
 Ion Ratio Lower Upper
 152 100
 150 158.3 119.5 179.3
 115 67.1 43.0 64.4#

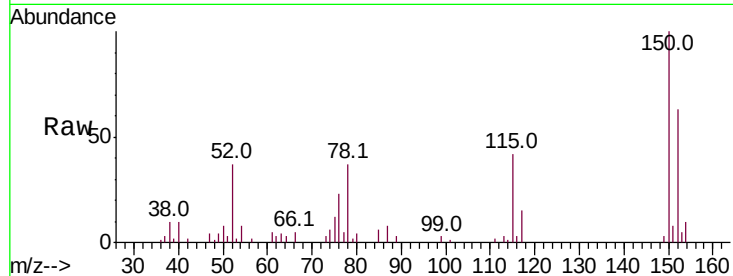


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

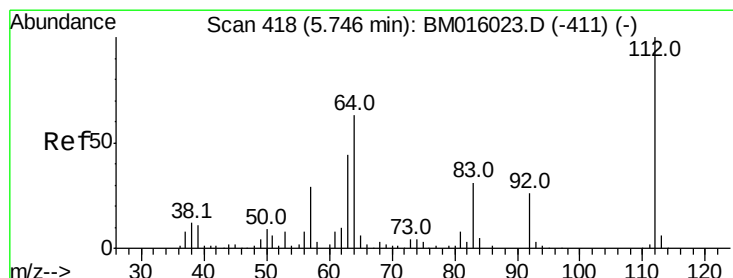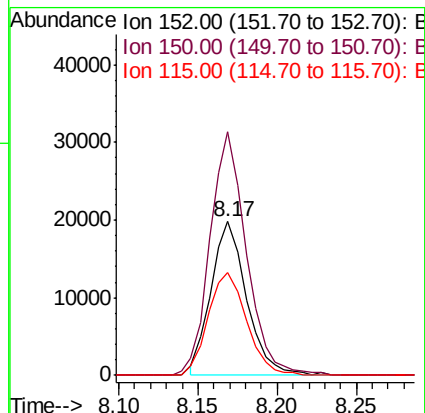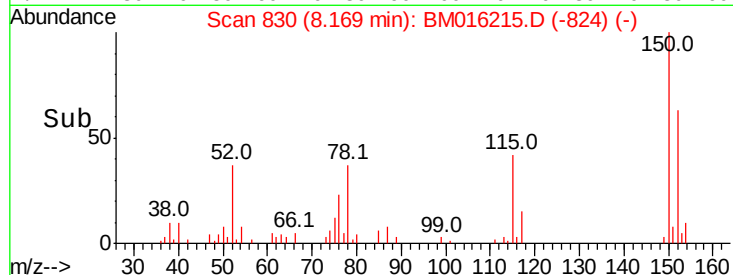



#5


2-Fluorophenol
 Concen: N.D. ng
 RT: 5.69 min Scan# 409
 Delta R.T. -0.05 min
 Lab File: BM016215.D
 Acq: 07 Aug 2018 06:14

Tgt Ion:112 Resp: 71656
 Ion Ratio Lower Upper
 112 100
 64 63.7 38.6 57.8#
 63 44.7 19.3 28.9#

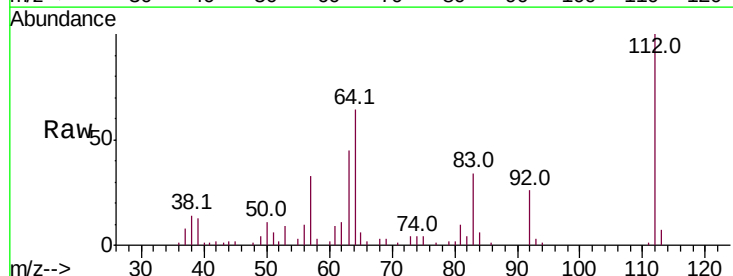

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BM
 Ion 63.00 (62.70 to 63.70): BM

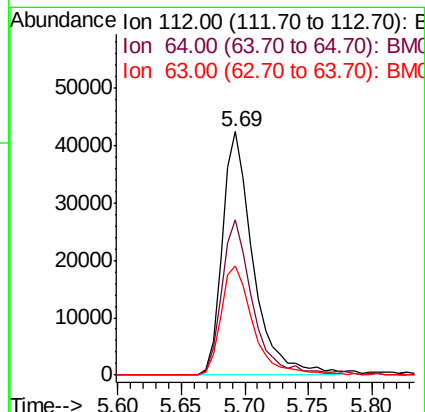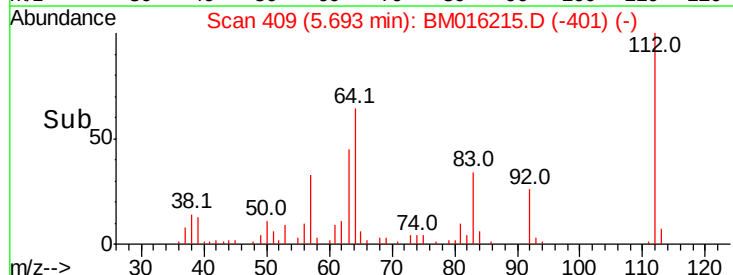

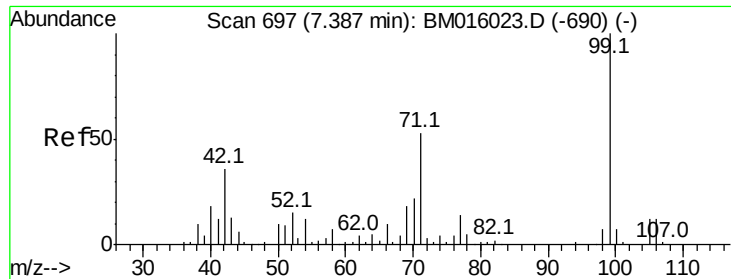

#7

Phenol-d6

Concen: N.D. ng

RT: 7.33 min Scan# 688

Delta R.T. -0.05 min

Lab File: BM016215.D

Acq: 07 Aug 2018 06:14

Instrument :

BNA_M

ClientSampleId :

080118-DBRI-E-D-B


Tot Ion: 99 Resp: 53413

Ion Ratio Lower Upper

99 100

42 35.7 11.0 16.4#




71 53.1 23.4 35.2#

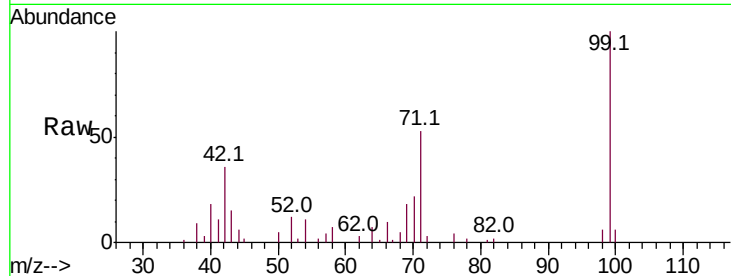

Abundance Ion 99.00 (98.70 to 99.70): BM016215.D (-680) (-)

Ion 42.00 (41.70 to 42.70): BM016215.D (-680) (-)

Ion 71.00 (70.70 to 71.70): BM016215.D (-680) (-)

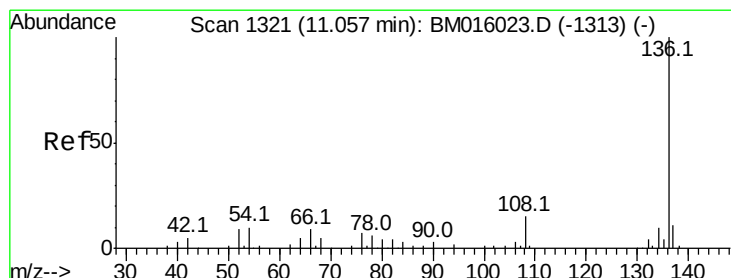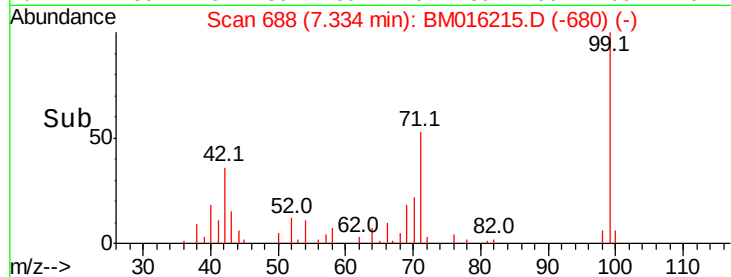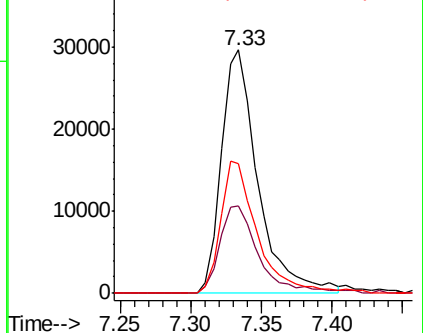

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.99 min Scan# 1309

Delta R.T. -0.07 min

Lab File: BM016215.D

Acq: 07 Aug 2018 06:14

Tgt Ion: 136 Resp: 117666


Ion Ratio Lower Upper

136 100

137 10.3 8.7 13.1

54 9.2 4.6 6.8#

68 3.6 3.7 5.5#


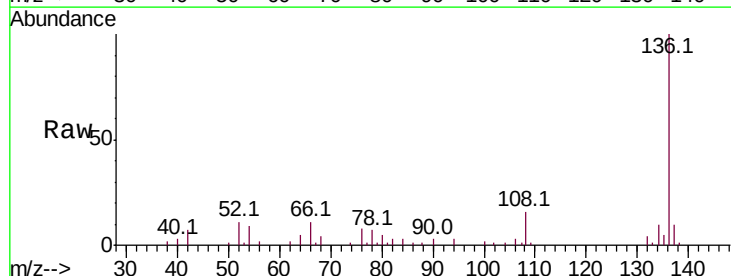



Abundance Ion 136.00 (135.70 to 136.70): BM016215.D (-1304) (-)

Ion 137.00 (136.70 to 137.70): BM016215.D (-1304) (-)

Ion 54.00 (53.70 to 54.70): BM016215.D (-1304) (-)

Ion 68.00 (67.70 to 68.70): BM016215.D (-1304) (-)



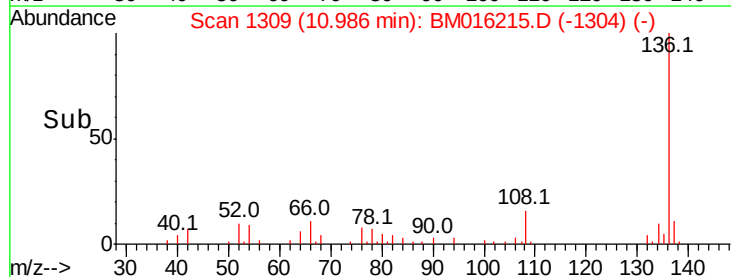
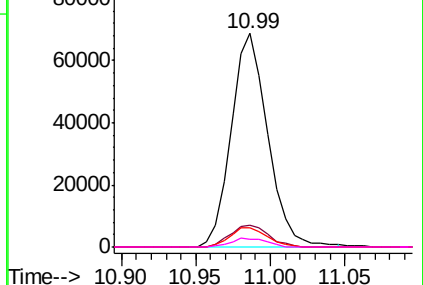


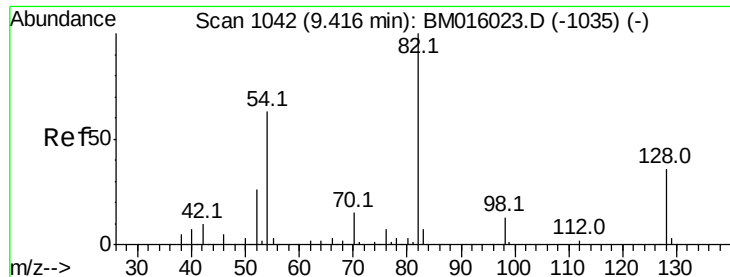

#23
 Nitrobenzene-d5
 Concen: N.D. ng
 RT: 9.35 min Scan# 1031
 Delta R.T. -0.07 min
 Lab File: BM016215.D
 Acq: 07 Aug 2018 06:14




Instrument :
 BNA_M
 ClientSampleId :
 080118-DBRI-E-D-B


Tot Ion: 82 Resp: 261746
 Ion Ratio Lower Upper
 82 100
 128 35.0 32.8 49.2
 54 63.1 40.6 60.8#

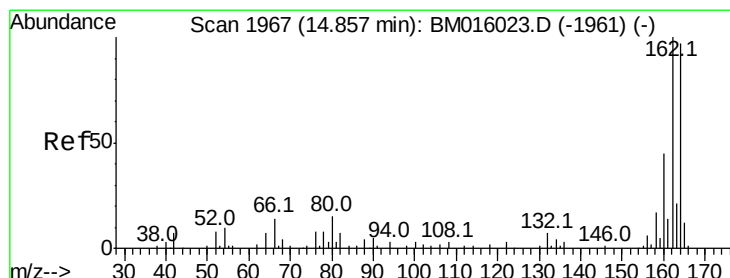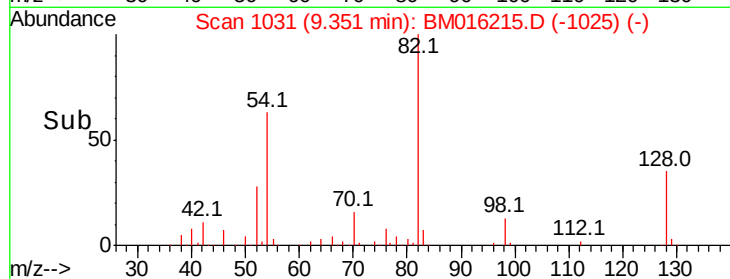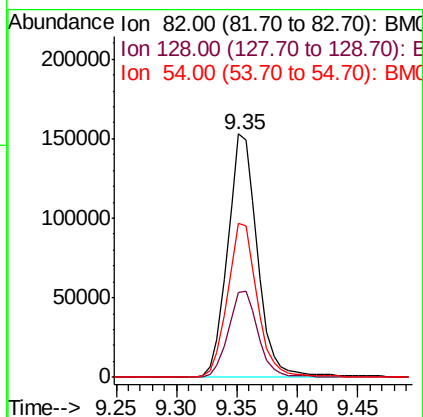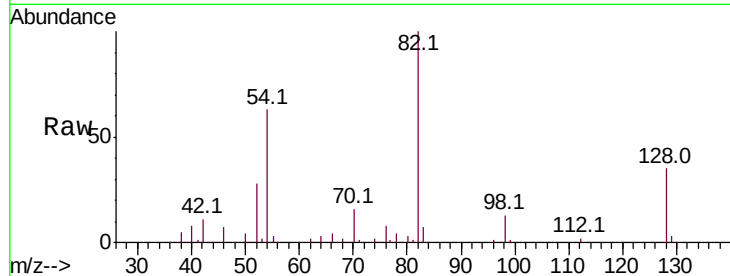

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.80 min Scan# 1957
 Delta R.T. -0.06 min
 Lab File: BM016215.D
 Acq: 07 Aug 2018 06:14

Tgt Ion: 164 Resp: 60695
 Ion Ratio Lower Upper
 164 100
 162 107.5 82.4 123.6
 160 51.1 35.8 53.6

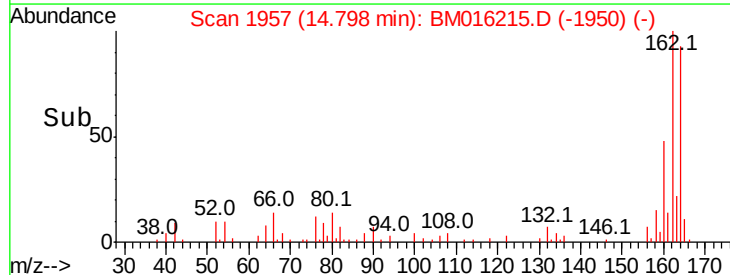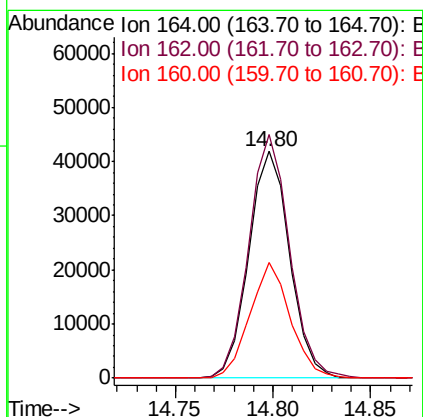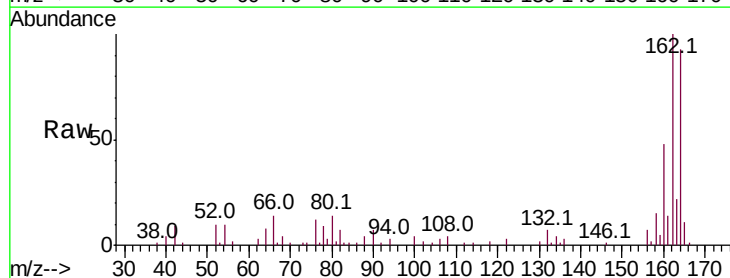


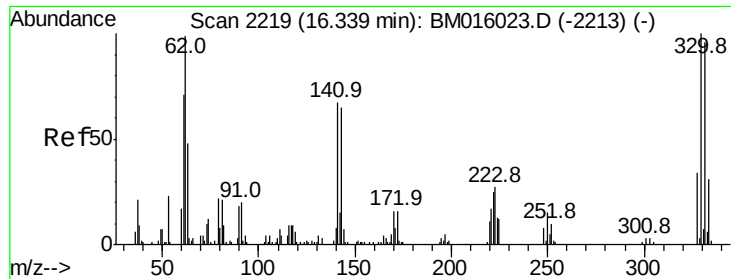




#41
 2,4,6-Tribromophenol
 Concen: N.D. ng
 RT: 16.29 min Scan# 2210
 Delta R.T. -0.05 min
 Lab File: BM016215.D
 Acq: 07 Aug 2018 06:14

Instrument :
 BNA_M
 ClientSampleId :
 080118-DBRI-E-D-B

Tot Ion:330 Resp: 68924
 Ion Ratio Lower Upper
 330 100
 332 96.4 0.0 0.0#
 141 80.4 0.0 0.0#

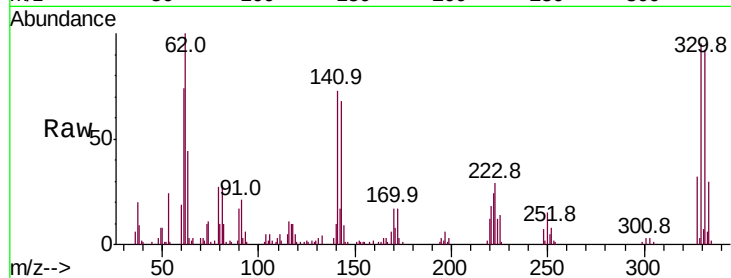


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

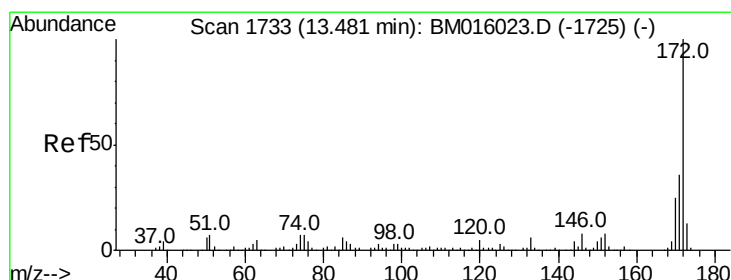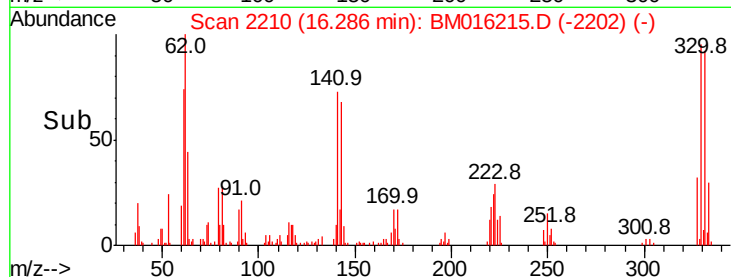
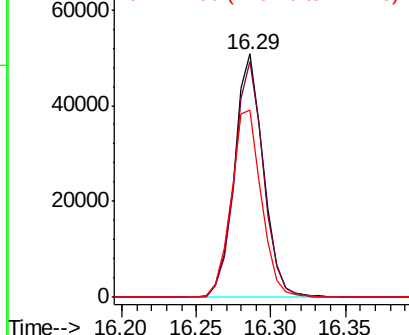



#44
 2-Fluorobiphenyl
 Concen: N.D. ng
 RT: 13.42 min Scan# 1723
 Delta R.T. -0.06 min
 Lab File: BM016215.D
 Acq: 07 Aug 2018 06:14

Tgt Ion:172 Resp: 499933
 Ion Ratio Lower Upper
 172 100
 171 36.9 28.5 42.7
 170 24.3 18.8 28.2

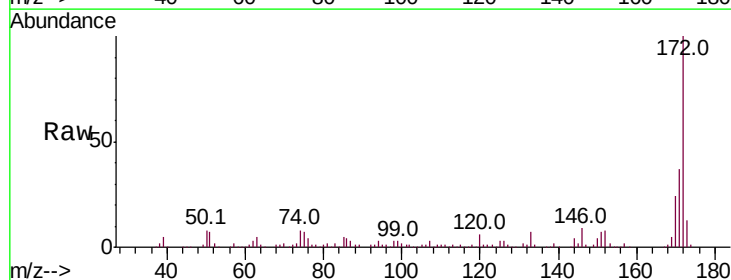

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

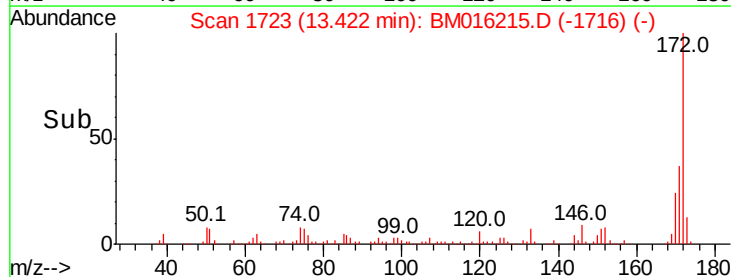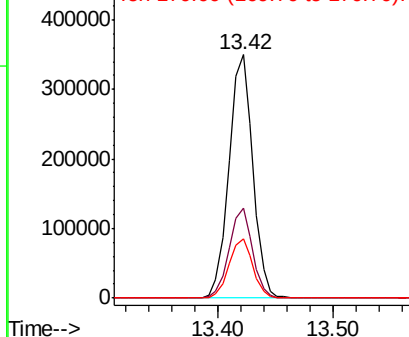


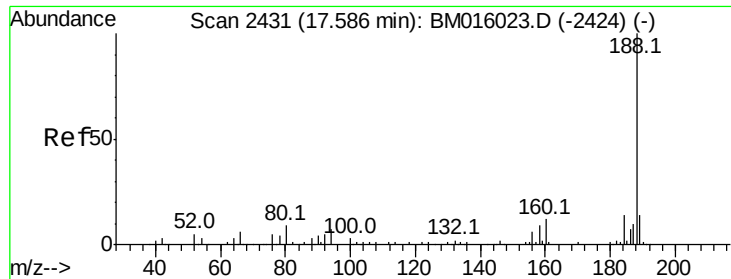




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.53 min Scan# 2422
Delta R.T. -0.05 min
Lab File: BM016215.D
Acq: 07 Aug 2018 06:14

Instrument :
BNA_M
ClientSampleId :
080118-DBRI-E-D-B

Tot Ion:188 Resp: 130349
Ion Ratio Lower Upper
188 100
94 6.3 8.7 13.1#
80 8.2 9.3 13.9#

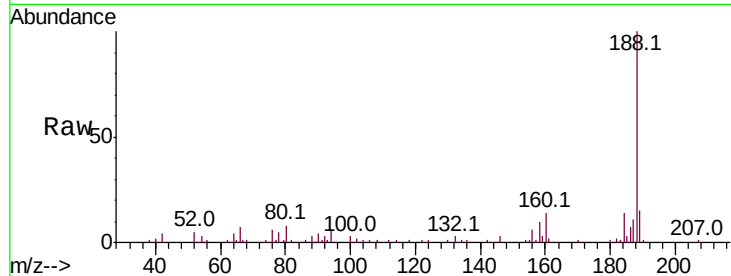


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM0
Ion 80.00 (79.70 to 80.70): BM0

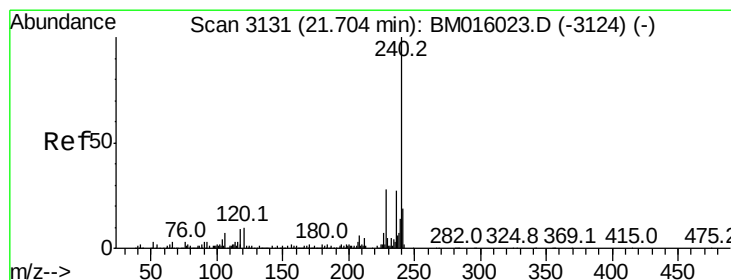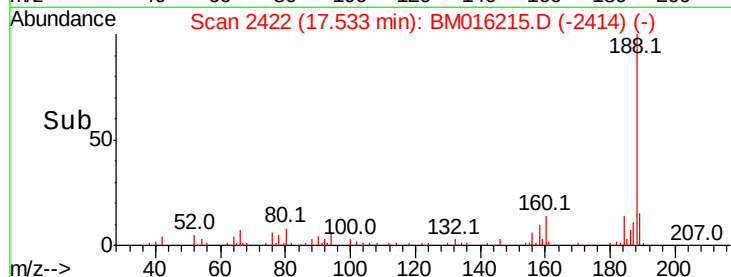
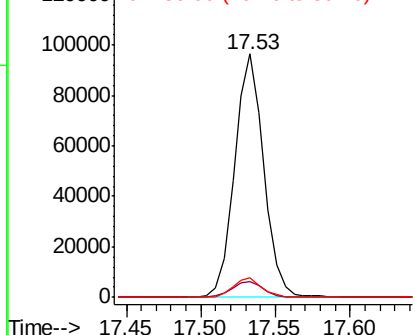



#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.66 min Scan# 3123
Delta R.T. -0.05 min
Lab File: BM016215.D
Acq: 07 Aug 2018 06:14

Tgt Ion:240 Resp: 143023
Ion Ratio Lower Upper
240 100
120 8.4 8.2 12.2
236 28.2 20.0 30.0

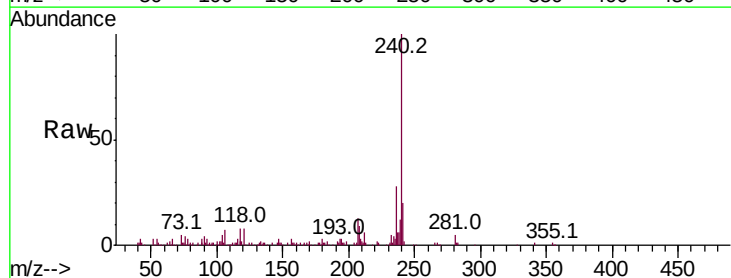

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



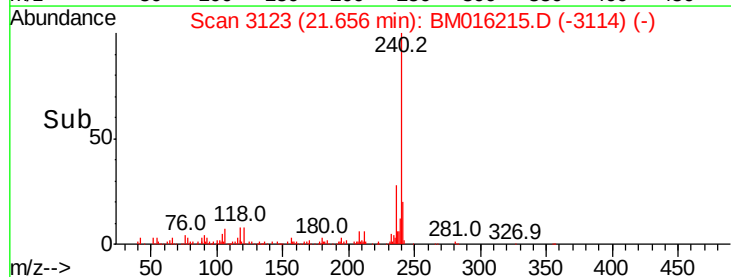
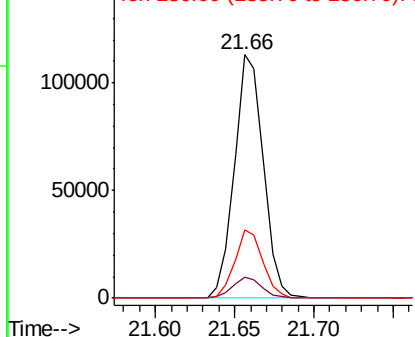


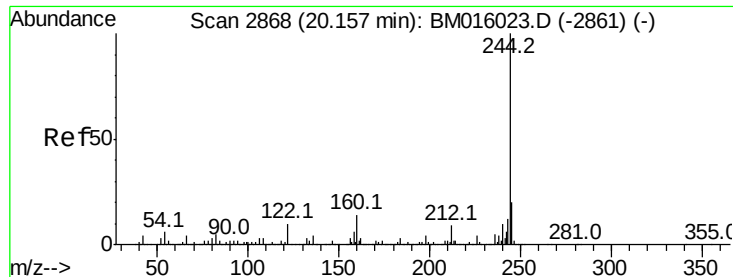

#78
 Terphenyl-d14
 Concen: N.D. ng
 RT: 20.11 min Scan# 2860
 Delta R.T. -0.05 min
 Lab File: BM016215.D
 Acq: 07 Aug 2018 06:14

Instrument :
 BNA_M
 ClientSampleId :
 080118-DBRI-E-D-B

Tot Ion	Ratio	Lower	Upper
244	100		
212	10.2	4.9	7.3#
122	8.8	6.2	9.4

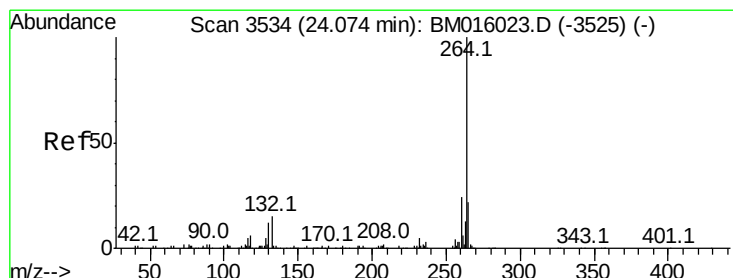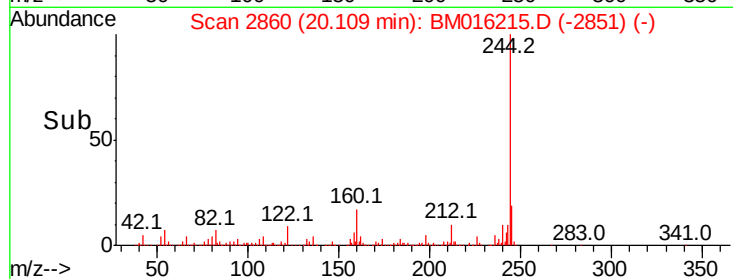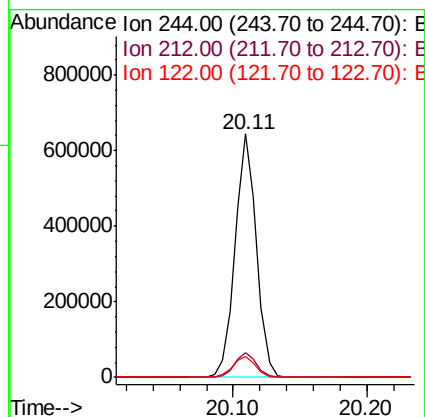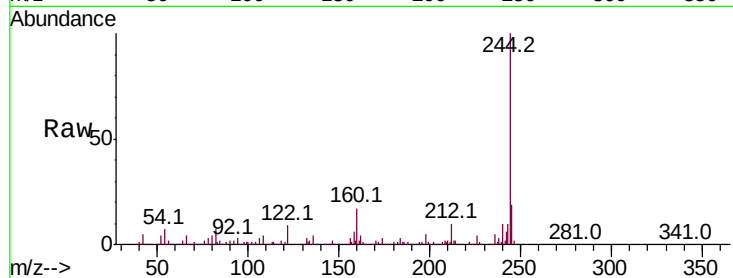

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.01 min Scan# 3523
 Delta R.T. -0.07 min
 Lab File: BM016215.D
 Acq: 07 Aug 2018 06:14

Tgt Ion	Ratio	Lower	Upper
264	100		
260	25.4	18.6	27.8
265	23.5	17.3	25.9

