

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080618\
 Data File : BM016208.D
 Acq On : 07 Aug 2018 01:25
 Operator : SJ/JU
 Sample : J4330-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 073018-TIPC-F-D-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.693	404	409	424	rBV	246738	405010	14.30%	3.351%
2	7.334	683	688	705	rBV	147004	261756	9.24%	2.166%
3	7.693	744	749	767	rBV	521183	872143	30.79%	7.216%
4	8.169	824	830	837	rBV	170087	273291	9.65%	2.261%
5	8.492	878	885	900	rBB	728570	1175650	41.50%	9.727%
6	9.357	1025	1032	1046	rBV	604223	1004941	35.47%	8.315%
7	10.986	1303	1309	1321	rBV	194341	328362	11.59%	2.717%
8	13.422	1717	1723	1730	rBV	1369696	1893142	66.83%	15.663%
9	14.798	1950	1957	1965	rBB2	252113	381426	13.46%	3.156%
10	16.068	2169	2173	2178	rBB	31612	36348	1.28%	0.301%
11	16.286	2204	2210	2222	rVB	731745	1003306	35.42%	8.301%
12	17.533	2416	2422	2432	rBV	324424	445132	15.71%	3.683%
13	18.380	2561	2566	2571	rBV	29609	37119	1.31%	0.307%
14	20.109	2855	2860	2866	rBV	2359779	2832871	100.00%	23.438%
15	21.533	3099	3102	3107	rBV	36916	41419	1.46%	0.343%
16	21.662	3119	3124	3130	rBV	429503	545469	19.25%	4.513%
17	24.015	3518	3524	3534	rVB	280939	549052	19.38%	4.543%


Sum of corrected areas: 12086437

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080618\
Data File : BM016208.D
Acq On : 07 Aug 2018 01:25
Operator : SJ/JU
Sample : J4330-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
073018-TIPC-F-D-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

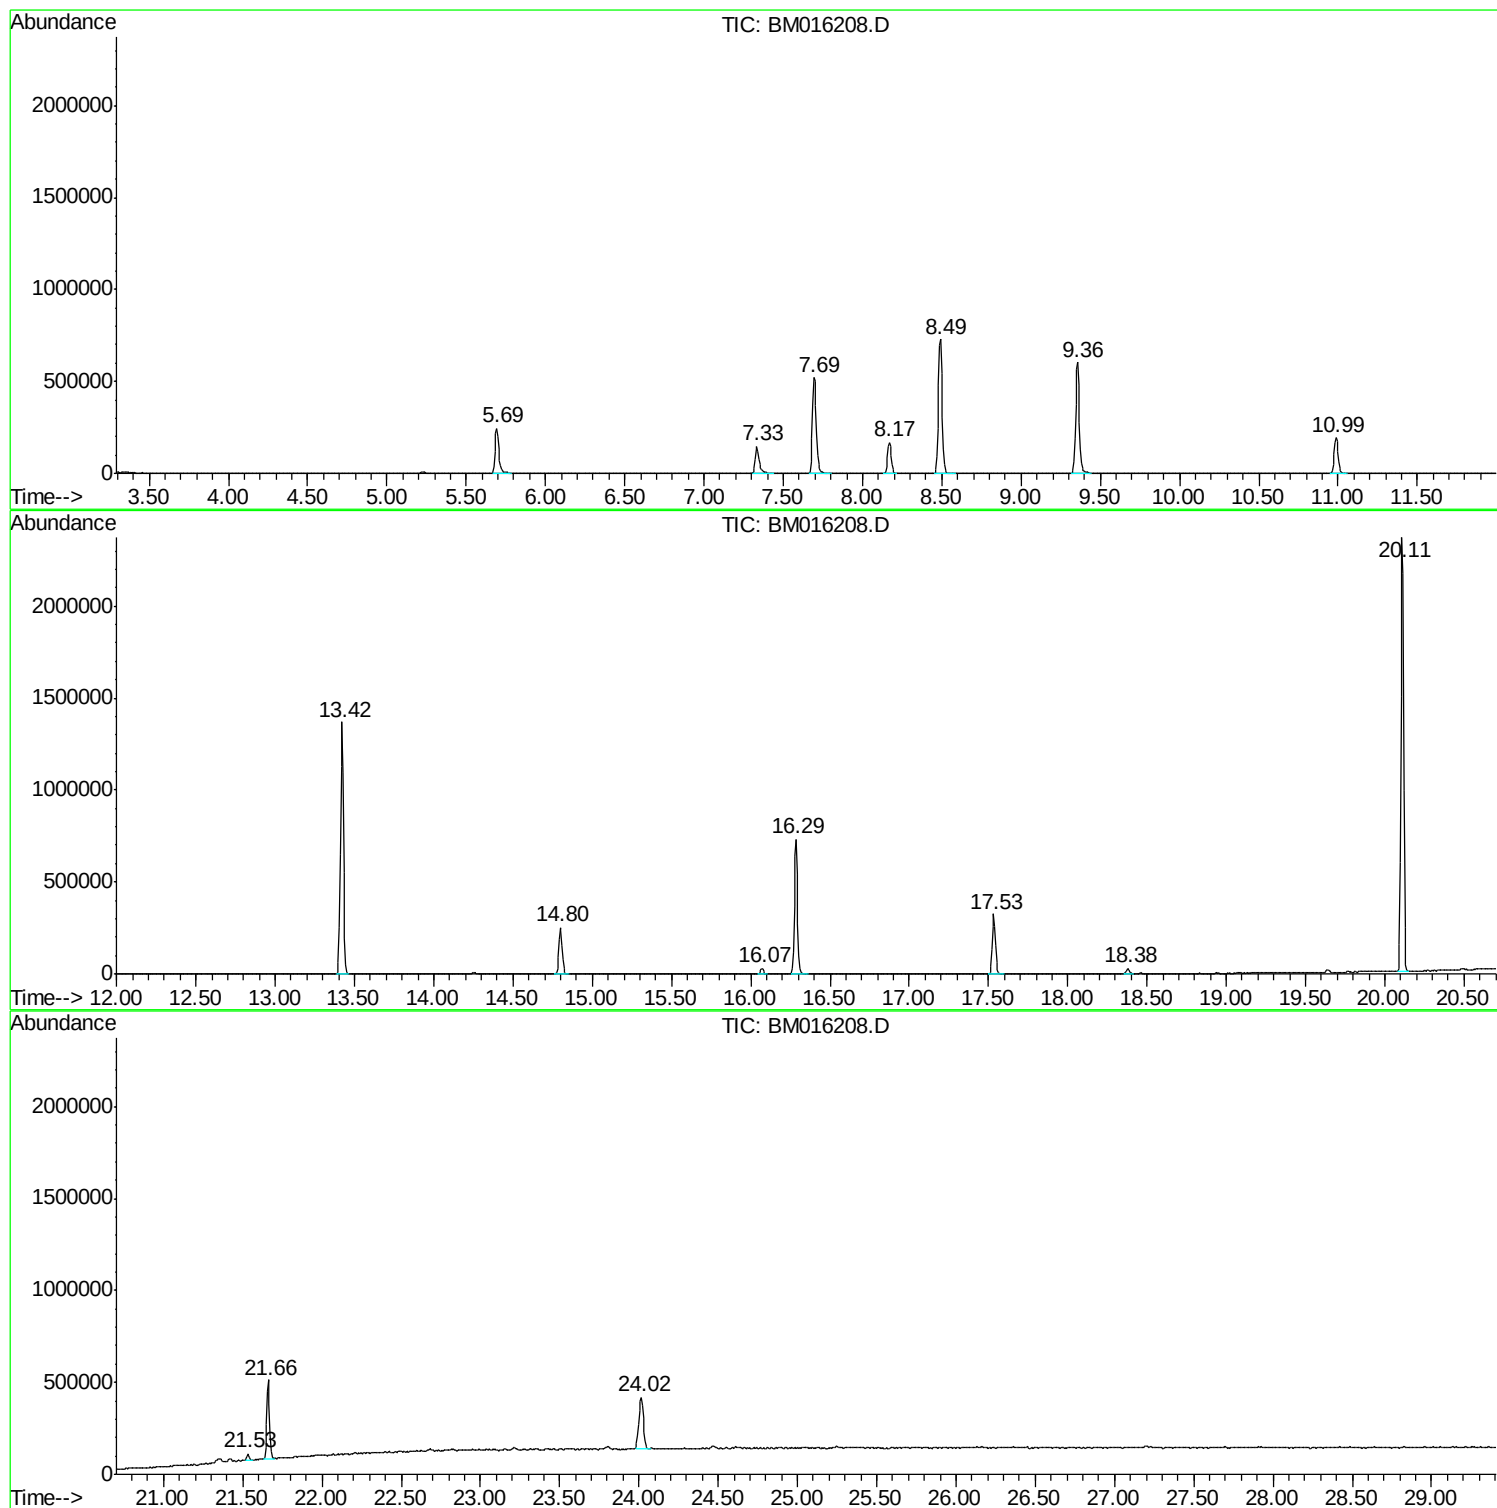

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080618\
Data File : BM016208.D
Acq On : 07 Aug 2018 01:25
Operator : SJ/JU
Sample : J4330-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
073018-TIPC-F-D-S










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.69 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.69	63.83 ng	872143	1,4-Dichlorobenzene-d4	8.17

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	27
2		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	18
3		3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	14
4		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	14
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	14

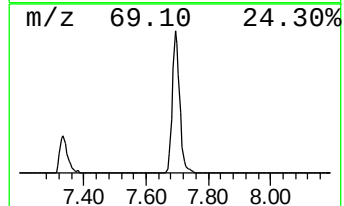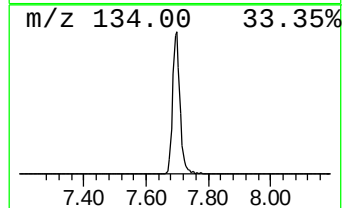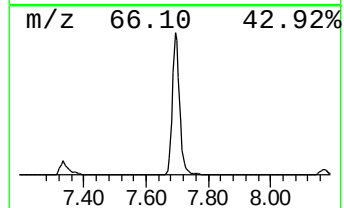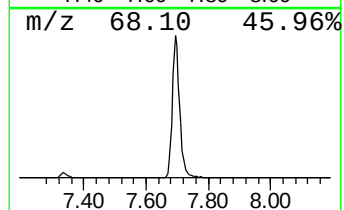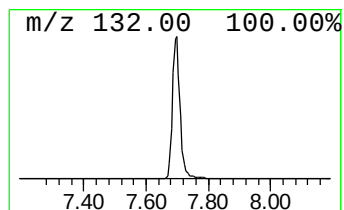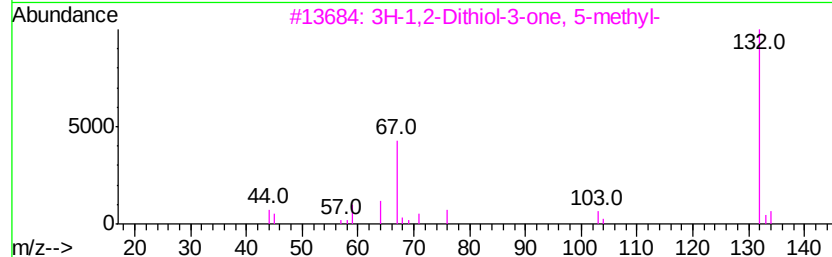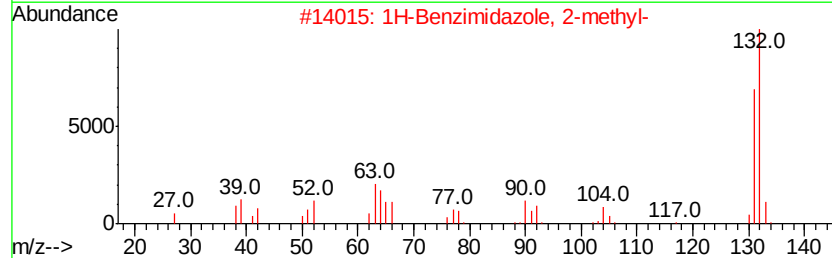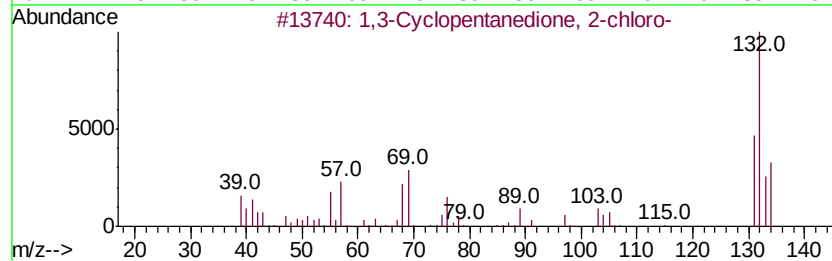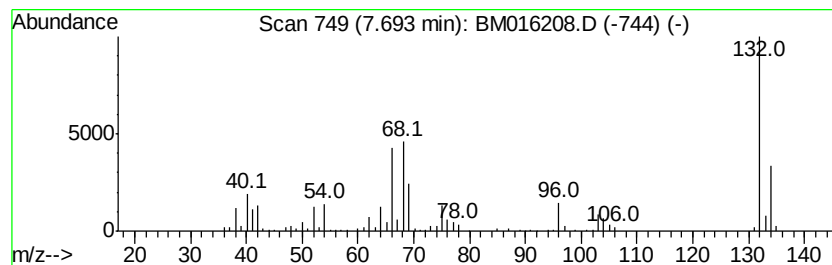

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080618\
Data File : BM016208.D
Acq On : 07 Aug 2018 01:25
Operator : SJ/JU
Sample : J4330-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
073018-TIPC-F-D-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.69	7.69	63.8	ng	872143	1	8.17	273291	20.0