

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080618\
 Data File : BM016216.D
 Acq On : 07 Aug 2018 06:50
 Operator : SJ/JU
 Sample : J4332-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 080118-DBRI-E-D-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.693	403	409	421	rBV	201332	334817	13.44%	3.099%
2	7.328	683	687	705	rBV	116492	209694	8.42%	1.941%
3	7.693	743	749	770	rBB	470536	770671	30.93%	7.134%
4	8.169	824	830	840	rBB	145884	241769	9.70%	2.238%
5	8.487	878	884	896	rBV	746893	1195017	47.96%	11.062%
6	9.352	1025	1031	1047	rBV	527380	890294	35.73%	8.241%
7	10.987	1302	1309	1317	rBV	170518	282228	11.33%	2.613%
8	13.422	1716	1723	1731	rVB	1288236	1816361	72.90%	16.814%
9	14.798	1949	1957	1964	rBB2	218918	320010	12.84%	2.962%
10	16.069	2169	2173	2178	rBB	25309	28148	1.13%	0.261%
11	16.281	2204	2209	2221	rVB	643173	918155	36.85%	8.499%
12	17.533	2416	2422	2429	rBV2	262834	364311	14.62%	3.372%
13	18.375	2561	2565	2572	rBV2	24053	28469	1.14%	0.264%
14	20.110	2854	2860	2865	rBV	2222906	2491522	100.00%	23.063%
15	21.657	3119	3123	3129	rVB	362753	452443	18.16%	4.188%
16	24.009	3516	3523	3531	rVB	233619	459017	18.42%	4.249%


Sum of corrected areas: 10802926

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080618\
Data File : BM016216.D
Acq On : 07 Aug 2018 06:50
Operator : SJ/JU
Sample : J4332-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
080118-DBRI-E-D-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

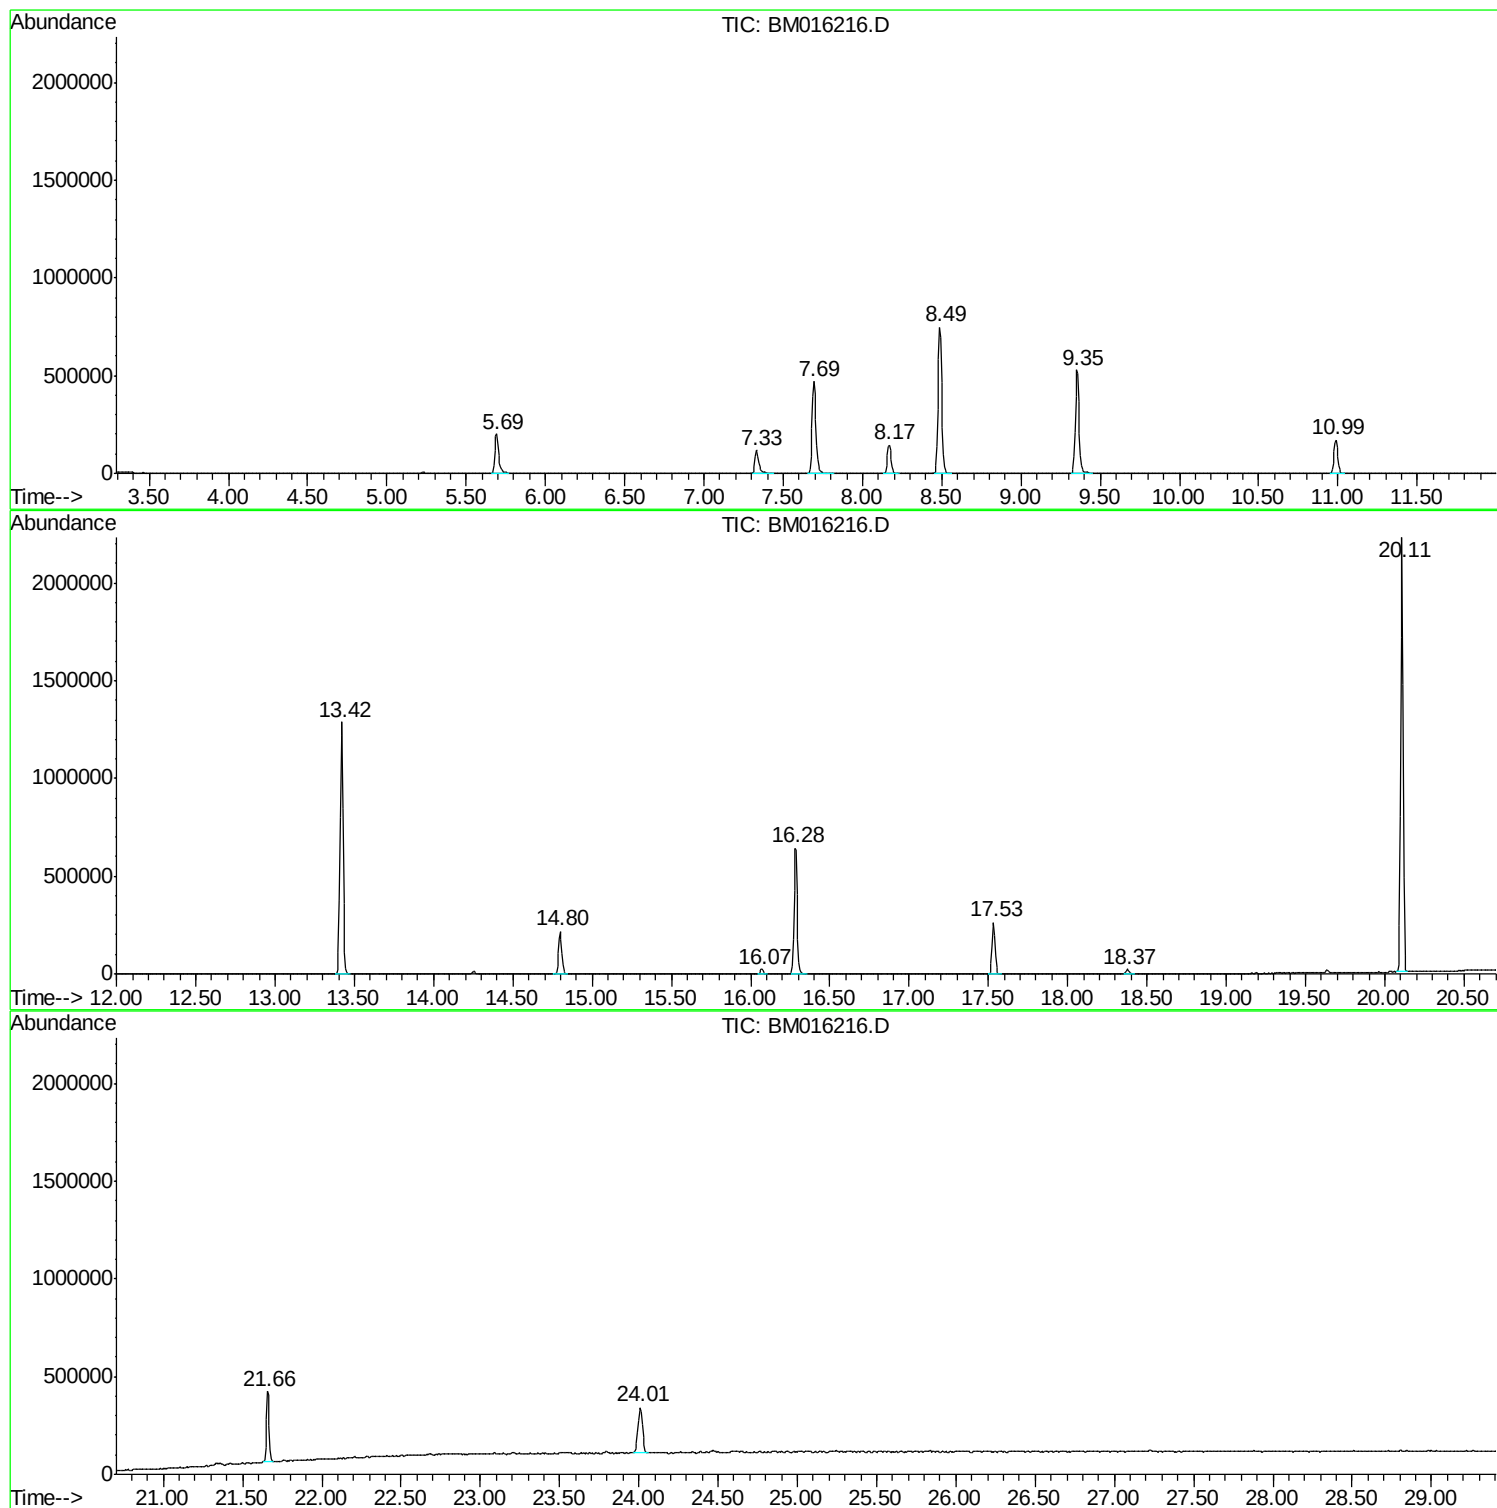

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080618\
Data File : BM016216.D
Acq On : 07 Aug 2018 06:50
Operator : SJ/JU
Sample : J4332-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
080118-DBRI-E-D-S










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.69 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.69	63.75 ng	770671	1,4-Dichlorobenzene-d4	8.17

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	14
2		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	14
3		3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	14
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	14
5		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	10

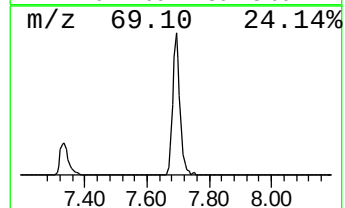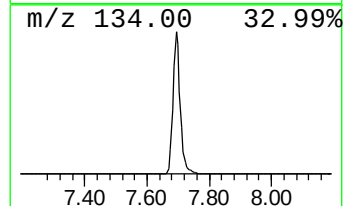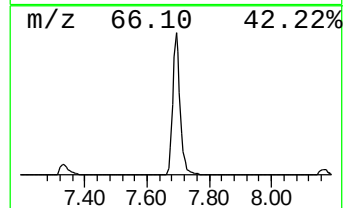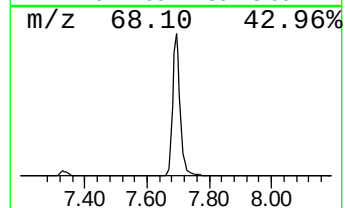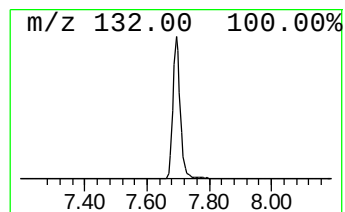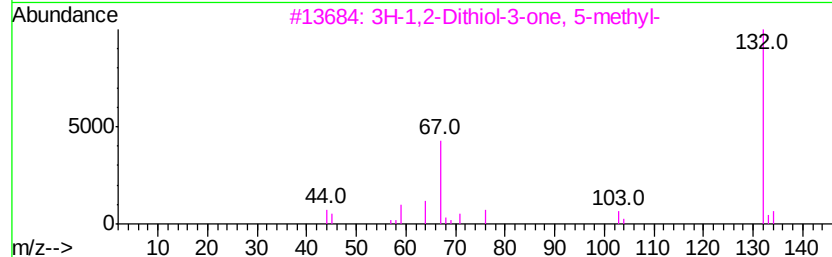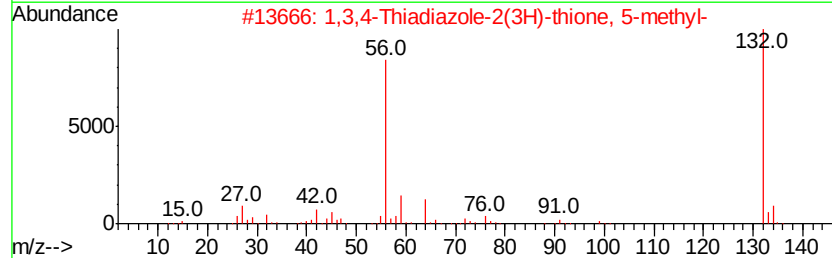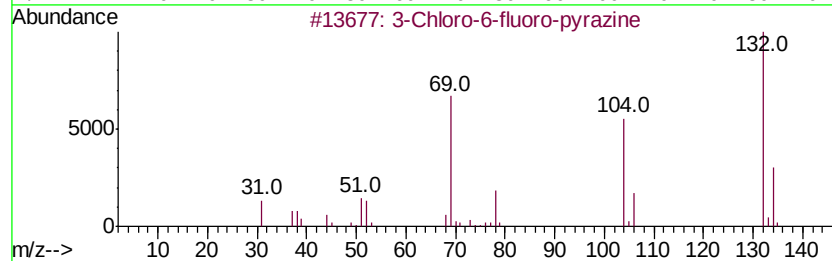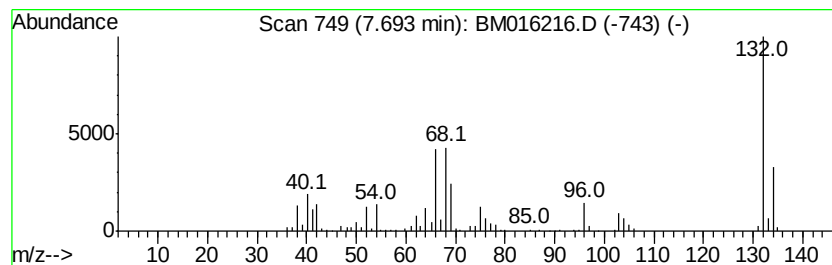

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080618\
Data File : BM016216.D
Acq On : 07 Aug 2018 06:50
Operator : SJ/JU
Sample : J4332-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
080118-DBRI-E-D-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.69	7.69	63.8	ng	770671	1	8.17	241769	20.0