


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080618\
 Data File : BM016192.D
 Acq On : 06 Aug 2018 13:01
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 07 16:15:57 2018

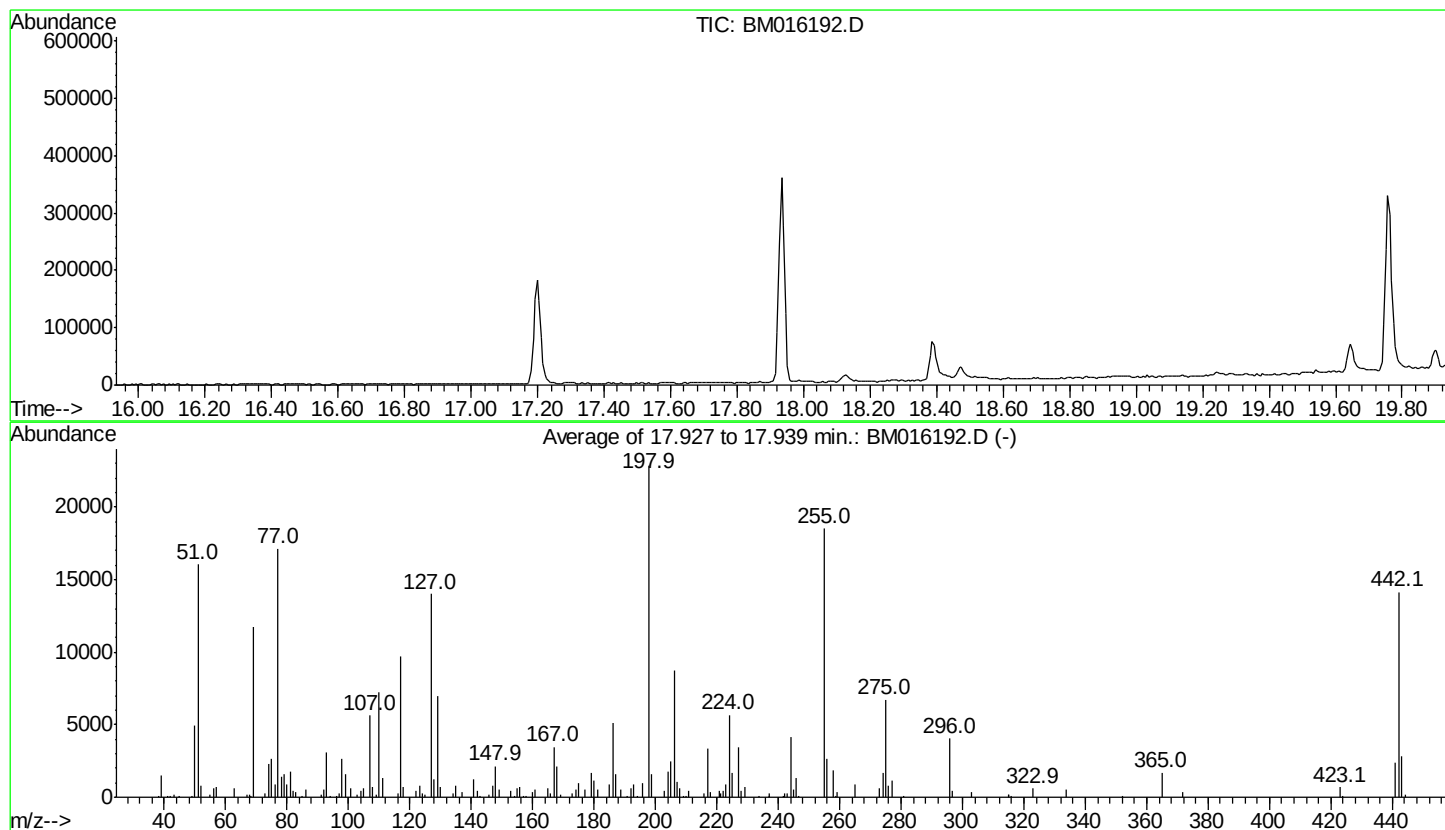

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	70.3	16047	PASS
68	69	0.00	2	1.3	151	PASS
69	198	0.00	100	51.4	11742	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	61.3	14011	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	22842	PASS
199	198	5	9	6.9	1576	PASS
275	198	10	60	29.4	6722	PASS
365	198	1	100	7.4	1699	PASS
441	198	0.01	100	10.6	2410	PASS
442	198	50	100	61.8	14113	PASS
443	442	15	24	20.1	2833	PASS