


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080618\
 Data File : BM016211.D
 Acq On : 07 Aug 2018 03:50
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 07 16:15:57 2018

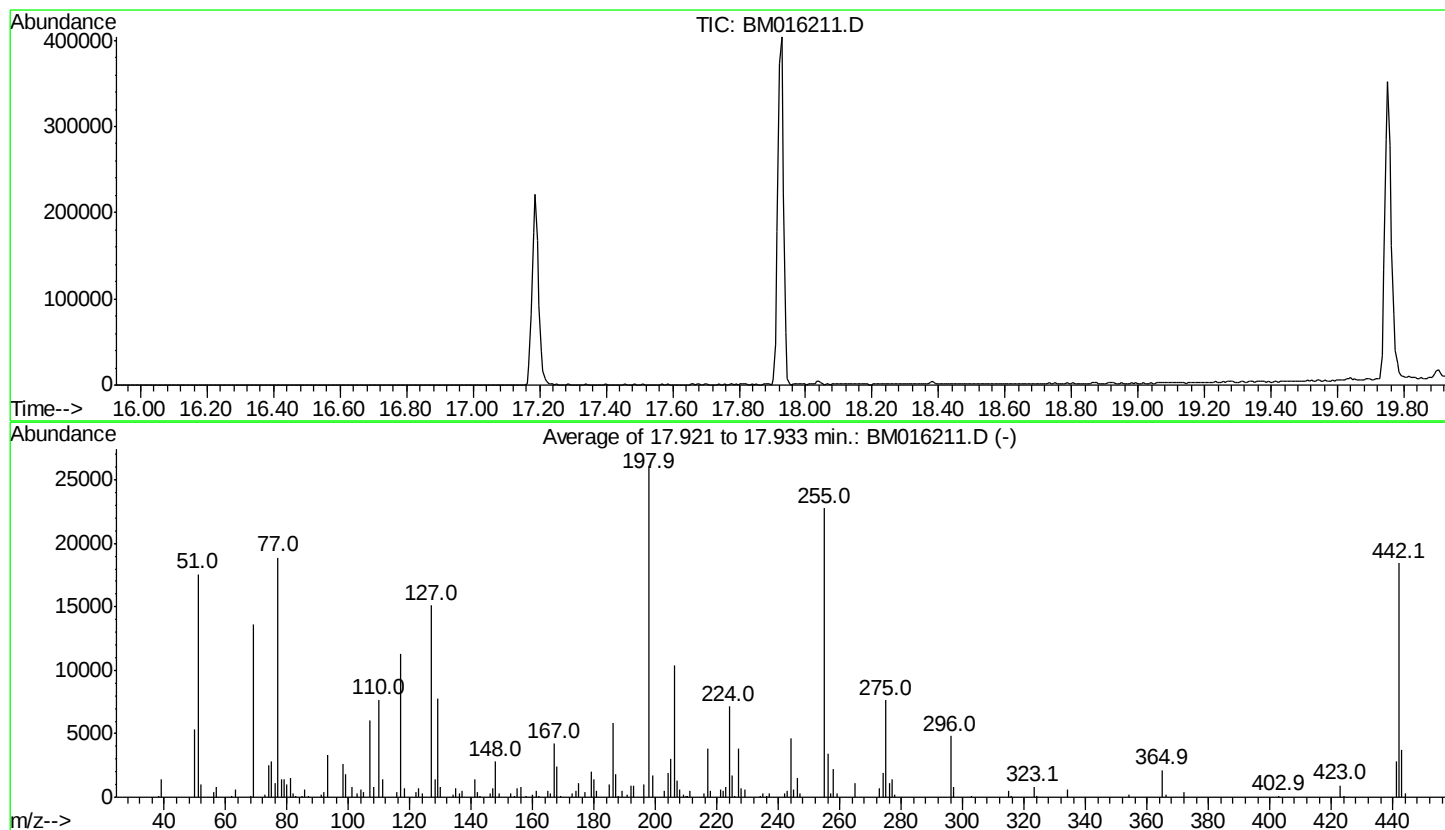

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	67.3	17585	PASS
68	69	0.00	2	1.0	136	PASS
69	198	0.00	100	51.9	13569	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	57.9	15118	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	26122	PASS
199	198	5	9	6.5	1707	PASS
275	198	10	60	29.2	7622	PASS
365	198	1	100	8.3	2165	PASS
441	198	0.01	100	10.8	2817	PASS
442	198	50	100	70.6	18440	PASS
443	442	15	24	20.4	3767	PASS