
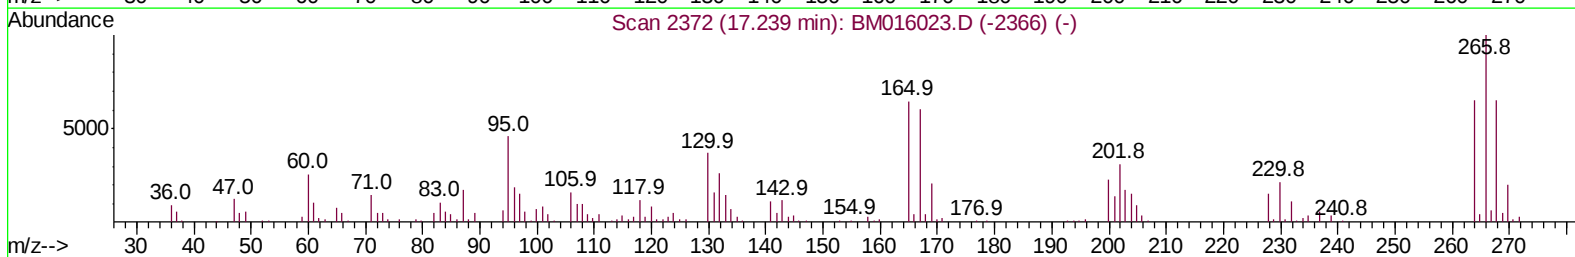
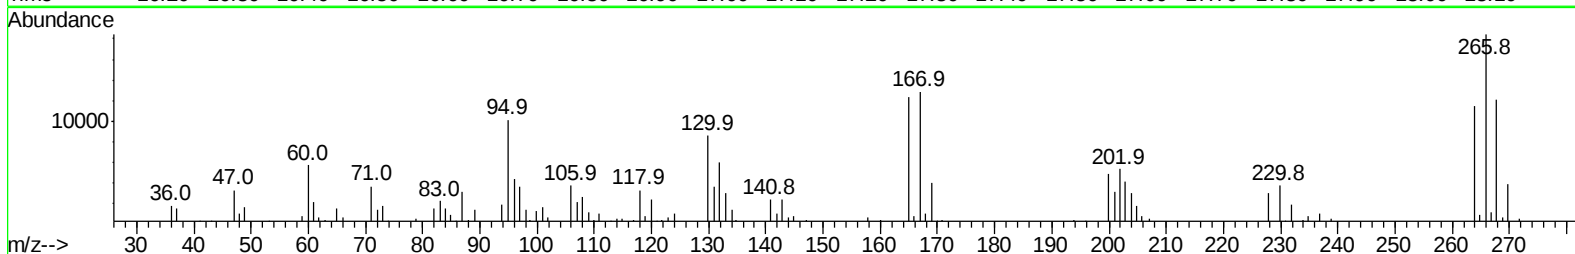


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080718\
Data File : BM016223.D
Acq On : 07 Aug 2018 19:04
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 08 05:12:06 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 07 16:15:57 2018
Response via : Initial Calibration

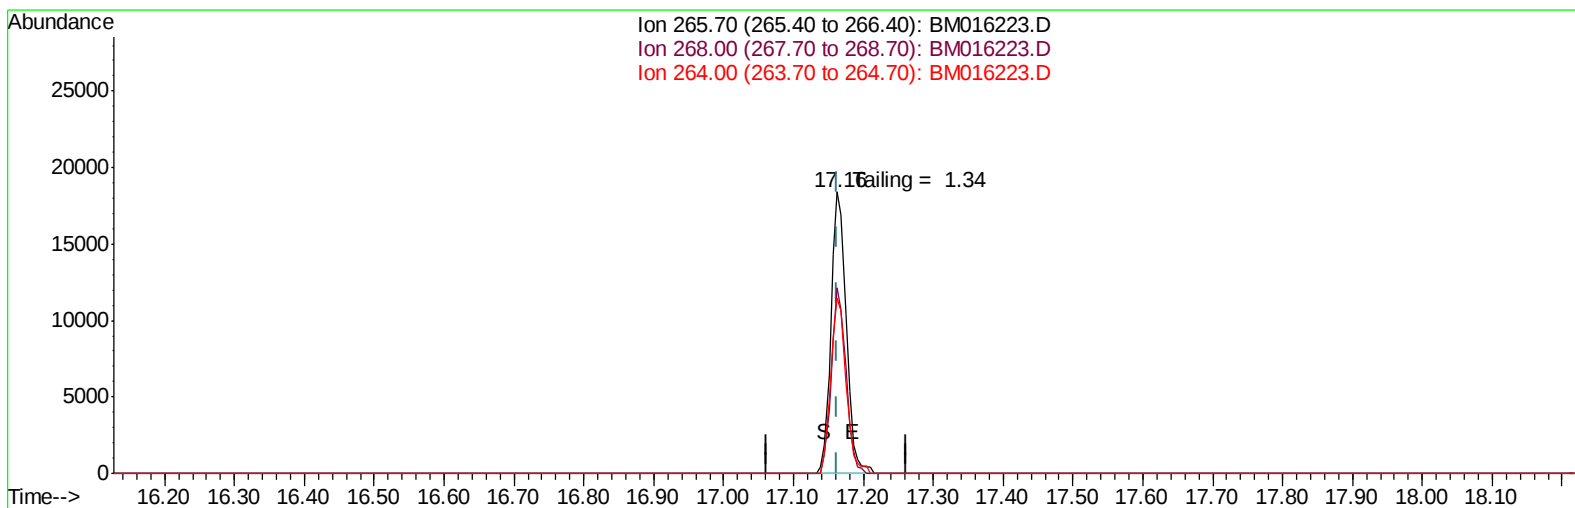

TIC: BM016223.D

(69) Pentachlorophenol (C)




17.162min (-0.000) 31895.49ng

response 27584

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	65.73
264.00	61.20	67.21
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080718\
Data File : BM016223.D
Acq On : 07 Aug 2018 19:04
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 08 05:12:06 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 07 16:15:57 2018
Response via : Initial Calibration

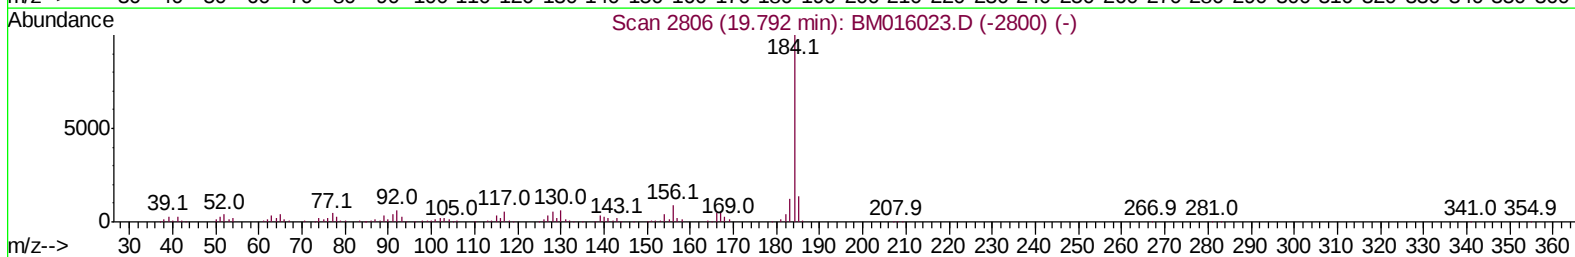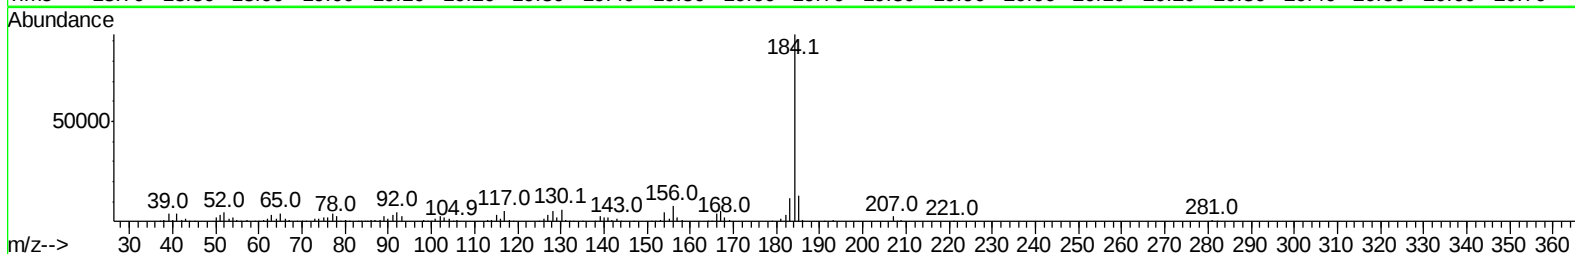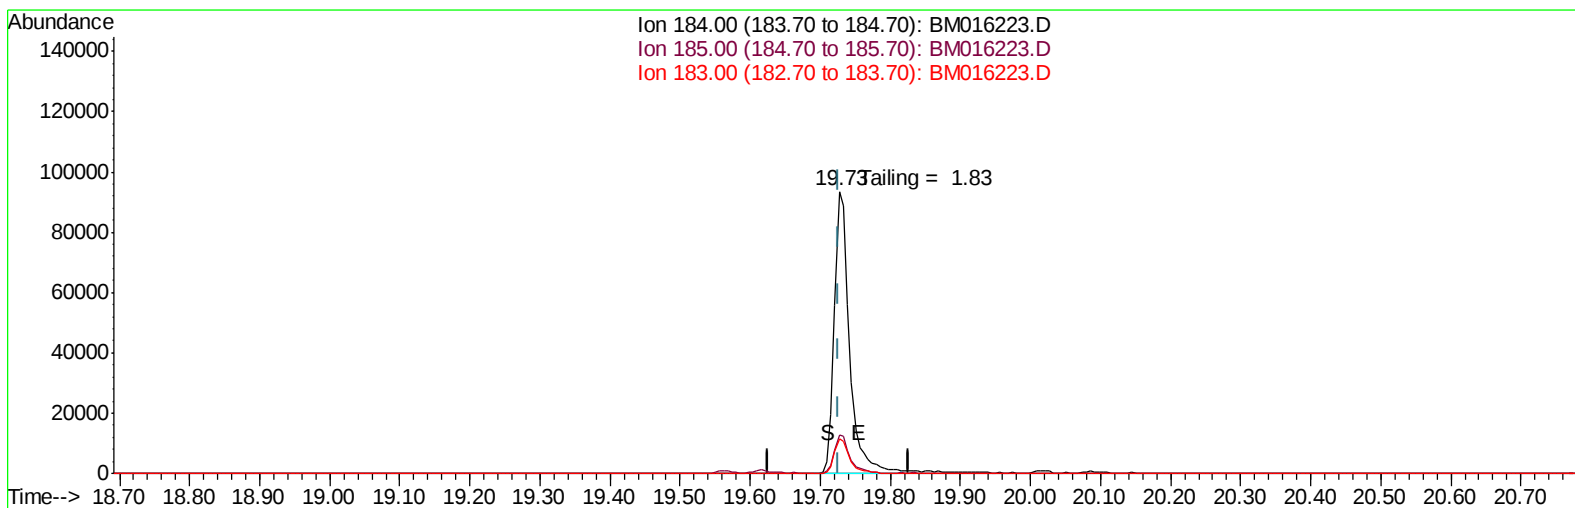

TIC: BM016223.D

(76) Benzidine

19.727min (-0.000) 529.49ng

response 137103

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.78
183.00	11.10	12.42
0.00	0.00	0.00