


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080718\
 Data File : BM016223.D
 Acq On : 07 Aug 2018 19:04
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 07 16:15:57 2018

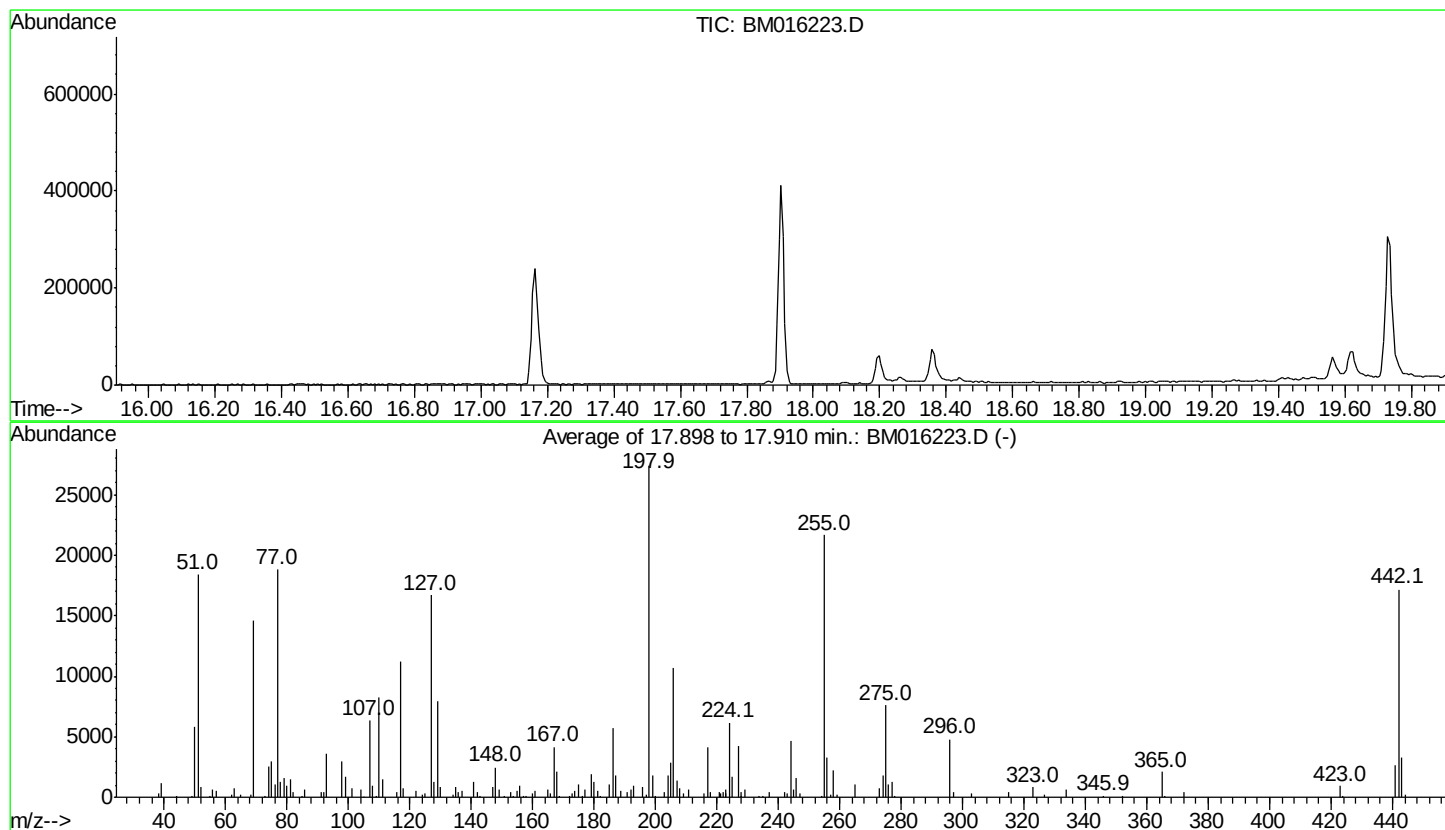

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	67.0	18361	PASS
68	69	0.00	2	1.5	224	PASS
69	198	0.00	100	53.3	14613	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	60.9	16694	PASS
197	198	0.00	2	0.9	259	PASS
198	198	100	100	100.0	27405	PASS
199	198	5	9	6.6	1800	PASS
275	198	10	60	27.8	7608	PASS
365	198	1	100	7.6	2090	PASS
441	198	0.01	100	9.6	2619	PASS
442	198	50	100	62.6	17144	PASS
443	442	15	24	18.9	3247	PASS