
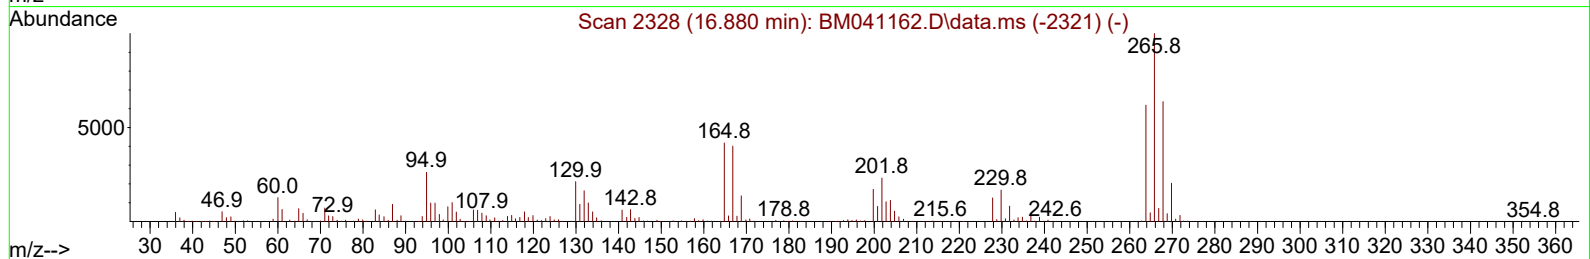
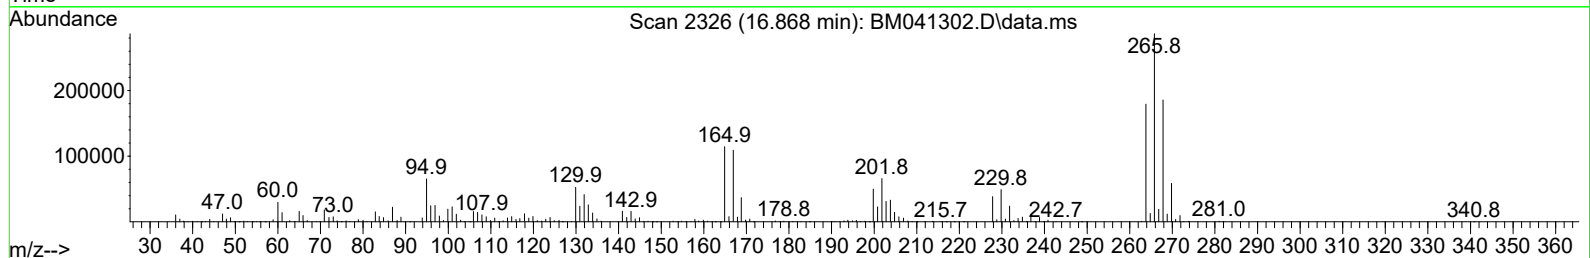


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080723\
Data File : BM041302.D
Acq On : 07 Aug 2023 08:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 11:09:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 19:20:51 2023
Response via : Initial Calibration

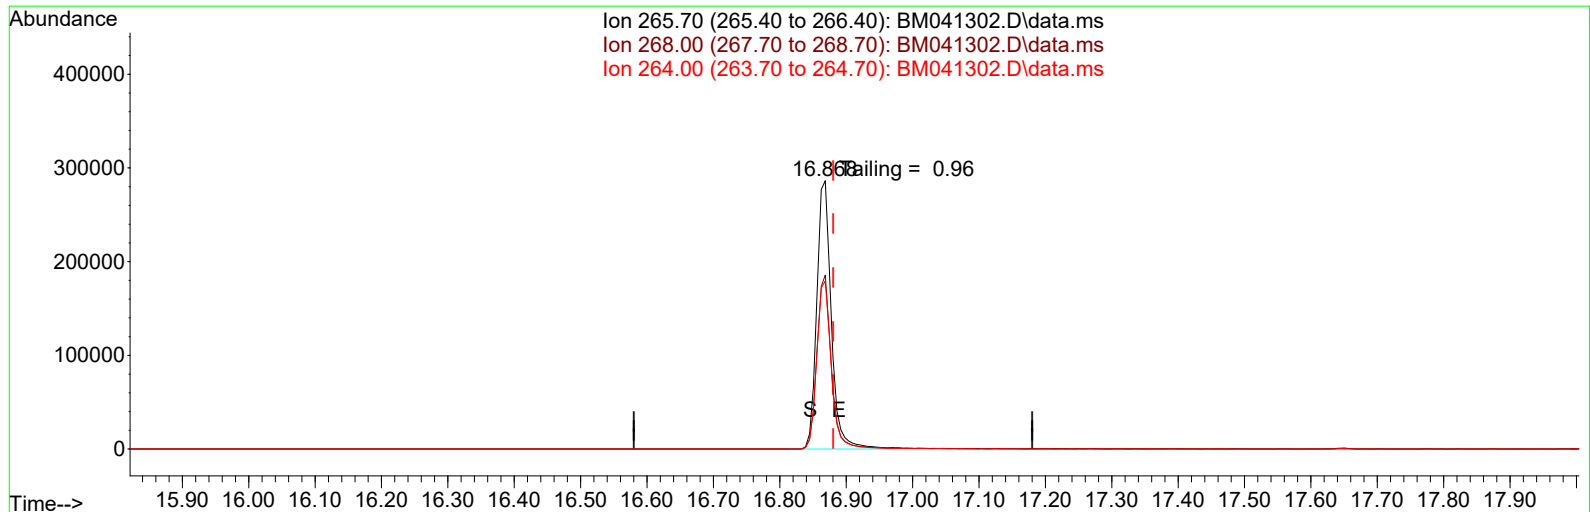

TIC: BM041302.D\data.ms

(70) Pentachlorophenol (C)




16.868min (-0.012) 0.00 ng

response 438381

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.81
264.00	61.80	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080723\
Data File : BM041302.D
Acq On : 07 Aug 2023 08:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 11:09:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 19:20:51 2023
Response via : Initial Calibration

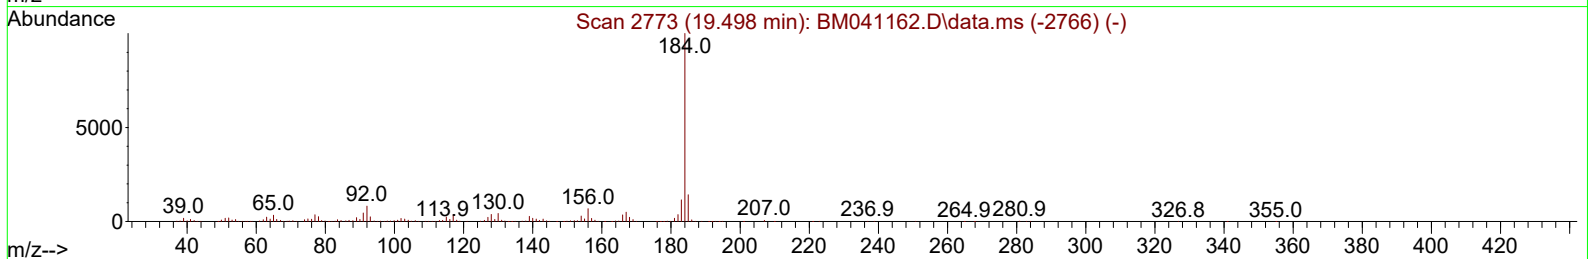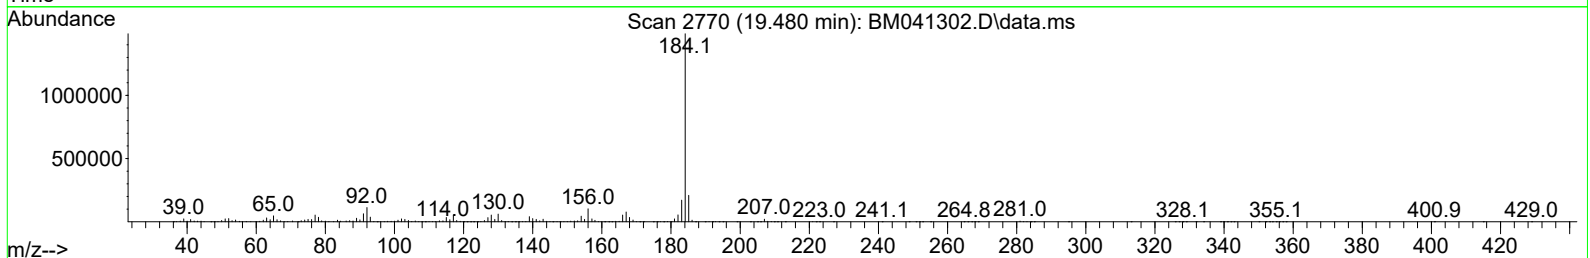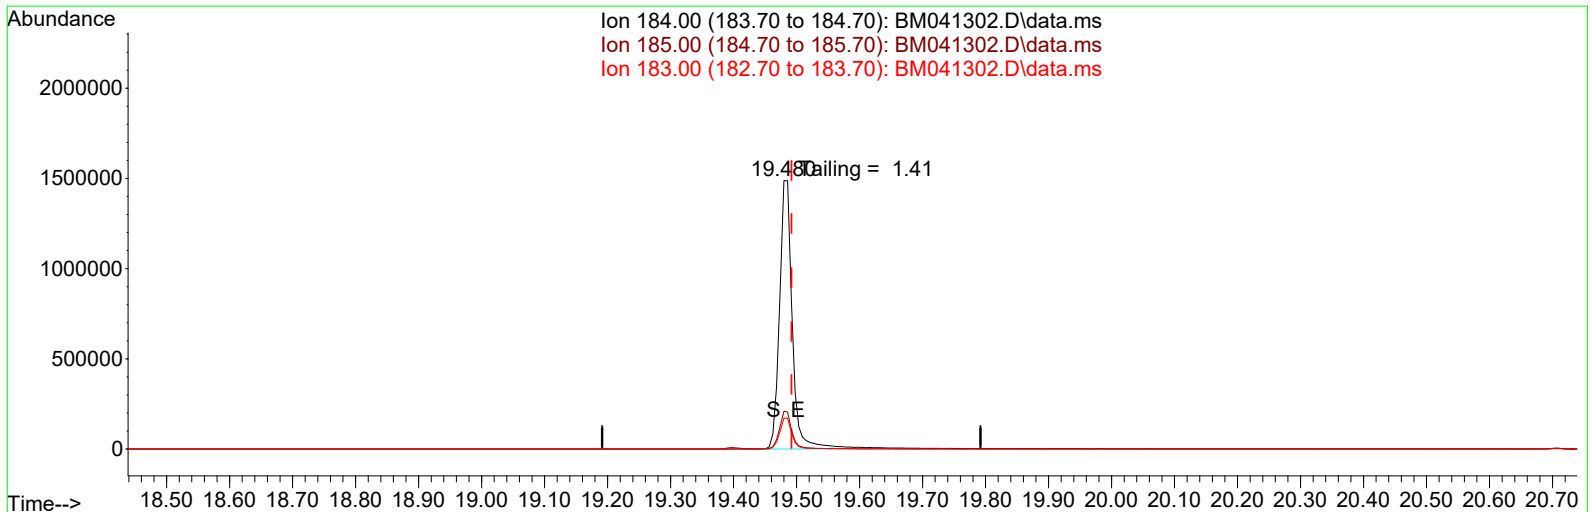

TIC: BM041302.D\data.ms

(77) Benzidine**19.480min (-0.012) 119721.93 ng****response 2140918**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.09
183.00	11.50	11.48
0.00	0.00	0.00