
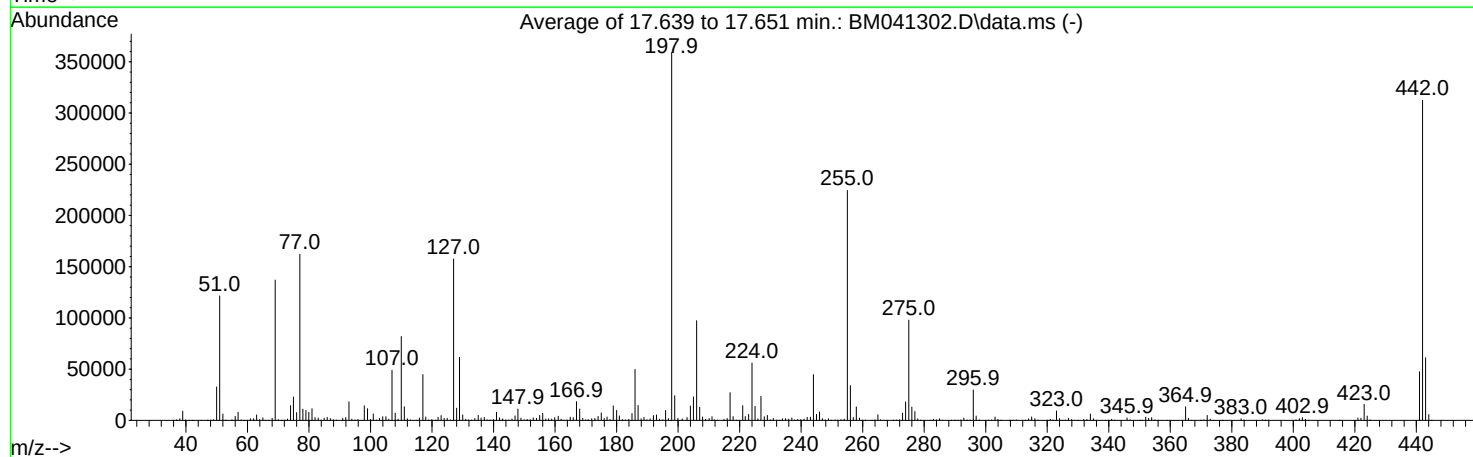


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080723\
Data File : BM041302.D
Acq On : 07 Aug 2023 08:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 07 17:25:06 2023

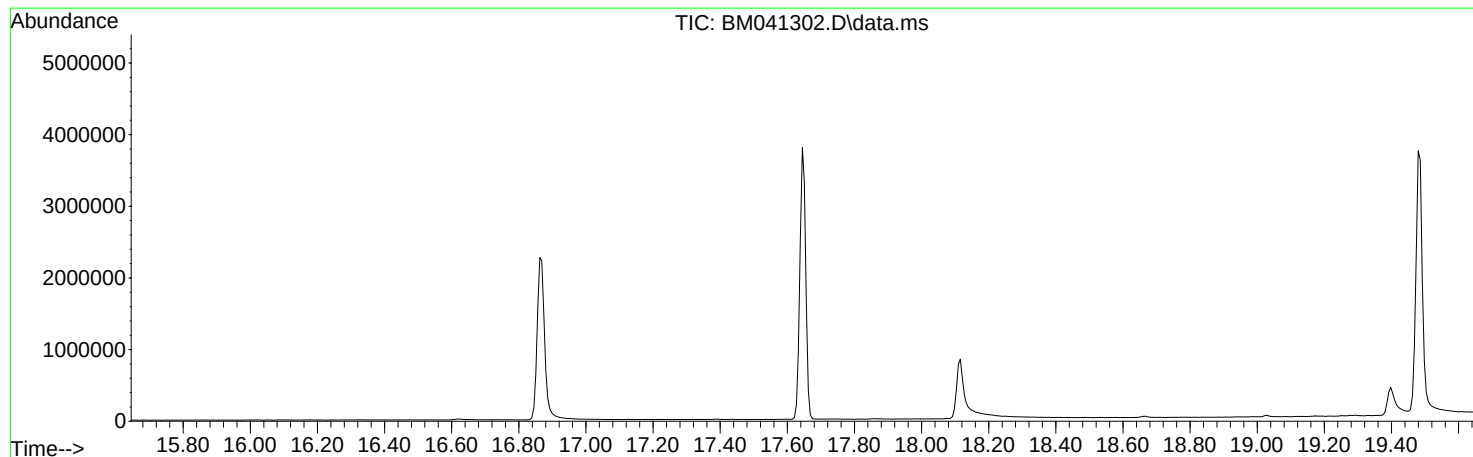




AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	121551	PASS
68	69	0.00	2	1.5	2104	PASS
69	198	0.00	100	38.1	136906	PASS
70	69	0.00	2	0.6	764	PASS
127	198	10	80	43.9	157525	PASS
197	198	0.00	2	0.5	1710	PASS
198	198	100	100	100.0	359040	PASS
199	198	5	9	6.7	24112	PASS
275	198	10	60	27.3	97856	PASS
365	198	1	100	3.7	13267	PASS
441	198	0.01	100	13.2	47453	PASS
442	442	50	100	100.0	312555	PASS
443	442	15	24	19.5	61096	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080723\
Data File : BM041302.D
Acq On : 07 Aug 2023 08:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 07 11:09:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 19:20:51 2023
Response via : Initial Calibration

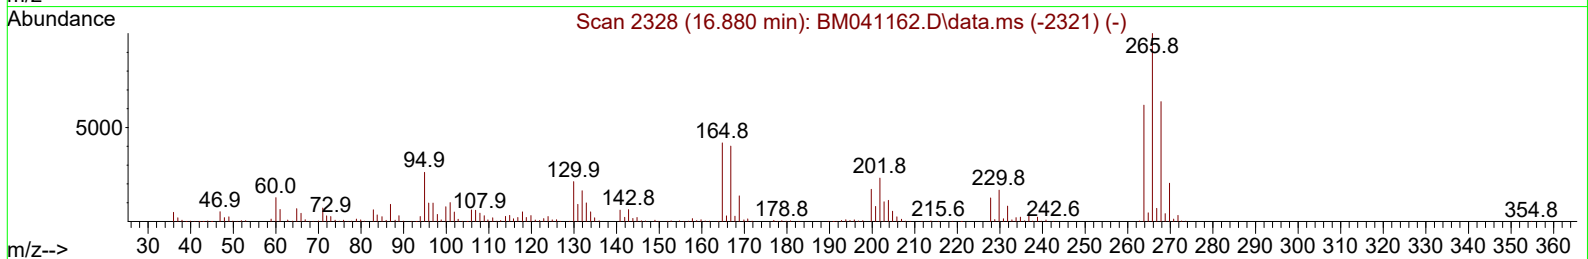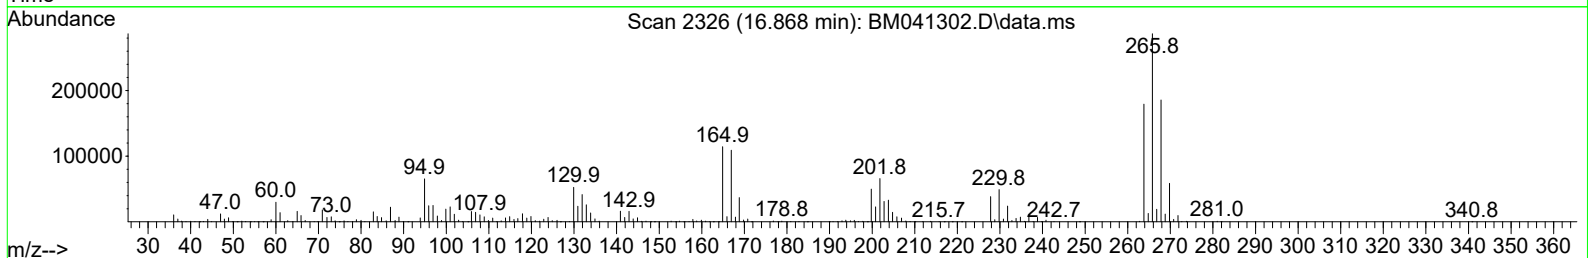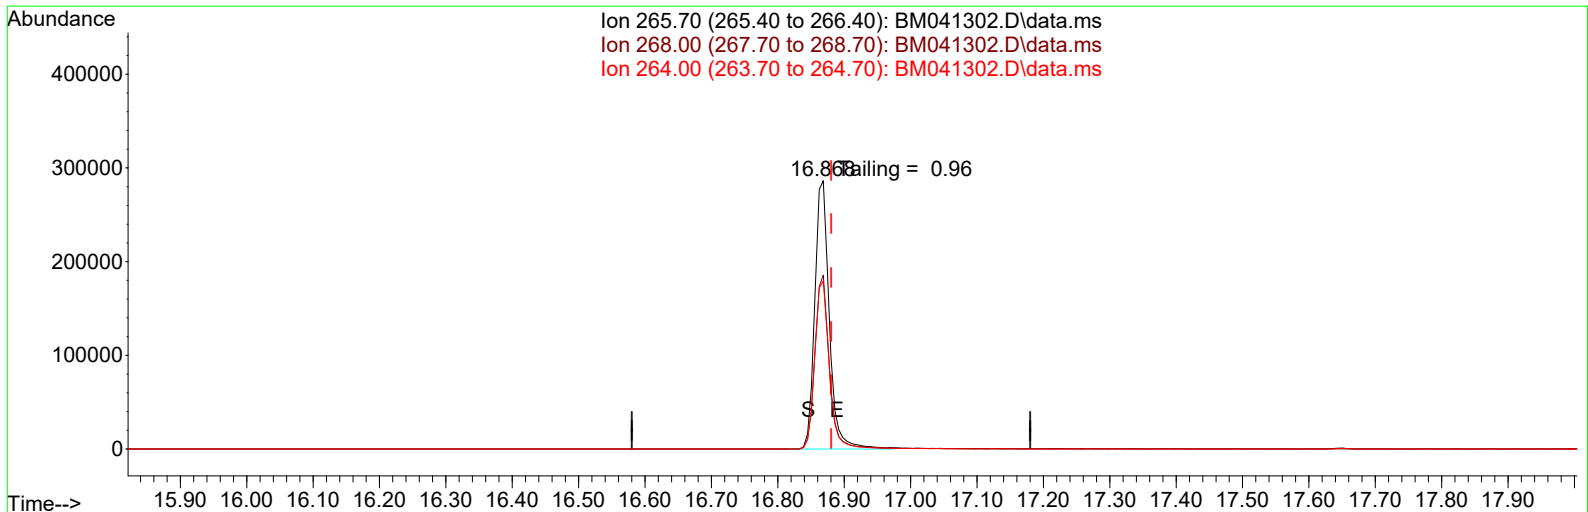

TIC: BM041302.D\data.ms

(70) Pentachlorophenol (C)

16.868min (-0.012) 0.00 ng




response 438381

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.81
264.00	61.80	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080723\
 Data File : BM041302.D
 Acq On : 07 Aug 2023 08:44
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 07 11:09:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 02 19:20:51 2023
 Response via : Initial Calibration

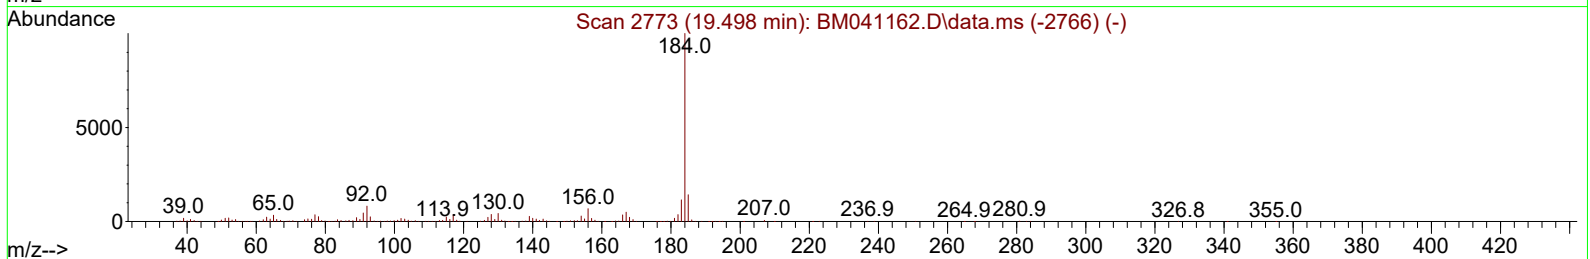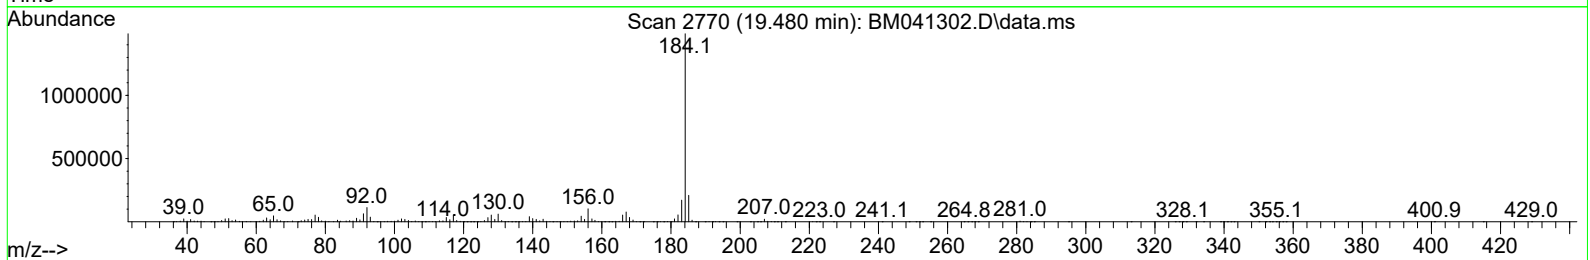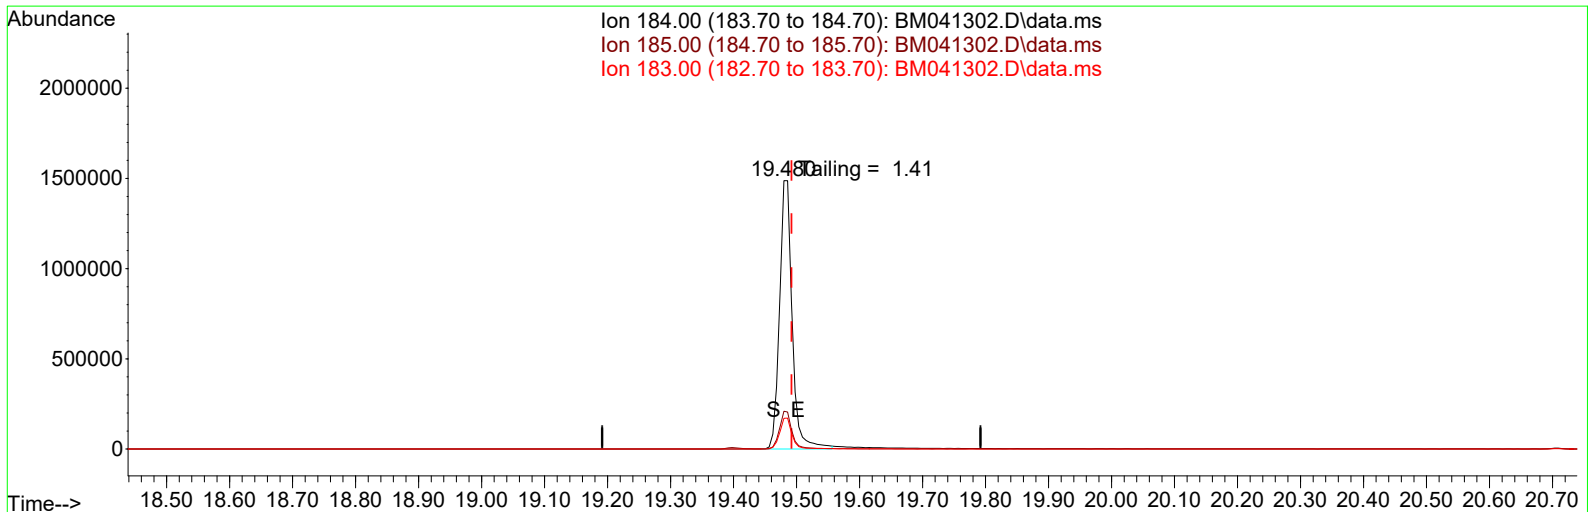

TIC: BM041302.D\data.ms

(77) Benzidine

19.480min (-0.012) 119721.93 ng

response 2140918

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.09
183.00	11.50	11.48
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/7/2023	BNA_M	<u>BM041302.D</u>
Compound Name	Response	Retention Time
DDT	1226280	20.709
DDD	27047	20.268
DDE	2052	19.756
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
29099	1255379	2.32

Instrument :
BNA_M
ClientSampleId :
DFTPP