

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080818\
 Data File : BM016251.D
 Acq On : 08 Aug 2018 15:51
 Operator : SJ/JU
 Sample : J4283-01 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TR-04-080318

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.193	317	324	335	rVB2	18001	29343	4.46%	0.632%
2	5.663	399	404	418	rBV	112953	191873	29.18%	4.130%
3	7.304	678	683	697	rBV	110948	199931	30.40%	4.303%
4	7.663	739	744	757	rBV	135177	225438	34.28%	4.852%
5	8.134	818	824	835	rBV	210070	336032	51.10%	7.233%
6	8.457	873	879	888	rBB	105413	171553	26.09%	3.692%
7	9.328	1021	1027	1037	rBV	63447	116535	17.72%	2.508%
8	10.951	1297	1303	1318	rVB	246340	405924	61.72%	8.737%
9	13.392	1712	1718	1726	rBV	160311	227207	34.55%	4.890%
10	14.228	1856	1860	1864	rBV	10025	12495	1.90%	0.269%
11	14.769	1946	1952	1961	rVB2	296684	441090	67.07%	9.494%
12	16.257	2200	2205	2214	rBV	105931	151272	23.00%	3.256%
13	17.504	2411	2417	2423	rBV	336700	466677	70.96%	10.044%
14	18.351	2557	2561	2569	rBV3	24576	37565	5.71%	0.809%
15	19.539	2761	2763	2770	rBV	9166	12309	1.87%	0.265%
16	19.615	2772	2776	2782	rBV6	15448	20627	3.14%	0.444%
17	19.904	2821	2825	2829	rBV3	14462	20518	3.12%	0.442%
18	20.086	2851	2856	2861	rVB	249512	291847	44.38%	6.282%
19	20.362	2897	2903	2909	rBV8	12206	31695	4.82%	0.682%
20	21.633	3114	3119	3124	rBV	460238	598516	91.01%	12.882%
21	23.974	3511	3517	3530	rVB2	322299	657659	100.00%	14.155%


Sum of corrected areas: 4646106

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080818\
Data File : BM016251.D
Acq On : 08 Aug 2018 15:51
Operator : SJ/JU
Sample : J4283-01 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
TR-04-080318

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

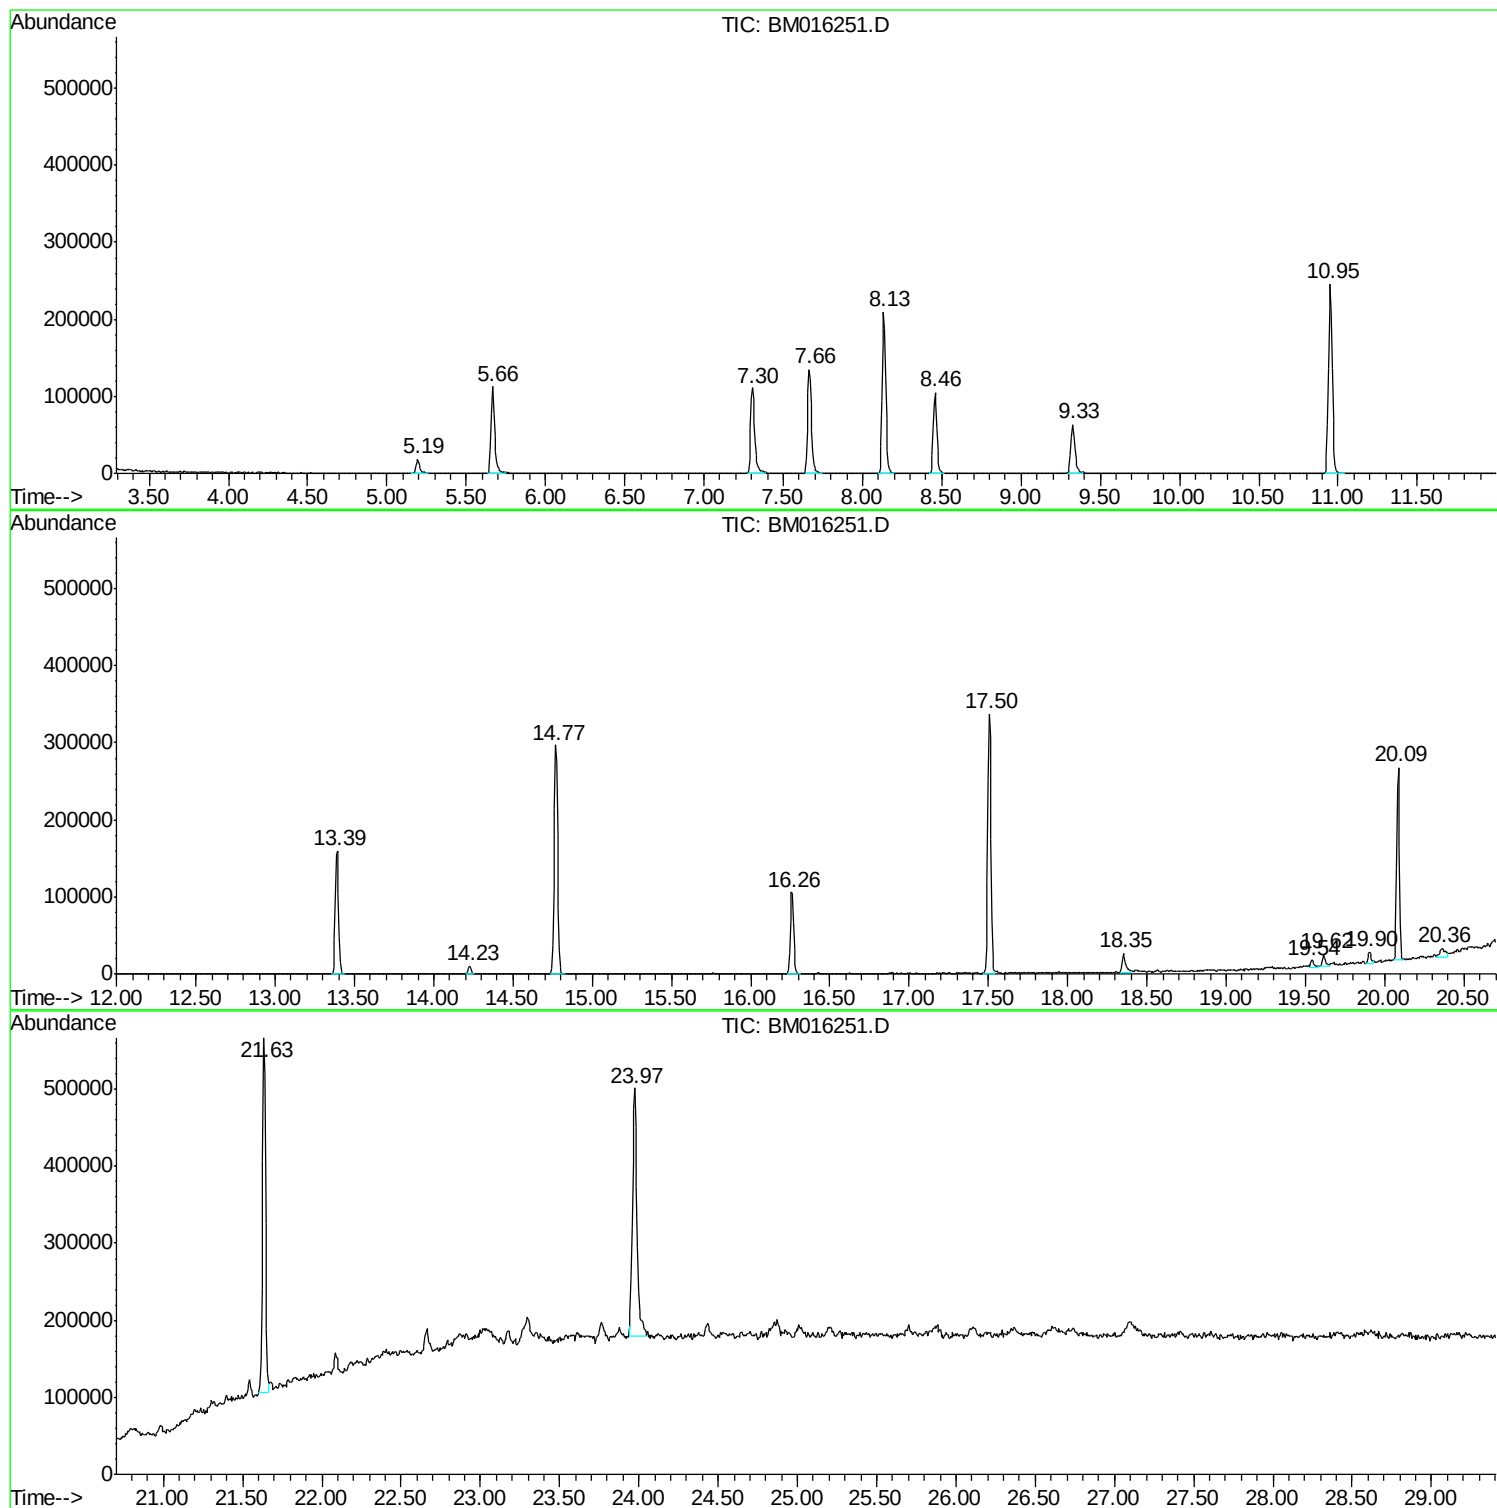

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080818\
Data File : BM016251.D
Acq On : 08 Aug 2018 15:51
Operator : SJ/JU
Sample : J4283-01 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TR-04-080318










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.66 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.66	13.42 ng	225438	1,4-Dichlorobenzene-d4	8.13

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	18
2		3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	14
3		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	14
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	14
5		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	14

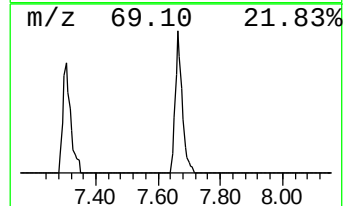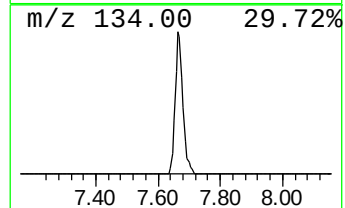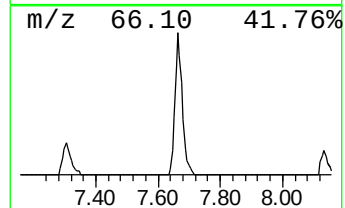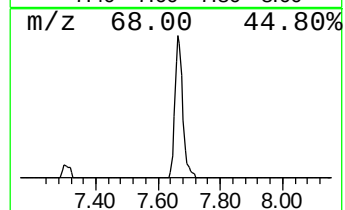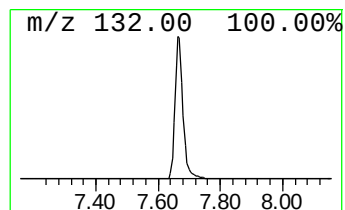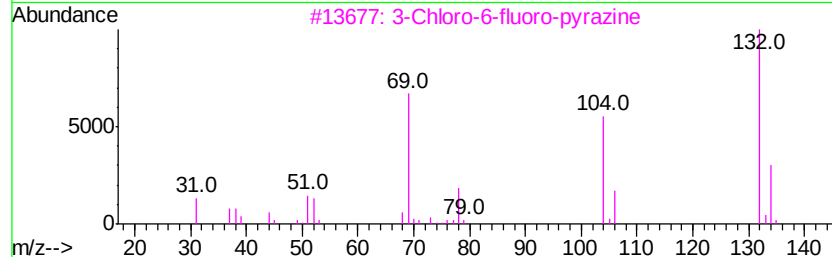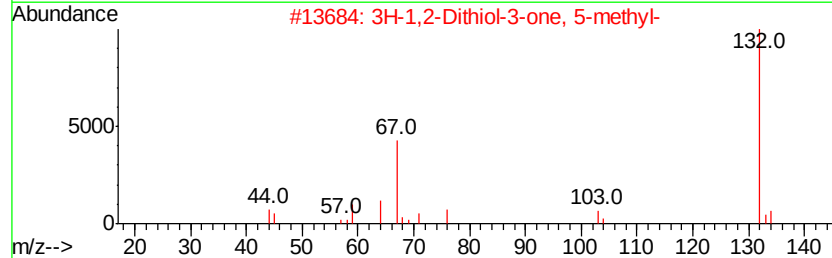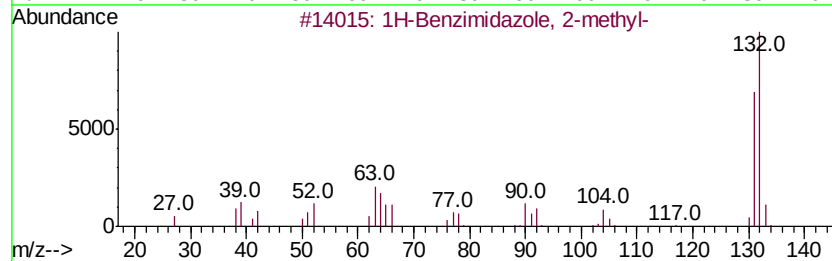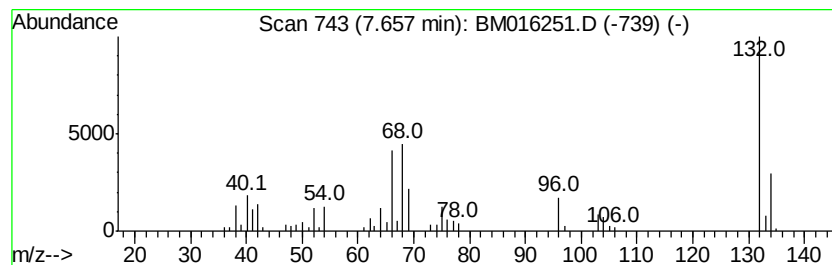

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080818\
Data File : BM016251.D
Acq On : 08 Aug 2018 15:51
Operator : SJ/JU
Sample : J4283-01 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TR-04-080318

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.66	7.66	13.4	ng	225438	1	8.13	336032	20.0