


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080818\
 Data File : BM016243.D
 Acq On : 08 Aug 2018 09:25
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 08 16:23:37 2018

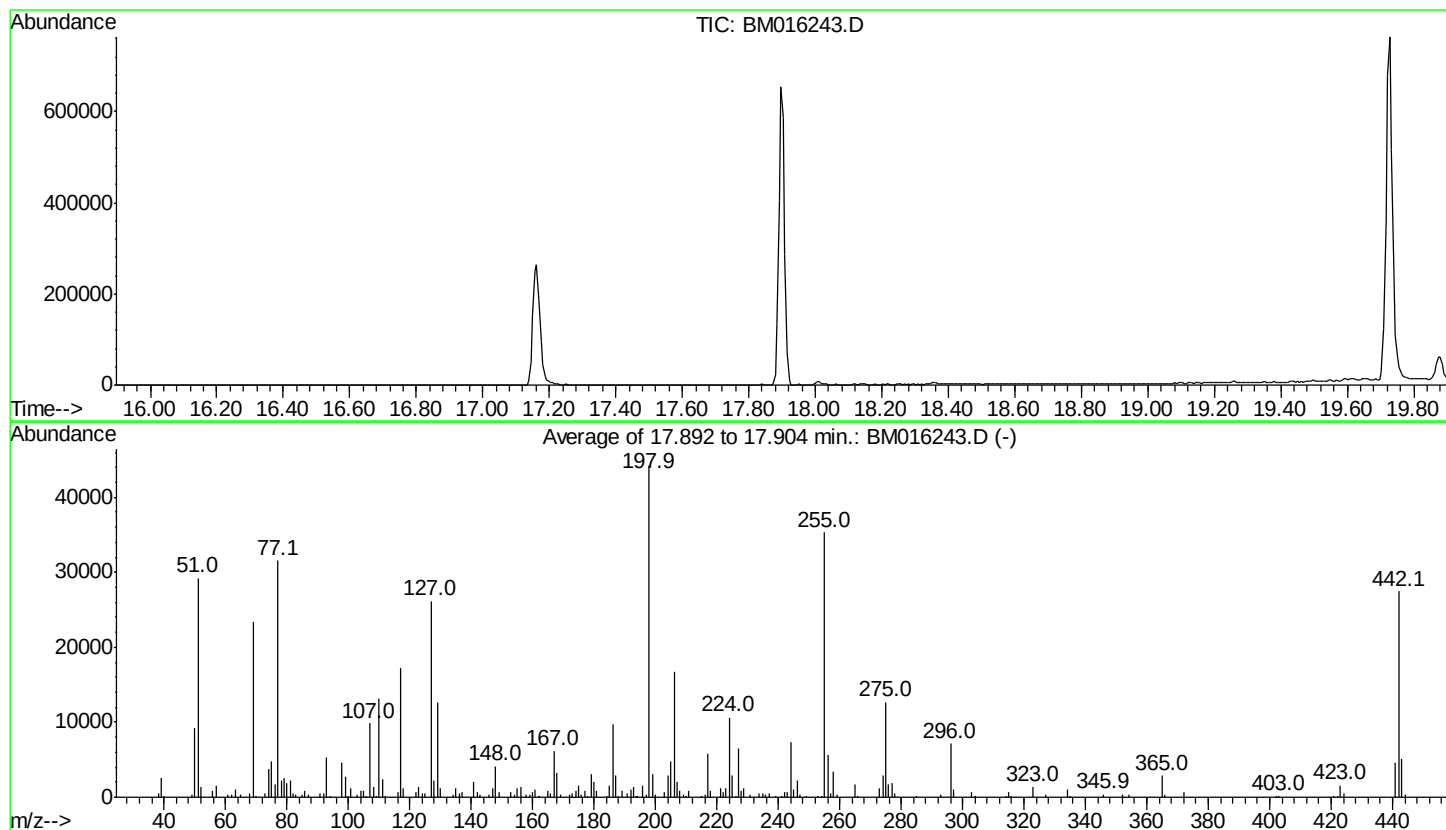

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	66.1	29253	PASS
68	69	0.00	2	1.9	451	PASS
69	198	0.00	100	52.8	23368	PASS
70	69	0.00	2	0.5	111	PASS
127	198	10	80	59.1	26149	PASS
197	198	0.00	2	0.8	372	PASS
198	198	100	100	100.0	44229	PASS
199	198	5	9	7.0	3076	PASS
275	198	10	60	28.6	12652	PASS
365	198	1	100	6.5	2875	PASS
441	198	0.01	100	10.4	4586	PASS
442	198	50	100	62.0	27431	PASS
443	442	15	24	18.7	5119	PASS