


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080818\  
 Data File : BM016261.D  
 Acq On : 08 Aug 2018 23:12  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM072318.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Aug 08 16:23:37 2018

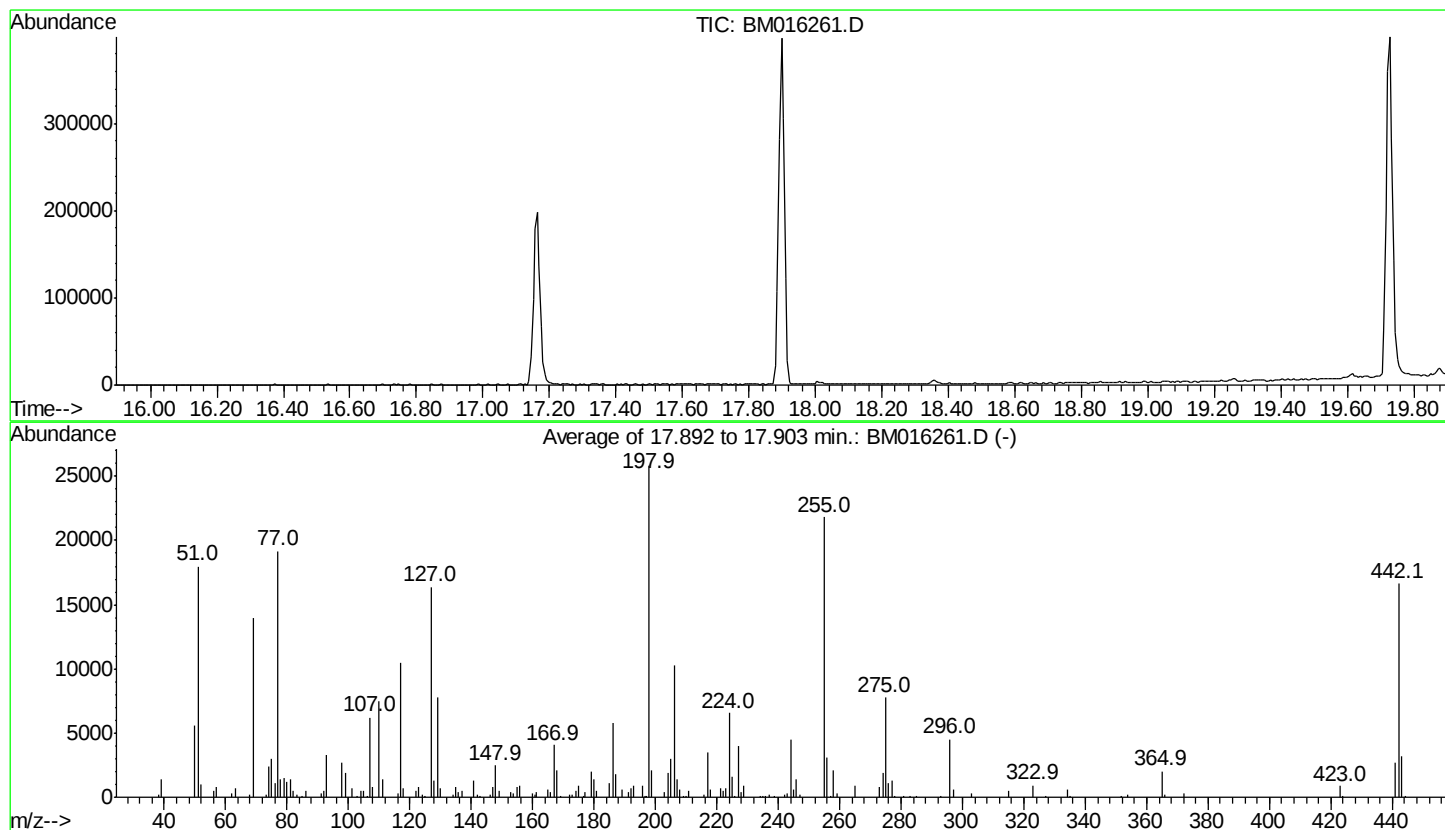

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2477

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 69.6      | 17966   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.7       | 239     | PASS             |
| 69          | 198          | 0.00         | 100          | 54.2      | 13996   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 63.3      | 16357   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.5       | 126     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 25829   | PASS             |
| 199         | 198          | 5            | 9            | 7.9       | 2048    | PASS             |
| 275         | 198          | 10           | 60           | 29.9      | 7731    | PASS             |
| 365         | 198          | 1            | 100          | 7.8       | 2007    | PASS             |
| 441         | 198          | 0.01         | 100          | 10.6      | 2734    | PASS             |
| 442         | 198          | 50           | 100          | 64.3      | 16612   | PASS             |
| 443         | 442          | 15           | 24           | 19.5      | 3233    | PASS             |