
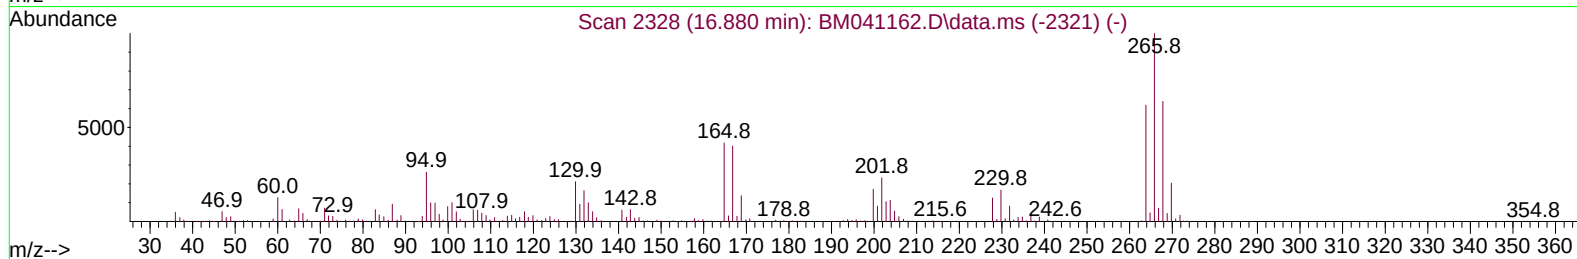
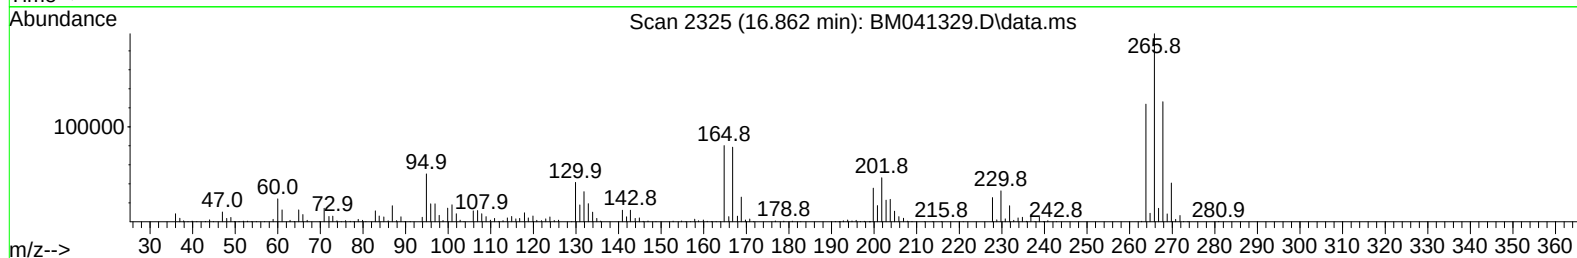


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080823\
Data File : BM041329.D
Acq On : 08 Aug 2023 14:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 02:35:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 07 17:25:06 2023
Response via : Initial Calibration

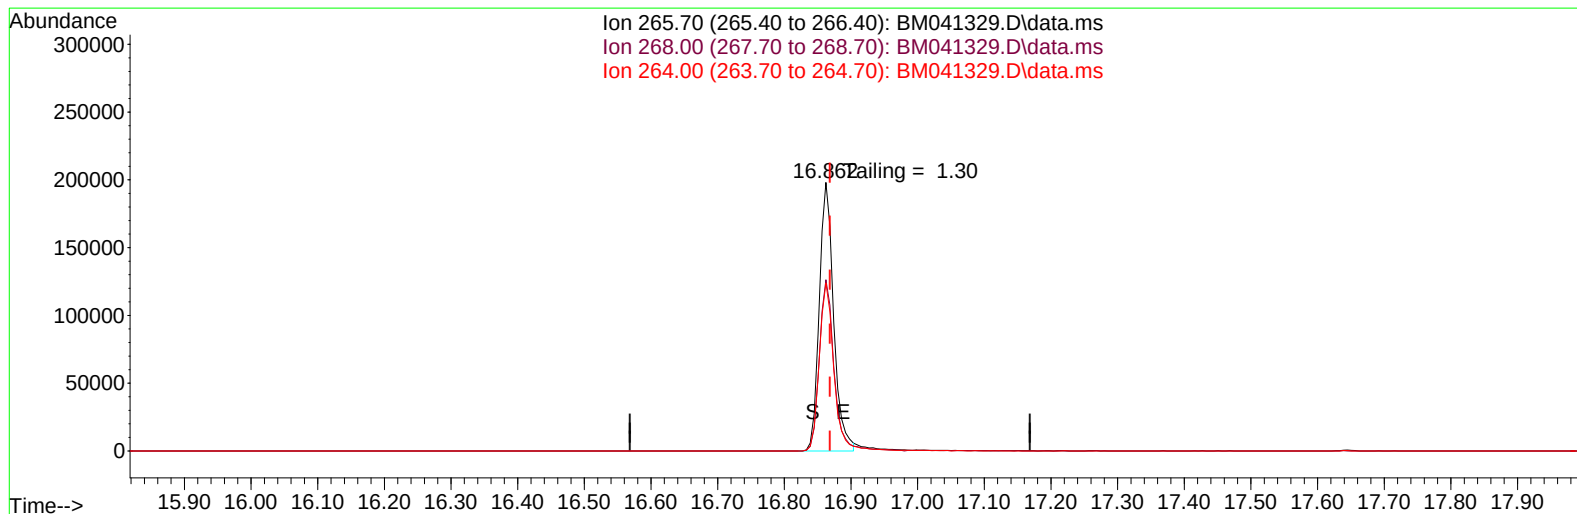

TIC: BM041329.D\data.ms

(70) Pentachlorophenol (C)




16.862min (-0.006) 0.00 ng

response 305110

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.80
264.00	61.80	62.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080823\
Data File : BM041329.D
Acq On : 08 Aug 2023 14:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 02:35:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 07 17:25:06 2023
Response via : Initial Calibration

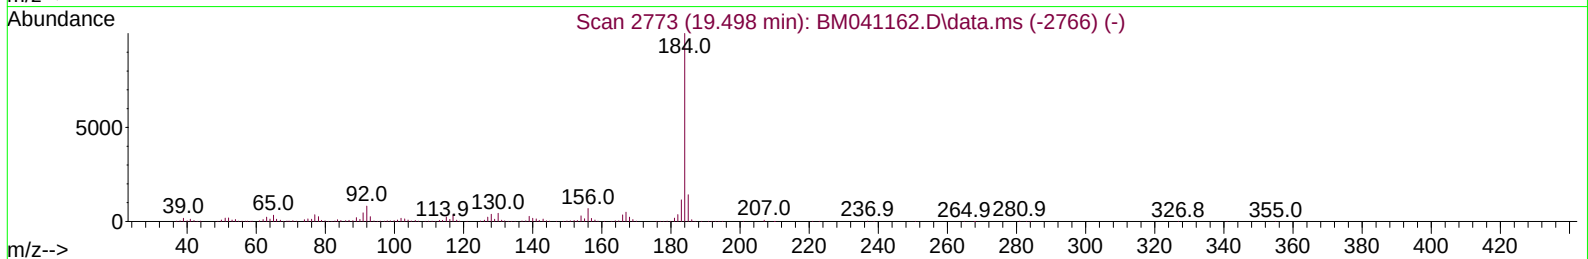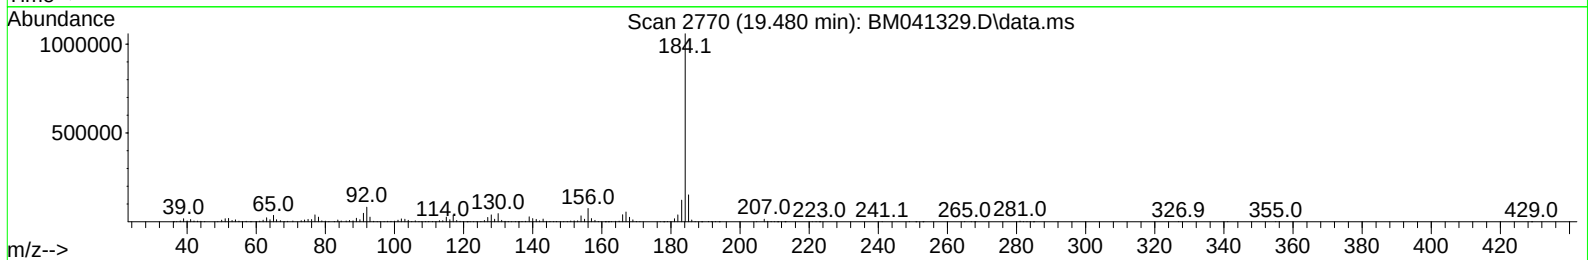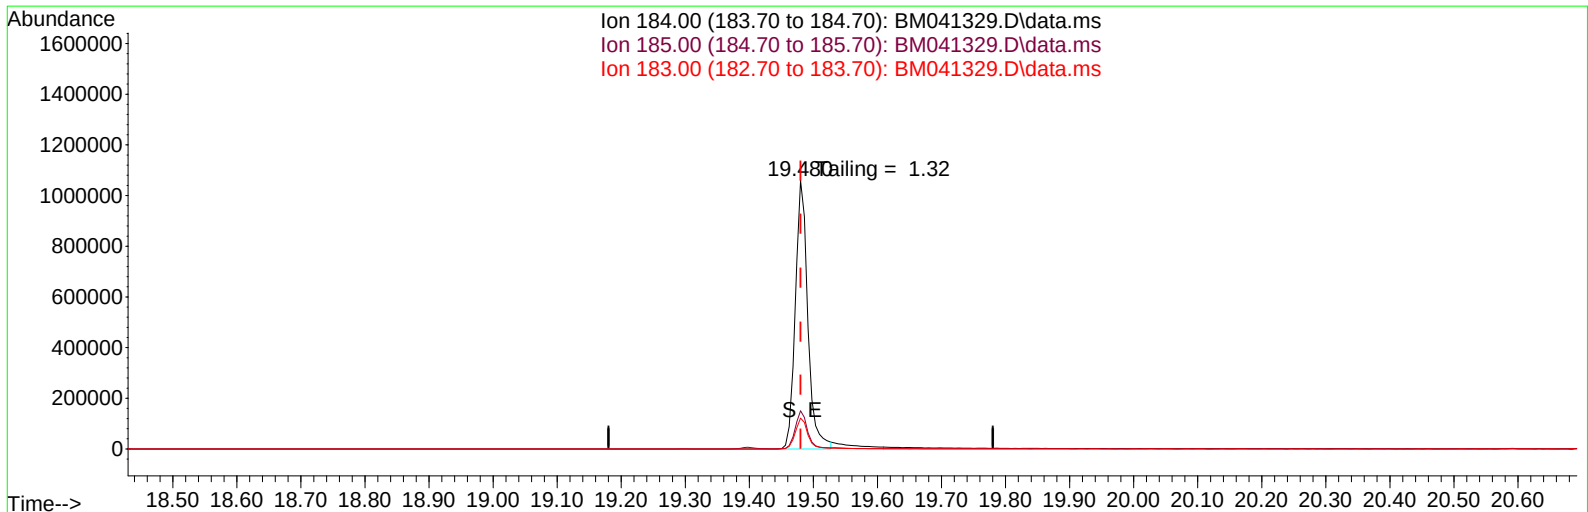

TIC: BM041329.D\data.ms

(77) Benzidine**19.480min (+ 0.000) 68868.71 ng****response 1525344**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.26
183.00	11.50	11.50
0.00	0.00	0.00