


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080823\
Data File : BM041329.D
Acq On : 08 Aug 2023 14:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 07 17:25:06 2023

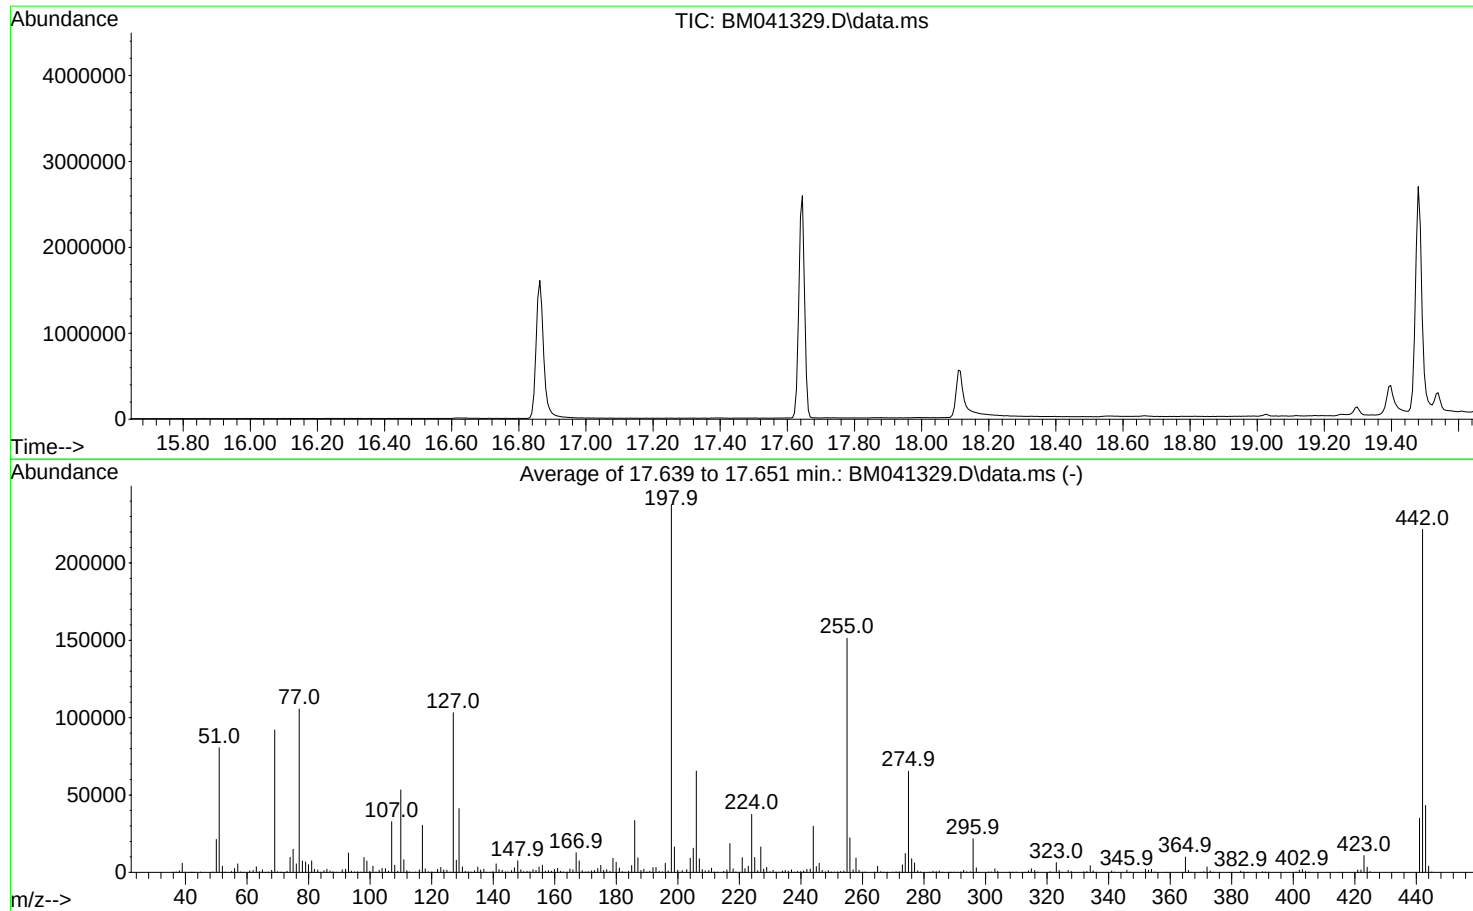




AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	80590	PASS
68	69	0.00	2	1.5	1382	PASS
69	198	0.00	100	38.7	92013	PASS
70	69	0.00	2	0.5	434	PASS
127	198	10	80	43.4	103229	PASS
197	198	0.00	2	0.4	989	PASS
198	198	100	100	100.0	237803	PASS
199	198	5	9	6.9	16414	PASS
275	198	10	60	27.5	65427	PASS
365	198	1	100	4.2	9906	PASS
441	198	0.01	100	14.7	34973	PASS
442	442	50	100	100.0	221739	PASS
443	442	15	24	19.5	43309	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080823\
Data File : BM041329.D
Acq On : 08 Aug 2023 14:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 09 02:35:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 07 17:25:06 2023
Response via : Initial Calibration

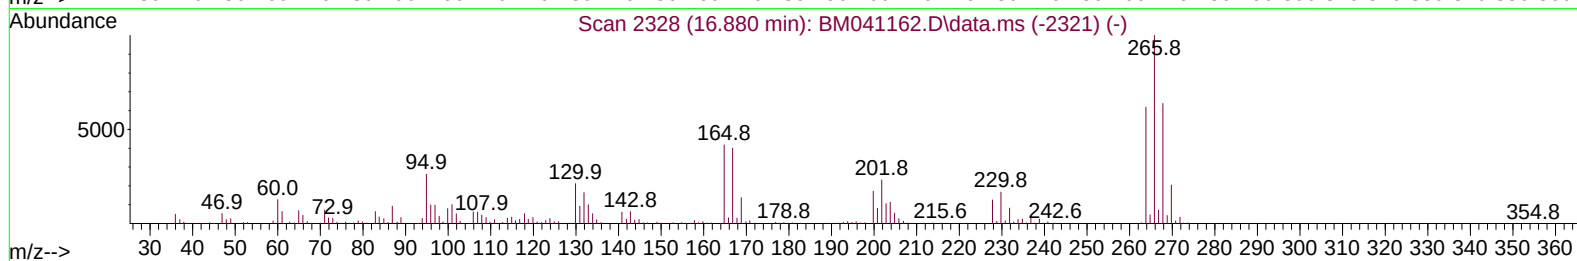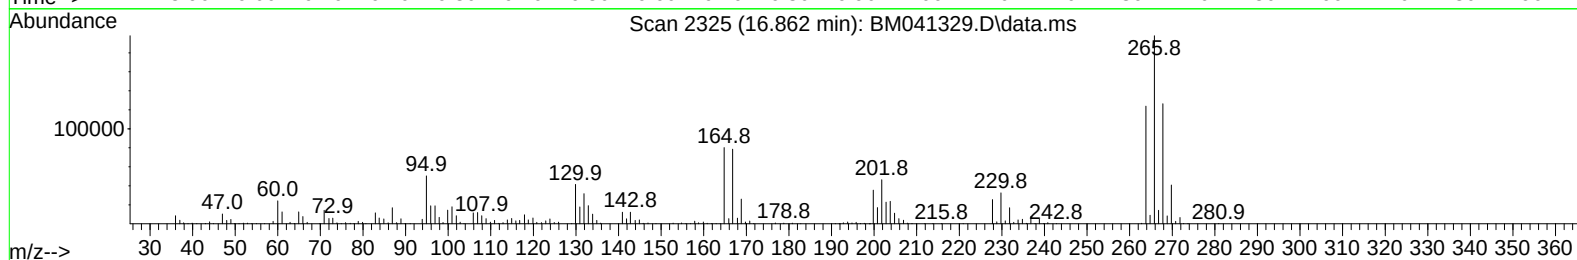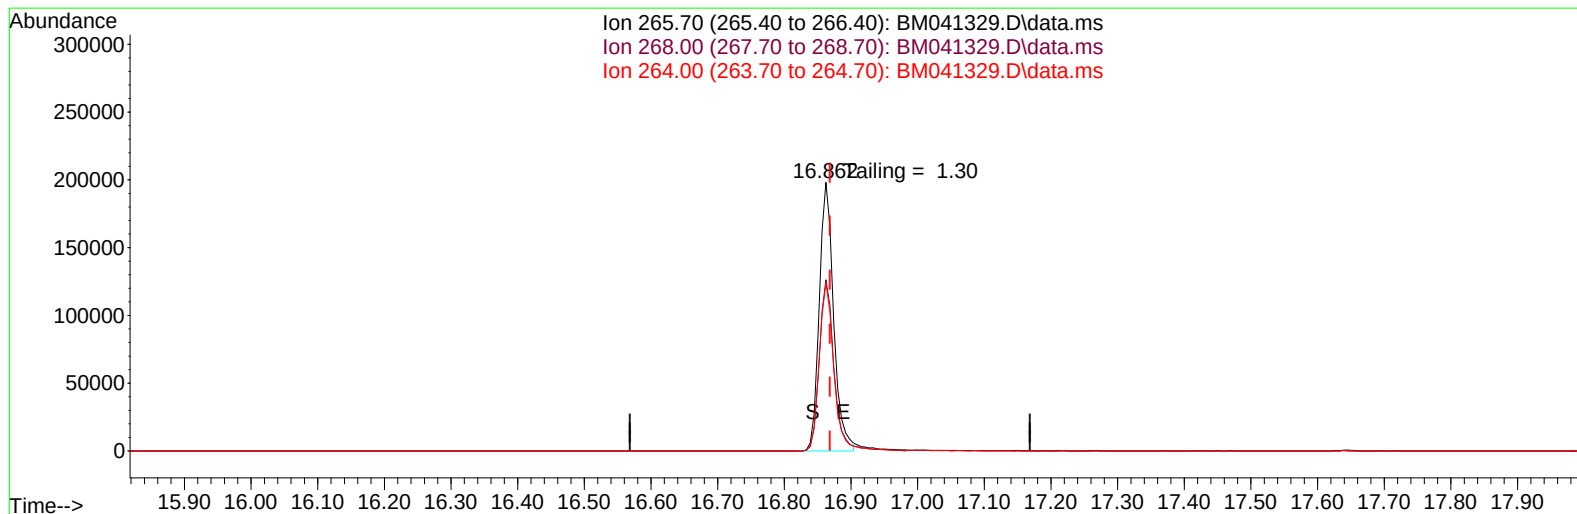

TIC: BM041329.D\data.ms

(70) Pentachlorophenol (C)

16.862min (-0.006) 0.00 ng




response 305110

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.80
264.00	61.80	62.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080823\
Data File : BM041329.D
Acq On : 08 Aug 2023 14:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 09 02:35:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 07 17:25:06 2023
Response via : Initial Calibration

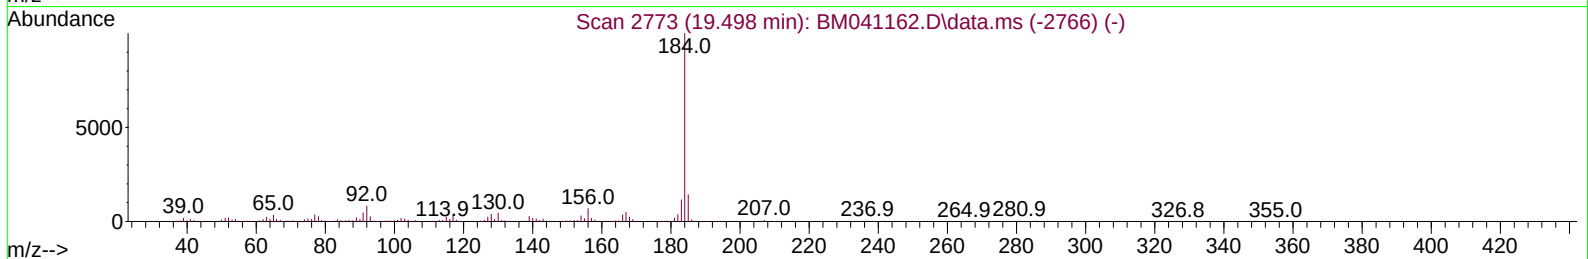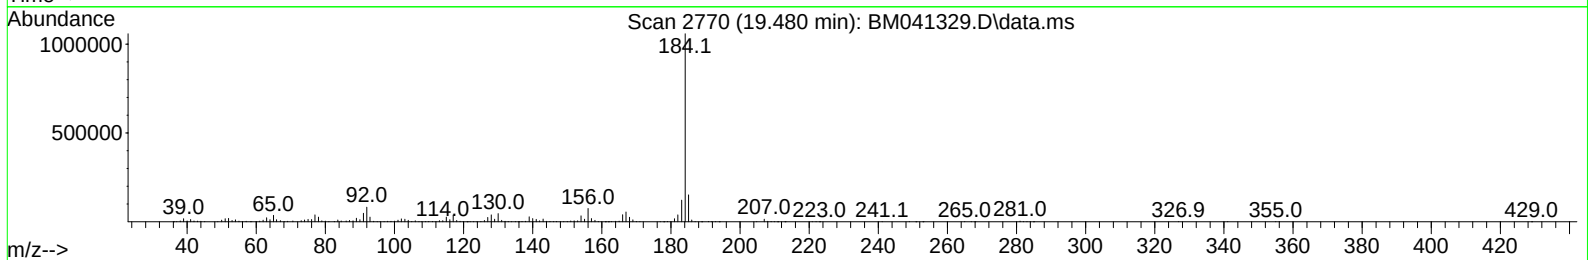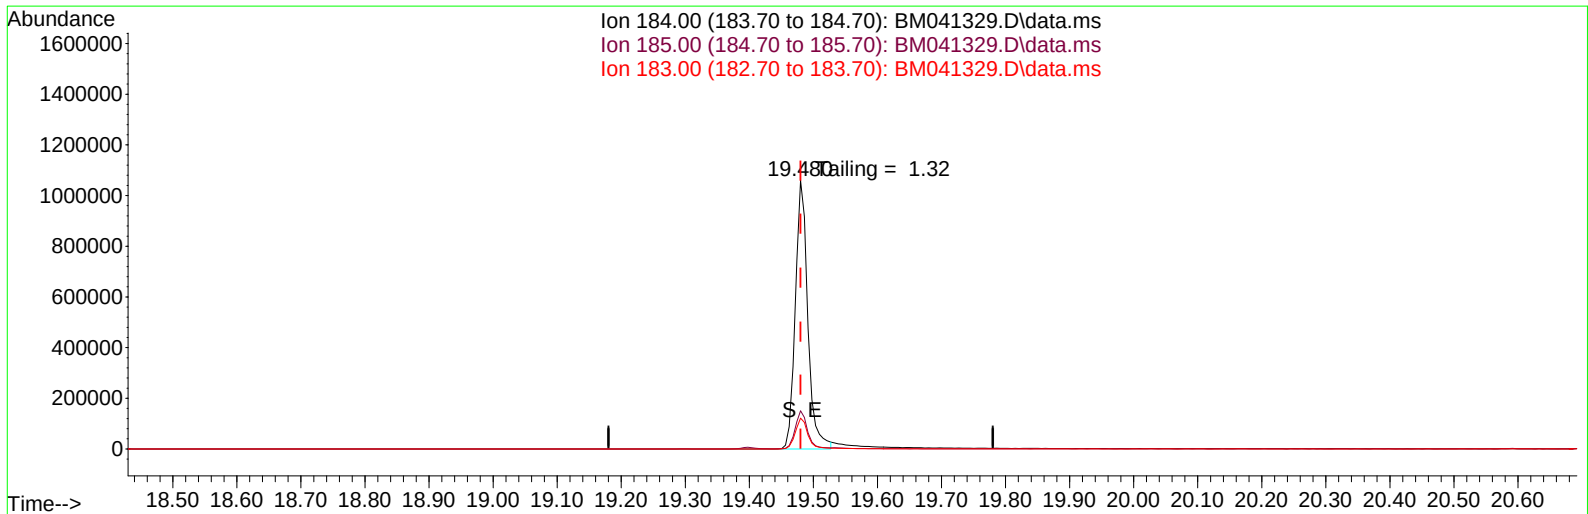

TIC: BM041329.D\data.ms

(77) Benzidine

19.480min (+ 0.000) 68868.71 ng

response 1525344

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.26
183.00	11.50	11.50
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/8/2023	BNA_M	<u>BM041329.D</u>
Compound Name	Response	Retention Time
DDT	933932	20.703
DDD	16313	20.268
DDE	1110	19.751
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17423	951355	1.83

Instrument :
BNA_M
ClientSampleId :
DFTPP