

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
 Data File : BM021975.D
 Acq On : 09 Aug 2019 18:36
 Operator : HP/JU
 Sample : K4117-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 10 05:23:24 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 09 01:29:50 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	784	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.39	136	3420	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.27	164	1968	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.12	188	226271	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.30	264	276123	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.99	152	1602	0.28	ng/ul	-0.03
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	10.48	128	1065	0.110	ng/ul	97
7) Acenaphthylene	13.99	152	212	0.023	ng/ul#	43


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
 Data File : BM021975.D
 Acq On : 09 Aug 2019 18:36
 Operator : HP/JU
 Sample : K4117-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :

Quant Time: Aug 10 05:23:24 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 09 01:29:50 2019
 Response via : Initial Calibration




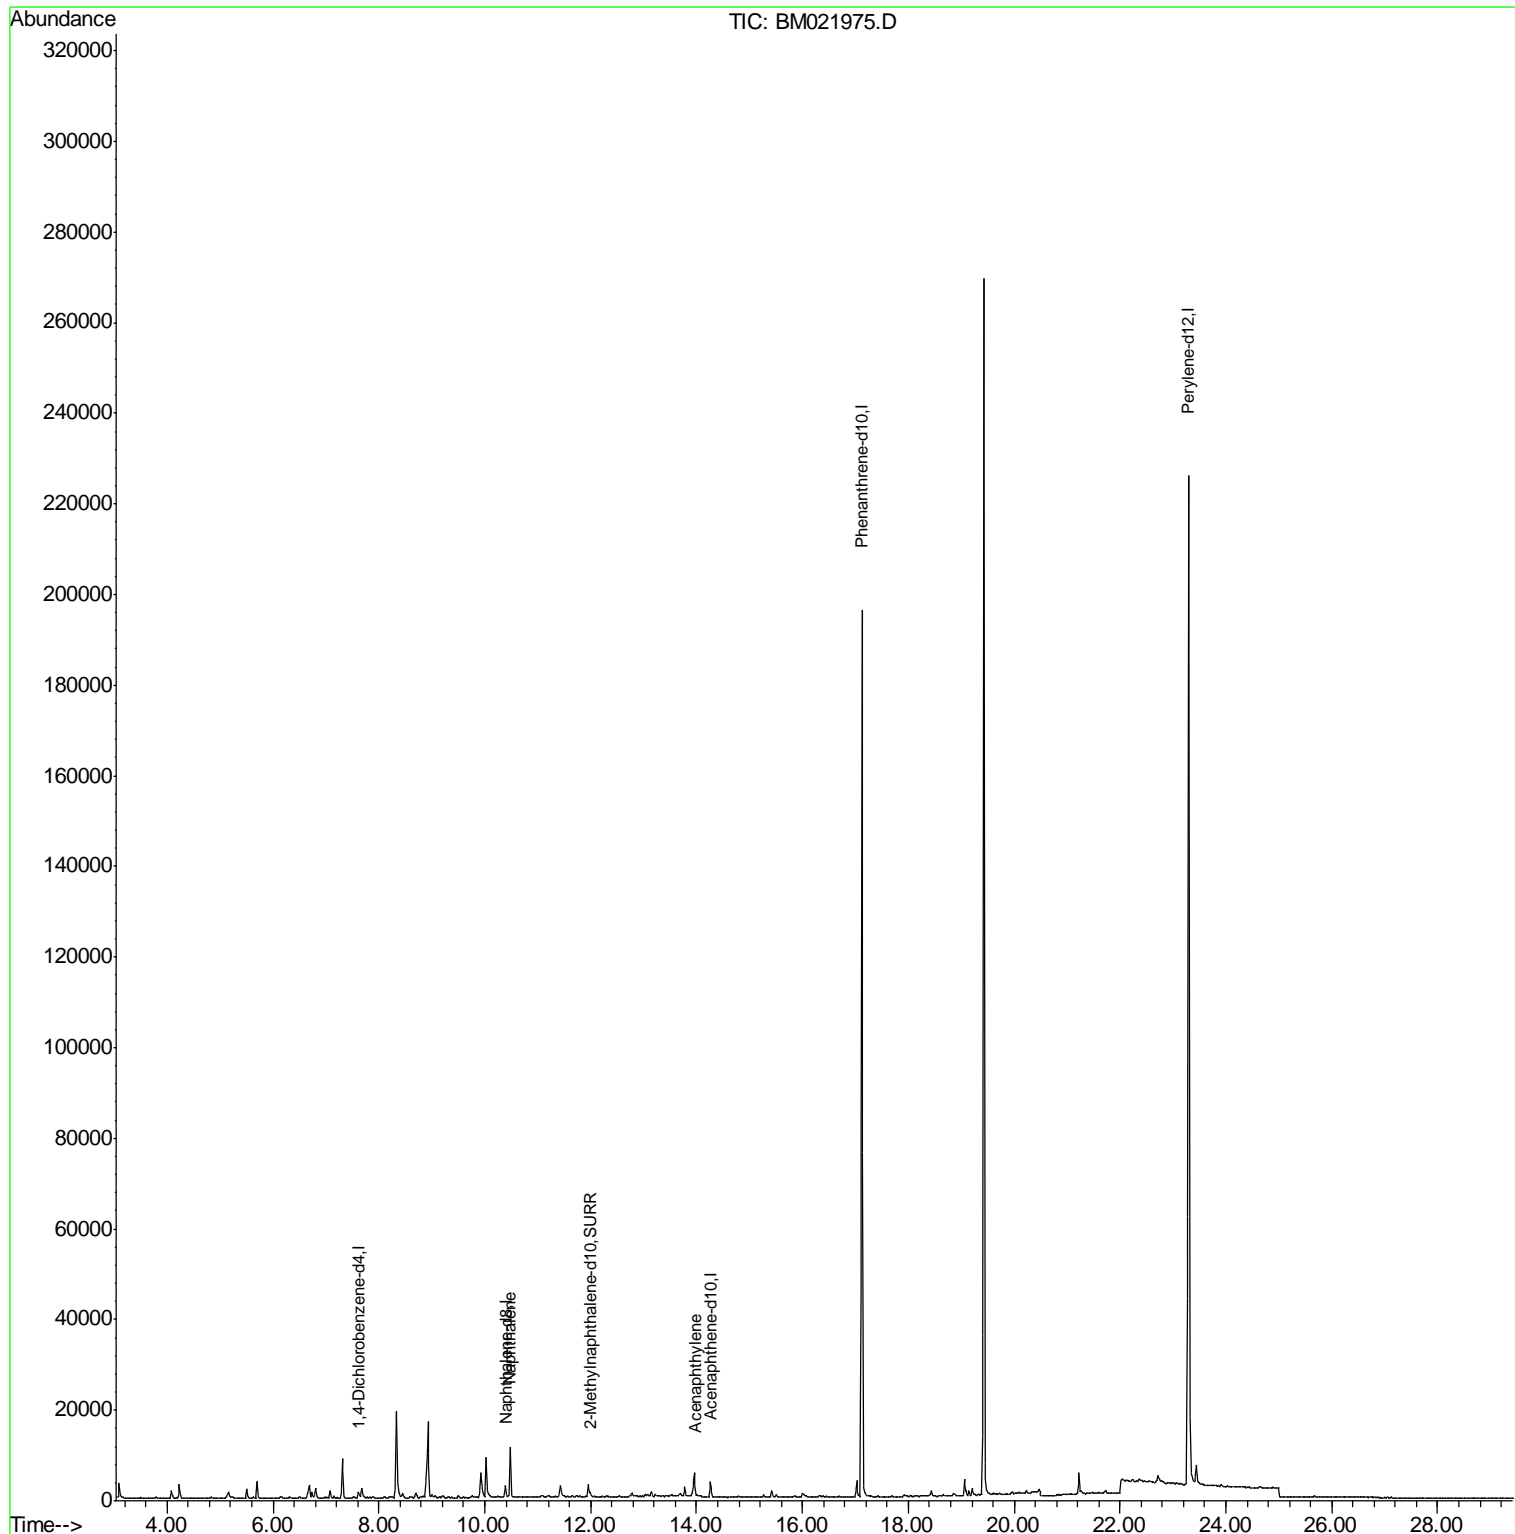


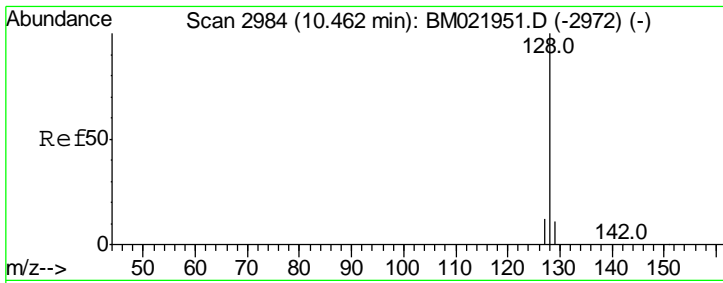

#3
 Naphthalene
 Concen: 0.110 ng/ul
 RT: 10.48 min Scan# 2989
 Delta R.T. 0.02 min
 Lab File: BM021975.D
 Acq: 09 Aug 2019 18:36

Instrument :
 BNA_M
 ClientSampled :

Tgt Ion	Resp	Lower	Upper
128	1065		
129	17.0	12.3	18.5
127	15.6	13.0	19.6

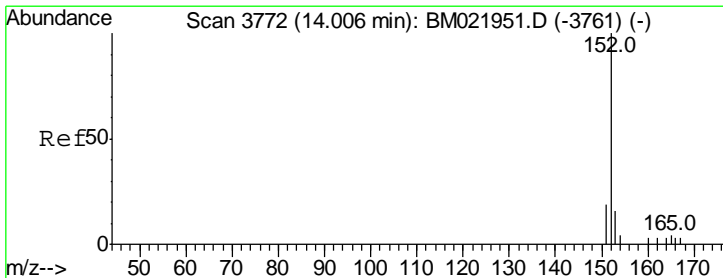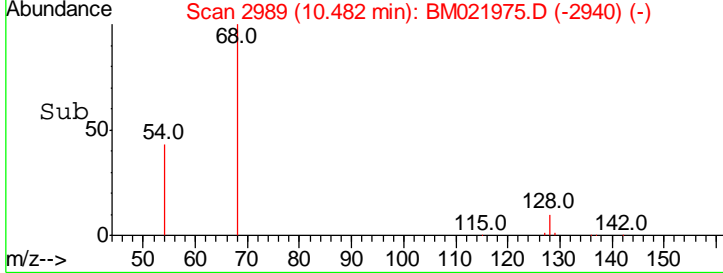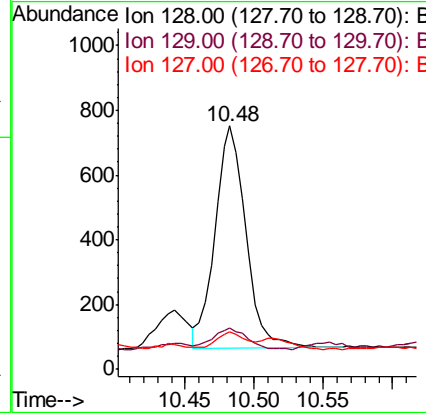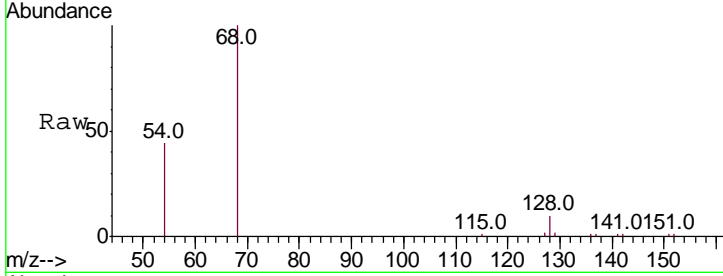

#7
 Acenaphthylene
 Concen: 0.023 ng/ul
 RT: 13.99 min Scan# 3769
 Delta R.T. -0.02 min
 Lab File: BM021975.D
 Acq: 09 Aug 2019 18:36

Tgt Ion	Resp	Lower	Upper
152	212		
151	57.1	18.3	27.5#
153	0.0	12.8	19.2#

