

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
 Data File : BM021981.D
 Acq On : 09 Aug 2019 22:17
 Operator : HP/JU
 Sample : PB121908BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 10 05:23:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 09 01:29:50 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	899	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.39	136	3858	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.27	164	2197	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.12	188	380264	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.30	264	456103	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.01	152	2206	0.35	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.27	166	746	0.080	ng/ul#	Ovalue 20




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
Data File : BM021981.D
Acq On : 09 Aug 2019 22:17
Operator : HP/JU
Sample : PB121908BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Aug 10 05:23:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration

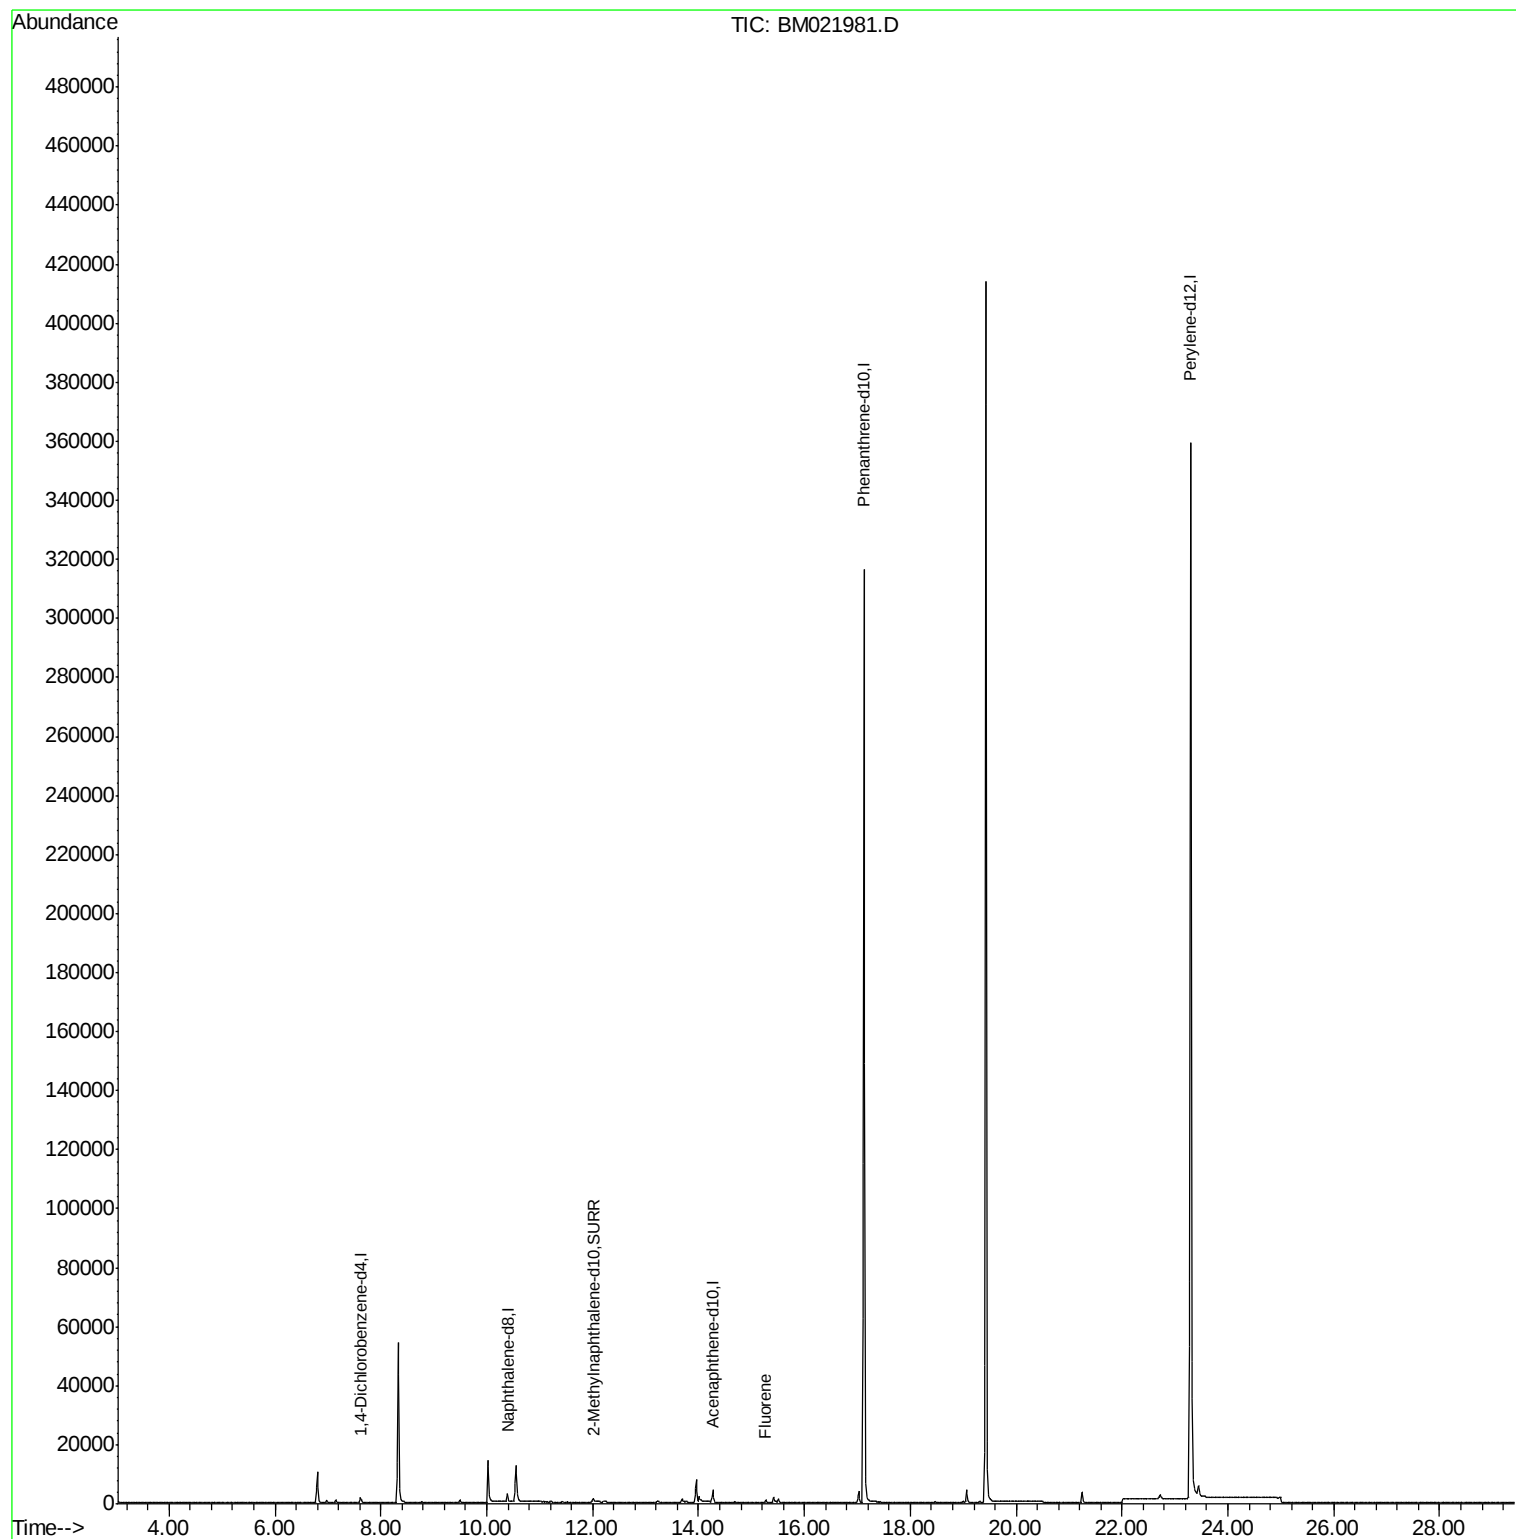

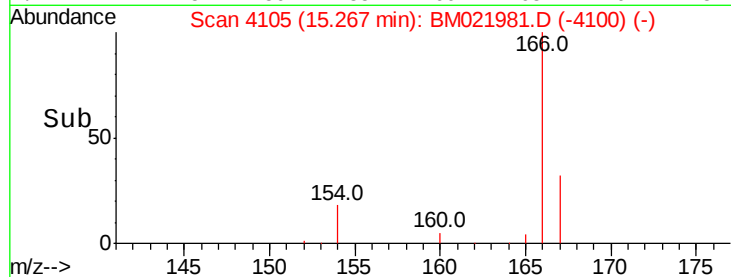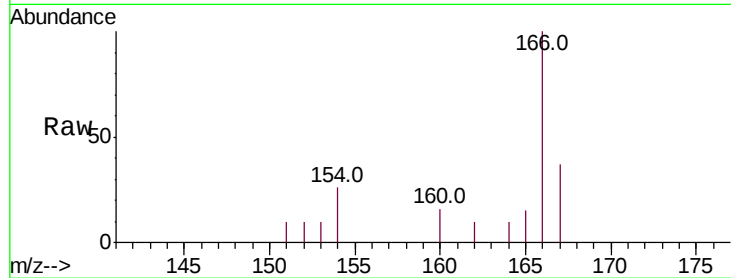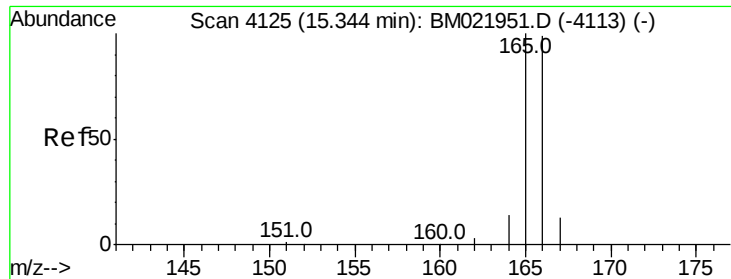

#9

Fluorene

Concen: 0.080 ng/ul

RT: 15.27 min Scan# 4105

Delta R.T. -0.08 min

Lab File: BM021981.D

Acq: 09 Aug 2019 22:17

Instrument :

BNA_M

ClientSampleId :

Tot Ion:166 Resp: 746

Ion Ratio Lower Upper

166 100

165 14.7 81.4 122.0#

167 36.9 13.7 20.5#

