


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
Data File : BM021989.D
Acq On : 10 Aug 2019 03:15
Operator : HP/JU
Sample : K4041-07
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENT1

Manual Integrations
APPROVED

Sohil
8/13/2019 8:45:57 AM

Quant Time: Aug 10 08:12:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration

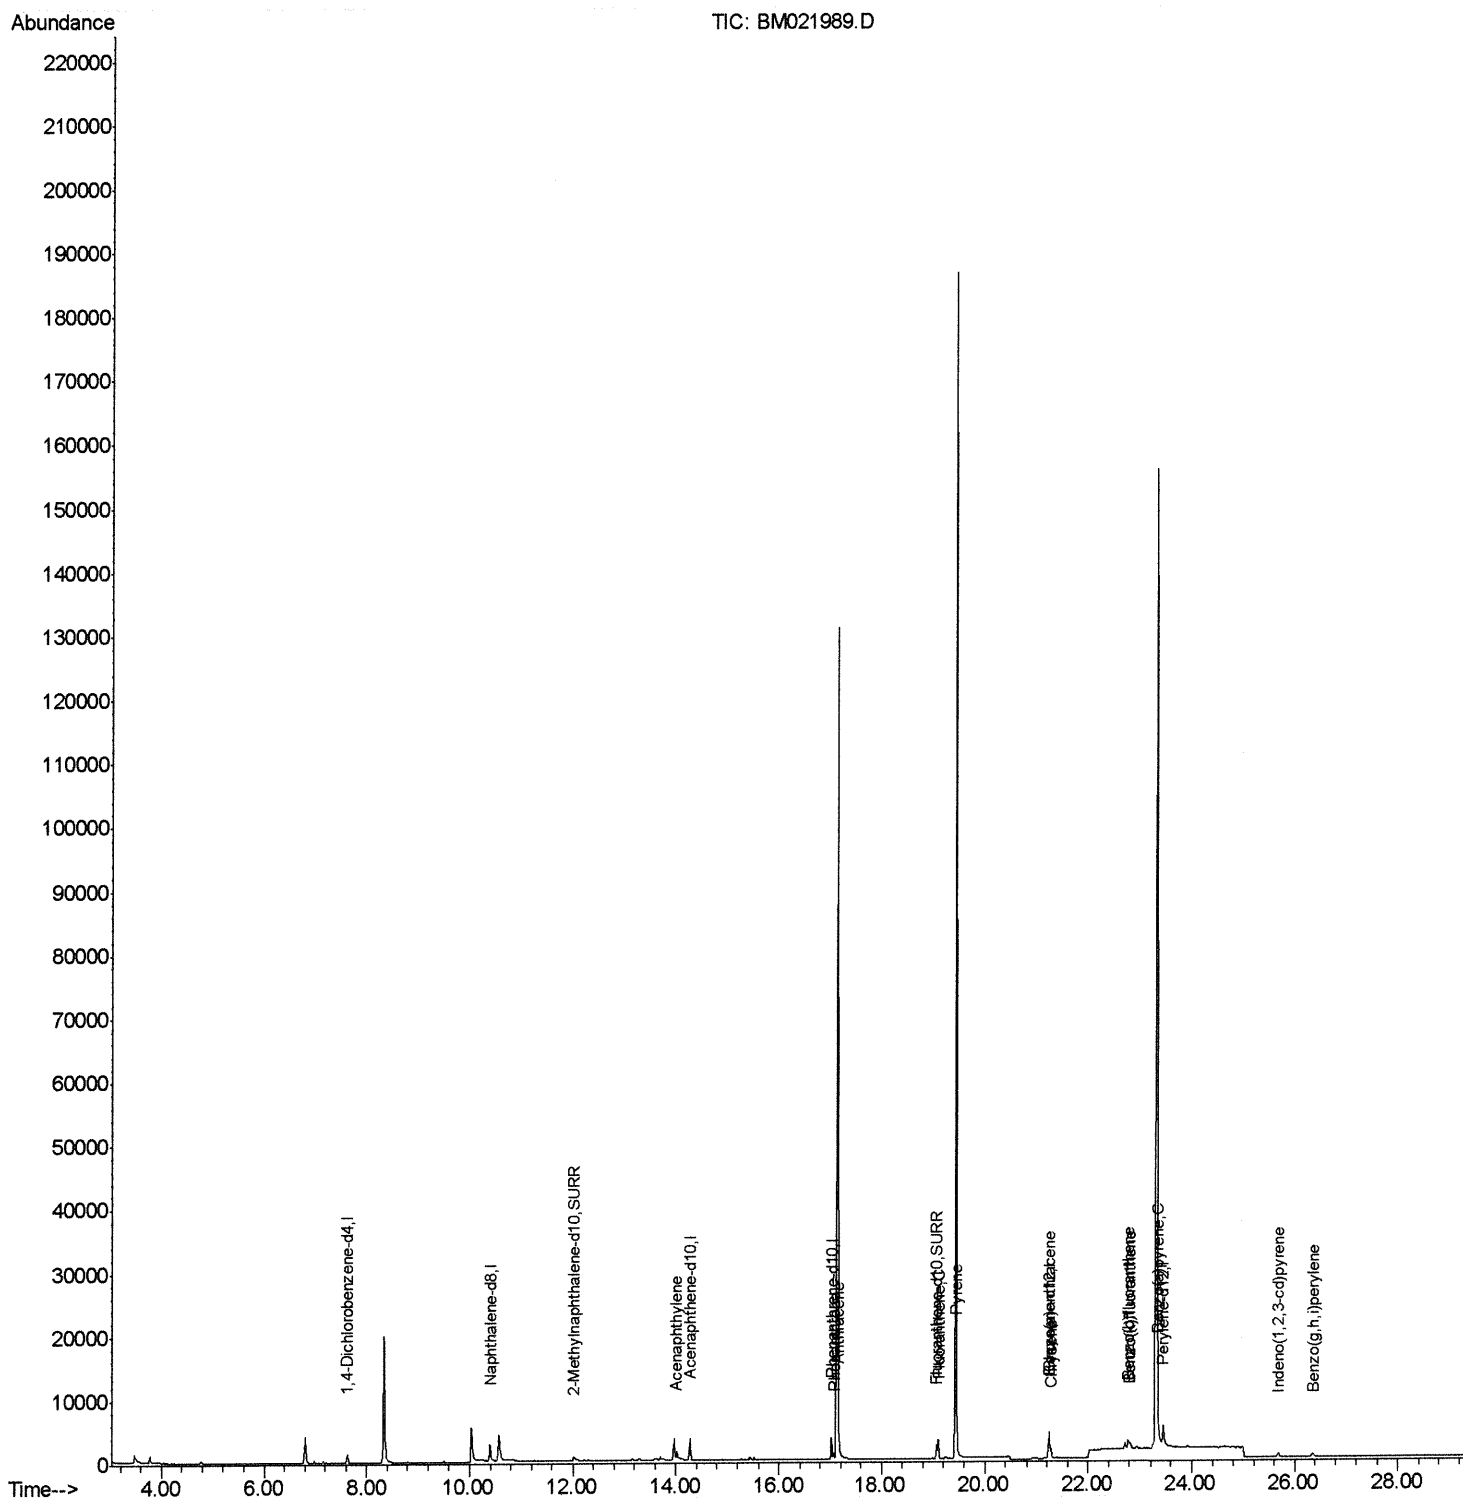

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
 Data File : BM021989.D
 Acq On : 10 Aug 2019 03:15
 Operator : HP/JU
 Sample : K4041-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 BENT1

Manual Integrations
APPROVED

Sohil
 8/13/2019 8:45:57 AM

Quant Time: Aug 10 05:24:35 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 09 01:29:50 2019
 Response via : Initial Calibration

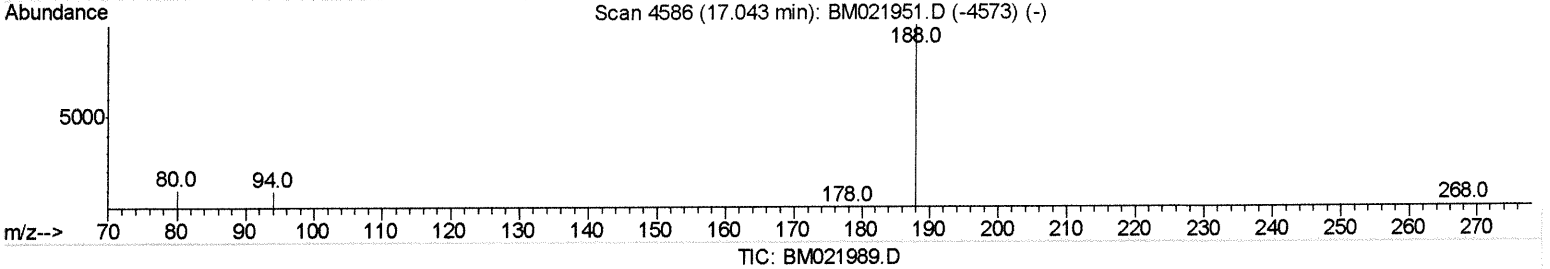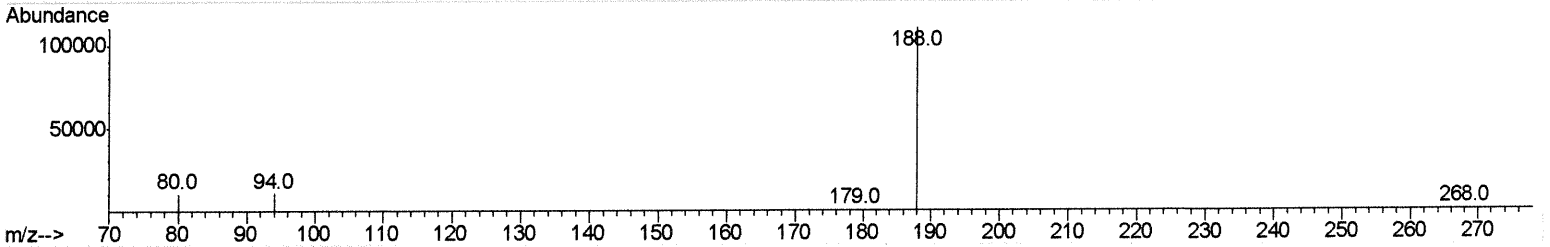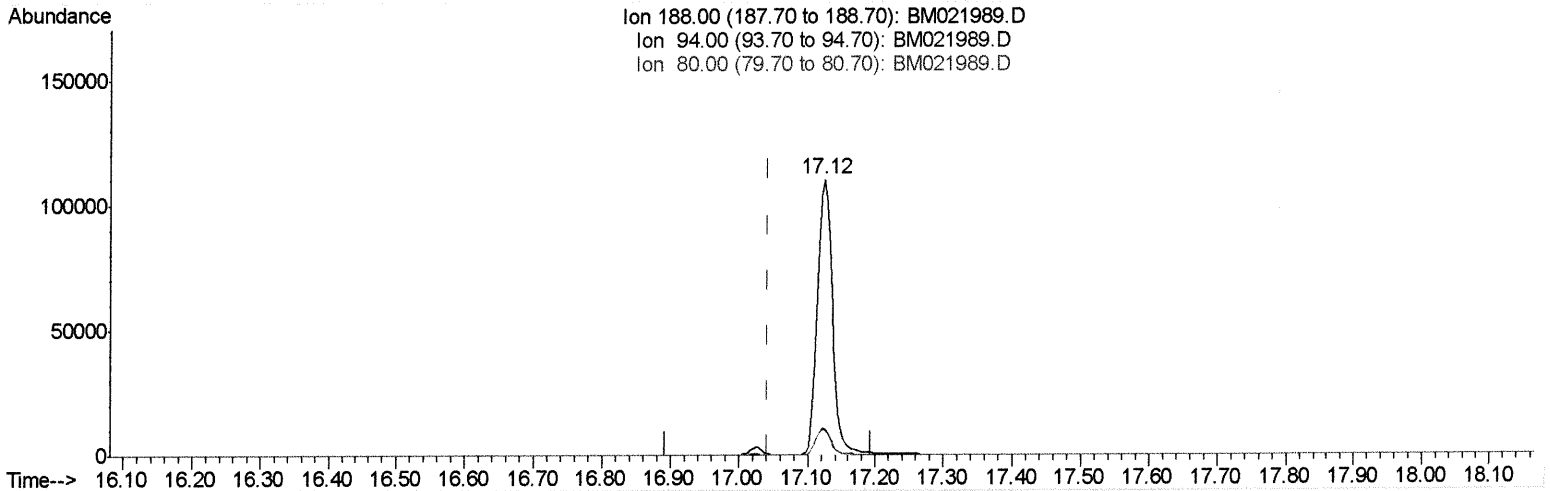

TIC: BM021989.D

(10) Phenanthrene-d10 (I)

17.124min (+0.080) 0.40ng/ul

response 164065

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	9.55
80.00	11.40	9.03#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
 Data File : BM021989.D
 Acq On : 10 Aug 2019 03:15
 Operator : HP/JU
 Sample : K4041-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENT1

Manual Integrations
 APPROVED

Sohil
 8/13/2019 8:45:57 AM

Quant Time: Aug 10 05:24:35 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 09 01:29:50 2019
 Response via : Initial Calibration

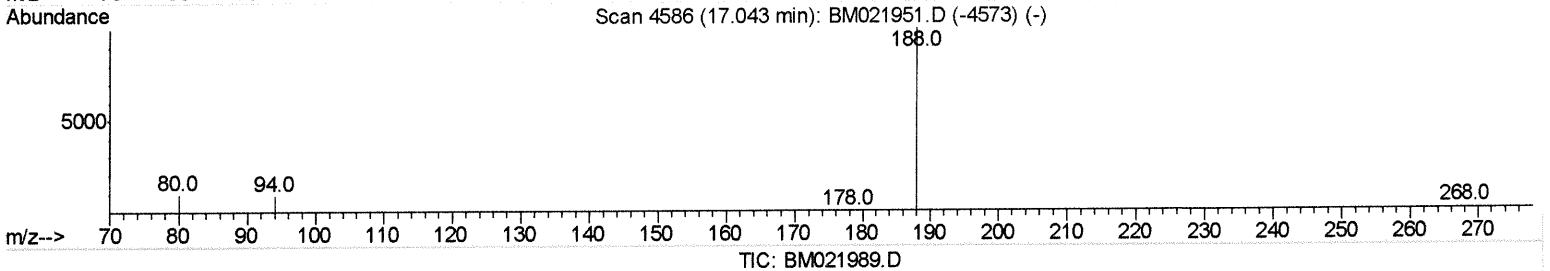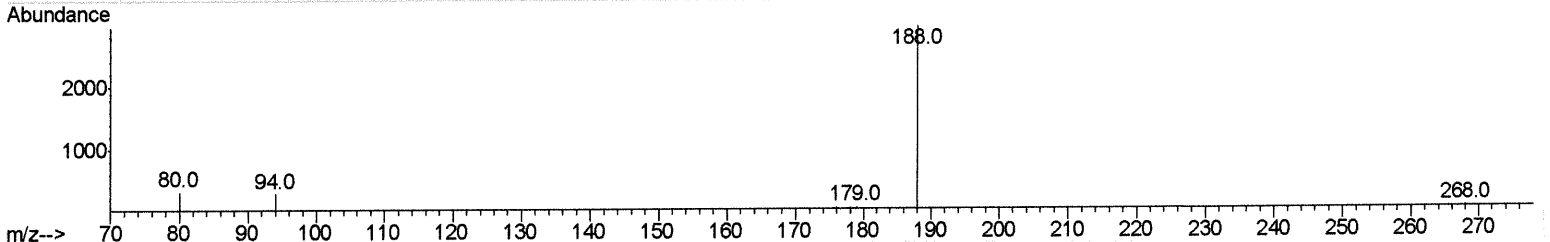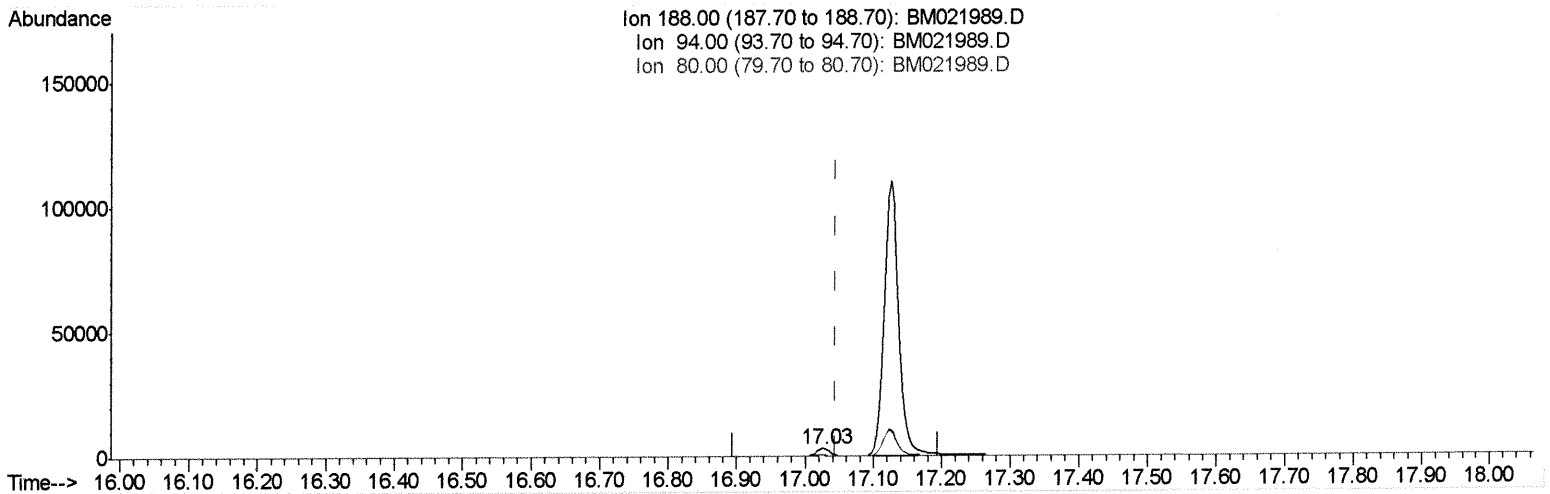

(10) Phenanthrene-d10 (I)

17.027min (-0.017) 0.40ng/ul m *JU 08/12/19*

response 4069

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	10.10
80.00	11.40	11.18
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
Data File : BM021989.D
Acq On : 10 Aug 2019 03:15
Operator : HP/JU
Sample : K4041-07
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENT1

Manual Integrations
APPROVED

Sohil
8/13/2019 8:45:57 AM

Quant Time: Aug 10 08:08:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration

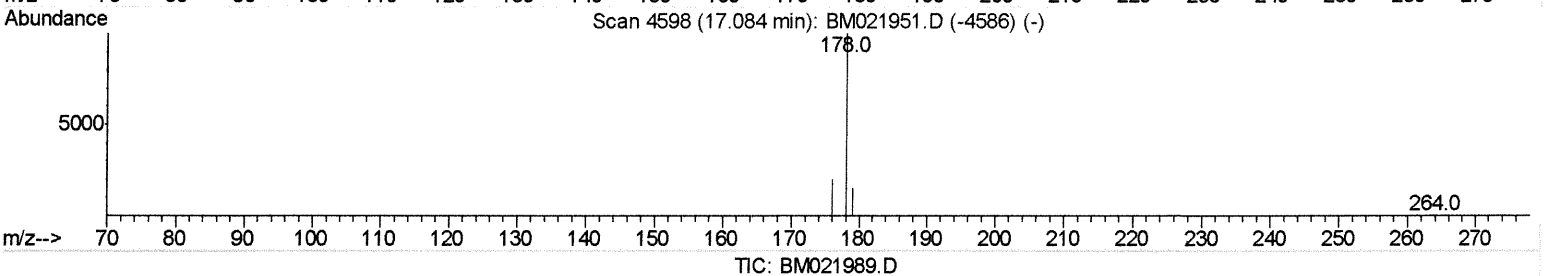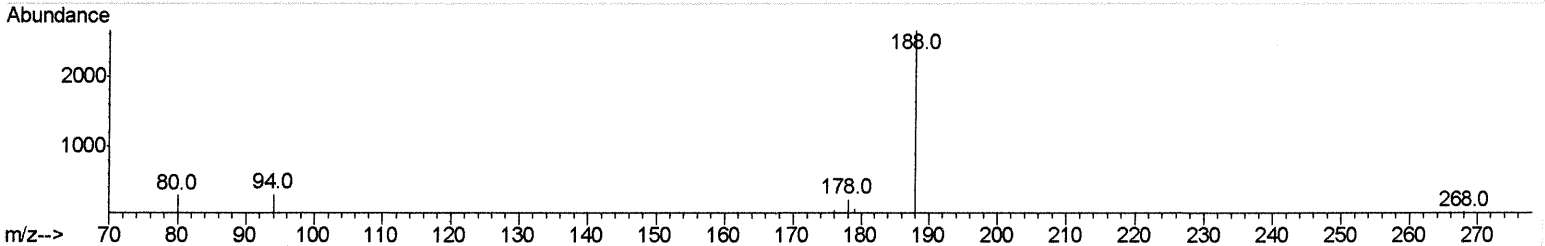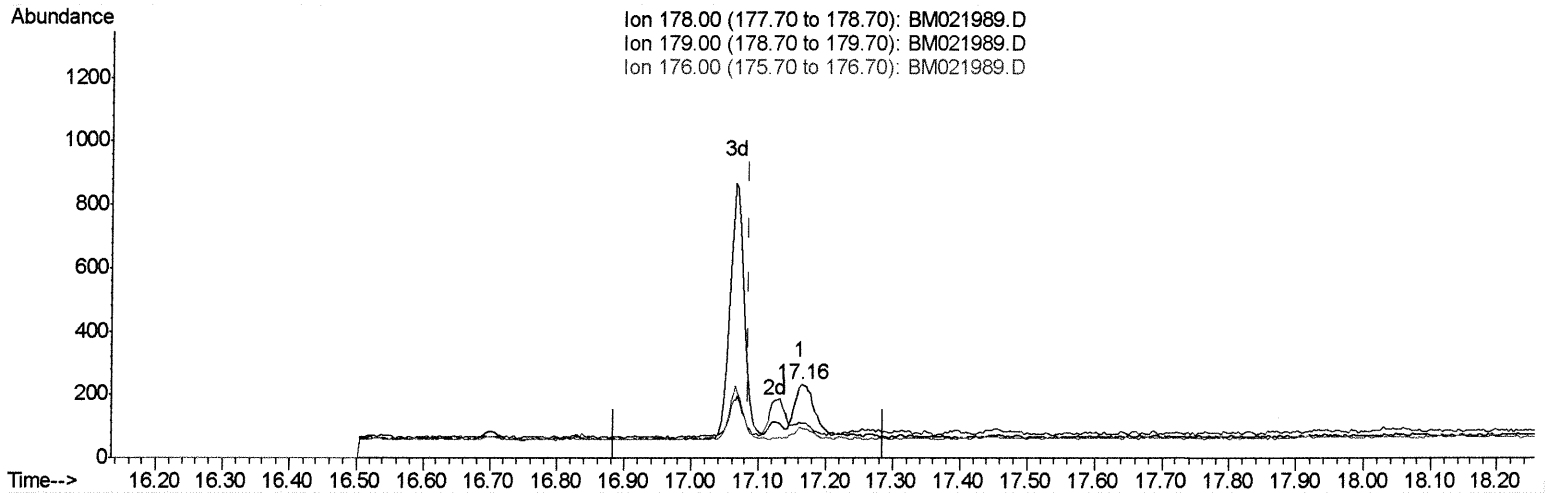

(12) Phenanthrene

17.162min (+0.077) 0.03ng/ul

response 362

Ion	Exp%	Act%
178.00	100	100
179.00	17.70	46.98#
176.00	21.00	40.09#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
 Data File : BM021989.D
 Acq On : 10 Aug 2019 03:15
 Operator : HP/JU
 Sample : K4041-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENT1

Manual Integrations
 APPROVED

Sohil
 8/13/2019 8:45:57 AM

Quant Time: Aug 10 08:08:45 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 09 01:29:50 2019
 Response via : Initial Calibration

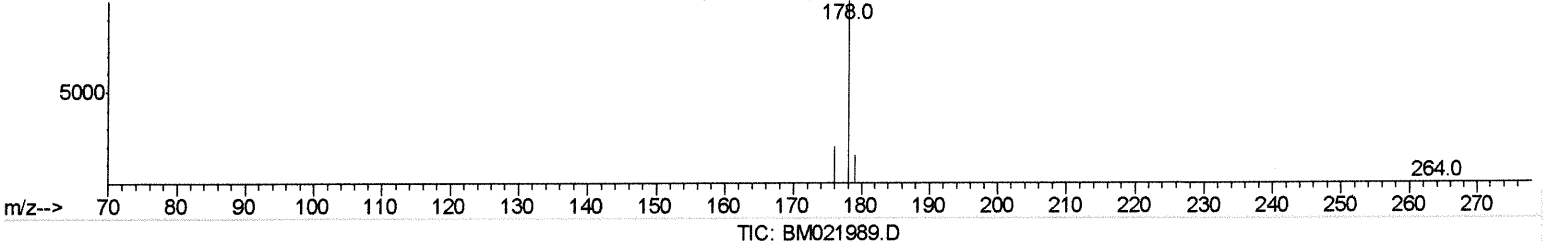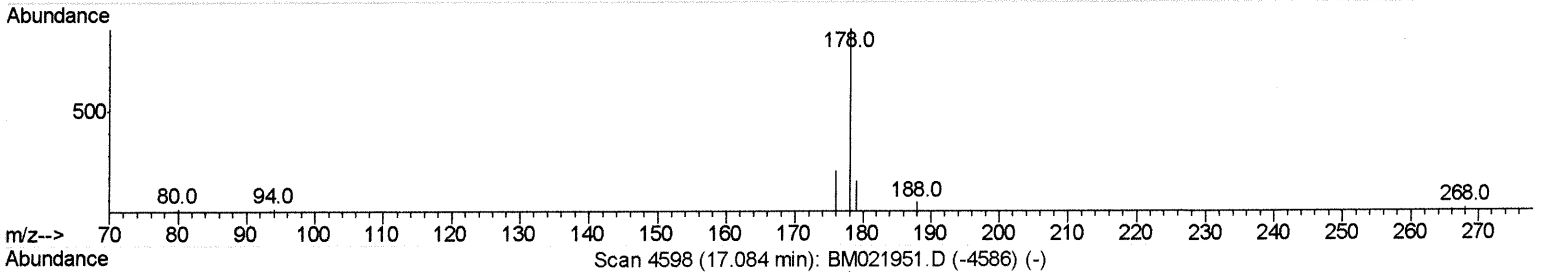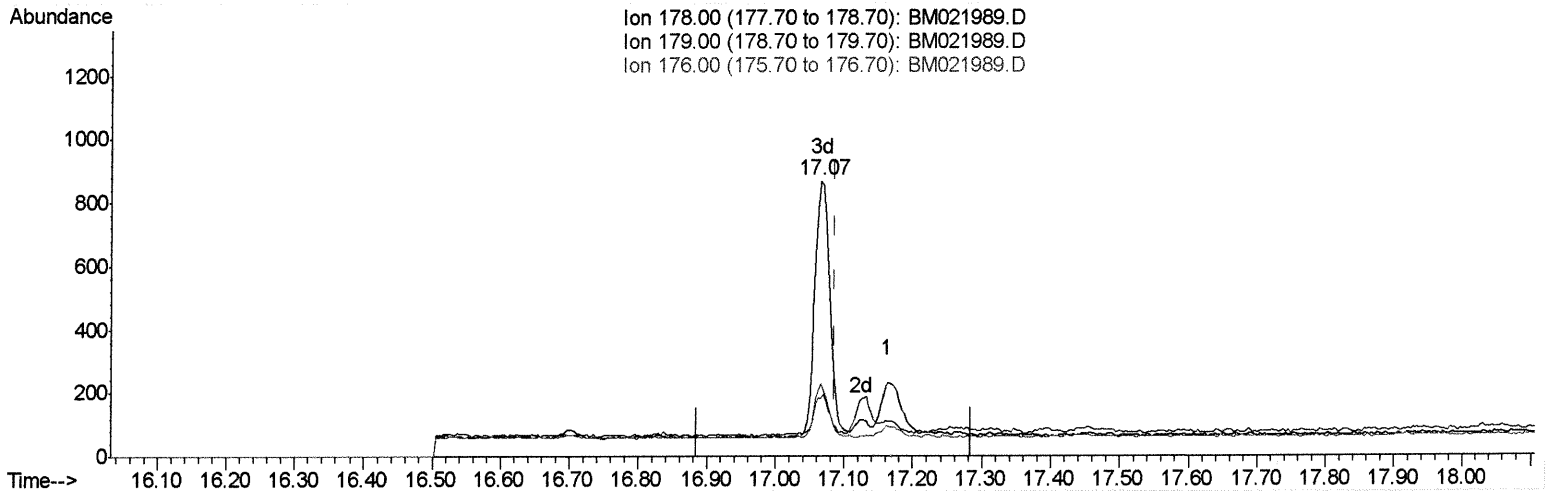

(12) Phenanthrene

17.065min (-0.021) 0.10ng/ul m *JU 08/12/19*

response 1212

Ion	Exp%	Act%
178.00	100	100
179.00	17.70	20.85
176.00	21.00	26.15#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
 Data File : BM021989.D
 Acq On : 10 Aug 2019 03:15
 Operator : HP/JU
 Sample : K4041-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENT1

Manual Integrations
 APPROVED

Sohil
 8/13/2019 8:45:57 AM

Quant Time: Aug 10 08:09:12 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 09 01:29:50 2019
 Response via : Initial Calibration

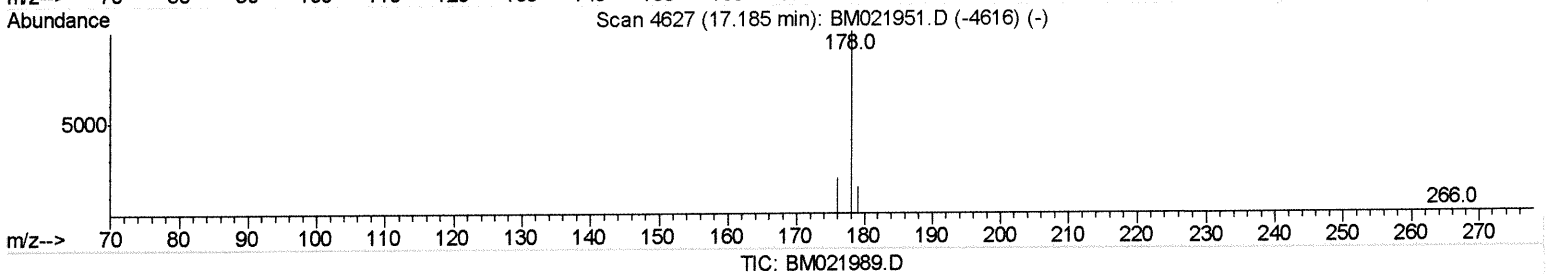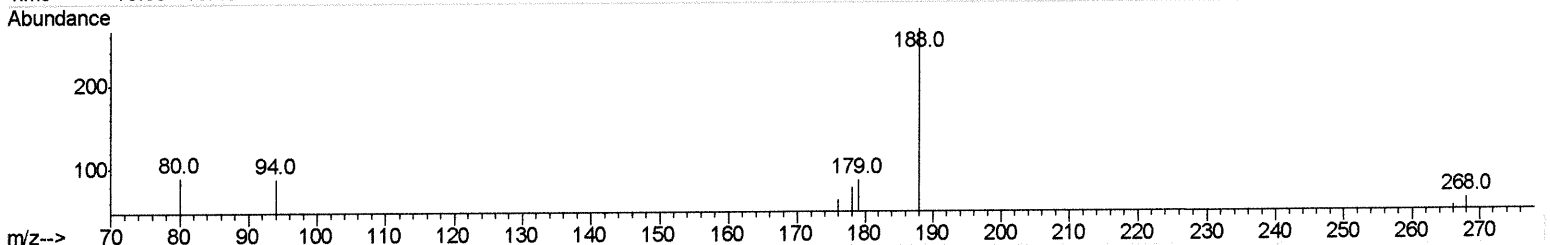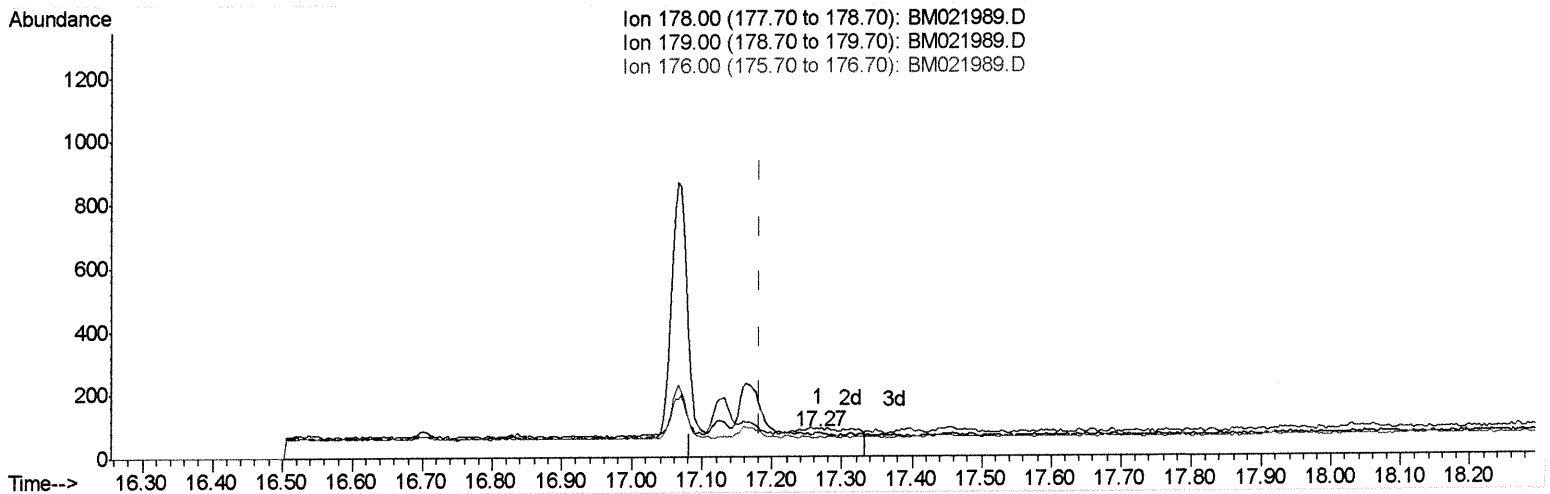

(13) Anthracene

17.267min (+0.084) 0.00ng/ul

response 14

Ion	Exp%	Act%
178.00	100	100
179.00	19.40	111.69#
176.00	20.80	80.52#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
 Data File : BM021989.D
 Acq On : 10 Aug 2019 03:15
 Operator : HP/JU
 Sample : K4041-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENT1

Manual Integrations
 APPROVED

Sohil
 8/13/2019 8:45:57 AM

Quant Time: Aug 10 08:09:12 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 09 01:29:50 2019
 Response via : Initial Calibration

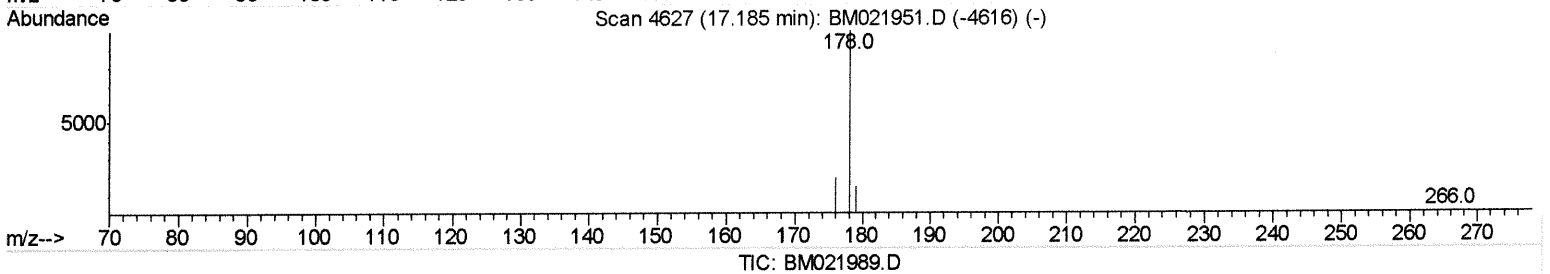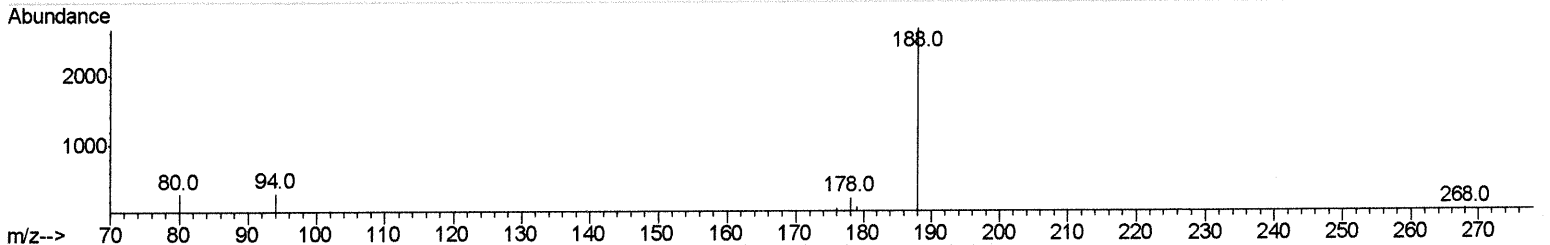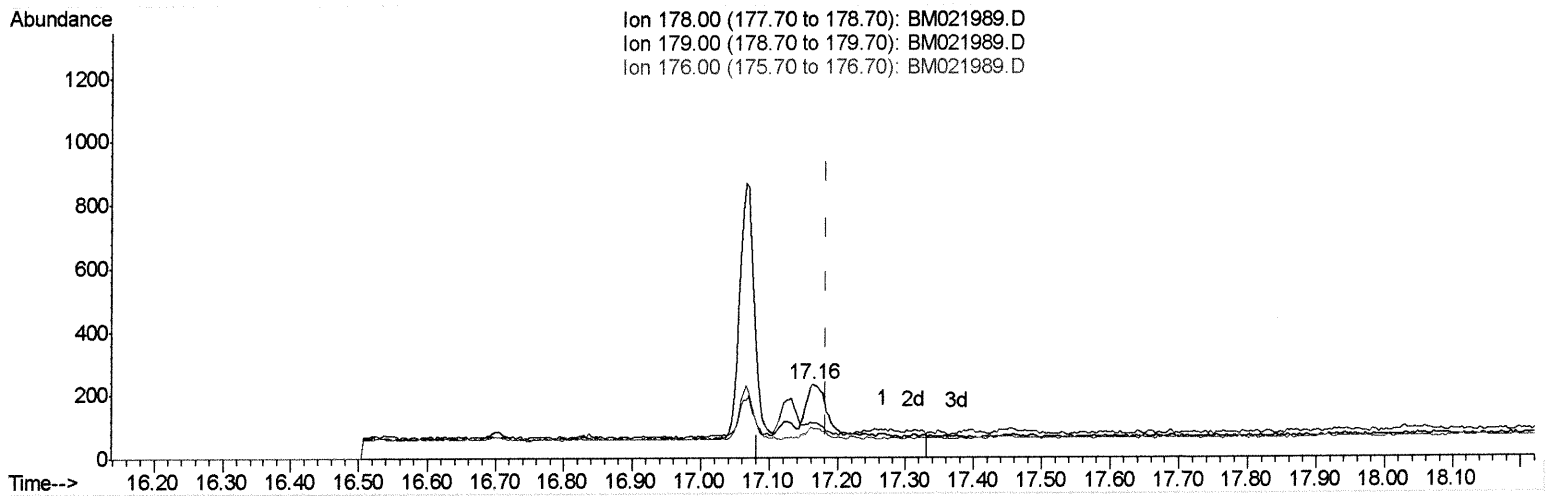

(13) Anthracene

17.162min (-0.021) 0.03ng/ul m *JU 08/12/19*

response 324

Ion	Exp%	Act%
178.00	100	100
179.00	19.40	46.98#
176.00	20.80	40.09#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
 Data File : BM021989.D
 Acq On : 10 Aug 2019 03:15
 Operator : HP/JU
 Sample : K4041-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 BENT1

Manual Integrations
APPROVED

Sohil
 8/13/2019 8:45:57 AM

Quant Time: Aug 10 08:09:12 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 09 01:29:50 2019
 Response via : Initial Calibration

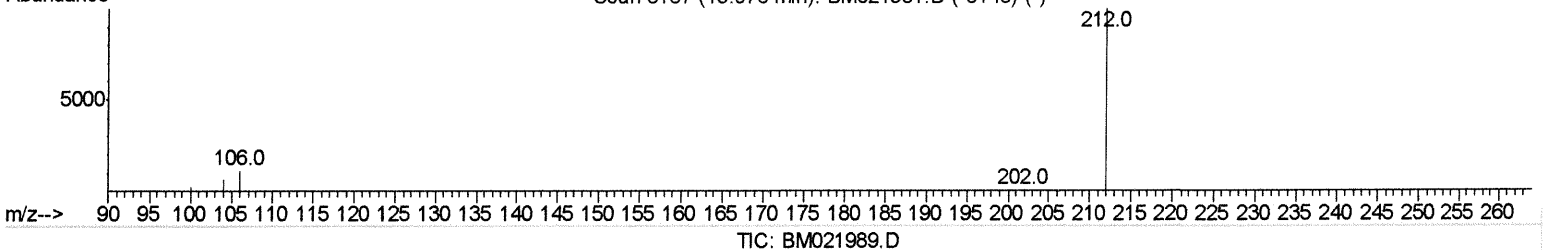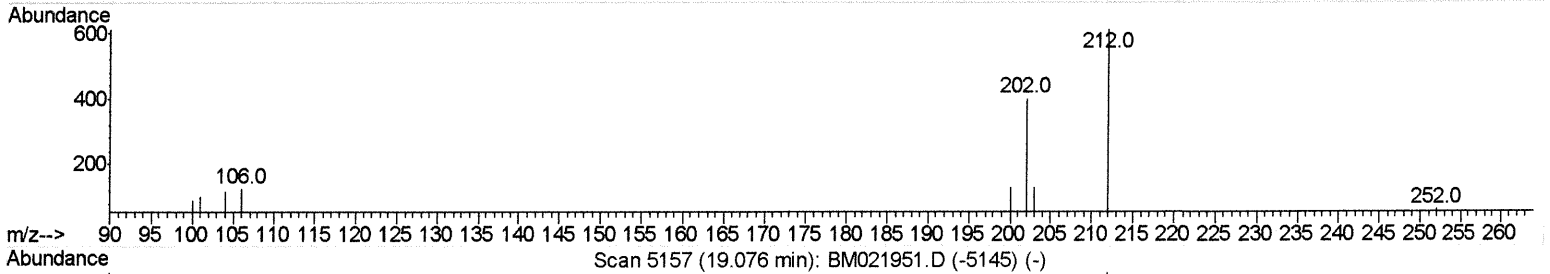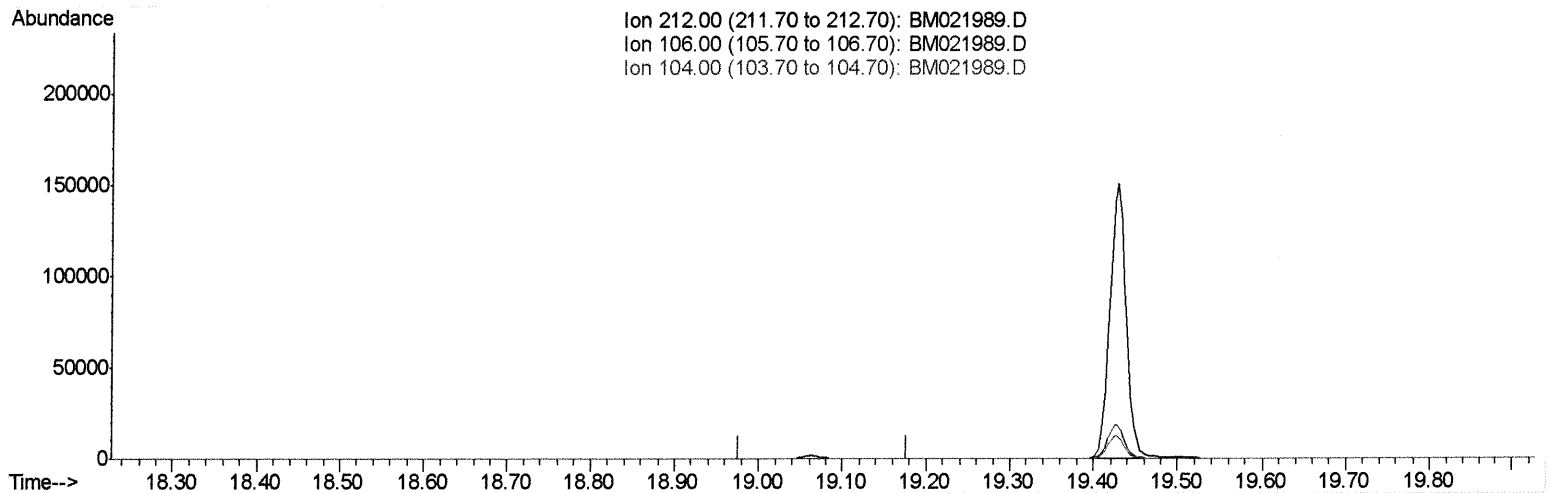

(14) Fluoranthene-d10 (SURR)

19.077min (-19.077) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	9.90	0.00#
104.00	6.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
 Data File : BM021989.D
 Acq On : 10 Aug 2019 03:15
 Operator : HP/JU
 Sample : K4041-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENT1

Manual Integrations
 APPROVED

Sohil
 8/13/2019 8:45:57 AM

Quant Time: Aug 10 08:09:12 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 09 01:29:50 2019
 Response via : Initial Calibration

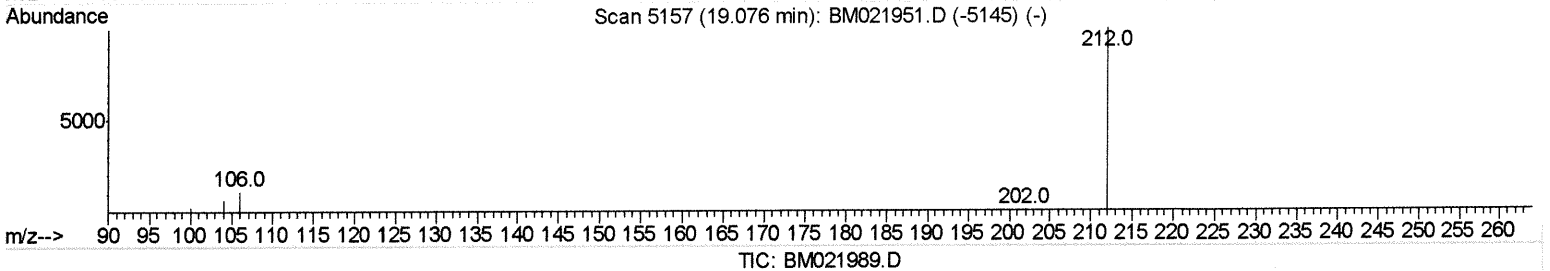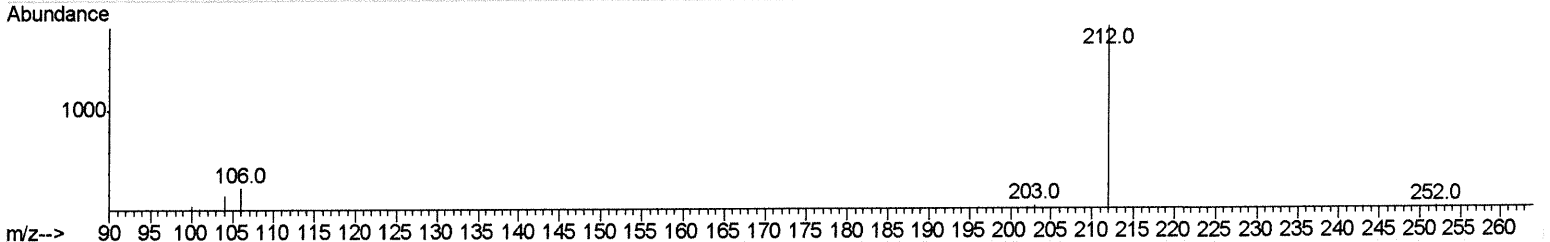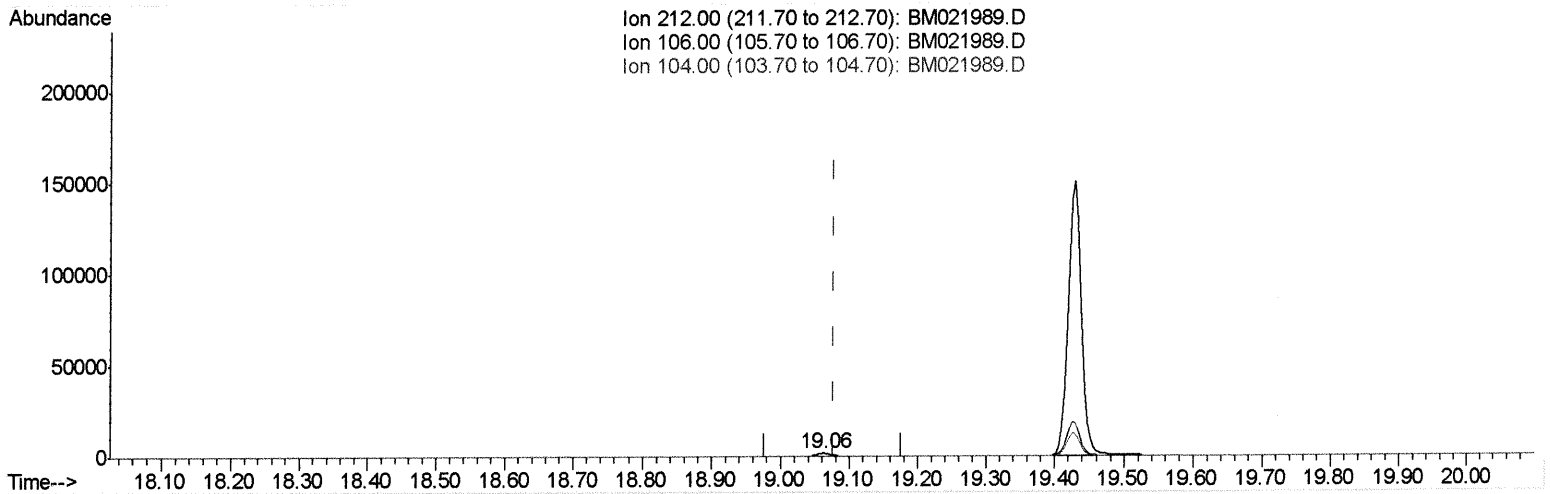

(14) Fluoranthene-d10 (SURR)

19.062min (-0.015) 0.18ng/ul m

JU
08/12/19

response 2503

Ion	Exp%	Act%
212.00	100	100
106.00	9.90	0.00#
104.00	6.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
 Data File : BM021989.D
 Acq On : 10 Aug 2019 03:15
 Operator : HP/JU
 Sample : K4041-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENT1

Manual Integrations
 APPROVED

Sohil
 8/13/2019 8:45:57 AM

Quant Time: Aug 10 08:09:12 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 09 01:29:50 2019
 Response via : Initial Calibration

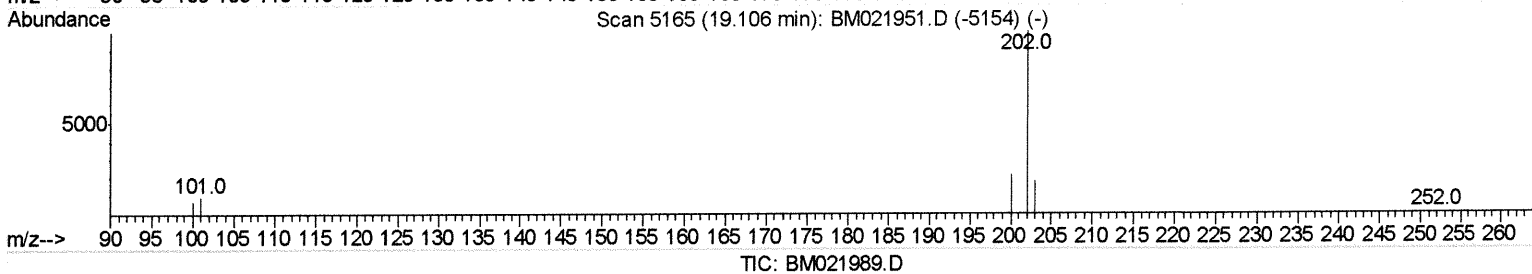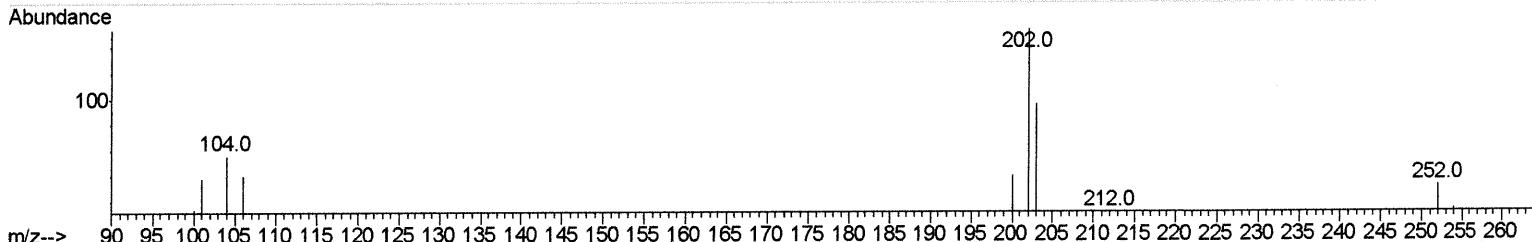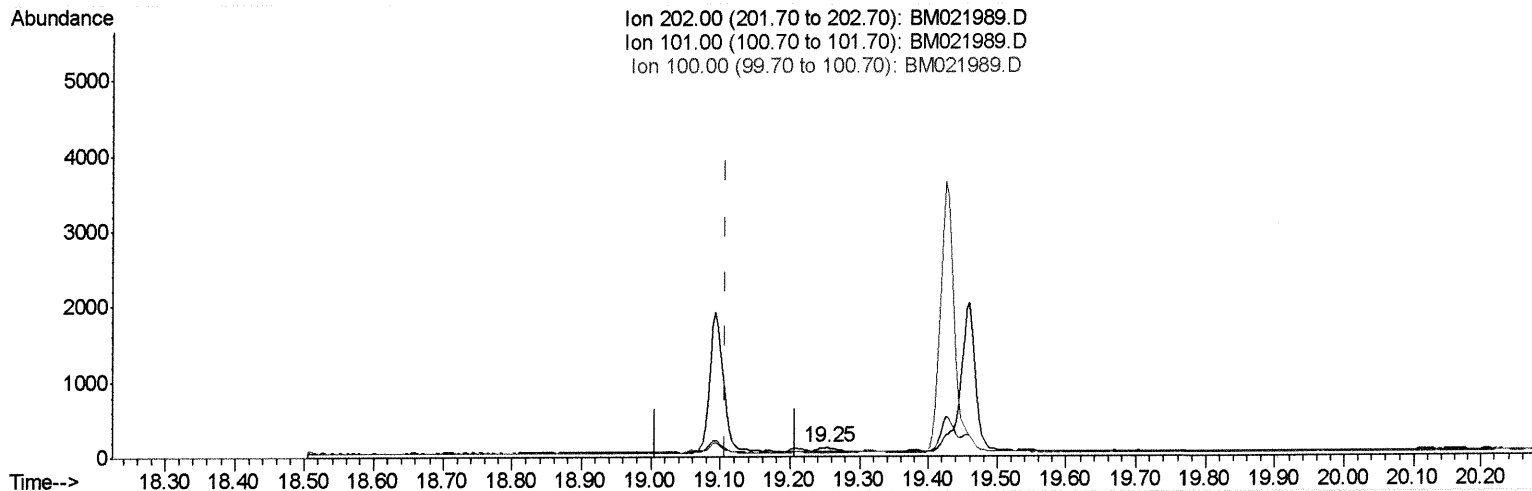

(15) Fluoranthene (C)

19.253min (+0.145) 0.00ng/ul

response 79

Ion	Exp%	Act%
202.00	100	100
101.00	10.20	54.33#
100.00	8.10	44.88#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
Data File : BM021989.D
Acq On : 10 Aug 2019 03:15
Operator : HP/JU
Sample : K4041-07
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENT1

Manual Integrations
APPROVED

Sohil
8/13/2019 8:45:57 AM

Quant Time: Aug 10 08:09:12 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration

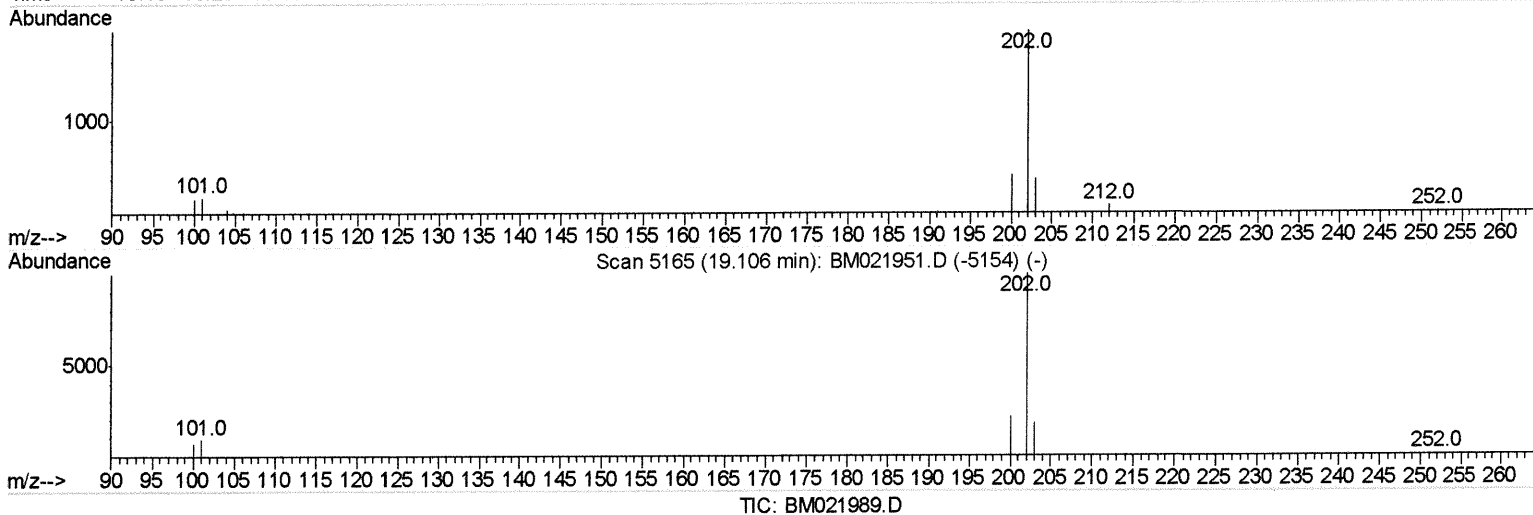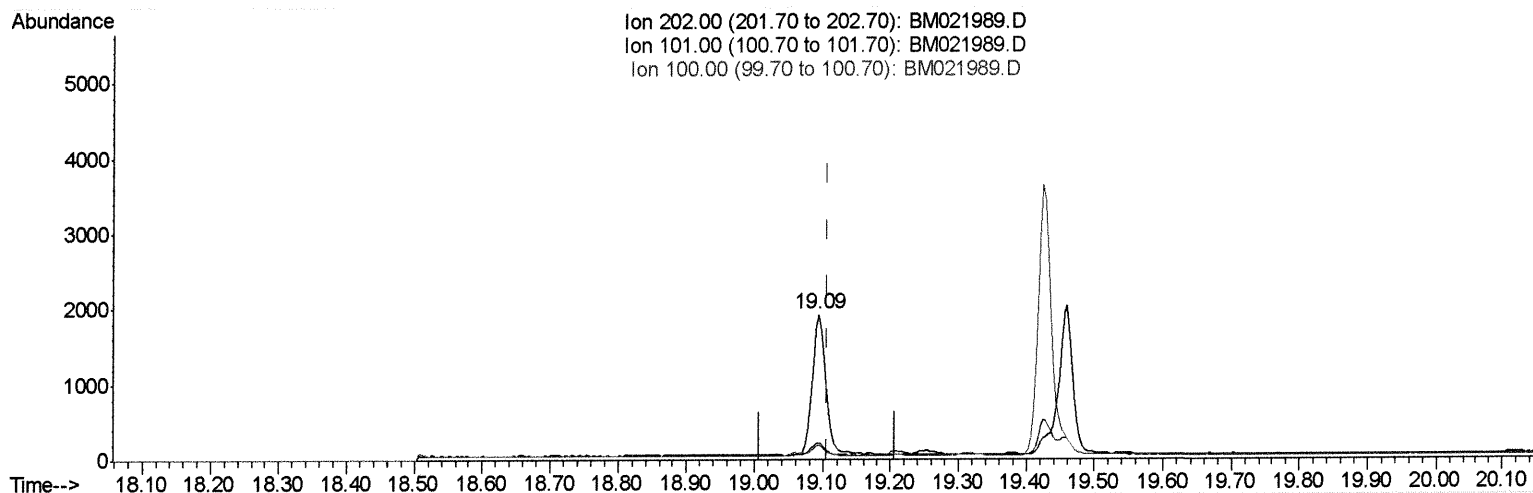

(15) Fluoranthene (C)

19.093min (-0.015) 0.16ng/ul m

JU
08/12/19

response 2602

Ion	Exp%	Act%
202.00	100	100
101.00	10.20	11.23
100.00	8.10	10.19
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
 Data File : BM021989.D
 Acq On : 10 Aug 2019 03:15
 Operator : HP/JU
 Sample : K4041-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 BENT1

Manual Integrations
APPROVED

Sohil
 8/13/2019 8:45:57 AM

Quant Time: Aug 10 08:09:12 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 09 01:29:50 2019
 Response via : Initial Calibration

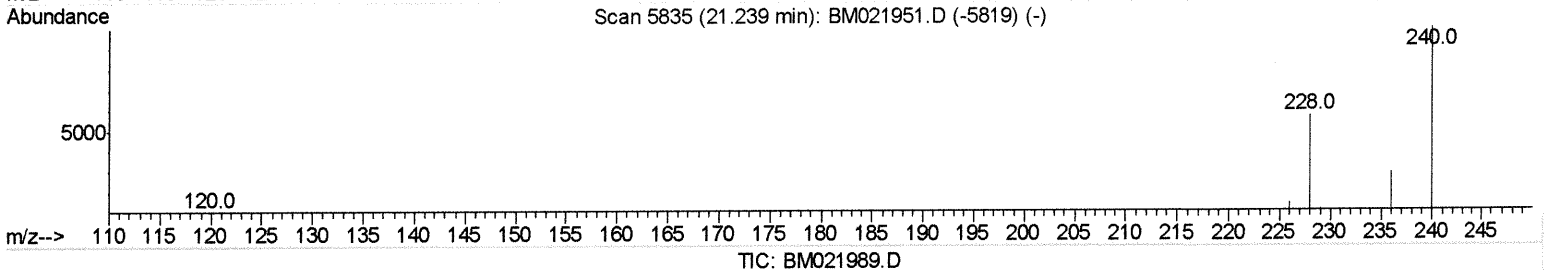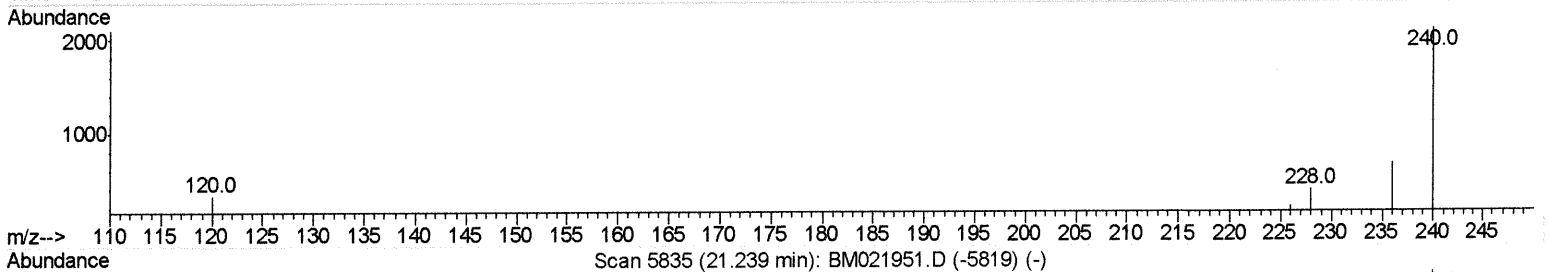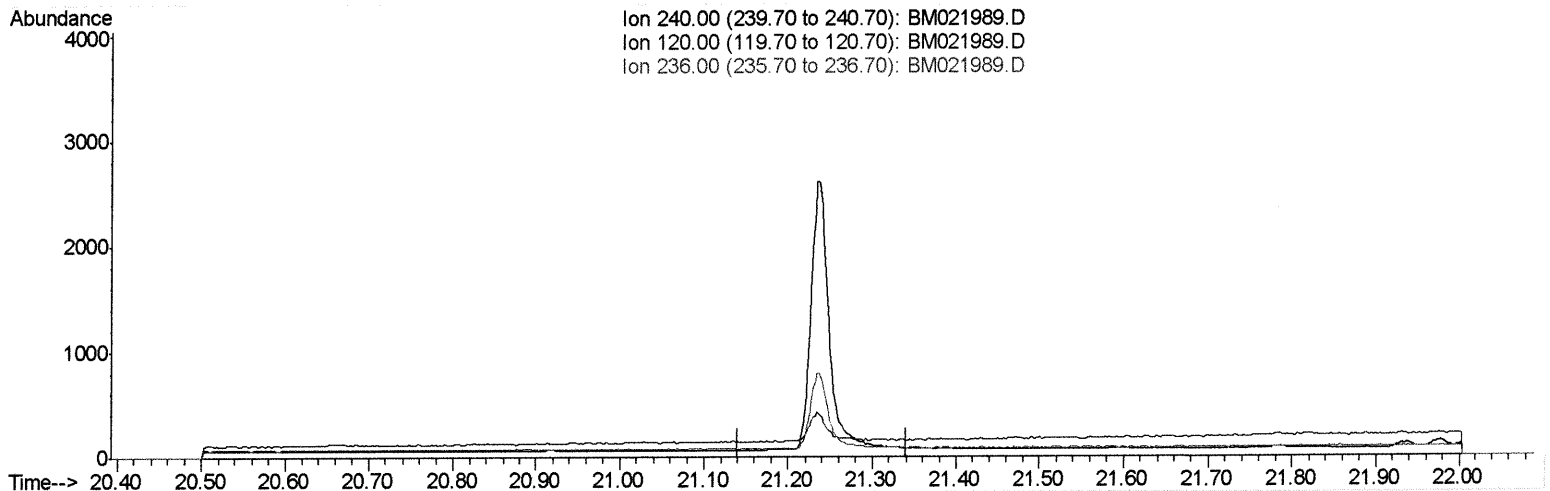

(16) Chrysene-d12 (I)
 21.241min (-21.241) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.20	0.00#
236.00	32.30	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
 Data File : BM021989.D
 Acq On : 10 Aug 2019 03:15
 Operator : HP/JU
 Sample : K4041-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENT1

Manual Integrations
 APPROVED

Sohil
 8/13/2019 8:45:57 AM

Quant Time: Aug 10 08:09:12 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 09 01:29:50 2019
 Response via : Initial Calibration

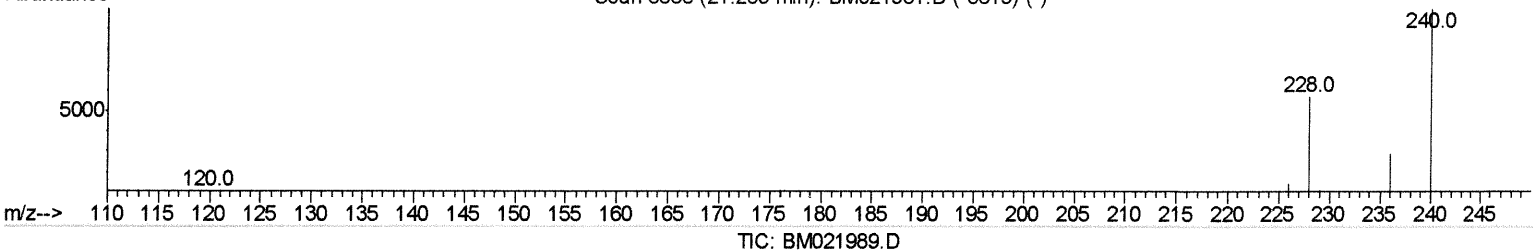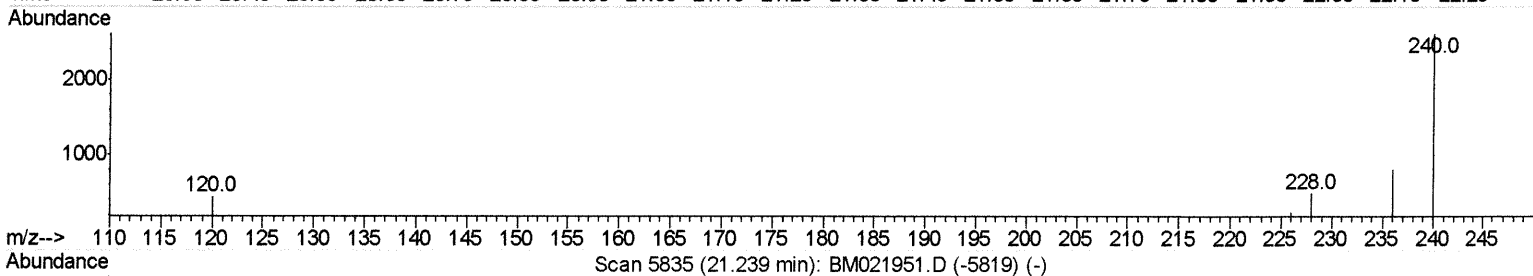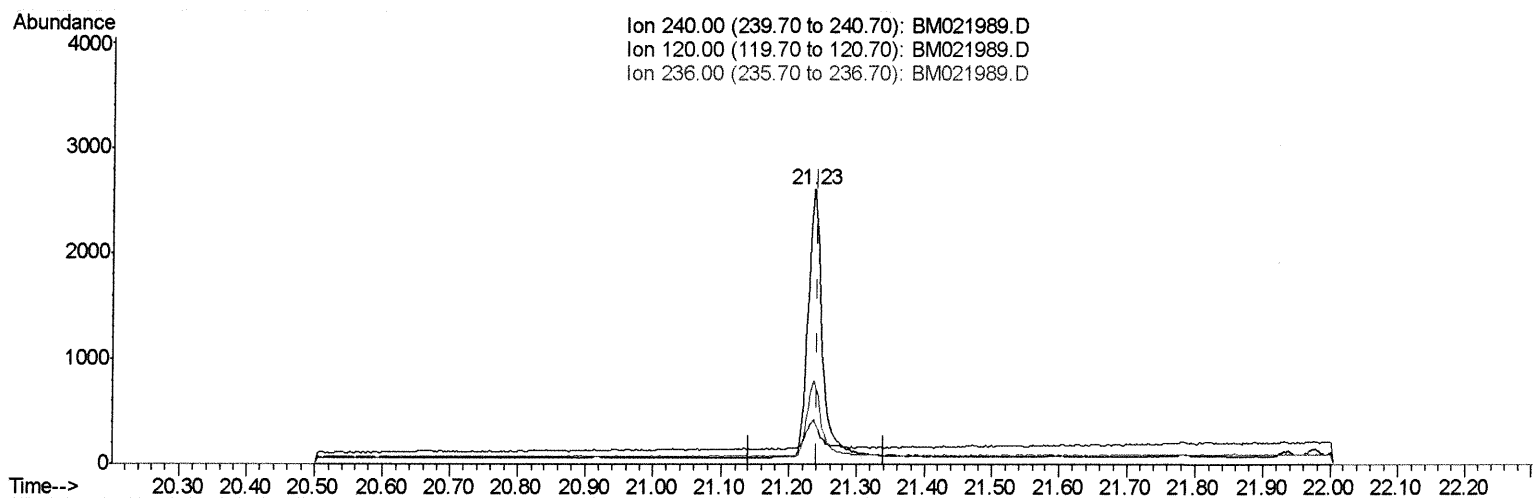

(16) Chrysene-d12 (I)

21.234min (-0.007) 0.40ng/ul m *JU* 08/12/19

response 3812

Ion	Exp%	Act%
240.00	100	100
120.00	16.20	16.48
236.00	32.30	30.47
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
 Data File : BM021989.D
 Acq On : 10 Aug 2019 03:15
 Operator : HP/JU
 Sample : K4041-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENT1

Manual Integrations
 APPROVED

Sohil
 8/13/2019 8:45:57 AM

Quant Time: Aug 10 08:10:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 09 01:29:50 2019
 Response via : Initial Calibration

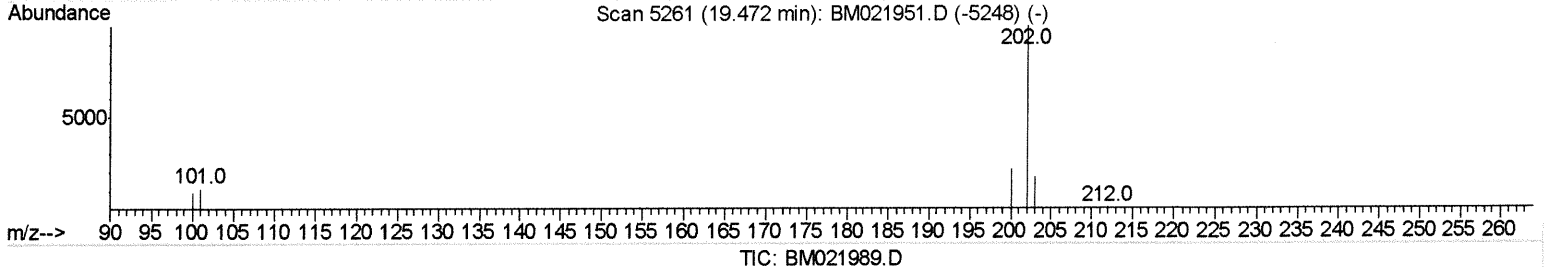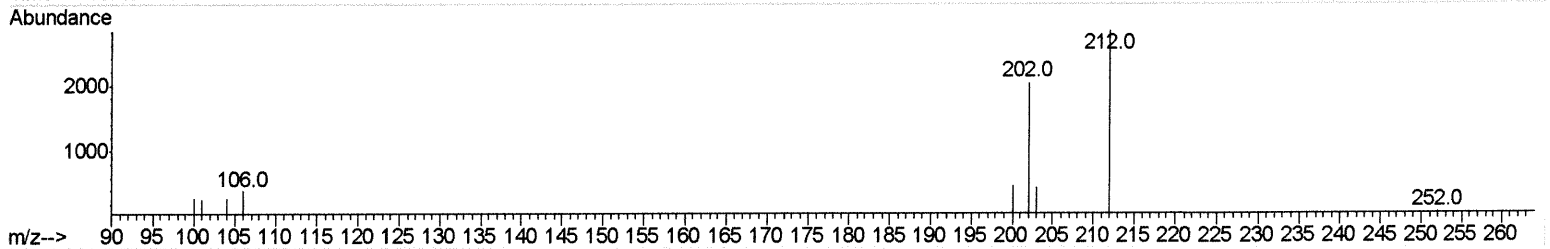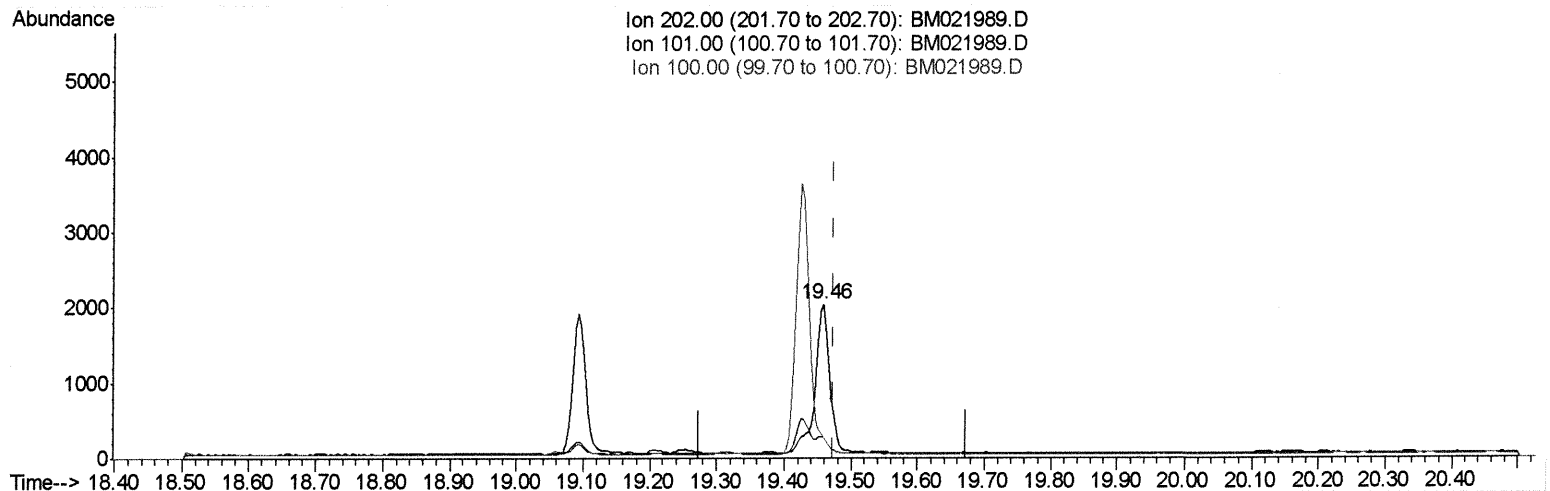

(17) Pyrene

19.459min (-0.015) 0.19ng/ul

response 3043

Ion	Exp%	Act%
202.00	100	100
101.00	10.40	13.49#
100.00	9.00	13.84#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
 Data File : BM021989.D
 Acq On : 10 Aug 2019 03:15
 Operator : HP/JU
 Sample : K4041-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENT1

Manual Integrations
 APPROVED

Sohil
 8/13/2019 8:45:57 AM

Quant Time: Aug 10 08:10:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 09 01:29:50 2019
 Response via : Initial Calibration

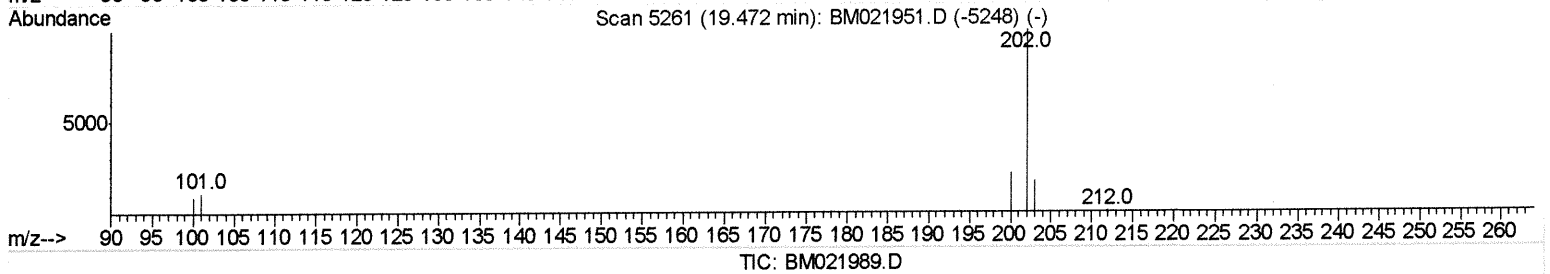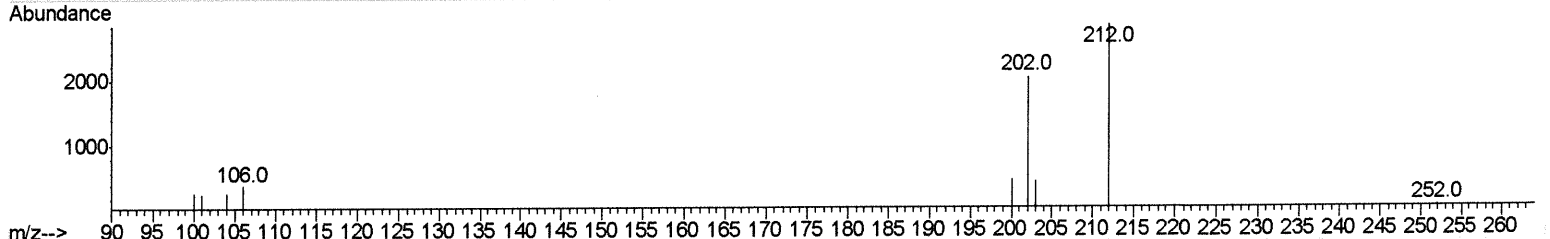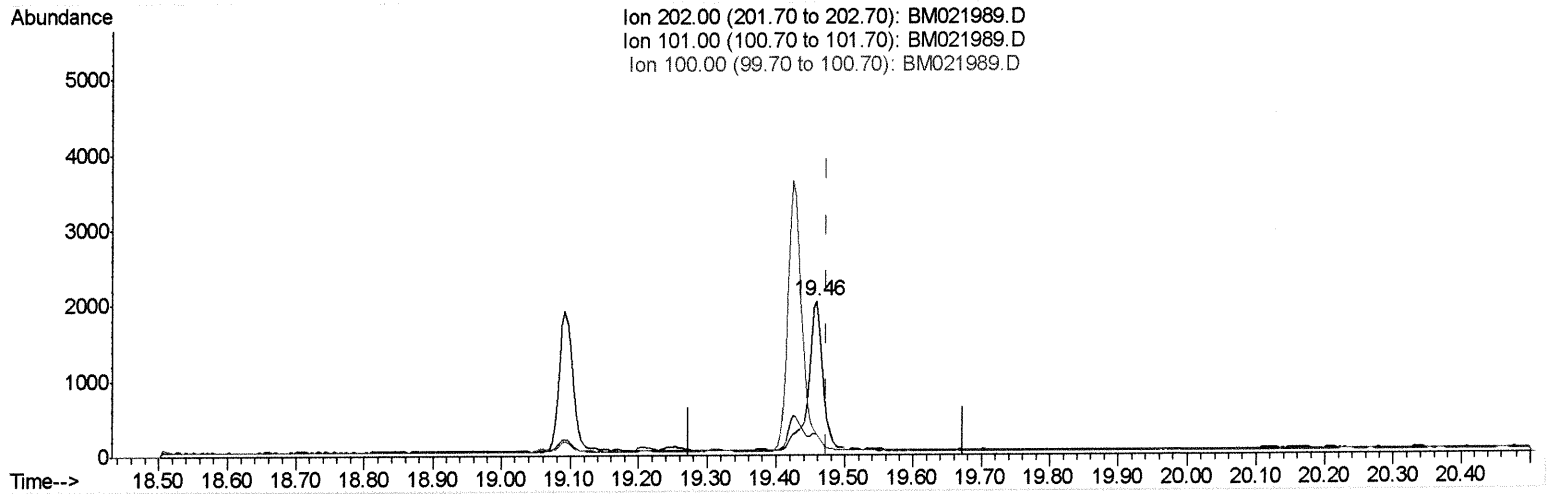

(17) Pyrene

19.459min (-0.015) 0.17ng/ul m *JU 08/12/19*

response 2677

Ion	Exp%	Act%
202.00	100	100
101.00	10.40	13.49#
100.00	9.00	13.84#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
Data File : BM021989.D
Acq On : 10 Aug 2019 03:15
Operator : HP/JU
Sample : K4041-07
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENT1

Manual Integrations
APPROVED

Sohil
8/13/2019 8:45:57 AM

Quant Time: Aug 10 08:10:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration

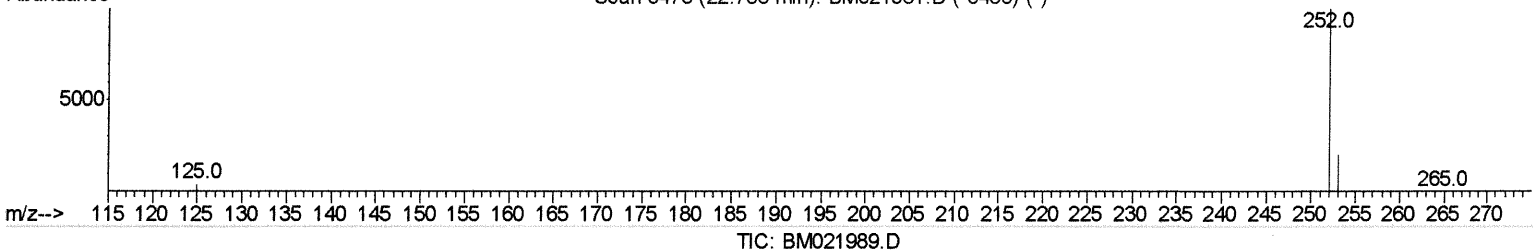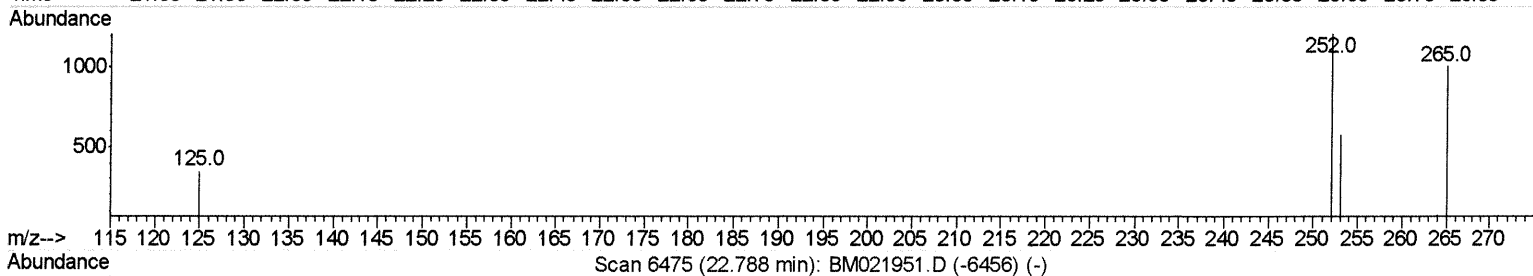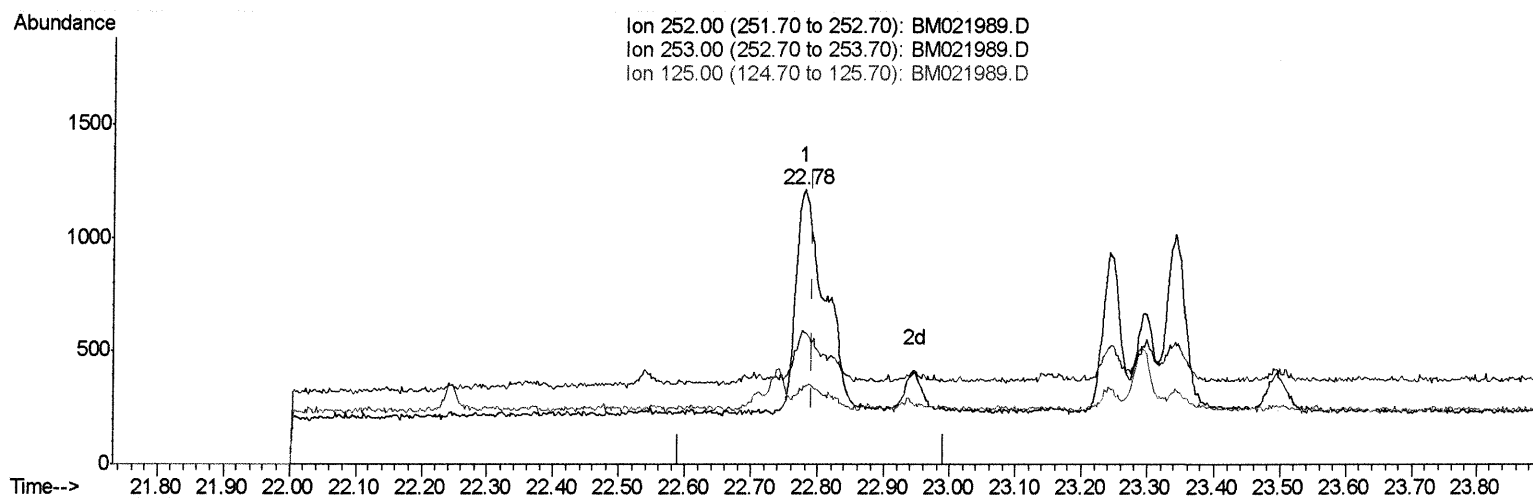

(21) Benzo(b)fluoranthene

22.779min (-0.012) 0.15ng/ul

response 3099

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	47.78
125.00	15.50	28.25
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
 Data File : BM021989.D
 Acq On : 10 Aug 2019 03:15
 Operator : HP/JU
 Sample : K4041-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENT1

Manual Integrations
 APPROVED

Sohil
 8/13/2019 8:45:57 AM

Quant Time: Aug 10 08:10:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 09 01:29:50 2019
 Response via : Initial Calibration

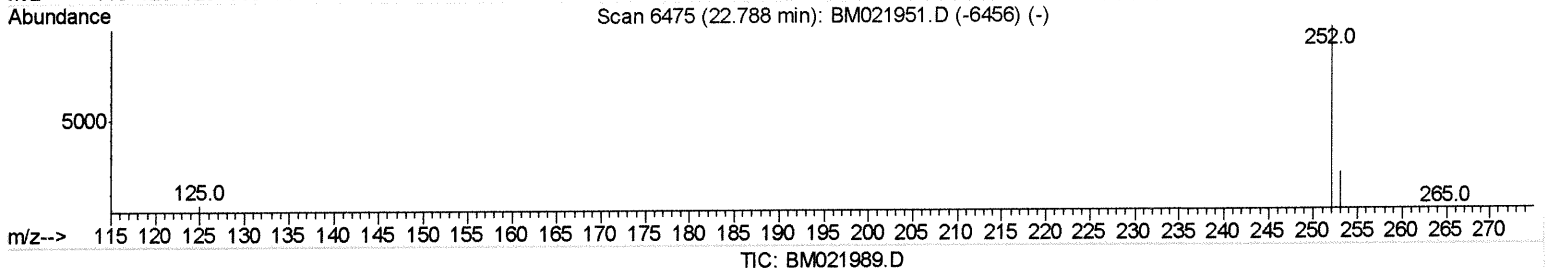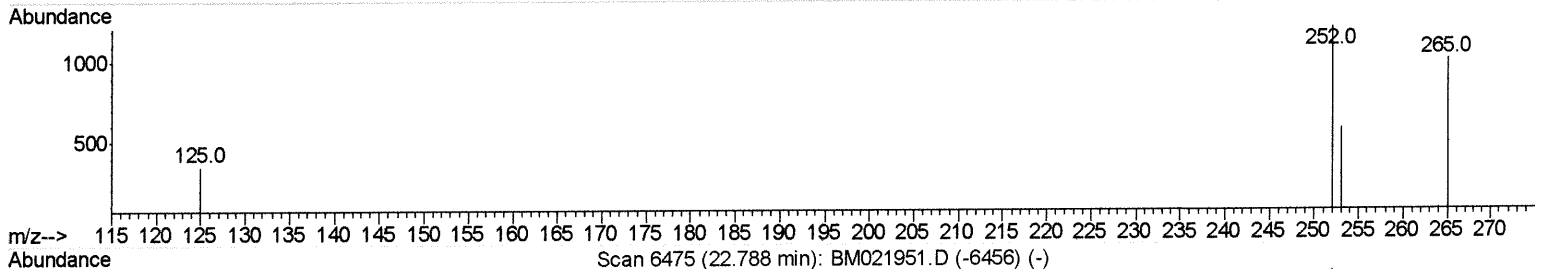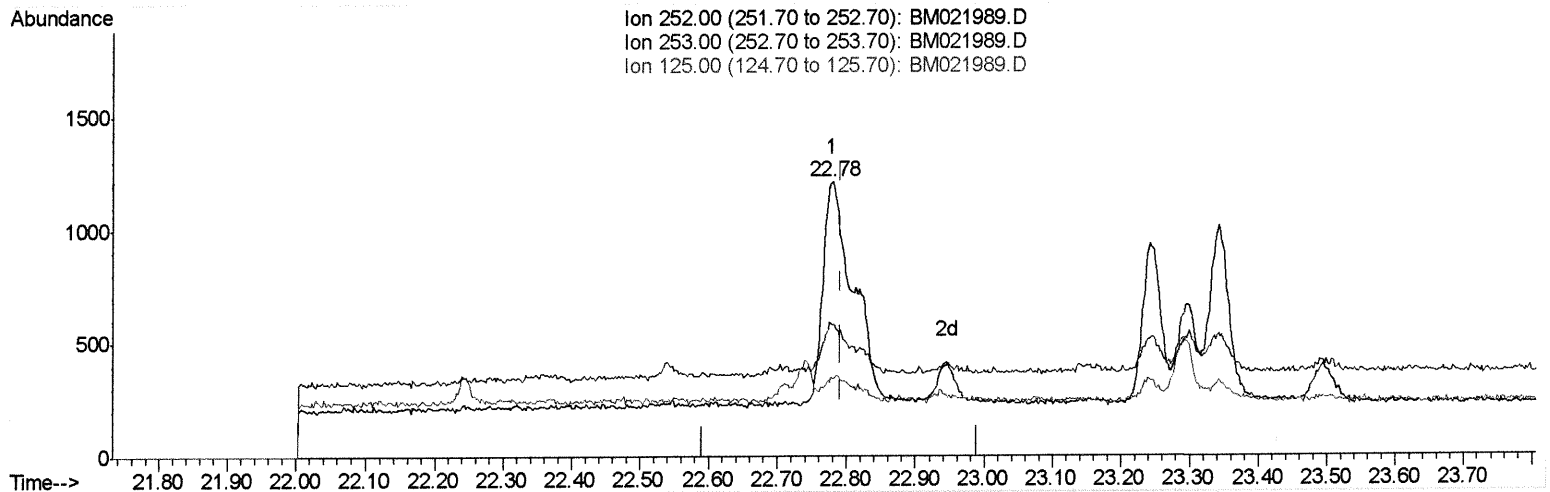

(21) Benzo(b)fluoranthene

22.779min (-0.012) 0.11ng/ul m *JU 08/12/19*

response 2306

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	47.78
125.00	15.50	28.25
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
 Data File : BM021989.D
 Acq On : 10 Aug 2019 03:15
 Operator : HP/JU
 Sample : K4041-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENT1

Manual Integrations
 APPROVED

Sohil
 8/13/2019 8:45:57 AM

Quant Time: Aug 10 08:10:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 09 01:29:50 2019
 Response via : Initial Calibration

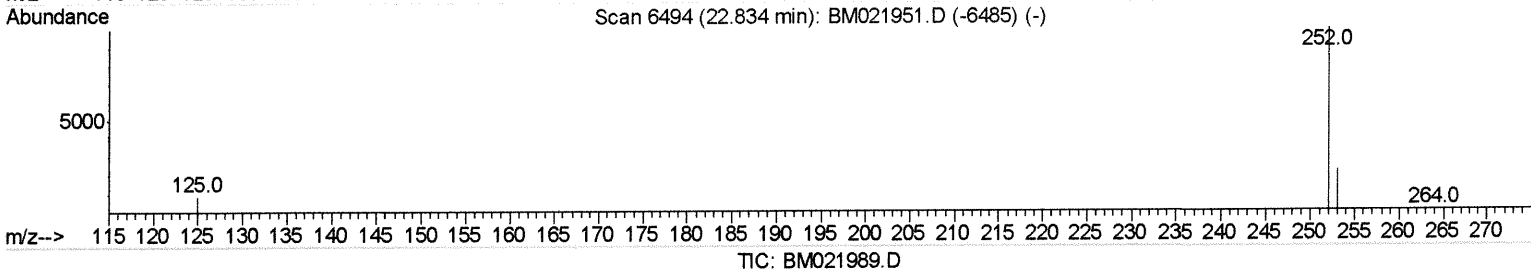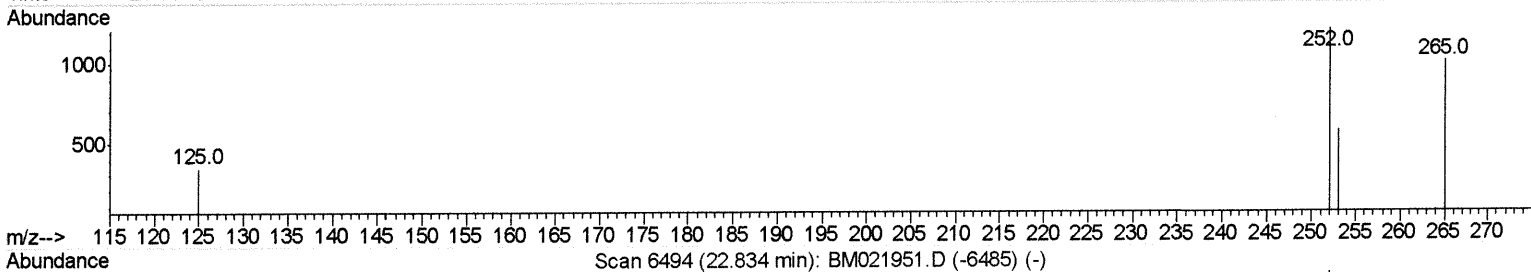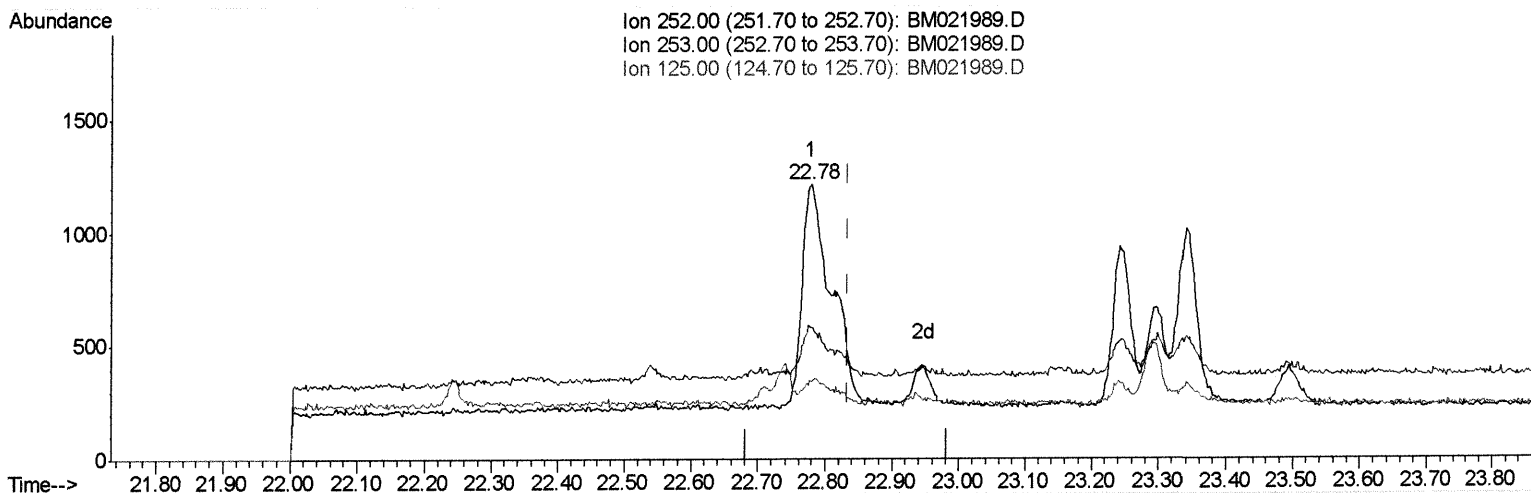

(22) Benzo(k)fluoranthene
 22.779min (-0.056) 0.13ng/ul
 response 3049

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	47.78#
125.00	15.20	28.25#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
 Data File : BM021989.D
 Acq On : 10 Aug 2019 03:15
 Operator : HP/JU
 Sample : K4041-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENT1

Manual Integrations
 APPROVED

Sohil
 8/13/2019 8:45:57 AM

Quant Time: Aug 10 08:10:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 09 01:29:50 2019
 Response via : Initial Calibration

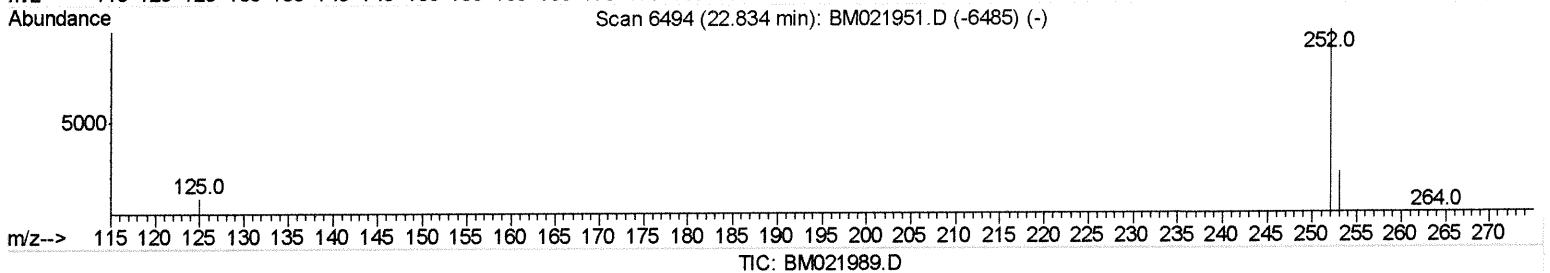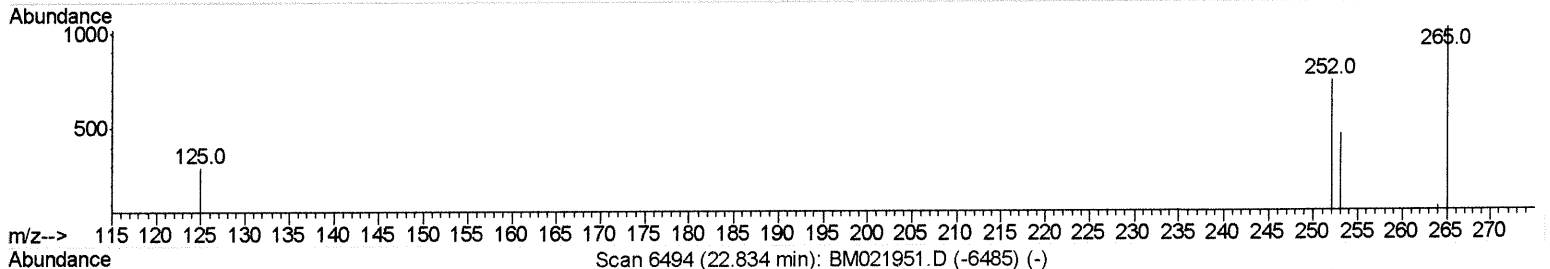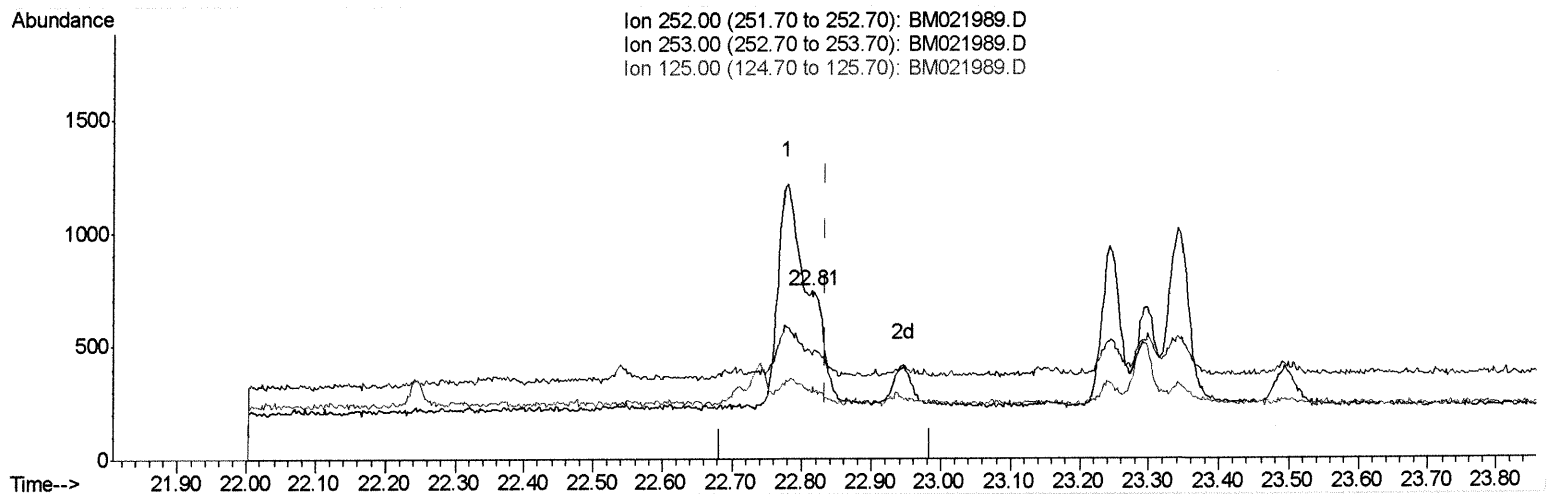

(22) Benzo(k)fluoranthene
 22.813min (-0.022) 0.03ng/ul m *JU 08/12/19*

response 701

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	61.91#
125.00	15.20	39.03#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080919\
 Data File : BM021989.D
 Acq On : 10 Aug 2019 03:15
 Operator : HP/JU
 Sample : K4041-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENT1

Manual Integrations
 APPROVED

Sohil
 8/13/2019 8:45:57 AM

Quant Time: Aug 10 08:12:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 09 01:29:50 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	774	0.40	ng/ul	0.00
2) Naphthalene-d8	10.39	136	3362	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.27	164	1836	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.03	188	4069m	0.40	ng/ul	-0.02
16) Chrysene-d12	21.23	240	3812m	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	6135	0.40	ng/ul	0.00

JU 08/12/19

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.02	152	1048	0.19	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	2503m	0.18	ng/ul	-0.02

JU 08/12/19

Target Compounds

					Ovalue	
7) Acenaphthylene	14.00	152	320	0.037	ng/ul#	64
12) Phenanthrene	17.07	178	1212m	0.102	ng/ul	
13) Anthracene	17.16	178	324m	0.032	ng/ul	
15) Fluoranthene	19.09	202	2602m	0.164	ng/ul	
17) Pyrene	19.46	202	2677m	0.171	ng/ul	
18) Benzo(a)anthracene	21.22	228	1477	0.108	ng/ul#	84
19) Chrysene	21.27	228	1378	0.079	ng/ul#	90
21) Benzo(b)fluoranthene	22.78	252	2306m	0.111	ng/ul	
22) Benzo(k)fluoranthene	22.81	252	701m	0.030	ng/ul	
23) Benzo(a)pyrene	23.34	252	1487	0.071	ng/ul#	74
24) Indeno(1,2,3-cd)pyrene	25.67	276	1128	0.045	ng/ul#	97
26) Benzo(a,h,i)perylene	26.36	276	1203	0.053	ng/ul#	71

JU 08/12/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed