

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080919\
 Data File : BM021986.D
 Acq On : 10 Aug 2019 01:23
 Operator : HP/JU
 Sample : K4041-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BENS8

Quant Time: Aug 10 07:43:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 09 01:29:50 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	845	0.40	ng/ul	0.00
2) Naphthalene-d8	10.40	136	3651	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.27	164	1984	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.03	188	4408	0.40	ng/ul	-0.02
16) Chrysene-d12	21.24	240	4079	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	6043	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	600	0.10	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	1427	0.10	ng/ul	-0.01
Target Compounds						
					Qvalue	
15) Fluoranthene	19.10	202	466	0.027	ng/ul#	52
17) Pyrene	19.46	202	442	0.026	ng/ul#	28


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080919\
Data File : BM021986.D
Acq On : 10 Aug 2019 01:23
Operator : HP/JU
Sample : K4041-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BENS8

Quant Time: Aug 10 07:43:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 09 01:29:50 2019
Response via : Initial Calibration




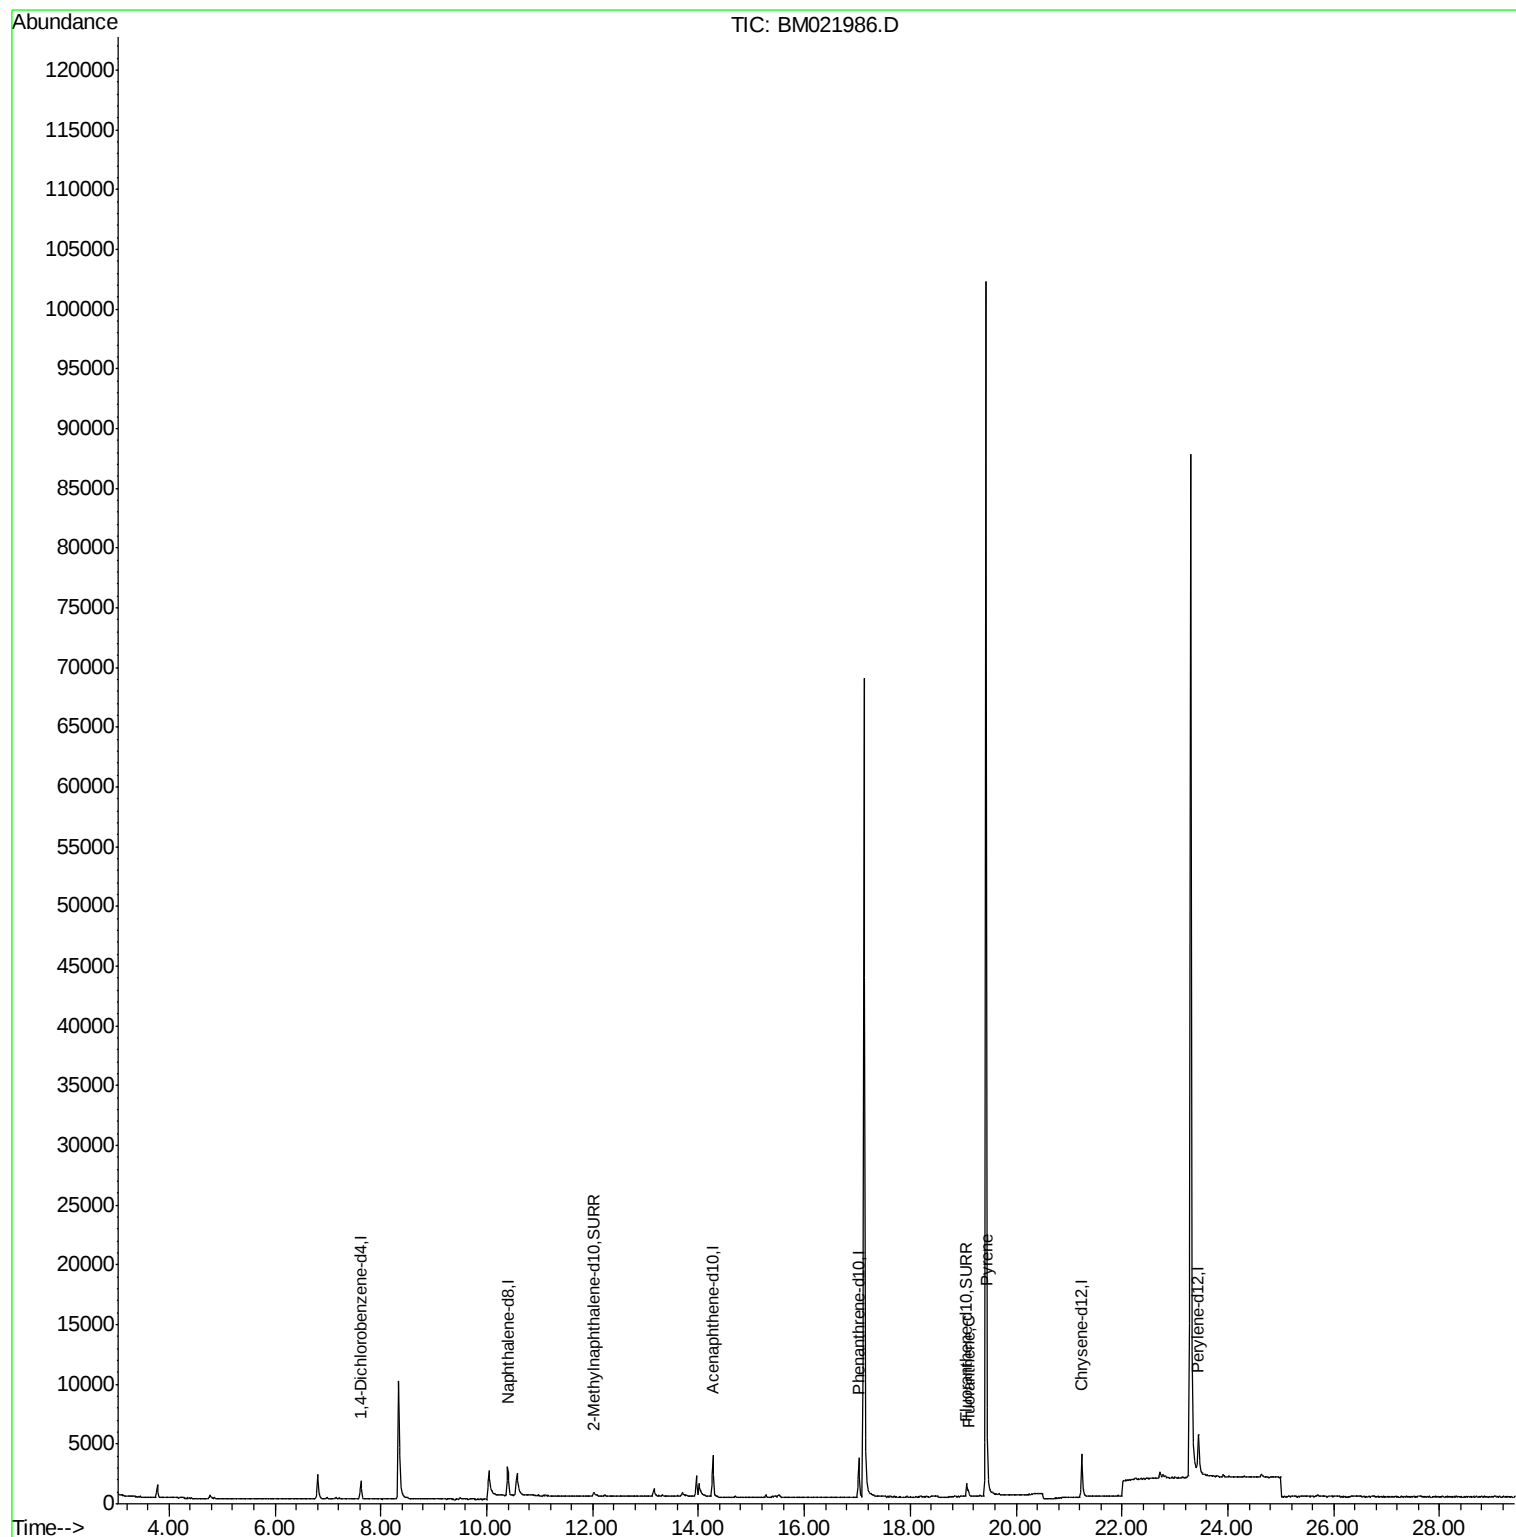


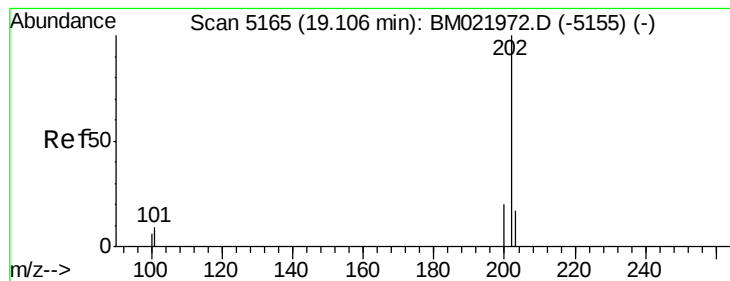

#15
Fluoranthene
 Concen: 0.027 ng/ul
 RT: 19.10 min Scan# 5163
 Delta R.T. -0.01 min
 Lab File: BM021986.D
 Acq: 10 Aug 2019 01:23

Instrument :
 BNA_M
 ClientSampleId :
 BENS8

Tgt Ion:202 Resp: 466
 Ion Ratio Lower Upper
 202 100
 101 23.4 0.0 30.2
 100 30.6 0.0 28.1#

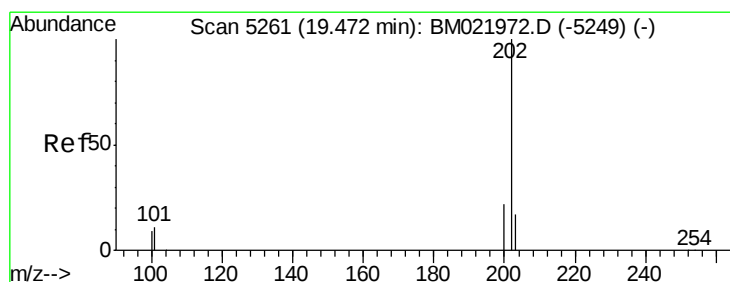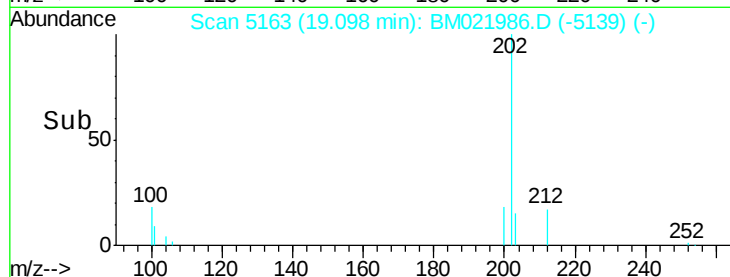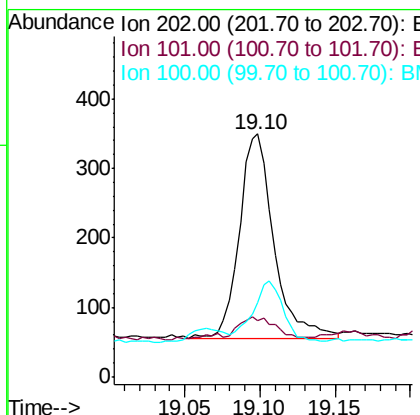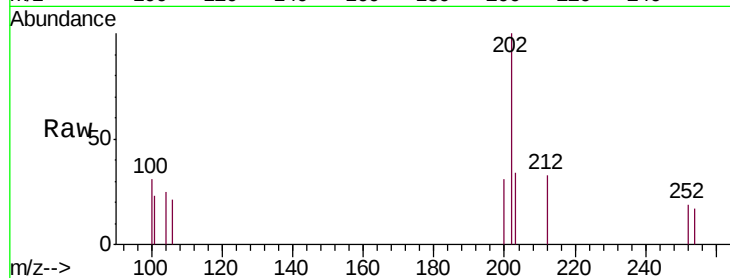

#17
Pyrene
 Concen: 0.026 ng/ul
 RT: 19.46 min Scan# 5257
 Delta R.T. -0.02 min
 Lab File: BM021986.D
 Acq: 10 Aug 2019 01:23

Tgt Ion:202 Resp: 442
 Ion Ratio Lower Upper
 202 100
 101 30.5 8.3 12.5#
 100 42.6 7.2 10.8#

