


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080919\
 Data File : BM021964.D
 Acq On : 09 Aug 2019 11:08
 Operator : HP/JU
 Sample : DFTPP02
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP02

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 12 18:02:08 2019

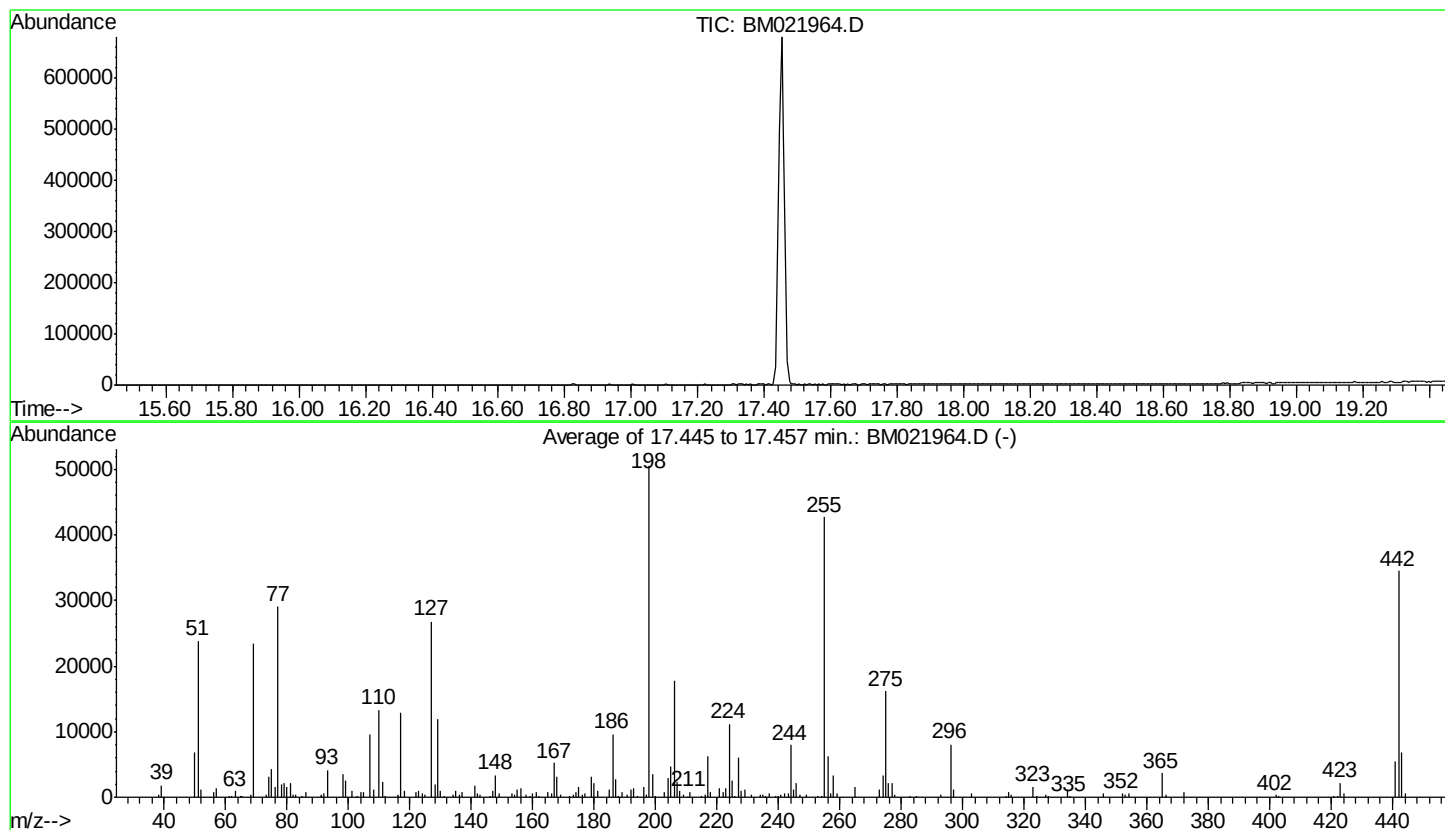

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.1	23829	PASS
68	69	0.00	2	1.5	341	PASS
69	198	0.00	100	46.5	23514	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.0	26818	PASS
197	198	0.00	2	0.6	300	PASS
198	198	100	100	100.0	50565	PASS
199	198	5	9	6.9	3491	PASS
275	198	10	60	31.9	16146	PASS
365	198	1	100	7.2	3620	PASS
441	198	0.01	100	10.8	5473	PASS
442	198	50	100	68.2	34469	PASS
443	442	15	24	19.9	6866	PASS

m/z	Abundance
37.90	356.0
39.00	1891.0
44.00	487.0
50.00	7087.0
51.00	24944.0
52.00	1292.0
55.90	775.0
57.00	1486.0
61.10	312.0
62.10	382.0
63.00	1170.0
64.90	412.0
68.10	508.0
69.00	24096.0
73.00	426.0
74.00	3490.0
75.00	4704.0
76.00	1434.0
77.00	29992.0
78.00	2123.0
79.00	1982.0
79.90	1715.0
81.00	1886.0
81.90	475.0
82.90	534.0
84.90	326.0
85.90	616.0
90.90	536.0
91.90	596.0
93.00	3896.0
98.00	3376.0
99.00	2924.0
101.00	1126.0
103.00	301.0
104.00	779.0
104.90	940.0
107.00	9238.0
108.00	1227.0
110.00	13008.0
111.00	2244.0
111.90	328.0
115.90	493.0
117.00	12357.0
118.00	991.0
122.00	675.0
123.00	946.0
124.00	538.0
125.00	404.0
127.00	25664.0
128.00	2073.0
129.00	11402.0
129.90	902.0
133.90	369.0
135.00	1032.0
135.90	450.0
137.00	730.0
140.90	1522.0
142.00	534.0
142.90	515.0
145.90	302.0
146.90	935.0
147.90	3110.0
149.00	590.0
153.00	716.0
154.00	442.0
155.00	1034.0
156.00	1437.0
157.90	481.0
159.90	537.0
160.90	754.0
162.00	357.0
165.00	769.0
166.00	610.0
167.00	5188.0
168.00	3212.0
168.90	348.0
171.90	321.0
173.00	470.0
173.90	941.0
175.00	1451.0
175.90	344.0
176.90	545.0
178.90	2802.0
179.90	2022.0
180.90	837.0
185.00	1075.0
186.00	8316.0
187.00	2724.0
188.00	424.0
188.90	589.0
190.90	438.0

Instrument :
BNA_M
ClientSampleId :
DFTPP02

192.00	1049.0
192.90	1039.0
193.90	352.0
195.90	1424.0
197.00	343.0
197.90	45032.0
198.90	3408.0
202.90	625.0
204.00	2631.0
205.00	4318.0
206.00	15071.0
207.00	2806.0
208.00	804.0
208.90	435.0
211.00	671.0
216.00	339.0
216.90	6022.0
217.90	609.0
220.90	1100.0
221.90	863.0
222.90	1191.0
224.00	9858.0
225.00	2266.0
227.00	5377.0
227.90	781.0
229.00	1068.0
230.90	366.0
233.90	350.0
236.90	738.0
240.90	306.0
242.00	543.0
243.00	442.0
244.00	6688.0
245.00	837.0
245.90	1763.0
246.90	368.0
248.90	348.0
255.00	35872.0
256.00	5637.0
256.90	637.0
257.90	2629.0
259.00	314.0
265.00	1120.0
272.90	941.0
273.90	2756.0
275.00	12784.0
276.00	1655.0
277.00	1746.0
285.00	307.0
292.90	323.0
296.00	6517.0
296.80	970.0
303.00	541.0
315.00	643.0
315.80	302.0
323.00	1075.0
326.90	351.0
333.90	811.0
346.00	386.0
351.90	311.0
352.90	308.0
353.90	488.0
365.00	2636.0
365.90	336.0
372.00	644.0
401.90	306.0
423.00	1410.0
423.90	366.0
441.00	3561.0
442.00	21520.0
443.00	4411.0
444.00	488.0

Instrument :
BNA_M
ClientSampleId :
DFTPP02

m/z	Abundance
38.00	619.0
39.00	2062.0
44.10	367.0
50.00	8257.0
51.00	28688.0
52.00	1292.0
56.00	880.0
57.00	1620.0
61.00	472.0
62.00	438.0
63.10	959.0
65.10	574.0
68.10	517.0
69.00	28456.0
73.00	471.0
74.00	3650.0
75.00	4998.0
76.00	1843.0
77.00	34920.0
78.00	2393.0
79.00	2686.0
80.00	1947.0
81.00	2690.0
82.00	532.0
82.90	562.0
85.00	426.0
86.00	886.0
90.90	483.0
92.00	618.0
93.00	5042.0
98.00	4035.0
99.00	2978.0
100.90	1295.0
102.90	533.0
103.90	782.0
105.00	939.0
107.00	12301.0
108.00	1529.0
110.00	16372.0
111.00	2800.0
111.90	341.0
116.10	587.0
117.00	15305.0
118.00	1084.0
122.00	814.0
123.00	1367.0
123.90	672.0
124.90	534.0
127.00	32896.0
128.00	2645.0
129.00	14776.0
129.90	1396.0
131.00	348.0
133.90	374.0
134.90	1203.0
135.90	511.0
136.90	801.0
141.00	2107.0
141.90	624.0
142.80	465.0
146.00	443.0
146.90	1244.0
148.00	4191.0
148.90	696.0
153.00	627.0
154.00	536.0
155.00	1263.0
155.90	1656.0
157.90	471.0
158.90	324.0
160.00	733.0
161.00	814.0
162.00	303.0
165.00	851.0
166.00	814.0
167.00	6286.0
167.90	3406.0
169.00	439.0
171.90	561.0
173.00	508.0
173.90	910.0
175.00	1991.0
176.00	417.0
177.00	894.0
178.90	3871.0
180.00	2733.0
180.90	987.0
184.90	1647.0
186.00	11899.0
187.00	3500.0
187.90	349.0

Instrument :
BNA_M
ClientSampleId :
DFTPP02

188.90	1053.0
190.90	457.0
192.00	1493.0
193.00	1580.0
196.00	1848.0
197.00	559.0
197.90	61184.0
198.90	4153.0
200.00	498.0
202.90	841.0
204.00	3395.0
205.00	5361.0
206.00	21256.0
207.00	3766.0
208.00	1149.0
208.90	580.0
210.20	306.0
210.90	979.0
214.90	325.0
216.10	575.0
217.00	7164.0
217.90	961.0
220.90	1730.0
221.90	796.0
222.90	1480.0
224.00	13598.0
225.00	3055.0
225.90	366.0
227.00	7294.0
227.90	1277.0
228.90	1411.0
231.00	458.0
233.90	510.0
234.90	533.0
235.90	374.0
236.90	531.0
238.90	401.0
239.90	368.0
240.90	380.0
242.00	741.0
243.10	769.0
244.00	9828.0
245.00	1244.0
245.90	2904.0
247.00	566.0
248.90	406.0
252.90	320.0
254.10	363.0
255.00	51880.0
256.00	7080.0
257.00	606.0
258.00	3939.0
258.90	714.0
265.00	2016.0
272.90	1562.0
274.00	3934.0
275.00	20616.0
276.00	2812.0
276.90	2694.0
278.00	497.0
282.90	386.0
284.90	406.0
292.90	462.0
296.00	9456.0
296.90	1544.0
302.90	844.0
314.00	446.0
314.90	1080.0
315.90	592.0
323.00	2191.0
324.00	408.0
326.90	577.0
327.90	362.0
334.00	1408.0
334.90	392.0
345.90	622.0
352.00	800.0
352.90	412.0
354.00	621.0
364.90	4247.0
366.00	540.0
372.00	810.0
402.00	431.0
403.00	463.0
420.90	379.0
421.90	356.0
423.00	2717.0
423.90	515.0
441.00	6938.0
442.00	42512.0
443.00	8483.0
444.00	674.0

Instrument :
BNA_M
ClientSampleId :
DFTPP02

m/z	Abundance
39.00	1327.0
40.00	311.0
44.00	585.0
50.00	5248.0
51.00	17856.0
52.00	945.0
56.00	524.0
56.90	1105.0
62.90	747.0
65.00	307.0
69.00	17992.0
73.00	469.0
74.00	2171.0
75.00	3333.0
76.00	1202.0
77.00	22288.0
78.00	1641.0
79.00	1554.0
80.00	1245.0
81.00	1770.0
82.00	425.0
86.00	663.0
91.10	432.0
91.90	553.0
93.00	3454.0
98.00	2915.0
99.00	1878.0
101.00	783.0
104.00	756.0
104.90	619.0
107.00	7467.0
108.00	935.0
110.00	10642.0
111.00	1741.0
115.90	472.0
117.00	10844.0
118.00	704.0
122.00	742.0
122.90	796.0
123.90	518.0
127.00	21896.0
128.00	1302.0
129.00	9497.0
129.90	721.0
133.90	326.0
134.90	847.0
135.90	401.0
136.90	587.0
141.00	1751.0
141.90	455.0
143.00	343.0
146.90	839.0
148.00	2856.0
148.90	535.0
153.00	433.0
153.80	390.0
154.90	1014.0
156.00	1137.0
158.00	375.0
159.90	382.0
160.90	852.0
164.90	737.0
165.80	583.0
167.00	4307.0
168.00	2763.0
168.90	300.0
173.00	500.0
173.90	676.0
175.00	1236.0
175.90	324.0
177.00	624.0
178.90	2623.0
180.00	1760.0
181.00	887.0
184.90	1047.0
186.00	8629.0
187.00	2193.0
188.90	648.0
190.90	392.0
191.90	1105.0
193.00	1235.0
193.90	300.0
196.00	1229.0
197.90	45480.0
198.90	2914.0
203.00	693.0
204.00	2642.0
205.00	4439.0
206.00	16952.0
207.00	3099.0
208.00	902.0

Instrument :
BNA_M
ClientSampleId :
DFTPP02

209.00	402.0
211.00	768.0
216.00	549.0
216.90	5641.0
217.90	793.0
220.90	1554.0
221.70	669.0
223.00	1357.0
224.00	10052.0
225.00	2515.0
227.00	5591.0
227.90	878.0
229.00	774.0
231.00	348.0
233.90	362.0
234.90	483.0
237.00	368.0
240.90	326.0
241.90	519.0
243.00	730.0
244.00	7311.0
245.00	1175.0
245.90	2018.0
246.90	476.0
248.90	301.0
255.00	40256.0
256.00	5877.0
256.90	475.0
257.90	3385.0
258.90	475.0
264.90	1502.0
272.90	1207.0
274.00	3163.0
275.00	15038.0
275.90	2274.0
277.00	2011.0
277.90	418.0
282.90	315.0
292.90	482.0
296.00	8214.0
297.00	985.0
303.00	602.0
313.90	354.0
314.90	850.0
315.90	383.0
323.00	1706.0
323.90	316.0
326.90	322.0
334.00	1374.0
345.90	490.0
351.90	598.0
353.00	337.0
354.00	483.0
365.00	3979.0
366.10	371.0
372.00	771.0
402.00	355.0
403.00	421.0
420.90	311.0
422.00	323.0
423.00	2479.0
424.00	666.0
441.00	5921.0
442.00	39376.0
443.00	7704.0
444.00	617.0

Instrument :

BNA_M

ClientSampleId :

DFTPP02

m/z	Abundance
44.00	623.0
207.00	789.0

Instrument :
BNA_M
ClientSampleId :
DFTPP02