


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080921\
Data File : BM031601.D
Acq On : 09 Aug 2021 13:41
Operator : CG/JU
Sample : M3163-12DL 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGEZ0DL

Manual Integrations
APPROVED

mohammad
8/10/2021 4:36:07 PM

Quant Time: Aug 09 14:14:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 09 10:16:43 2021
Response via : Initial Calibration

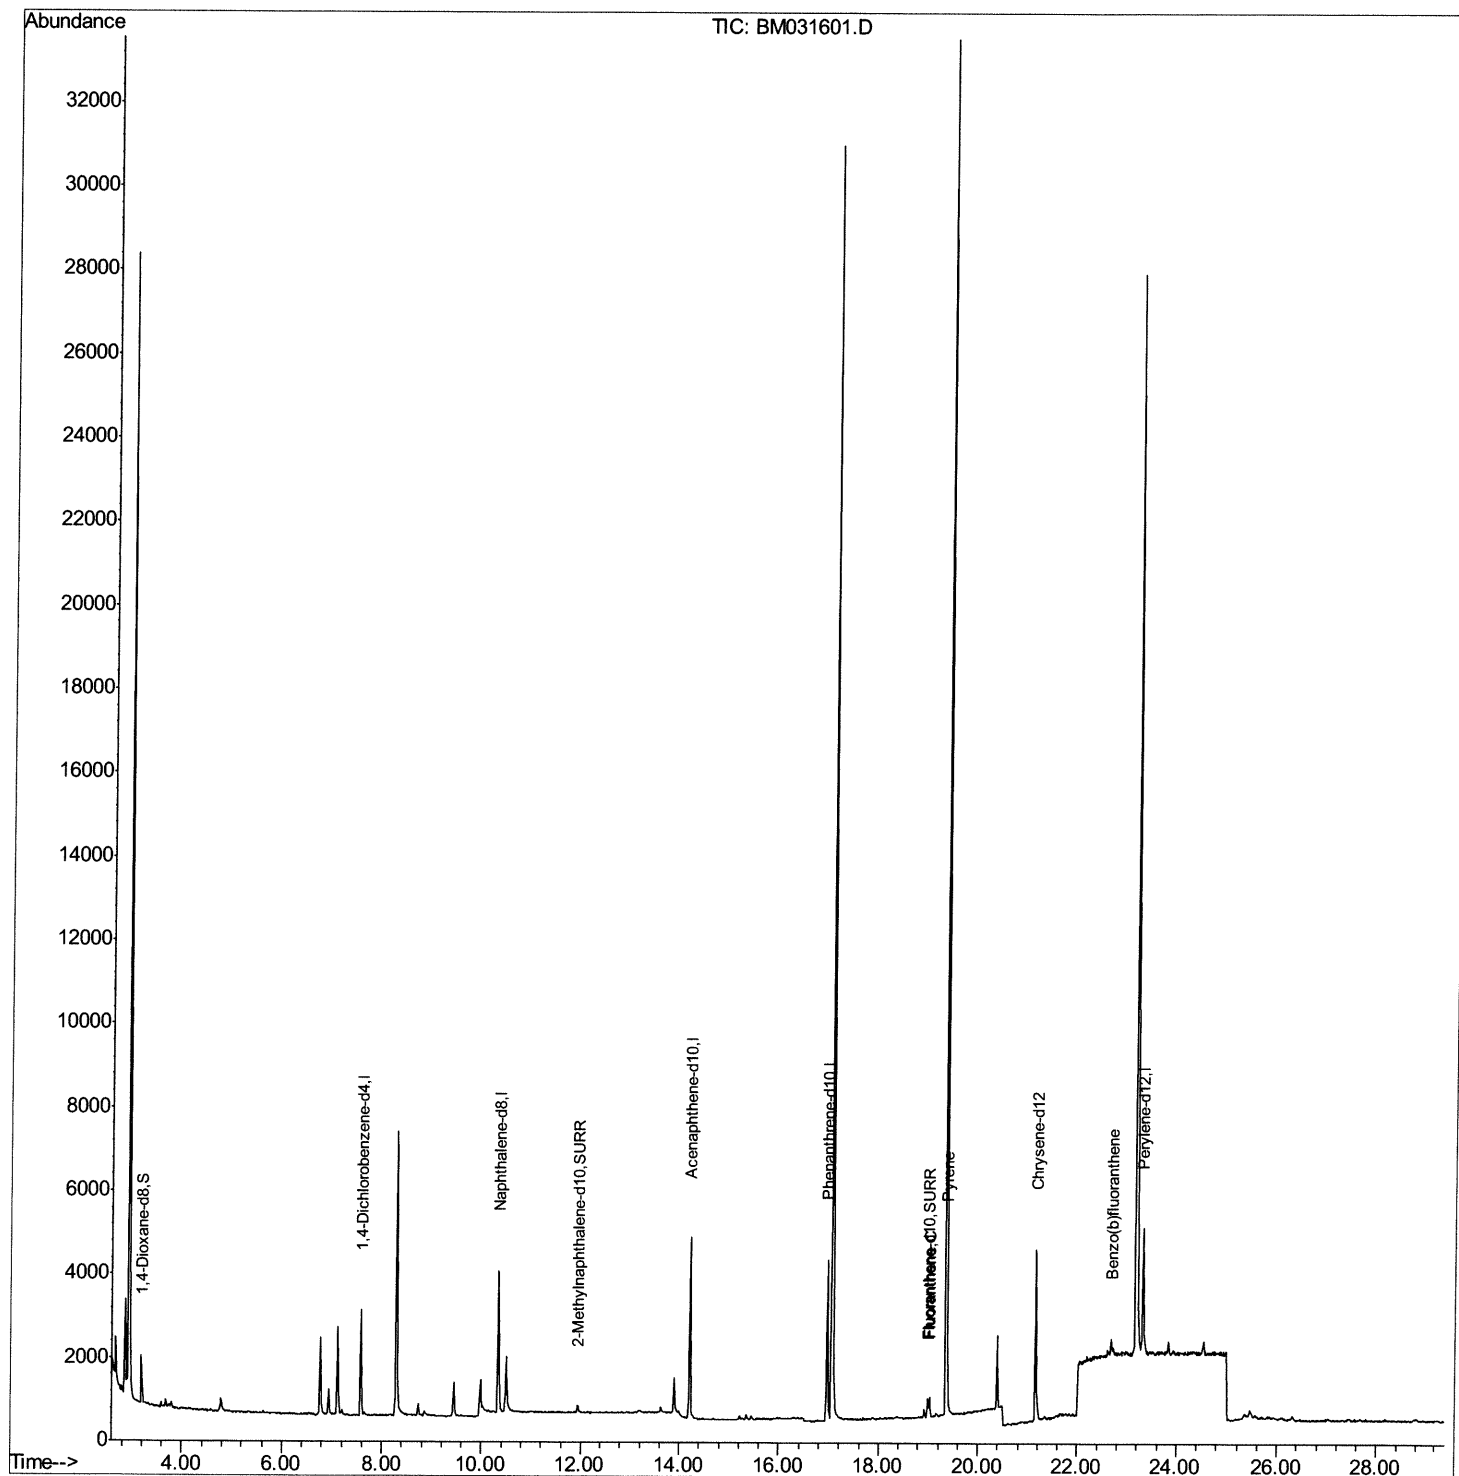

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080921\
Data File : BM031601.D
Acq On : 09 Aug 2021 13:41
Operator : CG/JU
Sample : M3163-12DL 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BGEZ0DL

Manual Integrations
APPROVED

mohammad
8/10/2021 4:36:07 PM

Quant Time: Aug 09 14:12:56 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 09 10:16:43 2021
Response via : Initial Calibration

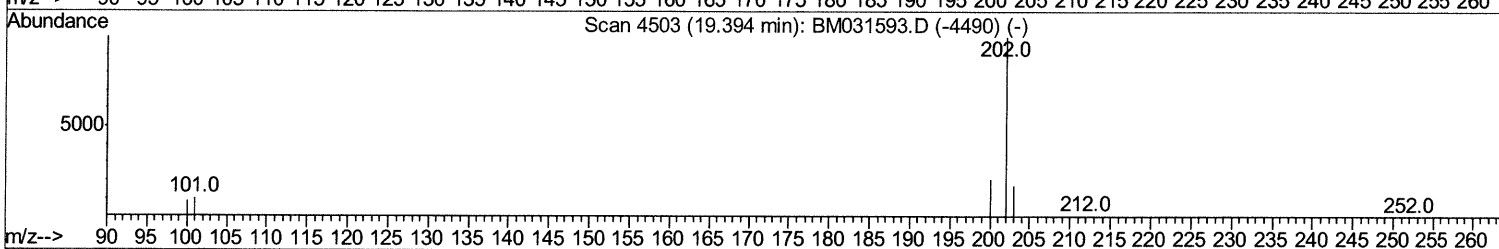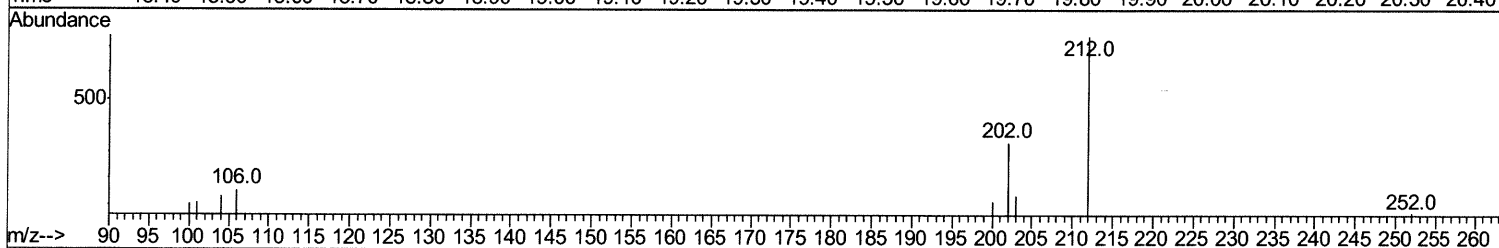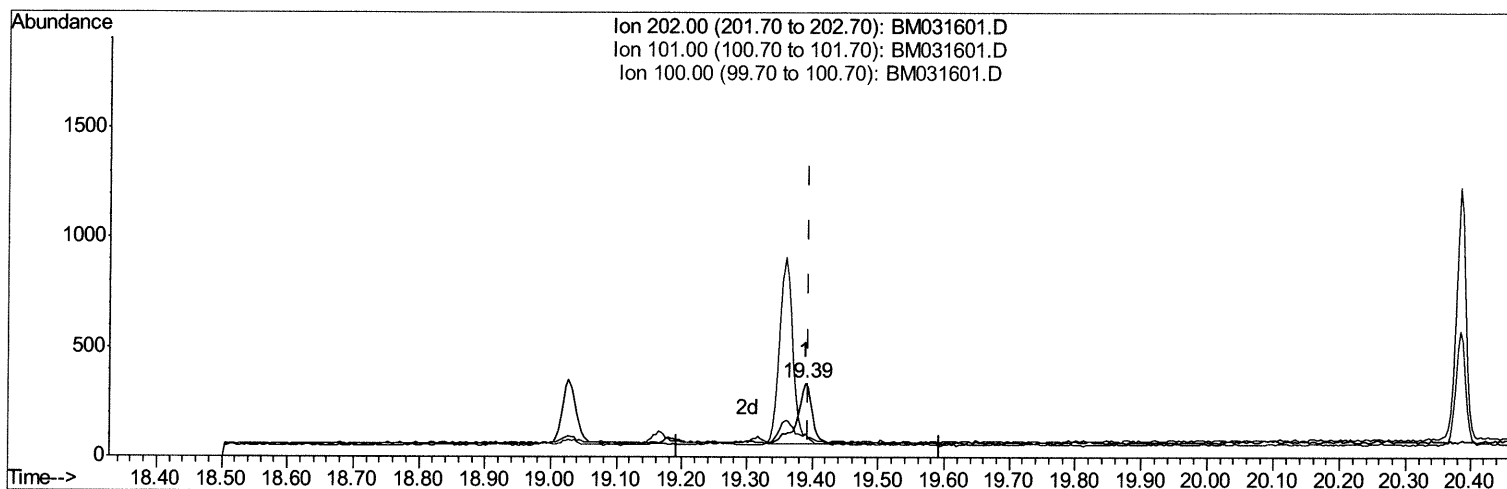

TIC: BM031601.D

(20) Pyrene

19.389min (-0.004) 0.03ng/ul

response 466

Ion	Exp%	Act%
202.00	100	100
101.00	9.70	32.05#
100.00	8.30	31.16#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080921\
 Data File : BM031601.D
 Acq On : 09 Aug 2021 13:41
 Operator : CG/JU
 Sample : M3163-12DL 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampled :
 BGEZ0DL

Manual Integrations
APPROVED

mohammad
 8/10/2021 4:36:07 PM

Quant Time: Aug 09 14:12:56 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 09 10:16:43 2021
 Response via : Initial Calibration

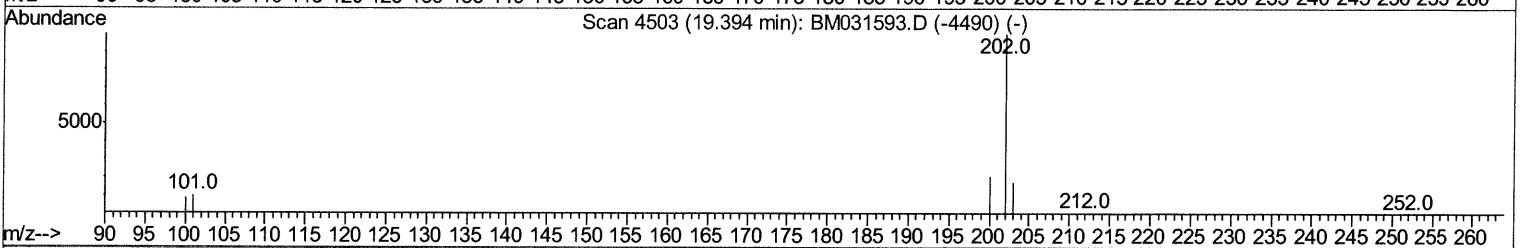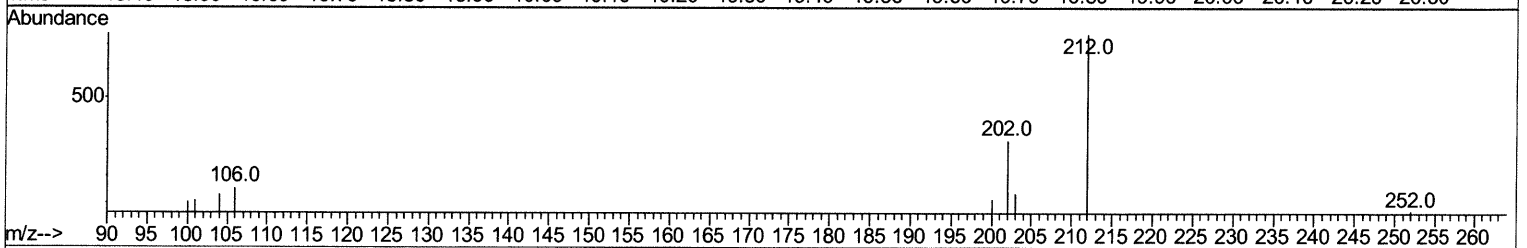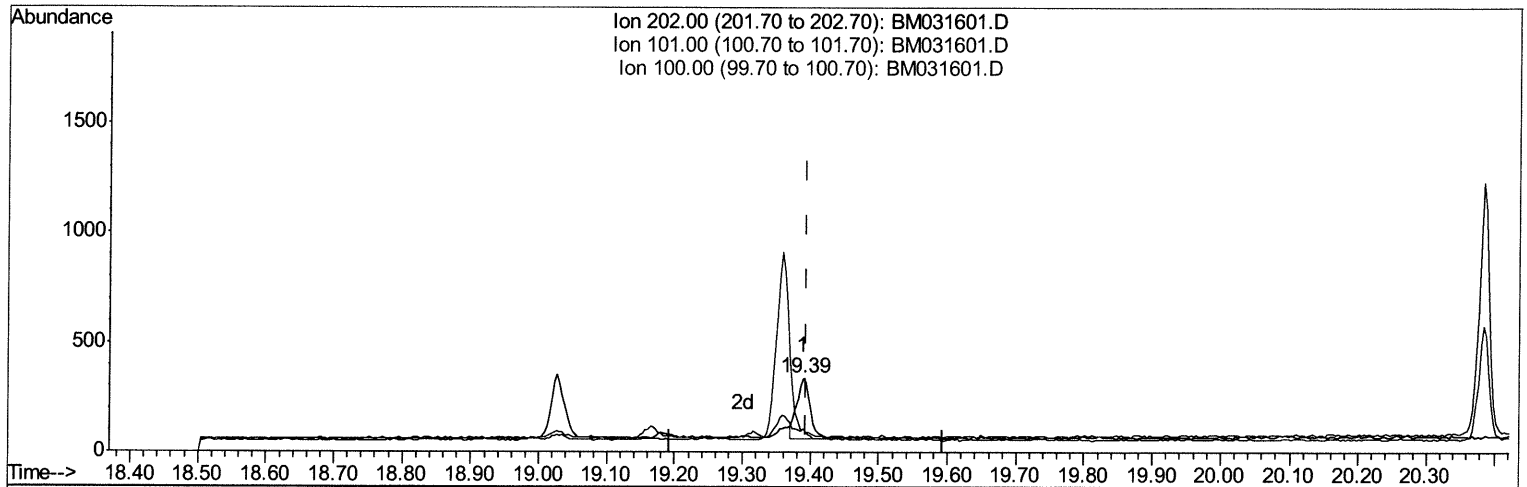

TIC: BM031601.D

(20) Pyrene

19.389min (-0.004) 0.02ng/ul m

response 385

Ion	Exp%	Act%
202.00	100	100
101.00	9.70	32.05#
100.00	8.30	31.16#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080921\
 Data File : BM031601.D
 Acq On : 09 Aug 2021 13:41
 Operator : CG/JU
 Sample : M3163-12DL 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGEZ0DL

Manual Integrations
 APPROVED

mohammad
 8/10/2021 4:36:07 PM

Quant Time: Aug 09 14:14:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 09 10:16:43 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	1241	0.40	ng/ul	0.00
4) Naphthalene-d8	10.34	136	4612	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.21	164	2520	0.40	ng/ul	0.00
13) Phenanthrene-d10	16.96	188	4805	0.40	ng/ul	0.00
17) Chrysene-d12	21.16	240	3857	0.40	ng/ul	0.00
23) Perylene-d12	23.32	264	3779	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.19	96	764	0.55	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.94	152	279	0.04	ng/ul	0.00
18) Fluoranthene-d10	19.00	212	517	0.04	ng/ul	0.00
Target Compounds						
19) Fluoranthene	19.03	202	395	0.024	ng/ul#	51
20) Pyrene	19.39	202	385m	0.023	ng/ul	
24) Benzo(b)fluoranthene	22.69	252	355	0.021	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed