

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080921\
 Data File : BM031634.D
 Acq On : 10 Aug 2021 10:35
 Operator : CG/JU
 Sample : M3169-19
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0063

Quant Time: Aug 10 11:15:19 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 09 10:16:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.580	152	1408	0.400	ng/ul	0.00
4) Naphthalene-d8	10.338	136	5202	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.208	164	3132	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.961	188	5704	0.400	ng/ul #	0.00
17) Chrysene-d12	21.159	240	4454	0.400	ng/ul #	0.00
23) Perylene-d12	23.317	264	4559	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.186	96	7262	4.644	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.935	152	2881	0.329	ng/ul	0.00
18) Fluoranthene-d10	18.997	212	6121	0.412	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.388	128	435	0.028	ng/ul#	63
10) Acenaphthylene	13.927	152	299	0.022	ng/ul#	50


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080921\
Data File : BM031634.D
Acq On : 10 Aug 2021 10:35
Operator : CG/JU
Sample : M3169-19
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0063

Quant Time: Aug 10 11:15:19 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 09 10:16:43 2021
Response via : Initial Calibration




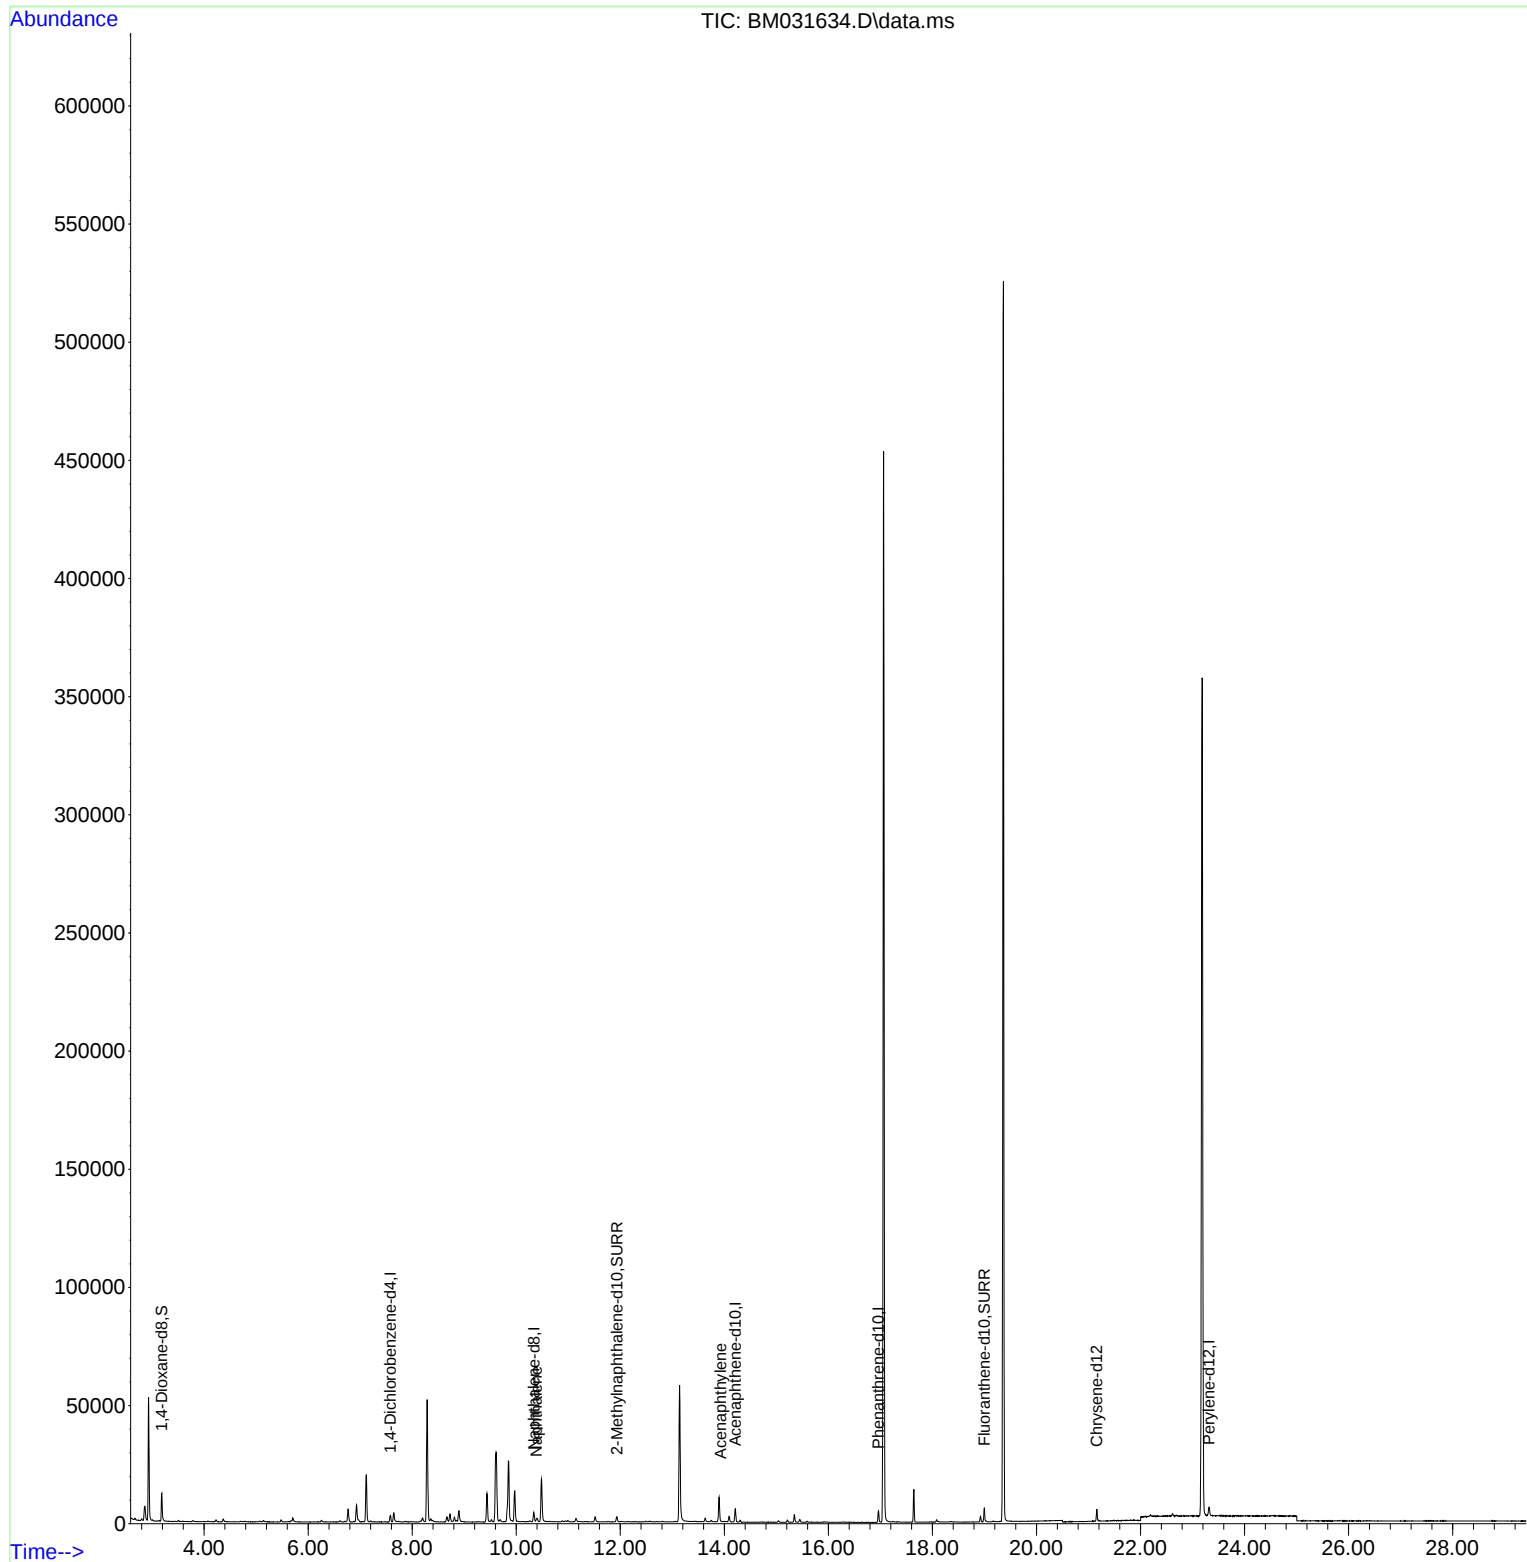


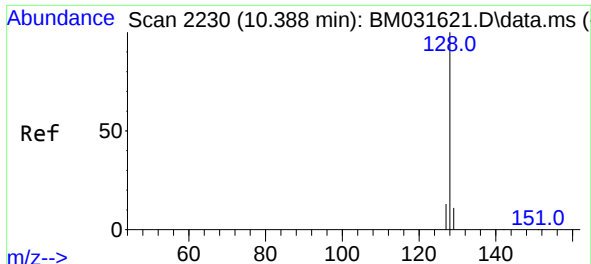

#5
Naphthalene
Concen: 0.028 ng/ul
RT: 10.388 min Scan# 2230
Delta R.T. -0.000 min
Lab File: BM031634.D
Acq: 10 Aug 2021 10:35

Instrument :
BNA_M
ClientSampleId :
C0063

Tgt Ion:	128	Resp:	435
Ion	Ratio	Lower	Upper
128	100		
129	30.2	10.0	15.0#
127	27.0	11.6	17.4#

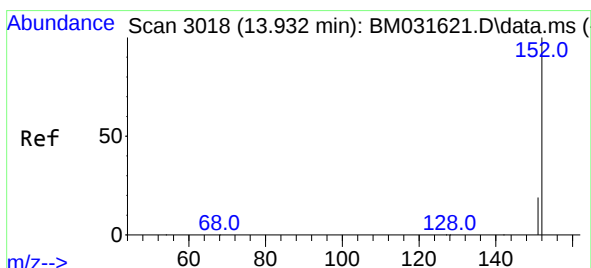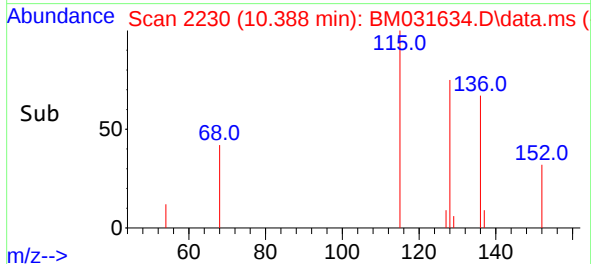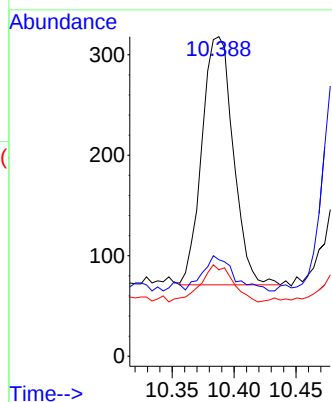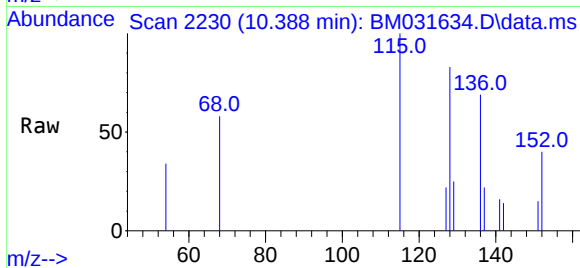

#10
Acenaphthylene
Concen: 0.022 ng/ul
RT: 13.927 min Scan# 3017
Delta R.T. -0.005 min
Lab File: BM031634.D
Acq: 10 Aug 2021 10:35

Tgt Ion:	152	Resp:	299
Ion	Ratio	Lower	Upper
152	100		
151	44.4	16.9	25.3#
153	0.0	0.0	0.0

