
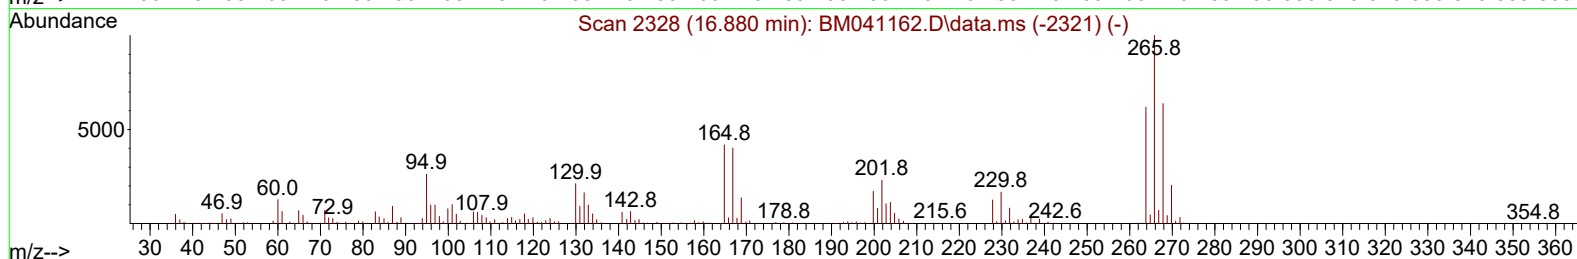
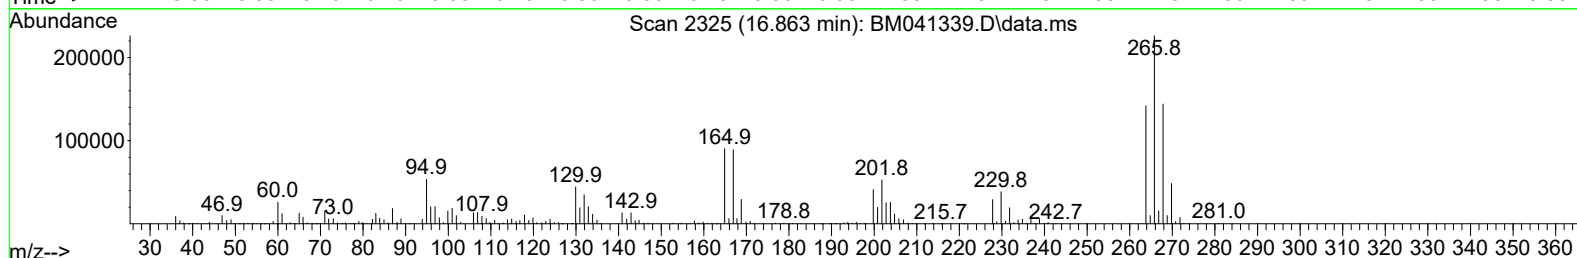


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM080923\  
 Data File : BM041339.D  
 Acq On : 09 Aug 2023 12:33  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 13:18:04 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM072823.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Aug 09 12:20:12 2023  
 Response via : Initial Calibration

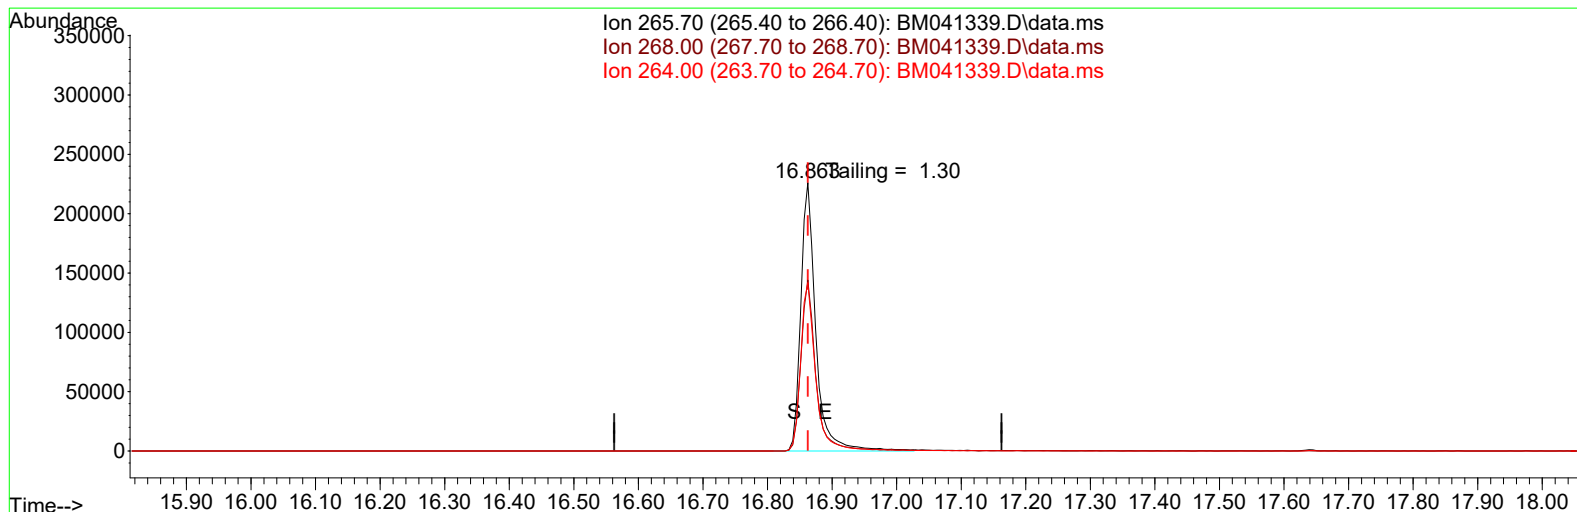

TIC: BM041339.D\data.ms

**(70) Pentachlorophenol (C)**




16.863min (-0.000) 0.00 ng

response 369000

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.80  | 63.67  |
| 264.00 | 61.80  | 62.73  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM080923\  
Data File : BM041339.D  
Acq On : 09 Aug 2023 12:33  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 09 13:18:04 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM072823.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 09 12:20:12 2023  
Response via : Initial Calibration

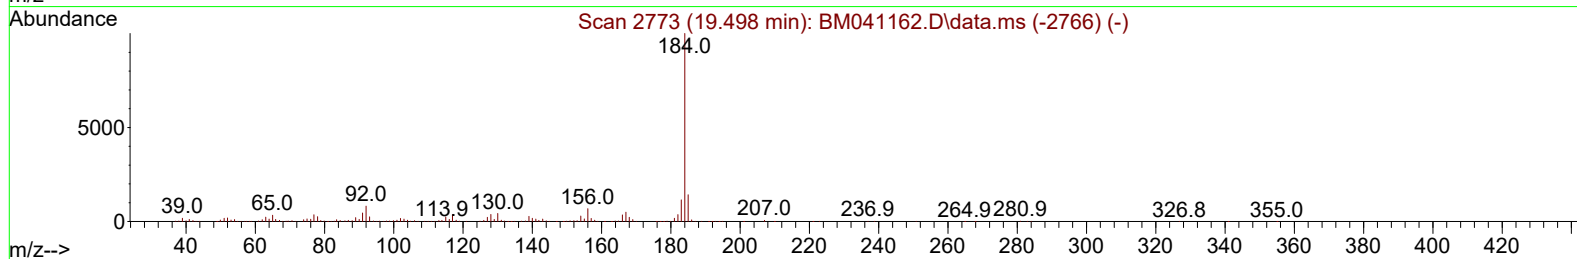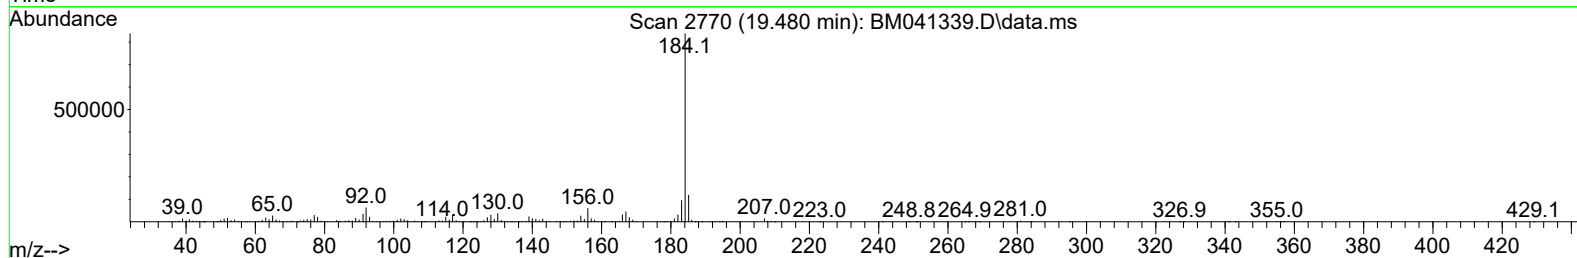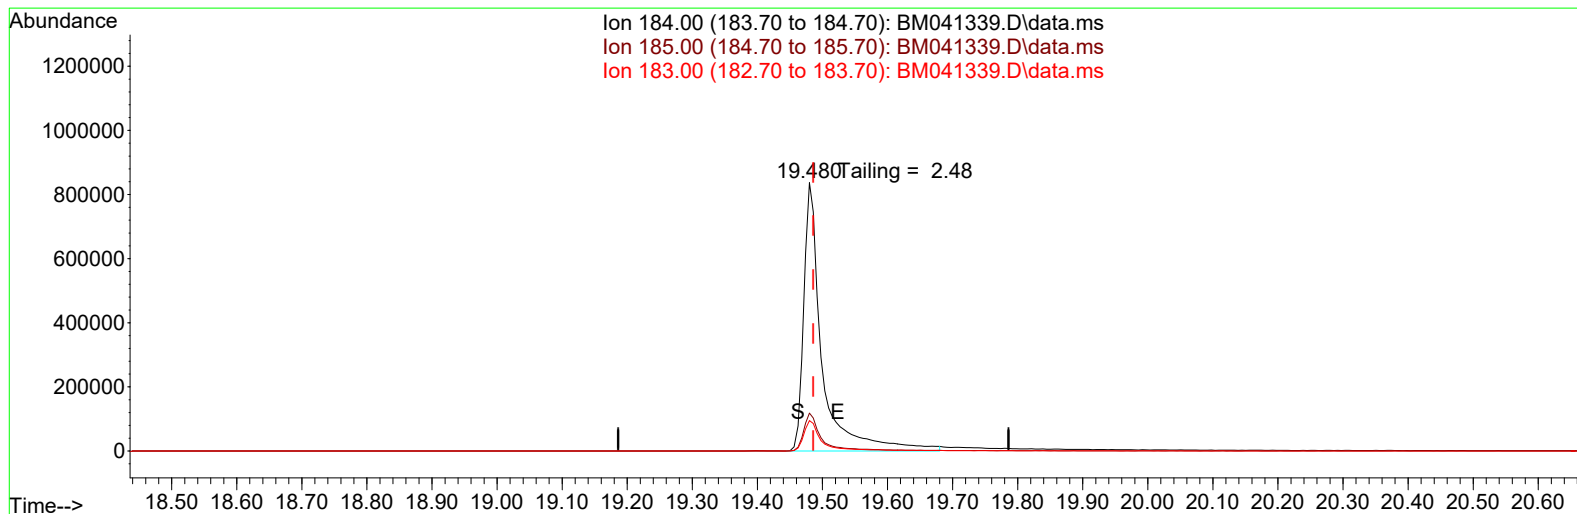

TIC: BM041339.D\data.ms

**(77) Benzidine****19.480min (-0.006) 137728.95 ng****response 1640700**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.20  | 14.14  |
| 183.00 | 11.50  | 11.32  |
| 0.00   | 0.00   | 0.00   |