

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080923\
 Data File : BM041345.D
 Acq On : 09 Aug 2023 18:31
 Operator : MA/JU
 Sample : 03905-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 FLY-ASH

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM041345.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	9	13	19	rVB	292962	301729	5.00%	0.950%
2	3.940	124	128	135	rVB2	54254	80589	1.34%	0.254%
3	4.216	171	175	181	rVB	71604	86617	1.44%	0.273%
4	4.404	202	207	212	rBV	79510	107680	1.79%	0.339%
5	4.469	214	218	225	rVB	55172	72174	1.20%	0.227%
6	4.851	278	283	288	rBV	132708	184162	3.05%	0.580%
7	4.904	288	292	305	rVB	92682	143719	2.38%	0.452%
8	5.357	363	369	386	rBV	1594236	2432263	40.33%	7.658%
9	6.969	636	643	668	rBV	1100675	1975851	32.77%	6.221%
10	7.781	774	781	788	rBV	406932	625195	10.37%	1.968%
11	8.957	973	981	1002	rBV	1006664	1747733	28.98%	5.503%
12	9.169	1011	1017	1031	rBV	86961	226582	3.76%	0.713%
13	10.586	1250	1258	1272	rBV	475414	811620	13.46%	2.555%
14	11.122	1342	1349	1355	rBV	347807	537895	8.92%	1.694%
15	11.186	1355	1360	1374	rVB	408893	699610	11.60%	2.203%
16	13.063	1672	1679	1703	rBV	2823894	4100884	68.00%	12.911%
17	13.339	1719	1726	1743	rBV	1688187	2681795	44.47%	8.443%
18	14.445	1906	1914	1934	rBV	631051	1057034	17.53%	3.328%
19	15.951	2163	2170	2190	rBV	1928099	3243599	53.79%	10.212%
20	17.209	2378	2384	2404	rBV	776137	1204543	19.97%	3.792%
21	18.115	2532	2538	2549	rBV	200321	492310	8.16%	1.550%
22	19.397	2752	2756	2770	rBV	129144	330417	5.48%	1.040%
23	19.845	2827	2832	2848	rBV	4941815	6030340	100.00%	18.986%
24	21.415	3095	3099	3110	rBV	842284	1282872	21.27%	4.039%
25	23.785	3497	3502	3520	rVB	541591	1304902	21.64%	4.108%




Sum of corrected areas: 31762115

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080923\
Data File : BM041345.D
Acq On : 09 Aug 2023 18:31
Operator : MA/JU
Sample : 03905-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FLY-ASH

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

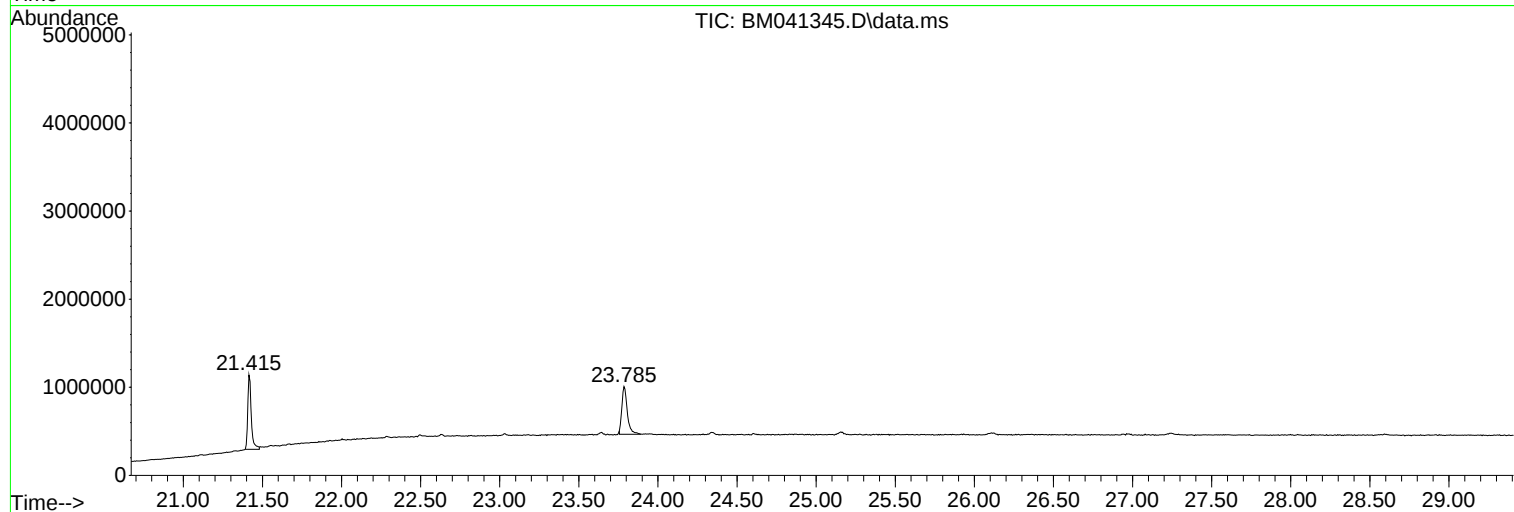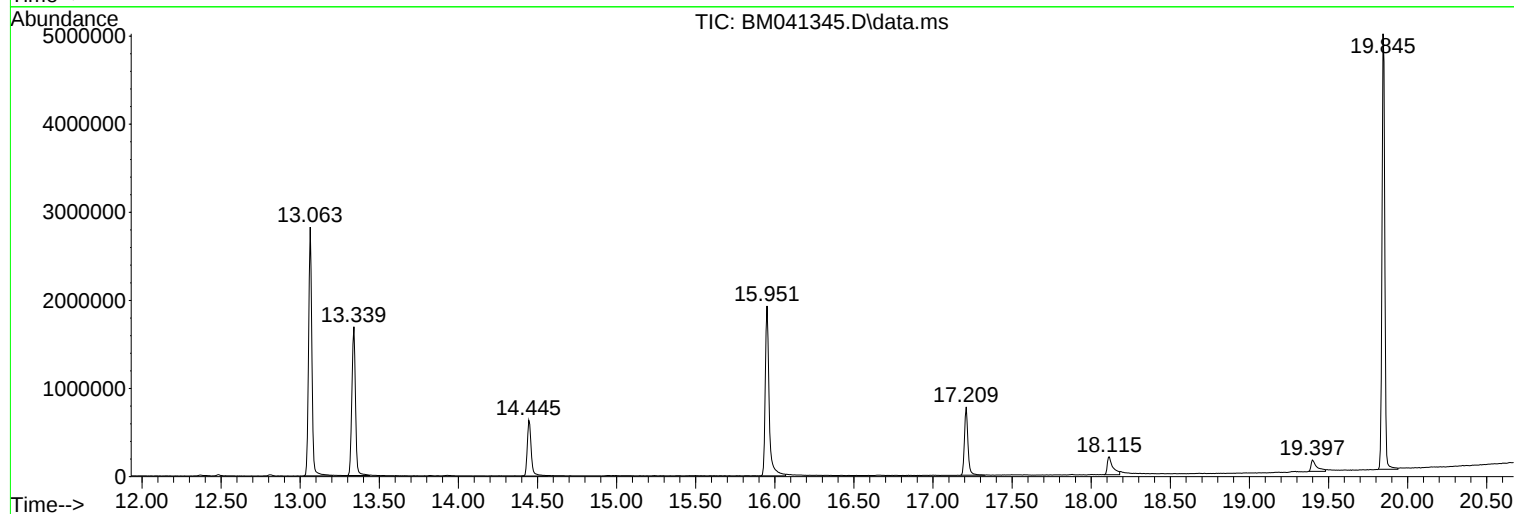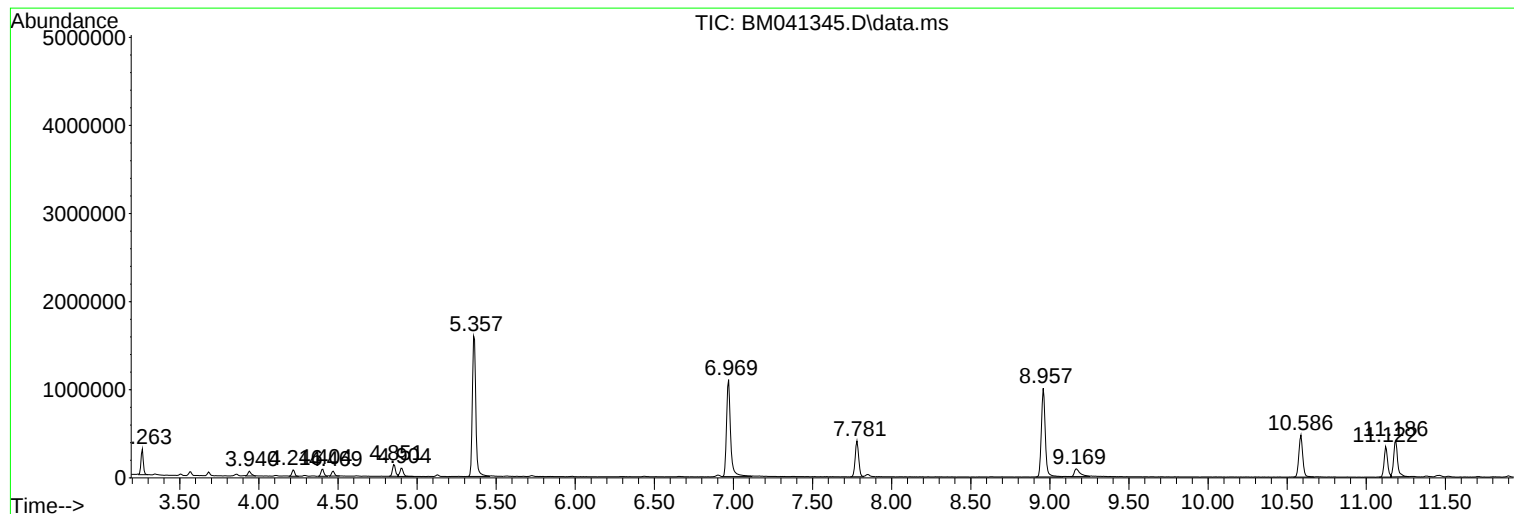

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080923\
Data File : BM041345.D
Acq On : 09 Aug 2023 18:31
Operator : MA/JU
Sample : 03905-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FLY-ASH

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080923\
Data File : BM041345.D
Acq On : 09 Aug 2023 18:31
Operator : MA/JU
Sample : 03905-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
FLY-ASH

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc