


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM080923\  
Data File : BM041339.D  
Acq On : 09 Aug 2023 12:33  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM072823.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed Aug 09 12:20:12 2023

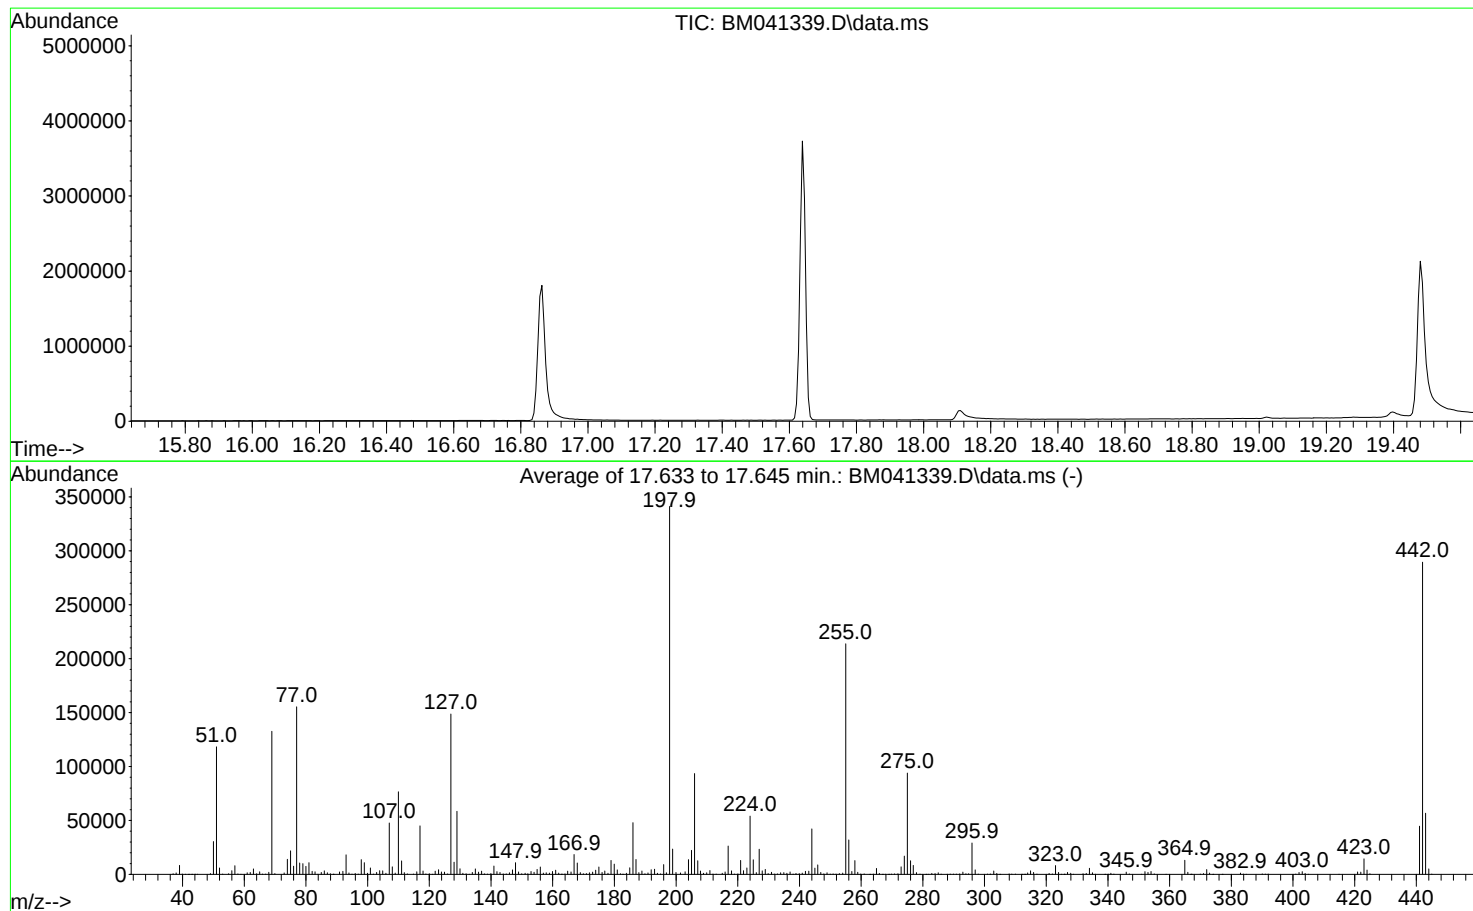




AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2449

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 34.7         | 118317     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.5          | 1933       | PASS                |
| 69             | 198             | 0.00            | 100             | 38.9         | 132562     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 726        | PASS                |
| 127            | 198             | 10              | 80              | 43.6         | 148651     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.4          | 1488       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 341077     | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 23421      | PASS                |
| 275            | 198             | 10              | 60              | 27.5         | 93851      | PASS                |
| 365            | 198             | 1               | 100             | 3.8          | 13030      | PASS                |
| 441            | 198             | 0.01            | 100             | 13.1         | 44725      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 289493     | PASS                |
| 443            | 442             | 15              | 24              | 19.6         | 56691      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM080923\  
 Data File : BM041339.D  
 Acq On : 09 Aug 2023 12:33  
 Operator : MA/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Quant Time: Aug 09 13:18:04 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM072823.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Aug 09 12:20:12 2023  
 Response via : Initial Calibration

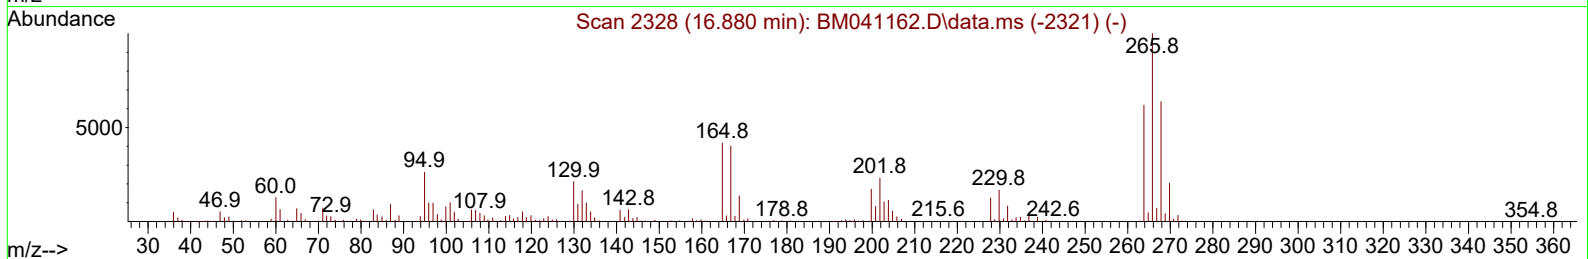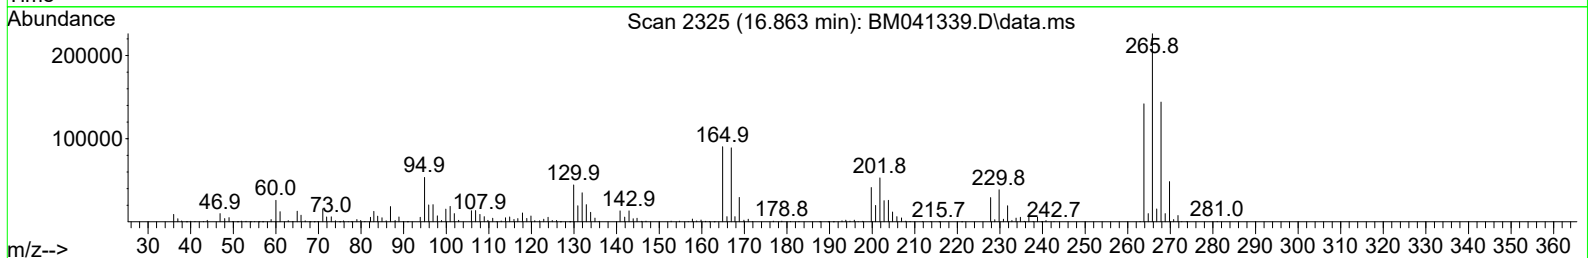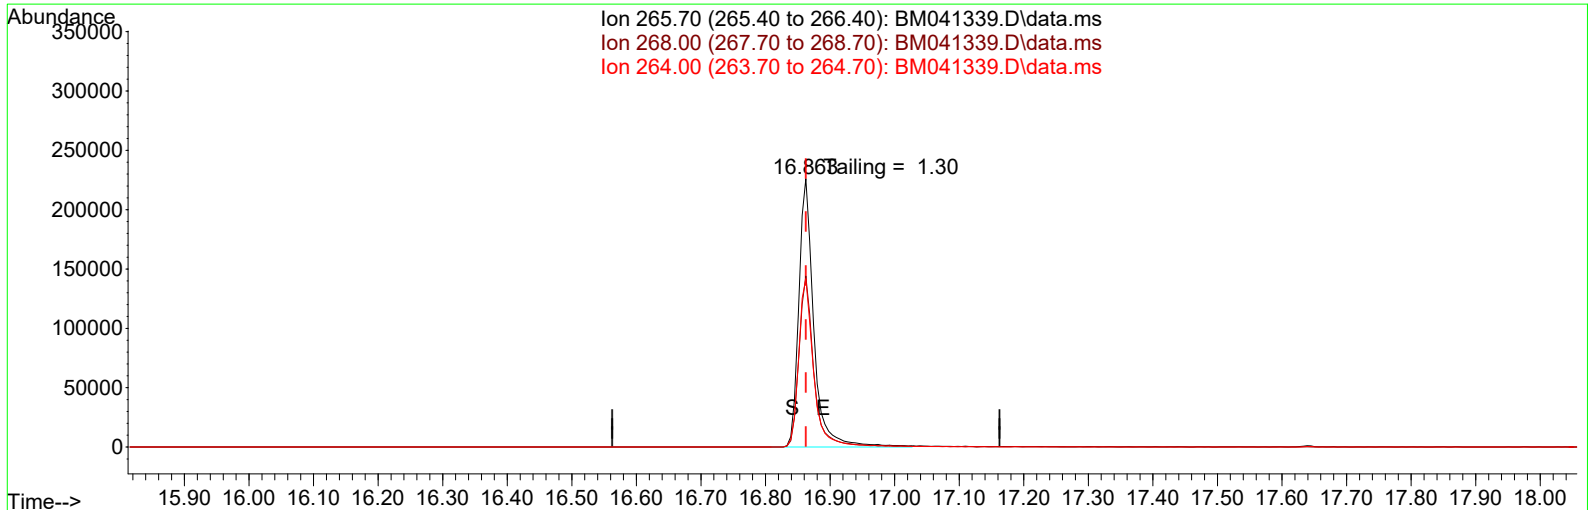

TIC: BM041339.D\data.ms

**(70) Pentachlorophenol (C)**

16.863min (-0.000) 0.00 ng




response 369000

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.80  | 63.67  |
| 264.00 | 61.80  | 62.73  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM080923\  
Data File : BM041339.D  
Acq On : 09 Aug 2023 12:33  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Aug 09 13:18:04 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM072823.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 09 12:20:12 2023  
Response via : Initial Calibration

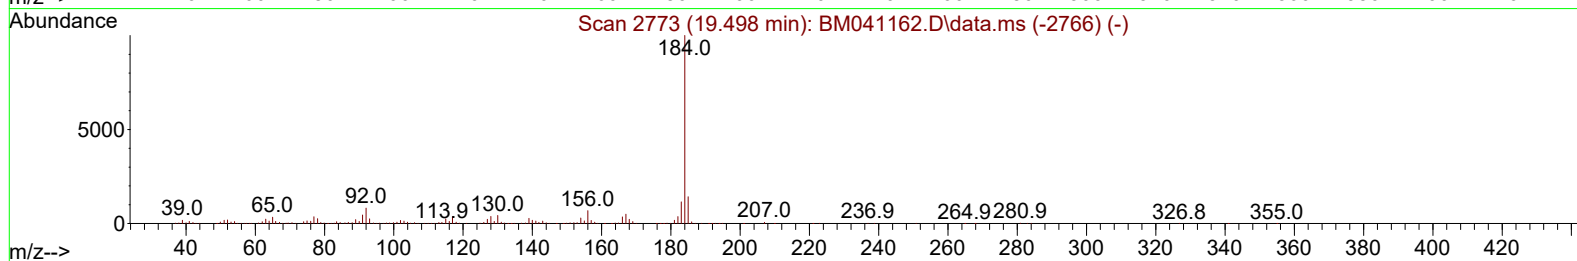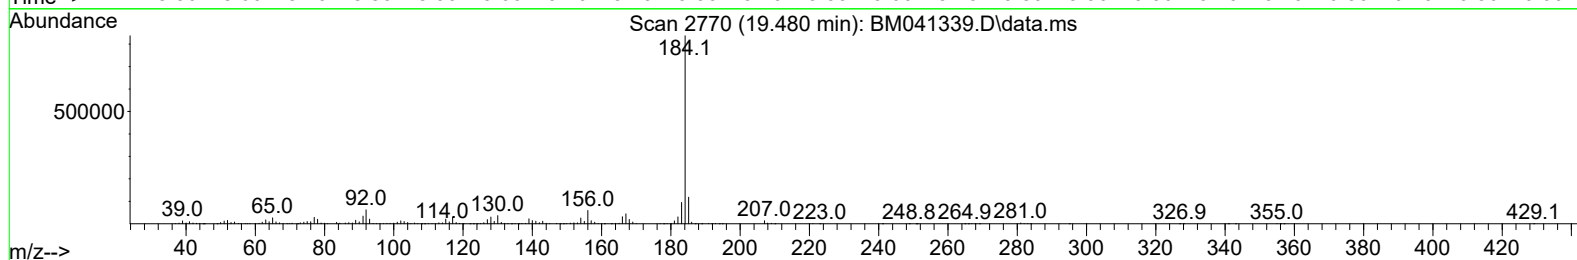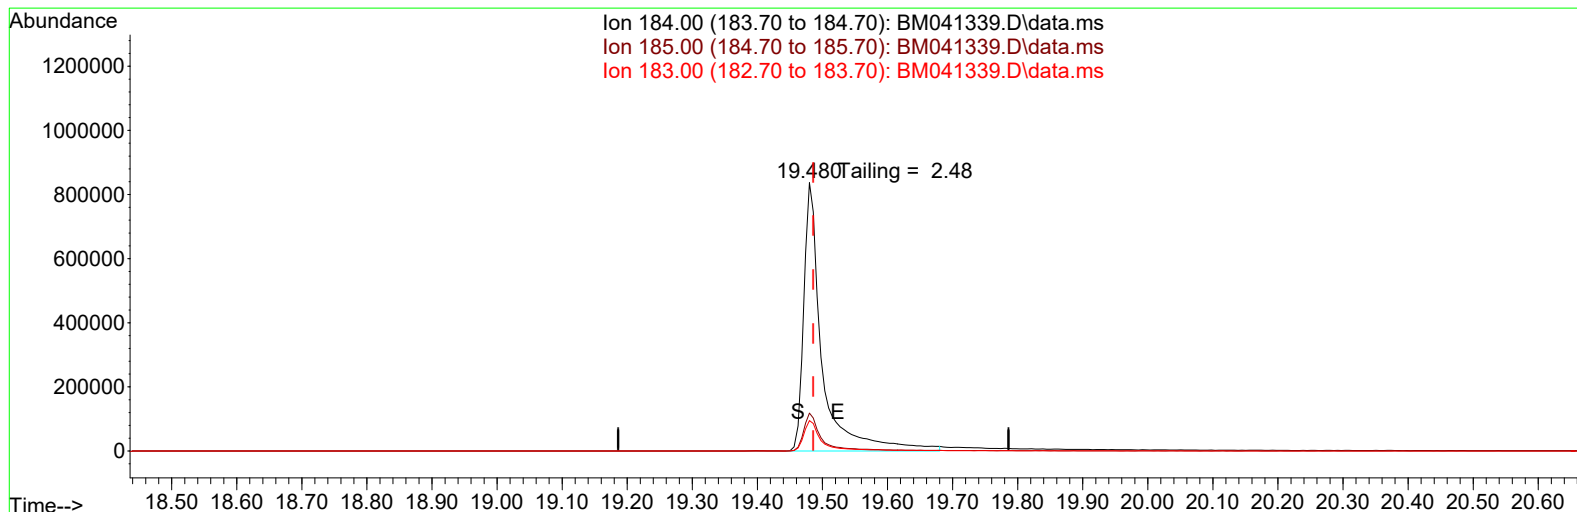

TIC: BM041339.D\data.ms

(77) Benzidine

19.480min (-0.006) 137728.95 ng

response 1640700

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.20  | 14.14  |
| 183.00 | 11.50  | 11.32  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 8/9/2023      | BNA_M            | <u>BM041339.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1097684          | 20.703             |
| DDD           | 37725            | 20.262             |
| DDE           | 3246             | 19.751             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 40971         | 1138655          | 3.60               |
|               |                  |                    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP